

INTERNATIONAL STANDARD



This extended version of IEC 60704-2-2:2023 includes the content of the references made to IEC 60704-1:2021

**Household and similar electrical appliances – Test code for the determination of airborne acoustical noise –
Part 2-2: Particular requirements for fan heaters**

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV





THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2023 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Secretariat
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

IEC publications search - webstore.iec.ch/advsearchform

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee, ...). It also gives information on projects, replaced and withdrawn publications.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: sales@iec.ch.

IEC Products & Services Portal - products.iec.ch

Discover our powerful search engine and read freely all the publications previews. With a subscription you will always have access to up to date content tailored to your needs.

Electropedia - www.electropedia.org

The world's leading online dictionary on electrotechnology, containing more than 22 300 terminological entries in English and French, with equivalent terms in 19 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IECNORM.COM : Click to view the full PDF of IEC 60305-2-2:2023 EXV



INTERNATIONAL STANDARD



This extended version of IEC 60704-2-2:2023 includes the content of the references made to IEC 60704-1:2021

Household and similar electrical appliances – Test code for the determination of airborne acoustical noise – Part 2-2: Particular requirements for fan heaters

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

ICS 17.140.20, 97.100.10

ISBN 978-2-8322-8046-1

Warning! Make sure that you obtained this publication from an authorized distributor.

CONTENTS

FOREWORD.....	4
INTRODUCTION.....	7
1 Scope.....	8
2 Normative references	8
3 Terms and definitions	9
4 Measurement methods and acoustical environments	10
4.1 General.....	10
4.2 Direct method	10
4.3 Comparison method.....	11
4.4 Acoustical environments	11
4.4.1 General requirements and criterion for adequacy of the test environment.....	11
4.4.2 Criterion for background noise level.....	11
4.4.3 Environmental conditions.....	12
4.5 Measurement uncertainties	12
4.5.1 General	12
4.5.2 Standard deviations on repeatability and reproducibility and standard deviations related to declaration and verification	12
5 Instrumentation.....	13
5.1 Instrumentation for measuring acoustical data	13
5.2 Instrumentation for measuring climatic conditions	13
5.3 Instrumentation for measuring operating conditions	13
6 Operation and location of appliances under test	13
6.1 Equipping and pre-conditioning of appliances	13
6.2 Supply of electric energy and of water or gas.....	14
6.3 Climatic conditions.....	14
6.4 Loading and operating of appliances during tests.....	15
6.5 Location and mounting of appliances	15
7 Measurement of sound pressure levels.....	17
7.1 Microphone array, measurement surface and RSS location for essentially free field conditions over reflecting plane(s).....	17
7.2 Microphone array and RSS location in hard-walled test rooms	21
7.3 Microphone array and RSS location in special reverberation test rooms.....	21
7.4 Measurements	21
8 Calculation of sound pressure and sound power levels	22
8.1 General.....	22
8.2 Corrections for background noise levels.....	22
8.3 Corrections for the test environment	23
8.4 Calculation of sound pressure level averaged over the microphone positions.....	23
8.5 Calculation of sound power levels with the comparison method	24
8.6 Calculation of sound power levels in free field conditions over a reflecting plane	24
8.7 Calculation of A-weighted sound power level with the direct method in special reverberation test rooms	24
9 Information to be recorded.....	25
9.1 General data.....	25
9.2 Description of appliance under test	25

9.3	Measurement method	25
9.4	Acoustical test environment	26
9.5	Instrumentation	26
9.6	Equipment and pre-conditioning of appliance under test	26
9.7	Electric supply, water supply, etc.	26
9.8	Climatic conditions	26
9.9	Operation of the appliance under test	27
9.10	Location and mounting of the appliance under test.....	27
9.11	Microphone array	27
9.12	Measurement data	27
9.13	Calculated sound pressure and sound power levels	28
9.14	Reporting	28
10	Information to be reported	28
10.1	General data	28
10.2	Appliance under test	28
10.3	Test conditions for the appliance.....	28
10.4	Acoustical data	29
Annex A (normative)	Standard test table.....	30
Annex B (normative)	Test enclosure	31
Annex C (informative)	Guidelines for the design of simple test rooms with essentially free field conditions.....	32
Bibliography	33
Figure 1	– Measurement surface – parallelepiped – with key microphone positions, for floor free-standing appliances	18
Figure 2	– Measurement surface – parallelepiped – with key microphone positions, for floor standing appliances placed against a wall.....	19
Figure 4	– Measurement surface – hemisphere – with key microphone positions, for hand-held, table type and floor-treatment appliances	20
Figure A.1	– Example of standard test table.....	30
Figure B.1	– Test enclosure	31
Table 1	– Standard deviations of sound power levels.....	12
Table 2	– Standard deviations for declaration and verification.....	12

INTERNATIONAL ELECTROTECHNICAL COMMISSION

**HOUSEHOLD AND SIMILAR ELECTRICAL APPLIANCES –
TEST CODE FOR THE DETERMINATION OF
AIRBORNE ACOUSTICAL NOISE –****Part 2-2: Particular requirements for fan heaters**

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) IEC draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). IEC takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, IEC had not received notice of (a) patent(s), which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at <https://patents.iec.ch>. IEC shall not be held responsible for identifying any or all such patent rights.

This extended version (EXV) of the official IEC Standard provides the user with the comprehensive content of the Standard.

IEC 60704-2-2:2023 EXV includes the content of IEC 60704-2-2:2023, and the references made to IEC 60704-1:2021.

The specific content of IEC 60704-2-2:2023 is displayed on a blue background.

IEC 60704-2-2 has been prepared by subcommittee 59C: Electrical heating appliances for household and similar purposes, of IEC technical committee 59: Performance of household and similar electrical appliances. It is an International Standard.

This third edition cancels and replaces the second edition published in 2009. This edition constitutes a technical revision.

This edition includes the following significant technical changes with respect to the previous edition:

- alignment with the latest edition of IEC 60704-1:2021,
- addition of several ISO standards,
- revision of built-in-conditions,
- addition of requirements on climatic conditions and on background noise.

The text of this International Standard is based on the following documents:

Draft	Report on voting
59C/284/CDV	59C/286/RVC

Full information on the voting for its approval can be found in the report on voting indicated in the above table.

The language used for the development of this International Standard is English.

This part 2-2 is intended to be used in conjunction with the fourth edition of IEC 60704-1:2021, *Household and similar electrical appliances – Test code for the determination of airborne acoustical noise – Part 1: General requirements*.

The relevant text of IEC 60704-1:2021 as amended by this publication establishes the test code for fan heaters.

This part 2-2 supplements or modifies the corresponding clauses in IEC 60704-1:2021.

When a particular subclause of IEC 60704-1:2021 is not mentioned in this part 2-2, that subclause applies as far as reasonable. Where this standard states "addition", "modification" or "replacement", the relevant requirement, test specifications or explanatory matter in IEC 60704-1:2021 shall be adapted accordingly.

Subclauses or figures which are additional to those in IEC 60704-1:2021 are numbered starting from 101.

Additional annexes are lettered AA, BB, etc.

This document was drafted in accordance with ISO/IEC Directives, Part 2, and developed in accordance with ISO/IEC Directives, Part 1 and ISO/IEC Directives, IEC Supplement, available at www.iec.ch/members_experts/refdocs. The main document types developed by IEC are described in greater detail at www.iec.ch/publications.

A list of all the parts in the IEC 60704 series, under the general title *Household and similar electrical appliances – Test code for the determination of airborne acoustical noise*, can be found on the IEC website.

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under webstore.iec.ch in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn, or
- revised.

IMPORTANT – The "colour inside" logo on the cover page of this document indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this document using a colour printer.

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

INTRODUCTION

The measuring conditions specified in this part 2-2 provide for sufficient accuracy in determining the noise emitted and comparing the results of measurements taken by different laboratories, whilst simulating as far as possible the practical use of fan heaters.

It is recommended to consider the determination of noise levels as part of a comprehensive testing procedure covering many aspects of the properties and performance of fan heaters.

NOTE As stated in the introduction to IEC 60704-1, this test code is concerned with airborne noise only.

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

HOUSEHOLD AND SIMILAR ELECTRICAL APPLIANCES – TEST CODE FOR THE DETERMINATION OF AIRBORNE ACOUSTICAL NOISE –

Part 2-2: Particular requirements for fan heaters

1 Scope

This part of IEC 60704 applies to electric fan heaters, designed for placing on the floor, table or counter, etc., or for mounting.

This document does not apply to

- electric storage room heaters;
- room humidifiers;
- room dehumidifiers;
- air cleaners;
- heaters designed exclusively for industrial purposes.

For determining and verifying noise emission values declared in product specifications, refer to IEC 60704-3:2019.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60704-2 (all parts), *Household and similar electrical appliances – Test code for the determination of airborne acoustical noise*

IEC 60704-3:2019, *Household and similar electrical appliances – Test code for the determination of airborne acoustical noise – Part 3: Procedure for determining and verifying declared noise emission values*

IEC 61260-1:2014, *Electroacoustics – Octave-band and fractional-octave-band filters – Part 1: Specifications*

IEC 61672-1:2013, *Electroacoustics – Sound level meters – Part 1: Specifications*

ISO 3743-1:2010, *Acoustics – Determination of sound power levels of noise sources – Engineering methods for small, movable sources in reverberant fields – Part 1: Comparison method for hard-walled test rooms*

ISO 3743-2:2018, *Acoustics – Determination of sound power levels of noise sources using sound pressure – Engineering methods for small, movable sources in reverberant fields – Part 2: Methods for special reverberation test rooms*

ISO 3744:2010, *Acoustics – Determination of sound power levels of noise sources using sound pressure – Engineering method in an essentially free field over a reflecting plane*

ISO 9614-1:1993, *Acoustics – Determination of sound power levels of noise sources using sound intensity – Part 1: Measurement at discrete points*

ISO 9614-2:1996, *Acoustics – Determination of sound power levels of noise sources using sound intensity – Part 2: Measurement by scanning*

ISO 9614-3:2002, *Acoustics – Determination of sound power levels of noise sources using sound intensity – Part 3: Precision method for measurement by scanning*

ISO 6926:2016, *Acoustics – Requirements for the performance and calibration of reference sound sources used for the determination of sound power levels*

ISO 12001:1996, *Acoustics – Noise emitted by machinery and equipment – Rules for the drafting and presentation of a noise test code*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply. Terms and definitions pertinent to the determination of sound power levels can be found in ISO 3743-1:2010, ISO 3743-2:2018 and ISO 3744:2010.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

3.1

measurement time interval

portion or a multiple of an operational period or operational cycle for which the sound power levels are determined

3.2

operational period

interval of time during which a specified process is accomplished by the appliance under test (for example, washing or rinsing or drying for a dishwasher)

3.3

operational cycle

specific sequence of operational periods occurring while the appliance under test performs a complete work cycle

Note 1 to entry: During the operational cycle, each operational period is associated with a specific process that can occur only once, or can be repeated (for example, washing and rinsing and drying for a dishwasher).

3.4

time history

continuous recording of the sound pressure level (for a distinct microphone position) as a function of time, which is obtained during one or more operational periods of an operational cycle

3.5

reference box

hypothetical right parallelepiped terminating on the reflecting plane(s) on which the noise source under test is located, that just encloses the source including all the significant sound radiating components and any test table on which the source is mounted

[SOURCE: ISO 3744:2010, 3.10, modified – The note has been omitted.]

3.6

test enclosure

enclosure used for simulating the typical acoustic built-in or/and mounting conditions

4 Measurement methods and acoustical environments

4.1 General

This document is concerned with objective methods of engineering accuracy grade 2 in accordance with ISO 12001:1996 for determining sound power levels L_W , expressed in decibels (dB), with reference to a sound power of one picowatt (1 pW), of airborne acoustical noise within the specified frequency range of interest (generally including the octave-bands with centre frequencies from 125 Hz to 8 000 Hz), and for prescribed operating conditions of the appliance to be measured.

Methods for determining sound power levels with precision accuracy grade 1 in accordance with ISO 12001:1996, as specified for example in ISO 3741 and ISO 3745, are not included in this document. They may, however, be applied if the appropriate test environment and instrumentation are available.

NOTE 1 The noise values obtained under the described conditions of this document will not necessarily correspond to the noise experienced under the operational conditions of practical use.

NOTE 2 For quality control during production etc., simplified methods can be appropriate. For noise reduction purposes, other measurement methods employing, for example, narrow-band analysis or intensity techniques usually have to be applied. These methods are not covered by this document.

The total noise emitted by machinery or equipment and radiated in all directions to the space surrounding the machine can be characterized by the sound power of the machine. Within the accuracy range of this document, the sound power of a machine is basically independent of the environment in which the machine is installed

Therefore, the concept of sound power level has been chosen for expressing the noise emission of appliances for household and similar purposes.

The preferred noise emission quantity is the A-weighted sound power level, L_{WA} , in dB (re 1 pW).

According to this document, two principal methods exist, the direct method and the comparison method, as described in 4.2 and 4.3. These two methods can be used alternatively.

Different types of environments, as described in 4.4, may be used. A part of the IEC 60704-2 series may, if necessary, exclude one or several combinations among those available.

4.2 Direct method

The direct method can be used only for measurements in qualified test environments in accordance with ISO 3744:2010 for free field conditions over reflecting plane(s), and in accordance with ISO 3743-2:2018 for special reverberation test rooms.

With this method, the sound power level is determined

- in free field conditions over reflecting plane(s), from time-averaged sound pressure levels (on a mean-square basis) over the measurement surface and from the area of the measurement surface, S , or
- in reverberation and special reverberation test rooms, from averaged sound pressure levels, and from the reverberation time and the volume of the test room.

If for a measurement in a free field, reverberation or special reverberation room is not possible because the appliance cannot be placed or operated in such an environment, the intensity method in accordance with ISO 9614-1:1993, ISO 9614-2:1996, and ISO 9614-3:2002 shall be applied. For the intensity method, the standard deviations given in the parts of the IEC 60704-2 series and IEC 60704-3:2019 are not applicable unless stated explicitly.

These methods yield results expressed in A-weighted sound power levels (and in octave- or 1/3 octave-band sound power levels, if required) that are calculated directly from measured sound pressure levels.

NOTE This method can also be used in conjunction with more precise methods, such as those given in ISO 3741 and ISO 3745.

NOTE If pure tone components are present in the noise emitted, proper precautions need to be taken as specified in ISO 3743-2.

4.3 Comparison method

The comparison method for measurement is explicitly described in ISO 3743-1:2010 and in ISO 3743-2:2018.

NOTE The term "comparison method" is not explicitly given in ISO 3744:2010, but when applying the "absolute comparison test" for the determination of the environmental correction given in A.3 of ISO 3744:2010, by using a reference sound source, the procedure is, in fact, a comparison method.

With this method, the sound power level is determined by comparing the averaged values (on a mean-square basis) of the sound pressure levels produced by the source in the test room to the averaged values of the sound pressure levels produced in the same room by a calibrated reference sound source (RSS) of known sound power output, complying with the requirements of ISO 6926:2016. The difference in sound pressure levels is equal to the difference in sound power levels when conditions are the same for both sets of measurements.

This method yields results expressed in octave- or 1/3 octave-band sound power levels, and the A-weighted sound power level is calculated from the octave- or 1/3 octave-band sound power levels.

To check whether there is a systematic difference between results obtained in different environments, the use of the comparison method is recommended.

NOTE If pure tone components are present in the noise emitted, proper precautions need to be taken as specified in ISO 3743-1 and 3743-2.

4.4 Acoustical environments

4.4.1 General requirements and criterion for adequacy of the test environment

ISO 3743-1, ISO 3743-2 and ISO 3744 can be used for measuring noise emitted by fan heaters.

The method specified in ISO 3744 is applicable to noise sources of any size. When applying ISO 3743-1 and ISO 3743-2, care shall be taken that the maximum size of the appliance under test fulfils the requirements specified in ISO 3743-1:2010, 1.3 and ISO 3743-2.

4.4.2 Criterion for background noise level

Requirements for the background noise level are given in 4.5 of ISO 3743-1:2010, in 6.5 of ISO 3743-2:2018 and in 4.2 of ISO 3744:2010. Averaged over the microphone positions, the background noise level shall be at least 6 dB below, and preferably more than 15 dB below, the sound pressure level to be measured.

NOTE If the difference between the sound pressure levels of the background noise and the appliance noise is less than 6 dB, see 8.2.

4.4.3 Environmental conditions

Environmental conditions having an adverse effect on the microphone used for the measurements (for example, strong electric or magnetic fields, wind, impingement of air discharge from the equipment being tested, high or low temperatures) shall be avoided by proper selection or positioning of the microphone.

The instructions of the manufacturers of the measurement instruments regarding adverse environmental conditions shall be followed. The microphone shall always be oriented in such a way that the angle of incidence of the sound waves is that for which the microphone is calibrated.

4.5 Measurement uncertainties

4.5.1 General

The estimated values of the standard deviations of reproducibility of sound power levels determined in accordance with this document are given in 9.1 of ISO 3743-1:2010, in 11.1 of ISO 3743-2:2018 and in 9.1 of ISO 3744:2010. But for a particular family of appliances of similar size with similar operating conditions, the standard deviations of reproducibility can be smaller than these values. Hence, in the IEC 60704-2 series, standard deviations smaller than those listed in ISO standards can be stated if substantiation is available from the results of suitable interlaboratory tests.

In the case of discrepancies between the measurements where the results normally remain inside the foreseen standard deviation, it can be helpful to perform measurements according to the upper grade of accuracy: grade 1, laboratory or precision, as described in ISO 3741 or ISO 3745.

4.5.2 Standard deviations on repeatability and reproducibility and standard deviations related to declaration and verification

The estimated values of standard deviations of sound power levels determined according to this document are given in Table 1:

Table 1 – Standard deviations of sound power levels

Standard deviation dB	
σ_r (repeatability)	σ_R (reproducibility)
0,4	1,0

For the purpose of determining and verifying declared noise emission values according to IEC 60704-3, the values given in Table 2 apply:

Table 2 – Standard deviations for declaration and verification

Standard deviation dB		
σ_P (production)	σ_t (total)	σ_M (reference)
0,3 to 1,1	1,0 to 1,6	1,5

5 Instrumentation

5.1 Instrumentation for measuring acoustical data

Requirements for the instrumentation system and for its calibration are given in Clause 5 of ISO 3743-1:2010, in Clause 7 of ISO 3743-2:2018 and in Clause 5 of ISO 3744:2010.

The instrumentation system shall meet the requirements for a type 1 instrument laid down in IEC 61672-1:2013, in accordance with the basic standard used. For measurements in octave- and 1/3 octave-bands, the instrumentation system shall meet the requirements of IEC 61260-1:2014.

RSS shall meet the requirements of ISO 6926:2016, and shall be calibrated annually.

Windscreens should be used and the relevant corrections for changes in the microphone sensitivity shall be added to the observed sound pressure levels.

5.2 Instrumentation for measuring climatic conditions

5.2.1 The temperature is determined with instruments having an accuracy of ± 1 °C.

5.2.2 The relative humidity is determined with instruments having an absolute accuracy of ± 2 % within the measuring range.

5.2.3 The absolute air pressure is determined with instruments having an accuracy of $\pm 0,5$ kPa.

5.3 Instrumentation for measuring operating conditions

5.3.1 The voltage at the plug of the cable or cord of mains-powered appliances is measured with voltmeters having an accuracy of class 0,5 instruments.

5.3.2 The voltage at the battery terminals of battery-powered appliances is measured with voltmeters having an accuracy of class 0,5 instruments.

5.3.3 The rotational speed of motors, attachments, etc. is measured, if necessary, with speed indicators having an accuracy of ± 1 % of full scale.

6 Operation and location of appliances under test

6.1 Equipping and pre-conditioning of appliances

6.1.1 The appliance is equipped with attachments, accessories, etc. as delivered by the manufacturer for the intended use or function.

Air filters, if any, shall be clean.

6.1.2 Care shall be taken to ensure that any auxiliary equipment (such as electrical conduits or cables, piping for water supply or drainage, air ducts, etc.) necessary for the operation of the appliance, does not radiate a significant amount of sound into the test environment or change the sound output of the appliance. Guidelines are given in 6.2 of ISO 3743-1:2010, in 8.4 of ISO 3743-2:2018 and in 6.2 ISO 3744:2010.

6.1.3 Prior to noise measurements, the appliance, equipped in accordance with 6.1.1, shall have been in operation for a total period of at least 2 h for running-in at the highest speed setting with the maximum heating switched on for normal permanent use.

Oscillating function if available shall be switched on.

During the running-in procedure, air filters, if any, shall be removed, if possible. If filters remain in the appliances during this running-in period, they shall be cleaned or renewed after this period.

6.1.4 Immediately before each series of noise measurements, the appliance equipped in accordance with 6.1.1 shall be operated for stabilizing at the highest speed setting and maximum heating switched on for normal permanent use for 5 min.

6.2 Supply of electric energy and of water or gas

6.2.1 Appliances with mains powered electric motor(s) are supplied at rated voltage and at rated frequency. Appliances designed for DC only are supplied with DC. If a voltage range and/or a frequency range are indicated, then the supply voltage and/or frequency shall be the nominal system voltage and/or system frequency of the country in which the appliance is intended to be used. Tolerances shall not exceed $\pm 2\%$ for voltage and $\pm 1\%$ for frequency throughout the test.

Modification:

The voltage tolerance shall be $\pm 0,5\%$.

The nominal system voltage and its values are defined in IEC 60038:2009.

If the rated voltage of a mains supplied appliance differs from the nominal system voltage as common in the country of use, measurements should be carried out at the nominal voltage as common in the country of use.

The supply voltage is measured at the plug of a non-detachable cable or cord, or at the appliance inlet if a detachable cable is provided, but in no case at the entrance of extension cables or cords.

6.2.2 Not applicable.

6.2.3 The appliance shall be operated with the heating elements switched on.

Special attention is required to be given to the possible effect of the temperature rise on the acoustical behaviour of the test room.

6.2.4 Not applicable.

6.3 Climatic conditions

In general, household appliances (unless otherwise specified for a special family) are operated under the following climatic conditions:

ambient temperature	18 °C to 28 °C
relative humidity	25 % to 70 %
atmospheric pressure	86 kPa to 106 kPa

6.4 Loading and operating of appliances during tests

6.4.1 General requirements are given in 6.5 of ISO 3743-1:2010, in 8.5 of ISO 3743-2:2018 and in 6.6 of ISO 3744:2010. For the purpose of establishing a noise test code, the following guidelines are given, unless otherwise specified in the relevant part of the IEC 60704-2 series.

In general, the loading and operating conditions should, as far as practicable, simulate normal use but, in every case, preference has to be given to simple conditions providing satisfactory repeatability and reproducibility.

The presence of an operator should be avoided. An operator shall be present only if the application of the load is not practicable without an operator. This operator shall not wear abnormally sound absorptive clothing that might influence the sound measurements.

6.4.2 The appliance shall be equipped according to 6.1.1.

The noise emission shall be determined with the appliance at the highest speed setting and maximum heating for normal permanent use. Oscillating function, if any, shall be switched on.

NOTE Other possible speed settings (minimum heat output, boost position, etc.) can be measured in addition. The respective noise levels need to be linked to the relevant heat output.

Appropriate adjustment of air intake or exhaust openings shall be done taking into account manufacturer's instructions if any, or otherwise selecting the configuration that gives the highest noise emission.

6.4.3 Not applicable.

6.4.4 When applying loading and operating conditions for determining noise emission, care shall be taken to avoid possible overheating of the appliance under test. Rated operating and resting times and/or the manufacturer's instructions shall be followed.

6.5 Location and mounting of appliances

6.5.1 The basic requirements in 6.3 and 6.4 of ISO 3743-1:2010, in 8.2 and 8.3 of ISO 3743-2:2018 and in 6.3 and 6.4 of ISO 3744:2010 shall be followed. The following guidelines are given, unless otherwise specified in the relevant part of the IEC 60704-2 series.

6.5.2 Floor-standing appliances, counter-top or table-type appliances, are placed in their normal position directly, without any resilient means other than those incorporated in the appliance:

- either on the floor of the hard-walled test room or of the special reverberation test room with a minimum distance of 1 m between any surface (including protruding parts) of the appliance and the nearest wall;
- or on the reflecting plane of the free field environment, taking into account the shape and size of the specified measurement surface.

Stand-type appliances (such as appliances designed for use on a stand, for example, hair drying hoods) are placed on the stand supplied with the appliance, or on a stand constructed in accordance with the manufacturer's instructions.

Sound radiation due to possible vibrations of the piece of floor covering shall be prevented. The piece of floor covering is considered to be a part of the appliance under test, and its possible influence on the acoustical characteristics of the test environment is not taken into account.

Table-top appliances, where a table is required for operation, are placed in the centre of the top of the standard test table described in Annex A.

The tests under the conditions stated in 6.5.4 shall be repeated for floor-standing appliances which may be placed either against or away from the wall.

For such appliances, both sets of results shall be recorded and the measurement that gives highest noise is then chosen.

6.5.3 Not applicable.

6.5.4 For measurements on floor-standing appliances intended for placing against a wall, including those for building-in into a cabinet, a vertical reflecting plane having an acoustic absorption coefficient of less than 0,06 shall be used.

When measurements are made in a reverberation test room, a part of the wall of the room will serve for this purpose. The minimum area of this part of the wall should be determined by the projection of the appliance extended by at least 0,5 m upwards and to both sides. The minimum distance between any surface of the appliance or its cabinet and the nearest corner of the room shall be 1 m.

When measurements are made in a free-field environment, the size of the vertical reflecting plane (supported by the horizontal reflecting plane) shall be at least equal to the size of the projection of the measurement surface.

For both types of test environment, the following requirements shall be complied with:

- the appliance shall be placed in the test environment without any resilient means of support other than those incorporated in the appliance;
- care should be taken to avoid any direct contact between the appliance (including protruding parts, worktops, spacers, etc.) and the vertical reflecting wall;
- the distance between the wall and the appliance shall be established by placing the appliance in direct contact with the wall and moving it away for a distance not exceeding $10\text{ cm} \pm 1\text{ cm}$.

6.5.5 Wall-mounted appliances, including their accessories, if any, are fastened or held by an appropriate fixture in close contact, without any resilient means other than those incorporated in the appliance:

- either on a wall of the hard-walled test room or of the special reverberation test room;
- or on a vertical reflecting plane in the free field environment. The minimum size of this vertical plane shall be at least equal to the size of the projection of the measurement surface. The acoustic absorption coefficient of the vertical reflecting plane shall be smaller than 0,06.

The height of the lowest edge of the appliance from the floor shall be $25\text{ cm} \pm 1\text{ cm}$.

NOTE For appliances intended for mounting close to the ceiling with the air stream directed towards the floor, measurements problems can be caused when the appliance is mounted as specified in 6.5.5. It can be necessary to mount such an appliance in an inverted position, with the top of the appliance facing towards the floor at a height of 0,25 m, or at the distance specified by the manufacturer for mounting close to the ceiling. The manufacturer's approval needs to be obtained before operating the appliance under the proposed test conditions.

The location of the appliance (fastened or held in an appropriate fixture) as for floor-standing appliances (see 6.5.2) may be adopted, if preliminary investigation has shown that the resulting sound power level value is not significantly different from that determined with the location prescribed in this subclause.

6.5.6 Appliances to be built-in are built-in in accordance with the manufacturer's installation instructions in an appropriate test enclosure in accordance with Annex B.

The manufacturer's instructions regarding installation and use of the appliance shall be followed. The front edge of the appliance (including the door) shall be aligned with the front edge of the test enclosure. If the manufacturer's installation instructions provide for a skirting board at the lower front side of the appliance, the test enclosure shall be provided with a skirting board of the maximum height compatible with the door assembly and of the same material and thickness as the test enclosure.

Care should be taken to ensure that no structure-borne noise is transmitted to the test enclosure.

If an appliance is provided with spacers, strips, or other special means of solid or resilient material for closing the gap(s) between the contours of the appliance and the cabinet or enclosure, these means shall be used accordingly. If such means are not provided, the gap(s) are left open.

At the rear left-hand or right-hand corner of the test enclosure, a cut-out at a minimum size shall be provided to enable, for example, power supply, water supply and drainage. This cut-out shall be sealed to avoid any noise leakage.

If necessary, the test enclosure shall be provided with ventilation openings in accordance with the manufacturer's instructions.

The test enclosure with the appliance shall be placed in accordance with 6.5.2, 6.5.4 or 6.5.5. If doors are protruding, the test enclosure shall be provided with a base shelf lying on the reflecting plane. The thickness of the base shelf shall be adapted to allow the opening of the protruding door. Care shall be taken that the base shelf does not transmit any structure-borne noise to the test enclosure.

Appliances to be integrated shall be installed in the same conditions as built-in appliances. In addition, they shall be equipped, in accordance with the manufacturer's instructions, with a door assembly of the maximum surface allowed by the manufacturer, and of the same material and thickness as the test enclosure.

Modification:

Built-in heaters such as plinth heaters shall be installed according to manufacturer's instructions.

7 Measurement of sound pressure levels

7.1 Microphone array, measurement surface and RSS location for essentially free field conditions over reflecting plane(s)

During measurements, care shall be taken to prevent direct blowing to the microphones.

7.1.1 The requirements in 7.1 to 7.2 of ISO 3744:2010 shall be followed. Guidance for the selection of the measurement surface and microphone array in the relevant part of IEC 60704-2 series is given below; care shall be taken to use only one of the following two shapes and one of the possible microphone arrays for a particular family of appliances, unless otherwise specified in the relevant part of the IEC 60704-2 series.

7.1.2 For floor-standing free-standing appliances, including built-in appliances, the measurement surface is a parallelepiped with nine microphone positions, as specified in 7.2.4 of ISO 3744:2010 and in Figure 1. Additional measurement positions can be required in

accordance with 8.1.2 of ISO 3744:2010 and Annex C of ISO 3744:2010. The number of microphone positions can also be reduced in accordance with 8.1.2 of ISO 3744:2010 and Annex C of ISO 3744:2010.


The preferred value of the measurement distance d is 1 m.

For determining time histories, frequency spectra, etc. of the appliance, microphone position no. 1 is recommended for the nine-microphone array.

NOTE The front of the appliance, unless otherwise stated in the relevant part of the IEC 60704-2 series, is directed in the direction of the x -axis.

Coordinates of microphone positions:

No.	x	y	z
1	a	0	$0,5 \cdot c$
2	0	b	$0,5 \cdot c$
3	$-a$	0	$0,5 \cdot c$
4	0	$-b$	$0,5 \cdot c$
5	a	b	c
6	$-a$	b	c
7	$-a$	$-b$	c
8	a	$-b$	c
9	0	0	c

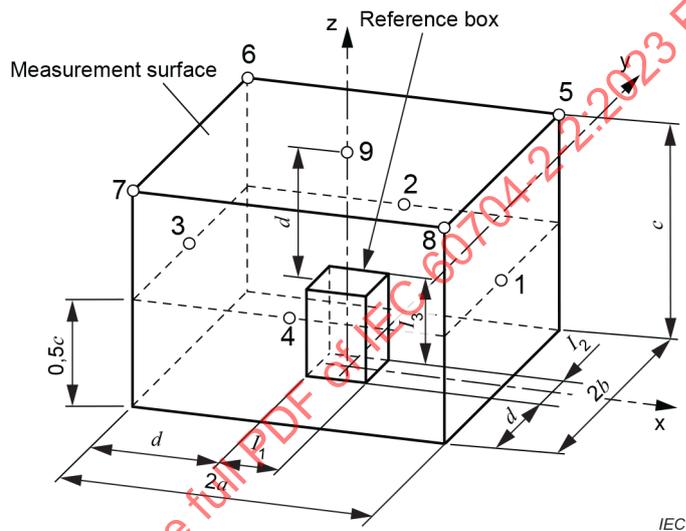

Measurement surface area:

$$S = 2 (2 \cdot b \cdot c + 2 \cdot a \cdot c + 2 \cdot a \cdot b)$$

Figure 1 – Measurement surface – parallelepiped – with key microphone positions, for floor free-standing appliances

7.1.3 For floor-standing or counter-type appliances for placing against a wall, including built-in appliances, the measurement surface is a parallelepiped, with six microphone positions, as specified in 7.2.4 of ISO 3744:2010 and in Figure 2 of this document. Additional measurement positions can be required in accordance with 8.1.2 of ISO 3744:2010 and Annex C of ISO 3744:2010. The number of microphones can also be reduced in accordance with 8.1.2 of ISO 3744:2010 and Annex C of ISO 3744:2010.

The preferred value of the measurement distance d is 1 m.

For determining time histories, frequency spectra, etc. of the appliance, microphone position no. 1 is recommended for the six-microphone array.

This measurement surface can also be used for wall-mounted appliances.

NOTE 1 The front of the appliance is directed in the direction of the x -axis.

NOTE 2 In this case, the x and y axes are located in the vertical reflecting plane, with the x -axis directed vertically upwards and the front of the appliance being directed in the direction of the z -axis.

Coordinates of microphone positions:

No.	x	y	z
1	$2 \cdot a$	0	$0,5 \cdot c$
2	a	b	$0,5 \cdot c$
3	a	$-b$	$0,5 \cdot c$
4	$2 \cdot a$	b	c
5	$2 \cdot a$	$-b$	c
6	a	0	c

Measurement surface area:

$$S = 2 (2 \cdot a \cdot c + 2 \cdot a \cdot b + b \cdot c)$$

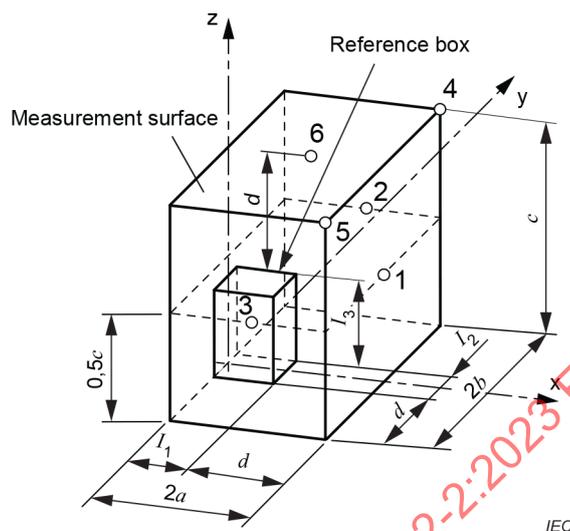


Figure 2 – Measurement surface – parallelepiped – with key microphone positions, for floor standing appliances placed against a wall

7.1.4 Not applicable.

7.1.5 For counter-top or table-type appliances, floor-treatment appliances and handheld appliances (mounted in test fixtures), with each of the dimensions of the reference box not exceeding 0,7 m, and placed during measurements on the horizontal reflecting plane, the measurement surface is a hemisphere with 10 microphone positions, as specified in 7.2.3 of ISO 3744:2010 and shown in Figure 4 of this document. Additional measurement positions can be required in accordance with 8.1.1 of ISO 3744:2010. In special cases, a different number and arrangement of microphone positions can be used, if the requirements in 8.1.1 of ISO 3744:2010 are satisfied.

If the reference box has a dimension exceeding 0,7 m, the microphone array and measurement surface described in 7.1.2 of this document shall be used.

The radius r , of the hemispherical measurement surface preferably shall be equal to 2 m, but in any case not less than 1,5 m.


NOTE The front of the appliance, unless otherwise specified in the relevant part of IEC 60704-2 series, is directed in the direction of the x -axis. For determining time histories, frequency spectra, etc. of the appliance, microphone position no.8 is recommended for the 10-microphone array.

Coordinates of microphone positions:

No.	x/R	y/R	z/R
1	-0,99	0	0,15
2	0,50	-0,86	0,15
3	0,50	0,86	0,15
4	-0,45	0,77	0,45
5	-0,45	-0,77	0,45
6	0,89	0	0,45
7	0,33	0,57	0,75
8	-0,66	0	0,75
9	0,33	-0,57	0,75
10	0	0	1,0

Measurement surface area:

$$S = 2 \cdot \pi \cdot R^2$$

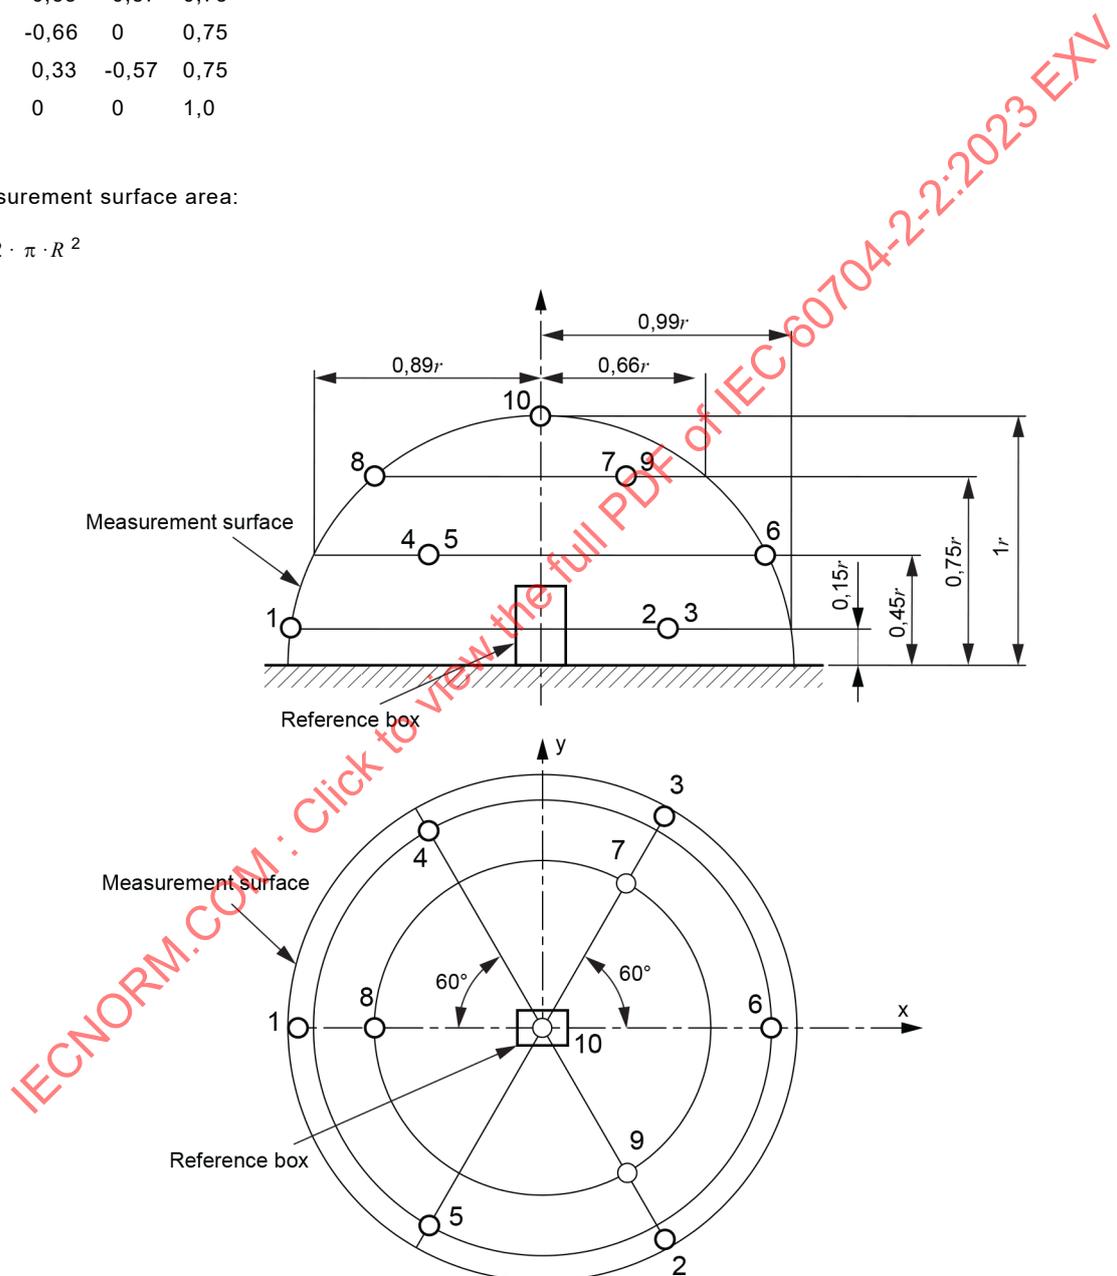

IEC

Figure 3 – Measurement surface – hemisphere – with key microphone positions, for hand-held, table type and floor-treatment appliances

7.1.6 Not applicable.

7.1.7 Not applicable.

7.1.8 If the appliance under test emits steady noise, it is permissible to measure the surface sound pressure level by traversing a microphone along measurement paths, instead of at individual microphone positions, as described in 7.4.3 of this document and in Annex B and Annex C of ISO 3744:2010.

7.1.9 Guidelines for the location of the RSS are given in Annex A of ISO 3744:2010.

7.2 Microphone array and RSS location in hard-walled test rooms

The requirements in Clause 7 of ISO 3743-1:2010 shall be followed.

In general, at least three microphone positions should be used.

According to 7.2 of ISO 3743-1:2010, the hard-walled test room is more suitable for sources not designed to be placed on the floor against a wall or to be wall-mounted. Should the source under test be closer than 1 m to the wall, the RSS shall not be placed at the position of the source, but at a position on the floor 1 m from the wall.

7.3 Microphone array and RSS location in special reverberation test rooms

The requirements in Clause 9 of ISO 3743-2:2018 shall be followed.

In general, the number of microphone positions $N_m = 6$ and the number of source locations $N_s = 1$.

A change of these numbers depends on the results of a preliminary measurement in accordance with 9.4 of ISO 3743-2:2018.

When, according to these preliminary investigations, the standard deviation S_M is above 4,0 dB, in order to reduce the effort of measuring in a special reverberation test room, the use of a moving microphone instead of 12 individual microphone positions is recommended; alternatively, measurements under free field conditions can be preferable.

NOTE The use of a moving microphone traversing a path, in accordance with 9.6 of ISO 3743-2:2018, is often more convenient than the use of a number of fixed microphones.

In general, the RSS used for the comparison method is measured with the same microphone array and with the same number of source locations as used for the appliance under test. The RSS is located on the floor so that the projection of the centre of its reference box coincides with the projection of the centre of the reference box of the appliance under test.

7.4 Measurements

7.4.1 For measurements in free-field conditions over a reflecting plane, the requirements in 4.1, Clause 5 and 8.2.1 of ISO 3744:2010 shall be followed; for measurements in hard-walled test rooms, the requirements in Clause 7 of ISO 3743-1:2010 shall be followed; for measurements in special reverberation test rooms, the requirements in Clause 9 of ISO 3743-2:2018 shall be followed.

The time-average sound pressure level has to be observed at each microphone position over a typical period of operation of the appliance. For noise that varies with time, the period of observation shall be specified carefully.

In the case of a moving microphone, the integration time should include at least one full traverse for measurements in accordance with ISO 3743-1:2010 or ISO 3743-2:2018, and at least two full traverses for measurements in accordance with ISO 3744:2010.

NOTE 1 The measurement time interval can be chosen to be representative of the period of maximum noise level.

The time-averaged A-weighted sound pressure levels shall be measured during at least 30 s and including complete cycles (at least two cycles) of the oscillating function, if any.

The frequency range of interest for sound power determination on fan heaters includes at least the octave bands with centre frequencies from 63 Hz to 8 000 Hz.

NOTE 2 In many cases, the 63 Hz octave band level does not participate significantly to the A-weighted level.

NOTE 3 When measuring this 63 Hz octave band, a special attention needs to be paid to the room effect.

7.4.2 The following data shall be measured and considered when using the comparison method in hard-walled test rooms, or in special reverberation test rooms:

- time-averaged octave- or 1/3 octave-band sound pressure levels at each microphone position (or each traverse) during operation of the appliance under test;
- time-averaged octave- or 1/3 octave-band sound pressure levels at each microphone position (or each traverse) when the RSS is operating;
- time-averaged octave- or 1/3 octave-band sound pressure levels produced by the background noise.

7.4.3 The following data shall be measured and considered for measurements in free field conditions over a reflecting plane, or when using the direct method in special reverberation test rooms:

- A-weighted or octave- or 1/3 octave-band time-averaged sound pressure levels during operation of the appliance under test;
- A-weighted or octave- or 1/3 octave-band time-averaged sound pressure levels produced by the background noise.

7.4.4 Not applicable.

8 Calculation of sound pressure and sound power levels

8.1 General

For measurements in hard-walled test rooms, the requirements in Clause 8 of ISO 3743-1:2010 shall be followed. For measurements in special reverberation test rooms, the requirements in Clause 10 of ISO 3743-2:2018 shall be followed. For measurements in free-field conditions over a reflecting plane, the requirements in 8.2 of ISO 3744:2010 shall be followed.

8.2 Corrections for background noise levels

If the background noise levels, L_p'' , are more than 6 dB below the measured sound pressure levels, L_p' , the values of L_p' shall be corrected to take into account the influence of background noise. The corrected value, L_p is given by

$$L_p = 10 \cdot \lg \left(10^{0,1L_p'} - 10^{0,1L_p''} \right) \text{ dB (re } 20 \mu\text{Pa)} \quad (2)$$

For measurements in hard-walled test rooms or in special reverberation test rooms, this formula applies to the sound pressure levels measured at each microphone position, before calculating the sound pressure level averaged over the microphone positions.

For measurements in free-field conditions over a reflecting plane, Formula (2) applies to the sound pressure level averaged over the microphone positions (see 8.4).

When the background noise levels are more than 15 dB below the sound pressure levels with the source operating, no correction is made.

Even if the measurement is invalid for one or more frequency bands, it can still be valid for the A-weighted value, provided that the difference between L_{pA}' and L_{pA}'' is greater than 6 dB.

If it can be demonstrated that the absolute criteria for background noise is fulfilled and the background noise levels in the test room at the time of the measurements are less than or equal to those given in 4.2.2 of ISO 3744:2010 for all bands within the frequency range of interest, the measurements can be taken as having met the background noise requirements of this document, even if the 6 dB requirement is not met for all bands. It can be assumed that the source emits little or no measurable noise in these frequency bands, and that the data reported represent an upper bound to the sound power level in these bands.

If the 6 dB criterion is not satisfied and the absolute criteria for background noise is not fulfilled, the accuracy of the result(s) is reduced. No correction for those levels is allowed if the measurements are made in hard-walled rooms or in special reverberation test rooms, and for measurements made in free field over a reflecting plane, a maximum correction of 1,3 dB can be subtracted from the measured values. The results may, however, be reported and may be useful in determining an upper bound to the sound power level of the appliance under test. If such data are reported, it shall be clearly stated in the text of the report, as well as in the graphs and tables of results, that the background noise requirements of this document have not been fulfilled.

8.3 Corrections for the test environment

For measurements in free-field conditions over a reflecting plane, the environmental correction K_2 (see 8.2.4 and Annex A of ISO 3744:2010) is applied to the sound pressure level averaged over the measurement surface, calculated according to the equation given in 8.2.4 of ISO 3744:2010.

The environmental correction is assumed to be zero for measurements made in hemi-anechoic rooms which meet the requirements of ISO 3745.

8.4 Calculation of sound pressure level averaged over the microphone positions

For the A-weighted sound pressure level or the level in each band of interest, an averaged sound pressure level over the microphone positions is calculated from the measured sound pressure levels, using the following equation:

$$L_{pm} = 10 \cdot \lg \left(\frac{1}{N} \sum_{i=1}^N 10^{0,1L_{p,i}} \right) \text{ dB (re } 20 \mu\text{Pa)}$$

where

L_{pm} is the sound pressure level averaged over the microphone positions or over the measurement surface, in dB, re 20 μ Pa;

$L_{p,i}$ is the sound pressure level resulting from the i -th microphone position, in dB, re 20 μ Pa;

N is the number of microphone positions (multiplied if necessary in reverberant field conditions by the number of source locations).

8.5 Calculation of sound power levels with the comparison method

For measurements in hard-walled test rooms or in special reverberation test rooms, the sound power level of the appliance under test, L_W , is calculated in each octave- or 1/3 octave-band within the frequency range of interest, using the equation

$$L_W = L_{W(RSS)} + (\overline{L_{p(AT)}} - \overline{L_{p(RSS)}})$$

where

$L_{W(RSS)}$ is the calibrated sound power level of the RSS, in dB (re 1 pW);

$\overline{L_{p(RSS)}}$ is the sound pressure level of the RSS averaged (energy basis) over the microphone positions or the microphone path, in dB (re 20 µPa);

$\overline{L_{p(AT)}}$ is the sound pressure level of the appliance under test averaged (energy basis) over the microphone positions or the microphone path, in dB (re 20 µPa).

Then, the A-weighted sound power level is calculated from the equation

$$L_{WA} = 10 \cdot \lg \left(\sum_j 10^{0,1(L_{W,j} + A_j)} \right) \text{ dB (re 1 pW)}$$

where

$L_{W,j}$ is the octave-band level, in band j , in dB (re 1 pW);

A_j is the A-weighted value of the midband frequency of octave- or 1/3 octave-band j , as given in Table B.1 of ISO 3743-1:2010.

8.6 Calculation of sound power levels in free field conditions over a reflecting plane

The sound power level of the appliance under test L_W is calculated from the value of the surface sound pressure level determined in accordance with 8.4, corrected from K_1 and K_2 (see 8.2 and 8.3) and from the area of the measurement surface, S , as follows:

$$L_W = L_{p_{mc}} + 10 \cdot \lg \left(\frac{S}{S_0} \right) \text{ dB}$$

where

$L_{p_{mc}}$ is the A-weighted or frequency band surface sound pressure level in accordance with 8.4, corrected from background noise and from environmental correction K_2 , in dB (re 20 µPa);

S is the area of the measurement surface in m²;

S_0 is 1 m².

8.7 Calculation of A-weighted sound power level with the direct method in special reverberation test rooms

The A-weighted sound power level of the appliance under test L_{WA} is calculated from the value of the mean sound pressure level over the microphone positions determined in accordance with 8.4 and the properties of the reverberation test room, as follows:

$$L_{WA} = L_{pmA} - \left(10 \cdot \lg \left(\frac{T_N}{T_0} \right) + 10 \cdot \lg \left(\frac{V}{V_0} \right) - 13 \right) \text{ dB}$$

where

L_{pmA} is the A-weighted sound pressure level averaged in dB over the microphone positions in accordance with 8.4 in dB (re 20 μ Pa);

T_N is the nominal reverberation time of the test room in seconds;

T_0 is 1 s;

V is the volume of the test room in cubic metres;

V_0 is 1 m³.

9 Information to be recorded

9.1 General data

9.1.1 Name and address of the laboratory where measurements are carried out.

9.1.2 File number and date(s) of measurements.

9.1.3 Name and address of the company, organisation, or person, who ordered the measurements.

9.1.4 Purpose of the measurements.

9.1.5 Statement of compliance with this document and the appropriate part of the IEC 60704-2 series.

9.2 Description of appliance under test

9.2.1 Category: for example, vacuum cleaner, washing machine, etc.

9.2.2 Design characteristics: for example, hand-held, table-type, floor-standing.

9.2.3 Manufacturer or dealer, trademark.

9.2.4 Model or type designation (name of product).

9.2.5 Serial number or production date.

9.2.6 Rating data (name plate data): for example, voltage, input capacity, water supply pressure, etc.

9.2.7 Power source and motor data: for example, mains-powered, battery-powered, induction motor, commutator motor, motor speed, etc.

9.2.8 Supplied and/or advertised attachments and/or accessories.

9.3 Measurement method

9.3.1 Direct method and/or comparison method.

9.3.2 Basic ISO standards used.

9.4 Acoustical test environment

9.4.1 Hard-walled test room and/or special reverberation test room and/or free field over reflecting plane.

9.4.2 Test room characteristics: for example, hemi-anechoic laboratory room, outdoor area, ordinary room with or without acoustical treatment, special reverberation test room, hard-walled test room.

9.4.3 Room inner (free) dimensions, volume.

9.4.4 Acoustical treatment of surfaces.

9.4.5 Room qualification, method and data.

9.5 Instrumentation

9.5.1 Instrumentation for measuring acoustical data: name, type, serial number, accuracy, manufacturer of equipment and auxiliaries, date of latest calibration.

9.5.2 Reference sound source with calibration data, manufacturer.

NOTE Calibration date can be according ISO 6926:2016.

9.5.3 Instrumentation for measuring climatic conditions: name, type, serial number, accuracy, manufacturer (if known).

9.5.4 Instrumentation for measuring operating conditions: name, type, serial number, accuracy, manufacturer (if known).

9.6 Equipment and pre-conditioning of appliance under test

9.6.1 Equipment, attachments, accessories selected for measurements.

9.6.2 Running-in procedure and period.

9.6.3 Stabilizing procedure and period.

9.7 Electric supply, water supply, etc.

9.7.1 Mains supply voltage with tolerances, AC, DC, frequency.

9.7.2 Not applicable.

9.7.3 Not applicable.

9.7.4 Not applicable.

9.8 Climatic conditions

9.8.1 Temperature.

9.8.2 Relative humidity.

9.8.3 Atmospheric pressure.

9.9 Operation of the appliance under test

9.9.1 Idling and/or loading conditions; description of the applied load(s).

9.9.2 Selected operation procedure(s): for example, period(s), cycle(s), speed of motor(s), position of controls, etc.

9.9.3 Description of period(s) or cycle(s) used for measurements.

9.10 Location and mounting of the appliance under test

9.10.1 Description of the location of the appliance under test and of the RSS in the test environment: for example, distances from floor and wall(s) (if necessary by making a sketch).

9.10.2 Description of the mounting of the appliance under test: for example, fixtures, built-in cabinets, resilient support(s), floor covering(s), etc.

9.11 Microphone array

9.11.1 Description of the array: for example, number of microphone positions, co-ordinates, measurement distance, radius of the hemisphere, area of the measurement surface, etc.

9.11.2 Description of the location of the microphone array in the test environment: for example, distances from the environment boundaries, etc.

9.11.3 Microphone angle of incidence and orientation with respect to the source.

9.11.4 Fixed microphone(s) or moving microphone, transfer of a single microphone or scanning of the output from all microphones of the array, scanning procedure.

9.11.5 Attachments for microphones: for example, wind shielding accessories with correction data, etc.

9.12 Measurement data

9.12.1 Measured octave- or 1/3 octave-bands and/or A-weighted sound pressure levels for each microphone position and for each of the selected load and operation conditions of the appliance under test, and the periods or cycles used for measurements.

9.12.2 Measured octave- or 1/3 octave-bands sound pressure levels for each microphone position of the RSS.

9.12.3 Measured octave- or 1/3 octave-bands and/or A-weighted sound pressure levels of the background noise before and after each series of measurements.

9.12.4 Applied corrections to the measured values for the appliance under test and for the reference sound source (influence of the background noise and microphone attachments, environmental correction).

9.12.5 Not applicable.

9.12.6 Determined frequency spectra.

9.12.7 Remarks on subjective impression of noise.

9.13 Calculated sound pressure and sound power levels

See Clause 8.

9.14 Reporting

Only those data, recorded in accordance with this clause, which are of importance for the purpose of the measurements, shall be reported. In general, the data of Clause 10 is important.

10 Information to be reported

	Subclause
10.1 General data	9.1
10.2 Appliance under test	9.2
10.2.1 Category	9.2.1
10.2.2 Design characteristics	9.2.2
10.2.3 Manufacturer, dealer, trademark	9.2.3
10.2.4 Model or type, designation	9.2.4
10.2.5 Serial number, production date	9.2.5
10.2.6 Rating data	9.2.6
10.2.7 Power source	9.2.7
10.2.8 Attachments, accessories	9.2.8
10.3 Test conditions for the appliance	Subclause
10.3.1 Selected attachments, accessories	9.6.1
10.3.2 Supply from mains	9.7.1
10.3.3 Not applicable	
10.3.4 Not applicable	
10.3.5 Not applicable	
10.3.6 Temperature	9.8.1
10.3.7 Relative humidity	9.8.2
10.3.8 Atmospheric pressure	9.8.3
10.3.9 Applied load	9.9.1
10.3.10 Operation procedure	9.9.2
10.3.11 Not applicable	
10.3.12 Location in the test room	9.10.1
10.3.13 Mounting	9.10.2

10.4 Acoustical data

	Subclause	
10.4.1	Direct and/or comparison method	9.3.1
10.4.2	Basic ISO standard(s) used	9.3.2
10.4.3	Reference sound source (RSS)	9.5.2
10.4.4	Test environment	9.4.1
10.4.5	Microphone array	9.11.1
10.4.6	Scanning procedure	9.11.4
10.4.7	Measured sound pressure levels of the appliance	9.12.1
10.4.8	Measured sound pressure levels of the RSS	9.12.2
10.4.9	Applied corrections	9.12.4
10.4.10	Not applicable	
10.4.11	Frequency spectra	9.12.6
10.4.12	Calculated sound power levels	9.13

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

Annex A (normative)

Standard test table

A suitable design for a standard test table is shown in Figure A.1. The top of the table shall be of bonded laminated wood 0,10 m thick, having a minimum area of 0,5 m² and a minimum lateral dimension of 0,7 m. The height of the standard test table shall be 0,75 m.


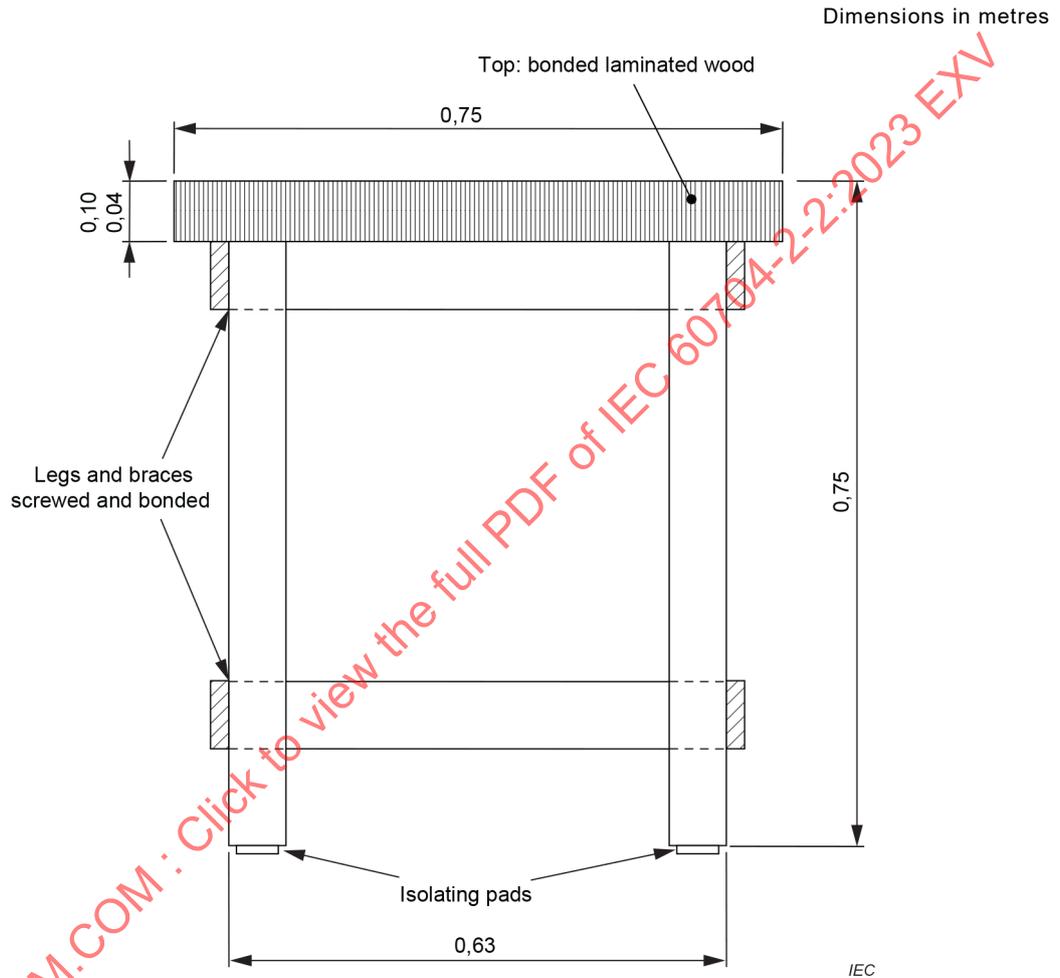


Figure A.1 – Example of standard test table

Annex B (normative)

Test enclosure

The test enclosure is shown in Figure B.1.

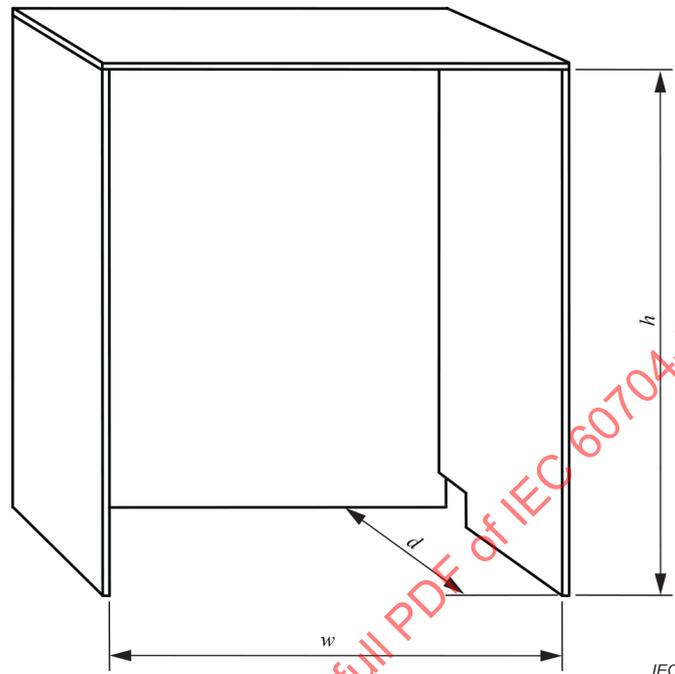

h is the inner height of the test enclosure $h = h_n + (3 \pm 1) \text{ mm}$

where

the nominal height, h_n , is the smallest integer multiple of 5 mm that accommodates the height of the installation opening in accordance with the manufacturer's installation instructions; calculated by:

$$h_n = i \cdot 5 \text{ mm with } i \cdot 5 \text{ mm} \geq z > (i - 1) \cdot 5 \text{ mm}, i = 1, 2, 3, \dots; \text{ where}$$

z is the height of the installation opening given in the manufacturer's installation instructions. If a range is given, z shall be the smallest value of the range.

w is the inner width of the test enclosure $w = w_n + (5 \pm 1) \text{ mm}$

where

the nominal width, w_n , is the smallest integer multiple of 5 mm that accommodates the width of the installation opening in accordance with the manufacturer's installation instructions; calculated by:

$$w_n = i \cdot 5 \text{ mm with } i \cdot 5 \text{ mm} \geq x > (i - 1) \cdot 5 \text{ mm}, i = 1, 2, 3, \dots; \text{ where}$$

x is the width of the installation opening given in the manufacturer's installation instructions. If a range is given, x shall be the smallest value of the range.

d is the inner depth of the test enclosure $d = d_n + (35 \pm 15) \text{ mm}$ (i.e. $d \geq 550 \text{ mm}$)

where

the nominal depth, d_n , is the smallest integer multiple of 5 mm, equal to or greater than 515 mm, that accommodates the depth of the installation opening in accordance with the manufacturer's installation instructions; calculated by:

$$d_n = i \cdot 5 \text{ mm with } i \cdot 5 \text{ mm} \geq y > (i - 1) \cdot 5 \text{ mm}, i = 1, 2, 3, \dots; \text{ where}$$

y is the depth of the installation opening given in the manufacturer's installation instructions. If a range is given, y shall be the smallest value of the range.

NOTE 1 The addition offers the laboratory personal the possibility to centre the appliance in the enclosure and ensures that the appliance does not contact the test enclosure.

NOTE 2 The front of the appliance is aligned parallel.

Material of the enclosure: $(19 \pm 1) \text{ mm}$ thick untreated particleboard (chipboard) or untreated plywood, having a density between 600 kg/m^3 and 750 kg/m^3 .

Figure B.1 – Test enclosure

Annex C (informative)

Guidelines for the design of simple test rooms with essentially free field conditions

The inner volume and the dimensions of the test room with essentially free field conditions depend on the size and the shape of the measurement surface used in the test. The measurement surface shall be at least 0,9 m distant from the absorptive surfaces of the test room

The floor of the test room shall be a hard, smooth, plane where the average sound absorption coefficient shall not exceed 0,06 over the 1/3 octave-band centre frequency range 100 Hz to 10 000 Hz. Usually, floors of painted poured concrete, or floors with asphalt or ceramic tiles, are satisfactory. If the floor is not a ground plane or integral with the building structure with adequate thickness, care shall be exercised that it does not radiate any appreciable sound due to vibrations.

The applicability of the test room for the purpose of this test code depends essentially on the quality of the acoustical treatment of its walls and ceiling.

A common treatment, consisting of wedges of absorptive material mounted (with a small airgap behind them) on the walls and on the ceiling of the building structure, will be extremely expensive, can be easily damaged in practical use, and will be hard to keep clean.

A very simple treatment consists of three layers of mineral wool (felt), each layer with a thickness of at least 80 mm, with different densities, the first layer being in contact with the building structure and having a density of approximately 55 kg/m³, the second layer having a density of approximately 33 kg/m³ and the third layer, forming the inner boundary of the test room, having a density of approximately 23 kg/m³.

The three layers are fastened together to the walls and to the ceiling of the building structure by a mesh with a size of approximately 50 mm of galvanized steel wires with a diameter of approximately 1 mm.

This treatment is not expensive, the risk of damage is small, and the room can be cleaned easily.

Bibliography

IEC 60038:2009, *IEC standard voltages*

ISO 3741:2010, *Acoustics – Determination of sound power levels of noise sources using sound pressure – Precision methods for reverberation rooms*

ISO 3745:2012, *Acoustics – Determination of sound power levels of noise sources using sound pressure – Precision method for anechoic and hemi-anechoic rooms*

ISO 3745:2012/AMD:2017

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

[IECNORM.COM](https://www.iecnorm.com) : Click to view the full PDF of IEC 60704-2-2:2023 EXV

INTERNATIONAL STANDARD

NORME INTERNATIONALE

**Household and similar electrical appliances – Test code for the determination of airborne acoustical noise –
Part 2-2: Particular requirements for fan heaters**

**Appareils électrodomestiques et analogues – Code d'essai pour la détermination du bruit aérien –
Partie 2-2: Exigences particulières pour les appareils de chauffage soufflants**

CONTENTS

FOREWORD.....	3
INTRODUCTION.....	5
1 Scope.....	6
2 Normative references	6
3 Terms and definitions	6
4 Measurement methods and acoustical environments	6
5 Instrumentation.....	7
6 Operation and location of appliances under test	8
7 Measurement of sound pressure levels.....	10
8 Calculation of sound pressure and of sound power levels	10
9 Information to be recorded.....	10
10 Information to be reported	11
Annexes	12
Bibliography.....	13
Table 1 – Standard deviations of sound power levels.....	7
Table 2 – Standard deviations for declaration and verification.....	7

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

INTERNATIONAL ELECTROTECHNICAL COMMISSION

**HOUSEHOLD AND SIMILAR ELECTRICAL APPLIANCES –
TEST CODE FOR THE DETERMINATION OF
AIRBORNE ACOUSTICAL NOISE –****Part 2-2: Particular requirements for fan heaters**

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) IEC draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). IEC takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, IEC had not received notice of (a) patent(s), which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at <https://patents.iec.ch>. IEC shall not be held responsible for identifying any or all such patent rights.

IEC 60704-2-2 has been prepared by subcommittee 59C: Electrical heating appliances for household and similar purposes, of IEC technical committee 59: Performance of household and similar electrical appliances. It is an International Standard.

This third edition cancels and replaces the second edition published in 2009. This edition constitutes a technical revision.

This edition includes the following significant technical changes with respect to the previous edition:

- alignment with the latest edition of IEC 60704-1:2021,
- addition of several ISO standards,
- revision of built-in-conditions,
- addition of requirements on climatic conditions and on background noise.

The text of this International Standard is based on the following documents:

Draft	Report on voting
59C/284/CDV	59C/286/RVC

Full information on the voting for its approval can be found in the report on voting indicated in the above table.

The language used for the development of this International Standard is English.

This part 2-2 is intended to be used in conjunction with the fourth edition of IEC 60704-1:2021, *Household and similar electrical appliances – Test code for the determination of airborne acoustical noise – Part 1: General requirements*.

The relevant text of IEC 60704-1:2021 as amended by this publication establishes the test code for fan heaters.

This part 2-2 supplements or modifies the corresponding clauses in IEC 60704-1:2021.

When a particular subclause of IEC 60704-1:2021 is not mentioned in this part 2-2, that subclause applies as far as reasonable. Where this standard states "addition", "modification" or "replacement", the relevant requirement, test specifications or explanatory matter in IEC 60704-1:2021 shall be adapted accordingly.

Subclauses or figures which are additional to those in IEC 60704-1:2021 are numbered starting from 101.

Additional annexes are lettered AA, BB, etc.

This document was drafted in accordance with ISO/IEC Directives, Part 2, and developed in accordance with ISO/IEC Directives, Part 1 and ISO/IEC Directives, IEC Supplement, available at www.iec.ch/members_experts/refdocs. The main document types developed by IEC are described in greater detail at www.iec.ch/publications.

A list of all the parts in the IEC 60704 series, under the general title *Household and similar electrical appliances – Test code for the determination of airborne acoustical noise*, can be found on the IEC website.

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under webstore.iec.ch in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn, or
- revised.

INTRODUCTION

The measuring conditions specified in this part 2-2 provide for sufficient accuracy in determining the noise emitted and comparing the results of measurements taken by different laboratories, whilst simulating as far as possible the practical use of fan heaters.

It is recommended to consider the determination of noise levels as part of a comprehensive testing procedure covering many aspects of the properties and performance of fan heaters.

NOTE As stated in the introduction to IEC 60704-1, this test code is concerned with airborne noise only.

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

HOUSEHOLD AND SIMILAR ELECTRICAL APPLIANCES – TEST CODE FOR THE DETERMINATION OF AIRBORNE ACOUSTICAL NOISE –

Part 2-2: Particular requirements for fan heaters

1 Scope

Replacement:

This part of IEC 60704 applies to electric fan heaters, designed for placing on the floor, table or counter, etc., or for mounting.

This document does not apply to

- electric storage room heaters;
- room humidifiers;
- room dehumidifiers;
- air cleaners;
- heaters designed exclusively for industrial purposes.

For determining and verifying noise emission values declared in product specifications, refer to IEC 60704-3:2019.

2 Normative references

This clause of IEC 60704-1:2021 is applicable.

3 Terms and definitions

This clause of IEC 60704-1:2021 is applicable.

4 Measurement methods and acoustical environments

This clause IEC 60704-1:2021 is applicable except as follows:

4.2 Direct method

Addition:

NOTE If pure tone components are present in the noise emitted, proper precautions need to be taken as specified in ISO 3743-2.

4.3 Comparison method

Addition:

NOTE If pure tone components are present in the noise emitted, proper precautions need to be taken as specified in ISO 3743-1 and 3743-2.

4.4 Acoustical environments

4.4.1 General requirements and criterion for adequacy of the test environment

Replacement:

ISO 3743-1, ISO 3743-2 and ISO 3744 can be used for measuring noise emitted by fan heaters.

The method specified in ISO 3744 is applicable to noise sources of any size. When applying ISO 3743-1 and ISO 3743-2, care shall be taken that the maximum size of the appliance under test fulfils the requirements specified in ISO 3743-1:2010, 1.3 and ISO 3743-2.

4.5 Measurement uncertainties

4.5.2 Standard deviations on repeatability and reproducibility and standard deviations related to declaration and verification

Replacement:

The estimated values of standard deviations of sound power levels determined according to this document are given in Table 1:

Table 1 – Standard deviations of sound power levels

Standard deviation dB	
σ_r (repeatability)	σ_R (reproducibility)
0,4	1,0

For the purpose of determining and verifying declared noise emission values according to IEC 60704-3, the values given in Table 2 apply:

Table 2 – Standard deviations for declaration and verification

Standard deviation dB		
σ_P (production)	σ_t (total)	σ_M (reference)
0,3 to 1,1	1,0 to 1,6	1,5

5 Instrumentation

This clause of IEC 60704-1:2021 is applicable except as follows:

5.1 Instrumentation for measuring acoustical data

Addition:

Windscreens should be used and the relevant corrections for changes in the microphone sensitivity shall be added to the observed sound pressure levels.

6 Operation and location of appliances under test

This clause of IEC 60704-1:2021 is applicable except as follows:

6.1 Equipping and pre-conditioning of appliances

6.1.1 *Addition:*

Air filters, if any, shall be clean.

6.1.3 *Replacement:*

Prior to noise measurements, the appliance, equipped in accordance with 6.1.1, shall have been in operation for a total period of at least 2 h for running-in at the highest speed setting with the maximum heating switched on for normal permanent use.

Oscillating function if available shall be switched on.

During the running-in procedure, air filters, if any, shall be removed, if possible. If filters remain in the appliances during this running-in period, they shall be cleaned or renewed after this period.

6.1.4 *Replacement:*

Immediately before each series of noise measurements, the appliance equipped in accordance with 6.1.1 shall be operated for stabilizing at the highest speed setting and maximum heating switched on for normal permanent use for 5 min.

6.2 Supply of electric energy and of water or gas

6.2.1 *Modification:*

The voltage tolerance shall be $\pm 0,5$ %.

6.2.2 Not applicable.

6.2.3 *Replacement:*

The appliance shall be operated with the heating elements switched on.

Special attention is required to be given to the possible effect of the temperature rise on the acoustical behaviour of the test room.

6.2.4 Not applicable.

6.4 Loading and operating of appliances during tests

6.4.2 *Replacement:*

The appliance shall be equipped according to 6.1.1.

The noise emission shall be determined with the appliance at the highest speed setting and maximum heating for normal permanent use. Oscillating function, if any, shall be switched on.

NOTE Other possible speed settings (minimum heat output, boost position, etc.) can be measured in addition. The respective noise levels need to be linked to the relevant heat output.

Appropriate adjustment of air intake or exhaust openings shall be done taking into account manufacturer's instructions if any, or otherwise selecting the configuration that gives the highest noise emission.

6.4.3 Not applicable.

6.5 Location and mounting of appliances

6.5.2 Addition:

The tests under the conditions stated in 6.5.4 shall be repeated for floor-standing appliances which may be placed either against or away from the wall.

For such appliances, both sets of results shall be recorded and the measurement that gives highest noise is then chosen.

6.5.3 Not applicable.

6.5.4 Replacement:

For measurements on floor-standing appliances intended for placing against a wall, including those for building-in into a cabinet, a vertical reflecting plane having an acoustic absorption coefficient of less than 0,06 shall be used.

When measurements are made in a reverberation test room, a part of the wall of the room will serve for this purpose. The minimum area of this part of the wall should be determined by the projection of the appliance extended by at least 0,5 m upwards and to both sides. The minimum distance between any surface of the appliance or its cabinet and the nearest corner of the room shall be 1 m.

When measurements are made in a free-field environment, the size of the vertical reflecting plane (supported by the horizontal reflecting plane) shall be at least equal to the size of the projection of the measurement surface.

For both types of test environment, the following requirements shall be complied with:

- the appliance shall be placed in the test environment without any resilient means of support other than those incorporated in the appliance;
- care should be taken to avoid any direct contact between the appliance (including protruding parts, worktops, spacers, etc.) and the vertical reflecting wall;
- the distance between the wall and the appliance shall be established by placing the appliance in direct contact with the wall and moving it away for a distance not exceeding $10\text{ cm} \pm 1\text{ cm}$.

6.5.5 Modification:

The height of the lowest edge of the appliance from the floor shall be $25\text{ cm} \pm 1\text{ cm}$.

NOTE For appliances intended for mounting close to the ceiling with the air stream directed towards the floor, measurements problems can be caused when the appliance is mounted as specified in 6.5.5. It can be necessary to mount such an appliance in an inverted position, with the top of the appliance facing towards the floor at a height of 0,25 m, or at the distance specified by the manufacturer for mounting close to the ceiling. The manufacturer's approval needs to be obtained before operating the appliance under the proposed test conditions.

6.5.6 Modification:

Built-in heaters such as plinth heaters shall be installed according to manufacturer's instructions.

7 Measurement of sound pressure levels

This clause of IEC 60704-1:2021 is applicable except as follows:

7.1 Microphone array, measurement surface and RSS location for essentially freefield conditions over reflecting plane(s)

Addition:

During measurements, care shall be taken to prevent direct blowing to the microphones.

7.1.4 Not applicable.

7.1.6 to 7.1.7 Not applicable.

7.4 Measurements

7.4.1 *Addition:*

The time-averaged A-weighted sound pressure levels shall be measured during at least 30 s and including complete cycles (at least two cycles) of the oscillating function, if any.

The frequency range of interest for sound power determination on fan heaters includes at least the octave bands with centre frequencies from 63 Hz to 8 000 Hz.

NOTE 2 In many cases, the 63 Hz octave band level does not participate significantly to the A-weighted level.

NOTE 3 When measuring this 63 Hz octave band, a special attention needs to be paid to the room effect.

7.4.4 Not applicable.

8 Calculation of sound pressure and of sound power levels

This clause of IEC 60704-1:2021 is applicable.

9 Information to be recorded

This clause of IEC 60704-1:2021 is applicable except as follows:

9.7 Electric supply, water supply, etc.

9.7.2 to 9.7.4 Not applicable.

9.12 Measurement data

9.12.5 Not applicable.

10 Information to be reported

This clause of IEC 60704-1:2021 is applicable except as follows:

10.3 Test conditions for the appliance

10.3.3 to 10.3.5 Not applicable.

10.3.11 Not applicable.

10.4 Acoustical data

10.4.10 Not applicable.

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

Annexes

The annexes of IEC 60704-1:2021 are applicable.

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

Bibliography

The Bibliography of IEC 60704-1:2021 is applicable.

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

SOMMAIRE

AVANT-PROPOS	15
INTRODUCTION.....	17
1 Domaine d'application	18
2 Références normatives	18
3 Termes et définitions	18
4 Méthodes de mesure et environnements acoustiques	18
5 Appareillage	19
6 Fonctionnement et emplacement des appareils en essai	20
7 Mesure des niveaux de pression acoustique.....	22
8 Calcul des niveaux de pression acoustique et de puissance acoustique	22
9 Informations à relever.....	22
10 Informations à consigner	23
Annexes	24
Bibliographie.....	25
Tableau 1 – Écarts-types des niveaux de puissance acoustique	19
Tableau 2 – Écarts-types pour la déclaration et la vérification.....	19

IECNORM.COM : Click to view the full PDF of IEC 60704-2-2:2023 EXV

COMMISSION ÉLECTROTECHNIQUE INTERNATIONALE

**APPAREILS ÉLECTRODOMESTIQUES ET ANALOGUES –
CODE D'ESSAI POUR LA DÉTERMINATION DU BRUIT AÉRIEN –****Partie 2-2: Exigences particulières pour
les appareils de chauffage soufflants**

AVANT-PROPOS

- 1) La Commission Électrotechnique Internationale (IEC) est une organisation mondiale de normalisation composée de l'ensemble des comités électrotechniques nationaux (Comités nationaux de l'IEC). L'IEC a pour objet de favoriser la coopération internationale pour toutes les questions de normalisation dans les domaines de l'électricité et de l'électronique. À cet effet, l'IEC – entre autres activités – publie des Normes internationales, des Spécifications techniques, des Rapports techniques, des Spécifications accessibles au public (PAS) et des Guides (ci-après dénommés "Publication(s) de l'IEC"). Leur élaboration est confiée à des comités d'études, aux travaux desquels tout Comité national intéressé par le sujet traité peut participer. Les organisations internationales, gouvernementales et non gouvernementales, en liaison avec l'IEC, participent également aux travaux. L'IEC collabore étroitement avec l'Organisation Internationale de Normalisation (ISO), selon des conditions fixées par accord entre les deux organisations.
- 2) Les décisions ou accords officiels de l'IEC concernant les questions techniques représentent, dans la mesure du possible, un accord international sur les sujets étudiés, étant donné que les Comités nationaux de l'IEC intéressés sont représentés dans chaque comité d'études.
- 3) Les Publications de l'IEC se présentent sous la forme de recommandations internationales et sont agréées comme telles par les Comités nationaux de l'IEC. Tous les efforts raisonnables sont entrepris afin que l'IEC s'assure de l'exactitude du contenu technique de ses publications; l'IEC ne peut pas être tenue responsable de l'éventuelle mauvaise utilisation ou interprétation qui en est faite par un quelconque utilisateur final.
- 4) Dans le but d'encourager l'uniformité internationale, les Comités nationaux de l'IEC s'engagent, dans toute la mesure possible, à appliquer de façon transparente les Publications de l'IEC dans leurs publications nationales et régionales. Toutes divergences entre toutes Publications de l'IEC et toutes publications nationales ou régionales correspondantes doivent être indiquées en termes clairs dans ces dernières.
- 5) L'IEC elle-même ne fournit aucune attestation de conformité. Des organismes de certification indépendants fournissent des services d'évaluation de conformité et, dans certains secteurs, accèdent aux marques de conformité de l'IEC. L'IEC n'est responsable d'aucun des services effectués par les organismes de certification indépendants.
- 6) Tous les utilisateurs doivent s'assurer qu'ils sont en possession de la dernière édition de cette publication.
- 7) Aucune responsabilité ne doit être imputée à l'IEC, à ses administrateurs, employés, auxiliaires ou mandataires, y compris ses experts particuliers et les membres de ses comités d'études et des Comités nationaux de l'IEC, pour tout préjudice causé en cas de dommages corporels et matériels, ou de tout autre dommage de quelque nature que ce soit, directe ou indirecte, ou pour supporter les coûts (y compris les frais de justice) et les dépenses découlant de la publication ou de l'utilisation de cette Publication de l'IEC ou de toute autre Publication de l'IEC, ou au crédit qui lui est accordé.
- 8) L'attention est attirée sur les références normatives citées dans cette publication. L'utilisation de publications référencées est obligatoire pour une application correcte de la présente publication.
- 9) L'IEC attire l'attention sur le fait que la mise en application du présent document peut entraîner l'utilisation d'un ou de plusieurs brevets. L'IEC ne prend pas position quant à la preuve, à la validité et à l'applicabilité de tout droit de brevet revendiqué à cet égard. À la date de publication du présent document, l'IEC n'a pas reçu notification qu'un ou plusieurs brevets pouvaient être nécessaires à sa mise en application. Toutefois, il y a lieu d'avertir les responsables de la mise en application du présent document que des informations plus récentes sont susceptibles de figurer dans la base de données de brevets, disponible à l'adresse <https://patents.iec.ch>. L'IEC ne saurait être tenue pour responsable de ne pas avoir identifié de tels droits de brevets.

L'IEC 60704-2-2 a été établie par le sous-comité 59C: Appareils de chauffage électrique à usage domestique et similaire, du comité d'études 59 de l'IEC: Aptitude à la fonction des appareils électrodomestiques et analogues. Il s'agit d'une Norme internationale.

Cette troisième édition annule et remplace la deuxième édition parue en 2009. Cette édition constitue une révision technique.