

# INTERNATIONAL STANDARD



**Semiconductor devices –  
Part 18-2: Semiconductor bio sensors – Evaluation process of lens-free  
CMOS photonic array sensor package modules**

IECNORM.COM : Click to view the PDF of IEC 60747-18-2:2020



**THIS PUBLICATION IS COPYRIGHT PROTECTED**  
**Copyright © 2020 IEC, Geneva, Switzerland**

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Central Office  
3, rue de Varembe  
CH-1211 Geneva 20  
Switzerland

Tel.: +41 22 919 02 11  
[info@iec.ch](mailto:info@iec.ch)  
[www.iec.ch](http://www.iec.ch)

**About the IEC**

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

**About IEC publications**

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

**IEC publications search - [webstore.iec.ch/advsearchform](http://webstore.iec.ch/advsearchform)**

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

**IEC Just Published - [webstore.iec.ch/justpublished](http://webstore.iec.ch/justpublished)**

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

**IEC Customer Service Centre - [webstore.iec.ch/csc](http://webstore.iec.ch/csc)**

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: [sales@iec.ch](mailto:sales@iec.ch).

**Electropedia - [www.electropedia.org](http://www.electropedia.org)**

The world's leading online dictionary on electrotechnology, containing more than 22 000 terminological entries in English and French, with equivalent terms in 16 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

**IEC Glossary - [std.iec.ch/glossary](http://std.iec.ch/glossary)**

67 000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR.

IECNORM.COM : Click to view the IEC Standard IEC 60377-102:2020

# INTERNATIONAL STANDARD



---

**Semiconductor devices –  
Part 18-2: Semiconductor bio sensors – Evaluation process of lens-free  
CMOS photonic array sensor package modules**

INTERNATIONAL  
ELECTROTECHNICAL  
COMMISSION

---

ICS 31.080.01

ISBN 978-2-8322-7803-1

**Warning! Make sure that you obtained this publication from an authorized distributor.**

## CONTENTS

FOREWORD.....	3
INTRODUCTION.....	5
1 Scope.....	6
2 Normative references .....	6
3 Terms and definitions .....	6
4 Measurement setup .....	7
4.1 General.....	7
4.2 Measurement system.....	7
5 Measurement.....	9
5.1 General.....	9
5.2 Measurement in the standard condition.....	11
5.2.1 General .....	11
5.2.2 A: Sensor characteristics .....	11
5.2.3 B: Spatial uniformity of user light .....	12
5.2.4 C: Middle layer effect under collimated light.....	13
5.2.5 D: Middle layer effect under user light.....	14
5.2.6 E: Middle layer effect under first and second user light.....	15
5.3 Measurement in general condition .....	16
5.3.1 D1: First user light condition .....	16
5.3.2 E1: First and second user light condition .....	17
5.4 Reference for establishing the representative output value in the effective area .....	17
5.5 Various wavelengths( $\lambda$ ) of light .....	17
6 Test report.....	17
Bibliography.....	18
Figure 1 – Example of lens-free CMOS photonic array sensor package modules .....	7
Figure 2 – Example of measurement system with incident parallel light.....	8
Figure 3 – Example of photoelectric measurement schematics.....	9
Figure 4 – Test and calibration flow diagram.....	10
Figure 5 – Test and calibration flow schematics .....	10
Figure 6 – Example of measurement for sensor characteristics.....	12
Figure 7 – Example of measurement for spatial uniformity of user light.....	13
Figure 8 – Example of measurement for middle layer effect under collimated light .....	14
Figure 9 – Example of measurement for middle layer effect under user light .....	15
Figure 10 – Example of measurement for middle layer effect under first and second user light.....	16

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

## SEMICONDUCTOR DEVICES –

**Part 18-2: Semiconductor bio sensors – Evaluation process of lens-free CMOS photonic array sensor package modules**

## FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 60747-18-2 has been prepared by subcommittee 47E: Discrete semiconductor devices, of IEC technical committee 47: Semiconductor devices.

The text of this International Standard is based on the following documents:

FDIS	Report on voting
47E/689/FDIS	47E/694/RVD

Full information on the voting for the approval of this International Standard can be found in the report on voting indicated in the above table.

This document has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts of the IEC 60747 series, published under the general title *Semiconductor devices*, can be found on the IEC website.

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

**IMPORTANT – The 'colour inside' logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this document using a colour printer.**

IECNORM.COM : Click to view the full PDF of IEC 60747-18-2:2020

## INTRODUCTION

The IEC 60747-18 series on semiconductor bio sensors is composed of the following parts:

- IEC 60747-18-1 defines the test method and data analysis for calibration of lens-free CMOS photonic array sensors
- IEC 60747-18-2 defines the evaluation process of lens-free CMOS photonic array sensor package modules
- IEC 60747-18-3 defines the fluid flow characteristics of lens-free CMOS photonic array sensor package modules with fluidic system

The IEC 60747-18 series includes subjects such as noise analysis, long-term reliability tests, test methods for lens-free CMOS photonic array sensor package modules under patchable environments, test methods under implantable environments, etc.

The International Electrotechnical Commission (IEC) draws attention to the fact that it is claimed that compliance with this document may involve the use of patents given in several subclauses as indicated in the table below. These patents are held by their respective inventors under license to SOL Inc.:

KR1020150187389	[SOL]	The method of calibration of packaged photonic sensor pixel array by evaluating its characteristic	Subclause 5.2.1, 5.2.2
PCT/KR2016/006109	[SOL]	METHOD FOR CORRECTING OPTICAL SENSOR ARRAY MODULE THROUGH CHARACTERISTIC EVALUATION	Subclause 5.2.3, 5.2.4, 5.2.5
US15/577586	[SOL]		
JP2017562062	[SOL]		

IEC takes no position concerning the evidence, validity and scope of this patent right.

The holder of this patent right has assured the IEC that he/she is willing to negotiate licences under reasonable and non-discriminatory terms and conditions with applicants throughout the world. In this respect, the statement of the holder of this patent right is registered with IEC. Information may be obtained from:

SOL Inc.  
H Business Park  
C1010, 26, Beobwon-ro 9-gil, SongPa-Gu  
Seoul 05838  
Republic of Korea

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights other than those identified above. IEC shall not be held responsible for identifying any or all such patent rights.

ISO ([www.iso.org/patents](http://www.iso.org/patents)) and IEC (<http://patents.iec.ch>) maintain on-line data bases of patents relevant to their standards. Users are encouraged to consult the data bases for the most up to date information concerning patents.

## SEMICONDUCTOR DEVICES –

### Part 18-2: Semiconductor bio sensors – Evaluation process of lens-free CMOS photonic array sensor package modules

#### 1 Scope

This part of IEC 60747 specifies the evaluation process of lens-free CMOS photonic array sensor package modules. This document includes the measurement environment of each process, statistical analysis of test data, middle layer effect under various user light, evaluation of calibrated lens-free CMOS photonic array sensor package modules, and test report.

#### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60747-18-1:2019, *Semiconductor devices – Part 18-1: Semiconductor bio sensors – Test method and data analysis for calibration of lens-free CMOS photonic array sensors*

#### 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

##### 3.1

##### **lens-free CMOS photonic array sensor package modules**

device composed of a lens-free CMOS photonic array sensor, middle layer, user light (first light source, second light source) and its own dark box

SEE: Figure 1.

Note 1 to entry: Lens-free CMOS photonic array sensors are extensively utilized in bio-diagnostic devices, healthcare devices, lens-free microscopes, and patchable/implantable medical devices.

Note 2 to entry: The sensing environments of such a lens-free CMOS photonic array sensors are typically different from those of general-purpose image sensors which are normally mounted with an external lens in module housings.

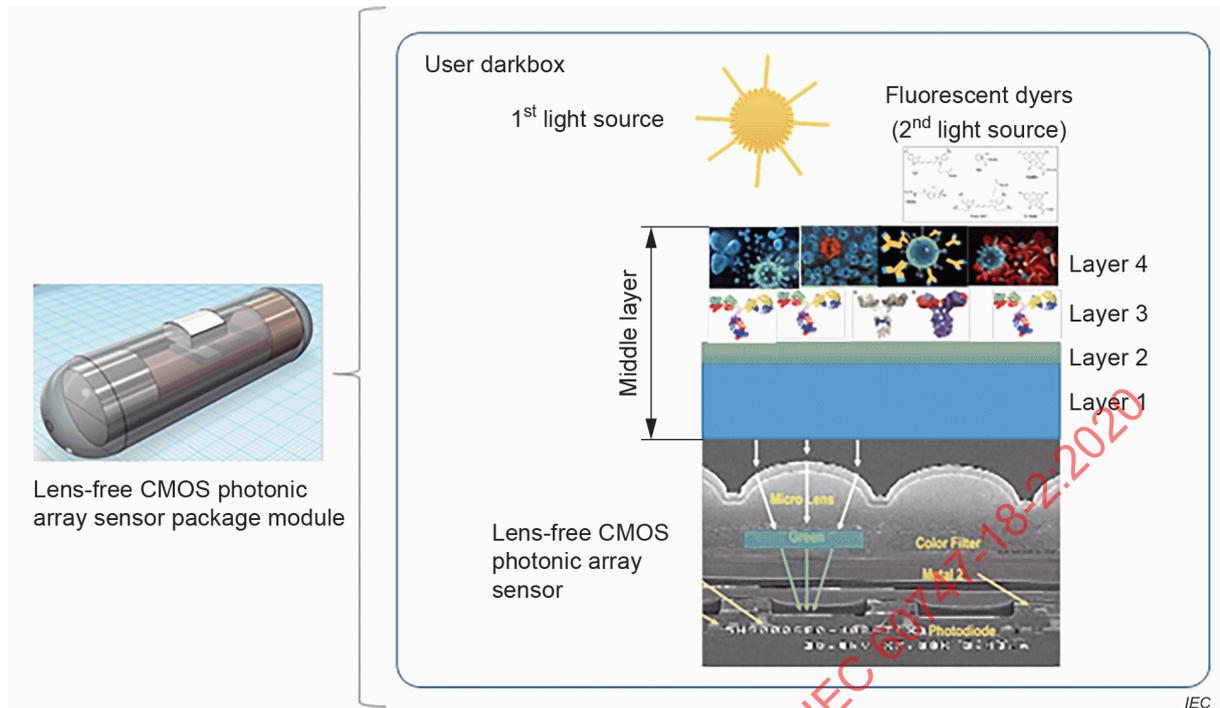


Figure 1 – Example of lens-free CMOS photonic array sensor package modules

### 3.2 photonic responsivity

ratio of the output electric signal of a sensor to the input light power

Note 1 to entry: It is in general a function of wavelength and of incident power.

Note 2 to entry: Photonic responsivity as a function of wavelength is referred to as spectral responsivity.

Note 3 to entry: Units for output electric signal are V, A, or DN.

### 3.3 linearity

ability of a pixel of an array sensor to provide an output having a linear relationship with an input light power

[SOURCE: IEC 60747-18-1:2019, 3.3].


## 4 Measurement setup

### 4.1 General

The lens-free CMOS photonic array sensor package modules can include a middle layer, user light sources as shown in Figure 1 to be evaluated at each step for a more precise calibration.

### 4.2 Measurement system

All measurements shall be performed under the standard conditions, according to 4.2 of IEC 60747-18-1:2019, as shown in Figure 2 and Figure 3. All items mentioned in 4.2 of IEC 60747-18-1:2019 shall also be defined.

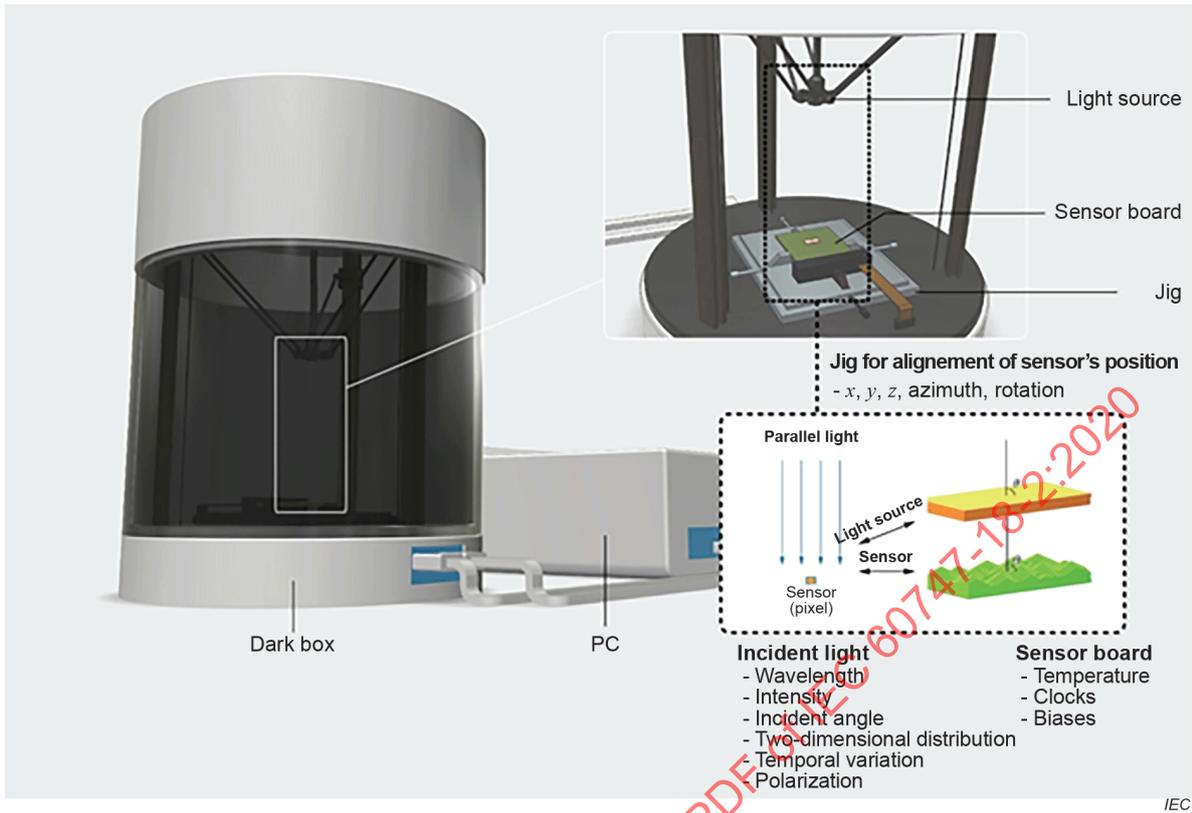

**Figure 2 – Example of measurement system with incident parallel light**

The photoelectric characteristics of a sensor board shall be measured using the system shown in Figure 3 by each step of the structure component of the package modules.

IECNORM.COM : Click to view the full PDF file IEC 60747-18-2:2020

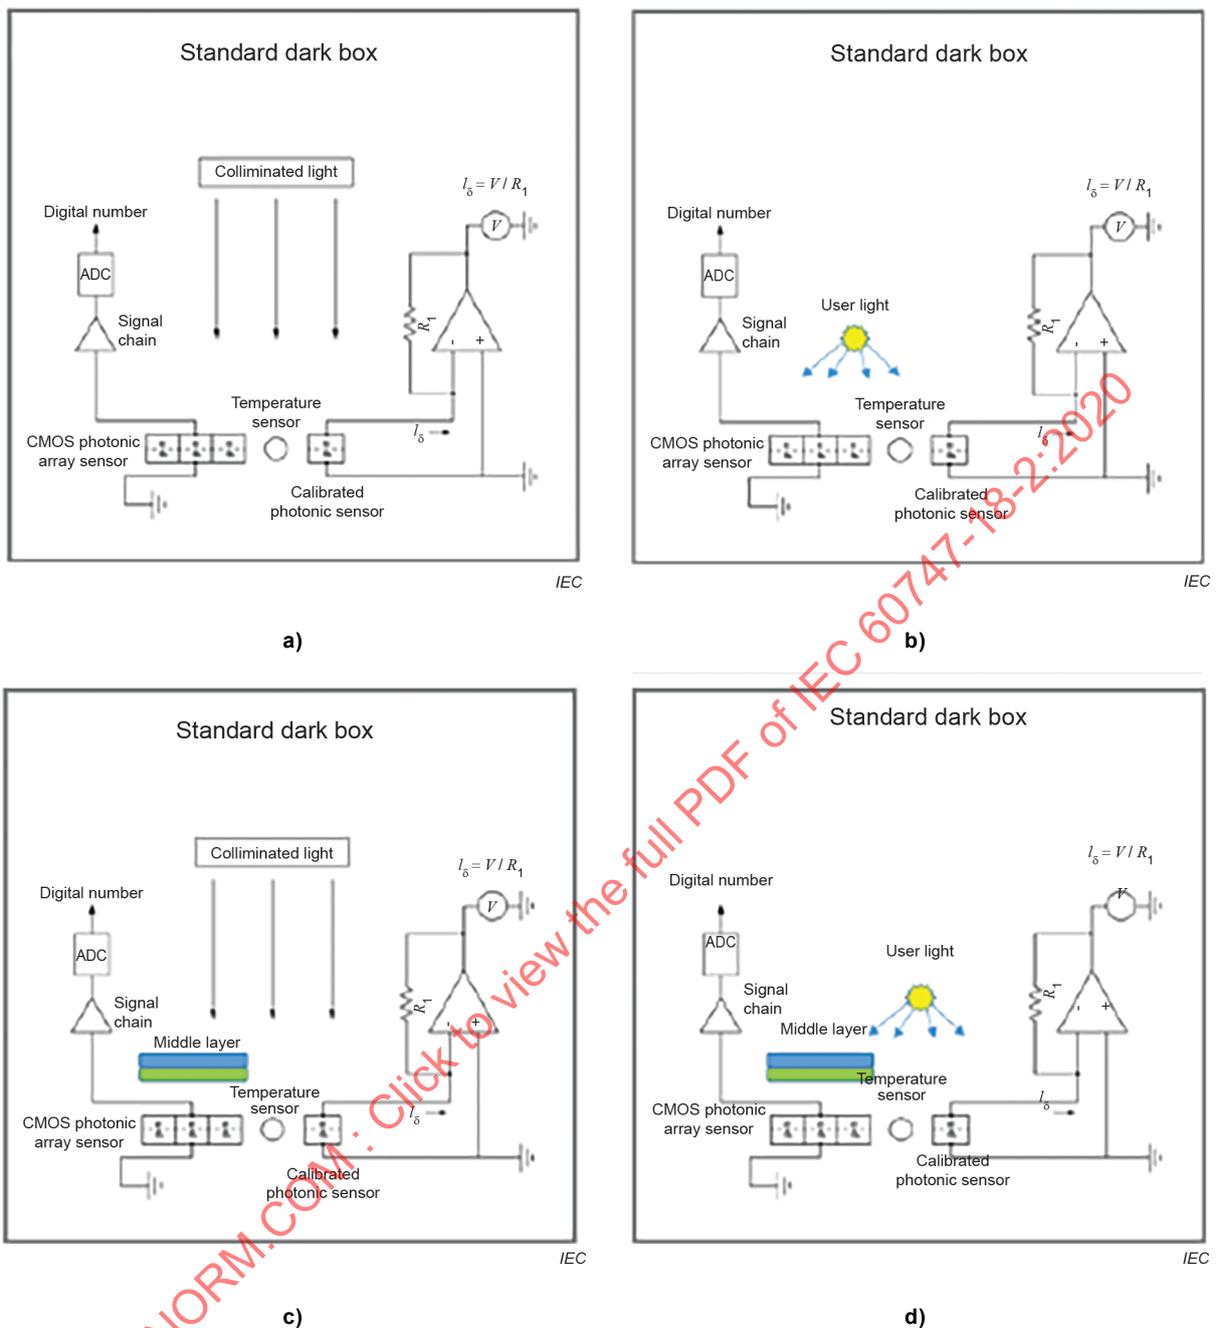



Figure 3 – Example of photoelectric measurement schematics

## 5 Measurement

### 5.1 General


All results shall include the accuracy information of the test performed and the information of the measurement system used for the product. The parameters defined in the product specifications shall be tested according to the procedure described in the test and calibration flow in Figure 4 and Figure 5.

The configurations in 4.2 shall be set up prior to the measurement of the lens-free CMOS photonic array sensor package modules. To ensure the best results, the key parameters (temperature change, wavelength, incident angle, etc.), which can affect the sensor characteristics and the measurement, shall be rechecked and managed properly. In other words, the factors which can affect the characteristic values of the sensors such as the ambient temperature, the condition of the incident light and the sensor board, etc. shall be checked and the corresponding configurations set up accordingly.

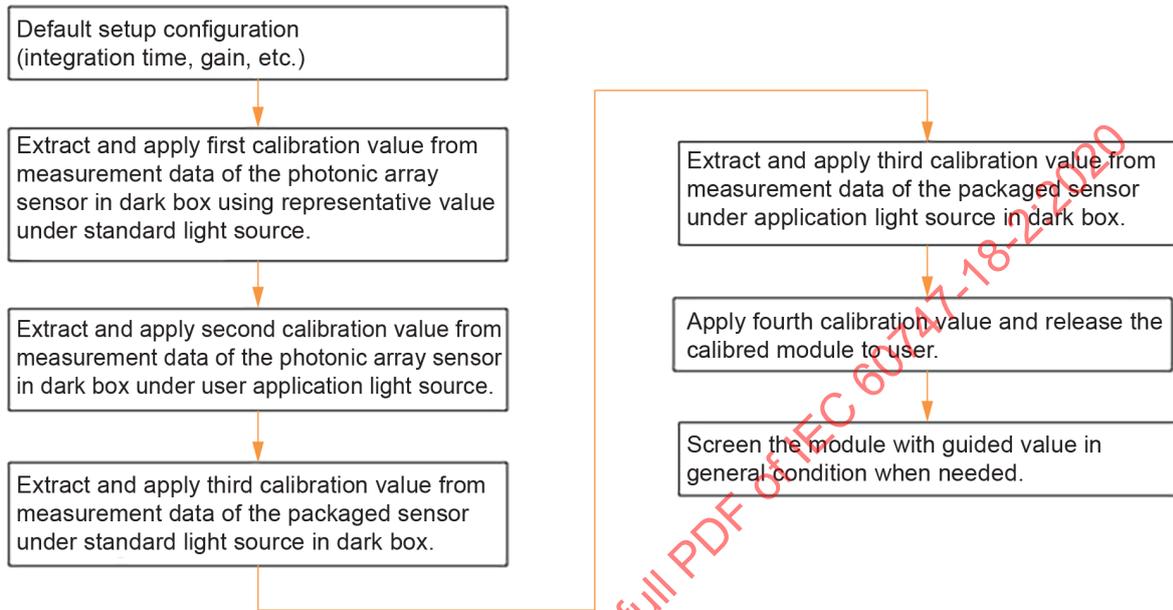

IEC

Figure 4 – Test and calibration flow diagram

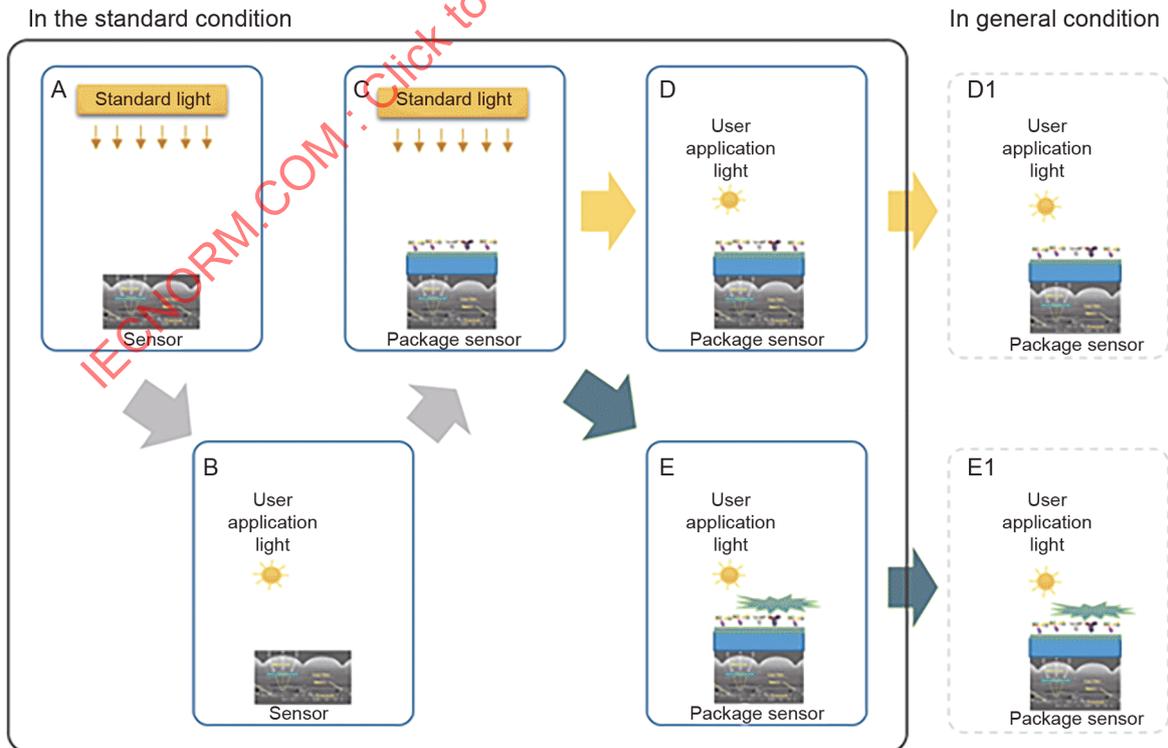

IEC

Figure 5 – Test and calibration flow schematics

## 5.2 Measurement in the standard condition

### 5.2.1 General

All tests shall be performed under well certified and defined conditions to avoid any external disturbances.

### 5.2.2 A: Sensor characteristics

#### 5.2.2.1 General

The purpose of this step is to test the sensor characteristics (planarization and linearity) in the standard condition. For example, the measurement for the sensor characteristics is performed as shown in Figure 3a) and Figure 6.

#### 5.2.2.2 Measurement

##### 5.2.2.2.1 Planarization

The frame measurement shall be performed according to 5.2.1 of IEC 60747-18-1:2019.

##### 5.2.2.2.2 Linearity

The frame measurement shall be performed according to 5.2.2 of IEC 60747-18-1:2019.

#### 5.2.2.3 Data analysis

##### 5.2.2.3.1 Planarization


The reference pixel shall be determined according to 6.2.1 of IEC 60747-18-1:2019. The lookup table of the representative value corresponding to each pixel shall be made according to 6.2.2 of IEC 60747-18-1:2019. The lookup table (Lookup table\_A\_RVP) shall be included in the test report.

##### 5.2.2.3.2 Linearity

Light intensity effective area for linearity shall be determined according to 6.3 of IEC 60747-18-1:2019. The lookup table of light intensity effective area for linearity shall be written in test report. The lookup table (Lookup table\_A\_RVL) shall also be included in the test report.

##### 5.2.2.4 Calibration

A calibration lookup table shall be created using the lookup table\_A\_RVP in 5.2.2.3.1 and the lookup table\_A\_RVL in 5.2.2.3.2 according to Table 1 of IEC 60747-18-1:2019. The calibration lookup table (Lookup table\_A\_CAL) shall also be included in the test report.

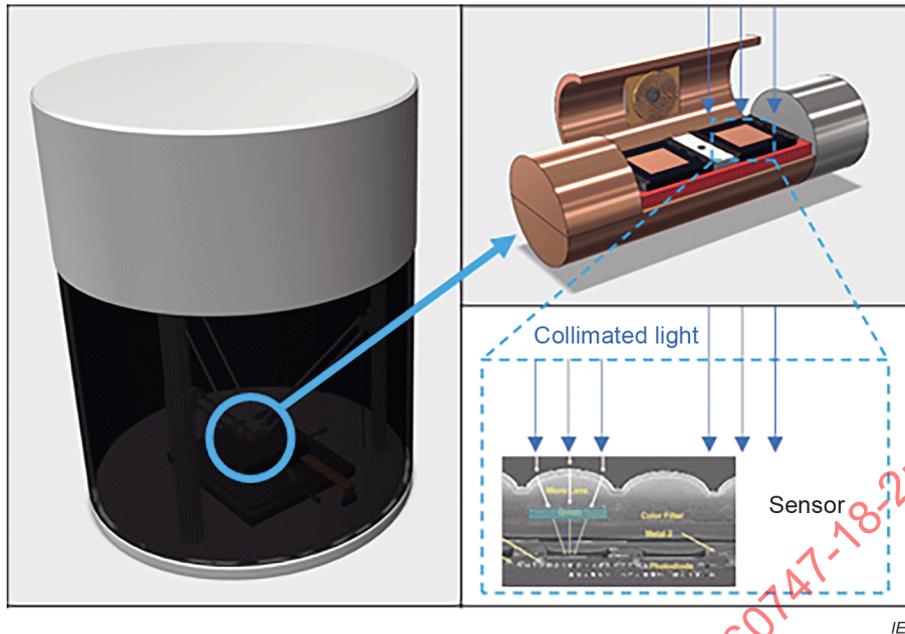

**Figure 6 – Example of measurement for sensor characteristics**

**5.2.3 B: Spatial uniformity of user light**

**5.2.3.1 General**

The purpose of this step is to test the spatial uniformity of the photonic responsivity of the pixel by the incident user light at each pixel. Based on the characteristics of the user light, the mounting position, the angle of the user light and the spatial non-uniformity of the surface shall be measured. The calibration table of the imbalance of the light source shall be created, comparing the sensor data. The measurement is performed as shown in Figure 3b) and Figure 7.

**5.2.3.2 Measurement**

**5.2.3.2.1 Planarization**

The frame measurement shall be performed according to 5.2.1 of IEC 60747-18-1:2019.

**5.2.3.2.2 Linearity**

The frame measurement shall be performed according to 5.2.2 of IEC 60747-18-1:2019.

**5.2.3.3 Data analysis**

**5.2.3.3.1 Planarization**

The reference pixel shall be determined according to 6.2.1 of IEC 60747-18-1:2019. The lookup table of the representative value corresponding to each pixel shall be created according to 6.2.2 of IEC 60747-18-1:2019. The lookup table (Lookup table\_B\_RVP) shall be included in the test report.

**5.2.3.3.2 Linearity**

The light intensity's effective area for linearity shall be determined according to 6.3 of IEC 60747-18-1:2019. The light intensity's effective area for linearity shall be written in the test report. The lookup table (Lookup table\_B\_RVL) shall also be included in the test report.

### 5.2.3.4 Calibration

A calibration lookup table shall be created using the lookup table\_B\_RVP in 5.2.3.3.1 and the lookup table\_B\_RVL in 5.2.3.3.2 according to Table 1 of IEC 60747-18-1:2019. The calibration lookup table (Lookup table\_B\_CAL) shall also be included in the test report.

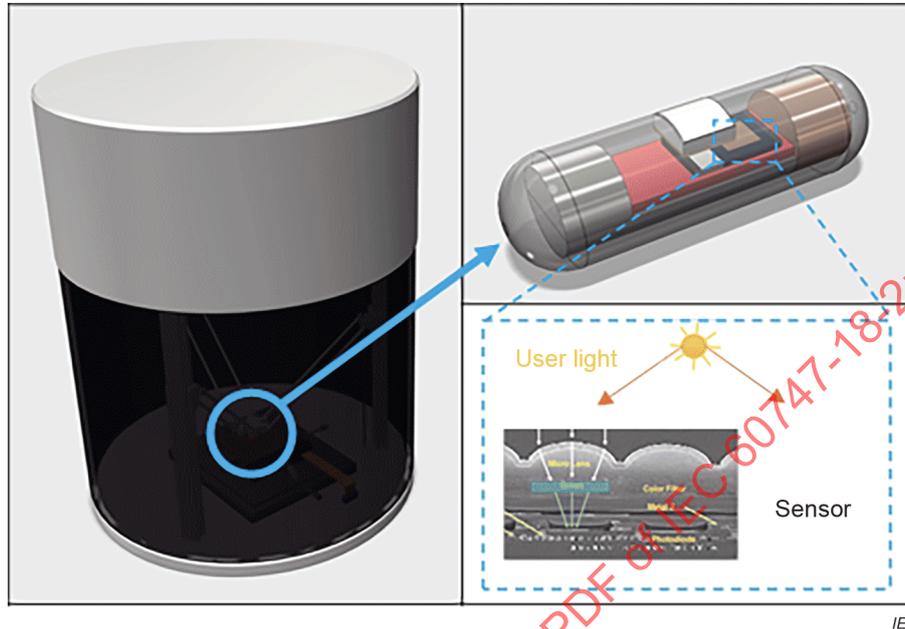


Figure 7 – Example of measurement for spatial uniformity of user light

## 5.2.4 C: Middle layer effect under collimated light

### 5.2.4.1 General

The purpose of this step is to test the effect of the middle layer on the sensor characteristics under collimated light. A calibration table measuring the degree of deformation during the exposure time (the time the light arrives to the sensor) shall be created by using the middle-layer number, characteristics, thickness, density and composition, etc. For example, the measurement is performed as shown in Figure 3c) and Figure 8.

### 5.2.4.2 Measurement

#### 5.2.4.2.1 Planarization

The frame measurement shall be performed according to 5.2.1 of IEC 60747-18-1:2019.

#### 5.2.4.2.2 Linearity

The frame measurement shall be performed according to 5.2.2 of IEC 60747-18-1:2019.

### 5.2.4.3 Data analysis

#### 5.2.4.3.1 Planarization


The reference pixel shall be determined according to 6.2.1 of IEC 60747-18-1:2019. The lookup table of the representative value corresponding to each pixel shall be created according to 6.2.2 of IEC 60747-18-1:2019. The lookup table (Lookup table\_C\_RVP) shall be included in the test report.

**5.2.4.3.2 Linearity**

The light intensity's effective area for linearity shall be determined according to 6.3 of IEC 60747-18-1:2019. The light intensity's effective area for linearity shall be included in the test report. The lookup table (Lookup table\_C\_RVL) shall also be included in the test report.

**5.2.4.4 Calibration**

A calibration lookup table shall be created using the lookup table\_C\_RVP in 5.2.4.3.1 and the lookup table\_C\_RVL in 5.2.4.3.2 according to Table 1 IEC 60747-18-1:2019. The calibration lookup table (Lookup table\_C\_CAL) shall also be included in the test report.

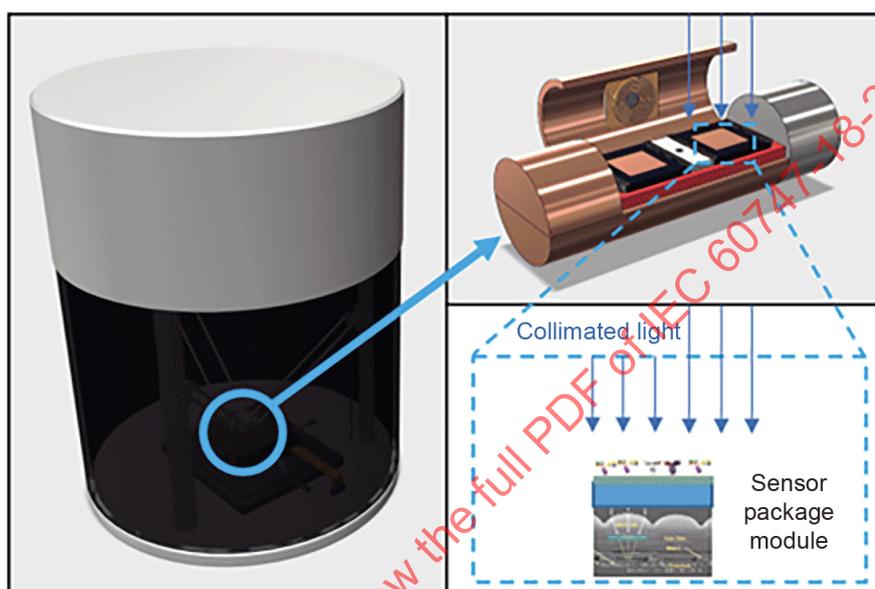

IEC

**Figure 8 – Example of measurement for middle layer effect under collimated light**

**5.2.5 D: Middle layer effect under user light**

**5.2.5.1 General**

The purpose of this step is to test the effect of the middle layer on the sensor characteristics under user light. A calibration table shall be created by measuring the binding imbalance caused by the user light source and middle layer. For example, measurement is performed as shown in Figure 3d) and Figure 9.

**5.2.5.2 Measurement**

**5.2.5.2.1 Planarization**

The frame measurement shall be performed according to 5.2.1 of IEC 60747-18-1:2019.

**5.2.5.2.2 Linearity**

The frame measurement shall be performed according to 5.2.2 of IEC 60747-18-1:2019.

### 5.2.5.3 Data analysis

#### 5.2.5.3.1 Planarization


The reference pixel shall be determined according to 6.2.1 of IEC 60747-18-1:2019. The lookup table of the representative value corresponding to each pixel shall be created according to 6.2.2 of IEC 60747-18-1:2019. The lookup table (Lookup table\_D\_RVP) shall be included in the test report.

#### 5.2.5.3.2 Linearity

The light intensity's effective area for linearity shall be determined according to 6.3 of IEC 60747-18-1:2019. The light intensity's effective area for linearity shall be included in the test report. The lookup table (Lookup table\_D\_RVL) shall also be included in the test report.

#### 5.2.5.4 Calibration

A calibration lookup table shall be created using the lookup table\_D\_RVP in 5.2.5.3.1 and the lookup table\_D\_RVL in 5.2.5.3.2 according to Table 1 of IEC 60747-18-1:2019. The calibration lookup table (Lookup table\_D\_CAL) shall also be included in the test report.

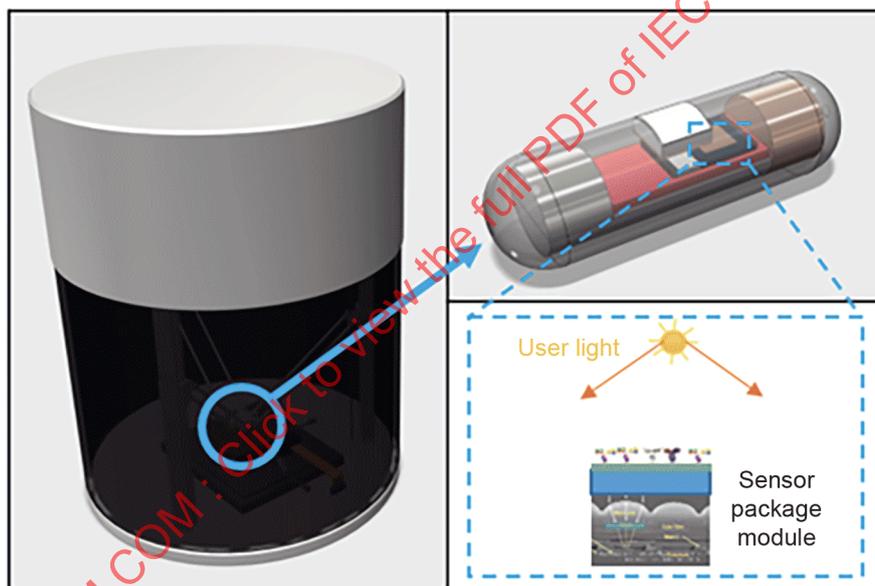

IEC

Figure 9 – Example of measurement for middle layer effect under user light

### 5.2.6 E: Middle layer effect under first and second user light

#### 5.2.6.1 General

The purpose of this step is to test the effect of the middle layer on the sensor characteristics under the first and second user light. In case the second light source emits light relying on user light, as there are two different light sources with different wavelength and incident angle, the calibration table shall be created by evaluating the characteristics of the second light source. For example, measurement is performed as shown in Figure 10.

#### 5.2.6.2 Measurement

##### 5.2.6.2.1 Planarization

The frame measurement shall be performed according to 5.2.1 of IEC 60747-18-1:2019.