

INTERNATIONAL STANDARD

IEC 61675-2

1998

AMENDMENT 1
2004-12

Amendment 1

**Radionuclide imaging devices –
Characteristics and test conditions –**

**Part 2:
Single photon emission computed tomographs**

© IEC 2004 Droits de reproduction réservés — Copyright - all rights reserved

International Electrotechnical Commission, 3, rue de Varembe, PO Box 131, CH-1211 Geneva 20, Switzerland
Telephone: +41 22 919 02 11 Telefax: +41 22 919 03 00 E-mail: inmail@iec.ch Web: www.iec.ch



Commission Electrotechnique Internationale
International Electrotechnical Commission
Международная Электротехническая Комиссия

PRICE CODE

U

For price, see current catalogue

FOREWORD

This amendment has been prepared by subcommittee 62C: Equipment for radiotherapy, nuclear medicine and radiation dosimetry, of IEC technical committee 62: Electrical equipment in medical practice.

The text of this amendment is based on the following documents:

FDIS	Report on voting
62C/378/FDIS	62C/379/RVD

Full information on the voting for the approval of this amendment can be found in the report on voting indicated in the above table.

The committee has decided that the contents of this amendment and the base publication will remain unchanged until the maintenance result date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

Introduction to this amendment

Since this International Standard was first published in 1998, further developments of single photon computer tomographs allow some of the tomographs to be operated in coincidence detection mode as well. To comply with this trend, this amendment describes test conditions in concordance with the test methods established for dedicated PET systems.

Page 2

CONTENTS

Add the title of new subclause 3.7 as follows:

3.7 Test methods for single photon computer tomographs operated in coincidence detection mode

Add the titles of new Figures 8 to 13 as follows:

- 8 Phantom insert with hollow spheres
- 9 Cross-section of body phantom
- 10 Arm phantom
- 11 Phantom configuration for COUNT RATE measurements according to 3.7.5.3.1.2
- 12 Scheme of the evaluation of COUNT LOSS correction
- 13 Phantom insert for the evaluation of ATTENUATION correction

Page 4

1.1 Scope and object

Add, after the first paragraph, the following new text:

This part of IEC 61675-2 also specifies test conditions for declaring the characteristics of single photon computer tomographs operated in coincidence mode as well as in single photon mode.

The test methods specified for coincidence mode are based on the test methods for dedicated PET tomographs as described in IEC 61675-1 to reflect as well as possible the clinical use of coincidence detection. Tests have been modified to reflect the limited sensitivity and COUNT RATE CHARACTERISTICS of the single photon computer tomographs operated in coincidence detection mode only when needed.

2 Terminology and definitions

Replace the first sentence by the following:

For the purposes of this part of IEC 61675 the definitions given in IEC 60788, IEC 60789 and IEC 61675-1 (some of which are repeated in this clause) and the following definitions apply.

Add, at the end of this clause, on page 9, the following new definitions:

2.10

POSITRON EMISSION TOMOGRAPHY

PET

emission computed tomography utilizing the annihilation radiation of positron emitting radionuclides by coincidence detection.

[IEC 61675-1, definition 2.1.3]

2.10.1

POSITRON EMISSION TOMOGRAPH

tomographic device, which detects the annihilation radiation of positron emitting radionuclides by coincidence detection.

[IEC 61675-1, definition 2.1.3.1]

2.10.2

ANNIHILATION RADIATION

IONIZING RADIATION that is produced when a particle and its antiparticle interact and cease to exist

[IEC 61675-1, definition 2.1.3.2]

2.10.3

LINE OF RESPONSE

LOR

axis of the PROJECTION BEAM

NOTE In PET, it is the line connecting the centres of two opposing detector elements operated in coincidence

[IEC 61675-1, definition 2.1.3.5]

2.10.4**TOTAL COINCIDENCES**

sum of all coincidences detected

[IEC 61675-1, definition 2.1.3.6]

2.10.4.1**TRUE COINCIDENCE**

result of COINCIDENCE DETECTION of two gamma events originating from the same positron annihilation

[IEC 61675-1, definition 2.1.3.6.1]

2.10.4.2**SCATTERED TRUE COINCIDENCE**

TRUE COINCIDENCE where at least one participating PHOTON was scattered before the COINCIDENCE DETECTION

[IEC 61675-1, definition 2.1.3.6.2]

2.10.4.3**UNSCATTERED TRUE COINCIDENCES**

difference between true coincidences and scattered true coincidences

[IEC 61675-1, definition 2.1.3.6.3]

2.10.4.4**RANDOM COINCIDENCE**

result of COINCIDENCE DETECTION in which both participating PHOTONS emerge from different positron annihilations

[IEC 61675-1, definition 2.1.3.6.4]

2.10.5**SINGLES RATE**

COUNT RATE measured without COINCIDENCE DETECTION, but with energy discrimination

[IEC 61675-1, definition 2.1.3.7]

2.10.6**TWO-DIMENSIONAL RECONSTRUCTION**

in TWO-DIMENSIONAL RECONSTRUCTION, the data are rebinned prior to reconstruction into sinograms, which are the PROJECTION data of transverse slices, which are considered being independent of each other and being perpendicular to the SYSTEM AXIS. So, each event will be assigned, in the axial direction, to that transverse slice passing the midpoint of the corresponding LINE OF RESPONSE. Any deviation from perpendicular to the SYSTEM AXIS is neglected. The data are then reconstructed by two-dimensional methods, i.e. each slice is reconstructed from its associated sinogram, independent of the rest of the data set

NOTE This is the STANDARD method of reconstruction for POSITRON EMISSION TOMOGRAPHS using small axial acceptance angles, i.e. utilizing septa. For POSITRON EMISSION TOMOGRAPHS using large axial acceptance angles, i.e. without septa, this method is also called "single slice rebinning".

[IEC 61675-1, definition 2.1.4.1]

2.10.7**THREE-DIMENSIONAL RECONSTRUCTION**

in THREE-DIMENSIONAL RECONSTRUCTION, the LINES OF RESPONSE are not restricted to being perpendicular to the SYSTEM AXIS. So, a LINE OF RESPONSE may pass several transverse slices. Consequently, transverse slices cannot be reconstructed independent of each other. Each slice has to be reconstructed utilizing the full three-dimensional data set

[IEC 61675-1, definition 2.1.4.2]

2.11**RECOVERY COEFFICIENT**

measured (image) ACTIVITY concentration of an active volume divided by the true ACTIVITY concentration of that volume, neglecting ACTIVITY CALIBRATION FACTORS

NOTE For the actual measurement, the true ACTIVITY concentration is replaced by the measured ACTIVITY concentration in a large volume.

[IEC 61675-1, definition 2.5]

2.12**NORMALIZED SLICE SENSITIVITY**

slice sensitivity divided by the axial slice width (EW) for that slice

[IEC 61675-1, definition 2.6.1.1]

2.12.1**COUNT RATE CHARACTERISTIC**

function giving the relationship between observed COUNT RATE and TRUE COUNT RATE

[IEC 60788, definition rm-34-21]

2.12.2**COUNT LOSS**

difference between measured COUNT RATE and TRUE COUNT RATE, which is caused by the finite RESOLVING TIME of the instrument

[IEC 61675-1, definition 2.7.1]

2.12.3**ADDRESS PILE UP**

<GAMMA CAMERA> false address calculation of an artificial event which passes the ENERGY WINDOW, but is formed from two or more events by the PILE UP EFFECT

[IEC 61675-1, definition 2.7.4, modified]

2.12.4**RADIOACTIVE SOURCE**

quantity of radioactive material having both an ACTIVITY and a specific ACTIVITY above specific levels

[IEC 60788, definition rm-20-02]

3 Test methods

Add, on page 15, the following subclauses:

3.7 Test methods for single photon computer tomographs operated in coincidence detection mode

For all measurements, the tomograph shall be set up according to its normal mode of operation, i.e. it shall not be adjusted specially for the measurement of specific parameters. If the tomograph is specified to operate in different modes influencing the performance parameters, for example with different energy windows, different axial acceptance angles, with and without septa, with TWO-DIMENSIONAL RECONSTRUCTION and THREE-DIMENSIONAL RECONSTRUCTION, the test results shall be reported in addition. The tomographic configuration (e.g. energy thresholds, axial acceptance angle, reconstruction algorithm, radius of rotation, configuration of heads) shall be chosen according to the manufacturer's recommendation and clearly stated.

If any test cannot be carried out exactly as specified in this standard, the reason for the deviation and the exact conditions under which the test was performed shall be stated clearly.

The test phantoms shall be centred within the tomograph's AXIAL FIELD OF VIEW, if not specified otherwise.

Single photon computer tomographs operated in coincidence mode must also conform to all planar and SPECT tests (e.g. 3.1 to 3.6).

NOTE For tomographs with an AXIAL FIELD OF VIEW greater than 16,5 cm, this centring will only produce performance estimates for the central part. However, if the phantoms were displaced axially in order to cover the entire AXIAL FIELD OF VIEW, false results could be obtained for the central planes, if the axial acceptance angle of the detectors was not fully covered with ACTIVITY.

3.7.1 SPATIAL RESOLUTION

3.7.1.1 General

SPATIAL RESOLUTION measurements are used to estimate the ability of a tomograph to reproduce the spatial distribution of a tracer in an object in a reconstructed image. The measurement is performed by imaging POINT (or LINE) SOURCES in air and reconstructing images using a sharp reconstruction filter. Although this does not represent the condition of imaging a patient, where tissue scatter is present and limited statistics require the use of a smooth reconstruction filter, the measured SPATIAL RESOLUTION provides a best-case comparison between tomographs, indicating the highest achievable performance.

3.7.1.2 Purpose

The purpose of this measurement is to characterize the ability of the tomograph to recover small objects by characterizing the width of the reconstructed TRANSVERSE POINT SPREAD FUNCTIONS of radioactive POINT SOURCES or of extended LINE SOURCES placed perpendicular to the direction of measurement. The width of the spread function is measured by the FULL WIDTH AT HALF MAXIMUM (FWHM) and the EQUIVALENT WIDTH (EW).

To define how well objects can be reproduced in the axial direction, the AXIAL SLICE WIDTH (commonly referred to as the slice thickness) is used. It is measured with a POINT SOURCE, which is stepped through the tomograph's TRANSVERSE FIELD OF VIEW axially in small increments and is characterized by the EW and the FWHM of the AXIAL POINT SPREAD FUNCTION for each individual slice.

The AXIAL RESOLUTION is defined for tomographs with sufficiently fine axial sampling (volume detectors) and could be measured with a stationary POINT SOURCE. For these systems the AXIAL RESOLUTION (EW and FWHM) is equivalent to the AXIAL SLICE WIDTH. These systems (fulfilling the sampling theorem in the axial direction) are characterized by the fact that the AXIAL POINT SPREAD FUNCTION of a stationary POINT SOURCE would not vary if the position of the source were varied in the axial direction for half the axial sampling distance.

3.7.1.3 Method

3.7.1.3.1 General

For all systems, the SPATIAL RESOLUTION shall be measured in the transverse IMAGE PLANE in two directions (i.e. radially and tangentially). In addition, for those systems having sufficiently fine axial sampling, an AXIAL RESOLUTION also shall be measured.

The TRANSVERSE FIELD OF VIEW and the IMAGE MATRIX size determine the PIXEL size in the transverse IMAGE PLANE. In order to measure accurately the width of the spread function, its FWHM should span at least ten PIXELS. A typical imaging study of a brain, however, requires a 260 mm TRANSVERSE FIELD OF VIEW, which together with a 128 x 128 IMAGE MATRIX and 6 mm SPATIAL RESOLUTION, results in a FWHM of only three PIXELS. The width of the response may be incorrect if there are fewer than ten PIXELS in the FWHM. Therefore, if possible, the PIXEL size should be made close to one-tenth of the expected FWHM during reconstruction and should be indicated as ancillary data for the TRANSVERSE RESOLUTION measurement. For volume imaging systems, the TRIXEL size, in both the transverse and axial dimensions, should be made close to one-tenth the expected FWHM, and should be indicated as ancillary data for the SPATIAL RESOLUTION measurement. For all systems, the AXIAL SLICE WIDTH is measured by moving the source in fine steps to sample the response function adequately. For the AXIAL SLICE WIDTH measurement, the step size should be close to one-tenth the expected EW. It is assumed that a computer-controlled bed will be used for accurate positioning of the RADIOACTIVE SOURCE.

3.7.1.3.2 RADIONUCLIDE

The RADIONUCLIDE for the measurement shall be ^{18}F , with an ACTIVITY such that the percent COUNT LOSS is less than 5 % and the RANDOM COINCIDENCE rate is less than 5 % of the TOTAL COINCIDENCE rate.

3.7.1.3.3 RADIOACTIVE SOURCE distribution

3.7.1.3.3.1 General

POINT SOURCES or LINE SOURCES, respectively, shall be used as described in 3.7.1.3.3.2 to 3.7.1.3.3.4.

3.7.1.3.3.2 TRANSVERSE RESOLUTION

Tomographs shall use LINE SOURCES, suspended in air to minimize scatter, for measurements of TRANSVERSE RESOLUTION. The sources shall be kept parallel to the long axis of the tomograph and shall be positioned radially at 100 mm intervals along Cartesian axes in a plane perpendicular to the long axis of the tomograph i.e. $r = 10 \text{ mm}, 100 \text{ mm}, 200 \text{ mm} \dots$ up to the edge of the TRANSVERSE FIELD OF VIEW. The last position shall be not more than 20 mm from the edge and shall be stated. Each of these positions yields two measurements of TRANSVERSE RESOLUTION, which shall be distinguished by being in the radial or tangential direction.

NOTE The SPATIAL RESOLUTION at $r = 0 \text{ mm}$ may yield artificial values due to sampling, so this measurement is done at the position $r = 10 \text{ mm}$.

3.7.1.3.3.3 AXIAL SLICE WIDTH

The AXIAL POINT SPREAD FUNCTION for POINT SOURCES suspended in air shall be measured for all systems. The POINT SOURCES shall be moved in fine increments along the axial direction over the length of the tomograph, at radial positions of $r = 0$ mm, 100 mm, ... in 100 mm steps up to the edge of the TRANSVERSE FIELD OF VIEW. The last position shall be not more than 20 mm from the edge and shall be stated. The source is stepped in the axial direction by one-tenth of the expected EW of the axial response function. For each radial position, the measured values shall be corrected for decay. This measurement does not apply to THREE-DIMENSIONAL RECONSTRUCTION.

3.7.1.3.3.4 AXIAL RESOLUTION

For systems having axial sampling at least three times smaller than the FWHM of the AXIAL POINT SPREAD FUNCTION the measurement of AXIAL RESOLUTION can be made with stationary POINT SOURCES. POINT SOURCES suspended in air are positioned at radial intervals of 100 mm, starting at the centre and extending to a distance which depends on the TRANSVERSE FIELD OF VIEW, as described in the measurement of AXIAL SLICE WIDTH (3.7.1.3.3.3). Each POINT SOURCE shall be imaged at axial intervals of ± 80 mm, starting at the centre of the tomograph and extending to within 20 mm from the edge of the AXIAL FIELD OF VIEW.

3.7.1.3.4 Data collection

Data shall be collected for all sources in all of the positions specified above, either singly or in groups of multiple sources, to minimize the data acquisition time. At least 50 000 counts shall be acquired in each response function, as defined below.

3.7.1.3.5 Data processing

Reconstruction using a ramp filter with the cut-off at the Nyquist frequency of the PROJECTION data shall be employed for all SPATIAL RESOLUTION data.

3.7.1.4 Analysis

The RADIAL RESOLUTION and the TANGENTIAL RESOLUTION shall be determined by forming one-dimensional response functions, which result from taking profiles through the TRANSVERSE POINT SPREAD FUNCTION in radial and tangential directions, passing through the peak of the distribution.

The AXIAL RESOLUTION of the POINT SOURCE measurements is determined by forming one-dimensional response functions (AXIAL POINT SPREAD FUNCTIONS), which result from taking profiles through the volume image in the axial direction, passing through the peak of the distribution in the slice nearest the source.

The AXIAL SLICE WIDTH is determined by forming one-dimensional response functions (AXIAL POINT SPREAD FUNCTIONS), which result from summing the counts per slice collected for each slice at each axial location of each radial source location.

Each FWHM shall be determined by linear interpolation between adjacent PIXELS at half the maximum PIXEL value, which is the peak of the response function (see Figure 6). Values shall be converted to millimetre units by multiplication with the appropriate PIXEL size.

Each EQUIVALENT WIDTH (EW) shall be measured from the corresponding response function.

EW is calculated from the formula

$$EW = \sum_i \frac{C_i \times PW}{C_m}$$

where

$\sum C_i$ is the sum of the counts in the profile between the limits defined by 1/20 cm on either side of the peak;

C_m is the maximum PIXEL value;

PW is the PIXEL width (or axial increment in the case of the AXIAL SLICE WIDTH) in millimetres (see Figure 7).

3.7.1.5 Report

RADIAL and TANGENTIAL RESOLUTIONS (FWHM and EW) for each radius, averaged over all slices, shall be calculated and reported as TRANSVERSE RESOLUTION VALUES. AXIAL SLICE WIDTHS (EW and FWHM) for each radius, averaged over all slices for each type (e.g. odd, even) shall be reported. Transverse PIXEL dimensions and axial step size shall also be reported.

For systems where AXIAL RESOLUTION is to be measured, AXIAL RESOLUTION (FWHM and EW), averaged over all slices, shall be reported. For these systems, the axial PIXEL dimension in millimetres shall also be reported.

For systems utilizing THREE-DIMENSIONAL RECONSTRUCTION, RESOLUTION data as listed above shall not be averaged. Graphs of TRANSVERSE RESOLUTION and AXIAL RESOLUTION shall be reported, showing the RESOLUTION values (RADIAL RESOLUTION, TANGENTIAL RESOLUTION, and AXIAL RESOLUTION) for each radius as a function of slice number.

3.7.2 RECOVERY COEFFICIENT

3.7.2.1 General

The finite RESOLUTION of a tomograph leads to a spreading of image counts beyond the geometrical boundaries of the object. This effect becomes more important as the object size decreases. The RECOVERY COEFFICIENT provides an assessment of the ability of the tomograph to quantify the ACTIVITY concentration as a function of the object size.

3.7.2.2 Purpose

The objective of the following procedures is to quantify the apparent decrease in tracer concentration in a region of interest (ROI) of an image of spherical sources of different diameters.

3.7.2.3 Method

A number of hollow spheres, filled with an ACTIVITY concentration of ^{18}F from a stock solution, are placed in the water-filled head phantom (see Figures 2 and 8), which is in turn placed in the centre of the TRANSVERSE FIELD OF VIEW. The phantom shall be held in position without introducing additional attenuating material. At least two samples from this solution are counted in a well counter. The spheres are arranged to be coplanar.

For systems utilizing THREE-DIMENSIONAL RECONSTRUCTION, the measurements shall be done at the axial centre of the tomograph and halfway between the axial centre and the edge of the AXIAL FIELD OF VIEW.

After data acquisition, the spheres are removed and the cylinder filled with a uniform solution of ^{18}F from which at least two samples are taken for well counting.

3.7.2.4 Data collection

The data collection shall be carried out at low COUNT RATES such that the COUNT LOSS is less than 5 % and the RANDOM COINCIDENCE rate is less than 5 % of the TOTAL COINCIDENCE rate.

Care should be taken to acquire sufficient counts so that statistical variations do not significantly affect the result. So, for the slice containing the spheres, at least 500 000 counts shall be acquired. COUNT RATES and scanning times shall be stated.

3.7.2.5 Data processing and analysis

Reconstruction shall be performed using a ramp filter with a cut-off at the Nyquist frequency and with all corrections applied. The method of ATTENUATION correction shall be by an analytical calculation. The ATTENUATION coefficient used shall be reported. The scatter correction method used shall be clearly described.

Circular ROIs of diameter as close as possible to the FWHM as measured in 3.7.1.3.3.3 are defined centrally on the image of each sphere. The precise ROI diameter should be stated.

A large ROI (diameter: 150 mm) is centred on the image of the uniform cylinder. Calculation of the RECOVERY COEFFICIENT (RC_{si}) for each sphere is obtained from the equation:

$$RC_{si} = \frac{\left(\frac{C_{si}}{SM_s} \right)}{\left(\frac{C_u}{SM_u} \right)}$$

where

- C_{si} are the ROI counts/pixel/s for sphere i ;
- SM_s are the sample counts/s/cm³ (stock solution spheres);
- C_u are the ROI counts/pixel/s (head phantom);
- SM_u are the sample counts/s/cm³ (head phantom);
- C_u/SM_u represents a calibration factor for a large reference object.

Care shall be taken to correct for any dead-time and sample volume effects in the well counter. RC_{si} is then plotted against sphere diameter to give recovery curves.

3.7.2.6 Report

Graphs of RECOVERY COEFFICIENTS for each axial position described in 3.7.2.3 shall be reported.

The scatter correction method used shall be clearly described, as well as the ATTENUATION coefficient used.

3.7.3 Tomographic sensitivity

3.7.3.1 General

Tomographic sensitivity is a parameter that characterizes the rate at which coincidence events are detected in the presence of a RADIOACTIVE SOURCE in the limit of low ACTIVITY where COUNT LOSSES and RANDOM COINCIDENCES are negligible. The measured rate of TRUE COINCIDENCE EVENTS for a given distribution of the RADIOACTIVE SOURCE depends upon many factors, including the detector material, size, and packing fraction, axial acceptance window and septa geometry, ATTENUATION, scatter, dead-time, and energy thresholds, radius of rotation and detector head geometry.

3.7.3.2 Purpose

The purpose of this measurement is to determine the detected rate of TRUE COINCIDENCE EVENTS per unit of ACTIVITY concentration for a standard volume source, i.e. a cylindrical phantom of given dimensions.

3.7.3.3 Method

The tomographic sensitivity test places a specified volume of radioactive solution of known ACTIVITY concentration in the TOTAL FIELD OF VIEW of the single photon computer tomograph operated in coincidence detection mode and observes the resulting COUNT RATE. The systems sensitivity is calculated from these values.

The test is critically dependent upon accurate assays of radioactivity as measured in a dose calibrator or well counter. It is difficult to maintain an absolute calibration with such devices to accuracies finer than 10 %. Absolute reference standards using positron emitters should be considered if higher degrees of accuracy are required.

3.7.3.3.1 RADIONUCLIDE

The RADIONUCLIDE used for these measurements shall be ^{18}F or ^{68}Ge . The amount of ACTIVITY used shall be such that the percentage of COUNT LOSSES is less than 5 % and the RANDOM COINCIDENCE rate is less than 5 % of the TOTAL COINCIDENCE rate.

3.7.3.3.2 RADIOACTIVE SOURCE distribution

The head phantom (Figure 2) shall be filled with a homogeneous solution of known ACTIVITY concentration. The phantom shall be held in position without introducing additional attenuating material. It shall be centred both axially and transaxially in the TOTAL FIELD OF VIEW.

3.7.3.3.3 Data collection

Each coincident event between individual detectors shall be taken into account only once. Data shall be assembled into SINOGRAMS. All events will be assigned to the transverse slice passing the midpoint of the corresponding LINE OF RESPONSE.

At least 20 000 counts shall be acquired for each slice within the lesser of the AXIAL FIELD OF VIEW or the central 16,5 cm where the phantom was placed.

3.7.3.3.4 Data processing

The ACTIVITY concentration in the phantom shall be corrected for decay to determine the average ACTIVITY concentration, a_{ave} , during the data acquisition time interval, T_{acq} , by the following equation:

$$a_{\text{ave}} = \frac{A_{\text{cal}}}{V} \frac{1}{\ln 2} \frac{T_{1/2}}{T_{\text{acq}}} \exp\left[\frac{T_{\text{cal}} - T_0}{T_{1/2}} \ln 2\right] \left[1 - \exp\left(-\frac{T_{\text{acq}}}{T_{1/2}} \ln 2\right)\right]$$

where

V is the volume of the phantom;

A_{cal} is the ACTIVITY times branching ratio ("positron activity") measured at time T_{cal} ;

T_0 is the acquisition start time;

$T_{1/2}$ is the half life of the RADIONUCLIDE.

It is not necessary to reconstruct these data. No corrections for detector normalization, COUNT LOSS, scatter, and ATTENUATION shall be applied. The data shall be corrected for RANDOM COINCIDENCES.

3.7.3.4 Analysis

The total counts, $C_{i,tot,120mm}$, on each slice i shall be obtained by summing all PIXELS in the corresponding SINOGRAM within a radius of 120 mm. The SLICE SENSITIVITY S_i for unscattered events shall be found by the following, taking into account that the acquisition time T_{acq} shall include the time required to move the detectors to collect a complete set of PROJECTIONS:

$$S_i = \frac{C_{i,tot,120mm}}{T_{acq}} \frac{1 - SF_i}{a_{ave}}$$

where SF_i is the corresponding SCATTER FRACTION (see 3.7.6).

The NORMALIZED SLICE SENSITIVITY for each slice nS_i shall be calculated as follows:

$$nS_i = \frac{S_i}{EW_{a,i}}$$

where $EW_{a,i}$ is the AXIAL SLICE WIDTH expressed as EW for slice i (see 3.7.1.4).

NOTE 1 The NORMALIZED SLICE SENSITIVITY allows for comparison of tomographs with different AXIAL SLICE WIDTH.

The VOLUME SENSITIVITY, S_{tot} , shall be the sum of S_i over all slices of the tomograph within the central 16,5 cm or the AXIAL FIELD OF VIEW, whichever is smaller.

NOTE 2 This will yield only the VOLUME SENSITIVITY for the central part of the tomograph, if the AXIAL FIELD OF VIEW is greater than 16,5 cm.

3.7.3.5 Report

For each slice i , tabulate the values of S_i and nS_i . The VOLUME SENSITIVITY S_{tot} shall also be reported.

3.7.4 Uniformity

No test has been specified to characterize the uniformity of reconstructed images, because all methods known so far will mostly reflect the noise in the image.

3.7.5 COUNT RATE CHARACTERISTIC

3.7.5.1 General

Coincidence COUNT RATE performance depends in a complex manner on the spatial distribution of ACTIVITY and scattering materials, which will be referred to as the different scatter conditions (see 3.7.5.3.1). The COUNT RATE CHARACTERISTIC of the TRUE COINCIDENCE COUNT RATE is highly dependent on the trues-to-singles ratio and on the COUNT RATE CHARACTERISTIC of the SINGLES RATE and consequently on the set-up of the measurement conditions, which therefore should simulate the range of clinical imaging situations. In addition, COUNT RATE performance is strongly influenced by the amount of RANDOM COINCIDENCES and by the accuracy of the subtraction of these events.

NOTE As the TRUE COINCIDENCE COUNT RATE includes scattered events, the relative SCATTER FRACTION must be considered when comparing tomographs with different design.

3.7.5.2 Purpose

The procedure described here is designed to evaluate deviations from the linear relationship between TRUE COINCIDENCE COUNT RATE and ACTIVITY, caused by COUNT LOSSES, and the evaluation of image distortions at high COUNT RATES, especially those leading to spatially misplaced events by ADDRESS PILE UP. As modern coincidence detection devices are operated with COUNT LOSS correction schemes, the accuracy of these correction algorithms is tested.

Coincidence COUNT RATE performance means:

- a) the relationship between measured TRUE COINCIDENCES (UNSCATTERED plus SCATTERED TRUE COINCIDENCES) and ACTIVITY, i.e. the COUNT RATE CHARACTERISTIC of TRUE COINCIDENCE COUNT RATE;
- b) a test to determine address errors caused by ADDRESS PILE UP;
- c) the evaluation of the accuracy of the COUNT LOSS correction scheme.

3.7.5.3 Method

For dedicated brain tomographs, only the scatter condition described in 3.7.5.3.1.1 applies, whereas for all other tomographs the scatter conditions described in 3.7.5.3.1.1 to 3.7.5.3.1.3 apply. For all tests the only correction to be applied is the subtraction of the multiple and the RANDOM COINCIDENCES (to calculate TRUE COINCIDENCE counts). No correction is made for COUNT LOSSES, ATTENUATION, and scatter, unless otherwise stated. The ACTIVITY shall generally be specified as the total amount of ACTIVITY within the phantom as specified in 3.7.5.3.1. As the variation of ACTIVITY is normally achieved by radioactive decay, care should be taken with respect to the radiochemical purity of the ACTIVITY used.

3.7.5.3.1 RADIOACTIVE SOURCE distribution

To describe various scatter conditions, three different experimental set-ups are to be used.

3.7.5.3.1.1 Head imaging

The head phantom (Figure 2) shall be filled homogeneously with ACTIVITY.

3.7.5.3.1.2 Cardiac imaging

The centre of the body phantom, Figure 9, (head phantom inserted) with outer section and arms (Figure 10) of the phantom filled with water, inner section (head phantom, Figure 2) filled with air, and a rod source (130 mm inside length x 21 mm inside diameter) containing the ACTIVITY and placed eccentrically as indicated in Figure 11 shall be centred to the SYSTEM AXIS, see Figures 9 and 11.

3.7.5.3.1.3 Abdominal imaging

The procedure described in 3.7.5.3.1.2 is followed but the head phantom is also filled with water. This configuration is used to mimic the worst-case scattering condition encountered in positron emission imaging.

3.7.5.4 Data acquisition and analysis

Each coincident event between individual detectors shall be taken into account only once.

3.7.5.4.1 Test of the TRUE COINCIDENCE COUNT RATE CHARACTERISTIC

For all scatter conditions, a COUNT RATE CHARACTERISTIC (measured TRUE COINCIDENCE COUNT RATE versus incident TRUE COINCIDENCE COUNT RATE or ACTIVITY within the TOTAL FIELD OF VIEW of the tomograph) shall be measured. The variation of ACTIVITY shall be accomplished by radioactive decay; ^{18}F or ^{11}C with continuous measurements over approximately 10 half lifes

can be used. The time per frame shall be less than one-half of the half life with the exception of the last three frames, which can be longer. The initial amount of ACTIVITY shall be chosen so that COUNT RATE saturation is exceeded, and the last frame shall be acquired with a COUNT LOSS of less than 1 %.

Data shall be assembled into SINOGRAMS. All events will be assigned to the transverse slice passing the midpoint of the corresponding LINE OF RESPONSE. The data to be inspected are for the TRANSVERSE FIELD OF VIEW restricted to 520 mm in diameter and without COUNT LOSS correction. For the sake of comparison with data published elsewhere, a second scale (kBq/cm³) shall be added to the abscissa for the scatter condition of 3.7.5.3.1.1.

The average of the decaying ACTIVITY, $A_{ave,i}$, during the data acquisition interval for time frame i , $T_{acq,i}$, shall be determined by the following equation, taking into account that $T_{acq,i}$ shall include the time required to rotate the detectors for a complete set of PROJECTIONS:

$$A_{ave,i} = A_{cal} \frac{1}{\ln 2} \frac{T_{1/2}}{T_{acq,i}} \exp \left[\frac{T_{cal} - T_{0,i}}{T_{1/2}} \ln 2 \right] \left[1 - \exp \left(- \frac{T_{acq,i}}{T_{1/2}} \ln 2 \right) \right]$$

where

A_{cal} is the ACTIVITY measured at time T_{cal} , corrected for branching ratio (see 3.7.3.3.4);

T_{0i} is the acquisition start-time of the time frame i ;

$T_{1/2}$ is the half life of ¹⁸F or ¹¹C, respectively.

From the above measurements, plot the COUNT RATE CHARACTERISTIC (e.g. measured TRUE COINCIDENCE COUNT RATE versus ACTIVITY) and the characteristic of the RANDOM COINCIDENCE rate (all data without ATTENUATION correction and normalization) for the total system (data for the TOTAL FIELD OF VIEW).

For the head phantom, the random rate shall be evaluated only for a circular region, with diameter of 24 cm, centred at the position of the phantom.

The conversion factor between ACTIVITY and TRUE COINCIDENCE COUNT RATE without COUNT LOSS shall be determined from each of the three frames with lowest ACTIVITY and averaged.

Care shall be taken to acquire enough counts in these frames to ensure sufficient statistical precision.

From the data set, for each slice and for the total system, determine the ACTIVITY at which the measured TRUE COINCIDENCE COUNT RATE reaches 20 % COUNT LOSS and plot these ACTIVITY levels versus slice number. Repeat this evaluation for 50 % COUNT LOSS. For the total system specify the measured TRUE COINCIDENCE COUNT RATE for 20 % COUNT LOSS and for 50 % COUNT LOSS.

From the data set measured (from the SINOGRAMS as described above when using TWO-DIMENSIONAL RECONSTRUCTION, from the full data set when using THREE-DIMENSIONAL RECONSTRUCTION) reconstruct a full set of slices for all time frames. For a region containing the ACTIVITY (21 mm in diameter for the rod source, 194 mm in diameter for the cylinder), plot ROI counts divided by measured TRUE COINCIDENCES for the whole slice versus ACTIVITY, as an indicator of image distortion at high COUNT RATES (ideally, this plot should yield a constant value).

3.7.5.4.2 Test of ADDRESS PILE UP

The ADDRESS PILE UP in the axial direction shall be checked from the set of reconstructed images according to 3.7.5.4.1. For a region just containing the source, calculate the ratio of ROI counts per slice at each COUNT RATE, normalized to the corresponding value at the lowest rate.

$$R_{i,j} = \frac{C_{i,j}}{C_{i,\text{low}}}$$

where

$R_{i,j}$ is the ratio of ROI counts for slice i and time frame j .

$C_{i,j}$ are the ROI counts for slice i at time frame j .

$C_{i,\text{low}}$ are the average ROI counts for slice i at the three time frames with lowest ACTIVITY, see 3.7.5.4.1.

By the above division, all normalizing factors with respect to different efficiencies per slice cancel out. Plot this ratio versus the slice number. In this graph, all deviations from a line parallel to the abscissa and positioned at the mean value are a measure of ADDRESS PILE UP in the axial direction. Determine the ACTIVITY in the phantom within the TOTAL FIELD OF VIEW corresponding to a 5 % deviation for any slice.

NOTE Axial variations at high COUNT RATES are most often caused by ADDRESS PILE UP, but may also result from other factors depending on the design of the tomograph.

For systems utilizing THREE-DIMENSIONAL RECONSTRUCTION, this test does not apply, because the complex relationship between a reconstructed slice and an axial crystal location obscures meaningful results from this test.

3.7.5.4.3 Test of COUNT LOSS correction scheme

From the set of reconstructed images according to 3.7.5.4.1 (and for each slice) plot a graph (see Figure 12) of:

- TRUE COINCIDENCE counts measured;
- TRUE COINCIDENCE counts corrected for COUNT LOSS;
- TRUE COINCIDENCE counts corrected for COUNT LOSS and decay.

The decay correction shall be done with the same half life according to Table 1 for all slices and for all scatter conditions. This half life should yield, in the low COUNT LOSS range (low COUNT LOSSES but high decay correction factor), a line parallel to the abscissa. All deviations from this parallel line are indicative of errors in the COUNT LOSS correction.

3.7.5.5 Report

3.7.5.5.1 TRUE COINCIDENCE COUNT RATE CHARACTERISTIC (see 3.7.5.4.1)

From the measurements according to 3.7.5.4.1, report the graphs showing the COUNT RATE CHARACTERISTIC (including the characteristic of the RANDOM COINCIDENCE rate) for the total system and the ACTIVITY levels at 20 % COUNT LOSS and at 50 % COUNT LOSS (without ATTENUATION correction and normalization) for each slice. For the total system, report the measured TRUE COINCIDENCE COUNT RATE at 20 % COUNT LOSS and at 50 % COUNT LOSS.

Report a plot of ROI counts (21 mm in diameter for the rod source, 194 mm in diameter for the cylinder) divided by measured TRUE COINCIDENCES for the whole slice versus ACTIVITY for each slice.

3.7.5.5.2 ADDRESS PILE UP (see 3.7.5.4.2)

Report a plot of normalized ROI counts according to 3.7.5.4.2. Report the observed ACTIVITY in the phantom within the TOTAL FIELD OF VIEW causing a 5 % deviation in the axial profile according to 3.7.5.4.2.

3.7.5.5.3 Accuracy of COUNT LOSS correction (see 3.7.5.4.3)

Report the plots according to 3.7.5.4.3. Report the maximum deviation from linearity up to the saturation point and the corresponding ACTIVITY for any slice for the three scatter conditions described in 3.7.5.3.1.1 to 3.7.5.3.1.3.

3.7.6 Scatter measurement

3.7.6.1 General

The scattering of primary gamma rays created in the annihilation of positrons results in coincidence events with false information for radiation source localization. Variations in design and implementation cause single photon computer tomographs operated in coincidence detection mode to have different sensitivities to scattered radiation.

3.7.6.2 Purpose

The purpose of this procedure is to measure the relative system sensitivity to scattered radiation, expressed by the SCATTER FRACTION (SF) as well as the values of the SCATTER FRACTION in each slice.

3.7.6.3 Method

The measurement shall be performed by imaging a single LINE SOURCE at three different radial positions within the water-filled head phantom (see Figures 2 and 3).

Unscattered events are assumed to lie within a $4 \times$ FWHM wide strip centred on the image of the LINE SOURCE in each SINOGRAM. This width region is chosen because the scatter value is insensitive to the exact width of the region, and negligible unscattered events lie more than $2 \times$ FWHM from the line image in SINGLE PHOTON COMPUTER TOMOGRAPHS operated in coincidence detection modes (see Figure 4).

The width of the scatter response function allows a simplified method of analysis. A linear interpolation across the strip from the points of intersection of the scatter tails and the edges of the $4 \times$ FWHM wide strip is used to estimate the amount of scatter present in the strip. The area under the line of interpolation, plus the contributions outside of the strip constitute the estimated scatter.

Estimates of SCATTER FRACTION for uniform source distributions are made under the assumption of slow radial dependence. The SCATTER FRACTION for a LINE SOURCE on-axis is assumed to be constant over a cross-sectional area out to a radius of 22,5 mm, the SCATTER FRACTION for a LINE SOURCE 45 mm off-axis is assumed to be constant within an annulus between 22,5 mm and 67,5 mm, and the SCATTER FRACTION for a LINE SOURCE 90 mm off-axis is assumed to be constant within an annulus between 67,5 mm and 100 mm (see Figure 3). The three values for SCATTER FRACTION are weighted by the areas to which they are applied, yielding a weighted average. The annular areas are in the ratios of 1:8:10,75, respectively.

3.7.6.3.1 RADIONUCLIDE

The RADIONUCLIDE for the measurement shall be ^{18}F , with an ACTIVITY such that the percentage of COUNT LOSSES is less than 10 % and the RANDOM COINCIDENCE rate is less than 10 % of the TOTAL COINCIDENCE rate.

3.7.6.3.2 RADIOACTIVE SOURCE distribution

The head phantom (Figure 2) shall be filled with non-radioactive water as a scatter medium.

The test phantom LINE SOURCE shall be inserted parallel to the axis of the cylinder sequentially at radii of 0 mm, 45 mm, and 90 mm, see Figure 3. The phantom shall be centred transaxially and axially in the field of view.

3.7.6.3.3 Data collection

Each coincident event between individual detectors shall be taken into account only once. Data shall be assembled into SINOGRAMS. All events will be assigned to the slice at the midpoint of the corresponding LINE OF RESPONSE. With the source at the specified positions, at least 10 000 counts shall be acquired for each slice within the central 16,5 cm or the AXIAL FIELD OF VIEW, whichever is the smaller.

3.7.6.3.4 Data processing

Data shall be corrected for RANDOM COINCIDENCES and COUNT LOSSES, but not for scatter or ATTENUATION.

3.7.6.4 Analysis

All SINOGRAMS corresponding to slices at least 1 cm from either end of the phantom shall be processed. Thus for tomographs with an AXIAL FIELD OF VIEW less than 16,5 cm, all slices shall be processed.

All PIXELS in each SINOGRAM i which are located further than 12 cm from the centre shall be set to zero. For each PROJECTION ANGLE within the SINOGRAM, the location of the centre of the LINE SOURCE shall be determined by finding the PIXEL with the largest value. Each PROJECTION shall be shifted so that the PIXEL containing the maximum value aligns with the central PIXEL column of the SINOGRAM. After realignment, a sum PROJECTION shall be produced.

The FWHM to be used for the analysis is the average of the RADIAL RESOLUTION and the TANGENTIAL RESOLUTION at radial position 10 cm off centre (see 3.7.1.5). The counts in the PIXELS at the left and right edges of the 4 x FWHM wide strip, $C_{L,i,k}$ and $C_{R,i,k}$ respectively, shall be obtained from the sum PROJECTION (see Figure 4). Linear interpolation shall be used to find the PIXEL intensities at ± 2 x FWHM from the central PIXEL of the PROJECTION. The average of the two count levels $C_{L,i,k}$ and $C_{R,i,k}$ shall be multiplied by the fractional number of PIXELS between the edges of the 4 x FWHM wide strip, with the product added to the counts in the PIXELS outside the strip, to yield the number of SCATTERED TRUE COINCIDENCE counts $C_{s,i,k}$ for the slice i and the source position k . The TRUE COINCIDENCE counts (scattered plus unscattered) $C_{tot,i,k}$ is the sum of all PIXELS in the sum PROJECTION.

The average ACTIVITY $A_{ave,k}$ during data acquisition over the time interval $T_{acq,k}$ (includes the time required to rotate the detectors for a complete set of PROJECTIONS) for the LINE SOURCE at position k , shall be calculated (see 3.7.3.3.4).

The SCATTER FRACTION SF_i for each slice (moving average over 10 slices), due to a uniform source distribution is calculated as follows:

$$SF_i = \frac{\frac{C_{s,i,1}}{A_{ave,1}} + 8 \frac{C_{s,i,2}}{A_{ave,2}} + 10,75 \frac{C_{s,i,3}}{A_{ave,3}}}{\frac{C_{tot,i,1}}{A_{ave,1}} + 8 \frac{C_{tot,i,2}}{A_{ave,2}} + 10,75 \frac{C_{tot,i,3}}{A_{ave,3}}}$$

where the subscripts 1, 2 and 3 refer to LINE SOURCES at radius 0 mm, 45 mm and 90 mm, respectively.

3.7.6.5 Report

For each slice that was processed, tabulate the value of SF_i . The average SF of the SF_i shall also be reported as the system SCATTER FRACTION.

3.7.7 ATTENUATION correction

3.7.7.1 General

POSITRON EMISSION TOMOGRAPHY has a valid theoretical basis for ATTENUATION correction for arbitrary attenuating media within the TOMOGRAPHIC VOLUME of a tomograph. The basis for the correction is a measurement of the transmission of ANNIHILATION RADIATION through the object within the TOTAL FIELD OF VIEW. The accuracy with which this is achieved in practice is an important measure of its quantitative ability.

3.7.7.2 Purpose

The purpose of this procedure is to measure the accuracy of the transmission method of ATTENUATION correction.

NOTE The outcome of this test is influenced also by scatter.

3.7.7.3 Method

Transmission of external radiation through a non-uniform attenuating medium is processed to give ATTENUATION correction matrices, which are applied to emission PROJECTION data as a part of the reconstruction process. Conformity of reconstructed emission values with true values is an indicator of the accuracy of ATTENUATION correction.

3.7.7.3.1 RADIONUCLIDE

The RADIONUCLIDE for the emission measurement shall be ^{18}F , with an ACTIVITY such that the percentage of COUNT LOSSES is less than 5 % and the RANDOM COINCIDENCE rate is less than 5 % of the TOTAL COINCIDENCE rate.

3.7.7.3.2 RADIOACTIVE SOURCE distribution

The head phantom (Figure 2) shall be centred in the AXIAL FIELD OF VIEW but (vertically) displaced 25 mm off-axis. It shall be used with the three 50 mm diameter cylinder inserts placed 60 mm from the axis of the phantom at 120° angular increments, arranged as in Figure 13. For the transmission measurement, the phantom shall be filled with non-radioactive water. One of the hollow inserts shall be filled with non-radioactive air and the other with non-radioactive water. The third insert is solid and made of polytetrafluoroethylene. For the emission measurement, a measured amount of ACTIVITY shall be added to the background of the test phantom and thoroughly mixed with the water.

3.7.7.3.3 Data collection

Transmission measurement of the head phantom shall be carried out by the method recommended by the manufacturer of the tomograph and shall be stated. For the emission measurement, the ACTIVITY shall be added to the head phantom and a standard image acquisition shall be performed.

The transmission and emission measurements can be performed in either order provided proper procedures are followed. If the head phantom must be removed between measurements, it should be precisely repositioned as before. If the emission scan is performed first, then at least ten half lives shall elapse before transmission data are acquired. Because the images are summed over slices in the analysis, it is important that the phantom axis be parallel to the axial direction (SYSTEM AXIS) of the tomograph.

3.7.7.3.4 Data processing

For tomographs with an AXIAL FIELD OF VIEW of 16,5 cm or less, all slices shall be reconstructed. For tomographs with an AXIAL FIELD OF VIEW greater than 16,5 cm, only slices in that part of the AXIAL FIELD OF VIEW where the phantom was placed, shall be reconstructed.

Images shall be reconstructed using the standard IMAGE MATRIX and TRIAXEL size and using a ramp filter with cut-off at the Nyquist frequency of the PROJECTION data. The emission data shall be reconstructed applying all corrections including ATTENUATION correction as obtained from the transmission measurement. Transmission processing shall be done according to the method recommended by the manufacturer and shall be stated.

3.7.7.4 Analysis

For each insert a 10 mm wide profile shall be drawn in the image, passing through the centre of the head phantom and through the centre of the insert.

3.7.7.5 Report

Graphs of the profiles through the three inserts shall also be reported.

Page 15

4 ACCOMPANYING DOCUMENTS

Add, at the end of this clause, the following new subclauses and table:

4.5 Parameters describing a single photon computer tomograph operated in coincidence detection mode

4.5.1 Design parameters

- detector element dimensions and number of elements
- detector orientation
- detector material
- number and configuration of detector elements per block, if applicable
- number of detector blocks per ring, if applicable
- COINCIDENCE WINDOW
- detector ring diameter or detector separation (radius of rotation)
- patient port diameter
- TRANSVERSE FIELD OF VIEW
- AXIAL FIELD OF VIEW
- SINOGRAM sampling (linear and angular)
- axial sampling
- septal length
- septal thickness
- septa design
- graded absorbers
- length of side shields
- type of transmission source and source ACTIVITY (nominal and recommended range)
- detector movement (e.g. rotational speed, angular range), if any

4.5.2 Configuration of the tomograph

- energy windows used
- axial acceptance angle (2D-mode, 3D-mode)
- reconstruction algorithm
- method of RANDOM COINCIDENCE estimation
- any additional information being considered essential by the manufacturer to characterize normal operation

4.5.3 SPATIAL RESOLUTION

- TRANSVERSE RESOLUTION (radial and tangential) according to 3.7.1.5
- AXIAL SLICE WIDTH according to 3.7.1.5
- AXIAL RESOLUTION according to 3.7.1.5
- axial PIXEL dimension according to 3.7.1.5
- transverse PIXEL dimensions according to 3.7.1.5
- axial step size according to 3.7.1.5

4.5.4 RECOVERY COEFFICIENT

- graphs of RECOVERY COEFFICIENT according to 3.7.2.6

4.5.5 Sensitivity

- SLICE SENSITIVITY according to 3.7.3.5
- NORMALIZED SLICE SENSITIVITY according to 3.7.3.5
- VOLUME SENSITIVITY according to 3.7.3.5

4.5.6 COUNT RATE performance

- COUNT RATE CHARACTERISTIC according to 3.7.5.5
- ACTIVITY levels at 20 % and 50 % COUNT LOSS according to 3.7.5.5
- measured TRUE COINCIDENCE COUNT RATE at 20 % COUNT LOSS and 50 % COUNT LOSS according to 3.7.5.5
- plots of normalized ROI counts versus ACTIVITY according to 3.7.5.5
- ADDRESS PILE UP according to 3.7.5.5
- accuracy of COUNT LOSS correction and associated plots according to 3.7.5.5

4.5.7 SCATTER FRACTION

- SCATTER FRACTIONS SF_i and SF according to 3.7.6.5

4.5.8 Accuracy of ATTENUATION correction

- profiles across inserts according to 3.7.7.5

Table 1 – RADIONUCLIDES to be used in performance measurements

RADIONUCLIDE	Half life	Branching ratio
¹⁸ F	109,70 ± 0,11 min	0,971± 0,002
¹¹ C	20,375 min	0,998
⁶⁸ Ge/ ⁶⁸ Ga	270,82 d	0,89


Page 22

Add, after Figure 7, the following new Figures 8 to 13.

IECNORM.COM: Click to view the full PDF of IEC 61675-2:1998/AMD1:2004

Withdrawn

Dimensions in millimetres

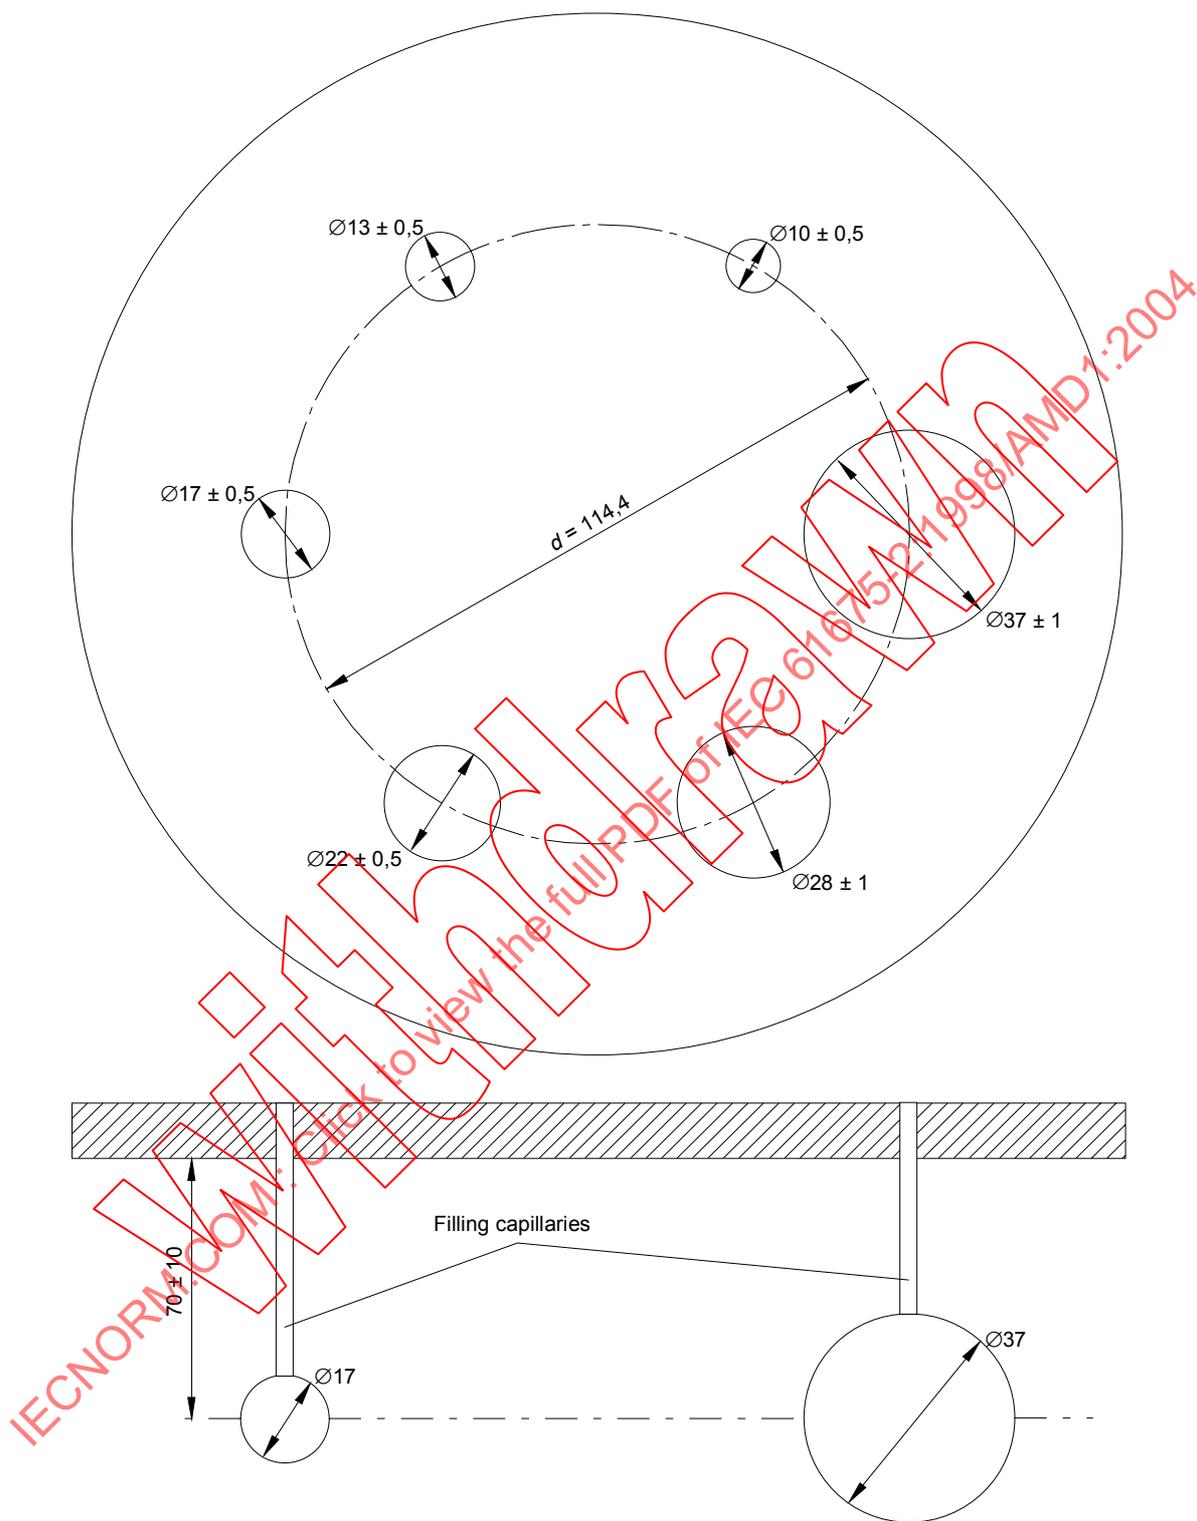

Material: polymethylmethacrylate.

IEC 1619/04

NOTE All diameters given are inside diameters.
 The wall thickness of the spheres shall be ≤ 1 mm.
 The centres of the spheres shall be at the same distance from the surface of the mounting plate.
 The mounting plate replaces the cover of the head phantom.
 The spheres can also be made from glass.

Figure 8 – Phantom insert with hollow spheres