

# INTERNATIONAL STANDARD

# IEC 62053-22

First edition  
2003-01

---

---

## Electricity metering equipment (a.c.) – Particular requirements –

### Part 22: Static meters for active energy (classes 0,2 S and 0,5 S)

*This **English-language** version is derived from the original **bilingual** publication by leaving out all French-language pages. Missing page numbers correspond to the French-language pages.*



Reference number  
IEC 62053-22:2003(E)

## Publication numbering

As from 1 January 1997 all IEC publications are issued with a designation in the 60000 series. For example, IEC 34-1 is now referred to as IEC 60034-1.

## Consolidated editions

The IEC is now publishing consolidated versions of its publications. For example, edition numbers 1.0, 1.1 and 1.2 refer, respectively, to the base publication, the base publication incorporating amendment 1 and the base publication incorporating amendments 1 and 2.

## Further information on IEC publications

The technical content of IEC publications is kept under constant review by the IEC, thus ensuring that the content reflects current technology. Information relating to this publication, including its validity, is available in the IEC Catalogue of publications (see below) in addition to new editions, amendments and corrigenda. Information on the subjects under consideration and work in progress undertaken by the technical committee which has prepared this publication, as well as the list of publications issued, is also available from the following:

- **IEC Web Site** ([www.iec.ch](http://www.iec.ch))

- **Catalogue of IEC publications**

The on-line catalogue on the IEC web site ([www.iec.ch/searchpub](http://www.iec.ch/searchpub)) enables you to search by a variety of criteria including text searches, technical committees and date of publication. On-line information is also available on recently issued publications, withdrawn and replaced publications, as well as corrigenda.

- **IEC Just Published**

This summary of recently issued publications ([www.iec.ch/online\\_news/justpub](http://www.iec.ch/online_news/justpub)) is also available by email. Please contact the Customer Service Centre (see below) for further information.

- **Customer Service Centre**

If you have any questions regarding this publication or need further assistance, please contact the Customer Service Centre:

Email: [custserv@iec.ch](mailto:custserv@iec.ch)  
Tel: +41 22 919 02 11  
Fax: +41 22 919 03 00

# INTERNATIONAL STANDARD

# IEC 62053-22

First edition  
2003-01

---

---

## Electricity metering equipment (a.c.) – Particular requirements –

### Part 22: Static meters for active energy (classes 0,2 S and 0,5 S)

© IEC 2003 Copyright - all rights reserved

No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Electrotechnical Commission, 3, rue de Varembe, PO Box 131, CH-1211 Geneva 20, Switzerland  
Telephone: +41 22 919 02 11 Telefax: +41 22 919 03 00 E-mail: inmail@iec.ch Web: www.iec.ch



Commission Electrotechnique Internationale  
International Electrotechnical Commission  
Международная Электротехническая Комиссия

## CONTENTS

FOREWORD .....	5
INTRODUCTION .....	7
1 Scope .....	9
2 Normative references.....	9
3 Terms and definitions .....	11
4 Standard electrical values.....	11
5 Mechanical requirements .....	11
6 Climatic conditions.....	11
7 Electrical requirements .....	11
7.1 Power consumption .....	11
7.2 Influence of short-time overcurrents.....	13
7.3 Influence of self-heating .....	13
7.4 AC voltage test.....	13
8 Accuracy requirements .....	15
8.1 Limits of error due to variation of the current.....	15
8.2 Limits of error due to influence quantities .....	17
8.3 Test of starting and no-load condition.....	21
8.4 Meter constant.....	23
8.5 Accuracy test conditions .....	23
8.6 Interpretation of test results.....	25
Annex A (normative) Test circuit diagram for sub-harmonics .....	27
Annex B (normative) Electromagnet for testing the influence of externally produced magnetic fields.....	31
Figure A.1 – Test circuit diagram (informative) .....	27
Figure A.2 – Burst fired wave-form .....	29
Figure A.3 – Informative distribution of harmonics (the Fourier analysis is not complete) .....	29
Figure B.1 – Electromagnet for testing the influence of externally produced magnetic fields .....	31
Table 1 – Power consumption including the power supply .....	11
Table 2 – Variations due to self-heating .....	13
Table 3 – AC voltage tests .....	15
Table 4 – Percentage error limits (single-phase meters and polyphase meters with balanced loads).....	15
Table 5 – Percentage error limits (polyphase meters carrying a single-phase load, but with balanced polyphase voltages applied to voltage circuits) .....	17
Table 6 – Influence quantities .....	17
Table 7 – Voltage and current balance .....	23
Table 8 – Reference conditions .....	25
Table 9 – Interpretation of test results .....	25

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

**ELECTRICITY METERING EQUIPMENT (AC) –  
PARTICULAR REQUIREMENTS –****Part 22: Static meters for active energy (classes 0,2 S and 0,5 S)**

## FOREWORD

- 1) The IEC (International Electrotechnical Commission) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of the IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, the IEC publishes International Standards. Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. The IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of the IEC on technical matters, express as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested National Committees.
- 3) The documents produced have the form of recommendations for international use and are published in the form of standards, technical specifications, technical reports or guides and they are accepted by the National Committees in that sense.
- 4) In order to promote international unification, IEC National Committees undertake to apply IEC International Standards transparently to the maximum extent possible in their national and regional standards. Any divergence between the IEC Standard and the corresponding national or regional standard shall be clearly indicated in the latter.
- 5) The IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with one of its standards.
- 6) Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 62053-22 has been prepared by IEC technical committee 13: Equipment for electrical energy measurement and load control.

This standard together with IEC 62052-11 cancels and replaces IEC 60687 second edition 1992 and constitutes a technical revision.

The text of this standard is based on the following documents:

FDIS	Report on voting
13/1283/FDIS	13/1290/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

The committee has decided that the contents of this publication will remain unchanged until 2012. At this date, the publication will be

- reconfirmed;
- withdrawn;
- replaced by a revised edition, or
- amended.

## INTRODUCTION

This part of IEC 62053 is to be used with the following relevant parts of the IEC 62052, IEC 62053 and IEC 62059 series, Electricity metering equipment:

- IEC 62052-11:2003, *Electricity metering equipment (a.c.) – General requirements, tests and test conditions – Part 11: Metering equipment*
- IEC 62053-11:2003, *Electricity metering equipment (a.c.) – Particular requirements – Part 11: Electromechanical meters for active energy (classes 0,5, 1 and 2)*  
Replaces particular requirements of IEC 60521: 1988 (2<sup>nd</sup> edition)
- IEC 62053-21:2003, *Electricity metering equipment (a.c.) – Particular requirements – Part 21: Static meters for active energy (classes 1 and 2)*  
Replaces particular requirements of IEC 61036: 2000 (2<sup>nd</sup> edition)
- IEC 62053-22:2003, *Electricity metering equipment (a.c.) – Particular requirements – Part 22: Static meters for active energy (classes 0,2 S and 0,5 S)*  
Replaces particular requirements of IEC 60687: 1992 (2<sup>nd</sup> edition)
- IEC 62053-31:1998, *Electricity metering equipment (a.c.) – Particular requirements – Part 31: Pulse output devices for electromechanical and electronic meters (two wires only)*
- IEC 62053-61:1998, *Electricity metering equipment (a.c.) – Particular requirements – Part 61: Power consumption and voltage requirements*
- IEC 62059-11:2002, *Electricity metering equipment (a.c.) – Dependability – Part 11: General concepts*
- IEC 62059-21:2002, *Electricity metering equipment (a.c.) – Dependability – Part 21: Collection of meter dependability data from the field*

This part is a standard for type testing electricity meters. It covers the particular requirements for meters, being used indoors. It does not deal with special implementations (such as metering-part and/or displays in separate housings).

This standard is intended to be used in conjunction with IEC 62052-11. When any requirement in this standard concerns an item already covered in IEC 62052-11, the requirements of this standard take precedence over the requirements of IEC 62052-11.

This standard distinguishes:

- between accuracy class index 0,2 S and accuracy class index 0,5 S meters;
- between protective class I and protective class II meters;
- between meters for use in networks equipped with or without earth fault neutralizers.

The test levels are regarded as minimum values that provide for the proper functioning of the meter under normal working conditions. For special application, other test levels might be necessary and should be agreed on between the user and the manufacturer.

## ELECTRICITY METERING EQUIPMENT (AC) – PARTICULAR REQUIREMENTS –

### Part 22: Static meters for active energy (classes 0,2 S and 0,5 S)

#### 1 Scope

This part of IEC 62053 applies only to newly manufactured static watt-hour meters of accuracy classes 0,2 S and 0,5 S, for the measurement of alternating current electrical active energy in 50 Hz or 60 Hz networks and it applies to their type tests only.

It applies only to transformer-operated static watt-hour meters for indoor application consisting of a measuring element and register(s) enclosed together in a meter case. It also applies to operation indicator(s) and test output(s). If the meter has a measuring element for more than one type of energy (multi-energy meters), or when other functional elements, like maximum demand indicators, electronic tariff registers, time switches, ripple control receivers, data communication interfaces, etc. are enclosed in the meter case, then the relevant standards for these elements also apply.

NOTE IEC 60044-1 describes transformers having a measuring range of  $0,01 I_n$  to  $1,2 I_n$ , or of  $0,05 I_n$  to  $1,5 I_n$ , or of  $0,05 I_n$  to  $2 I_n$  and transformers having a measuring range of  $0,01 I_n$  to  $1,2 I_n$  for accuracy classes 0,2 S and 0,5 S. As the measuring ranges of a meter and its associated transformers have to be matched and as only transformers of classes 0,2 S and 0,5 S have the accuracy required to operate the meters of this standard, the measuring range of the meter will be  $0,01 I_n$  to  $1,2 I_n$ .

It does not apply to:

- watt-hour meters where the voltage across the connection terminals exceeds 600 V (line-to-line voltage for meters for polyphase systems);
- portable meters and meters for outdoor use;
- data interfaces to the register of the meter;
- reference meters.

The dependability aspect is covered by the documents of the IEC 62059 series.

#### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60044-1:1996, *Instrument transformers – Part 1: Current transformers*

IEC 60736:1982, *Testing equipment for electrical energy meters*

IEC 62052-11:2002, *Electricity metering equipment (a.c.) – General requirements, tests and test conditions – Part 11: Metering equipment*

IEC 62053-61:1998, *Electricity metering equipment (a.c.) - Particular requirements - Part 61: Power consumption and voltage requirements*

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in IEC 62052-11 apply.

### 4 Standard electrical values

The values given in IEC 62052-11 apply.

### 5 Mechanical requirements

The requirements of IEC 62052-11 apply.

### 6 Climatic conditions

The conditions given in IEC 62052-11 apply.

### 7 Electrical requirements

In addition to the electrical requirements in IEC 62052-11, meters shall fulfil the following requirements.

#### 7.1 Power consumption

The power consumption in the voltage and current circuits shall be determined at reference conditions given in 8.5 by any suitable method. The overall maximum error of the measurement of the power consumption shall not exceed 5 %.

The active and apparent power consumption taken at reference temperature and reference frequency, by each voltage circuit at reference voltage and by each current circuit at rated current, shall not exceed the values shown in Table 1.

**Table 1 – Power consumption including the power supply**

	Power supply connected to the voltage circuits	Power supply not connected to the voltage circuits
Voltage circuit	2 W and 10 VA	0,5 VA
Current circuit	1 VA	1 VA
Auxiliary power supply	–	10 VA

NOTE 1 In order to match voltage and current transformers to meters, the meter manufacturer should state whether the burden is inductive or capacitive.

NOTE 2 The above figures are mean values. Switching power supplies with peak power values in excess of these specified values are permitted, but it should be ensured that the rating of associated voltage transformers is adequate.

NOTE 3 For multifunctional meters see IEC 62053-61.

## 7.2 Influence of short-time overcurrents

Short-time overcurrents shall not damage the meter. The meter shall perform correctly when back to its initial working condition and the variation of error at rated current and unity power factor shall not exceed 0,05 %.

The test circuit shall be practically non-inductive and the test shall be performed for polyphase meters phase-by-phase.

After the application of the short-time overcurrent with the voltage maintained at the terminals, the meter shall be allowed to return to the initial temperature with the voltage circuit(s) energized (about 1 h).

The meter shall be able to carry for 0,5 s a current equal to  $20 I_{\max}$  with a relative tolerance of +0 % to –10 %.

## 7.3 Influence of self-heating

The variation of error due to self-heating shall not exceed the values given in Table 2.

**Table 2 – Variations due to self-heating**

Value of current	Power factor	Limits of variations in percentage error for meters of class	
		0,2 S	0,5 S
$I_{\max}$	1	0,1	0,2
	0,5 inductive	0,1	0,2

The test shall be carried out as follows: after the voltage circuits have been energized at reference voltage for at least 2 h without any current in the current circuits, the maximum current shall be applied to the current circuits. The meter error shall be measured at unity power factor immediately after the current is applied and then at intervals short enough to allow a correct drawing to be made of the curve of error variation as a function of time. The test shall be carried out for at least 1 h, and in any event until the variation of error during 20 min does not exceed 0,05 %.

The same test shall then be carried out at 0,5 (inductive) power factor.

The cable to be used for energizing the meter shall have a length of 1 m and a cross-section of between  $1,5 \text{ mm}^2$  and  $2,5 \text{ mm}^2$ .

## 7.4 AC voltage test

The a.c. voltage test shall be carried out in accordance with Table 3.

The test voltage shall be substantially sinusoidal, having a frequency between 45 Hz and 65 Hz, and applied for 1 min. The power source shall be capable of supplying at least 500 VA.

During the tests relative to earth, the auxiliary circuits with reference voltage equal to or below 40 V shall be connected to earth.

All these tests shall be carried out with the case closed and the cover and terminal covers in place.

During this test no flashover, disruptive discharge or puncture shall occur.

**Table 3 – AC voltage tests**

Test	Applicable to	Test voltage r.m.s	Points of application of the test voltage
A	Protective class I meters	2 kV	a) Between, on the one hand, all the current and voltage circuits as well as the auxiliary circuits whose reference voltage is over 40 V, connected together, and, on the other hand, earth.
		2 kV	b) Between circuits not intended to be connected together in service.
B	Protective class II meters	4 kV	a) Between, on the one hand, all the current and voltage circuits as well as the auxiliary circuits whose reference voltage is over 40 V, connected together, and, on the other hand, earth.
		2 kV	b) Between circuits not intended to be connected together in service.
		–	c) A visual inspection for compliance with the conditions of 5.7 of IEC 62052-11.

## 8 Accuracy requirements

Tests and test conditions given in IEC 62052-11 apply.

### 8.1 Limits of error due to variation of the current

When the meter is under the reference conditions given in 8.5, the percentage errors shall not exceed the limits for the relevant accuracy class given in Tables 4 and 5.

If the meter is designed for the measurement of energy in both directions, the values in Table 4 and Table 5 shall apply for each direction.

**Table 4 – Percentage error limits  
(single-phase meters and polyphase meters with balanced loads)**

Value of current	Power factor	Percentage error limits for meters of class	
		0,2 S	0,5 S
$0,01 I_n \leq I < 0,05 I_n$	1	±0,4	±1,0
$0,05 I_n \leq I \leq I_{max}$	1	±0,2	±0,5
$0,02 I_n \leq I < 0,1 I_n$	0,5 inductive	±0,5	±1,0
	0,8 capacitive	±0,5	±1,0
$0,1 I_n \leq I \leq I_{max}$	0,5 inductive	±0,3	±0,6
	0,8 capacitive	±0,3	±0,6
When specially requested by the user: from	0,25 inductive	±0,5	±1,0
	0,5 capacitive	±0,5	±1,0

**Table 5 – Percentage error limits (polyphase meters carrying a single-phase load, but with balanced polyphase voltages applied to voltage circuits)**

Value of current	Power factor	Percentage error limits for meters of class	
		0,2 S	0,5 S
$0,05 I_n \leq I \leq I_{max}$	1	$\pm 0,3$	$\pm 0,6$
$0,1 I_n \leq I \leq I_{max}$	0,5 inductive	$\pm 0,4$	$\pm 1,0$

The difference between the percentage error when the meter is carrying a single-phase load and a balanced polyphase load at rated current  $I_n$  and unity power factor shall not exceed 0,4 % and 1,0 % for meters of classes 0,2 S and 0,5 S respectively.

NOTE When testing for compliance with Table 5, the test current should be applied to each measuring element in sequence.

## 8.2 Limits of error due to influence quantities

The additional percentage error due to the change of influence quantities with respect to reference conditions, as given in 8.5, shall not exceed the limits for the relevant accuracy class given in Table 6.

**Table 6 – Influence quantities**

Influence quantity	Value of current (balanced unless otherwise stated)	Power factor	Mean temperature coefficient %/K for meters of class	
			0,2 S	0,5 S
Ambient temperature variation <sup>9)</sup>	$0,05 I_n \leq I \leq I_{max}$	1	0,01	0,03
	$0,1 I_n \leq I \leq I_{max}$	0,5 inductive	0,02	0,05
			Limits of variation in percentage error for meters of class	
			0,2 S	0,5 S
Voltage variation $\pm 10$ % <sup>1) 8)</sup>	$0,05 I_n \leq I \leq I_{max}$	1	0,1	0,2
	$0,1 I_n \leq I \leq I_{max}$	0,5 inductive	0,2	0,4
Frequency variation $\pm 2$ % <sup>8)</sup>	$0,05 I_n \leq I \leq I_{max}$	1	0,1	0,2
	$0,1 I_n \leq I \leq I_{max}$	0,5 inductive	0,1	0,2
Reversed phase sequence	$0,1 I_n$	1	0,05	0,1
Voltage unbalance <sup>3)</sup>	$I_n$	1	0,5	1,0
Auxiliary voltage $\pm 15$ % <sup>4)</sup>	$0,01 I_n$	1	0,05	0,1
Harmonic components in the current and voltage circuits <sup>5)</sup>	$0,5 I_{max}$	1	0,4	0,5
Sub-harmonics in the a.c. current circuit <sup>5)</sup>	$0,5 I_n$ <sup>2)</sup>	1	0,6	1,5
Continuous magnetic induction of external origin <sup>5)</sup>	$I_n$	1	2,0	2,0
Magnetic induction of external origin 0,5 mT <sup>6)</sup>	$I_n$	1	0,5	1,0

Influence quantity	Value of current (balanced unless otherwise stated)	Power factor	Limits of variation in percentage error for meters of class	
			0,2 S	0,5 S
Electromagnetic RF fields	$I_n$	1	1,0	2,0
Operation of accessories <sup>7)</sup>	$0,01 I_n$	1	0,05	0,1
Conducted disturbances, induced by radio-frequency fields	$I_n$	1	1,0	2,0
Fast transient burst	$I_n$	1	1,0	2,0
Damped oscillatory waves immunity	$I_n$	1	1,0	2,0

1) For the voltage ranges from –20 % to –10 % and +10 % to +15 %, the limits of variation in percentage errors are three times the values given in this table.

Below  $0,8 U_n$  the error of the meter may vary between +10 % and –100 %.

2) The distortion factor of the voltage shall be less than 1 %. For test conditions see 8.2.2.

3) Polyphase meters with three measuring elements shall measure and register, within the limits of variation in percentage error shown in this table, if the following phases are interrupted

- in a three-phase, four-wire network one or two phases;
- in a three-phase, three-wire network (if the meter is designed for this service) one of the three phases.

This only covers phase interruptions and does not cover events such as transformer fuse failures.

4) Applicable only if the auxiliary supply is not internally connected to the voltage measuring circuit.

5) The test conditions are specified in 8.2.1 to 8.2.3.

6) A magnetic induction of external origin of 0,5 mT produced by a current of the same frequency as that of the voltage applied to the meter and under the most unfavourable conditions of phase and direction shall not cause a variation in the percentage error of the meter exceeding the values shown in this table.

The magnetic induction shall be obtained by placing the meter in the centre of a circular coil, 1 m in mean diameter, of square section and of small radial thickness relative to the diameter, and having 400 At.

7) Such an accessory, when enclosed in the meter case, is energized intermittently, for example the electromagnet of a multi-rate register.

It is preferable that the connection to the auxiliary device(s) is marked to indicate the correct method of connection. If these connections are made by means of plugs and sockets, they should be irreversible.

However, in the absence of those markings or irreversible connections, the variations of errors shall not exceed those indicated in Table 6 if the meter is tested with the connections giving the most unfavourable condition.

8) The recommended test point for voltage variation and frequency variation is  $I_n$ .

9) The mean temperature coefficient shall be determined for the whole operating range. The operating temperature range shall be divided into 20 K wide ranges. The mean temperature coefficient shall then be determined for these ranges by taking measurements 10 K above and 10 K below the middle of the range. During the test, the temperature shall be in no case outside the specified operating temperature range.

Tests for variation caused by influence quantities should be performed independently with all other influence quantities at their reference conditions (see Table 8).

### 8.2.1 Accuracy test in the presence of harmonics

Test conditions:

- fundamental frequency current:  $I_1 = 0,5 I_{max}$
- fundamental frequency voltage:  $U_1 = U_n$

- fundamental frequency power factor: 1
- content of 5<sup>th</sup> harmonic voltage:  $U_5 = 10\%$  of  $U_n$
- content of 5<sup>th</sup> harmonic current:  $I_5 = 40\%$  of fundamental current
- harmonic power factor: 1
- fundamental and harmonic voltages are in phase, at positive zero crossing.

Resulting harmonic power due to the 5<sup>th</sup> harmonic is  $P_5 = 0,1 U_1 \times 0,4 I_1 = 0,04 P_1$  or total active power =  $1,04 P_1$  (fundamental + harmonics).

### 8.2.2 Tests of the influence of sub-harmonics

The tests of the influence of sub-harmonics shall be made with the circuit shown in Figure A.1 or with other equipment able to generate the required wave-forms, and the current wave-forms as shown in Figure A.2.

The variation in percentage error when the meter is subjected to the test wave-form given in Figure A.2 and when it is subjected to the reference wave-form shall not exceed the limits of variation given in Table 6.

NOTE The values given in the figures are for 50 Hz only. For other frequencies the values have to be adapted accordingly.

### 8.2.3 Continuous magnetic induction of external origin

The continuous magnetic induction may be obtained by using the electromagnet according to Annex B, energized with a d.c. current. This magnetic field shall be applied to all accessible surfaces of the meter when it is mounted as for normal use. The value of the magneto-motive force applied shall be 1 000 At (ampere-turns).

### 8.3 Test of starting and no-load condition

For these tests, the conditions and the values of the influence quantities shall be as stated in 8.5 except for any changes specified below.

#### 8.3.1 Initial start-up of the meter

The meter shall be functional within 5 s after the reference voltage is applied to the meter terminals.

#### 8.3.2 Test of no-load condition

When the voltage is applied with no current flowing in the current circuit, the test output of the meter shall not produce more than one pulse.

For this test the current circuit shall be open-circuit and a voltage of 115 % of the reference voltage shall be applied to the voltage circuits.

The minimum test period  $\Delta t$  shall be

$$\Delta t \geq \frac{900 \times 10^6}{k m U_n I_{\max}} \text{ [min] for meters of class 0,2 S}$$

$$\Delta t \geq \frac{600 \times 10^6}{k m U_n I_{\max}} \text{ [min] for meters of class 0,5 S}$$

where

$k$  is the number of pulses emitted by the output device of the meter per kilowatthour (imp/kWh);

$m$  is the number of measuring elements;

$U_n$  is the reference voltage in volts;

$I_{\max}$  is the maximum current in amperes.

NOTE For transformer-operated meters with primary or half-primary registers, the constant  $k$  shall correspond to the secondary values (voltage and currents).

### 8.3.3 Starting

The meter shall start and continue to register at  $0,001 I_n$  and unity power factor (and in case of polyphase meters, with balanced load).

If the meter is designed for the measurement of energy in both directions, then this test shall be applied with energy flowing in each direction.

### 8.4 Meter constant

The relation between the test output and the indication in the display shall comply with the marking on the name-plate.

### 8.5 Accuracy test conditions

To test the accuracy requirements, the following test conditions shall be maintained:

- a) the meter shall be tested in its case with the cover in position; all parts intended to be earthed shall be earthed;
- b) before any test is made, the circuits shall have been energized for a time sufficient to reach thermal stability;
- c) in addition, for polyphase meters:
  - the phase sequence shall be as marked on the diagram of connections;
  - the voltages and currents shall be substantially balanced (see Table 7).

**Table 7 – Voltage and current balance**

Polyphase meters	Class of meter	
	0,2 S	0,5 S
Each of the voltages between phase and neutral and between any two phases shall not differ from the average corresponding voltage by more than	±1 %	±1 %
Each of the currents in the conductors shall not differ from the average current by more than	±1 %	±1 %
The phase displacements of each of these currents from the corresponding phase-to-neutral voltage, irrespective of the phase angle, shall not differ from each other by more than	2°	2°

d) the reference conditions are given in Table 8;

e) for requirements regarding test stations, see IEC 60736.

**Table 8 – Reference conditions**

Influence quantity	Reference value	Permissible tolerances for meters of class	
		0,2 S	0,5 S
Ambient temperature	Reference temperature or, in its absence, 23 °C <sup>1)</sup>	±2 °C	±2 °C
Voltage	Reference voltage	±1,0 %	±1,0 %
Frequency	Reference frequency	±0,3 %	±0,3 %
Phase sequence	L1 – L2 – L3	–	–
Voltage unbalance	All phases connected	–	–
Wave-form	Sinusoidal voltages and currents	<b>Distortion factor less than:</b> 2 %	
Continuous magnetic induction of external origin	Equal to zero	–	–
Magnetic induction of external origin at the reference frequency	Magnetic induction equal to zero	Induction value which causes a variation of error not greater than: ±0,1 % but should in any case be smaller than 0,05 mT <sup>2)</sup>	
Electromagnetic RF fields, 30 kHz to 2 GHz	Equal to zero	<1 V/m	<1 V/m
Operation of accessories	No operation of accessories	–	–
Conducted disturbances, induced by radiofrequency fields, 150 kHz to 80 MHz	Equal to zero	<1 V	<1 V
<p>1) If the tests are made at a temperature other than the reference temperature, including permissible tolerances, the results shall be corrected by applying the appropriate temperature coefficient of the meter.</p> <p>2) The test consists of:</p> <p>a) for a single-phase meter, determining the errors first with the meter normally connected to the mains and then after inverting the connections to the current circuits as well as to the voltage circuits. Half of the difference between the two errors is the value of the variation of error. Because of the unknown phase of the external field, the test should be made at 0,05 <math>I_n</math> at unity power factor and 0,1 <math>I_n</math> at 0,5 power factor;</p> <p>b) for a three-phase meter, making three measurements at 0,05 <math>I_n</math> at unity power factor, after each of which the connection to the current circuits and to the voltage circuits are changed over 120° while the phase sequence is not altered. The greatest difference between each of the errors so determined and their average value is the value of the variation of error.</p>			

### 8.6 Interpretation of test results

Certain test results may fall outside the limits indicated in Tables 4 and 5, owing to uncertainties of measurements and other parameters capable of influencing the measurements. However, if by one displacement of the zero line parallel to itself by no more than the limits indicated in Table 9, all the test results are brought within the limits indicated in Tables 4 and 5, the meter type shall be considered acceptable.

**Table 9 – Interpretation of test results**

	Class of meter	
	0,2 S	0,5 S
Permissible displacement of the zero line (%)	0,1	0,2

## Annex A (normative)

### Test circuit diagram for sub-harmonics

NOTE The values given in the Figures A.2 and A.3 are for 50 Hz only. For other frequencies the values have to be adapted accordingly.

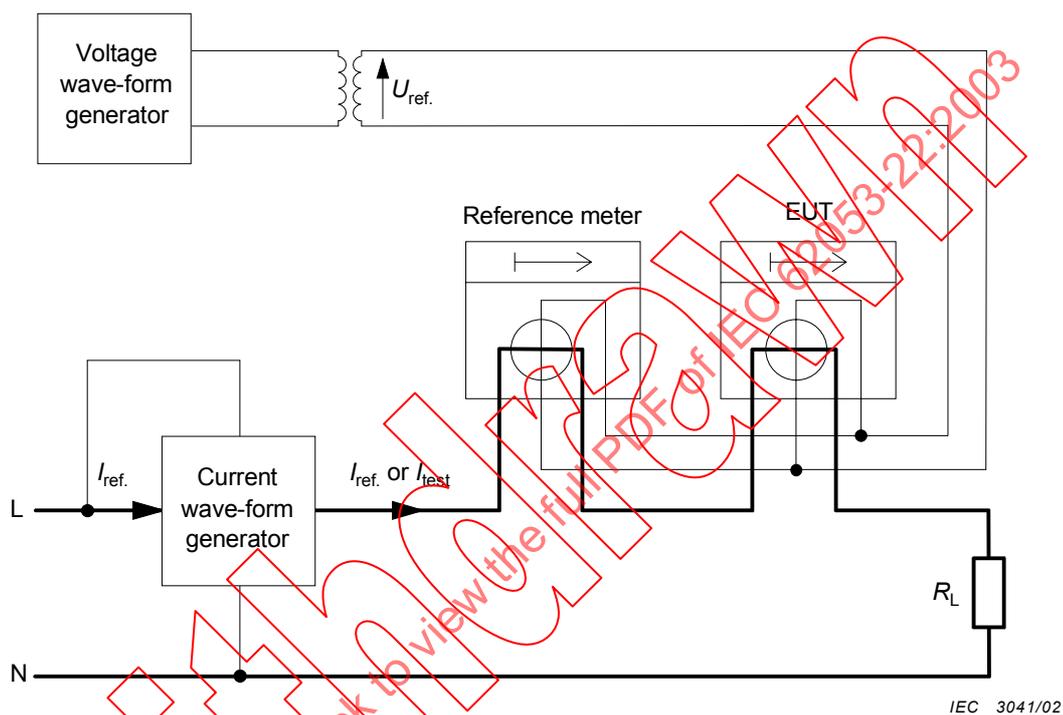


Figure A.1 – Test circuit diagram (informative)

NOTE The reference meter shall measure the total active energy (fundamental + harmonics) in the presence of harmonics.