


Medical electrical equipment - Part 2-30: Particular requirements for the basic safety  
and essential performance of automated non-invasive sphygmomanometers

CORRIGENDUM 1

Figure 201.101 – CUFF pressure PROTECTION DEVICE, triggered by overpressure in SINGLE FAULT CONDITION

Replace the existing figure with the following new figure:

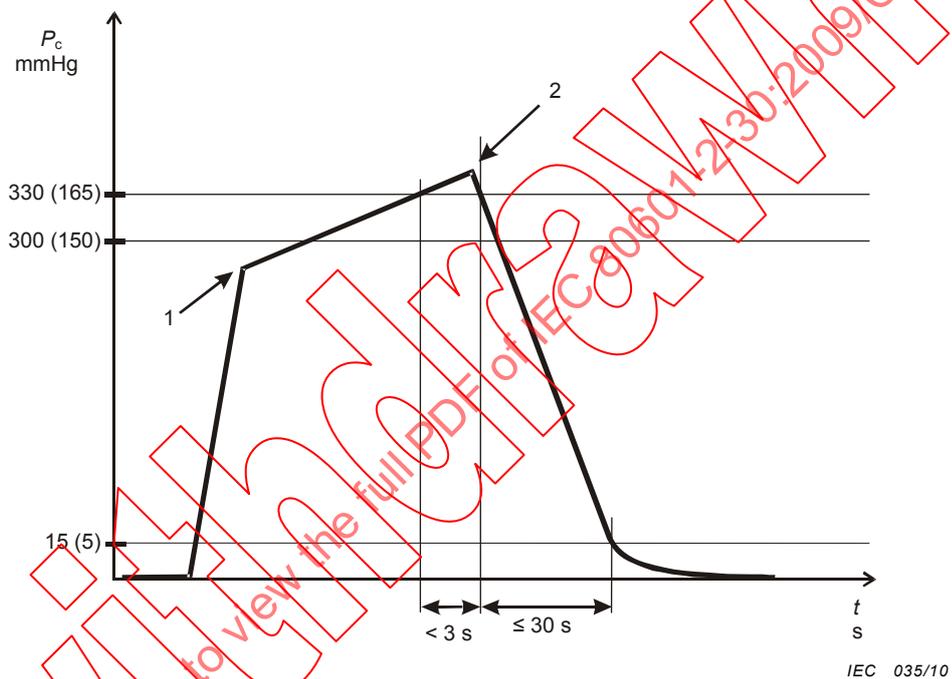

201.105.1 LONG-TERM AUTOMATIC MODE

In item a), delete “either” at the end of the first line and replace “or” with “and” at the end of the first dash.

201.105.3.2 NORMAL CONDITION

Delete “either” at the end of the first line and replace “or” with “and” at the end of the first dash.