

PUBLICLY AVAILABLE SPECIFICATION

PRE-STANDARD

**Waveguide type dielectric resonators –
Part 1-5: General information and test conditions – Measurement method
of conductivity at interface between conductor layer and dielectric substrate
at microwave frequency**

IECNORM.COM · Click to view the full PDF of IEC PAS 61338-1-5:2010



THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2010 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester.

If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland
Email: inmail@iec.ch
Web: www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

- Catalogue of IEC publications: www.iec.ch/searchpub

The IEC on-line Catalogue enables you to search by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, withdrawn and replaced publications.

- IEC Just Published: www.iec.ch/online_news/justpub

Stay up to date on all new IEC publications. Just Published details twice a month all new publications released. Available on-line and also by email.

- Electropedia: www.electropedia.org

The world's leading online dictionary of electronic and electrical terms containing more than 20 000 terms and definitions in English and French, with equivalent terms in additional languages. Also known as the International Electrotechnical Vocabulary online.

- Customer Service Centre: www.iec.ch/webstore/custserv

If you wish to give us your feedback on this publication or need further assistance, please visit the Customer Service Centre FAQ or contact us:

Email: csc@iec.ch
Tel.: +41 22 919 02 11
Fax: +41 22 919 03 00

IECNORM.COM: Click to view the PDF of IEC Pub. 61338-1-5:2010

PUBLICLY AVAILABLE SPECIFICATION

PRE-STANDARD

**Waveguide type dielectric resonators –
Part 1-5: General information and test conditions – Measurement method
of conductivity at interface between conductor layer and dielectric substrate
at microwave frequency**

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

PRICE CODE

R

ICS 31.140

ISBN 978-2-88910-935-7

CONTENTS

FOREWORD.....	4
INTRODUCTION.....	6
1 Scope.....	7
2 Normative references	8
3 Measurement and related parameters	8
4 Calculation equations for R_i and σ_i	9
5 Preparation of specimen.....	13
6 Measurement equipment and apparatus	13
6.1 Measurement equipment	13
6.2 Measurement apparatus.....	13
7 Measurement procedure.....	14
7.1 Set up of measurement equipment and apparatus.....	14
7.2 Measurement of reference level	14
7.3 Measurement procedure of Q_u	14
7.4 Determination of σ_i and measurement uncertainty.....	16
8 Example of measurement result	16
Annex A (informative) Derivation of equation (4) for R_i	18
Annex B (informative) Calculation uncertainty of parameters in Figure 3.....	19
Bibliography.....	20
Figure 1 – Surface resistance R_s , surface conductivity σ_s , interface resistance R_i , and interface conductivity σ_i	7
Figure 2 – The $TE_{01\delta}$ mode dielectric rod resonator to measure σ_i	9
Figure 3 – Parameters chart of f_0 , g , P_{rod} and P_{sub} for reference sapphire rod. Calculation conditions: $\epsilon'_{rod} = 9.4$, $d = 10.00$ mm and $h = 5.00$ mm	11
Figure 4 – Parameters chart of f_0 , g , P_{rod} and P_{sub} for reference (Zr,Sn)TiO ₄ rod. Calculation conditions: $\epsilon'_{rod} = 39$, $d = 14.00$ mm and $h = 6.46$ mm.....	12
Figure 5 – Schematic diagram of measurement equipments.....	13
Figure 6 – Schematic diagram of measurement apparatus for σ_{ri}	14
Figure 7 – Frequency response for reference sapphire rod with two dielectric substrates as shown in figure 2.....	15
Figure 8 – Resonance frequency f_0 , insertion attenuation IA_0 and half-power band width f_{BW}	16
Table 1 – Specifications of reference rods.	10
Table 2 – ϵ'_{rod} and $\tan \delta_{rod}$ of reference rods measured by the method (IEC 61338-1-3).....	16
Table 3 – ϵ'_{sub} and $\tan \delta_{sub}$ of a LTCC test substrate measured by the method (IEC 61338-1-4).....	17

Table 4 – Measurement results of σ_i and σ_{ri} of a copper layer in LTCC substrate with $\epsilon'_{sub}=4.76$, $d'=45$ mm and $t=0.415$ mm.....	17
Table B.1 – Parameters obtained by FEM and rigorous analysis (IEC61338-1-3) for the TE_{011} mode resonator with $\epsilon'_{rod}=9.4$, $d=10.0$ mm, and $h=5.0$ mm.....	19
Table B.2 – Calculated parameters f_0 , g , P_{rod} , P_{sub} , R_i , σ_i and σ_{ri} for the $TE_{01\delta}$ mode resonator with $\epsilon'_{rod}=9.4$ and 9.3 , with the test condition of $\epsilon'_{sub}=6.0$, $\tan\delta_{sub}=0.001$, $t=0.5$ mm, and $Q_u=6000$	19

IECNORM.COM: Click to view the full PDF of IEC PAS 61338-1-5:2010

Withdrawn

INTERNATIONAL ELECTROTECHNICAL COMMISSION

WAVEGUIDE TYPE DIELECTRIC RESONATORS –

Part 1-5: General information and test conditions – Measurement method of conductivity at interface between conductor layer and dielectric substrate at microwave frequency

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.

A PAS is a technical specification not fulfilling the requirements for a standard, but made available to the public.

IEC/PAS 61338-1-5 has been processed by IEC technical committee 49: Piezoelectric and dielectric devices for frequency control and selection.

The text of this PAS is based on the following document:

This PAS was approved for publication by the P-members of the committee concerned as indicated in the following document

Draft PAS	Report on voting
49/873/PAS	49/902/RVD

Following publication of this PAS, which is a pre-standard publication, the technical committee or subcommittee concerned may transform it into an International Standard.

This PAS shall remain valid for an initial maximum period of 3 years starting from the publication date. The validity may be extended for a single period up to a maximum of 3 years,

at the end of which it shall be published as another type of normative document, or shall be withdrawn.

A list of all parts of IEC 61338 series under the general title *Waveguide type dielectric resonators* can be found on the IEC website.

IEC 61338 consists of the following parts, under the general title *Waveguide type dielectric resonators*:

Part 1: Generic specification

Part 1-3: General information and test conditions - Measurement method of complex relative permittivity for dielectric resonator materials at microwave frequency

Part 1-4: General information and test conditions - Measurement method of complex relative permittivity for dielectric resonator materials at millimeter-wave frequency

Part 2: Guidelines for oscillator and filter applications

Part 4: Sectional specification

Part 4-1: Blank detail specification

IECNORM.COM · Click to view the full PDF of IEC PAS 61338-1-5:2010

Withdrawn

INTRODUCTION

The International Electrotechnical Commission (IEC) draws attention to the fact that it is claimed that compliance with this PAS may involve the use of a patent concerning:

“Measurement method of conductivity at interface of conductor layer”

“Measurement method of conductivity of conductor layer”

IEC takes no position concerning the evidence, validity and scope of this patent right.

The holder of this patent right has assured the IEC that he/she is willing to negotiate licences under reasonable and non-discriminatory terms and conditions with applicants throughout the world. In this respect, the statement of the holder of this patent right is registered with IEC. Information may be obtained from:

KYOCERA Corporation

6 Takeda Tobadono-cho, Fushimiku, Kyoto 612-5801, Japan

Attention is drawn to the possibility that some of the elements of this PAS may be the subject of patent rights other than those identified above. IEC shall not be held responsible for identifying any or all such patent rights.

ISO (www.iso.org/patents) and IEC (http://www.iec.ch/tctools/patent_decl.htm) maintain on-line data bases of patents relevant to their standards. Users are encouraged to consult the data bases for the most up to date information concerning patents.

IECNORM.COM : Click to view the full PDF IEC PAS 61338-1-5:2010

WAVEGUIDE TYPE DIELECTRIC RESONATORS –

Part 1-5: General information and test conditions – Measurement method of conductivity at interface between conductor layer and dielectric substrate at microwave frequency

1 Scope

Microwave circuits are popularly formed on multi-layered organic or non-organic substrates. In the microwave circuits, the attenuation of planar transmission lines such as striplines, microstrip lines, and coplanar lines are determined by their conductor loss, dielectric loss and radiation loss. Among them, the conductor loss is a major factor in the attenuation of the planar transmission lines. A new measurement method is needed to evaluate the conductivity of transmission line on or in the substrates such as the organic, ceramic and LTCC (low temperature co-fired ceramics) substrates.

The IEC 61338-1-3 described the measurement method for the surface resistance R_s and effective conductivity σ on the surface of the conductor. The term σ is designated as σ_s in this PAS, and is called surface conductivity (Figure 1). This PAS describes a measurement method for resistance and effective conductivity at the interface between conductor layer and dielectric substrate designated as R_i and σ_i respectively, and are called interface resistance and interface conductivity.

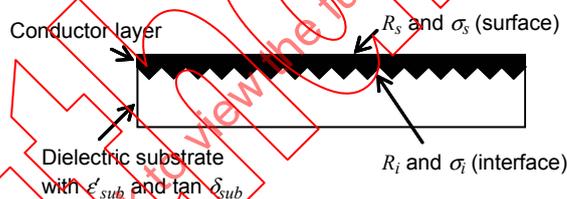


Figure 1 – Surface resistance R_s , surface conductivity σ_s , interface resistance R_i , and interface conductivity σ_i .

For the transmission line in the substrates, the electric current is concentrated at the interface between conductor layer and dielectric substrate, because the skin depth δ in the conductor is the order of μm in thickness at the microwave frequencies. In microstrip lines, the current is concentrated at the interface, rather than at the open face of the conductor. Furthermore, in copper-clad organic substrates, the interface side of the copper foil has rugged structure to hold the strong adhesive strength. In LTCC substrates, the interface between the conductor and ceramics has a rough structure, depending on the co-firing process and the material compositions. The interface conditions increase the conductor loss. Therefore, the evaluation of R_i and σ_i is important to design microwave circuit and to improve the conductor fabrication process.

This measurement method has the following characteristics:

- the interface resistance R_i is obtained by measuring the resonant frequency f_0 and unloaded quality factor Q_u of a $\text{TE}_{01\delta}$ mode dielectric rod resonator shown in Figure 2;

- the interface conductivity σ_i and the relative interface conductivity $\sigma_{ri} = \sigma_i / \sigma_0$ are calculated from the measured R_i value, where $\sigma_0 = 5,8 \times 10^7$ S/m is the conductivity of standard copper;
- the measurement uncertainty of σ_{ri} ($\Delta\sigma_{ri}$) is less than 5%.

2 Normative references

The following referenced documents are indispensable for the application of this PAS. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 61338-1-3: *Waveguide type dielectric resonators - Part 1-3: General information and test conditions – Measurement method of complex relative permittivity for dielectric resonator materials at microwave frequency*

IEC 61338-1-4: *Waveguide type dielectric resonators - Part 1-4: General information and test conditions – Measurement method of complex relative permittivity for dielectric resonator materials at millimetre-wave frequency*

3 Measurement and related parameters

The relationship between R_s and σ_s is given by

$$R_s = \sqrt{\frac{\pi f_0 \mu}{\sigma_s}} \quad , \quad \sigma_s = \sigma_{rs} \sigma_0 \quad (1)$$

where

- R_s is the surface resistance;
- f_0 is the resonance frequency;
- μ is the permeability of the conductor;
- σ_s is the surface conductivity;
- σ_{rs} is the relative surface conductivity.

Particularly, μ equals μ_0 ($\mu_0 = 4\pi \times 10^{-7}$ H/m) for nonmagnetic conductors such as copper and silver.

The relationship between R_i and σ_i is given by

$$R_i = \sqrt{\frac{\pi f_0 \mu}{\sigma_i}} \quad , \quad \sigma_i = \sigma_{ri} \sigma_0 \quad (2)$$

where

- R_i is the interface resistance;
- σ_i is the interface conductivity;
- σ_{ri} is the relative interface conductivity.

The skin depth δ is given by

$$\delta = \sqrt{\frac{1}{\pi f \mu \sigma}} \quad (3)$$

where

f is the frequency;
 σ is the conductivity of the conductor.

To obtain high accuracy in this measurement method, the σ_{ri} of the conductor is preferable to be higher than 5%, and the thickness of conductor to be three times greater than skin depth δ . The measurement frequencies are limited to be 5 GHz and 13 GHz in this PAS because of the reference dielectric rods used in this PAS.

4 Calculation equations for R_i and σ_i

Figure 2 shows the structure of a $TE_{01\delta}$ mode dielectric rod resonator for the R_i measurement. The resonator consists of a dielectric rod and a pair of dielectric substrates with a conductor layer at one side. The dielectric rod has diameter d , height h , relative permittivity ϵ'_{rod} , and loss tangent $\tan \delta_{rod}$. The pair of dielectric substrates have the same values of diameter d' , thickness t , relative permittivity ϵ'_{sub} , and loss tangent $\tan \delta_{sub}$. To suppress the radiation loss, the diameter d' shall be three times greater than d . The conductor layers on each dielectric substrate are supposed to have the same value of R_i .

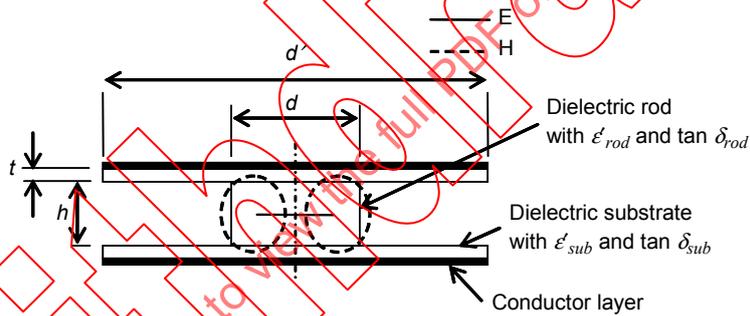


Figure 2 – The $TE_{01\delta}$ mode dielectric rod resonator to measure σ_i .

In this structure, the conductive loss of the $TE_{01\delta}$ mode resonator is caused by the interface resistance R_i . The value of $1/Q_u$ is given by a sum of power losses due to R_i , $\tan \delta_{rod}$ and $\tan \delta_{sub}$.

$$\frac{1}{Q_u} = \frac{R_i}{g} + P_{rod} \tan \delta_{rod} + P_{sub} \tan \delta_{sub}, \quad (4)$$

where

g is the geometric factor of the resonator (Ω);
 P_{rod} is the partial electric energy filling factor of the dielectric rod;
 P_{sub} is the partial electric energy filling factor of the dielectric substrate.

The equation for R_i is derived from Equation (4):

$$R_i = g \left(\frac{1}{Q_u} - P_{rod} \tan \delta_{rod} - P_{sub} \tan \delta_{sub} \right) \tag{5}$$

The value σ_i is calculated from this R_i value by Equation (2).

The derivation of Equation (4) is given in Annex A, together with definitions of the parameters g , P_{rod} and P_{sub} . These parameters for the $TE_{01\delta}$ mode resonator can be calculated by using the FEM or the mode matching method. However, the calculation requires complicated and tedious works. To make the treatment simple and easy, this PAS recommends to use the graphical charts that are prepared for the parameters of reference dielectric rod resonators; a sapphire single crystal and a (Zr,Sn)TiO₄ ceramic (Table 1). The (Zr,Sn)TiO₄ ceramic rod is provided from Japan fine ceramics center. The parameters f_0 , g , P_{rod} and P_{sub} for the reference rods were calculated by a FEM analyzed in cylindrical coordinate and are shown in Figures 3 and 4 graphically. The calculation uncertainty on the parameters is shown in Annex B.

To calculate the R_i in Equation (5), the complex permittivity values of the dielectric rod and the substrate are necessary to be given in advance. The values of ϵ'_{rod} and $\tan \delta_{rod}$ are measured by the dielectric rod resonator method described in IEC 61338-1-3. The values of ϵ'_{sub} and $\tan \delta_{sub}$ can be measured by the cavity resonator method described in IEC 61338-1-4.

Table 1 – Specifications of reference rods.

Reference rod	f_0 GHz	ϵ'_{rod}	$\tan \delta_{rod}$	diameter d mm	height h mm
Sapphire single crystal	13	$9,4 \pm 0,1$	13×10^{-6}	$10,00 \pm 0,05$	$5,00 \pm 0,05$
(Zr,Sn)TiO ₄ ceramics	5	39 ± 1	$<10 \times 10^{-4}$	$14,00 \pm 0,05$	$6,46 \pm 0,05$

NOTE 1 The axis of sapphire rod should be parallel to the c-axis within 0,3 degree.

NOTE 2 The reference dielectric rod of (Zr,Sn)TiO₄ is provided by JFCC (Japan fine ceramics center) as ER-ZST.

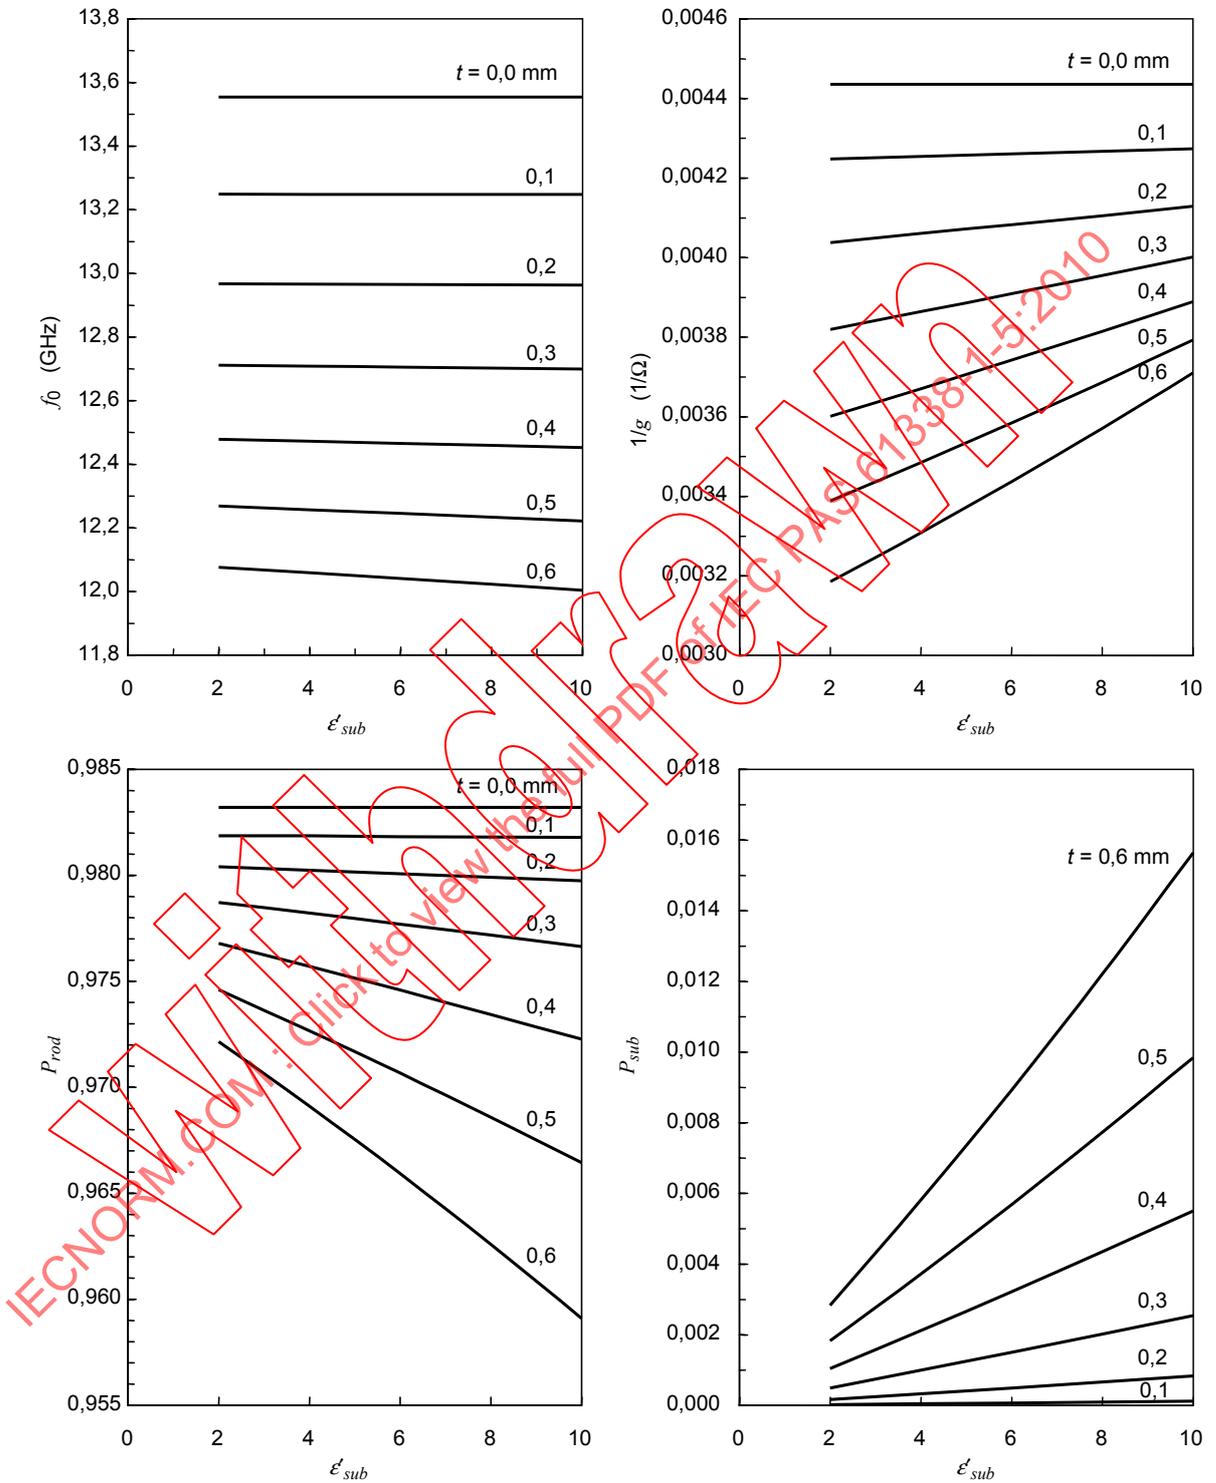


Figure 3 – Parameters chart of f_0 , g , P_{rod} and P_{sub} for reference sapphire rod
Calculation conditions: $\epsilon'_{rod} = 9,4$, $d = 10,00$ mm and $h = 5,00$ mm

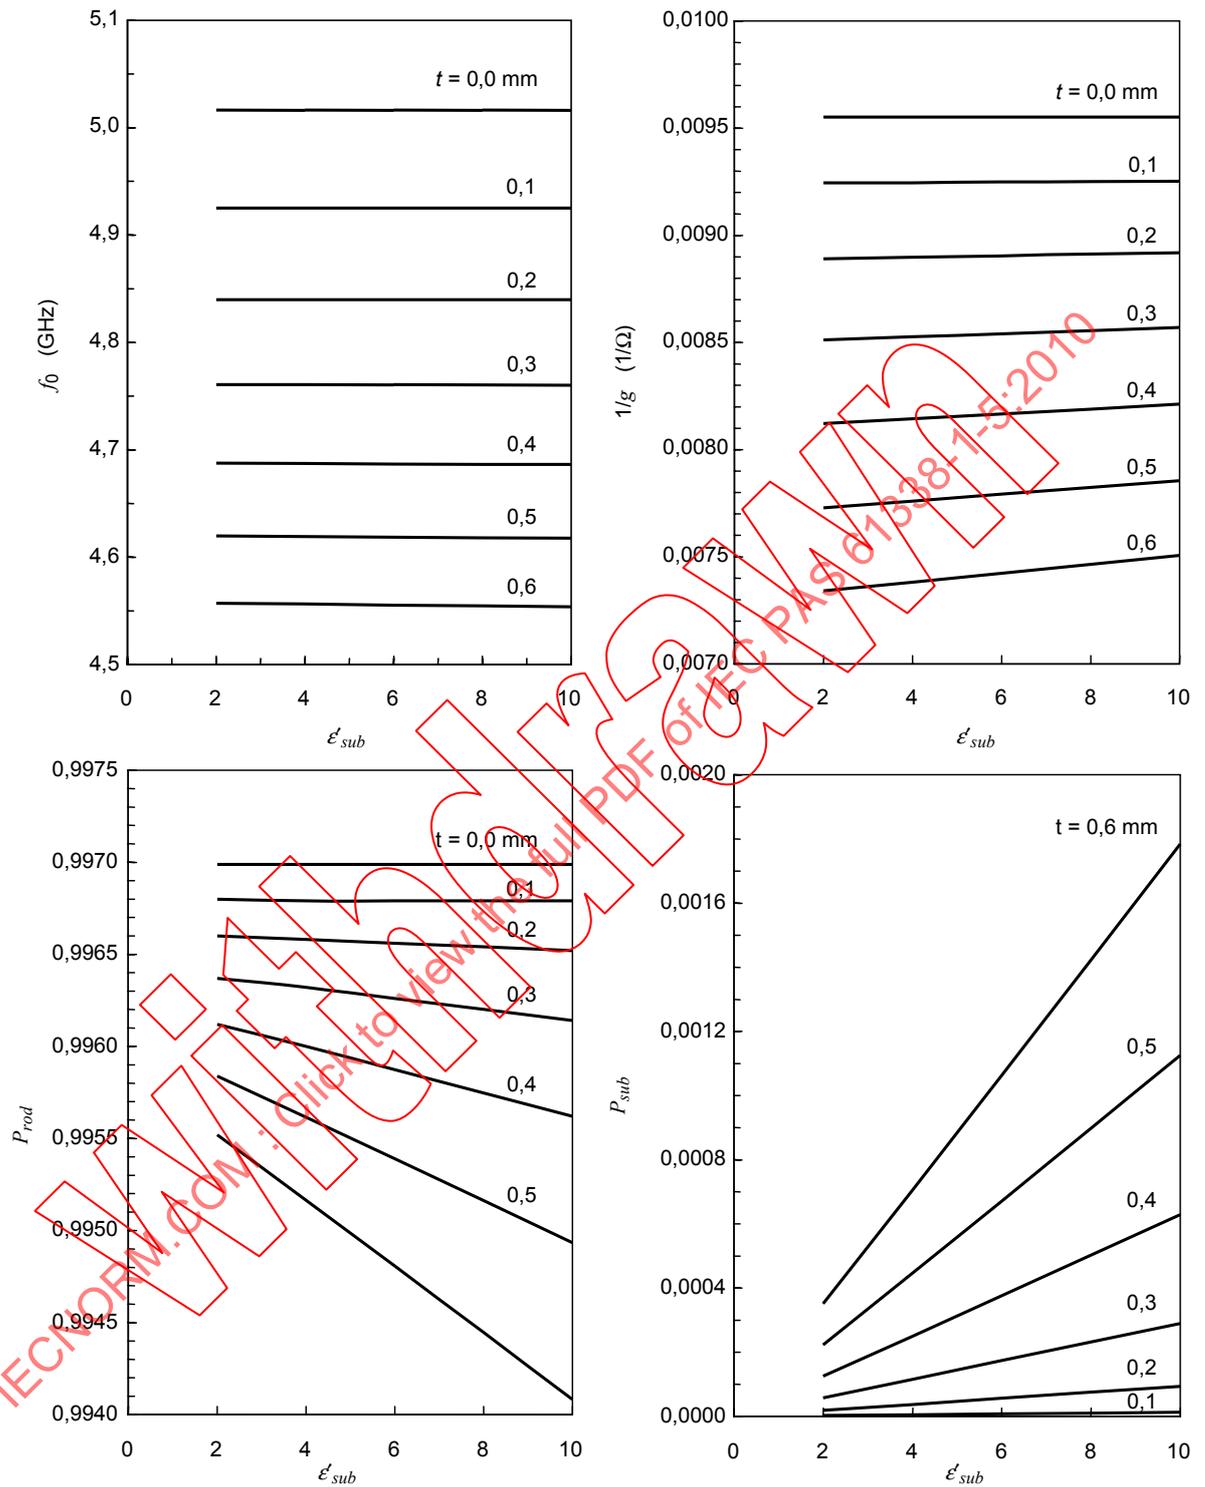


Figure 4 – Parameters chart of f_0 , g , P_{rod} and P_{sub} for reference (Zr,Sn)TiO₄ rod
Calculation conditions: $\epsilon'_{rod} = 39$, $d = 14,00$ mm and $h = 6,46$ mm

5 Preparation of specimen

Two test specimens of dielectric substrates with a conductor at one side are prepared for the σ_{ri} measurement. The thickness of the conductor t_c shall be three times greater than the skin depth δ . The values of δ is 0,9 μm for copper and 1,7 μm for tungsten at 5 GHz. The diameter d' of dielectric substrate shall be three times greater than the diameter d of the reference dielectric rod. Dielectric substrates with any shape larger than the diameter $3 \times d$ is used in practical measurement. Bending of specimen causes measurement error of σ_{ri} . A substrate/conductor/substrate layer structure, where a conductor is formed between two dielectric substrates, is effective to avoid the bending of specimen.

6 Measurement equipment and apparatus

6.1 Measurement equipment

Figure 5 shows a schematic diagram of two measurement systems. For the measurement of Q_u of the resonator to evaluate σ_{ri} , only the information on the amplitude of transmitted power is needed, that is, the information on the phase of the transmitted power is not required. Therefore, a scalar network analyzer can be used for the measurement shown in Figure 5(a). However, a vector network analyzer shown in Figure 5(b) has better measurement accuracy than a scalar network analyzer due to its wide dynamic range.

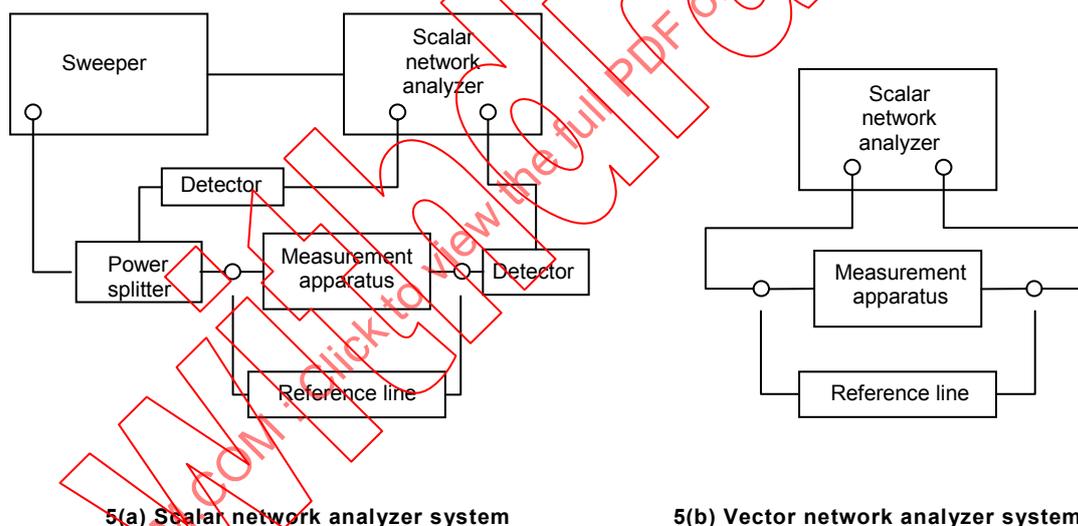


Figure 5 – Schematic diagram of measurement equipments

6.2 Measurement apparatus

Figure 6 shows a measurement apparatus for σ_{ri} . The reference dielectric rod is placed between the dielectric sides of two substrates with a conductor at one side. Two substrates are set to be parallel to each other.

Each of the two semi-rigid coaxial cables have a small loop at the top. The semi-rigid cable with the outer diameter of 1,2 mm is recommended. The two loops have the same diameter and the length shall be less than the quarter wavelength of measurement frequency. In practice, the loop with a diameter from 1 mm to 2 mm is preferable for the measurement around 10 GHz. The plane of the loop is set parallel to the dielectric substrates to suppress the excitation of the unwanted TM mode. The cables can move right and left to adjust the

insertion attenuation IA_0 at f_0 to be around 30 dB (as shown in Figure 8). The IA_0 value is recommended to be between 20 dB and 30 dB, in order to decrease the field disturbance due to the coupling loop and to decrease the noise influence on the resonance curve of the network analyzer.

A reference line made of a semi-rigid cable, shown in Figure 6, is used to measure the full transmission power level, i.e., the reference level as shown in Figure 8. This cable has a length equal to the sum of the two cables with a loop.

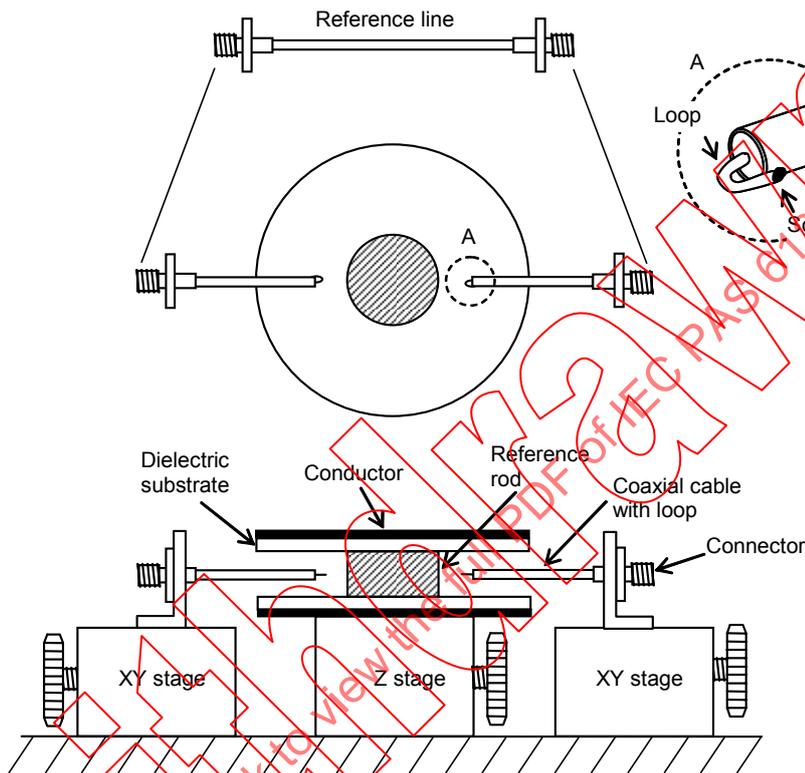


Figure 6 – Schematic diagram of measurement apparatus for σ_{ri}

7 Measurement procedure

7.1 Set up of measurement equipment and apparatus

Set up the measurement equipment and apparatus as shown in Figures 5 and 6. Relative humidity shall be less than 60 %, because high humidity degrades Q_u .

7.2 Measurement of reference level

Measure the reference transmission level, shown in Figure 8, over the entire measurement frequency range.

7.3 Measurement procedure of Q_u

Place the reference dielectric rod between the dielectric sides of two substrates. Adjust the distance between the reference rod and each of the loops of the semi-rigid cables to be equal.

Find the $TE_{01\delta}$ mode resonance peak of the resonator on the display of the network analyzer, by reading the approximate f_0 value of the $TE_{01\delta}$ mode resonance from Figures 3 or 4 for each reference rod. This peak can be identified as the one which shifts downward in frequency when the upper substrate is slowly separated from the top of the reference dielectric rod. Figure 7 shows an example of frequency response for a resonator.

Narrow the frequency span, so that only the resonance peak of $TE_{01\delta}$ mode can be shown on the display as shown in Figure 8. By changing the distance between the reference dielectric rod and the loops of the semi-rigid cables, adjust IA_0 to be around 30 dB from the reference level.

Measure f_0 , the half-power band-width f_{BW} and IA_0 . The loaded quality factor Q_L and the unloaded quality factor Q_u of this resonance mode are given by

$$Q_L = \frac{f_0}{f_{BW}} \quad (6)$$

$$Q_u = \frac{Q_L}{1 - A_t}, \quad A_t = 10^{-|IA_0(\text{dB})|/20} \quad (7)$$

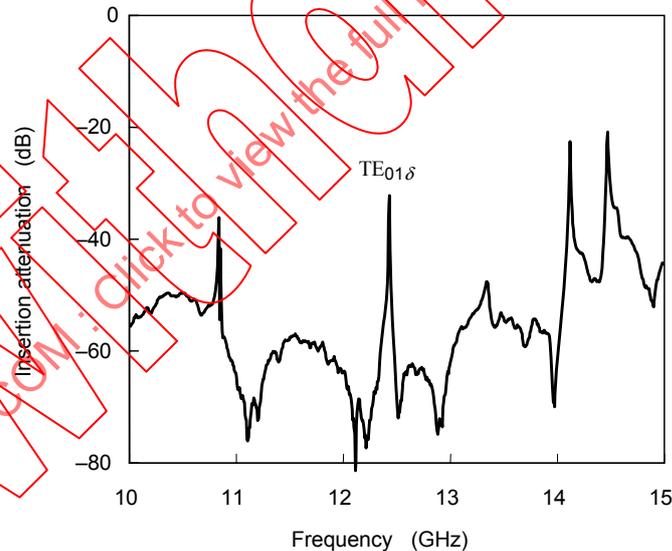


Figure 7 – Frequency response for reference sapphire rod with two dielectric substrates as shown in Figure 2

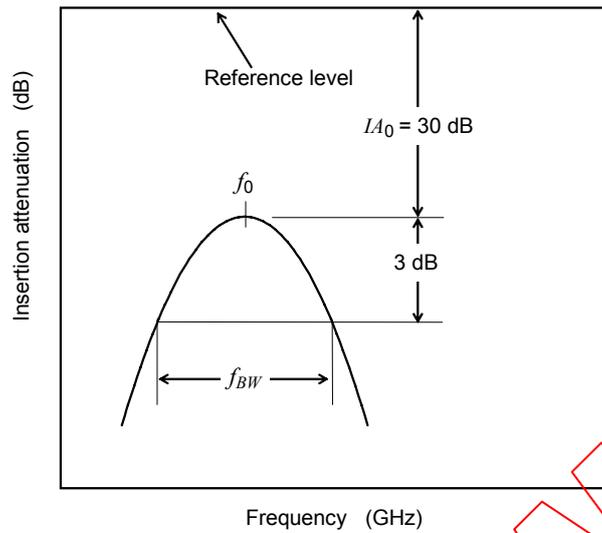


Figure 8 – Resonance frequency f_0 , insertion attenuation IA_0 and half-power band width f_{BW}

7.4 Determination of σ_i and measurement uncertainty

Repeat this measurement several times. Then, calculate R_i from the mean value of Q_u using Equation (5). The values g , P_{rod} and P_{sub} are given from Figures 3 and 4 using the ϵ'_{sub} and thickness t of the test substrate. The values σ_i and σ_{ri} are given from R_i using Equation (2).

Measurement uncertainty of σ_i , $\Delta\sigma_i$, estimated as the mean square errors is given by

$$(\Delta\sigma_i)^2 = (\Delta\sigma_{i,Q_u})^2 + (\Delta\sigma_{i,\tan\delta_{rod}})^2 + (\Delta\sigma_{i,\tan\delta_{sub}})^2 \tag{8}$$

where

- $\Delta\sigma_{i,Q_u}$ is the uncertainty of σ_i due to standard deviations of Q_u ;
- $\Delta\sigma_{i,\tan\delta_{rod}}$ is the uncertainty of σ_i due to standard deviations of $\tan\delta_{rod}$;
- $\Delta\sigma_{i,\tan\delta_{sub}}$ is the uncertainty of σ_i due to standard deviations of $\tan\delta_{sub}$.

8 Example of measurement result

Table 2 shows the values of ϵ'_{rod} and $\tan\delta_{rod}$ for the reference rods measured by the dielectric rod resonator method (IEC 61338-1-3). Table 3 shows the values of ϵ'_{sub} and $\tan\delta_{sub}$ of a LTCC test substrate measured by the cavity resonator method (IEC 61338-1-4). A copper layer was co-fired in this substrate and the σ_i and σ_{ri} were measured. The results are shown in Table 4.

Table 2 – ϵ'_{rod} and $\tan\delta_{rod}$ of reference rods measured by the method (IEC 61338-1-3)

Reference Rod	d mm	h mm	f_0 GHz	Q_u	ϵ'_{rod}	$\tan\delta_{rod}$ (10^{-4})
Sapphire	10,000 $\pm 0,001$	5,004 $\pm 0,001$	13,524 $\pm 0,002$	6 413 ± 52	9,435 $\pm 0,004$	0,13 $\pm 0,01$
(Zr,Sn)TiO ₄	14,000 $\pm 0,001$	6,465 $\pm 0,001$	4,9966 $\pm 0,0004$	3 612 ± 21	39,27 $\pm 0,01$	0,90 $\pm 0,02$

Table 3 – ε'_{sub} and $\tan \delta_{sub}$ of a LTCC test substrate measured by the method (IEC 61338-1-4)

d' mm	t mm	f_0 GHz	Q_u	ε'_{sub}	$\tan \delta_{sub}$ (10^{-4})
50	0,965 $\pm 0,08$	10,287 $\pm 0,003$	3 313 ± 22	4,76 $\pm 0,04$	7,18 $\pm 0,05$

Table 4 – Measurement results of σ_i and σ_{ri} of a copper layer in LTCC substrate with $\varepsilon'_{sub} = 4,76$, $d' = 45$ mm and $t = 0,415$ mm

Reference Rod	f_0 GHz	Q_u	σ_i 10^7 S/m	σ_{ri} %
Sapphire	12,426 $\pm 0,002$	6 725 ± 5	3,68 $\pm 0,05$	63,5 $\pm 0,9$
(Zr,Sn)TiO ₄	4,6626 $\pm 0,0003$	3 738 ± 20	3,83 $\pm 0,10$	66,0 $\pm 1,8$