

ISO/IEC 11801-1

Edition 1.0 2017-11

**INFORMATION TECHNOLOGY –
GENERIC CABLING FOR CUSTOMER PREMISES**

Part 1: General requirements

CORRIGENDUM 1

Foreword

Replace, in list item d), “Category BCT-B, 8.1, and 8.2;” with “Categories BCT-B, 8.1 and 8.2;”.

Replace list item f) with the following new list item:

f) addition of cabled optical fibre Categories OS1a and OM5;

Replace, in list item g), “silica optical fibre cabling;” with “optical fibre classes;”

Replace list item h) with the following new list item:

h) cabled optical fibre Categories OM1, OM2 and OS1 have been moved to an informative annex.


Introduction

Replace the first paragraph with the following new paragraph:

This document contains general requirements in support of the other premises-specific referenced cabling design documents developed by ISO/IEC JTC 1/SC 25 including ISO/IEC 11801-2, ISO/IEC 11801-3, ISO/IEC 11801-4, ISO/IEC 11801-5, ISO/IEC 11801-6, related Technical Specifications and Technical Reports (including the ISO/IEC TR 11801-99xx series, ISO/IEC TR 24704, ISO/IEC TR 24750 and ISO/IEC TS 29125).

Figure 1 – Relationships between the generic cabling documents produced by ISO/IEC JTC 1/SC 25

Replace the figure graphic with the following new figure graphic:

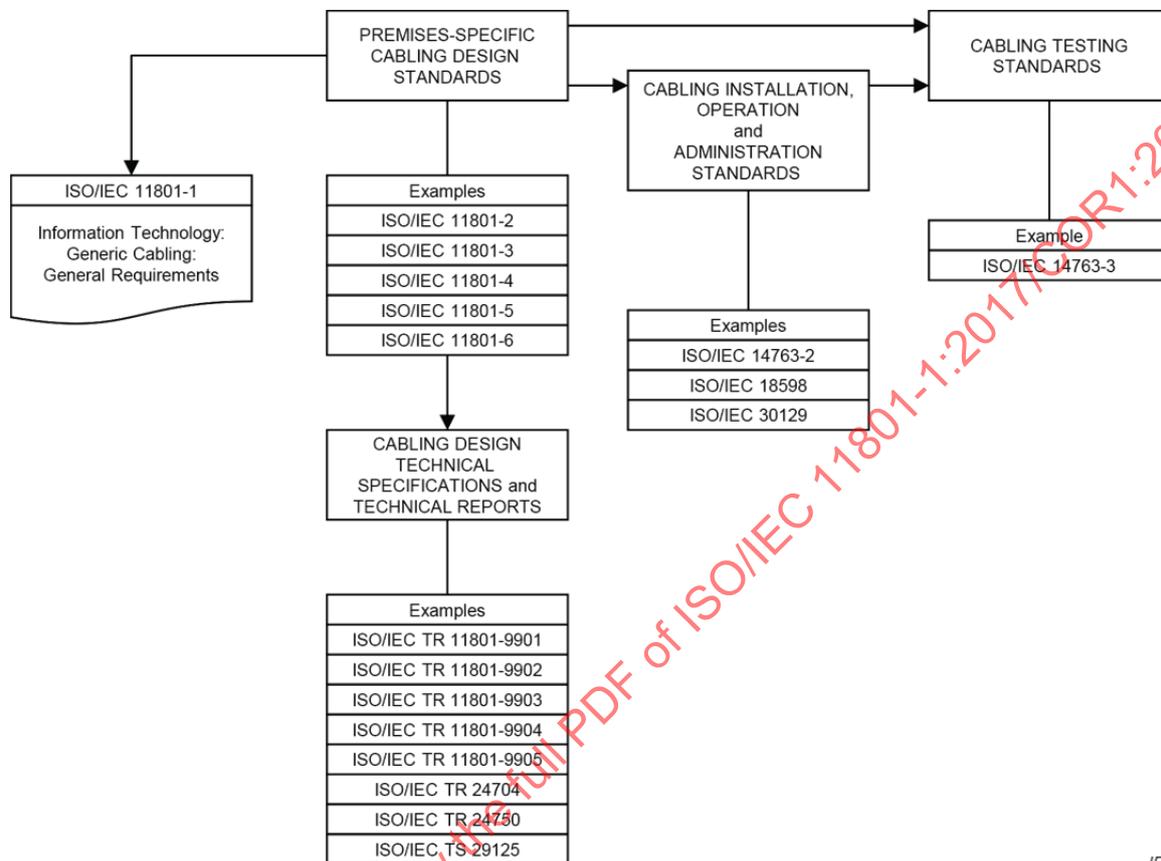

IEC

3.1 Terms and definitions

In 3.1.26, delete “end-to-end” from the definition.

Delete the entire entry 3.1.32.

3.2 Abbreviations

Insert the following abbreviation:

C connection

Replace:

FEXT far-end crosstalk attenuation (loss)

with:

FEXT far-end crosstalk (loss)

Replace:

NEXT near-end crosstalk attenuation (loss)

with:

NEXT near-end crosstalk (loss)

3.3.1 Variables

Delete the following line:

☐ connection

3.3.2 Indices

Delete the following line:

TO index to denominate a characteristic, measured from the TO

5.1 Functional elements


After the sentence “Groups of these functional elements are connected together to form cabling subsystems.”, insert the following new note:

NOTE The numbering of the cabling subsystems does not imply a hierarchy.

Figure 5 – Equipment and test interfaces

Replace the figure graphic with the following new figure graphic:

Cabling subsystem 1

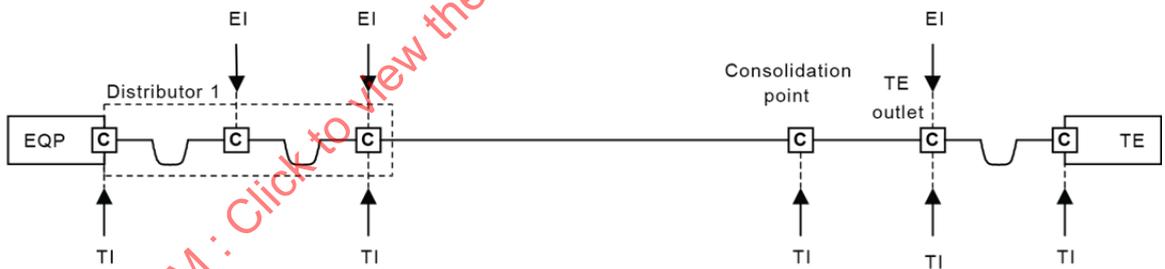

Cabling subsystems 2, 3 and 4



IEC

Table 2 – Details of environmental classification

In row 20, insert “g/m³” after each numerical value in columns 2, 3 and 4, as follows:

Sodium chloride (salt/sea water)	0 g/m ³	< 0,3 g/m ³	< 0,3 g/m ³
----------------------------------	--------------------	------------------------	------------------------

In row 21, insert “mg/m³” after each numerical value in columns 2, 3 and 4, as follows:

Oil (dry-air concentration) (for oil types see ^b)	0 mg/m ³	< 0,005 mg/m ³	< 0,5 mg/m ³
--	---------------------	---------------------------	-------------------------

In row 22, insert “mg/m³” after each numerical value in columns 3 and 4, as follows:

Sodium stearate (soap)	None	> 5 × 10 ⁴ mg/m ³ aqueous non-gelling	> 5 × 10 ⁴ mg/m ³ aqueous gelling
------------------------	------	--	--

In rows 26 to 35, insert “mg/m³” after each numerical value in columns 2, 3 and 4, as follows:

Hydrogen sulphide	< 0,003 mg/m ³ / < 0,01 mg/m ³	< 0,05 mg/m ³ / < 0,5 mg/m ³	< 10 mg/m ³ / < 50 mg/m ³
Sulphur dioxide	< 0,01 mg/m ³ / < 0,03 mg/m ³	< 0,1 mg/m ³ / < 0,3 mg/m ³	< 5 mg/m ³ / < 15 mg/m ³
Sulphur trioxide (ffs)	< 0,01 mg/m ³ / < 0,03 mg/m ³	< 0,1 mg/m ³ / < 0,3 mg/m ³	< 5 mg/m ³ / < 15 mg/m ³
Chlorine wet (> 50 % humidity)	< 0,000 5 mg/m ³ / < 0,001 mg/m ³	< 0,005 mg/m ³ / < 0,03 mg/m ³	< 0,05 mg/m ³ / < 0,3 mg/m ³
Chlorine dry (< 50 % humidity)	< 0,002 mg/m ³ / < 0,01 mg/m ³	< 0,02 mg/m ³ / < 0,1 mg/m ³	< 0,2 mg/m ³ / < 1,0 mg/m ³
Hydrogen chloride	– / < 0,06 mg/m ³	< 0,06 mg/m ³ / < 0,3 mg/m ³	< 0,6 mg/m ³ / 3,0 mg/m ³
Hydrogen fluoride	< 0,001 mg/m ³ / < 0,005 mg/m ³	< 0,01 mg/m ³ / < 0,05 mg/m ³	< 0,1 mg/m ³ / < 1,0 mg/m ³
Ammonia	< 1 mg/m ³ / < 5 mg/m ³	< 10 mg/m ³ / < 50 mg/m ³	< 50 mg/m ³ / < 250 mg/m ³
Oxides of nitrogen	< 0,05 mg/m ³ / < 0,1 mg/m ³	< 0,5 mg/m ³ / < 1 mg/m ³	< 5 mg/m ³ / < 10 mg/m ³
Ozone	< 0,002 g/m ³ / < 0,005 g/m ³	< 0,025 g/m ³ / < 0,05 g/m ³	< 0,1 g/m ³ / < 1 g/m ³

6.3.1 General

In the first sentence after list item 2), replace “two sub-Classes, L and M.” with “two sub-Classes, L and M (see Table 5).”

6.3.3.2 Insertion loss/attenuation

In the last paragraph before Table 5, delete “, at maximum implementation,”.

6.3.3.6 Direct current loop resistance

Replace the first paragraph with the following new paragraph:

The DC loop resistance requirements are applicable to all cabling Classes.

6.3.3.7 Direct current resistance unbalance

Replace the first paragraph with the following new paragraph:

The DC resistance unbalance requirements are applicable to all cabling Classes.

6.3.3.10 Propagation delay

Replace the first paragraph with the following new paragraph:

The propagation delay requirements are applicable to all cabling Classes.

6.3.3.11 Delay skew

Replace the first paragraph with the following new paragraph:

The delay skew requirements are applicable to all cabling Classes.

6.3.3.12.2 Unbalance attenuation, near-end

In the second paragraph, first sentence, replace the two instances of the word “systems” with “channels”.

Table 21 – TCL for channel for unscreened systems

In the title of Table 21, replace the word “systems” with “channels”.

At the end of footnote b, add the following new text:

“ f_u is the upper frequency of the Class.”

Table 25 – ELTCTL for channel for unscreened systems

In the title of Table 25, replace the word “systems” with “channels”.

Table 29 – Coupling attenuation for a channel for screened systems

In the title of Table 29, replace the word “systems” with “channels”.

6.3.3.13.2 Power sum alien NEXT

In the second paragraph, delete “, at maximum implementation,”.

Figure 7 – Link designations

Replace the figure graphic with the following new figure graphic: