

---

---

**Ophthalmic optics — Semi-finished  
spectacle lens blanks —**

**Part 2:  
Specifications for progressive-power  
and degressive-power lens blanks**

*Optique ophtalmique — Verres de lunettes semi-finis —  
Partie 2: Spécifications pour les verres progressifs et dégressifs*

STANDARDSISO.COM : Click to view the full PDF of ISO 10322-2:2016



STANDARDSISO.COM : Click to view the full PDF of ISO 10322-2:2016



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2016, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Ch. de Blandonnet 8 • CP 401  
CH-1214 Vernier, Geneva, Switzerland  
Tel. +41 22 749 01 11  
Fax +41 22 749 09 47  
copyright@iso.org  
www.iso.org

# Contents

	Page
Foreword.....	iv
Introduction.....	v
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Classification</b> .....	<b>1</b>
<b>5 Requirements</b> .....	<b>1</b>
5.1 General.....	1
5.2 Optical requirements for the finished surface.....	1
5.2.1 General.....	1
5.2.2 Tolerances on the surface power.....	2
5.2.3 Tolerances on the surface addition power for progressive-power lens blanks.....	2
5.3 Geometrical tolerances.....	2
5.3.1 Tolerances on the size.....	2
5.3.2 Tolerances on thickness.....	3
5.4 Orientation requirement for polarizing lens blanks.....	3
<b>6 Test methods</b> .....	<b>3</b>
6.1 General.....	3
6.2 Determination of surface power.....	3
6.3 Surface addition power measurement for progressive-power lens blanks.....	3
6.3.1 General.....	3
6.3.2 Measurement.....	4
6.4 Inspection method for material and surface quality.....	4
<b>7 Marking and identification</b> .....	<b>4</b>
7.1 Marking.....	4
7.1.1 Permanent marking.....	4
7.1.2 Optional non-permanent marking.....	4
7.2 Identification required on the package.....	4
7.3 Information to be made available.....	5
<b>8 Reference to this part of ISO 10322</b> .....	<b>5</b>
<b>Annex A (informative) Material and surface quality</b> .....	<b>6</b>
<b>Annex B (informative) Conversion of surface power tolerances from the refractive index of the lens blank to that of an instrument's fixed reference</b> .....	<b>7</b>
<b>Annex C (informative) Addition power measurement by transmission</b> .....	<b>8</b>
<b>Bibliography</b> .....	<b>9</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#).

The committee responsible for this document is ISO/TC 172, *Optics and photonics*, Subcommittee SC 7, *Ophthalmic optics and instruments*.

This fourth edition cancels and replaces the third edition (ISO 10322-2:2006), which has been technically revised.

ISO 10322 consists of the following parts, under the general title *Ophthalmic optics — Semi-finished spectacle lens blanks*:

- *Part 1: Specifications for single-vision and multifocal lens blanks*
- *Part 2: Specifications for progressive-power and degressive-power lens blanks*

## Introduction

Compared with previous editions of this part of ISO 10322, the scope now includes degressive-power semi-finished lens blanks.

STANDARDSISO.COM : Click to view the full PDF of ISO 10322-2:2016

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 10322-2:2016

# Ophthalmic optics — Semi-finished spectacle lens blanks —

## Part 2: Specifications for progressive-power and degressive-power lens blanks

### 1 Scope

This part of ISO 10322 specifies requirements for the optical and geometrical properties of semi-finished lens blanks with finished progressive-power and degressive-power surfaces.

### 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 7944, *Optics and optical instruments — Reference wavelengths*

ISO 13666, *Ophthalmic optics — Spectacle lenses — Vocabulary*

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 13666 apply.

### 4 Classification

Semi-finished lens blanks (shortened to lens blanks in the remainder of this part of ISO 10322 for easier reading) are classified according to the finished surface as follows:

- a) single-vision lens blanks;
- b) multifocal lens blanks;
- c) progressive-power and degressive-power lens blanks.

### 5 Requirements

#### 5.1 General

The tolerances shall apply at a temperature of  $23\text{ °C} \pm 5\text{ °C}$ .

#### 5.2 Optical requirements for the finished surface

##### 5.2.1 General

The optical tolerances shall apply to the manufacturer's stated values at the reference points of the lens blank at one of the reference wavelengths specified in ISO 7944.

The optical tolerances in [Table 1](#) and [Table 2](#) are expressed as surface power values, in dioptres, in the refractive index of the material of the lens blank being measured.

### 5.2.2 Tolerances on the surface power

The tolerances on the surface power as specified in [Table 1](#) shall apply at the distance reference point of progressive-power lenses and at the near reference point of degressive-power lenses and shall be measured using the method described in [6.2](#).

**Table 1 — Tolerances on the surface power**

Values in dioptres (D)

Surface power	Tolerance on the surface power	Tolerance on surface cylindrical power <sup>a</sup>
	$\frac{F_1 + F_2}{2}$	$ F_1 - F_2 $
≥0,00 and ≤10,00	±0,09	0,09
>10,00 and ≤15,00	±0,12	0,12

NOTE  $F_1$  and  $F_2$  are the maximum and minimum values of the surface power expressed in the refractive index of the material.

<sup>a</sup> Relative to zero, or to any intended surface cylindrical power of the lens blank's design.

### 5.2.3 Tolerances on the surface addition power for progressive-power lens blanks

The tolerances on the surface addition power as specified in [Table 2](#) shall apply at the reference points and shall be measured using the method described in [6.2](#).

**Table 2 — Tolerances on the surface addition power**

Values in dioptres (D)

Surface addition power	Tolerance
≤4,00	±0,12
>4,00	±0,18

## 5.3 Geometrical tolerances

### 5.3.1 Tolerances on the size

The sizes are classified as follows:

- a) nominal size ( $d_n$ ): dimension(s), in millimetres, indicated by the manufacturer;
- b) effective size ( $d_e$ ): actual dimension(s), in millimetres;
- c) usable size ( $d_u$ ): dimension(s), in millimetres, of the area that is optically usable:
  - 1) effective size,  $d_e$ :  
 $d_n - 1 \text{ mm} \leq d_e \leq d_n + 2 \text{ mm}$ ;
  - 2) usable size,  $d_u$ :  
 $d_u \geq d_n - 1 \text{ mm}$  for  $d_n \leq 65 \text{ mm}$ ;  
 $d_u \geq d_n - 2 \text{ mm}$  for  $d_n > 65 \text{ mm}$ .

The tolerance on usable sizes does not apply to lens blanks for lenses with a carrier curve, such as lenticulars.

### 5.3.2 Tolerances on thickness

#### 5.3.2.1 Centre thickness

The centre thickness, when measured at the geometric centre (unless otherwise stated by the manufacturer), shall be neither less than the minimum thickness stated by the manufacturer nor exceed this minimum thickness by more than 3 mm.

#### 5.3.2.2 Edge thickness

When measured at the point stated by the manufacturer, the edge thickness shall be neither less than the minimum thickness stated by the manufacturer nor exceed this minimum thickness by more than 3 mm.

### 5.4 Orientation requirement for polarizing lens blanks

For polarizing lens blanks intended for sun glare attenuation, the plane of transmission shall be aligned to the permanent alignment reference markings at  $90^\circ \pm 3^\circ$ .

## 6 Test methods

### 6.1 General

Alternative measurement methods are acceptable if shown to perform equivalently to the reference test methods in [6.2](#) to [6.4](#).

### 6.2 Determination of surface power

Surface power at the reference point shall be determined using a suitable instrument capable of measuring surface power, by reflection, with an accuracy that is appropriate to the tolerances listed in [Table 1](#).

The optical tolerances in [Table 1](#) are expressed as surface power values, in dioptres, in the refractive index of the material of the lens blank being measured.

NOTE 1 Some surface power instruments allow setting of the reference refractive index to match that of the actual lens blank being measured. Conversion might be required to establish the tolerance values if the lens blank is measured with equipment calibrated for a different reference refractive index (see [Annex B](#)).

NOTE 2 It might be necessary to use a device that limits the aperture of measurement. The recommended range for the measurement aperture is 4 mm to 8 mm.

### 6.3 Surface addition power measurement for progressive-power lens blanks

#### 6.3.1 General

Surface addition power shall be measured using a suitable instrument capable of measuring surface power, by reflection, with an accuracy that is appropriate to the tolerances listed in [Table 2](#). Measure the powers at the distance reference point and at the near reference point.

NOTE The test method for determining addition power requires the measurement of surface addition power.

When no surface measurement capability exists, an alternative method for addition power measurement using a focimeter is provided in [Annex C](#).

### 6.3.2 Measurement

The surface chosen for measurement shall be the progressive side. Measure the power at the near and distance reference points, and calculate the addition as the difference between the powers at these points. The powers at the distance and near reference points should be taken as the mean of the principal meridional surface powers.

### 6.4 Inspection method for material and surface quality

Material and surface quality can be assessed using the method in [Annex A](#).

## 7 Marking and identification

### 7.1 Marking

#### 7.1.1 Permanent marking

The lens blank shall be permanently marked on the finished surface with at least the following:

- a) alignment reference markings comprising two marks located 34 mm apart, equidistant to a vertical plane through the fitting point or prism reference point; in special cases, the alignment reference marking may be applied only after finishing the second surface;
- b) for progressive-power lens blanks, an indication of the addition power in dioptres (under the temporal alignment reference mark); in special cases, the addition power marking may be applied only after finishing the second surface;

For degressive-power lens blanks, if available in more than one degression power, an appropriate indication shall be given by the manufacturer;

- c) indicator of the manufacturer or supplier, or the trade name or trademark.

#### 7.1.2 Optional non-permanent marking

The following optional non-permanent marking is recommended:

- a) alignment reference marking;
- b) for progressive-power lens blanks, the indicator of the distance reference point;
- c) indicator of the near reference point;
- d) indicator of the fitting point;
- e) indicator of the prism reference point, where applicable.

### 7.2 Identification required on the package

The lens blank shall be supplied in a package. The package shall be labelled with at least the following information (see also [Clause 8](#)):

- a) nominal surface power, in dioptres;
- b) nominal surface cylindrical power, in dioptres, and orientation (if applicable);
- c) nominal size, in millimetres;
- d) colour (if not clear);
- e) identification of any coating;

- f) material of which the lens blank is made, its refractive index or the trade name indicating the material or equivalent;
- g) for progressive-power lens blanks, the addition power, in dioptres; for degressive-power lens blanks, if available in more than one degression power, an appropriate indicator;
- h) style designation or trade name or trademark;
- i) an indicator stating right or left lens (if applicable).

### 7.3 Information to be made available

The following information shall be available on request:

- a) minimum centre thickness, in millimetres, and, if not measured at the geometric centre, where it is measured (see [5.3.2.1](#));
- b) minimum edge thickness, in millimetres, and identification of the measurement point (see [5.3.2.2](#));
- c) radius of curvature both of the finished surface (measured at the distance reference point for progressive-power surfaces and at the near reference point for degressive-power surfaces) and of the unfinished surface, in millimetres;
- d) optical properties of the material;
- e) method of measurement of the addition power used by the manufacturer including reflection or transmission method, and if applicable, focimeter type;
- f) prism thinning (if applicable);
- g) centration chart for reconstruction of the non-permanent markings relative to the permanent markings;
- h) for surfaces with intended surface cylindrical power, the magnitude and orientation of the intended surface cylindrical power, and, if applicable, the tolerance on the direction of the cylinder axis.

## 8 Reference to this part of ISO 10322

If the manufacturer or supplier claims compliance with this part of ISO 10322, reference shall be made to ISO 10322-2, either on the package or in the available literature.

## Annex A (informative)

### Material and surface quality

#### A.1 Assessment

##### A.1.1 Finished surface

The lens blank should not exhibit any defect either internally or on the finished surface which might impair vision. Small isolated material and/or surface defects not likely to impair vision may be acceptable.


##### A.1.2 Unfinished surface

The surface quality of the unfinished surface should be sufficient to allow marking, inspection and measurement.

#### A.2 Test method

Carry out the inspection at a light/dark boundary and without the aid of magnifying optics. The recommended system is shown in [Figure A.1](#). Inspect the lens blank within a room with ambient lighting of about 200 lx. Use a source of at least 400 lm as an inspection lamp, for example a fluorescent tube of 15 W or a partly shaded 40 W incandescent clear lamp.

NOTE This observation is subjective and requires some experience.

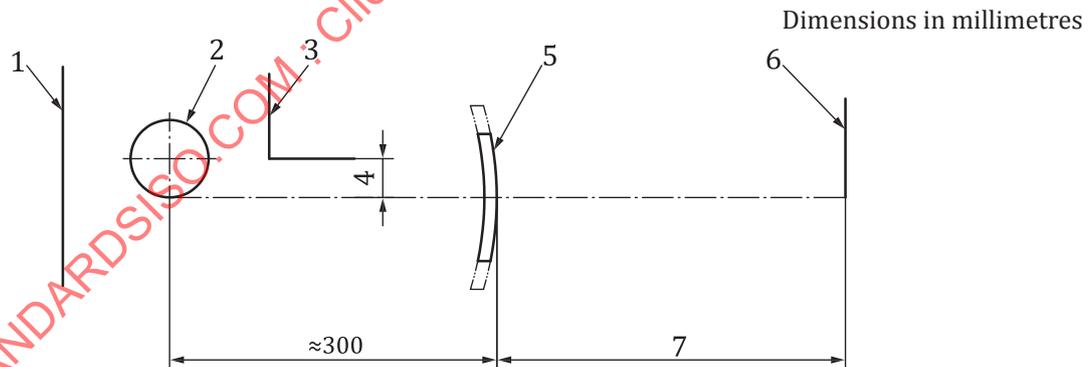

**Key**

- |   |                                   |   |                             |
|---|-----------------------------------|---|-----------------------------|
| 1 | matt black background (150 × 360) | 5 | movable lens blank          |
| 2 | light source, ≥400 lm             | 6 | plane of the observer's eye |
| 3 | diaphragm                         | 7 | unobstructed vision         |
| 4 | adjustable opaque mask            |   |                             |

NOTE The diaphragm is adjusted to shield the eye from the light source and to allow the lens blank to be illuminated.

**Figure A.1 — Recommended system for visually inspecting a lens blank for defects**