

Third edition
2019-10

Corrected version
2020-01

**Optics and photonics — Lasers and
laser-related equipment — Test
method for absorptance of optical
laser components**

*Optique et photonique — Lasers et équipements associés aux lasers
— Méthode d'essai du facteur d'absorption des composants optiques
pour lasers*

STANDARDSISO.COM : Click to view the full PDF of ISO 11551:2019



Reference number
ISO 11551:2019(E)

© ISO 2019

STANDARDSISO.COM : Click to view the full PDF of ISO 11551:2019



COPYRIGHT PROTECTED DOCUMENT

© ISO 2019

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	vi
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Symbols and units of measure.....	1
5 Preparation of test sample and measuring arrangement.....	2
6 Characteristic features of the laser radiation.....	3
7 Test procedure.....	4
7.1 General.....	4
7.2 Calibration.....	4
7.2.1 Calibration of the power signal.....	4
7.2.2 Calibration of the temperature signal.....	4
7.2.3 Calibration of the thermal response.....	4
7.2.4 Measurement of the background signal.....	5
7.3 Determining the absorptance.....	5
8 Evaluation.....	5
8.1 General.....	5
8.2 Elimination of drift.....	6
8.3 Exponential method.....	6
8.4 Pulse method.....	7
9 Test report.....	7
Annex A (informative) Effects changing absorptance.....	10
Annex B (informative) Influence of signal distortions.....	12
Annex C (informative) Algorithm for parameterizing the temperature data.....	15
Bibliography.....	16

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 172, *Optics and photonics*, Subcommittee 9, *Laser and electro-optical systems*.

This third edition cancels and replaces the second edition ISO 11551:2003 which has been technically revised.

The main changes compared to the previous edition are as follows:

- a) Introduction: The assumptions were revised in the second paragraph. Minor wording and example adjustment in third paragraph.
- b) [Clause 4](#): Table for symbols and units was corrected.
- c) [Clause 5](#): More detailed specification of environmental conditions for UV- and IR applications are provided in the second paragraph. ISO 7 specification was deleted.

In the fourth paragraph, [Annex A](#) is explicitly mentioned for the dependence of absorption on other test parameters.

In the fifth paragraph, [Annex B](#) is explicitly mentioned to account for the critical issue of finite heat conductivity.

- d) In [7.2.3](#): In the first paragraph, the calibration procedure is specified in more detail, including the consideration of the heating scheme for thick samples.

Note 1 is complemented by the restriction for thin samples.

Note 2 is complemented with the consideration of heating scheme for finite heat conduction.

- e) In [7.3](#): In the first paragraph the specifications for the ambient temperature drift were clarified.

The requirements to the total temperature rise during heating were generalized.

In the third paragraph the terminology “pre-irradiation” was replaced by “drift record”. The description of the duration of the cooling period was complemented.

- f) In [8.1](#): In the first paragraph “heat capacity” was replaced by “specific heat capacity”.
- g) In [A.1](#): “irradiation dose” added as influencing parameter.
- h) In [A.3](#): Generalization of nonlinear absorption dependencies.
- i) In [B.3](#): More detailed comments on the convergence of the temperature curves in [Figure B.1](#). Correction of [Formulae \(B.2\)](#) and [\(B.3\)](#). An additional paragraph with explanations for thick test samples, including two references.

This corrected version of ISO 11551:2019 incorporates the following corrections:

- In [7.2.3](#), [Formulae \(B.1\)](#), [\(B.2\)](#) and [\(B.3\)](#), the symbol " α " has been changed into " a ".
- Two signs have been corrected in [Formula \(C.4\)](#) to read " $-B_{exp}$ " and " $-t_k$ " instead of " B_{exp} " and " t_k ".

STANDARDSISO.COM : Click to view the full PDF of ISO 11551:2019

Introduction

To characterize an optical component, it is important to know its absorptance. When radiation impinges upon a component, a part of that radiation is absorbed, increasing the temperature of the component. In this document only the part of the absorbed power/energy, that is converted into heat, is measured. If enough energy is absorbed, the optical properties of the component can change, and the component can even be destroyed. Absorptance is the ratio of the radiant flux absorbed to the radiant flux of the incident radiation.

In the procedures described in this document, the absorptance is determined calorimetrically as the ratio of power or energy absorbed by the component to the total power or energy, respectively, impinging upon the component. The assumption is made that the absorptance of the test sample is constant within the temperature fluctuations experienced by the component during the measurement.

For most optical bulk materials, the absorptance depends on the position of the irradiating beam on the sample surface. Several infrared materials exhibit a strong dependence of absorptance on temperature, especially at high temperatures.

STANDARDSISO.COM : Click to view the full PDF of ISO 11551:2019

Optics and photonics — Lasers and laser-related equipment — Test method for absorptance of optical laser components

1 Scope

This document specifies procedures and techniques for obtaining comparable values for the absorptance of optical laser components.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 11145, *Optics and photonics — Lasers and laser-related equipment — Vocabulary and symbols*

ISO 14644-1:2015, *Cleanrooms and associated controlled environments — Part 1: Classification of air cleanliness by particle concentration*

ISO 80000-7, *Quantities and units — Part 7: Light and radiation*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 11145 and ISO 80000-7 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at <https://www.iso.org/obp>

— IEC Electropedia: available at <http://www.electropedia.org/>

3.1

absorptance

a

ratio of the radiant flux absorbed to the radiant flux of the incident radiation

Note 1 to entry: The definition of absorptance used for this document is limited to absorptance processes which convert the absorbed energy into heat. For certain types of optics and radiation, additional non-thermal processes can result in absorption losses which will not be detected by the test procedure described here (see [Annex A](#)).

4 Symbols and units of measure

Symbol	Term	Unit
C_{eff}	Thermal capacity of test sample, holder, etc.	J/K
c_p	Specific heat capacity of test sample	J/(kg·K)
$d_{\sigma_x}, d_{\sigma_y}$	Beam width on test sample	mm
m_i	Mass of test sample, holder, etc.	kg
P	cw power	W

Symbol	Term	Unit
P_{av}	Average laser power for continuous pulse mode operation	W
P_{pk}	Typical peak power for repetitive pulse mode operation	W
t_B	Duration of irradiation	s
Δt	Time interval	s
T_{amb}	Ambient temperature	K
ΔT	Temperature difference	K
a	Absorptance	1
β	Angle of incidence	Rad
γ	Thermal loss coefficient	1/s
λ	Wavelength	nm
κ	Heat conductivity	W/(mK)
η	Mass density	kg/m ³
Q	Heat source	W/m ³

5 Preparation of test sample and measuring arrangement

Storage, cleaning and the preparation of the test samples are carried out in accordance with the manufacturer's instructions for normal use.

The environment of the testing place shall be adapted to the application and test wavelength. It should consist of dust-free filtered air with less than 50 % relative humidity. The residual dust shall be reduced in accordance with cleanroom class 7 as defined in ISO 14644-1:2015. However, some specific spectral ranges might require nitrogen purged environments (deep UV) or zero humidity (several IR wavelengths). Nitrogen quality for the deep UV range should be at 99,999 % or higher. If these conditions cannot be supplied, absorption within the surrounding atmosphere will be included in the test result. An environment free from draughts is very important in order to keep thermal disturbances and heat loss by convection as small as possible. Measurements in ambient atmosphere and vacuum can have different influences on the measured absorptance.

A laser shall be used as the radiation source. To keep errors as low as possible, the laser power chosen for measurements is as high as possible but without causing any deterioration to the component.

Wavelength, angle of incidence and state of polarization of the laser radiation used for the measurement shall correspond to the values specified by the manufacturer for the use of the test sample. If also ranges are accepted for these three quantities, any combination of wavelength, angle of incidence and state of polarization may be chosen from those ranges. The absorption of an optical component can depend on further parameters, e.g. power density or irradiation dose. In such cases, the measurement sequence should be chosen individually. For more details, refer to [Annex A](#).


The test sample is mounted in a suitable holder. It is preferable to mount the sample in a manner that minimizes any thermal contact between the sample and the holder. In this arrangement, the thermal sensor is attached directly to the sample surface. Reproducible thermal contact between the thermal sensor and the sample surface is important. Also, care should be taken to maintain constant thermal impedance between the sample and the holder. Accurate calibration is critically dependent on the location of the thermal sensor, on the material the sample is made of, and on the sample geometry. Refer to [Annex B](#) for a detailed discussion of these considerations.

It can be difficult to attach the thermal sensor to a small test sample or a sample having an irregular shape. Such a sample is mounted to the holder in a manner that maximizes thermal contact between the sample and the holder, while the thermal sensor is attached to or integrated into the holder. Reproducible thermal contact between the thermal sensor and the holder is important. Also, care should be taken to maintain constant thermal conductance between the sample and the holder.

In order to increase the precision of the measurements, the sample should be mounted inside a chamber designed for thermal shielding, with apertures for the laser beam. Special attention shall be given to ensure that the temperature measurement itself does not cause a change of the sample temperature.

Suitable diaphragms should be placed in the beam path in front of and behind the test sample to ensure that only the test sample is irradiated by the measuring beam and that reflected or stray radiation will not strike the holder or the chamber walls. The number of transmissive optics employed for beam guiding should be minimized in order to reduce possible distortions by multi-reflections or scattered radiation. The transmitted and reflected partial beams shall be directed on to beam dumps with minimized back scatter.

Figure 1 shows a schematic measuring arrangement. The curved folding mirror M1 is recommended for imaging the laser output window on to the sample in order to avoid diffracted radiation influencing the measurement.

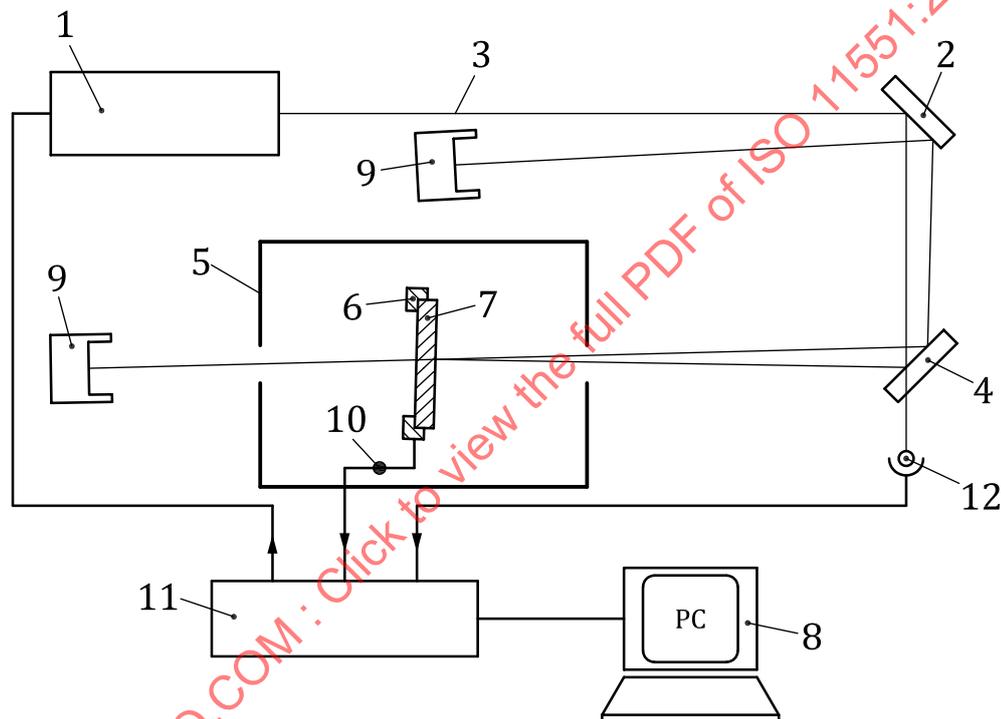

Key

1	laser	7	test sample
2	mirror M1	8	personal computer
3	optical axis	9	beam stop
4	mirror M2	10	thermal sensor
5	test chamber	11	control unit
6	sample holder	12	power detector

Figure 1 — Typical arrangement for measurement of the absorptance

6 Characteristic features of the laser radiation

The following physical quantities are needed for characterizing the laser radiation used for the test:

- wavelength, λ ;
- angle of incidence, β ;
- state and degree of polarization;

- beam widths on the test sample, $d_{\sigma x}$, $d_{\sigma y}$;
- average power, P_{av} , for cw or continuously pulsed lasers;
- typical peak power, P_{pk} , and pulse energy Q in the case of continuously pulsed lasers;
- duration of irradiation, t_B .

7 Test procedure

7.1 General

The following auxiliary tests shall be performed on a regular basis and whenever the measuring arrangement has been altered.

7.2 Calibration

7.2.1 Calibration of the power signal

Calibrate the power signal by placing a calibrated laser power detector at the location of the test components and, in order to obtain correct calibration, compare the measured laser power to the signal of the power monitor used during absorptance tests.

7.2.2 Calibration of the temperature signal

Calibrate the temperature signal by fixing a test sample, to which a calibrated thermal sensor is attached, to the sample holder. Compare the temperature signals of this calibrated sensor and the sensors used during absorptance tests while varying the ambient temperature slowly over the linearity range of the temperature detectors at the typical test temperature.

7.2.3 Calibration of the thermal response

For certain types of sample materials and geometries, the temperature rise induced by the absorbed heat may differ from the theoretical response expected for ideal materials having infinite thermal conductivity. In these cases, a correction factor f_c shall be determined, which compensates for the influence of such phenomena on the absorptance test result. f_c is unity if the influence of limited thermal conductivity can be neglected. In order to derive a correct value for f_c , the heating scheme of the calibration routine needs to be consistent with the heating characteristic of the samples to be tested. Surface absorbers shall be related to a correction factor derived from a calibration based on surface heating. And a bulk absorber shall be corrected with a bulk heated calibration sample.

For calibration, a reference sample of known absorptance, which is identical to the samples under investigation with respect to substrate geometry and thermal diffusivity, is tested for absorptance as described below. The irradiation time and evaluation method used for calibration shall be the same as for the sample under test.

Depending on the evaluation method used for the absorptance test, the correction coefficient can be calculated by substituting the value of the known calibration sample absorptance for a in [Formula \(2\)](#) (see [8.3](#)) or [Formula \(5\)](#) (see [8.4](#)), and solving for f_c .

A known absorptance can be achieved by applying a thin, high-absorbing coating to the sample surface area that is exposed to irradiation. High absorptance values can be determined with sufficient accuracy, e.g. by measuring the fraction of transmitted, reflected and scattered radiation. For absorptance testing of samples with high absorptance values, the laser power should be suitably attenuated in order to avoid damage to the samples and to ensure that the resulting temperature rise is in the same order of magnitude as the temperature which is achieved for typical measurements. This procedure applies only for samples of high surface absorption, where bulk absorption can be neglected.

As an alternative to irradiating a calibration sample of known absorptance with the laser beam, the thermal energy may be deposited electrically in the test sample by attaching an electric resistor to the tested surface. The absorbed power is given by RI^2 , where R is the electrical resistance and I is the electric current during “irradiation”. Care should be taken to ensure good thermal contact between resistor and sample. Furthermore, especially in the case of samples with low thermal conductivity, the area of the resistor should match the area irradiated by the laser beam under normal test conditions. This procedure can in principle be applied to both surface and bulk absorbing samples. Care should be taken to ensure that the heating scheme of the calibration sample is close or identical to the expected heating scheme of the test samples.

7.2.4 Measurement of the background signal

For maximum accuracy and suppression of possible signal distortions, the imaging and alignment of the laser beam shall be optimized. A measurement with an empty holder or with an absorptance-free component can be used to verify that the measuring arrangement is not influenced by reflected or stray radiation. The amplitude of the temperature fluctuations during the test interval shall be at least one order of magnitude below the temperature rise occurring during an absorptance test.

7.3 Determining the absorptance

The absorptance of optical components is determined calorimetrically by means of a measuring arrangement as shown in [Figure 1](#). Before measurement commences, thermal equilibrium shall be established, so that the ambient temperature drift is approximately linear and the temperature noise (standard deviation) is at least one order of magnitude below the maximum temperature rise induced by irradiation. The maximum temperature rise during the test should be in accordance to the linearity of the temperature detector.

If the absorptance is dependent either on the power or energy density of the impinging radiation, or the irradiation dose, this shall be noted in the test report. The test shall be performed under the conditions of the foreseen use of the components.

The test is performed in three successive intervals:

- the drift recording interval $[t_0, t_1]$ (at least 30 s);
- the heating interval $[t_1, t_2]$ ($t_B = t_2 - t_1 = 5 \text{ s to } 300 \text{ s}$) during which the laser beam impinges on the test sample surface;
- the cooling interval of at least 200 s.

For test samples with high thermal losses, the irradiation should end significantly before the temperature rise saturates due to a balance of absorbed power and thermal loss.

During the test, the sample temperature signal $T(t)$ and the laser power signal $P(t)$ are recorded. The resulting calorimetric data sets $[t_k, T(t_k)]$ and $[t_k, P(t_k)]$ with k , enumeration index, are stored for the evaluation of the absorptance.

8 Evaluation

8.1 General

The mass, m_i , of components heated during irradiation (test sample, holder, etc.) is determined by weighing. The specific heat capacity c_{pi} is taken from tables.

For the calculation of absorptance, two alternative methods can be used: the exponential method or the pulse method. In general, the pulse method is applicable for irradiation times up to 120 s, while the exponential method can be applied for irradiation times from 60 s. Which method is preferable depends also on the individual properties of the tested specimen and the circumstances of the test. In

many cases it can be helpful to apply both methods and gain additional information on the uncertainty in the result by comparing the two results.

8.2 Elimination of drift

Preceding the calculation of absorptance, the calorimetric data shall be analysed with respect to the possible occurrence of temperature drift phenomena. In the presence of temperature drift, a linear fit shall be performed to the temperature data sampled before irradiation. The approximated drift influence described by the resulting linear fit function is eliminated by subtracting the extrapolated fit values from the raw temperature data recorded during the test.

8.3 Exponential method

Determine the parameters A_h , B_h , γ_h by fitting an exponential function to the temperature data $[t_k, T(t_k)]$ recorded during the irradiation interval (heating period of the component):


$$\sum [T(t_k) - A_h - B_h \exp(-\gamma_h t_k)]^2 = \min \tag{1}$$

NOTE γ_h corresponds to the thermal loss coefficient of the heated system, which describes the cooling process in absence of heat sources as $\dot{T} = -\gamma(T - T_{amb})$. If γ_h is known from earlier measurements or other sources, the fitting procedure can be simplified by fixing γ_h at this value. A useful algorithm for parametrizing the temperature data to determine the fit parameters by linear regressions is given in [Annex C](#).

Calculate the absorptance from these fit parameters as

$$a = \frac{f_c \gamma_h A_h \sum_i m_i c_{pi}}{P} \tag{2}$$

In case of pulsed laser operation, substitute P by P_{av} . See [Figure 2](#).

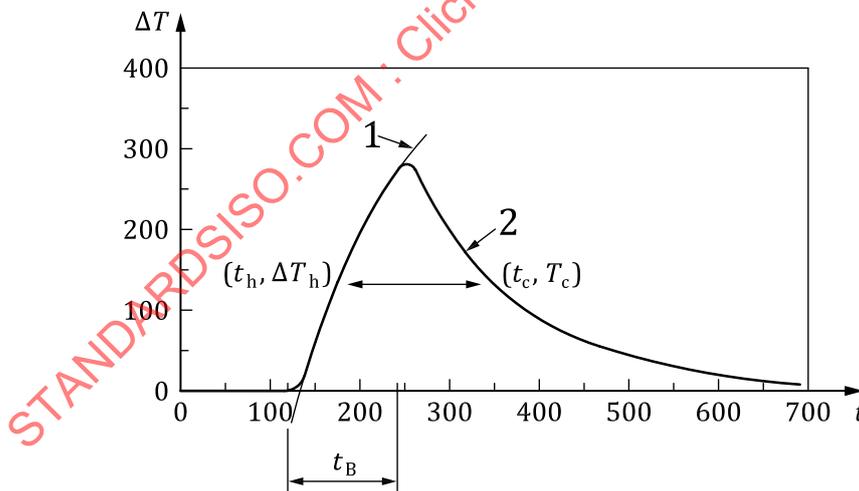

Key

- 1 fit
- 2 relative temperature

Figure 2 — Example for exponential method evaluation

8.4 Pulse method

The temperature decay curve after irradiation shall be extrapolated graphically to the time $t_1 + \frac{t_B}{2}$ (middle of irradiation interval), providing the extrapolation temperature T_{ext} . It is recommended to carry out this extrapolation by calculating the best fit parameters A_c , B_c , γ_c , performed on the temperature data with negative slope recorded after irradiation:

$$\Sigma [T(t_k) - A_c - B_c \exp(-\gamma_c t_k)]^2 = \min \quad (3)$$

and to calculate the extrapolation temperature T_{ext} as

$$T_{\text{ext}} = A_c + B_c \exp\left(-\gamma_c \frac{t_1 + t_2}{2}\right) \quad (4)$$

The absorptance is calculated as

$$a = \frac{f_c T_{\text{ext}} \sum_i m_i c_{pi}}{P t_B} 0,5 \gamma_c t_B / \sinh(\gamma_c t_B / 2) \quad (5)$$

In case of pulsed laser operation, substitute P with P_{av} . See [Figure 3](#).

$$0,5 \gamma_c t_B / \sinh(\gamma_c t_B / 2)$$

NOTE The term $0,5 \gamma_c t_B / \sinh(\gamma_c t_B / 2)$ can be approximated by unity, if $\gamma_c t_B < 0,5$ is valid. If $0,5 \leq \gamma_c t_B \leq 2$ the term $0,5 \gamma_c t_B / \sinh(\gamma_c t_B / 2)$ can be approximated by $(1 - \gamma_c^2 t_B^2 / 24)$. For $\gamma_c t_B > 2$ [Formula \(5\)](#) is applicable.

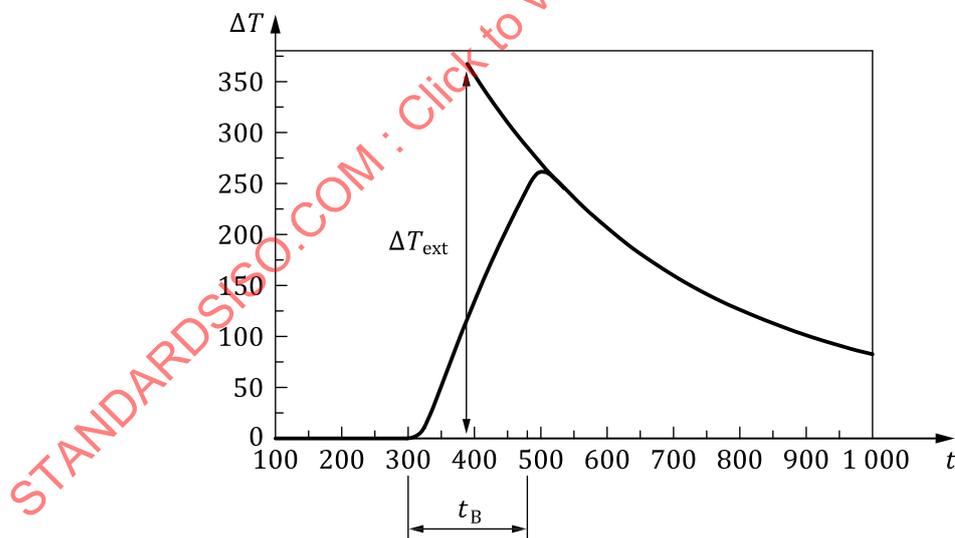


Figure 3 — Example for pulse method evaluation

9 Test report

The test report shall contain the following information.

- a) General information;
 - 1) test has been performed in accordance with ISO 11551:2019
 - 2) date of test;

- 3) name and address of test organization;
- 4) name of individual performing the test;
- b) Information concerning the test sample (if available);
 - 1) type of test sample;
 - 2) manufacturer of test sample;
 - 3) part identification, date of production;
 - 4) specifications by the manufacturer concerning storage, cleaning, etc.;
 - 5) specifications by the manufacturer for normal use;
- c) Information concerning the test facility;
 - 1) beam source;
 - type of beam source;
 - manufacturer;
 - manufacturer's model designation;
 - 2) description of other relevant test equipment;
- d) Test conditions;
 - 1) wavelength;
 - 2) operating mode cw/pulsed;
 - 3) source parameter settings;
 - output power or energy (irradiation time);
 - pulse energy;
 - pulse duration;
 - pulse repetition rate;
 - 4) spatial and/or temporal beam profile, if necessary;
 - 5) beam width on test sample;
 - 6) angle of incidence;
 - 7) polarization;
 - 8) environmental conditions;
 - 9) cleaning;
 - 10) method of mounting of optical component;
- e) Information concerning testing and evaluation;
 - 1) test method used;
 - 2) surface quality/imperfections/contamination;
- f) Comments concerning effects of changing absorptance, if relevant;

- g) Error budget;
- h) Test result(s).

STANDARDSISO.COM : Click to view the full PDF of ISO 11551:2019

Annex A (informative)

Effects changing absorptance

A.1 General

The absorptance measured according to the methods given in this document is, in certain cases, dependent on the parameters of the measurement (power, power density, irradiation time, irradiation dose, etc.). Furthermore, absorptance can be influenced by ageing of the specimen and nonlinear behaviour. These effects can be observed especially for measurements with UV radiation. The following mechanisms can contribute to the measured absorptance.

A.2 Colour centre formation

Especially in the UV spectral range, colour centres can be formed by irradiation. In this case the absorptance increases with time and a saturation can occur after irradiation with a certain radiation dose. Some colour centres can be annealed by heating the component resulting in a reduction of absorptance.

In the case of coated optics, high power irradiation can cause structural changes in optical coatings (e.g. post-oxidation). This can lead either to an increase or to a decrease of absorptance.

Thus, a single measurement reflects the absorptance only at the time the measurement is performed. For a detailed analysis of the data, the history of the sample (parameters of former irradiation cycles etc.) is important.

A.3 Nonlinear absorption

In many samples, absorptance increases reversibly with increasing power density due to multi-photon absorption. The change depends on the wavelength of the radiation and can be large especially for UV radiation. For ultra-short pulses it can also influence absorptance in the VIS and NIR spectral range. For the power densities of practical use, multi-photon absorption is of importance, leading to a linear and for some materials also to a nonlinear increase of absorptance with increasing power density.

If nonlinear absorption is assumed to significantly influence the absorptance of a sample, absorptance should be measured for a variety of power densities. In most cases, the obtained data are fitted linearly as a function of the power density. The linear absorptance is then given by the intercept with the ordinate, the nonlinear absorption is given by the slope of the linear fit. In some cases, for example for fused silica at 193 nm, a nonlinear fit has to be applied.

A.4 Further parameters influencing the measured absorptance value

Additional effects should be considered, which can change the measured absorptance value of the specimen:

- high power irradiation can cause cleaning effects on the surface of optical components, reducing the total absorptance;
- high power irradiation can cause degradation or ageing of optical components and optical coatings; in this case the absorptance can increase with time and with power density;

- laser induced contamination can occur in dependence on the atmospheric conditions and surrounding components, increasing in general the absorptance;
- cleaning procedures that are not appropriate for the specimen can cause an increase of absorptance.

STANDARDSISO.COM : Click to view the full PDF of ISO 11551:2019

Annex B (informative)

Influence of signal distortions

B.1 Influence of the resolution of temperature measurement

It is important to be sure that the temperature rise is significantly higher than the resolution of the temperature measurement.

B.2 Influence of scattered radiation

Scattered radiation emerging from the component itself, or the coating, may hit the temperature sensor. Similar to the scattered radiation coming from the beam-forming components, this direct heating of the sensors can lead to an overestimation of the absorption. In particular, this is important for the UV range.

B.3 Influence of low thermal conductivity in the specimen

The standard evaluation methods given for the determination of the absorptance are based on a fundamental physical model, assuming a small temperature increase and a homogeneous temperature T_s of sample and holder at all times. For such a system, the temperature dynamics are described by the formula

$$\frac{dT}{dt} = \frac{aP_{av}}{C_{eff}} - \gamma T \quad (B.1)$$

which renders the following exponential functions as solutions for the temperature signal $T(t)$ during irradiation:

$$T(t) = T(t_1) + \frac{aP}{\gamma C_{eff}} \{1 - \exp[-\gamma(t - t_1)]\} \quad (B.2)$$

And after irradiation

$$T(t) = T(t_1) + \frac{aP}{\gamma C_{eff}} [\exp(\gamma t_2) - \exp(\gamma t_1)] \exp(-\gamma t) \quad (B.3)$$

If laser components are constituted of materials with low thermal conductivities, the temperature dynamics during an absorptance measurement cannot be accurately described by this simple model of homogeneous temperature distribution. Instead, the finite sample thermal conductivity can be taken into account by solving a three-dimensional formula of the form

$$\nabla(\kappa/c_p \nabla T) + Q(x, y, z)/c_p = \eta \dot{T} \quad (B.4)$$

where


η is the mass density;

κ is the thermal conductivity;

Q is the heat source.

The boundary conditions at the sample surfaces are determined by the thermal convection and radiation losses and by the thermal coupling to the holder and thermal sensors. Below an example is presented to illustrate the effects of limited thermal conductivity on laser calorimetry.

For a thin cylindrical test sample (absorptance: 1, thickness 3 mm, diameter 25 mm), the temperature signals have been simulated for a range of thermal diffusivities and for different radial locations of the thermal sensors. The beam diameter was assumed to be much smaller than the diameter of the sample. [Figure B.1](#) shows the calculated temperature behaviour for one thermal diffusivity and for different radial locations of the temperature sensor. For comparison, the temperature curve for infinite thermal conductivity is included in the plot (0D model).

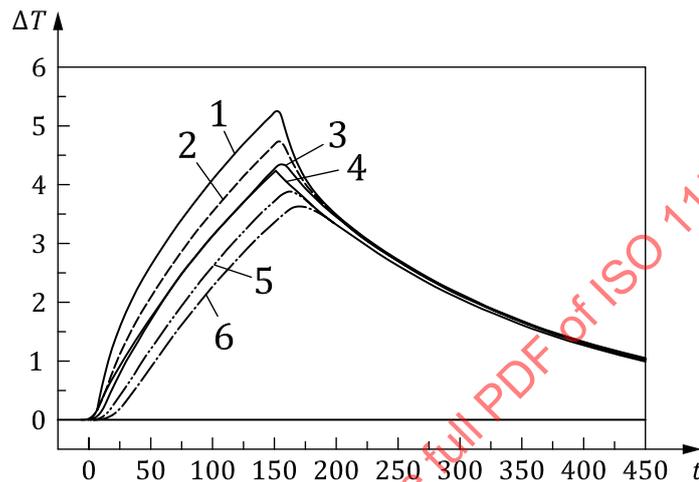

Key

- 1 $r = 5$ mm
- 2 $r = 6$ mm
- 3 $r = 7$ mm
- 4 0D model
- 5 $r = 9$ mm
- 6 $r = 12$ mm

Figure B.1 — Dependence of temperature signal and thermal sensor location

It can be seen, that with increasing distance of the temperature sensor from the laser beam (the sample centre), the temperature rise is delayed. Also, the maximum temperature is smaller.

After irradiation and a characteristic time delay, all curves converge.

Obviously, there is an optimum location of the thermal sensor with respect to the best similarity between theoretical curves regarding thermal conductivity and the infinite thermal conductivity model (for this example, approximately 7 mm.)

Further theoretical calculations for other ratios of thermal conductivity to specific heat capacity were performed. The absorptance values determined from the simulated data are plotted in [Figure B.2](#). The absorptance results are given relative to the theoretical absorptance value for infinite thermal conductivity.