

---

---

**Nuclear energy — Radiation protection —  
Individual thermoluminescence dosimeters  
for extremities and eyes**

*Énergie nucléaire — Radioprotection — Dosimètres individuels  
thermoluminescents pour yeux et extrémités*

STANDARDSISO.COM : Click to view the full PDF of ISO 12794:2000



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 12794:2000

© ISO 2000

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 734 10 79  
E-mail [copyright@iso.ch](mailto:copyright@iso.ch)  
Web [www.iso.ch](http://www.iso.ch)

Printed in Switzerland

## Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope .....	1
2 Normative references .....	1
3 Terms and definitions .....	2
4 Units .....	5
5 General test conditions.....	5
6 Classification.....	5
7 Performance requirements.....	6
8 Test methods.....	6
9 Certification .....	6
Annex A (normative) Reference conditions and standard test conditions.....	8
Annex B (normative) Confidence limits.....	9
Annex C (normative) Performance tests.....	12
Annex D (informative) Determination of evaluated value ( <i>E</i> ) from readout values .....	17
Annex E (normative) Conversion tables.....	18
Bibliography.....	20

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 12794 was prepared by Technical Committee ISO/TC 85, *Nuclear energy*, Subcommittee SC 2, *Radiation protection*.

Annexes A, B, C and E form integral parts of this International Standard. Annex D is for information only.

STANDARDSISO.COM : Click to view the full PDF of ISO 12794:2000

## Introduction

This International Standard covers dosimeters for the eyes and extremities.

This International Standard should be used in conjunction with IEC 1066:1991, which provides performance criteria and tests for thermoluminescence dosimetry systems comprising dosimeters, readers, ancillary equipment and procedures for converting light output into dose, for the assessment of personal or environmental doses, excluding extremities. It also includes some performance criteria and tests for thermoluminescent detectors and thermoluminescence dosimeters where these criteria are dependent on the characteristics of the detectors or dosimeters, rather than on the reader or ancillary equipment.

This document was prepared and discussed by Working Group WG 7 of ISO/TC85/SC2 following meetings in Paris in August 1988, Moscow in May 1990, Rome in November 1991, Paris in September 1992 and London in October 1993. It was not possible to hold a WG meeting in Orlando in October 1994. The draft was agreed at the Paris meeting by the working group and circulated by the Secretariat as a CD. A further meeting of the WG was held in London in October but the results of the voting were not available until later in October 1995. A final draft, dated February 1996, incorporating comments included with the results of the voting on ISO/CD (WI 7-2.07.1), circulated as ISO/TC85/SC2 N 475 in October 1993, was agreed by WG 7 in Albuquerque in February 1996. The comments following circulation as a DIS were considered by the WG in July 1997 and this International Standard incorporates those that were agreed upon.

STANDARDSISO.COM : Click to view the full text of ISO 12794:2000



# Nuclear energy — Radiation protection — Individual thermoluminescence dosimeters for extremities and eyes

## 1 Scope

This International Standard provides performance criteria and tests for determining the performance of thermoluminescence dosimeters intended to be used for the measurement of radiation doses to the eyes and extremities (fingers, and limbs defined as hands, feet, forearms including the elbow, and leg including the patella), for photons from 15 keV to 3 MeV and beta radiation from 0,5 MeV to 3 MeV. It is conditional upon the use of an appropriate reader, procedures and ancillary equipment. It does not cover information access and data processing.

This International Standard provides performance criteria and tests for dosimeters intended to measure dose equivalent at depths of  $7 \text{ mg}\cdot\text{cm}^{-2}$  in tissue for fingers and limbs and  $300 \text{ mg}\cdot\text{cm}^{-2}$  in tissue for the eyes, including provision for the use of dosimeters only intended to be used once. Appropriate phantoms and dose conversion coefficients are recommended but others are not precluded.

In all cases, performance is assessed under laboratory conditions which may not adequately simulate conditions actually experienced in personal dosimetry. For example, it may be necessary to sterilize dosimeters for medical applications. Therefore, caution is necessary in applying the results of these performance tests in real situations.

## 2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 31-0, *Quantities and units — Part 0: General principles*.

ISO 4037-3:1999, *X and gamma reference radiation for calibrating dosimeters and dose-rate meters and for determining their response as a function of photon energy — Part 3: Calibration of area and personal dosimeters and the measurement of their response as a function of energy and angle of incidence*.

ISO 6980, *Reference beta radiations for calibrating dosimeters and dose-rate meters and for determining their response as a function of beta-radiation energy*.

### 3 Terms and definitions

For the purposes of this International Standard, the following terms and definitions apply.

#### 3.1

**thermoluminescence**  
**radiothermoluminescence**  
**TL**

property exhibited by certain substances, namely the emission of light, which is induced by irradiation when the substance is heated following exposure to ionizing radiation or UV

NOTE Strictly speaking, the property should be referred to as radiothermoluminescence but the abbreviated form thermoluminescence is usually adequate.

#### 3.2

**thermoluminescent material**  
**TL material**

substance exhibiting the property of thermoluminescence

#### 3.3

**thermoluminescent detector**  
**TL detector**  
**detector**

specified quantity of TL material, or such material incorporated with other non-luminescent material into a matrix, defined by mass, shape or size or the mass of material incorporated in the matrix

#### 3.4

**thermoluminescence dosimeter**  
**TL dosimeter**  
**dosimeter**

passive device consisting of one or more TL detectors, which may be mounted in a holder (appropriate for the application), intended to be worn on a person's body or placed in an environment for the purpose of assessing the appropriate dose equivalent at or near the position where it is placed

#### 3.5

**thermoluminescence dosimeter reader**  
**TL dosimeter reader**  
**reader**

instrument used to measure the light emitted from the detectors in thermoluminescence dosimeters; consisting essentially of a heating device, a light measuring device and the associated electronics

#### 3.6

**extremity dosimeter**

dosimeter intended to be worn on the finger or limb [hands, feet, forearms (including the elbow), and lower leg (including the patella)]

#### 3.7

**eye dosimeter**

dosimeter intended to be worn near the eyes

#### 3.8

**reusable dosimeter**

dosimeter intended to be reused, as opposed to one which is discarded after one use

NOTE When used in medical applications, appropriate sterilization may be necessary.

**3.9****batch**

collection of detectors or dosimeters made to a specific design or specification and intended to have the same performance characteristics consistent with the appropriate requirements of this International Standard

**3.10****annealing**

controlled thermal treatment of a TL detector or dosimeter during or after readout

**3.11****prepare****reprepare**

normal treatment of annealing, cleaning, etc. which the dosimeters or detectors are intended to be subjected to in routine use

**3.12****readout**

process of measuring the light emitted when a TL detector or dosimeter is heated in a reader

**3.13****readout value**

*m*

value indicated by a TL reader after readout of a detector or dosimeter expressed in units appropriate to the output of the reader

**3.14****absorbed dose**

*D*

quotient of  $d\bar{\epsilon}$  by  $dm$ , where  $d\bar{\epsilon}$  is the mean energy imparted by ionizing radiation to matter of mass  $dm$ .

NOTE 1 The special name for the unit of absorbed dose is gray (Gy) ( $1 \text{ Gy} = 1 \text{ J}\cdot\text{kg}^{-1}$ ). In this International Standard, absorbed doses are specified in grays.

NOTE 2 Where no ambiguity could be involved, the term "absorbed dose" is abbreviated to "dose".

**3.15****kerma**

*K*

quotient of  $d\bar{\epsilon}_{\text{tr}}$  by  $dm$ , where  $d\bar{\epsilon}_{\text{tr}}$  is the sum of the initial kinetic energies of all the charged ionising particles liberated by uncharged ionising particles in a matter of mass  $dm$ :

$$K = \frac{d\bar{\epsilon}_{\text{tr}}}{dm} \quad (1)$$

**3.16****dose equivalent**

*H*

product of *D* and *Q* at the point of interest in tissue where *D* is the absorbed dose and *Q* is the quality factor:

$$H = DQ \quad (2)$$

NOTE The SI unit for both *D* and *H* is joule per kilogram. The special name for the unit of dose equivalent is the sievert (Sv): ( $1 \text{ Sv} = 1 \text{ J}\cdot\text{kg}^{-1}$ ).

**3.17****personal dose equivalent**

$H_p(d)$

dose equivalent in soft tissue below a specified point at an appropriate depth, *d*

NOTE The SI unit for  $H_p(d)$  is joule per kilogram. The special name is sievert (Sv) ( $1 \text{ Sv} = 1 \text{ J}\cdot\text{kg}^{-1}$ ).

**3.18  
evaluated value**

*E*

value of the quantity of interest, e.g. dose equivalent ( $H$ ), air kerma ( $K_a$ ), free-air absorbed dose ( $D_a$ ), obtained by applying the appropriate evaluation coefficient ( $F_e$ ) to the readout value or values ( $m$ )

**3.19  
conventional true value**

*C*

best estimate of the quantity of interest at the point of measurement, e.g. dose equivalent ( $H$ ), air kerma ( $K_a$ ), free air absorbed dose ( $D_a$ )

NOTE This is a widely used standardized term. The grammatically correct synonymous term is Conventionally True Value.

**3.20  
evaluation coefficient**

$F_e$

factor or collection of factors, used to convert the readout value or values, ( $m$ ), to the evaluated value of interest ( $E$ )

NOTE See annex D.

**3.21  
residue**

readout signal obtained on second readout following normal readout and annealing procedures

**3.22  
conversion coefficient**

$F_e$

factor used to convert from air kerma or free-air absorbed dose to the corresponding dose equivalent

NOTE See annex E.

**3.23  
response**

*R*

quotient of the evaluated value and the conventional true value

**3.24  
self-irradiation**

irradiation of the detector due to radioactive impurities contained in the dosimeter holder or detector itself

**3.25  
phantom**

specified object used to simulate the human body or parts thereof in terms of its scattering and absorption of gamma and beta radiation

**3.26  
zero point**

evaluated value of an unirradiated prepared dosimeter or detector

**3.27  
reader background**

evaluated value corresponding to the readout value obtained when the reader is operated without a dosimeter or detector

**3.28****detection threshold**

minimum evaluated value for which the readout value of a dosimeter or detector is significantly different (at the 95 % confidence level) from the readout value of an unirradiated dosimeter or detector

**3.29****coefficient of variation**

ratio of the standard deviation  $s$ , to the arithmetic mean  $\bar{x}$  of a set of  $n$  measurements  $x_i$ ; is given by the following formula:

$$V = \frac{s}{\bar{x}} = \frac{1}{\bar{x}} \sqrt{\frac{1}{n-1} \sum_{i=1}^n (x_i - \bar{x})^2} \quad (3)$$

NOTE The coefficient of variation is generally expressed as a percentage.

**3.30****quality control test****QT**

test performed on a number of TL dosimeter systems, dosimeters, detectors or readers of a given batch or production designed to assure quality control

**3.31****type test****TT**

test performed on a small number of TL dosimeter systems, dosimeters, detectors or readers of a given type to determine performance characteristics of that type

**4 Units**

This International Standard uses SI units. However, the following units of practical importance for time are used where necessary: days (d), hours (h). The symbols of the units for time are provided by International Standard ISO 31-0.

**5 General test conditions****5.1 Test conditions**

All tests shall be performed under standard test conditions (see annex A), except where otherwise stated. Dosimeters shall be subjected to the annealing, cleaning and handling procedures which are recommended by the manufacturer.

**5.2 Reference radiations**

The radiation sources specified in ISO 4037-3 and ISO 6980 shall be used in the manner specified in these International Standards. Photon reference radiations used for spectral response checks shall be chosen from the first column of table 1 in 4 of ISO 4037-3:1999. Sources for beta spectral response shall be  $^{90}\text{Sr}$  (in equilibrium with  $^{90}\text{Y}$ ),  $^{106}\text{Ru}$ , and  $^{204}\text{Tl}$ . Calibration of radiation sources shall be traceable to the appropriate primary or secondary standards.

**6 Classification**

Dosimeters shall be classified in accordance with body part and the depth of intended measurement, and method of intended use viz:

F(7)D Finger, depth 7 mg·cm<sup>-2</sup>, disposable;

F(7)R Finger, depth 7 mg·cm<sup>-2</sup>, re-usable;

L(7)D	Limb, depth 7 mg·cm <sup>-2</sup> , disposable;
L(7)R	Limb, depth 7 mg·cm <sup>-2</sup> , re-usable;
E(300)D	Eye, depth 300 mg·cm <sup>-2</sup> , disposable;
E(300)R	Eye, depth 300 mg·cm <sup>-2</sup> , re-usable.

## 7 Performance requirements

The performance criteria are listed in Table 1. All dose values listed in the criteria are in terms of dose equivalent to tissue at the intended depth of measurement. The conventional true value of the dose equivalent,  $C$ , for any specific tests may be obtained by using the conversion coefficients specified in annex E, for each type of intended measurement (finger, limb or eyes). In this International Standard, conversion coefficients are only provided for tissue depths of 7 mg·cm<sup>-2</sup> and 300 mg·cm<sup>-2</sup>.

Annex E includes conversion coefficients for selected phantoms for photons and beta radiation. The selected phantoms are a solid 19 mm diameter cylinder of PMMA (ISO PMMA rod) for the finger, a 73 mm diameter water-filled cylinder of PMMA (ISO water pillar) for the limb, both of length 300 mm, and the ICRU sphere or 30 cm × 30 cm × 15 cm water-filled PMMA slab (ISO water slab) for the eyes. The use of other coefficients or phantoms is not precluded and shall be agreed between the manufacturer and the purchaser. The evaluated value of the dose equivalent, (E), shall be determined from the readout value in accordance with annex E. However, in the case of purely comparative tests (i.e. all except energy response and isotropy), the readout values may be used instead of evaluated values.

The performance requirements are identified in Table 1 as type tests (T) or quality control tests (Q). Type tests are intended to demonstrate the basic performance of the type of dosimeter and quality control tests are intended to verify the performance of a specific production or delivery batch of dosimeters.

The number of dosimeters used for each test or repeated tests shall be such that the performance requirements are demonstrated to be met to 95 % confidence. The number,  $n$ , of dosimeters (or irradiations) used for any test need not be the same for each test but may be determined using annex B. However, it may be convenient to use, arbitrarily, 5, 10 or 20 dosimeters (or irradiations), in which case the Student's  $t$ -value, obtained from annex B, Table B.1, would be 2,78, 2,26 or 2,09 respectively.

Where the response to neutrons is greater than 1 % of the response to photons, in terms of dose equivalent, the manufacturer shall draw the attention of the user to this fact and provide appropriate quantitative information.

Performance requirements are specified in terms of the dose equivalent at appropriate tissue depths, the conventional true value in testing being determined using conversion coefficients for appropriate phantoms. One school of thought suggests that this quantity should be called  $H_p(d)$ , analogous with measurements on the body. However, neither the International Commission on Radiological Protection (ICRP) nor the International Commission on Radiation Units and Measurements ICRU have specifically addressed the question of a name for the measurement quantity for extremities. The measurement quantity is therefore specified in this International Standard in the way described but is not named.

## 8 Test methods

Suggested tests to demonstrate compliance with the specified performance requirements are specified in annex C. Alternative tests which equally demonstrate compliance are not precluded.

## 9 Certification

Manufacturers claiming compliance (or part compliance) with the performance requirements of this International Standard should provide a signed certificate including the following details:

- a) names and addresses of the manufacturer and test laboratories;
- b) description/specification of the dosimeters under consideration, including dosimeter classification;
- c) description of reader, procedures and ancillary equipment used for the tests (Model, No., etc.);
- d) statements certifying the results of each test, and dates undertaken (test reports should be available for inspection by the purchaser);
- e) statement giving the quantitative response to neutrons, if required;
- f) details of conversion coefficients and phantoms agreed between the manufacturer and the purchaser, where those specified in this International Standard are not used.

NOTE In the situation where all tests are not done in the same establishment, the certificate should clearly identify the individual test laboratories for each test.

**Table 1 — Performance requirements for extremity and eye dosimeters**

No.	Performance characteristic	Class of dosimeter	Performance requirements	Test required <sup>a</sup>
1	Batch homogeneity	R/D	The coefficient of variation of the evaluated value for <i>n</i> dosimeters shall not exceed 15 % for a dose of 10 mSv or less	Q
2	Reproducibility	R D	The coefficient of variation of the evaluated value for <i>n</i> dosimeters shall not exceed 10 % for each dosimeter separately for a dose of 10 mSv or less No requirement	Q
3	Linearity	R/D	The response shall not vary by more than 10 % over the dose equivalent range 1 mSv to 1 Sv	T
4	Stability of dosimeters under various climatic conditions	R/D	The evaluated values of dosimeters irradiated either at the beginning or at the end of a storage period shall not differ from the conventional true value by more than 5 % for 30 d storage under standard test conditions, or 10 % for 48 h storage at 40 °C and 90 % relative humidity	T
5	Detection threshold	R/D	The detection threshold shall not exceed 1 mSv	T
6	Self- irradiation	R/D	After a storage period of 60 days, the zero point shall not exceed 2mSv	T
7	Residue	R	After irradiation with a conventional true value of 100 mSv, the detection threshold limit shall not be exceeded and the response shall remain within the requirement for linearity at a dose level of 2 mSv	T
8	Effect of light exposure on the dosimeter	R/D	As a result of exposure to 1 000 W·m <sup>-2</sup> equivalent to bright sunlight (295 nm to 769 nm) for 1 d, the zero point shall not change by more than 1 mSv and, for exposure during one week, the evaluated value shall not differ from the evaluated value of a dosimeter kept in the dark by more than 10 %	T
9	Isotropy (photons)	R/D	When irradiated with photons of (60 ± 5) keV, the mean value of the response at angles of incidence of 0°, 20°, 40° and 60° from normal shall not differ from the corresponding response for normal incidence by more than 15 %	T
10	Energy response (photons)	R/D	When irradiated with photons in the energy range 15 keV to 3 MeV, response shall not vary by more than ± 50 %	T
11	Energy response (beta radiation)	R/D	When irradiated with beta radiation in the energy range ( <i>E</i> <sub>max</sub> ) 0,5 MeV to 3 MeV, the response shall not vary by more than ± 50 %	T

<sup>a</sup> T: Type.  
Q: Quality control.

## Annex A (normative)

### Reference conditions and standard test conditions

Influence quantity	Reference conditions (unless otherwise stated by the manufacturer)	Standard test conditions (unless otherwise stated by the manufacturer)
Reference photon radiation	To conform to ISO 4037-3	To conform to ISO 4037-3
Reference beta radiation	To conform to ISO 6980	To conform to ISO 6980
Ambient temperature	20 °C	18 °C to 22 °C
Relative humidity	65 %	55 % to 75 %
Gamma radiation background	$\leq 0,2 \mu\text{Gy}\cdot\text{h}^{-1}$	$\leq 0.2 \mu\text{Gy}\cdot\text{h}^{-1}$
Contamination by radioactive elements	Negligible	Negligible
Light intensity	$50 \text{ W}\cdot\text{m}^{-2}$	$< 100 \text{ W}\cdot\text{m}^{-2}$


STANDARDSISO.COM : Click to view the full PDF of ISO 12794:2000

## Annex B (normative)

### Confidence limits

#### B.1 General

If the magnitude of the random uncertainty of a measured value is a significant fraction of the permitted tolerances of this measured value, the random uncertainty has to be considered by taking more than one measurement. The number of measurements or the sample size has to be chosen in such a way that the confidence interval obtained for each mean,  $\bar{x}$ , for a confidence level of 95 % lies either within the limits of variation of the measured value permitted in the test (test passed, points  $\Delta$  in Figure B.1) or outside of these limits (test failed, points  $\circ$  in Figure B.1). If one of the permitted limits of variation,  $x_u$  or  $x_l$ , lies within the confidence interval of the mean (points  $\square$  in Figure B.1) the number of measurements or the sample size can be increased to reduce the width  $2I$  of the confidence interval of the mean  $\bar{x}$ , in order to reach one of the two cases mentioned above, which are necessary for an unequivocal decision of passing the test or not.

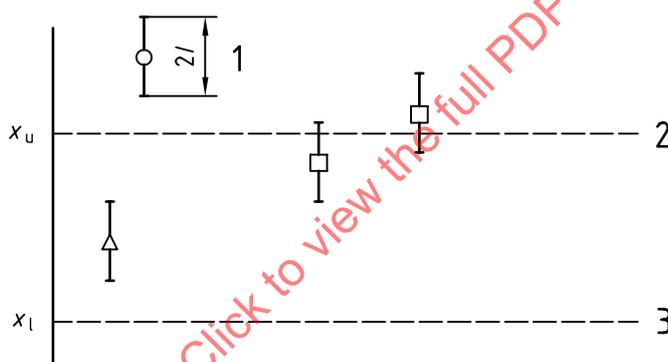

#### Key

- 1 Confidence interval of the mean width  $2I$
- 2 Permitted upper limit of variation,  $x_u$
- 3 Permitted lower limit of variation,  $x_l$

**Figure B.1 — Test for confidence interval**

The test is passed if the confidence interval of width  $2I$  around  $\bar{x}$  lies between the permitted upper and lower limit of variation,  $x_u$  and  $x_l$ :

$$x_l + I < \bar{x} < x_u - I \quad (\text{B.1})$$

In each test, it is recommended to start with 10 measurements for each dosimeter. If it turns out to be necessary to reduce the width  $2I$  of the confidence interval of the experimental standard deviation, the number of measurements should be increased (see B.2).

Occasionally, it is more convenient to carry out a test (including, for example, an irradiation) with a certain number of different dosimeters withdrawn at random from the batch instead of repeating a number of measurements with the same dosimeter. There are no objections to such a procedure but the random uncertainties of the test results may be increased.

## B.2 Confidence interval for the standard deviation, $s$

The confidence interval for the standard deviation of the means  $s$  is:

$$(s - I_s, s + I_s) \tag{B.2}$$

where  $I_s$  is the half-width of the confidence interval of  $s$ . If  $s$  is calculated from  $n_s$  measurements, the upper limit of  $I_s$  at a confidence level of 95 % is given by:

$$I_s(n_s) = t_{ns} \cdot s \sqrt{\frac{1}{2(n_s - 1)}} \tag{B.3}$$

where  $t_{ns}$  is taken from table B.1 for  $n_s$  measurements. By way of example,  $I_s(10) = 0,53s$  is obtained for 10 dosimeters.

## B.3 Confidence interval for the mean, $\bar{x}$

The confidence interval for the mean  $\bar{x}$  is:

$$(\bar{x} - I_i, \bar{x} + I_i) \tag{B.4}$$

where  $I_i$  is the half-width of the confidence interval of  $x$  relative to the  $i$ th set of measurements. When calculating  $\bar{x}$  from  $n_i$  measurements, the half-width of the confidence interval is given by:

$$I_i = \frac{t_n s_i}{\sqrt{n_i}} \tag{B.5}$$

where  $s_i$  is the standard deviation for the  $i$ th group of measurements, and  $t_n$  is taken from Table B.1 for  $n_i$  measurements.

For example, for  $n_i = 10$ ,  $I_i = \frac{2,26s_i}{\sqrt{10}} = 0,71s_i$

Table B.1 — Student's  $t$ -values for 95 % confidence interval

$n_i$	$t_n$	$n_i$	$t_n$
2	12,71	15	2,15
3	4,30	20	2,09
4	3,18	25	2,06
5	2,78	30	2,05
6	2,57	40	2,02
7	2,45	60	2,00
8	2,37	120	1,98
9	2,31	$\infty$	1,96
10	2,26		

#### B.4 Confidence interval for a combined quantity

If the limits of variation are stated for a quantity  $x$ , the mean value calculated from  $k$  means,  $\bar{x}_1, \bar{x}_2, \bar{x}_3, \dots, \bar{x}_k$ , is:

$$\bar{x} = f(\bar{x}_1, \bar{x}_2, \bar{x}_3, \dots, \bar{x}_k) \quad (\text{B.6})$$

and the half-width of the confidence interval of the  $i$ th mean is  $I_i$ , the half-width,  $I$ , of the confidence interval for  $\bar{x}$  is given by :

$$I = \sqrt{\sum_{i=1}^k \left( \frac{\delta \bar{x}}{\delta x_i} \right)^2 I_i^2} \quad (\text{B.7})$$

EXAMPLE 1  $\bar{x} = \bar{x}_1 \pm \bar{x}_2$  hence  $I = \sqrt{(I_1^2 + I_2^2)}$ .

in general  $\bar{x} = \sum_{i=1}^n \bar{x}_i$  hence  $I = \sqrt{\sum_{i=1}^n I_i^2}$

EXAMPLE 2  $\bar{x} = \frac{\bar{x}_1}{\bar{x}_2}$  hence  $I = \frac{\bar{x}_1}{\bar{x}_2} \sqrt{\left( \frac{I_1}{x_1} \right)^2 + \left( \frac{I_2}{x_2} \right)^2}$

EXAMPLE 3  $\bar{x} = \frac{x_1 / x_2}{x_1 + x_2}$  hence  $I = \frac{2}{(\bar{x}_1 + \bar{x}_2)^2} \sqrt{(\bar{x}_2 I_1)^2 + (\bar{x}_1 I_2)^2}$

## Annex C (normative)

### Performance tests

#### C.1 Batch homogeneity (Types R and D)

Prepare and irradiate  $n$  dosimeters to the same conventionally true value ( $C$ ) of 10 mSv or less. Determine the evaluated value ( $E$ ) for each dosimeter and show that the coefficient of variation for the  $n$  dosimeters does not exceed 15 %.

#### C.2 Reproducibility (Type R)

Prepare, irradiate and read out  $n$  dosimeters. Repeat this 10 times. The conventional true value shall be exactly the same each time and about 10 mSv or less.

For each of the  $n$  dosimeters, determine the mean evaluated value,  $\bar{E}_j$ , and the standard deviation,  $s_{Ej}$ .

Show that for each of the  $n$  dosimeters:

$$\frac{100 (s_{Ej} + I_s)}{\bar{E}_j} \leq 10 \quad (\text{C.1})$$

Where  $I_s$  is given in expression (B.2).

#### C.3 Linearity (Types R and D)

Prepare, irradiate and read out four groups of dosimeters. Let  $n_i$  be the number of dosimeters in the  $i$ th group. The conventional true values ( $C_i$ ) given to each group shall be 0,001 Sv, 0,01 Sv, 0,1 Sv and 1 Sv.

Calculate the mean evaluated value ( $\bar{E}_i$ ) at each irradiation level and its standard deviation  $S_{\bar{E}}$ .

Show that:

$$0,90 \leq \frac{\bar{E}_i \pm I_i}{C_i} \leq 1,10 \quad (\text{C.2})$$

Where  $I_i$  is obtained from equation (B.5) for  $n$  dosimeters. The uncertainties in  $C_i$  are considered negligible.

#### C.4 Stability of dosimeters under various climatic conditions (Types R and D)

Prepare two groups of  $n$  dosimeters each. Store both groups for 24 h under standard conditions.

Irradiate group 1 to a known conventional true value ( $C$ ) of about 10 mSv.

Store both groups of dosimeters in a climatic chamber in which standard test conditions prevail.

After a continuous period of 30 d, remove both groups of dosimeters from the climatic chamber. Irradiate group 2 to the same conventional true value as group 1.

Store both groups for 1 d under standard test conditions. Determine the evaluated values ( $E$ ) for each dosimeter and calculate the mean of the evaluated values ( $\bar{E}$ ) for each of the two groups and the respective standard deviations,  $s$ .

Show that for each group:

$$0,95 \leq \frac{\bar{E} \pm I_i}{C} \leq 1,05 \quad (\text{C.3})$$

where  $I_i$  is calculated according to equation (B.5).

Repeat the test for a storage period of 2 d but in a climatic chamber in which the temperature is  $40^\circ\text{C} \pm 2^\circ\text{C}$  and the relative humidity is at least 90 %.

Show that for each group :

$$0,90 \leq \frac{\bar{E} \pm I_i}{C} \leq 1,10 \quad (\text{C.4})$$

where  $I_i$  is calculated according to equation (B.5).

### C.5 Detection threshold (Types R and D)

Prepare and read out  $n$  dosimeters.

Determine the evaluated value ( $E$ ) for each (unirradiated) dosimeter and calculate the standard deviation ( $s_{\bar{E}}$ ) for all  $n$  dosimeters.

Show that:

$$E + 1 \leq 10 \text{ mSv} \quad (\text{C.5})$$

### C.6 Self irradiation (Types R and D)

Prepare  $n$  dosimeters. Store them for 60 d under standard test conditions in a location where the background dose rate is known.

Read out the dosimeters and determine the evaluated value ( $E$ ). Calculate the mean of the evaluated values ( $\bar{E}$ ) for all  $n$  dosimeters and the standard deviation. Determine the conventional true value,  $C_B$  (background), due to the background irradiation during storage.

Show that:

$$(\bar{E} + I_i) - C_B \leq 2 \text{ mSv} \quad (\text{C.6})$$

where  $I_i$  is the half-width of the confidence interval, determined as in equation (B.5).

## C.7 Residue (Type R)

### C.7.1 Effect on detection threshold

Prepare, irradiate and read out the  $n$  dosimeters used for the detection-threshold test. The conventional true value ( $C$ ) shall be about 100 mSv.

Using the same dosimeters, repeat the test for detection threshold.

### C.7.2 Effect on response

Prepare, irradiate and read out the same  $n$  dosimeters used above. The conventional true value, ( $C$ ) shall be about 2 mSv.

Determine the evaluated value ( $E$ ) for each dosimeter and calculate the mean of the evaluated values ( $\bar{E}$ ) and the standard deviation,  $s_E$ .

Show that:

$$0,90 \leq \frac{\bar{E} \pm I_i}{C} \leq 1,10 \quad (\text{C.7})$$

where  $I_i$  is determined according to equation (B.5).

## C.8 Effect of exposure to light (Types R and D)

### C.8.1 Effect on zero point

Prepare two groups of 20 dosimeters each.

Expose group 1 to 1 000  $\text{W}\cdot\text{m}^{-2}$  of light for 1 d. Ensure that the temperature of the dosimeters is maintained at less than 40°.

To produce 1 000  $\text{W}\cdot\text{m}^{-2}$  of light, use apparatus which produces light whose spectrum corresponds to that of bright sunlight (295 nm to 769 nm), (for example with a xenon lamp equipped if necessary with appropriate filters), or use a daylight fluorescent lamp.

NOTE 1 000  $\text{W}\cdot\text{m}^{-2}$  bright sunlight includes 60  $\text{W}\cdot\text{m}^{-2}$  of UV.

Store the group 2 dosimeters in the dark in an otherwise identical environment. Ensure that the temperature of group 2 dosimeters is within  $\pm 5$  °C of the group 1 dosimeters.

After 1 d, read out all dosimeters.

Determine the evaluated value ( $E$ ) for each group and calculate the mean of the evaluated values ( $\bar{E}$ ) for each of the two groups and their respective standard deviations.

Show that:

$$\left| \left( \bar{E}_{\text{group 1}} - \bar{E}_{\text{group 2}} \right) \right| + I \leq 1,0 \text{ mSv} \quad (\text{C.8})$$

where  $I$  is calculated according to equation (B.7) for the difference of two means.

### C.8.2 Effect on response

Prepare and irradiate two groups of 20 dosimeters each. The conventional true value ( $C$ ) shall be about 10 mSv.

Expose and store groups 1 and 2 respectively as above.

After one week, read out all dosimeters.

Determine the evaluated value ( $E$ ) for each and calculate the mean of the evaluated values ( $\bar{E}$ ) for each of the two groups, and their respective standard deviations.

Show that:

$$0,90 \leq \frac{\bar{E}_{\text{group 1}}}{\bar{E}_{\text{group 2}}} \pm I \leq 1,10 \quad (\text{C.9})$$

where  $I$  is calculated from equation (B.7) for the quotient of two means.

### C.9 Isotropy (photons) (Types R and D)

Prepare, irradiate on a phantom and read out four groups of  $n$  dosimeters. Let  $n_i$  be the number of dosimeters of the  $i$ th group. The conventional true value  $C$  shall be about 10 mSv using photons of energy  $(60 \pm 5)$  keV (X-radiation or  $^{241}\text{Am}$ ) and for the following conditions:

- group 1: normal incidence;
- group 2: 20° off normal;
- group 3: 40° off normal;
- group 4: 60° off normal.

For each group, the angle of incidence for the  $n$  irradiations is varied in a positive and negative direction in two planes perpendicular to each other and to the plane of the dosimeter.

Determine the evaluated value ( $E$ ) for each dosimeter (see Table E.1) and calculate the mean of the evaluated values ( $\bar{E}_i$ ) for each of the four groups and the respective standard deviations.

Show that:

$$0,85 \leq \frac{\sum \bar{E}_i}{4E_1} \pm I \leq 1,15 \quad (\text{C.10})$$

where  $I$  is determined according to equation (B.7).

### C.10 Energy response (photons) (Types R and D)

Prepare, irradiate on a phantom and read out four groups of  $n$  dosimeters each. The conventional true value ( $C$ ) shall be about 10 mSv using the following reference radiations:

- group 1: 15,8 keV;
- group 2: in the range 30 to 40 keV;
- group 3: in the range 80 to 100 keV;
- group 4:  $^{137}\text{Cs}$  or  $^{60}\text{Co}$ .

NOTE These are the minimum requirements to fully comply with this International Standard. Additional reference radiations may be used.

Determine the evaluated value ( $E$ ) for each dosimeter (see Table E.2) and calculate the mean of the evaluated values, ( $\bar{E}$ ) for each of the four groups and the respective standard deviations.

For each group show that:

$$0,5 \leq \frac{\bar{E}_i \pm I_i}{C} \leq 1,5 \quad (\text{for } i = 1, 2, 3, 4) \quad (\text{C.11})$$

where  $I_i$  is determined according to equation (B.5).

### C.11 Energy response (beta radiation) (Types R and D)

Prepare, irradiate on a phantom and read out two groups of  $n$  dosimeters each. The conventional true value ( $C$ ) shall be about 10 mSv using the following reference radiations:

- group 1:  $^{90}\text{Sr}/^{90}\text{Y}$ ;
- group 2:  $^{204}\text{Tl}$ .

Determine the evaluated value ( $E$ ) for each dosimeter (see Table E.3) and calculate the mean of the evaluated values ( $\bar{E}$ ) for each of the two groups.

For each group show that:

$$0,5 \leq \frac{\bar{E}_i \pm I_i}{C} \leq 1,5 \quad (\text{C.12})$$

where  $I_i$  is determined according to equation (B.5).