
**Plastics — Simple heat release test
using a conical radiant heater and a
thermopile detector**

*Plastiques — Essai simple pour la détermination du débit calorifique
au moyen d'un radiateur conique et d'une sonde à thermopile*

STANDARDSISO.COM : Click to view the full PDF of ISO 13927:2023



STANDARDSISO.COM : Click to view the full PDF of ISO 13927:2023



COPYRIGHT PROTECTED DOCUMENT

© ISO 2023

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	v
Introduction.....	vi
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Symbols.....	2
5 Principle.....	2
6 Apparatus.....	2
6.1 General.....	2
6.2 Cone-shaped radiant electrical heater.....	4
6.3 Heat flux controller.....	4
6.4 Chimney and thermopiles.....	5
6.5 Specimen holder.....	5
6.6 Retainer frame.....	5
6.7 Fume extraction system.....	7
6.8 Ignition circuit.....	8
6.9 Ignition timer.....	8
6.10 Heat flux meter.....	8
6.11 Calibration burner.....	8
6.12 Data collection system.....	8
7 Suitability of a product for testing.....	10
7.1 Surface characteristics.....	10
7.2 Asymmetrical products.....	10
7.3 Thin materials.....	10
7.4 Composite specimens.....	10
7.5 Dimensionally unstable materials.....	10
7.6 Materials that require testing under compression.....	11
8 Specimen construction and preparation.....	12
8.1 Specimens.....	12
8.2 Conditioning of specimens.....	12
8.3 Preparation.....	13
8.3.1 Specimen wrapping.....	13
8.3.2 Specimen preparation.....	13
8.3.3 Preparing specimens of materials that require testing under compression.....	13
9 Calibration.....	14
9.1 Heater calibration.....	14
9.2 Thermopile calibration.....	14
9.2.1 General.....	14
9.2.2 Initial calibration.....	14
9.2.3 Daily calibration.....	15
10 Test procedure.....	15
10.1 General precautions.....	15
10.2 Initial preparation.....	15
10.3 Procedure.....	16
11 Precision.....	16
12 Test report.....	16
Annex A (normative) Calibration of the heat flux meter.....	18
Annex B (informative) Guidance notes for operators.....	19

Annex C (informative) Guidance on measuring mass loss during testing	20
Annex D (informative) Example of thermopile calibration — Relation of heat release and thermopile output	21
Annex E (informative) Calculation of effective critical heat flux for ignition	23
Bibliography	24

STANDARDSISO.COM : Click to view the full PDF of ISO 13927:2023

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 4, *Burning behaviour*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 249, *Plastics*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This third edition cancels and replaces the second edition (ISO 13927:2015), which has been technically revised.

The main changes are as follows:

- the normative references have been updated to the latest editions (see [Clause 2](#));
- use of mass flow rate of methane gas corresponding to the net heat of combustion for calibration of the thermopile has been added in [Clause 9](#);
- a new [Annex D](#) giving an example of thermopile calibration has been added and subsequent annex has been renamed as [Annex E](#).

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

Fire is a complex phenomenon; its behaviour and effects depend upon a number of interrelated factors. The behaviour of materials and products depends upon the characteristics of the fire, the method of use of the materials, and the environment in which they are exposed (see also ISO 13943).

A test, such as the one specified in this document, deals only with a simple representation of a particular aspect of the potential fire situation, typified by a radiant heat source, and it cannot alone provide any direct guidance on the behaviour or safety in fire (see ISO/TS 3814). A test of this type can, however, be used for comparative purposes or to ensure the existence of a certain quality of performance (in this case, heat release from a composite material or an assembly) considered to have a bearing on fire performance generally. It would be wrong to attach any other meaning to performance in this test. The attention of all users of this test is drawn to the warning that immediately precedes [Clause 10](#).

STANDARDSISO.COM : Click to view the full PDF of ISO 13927:2023

Plastics — Simple heat release test using a conical radiant heater and a thermopile detector

1 Scope

This document specifies a method suitable for the production control or product development purposes for assessing the heat release rate of essentially flat products exposed in the horizontal orientation to controlled levels of radiant heating with an external igniter. The heat release rate is determined by the use of a thermopile instead of the more accurate oxygen consumption techniques. The time to ignition and sustained flaming are also measured in this test. The mass loss of the test specimen can also be measured optionally.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 291, *Plastics — Standard atmospheres for conditioning and testing*

ISO 5660-1, *Reaction-to-fire tests — Heat release, smoke production and mass loss rate — Part 1: Heat release rate (cone calorimeter method) and smoke production rate (dynamic measurement)*

ISO 13943, *Fire safety — Vocabulary*

ISO 14697, *Reaction-to-fire tests — Guidance on the choice of substrates for building and transport products*

ISO 14934-3, *Fire tests — Calibration and use of heat flux meters — Part 3: Secondary calibration method*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 13943 and the following apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at <https://www.iso.org/obp>

— IEC Electropedia: available at <https://www.electropedia.org/>

3.1

flat surface

surface whose irregularity from a plane does not exceed ± 1 mm

3.2

ignition

onset of *sustained flaming* (3.7)

3.3

material

single substance or uniformly dispersed mixture, for example, metal, stone, timber, concrete, mineral fibre or polymer

**3.4
orientation**

plane in which the exposed face of the *test specimen* (3.6) is located during testing either vertical or horizontal face upwards

**3.5
product**

material (3.3), composite or assembly, about which information is required

**3.6
test specimen**

representative piece of the *product* (3.5) which is to be tested together with any substrate or surface treatment

Note 1 to entry: The test specimen may include an air gap.

**3.7
sustained flaming**

existence of flame on or over the surface of the *test specimen* (3.6) for a period of over 10 s

**3.8
transitory flaming**

existence of flame on or over the surface of the *test specimen* (3.6) for a period of between 1 s and 10 s

4 Symbols

t_{ig}	time to ignition (onset of sustained flaming), expressed in seconds (s)
\dot{q}''_{180}	heat release rate per unit area at 180 s after ignition, expressed in kilowatts (kW/m ²)
\dot{q}''_{300}	heat release rate per unit area at 300 s after ignition, expressed in kilowatts (kW/m ²)
\dot{q}''_{max}	maximum heat release rate per unit area, expressed in kilowatts (kW/m ²)

5 Principle

The heat release rate is assessed by measurement of the output of a thermopile located in a chimney situated above a burning test specimen that is subjected to a known heat flux from a conical heater. The output (in mV) is converted into heat release rate per unit area (in kW/m²) by use of a calibration graph obtained previously by burning methane gas of known heat of combustion in the same apparatus. Guidance is given in [Annex B](#). The specimen mass loss rate during the test can also be measured by continuously recording the specimen load cell output. Guidance is given in [Annex C](#).


6 Apparatus

6.1 General

The test apparatus shall consist essentially of the following components: a cone-shaped radiant heater, a chimney housing a thermopile, a load cell, a specimen holder, and a fume extraction system. A schematic representation of the assembly is given in [Figure 1](#). The individual components are described in this clause.

Intoleranced dimensions are recommended values. Accrual dimensions of apparatus should be close to the dimensions as much as practicable.

Dimensions in millimetres

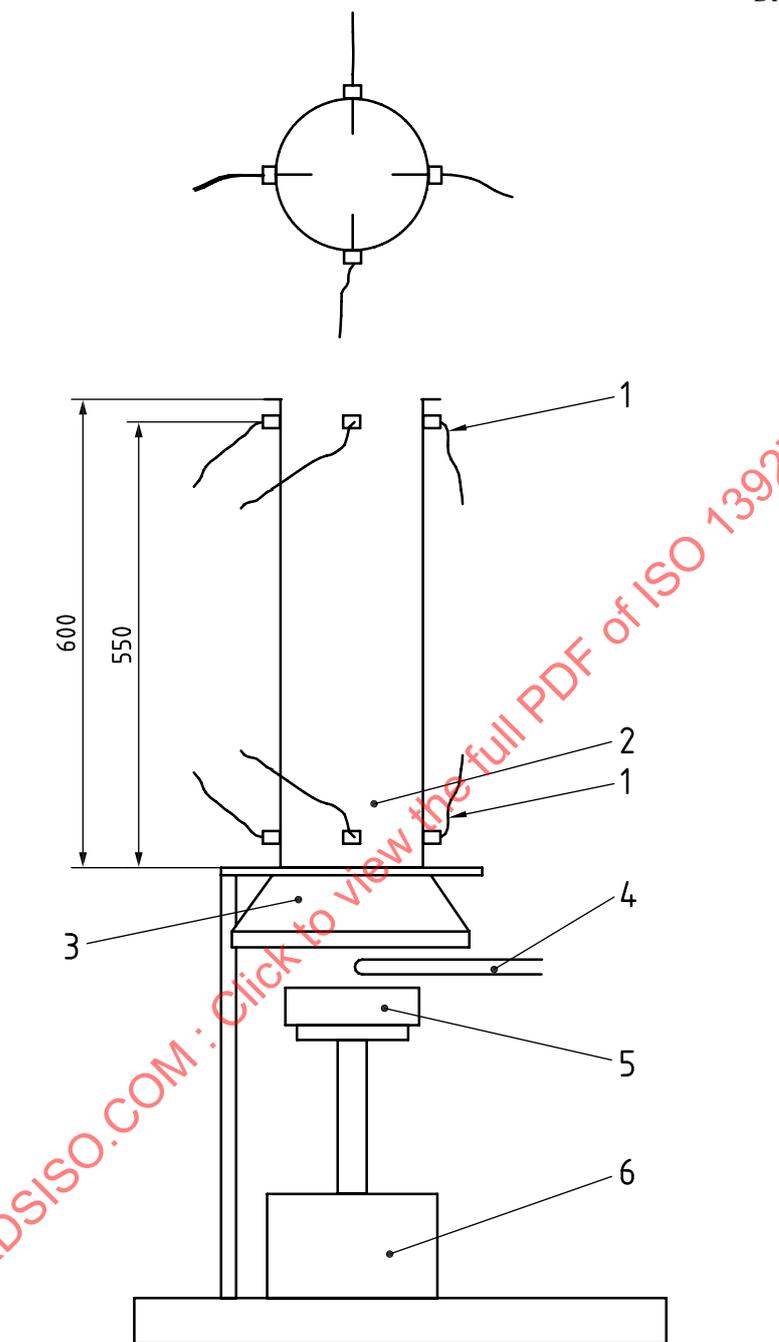

Key

- 1 thermopile
- 2 chimney
- 3 cone heater
- 4 spark igniter
- 5 specimen
- 6 load cell (optional)

Figure 1 — Schematic drawing of apparatus


6.2 Cone-shaped radiant electrical heater

The active element of the heater shall consist of an electrical heater rod, capable of delivering 5 000 W at the operating voltage, tightly wound into the shape of a truncated cone (see Figure 2). The heater shall be encased on the outside with a double-walled, stainless-steel cone filled between the walls with a refractory blanket of nominal thickness 13 mm and nominal density 100 kg/m³. The heat flux from the heater shall be maintained at a pre-set level by controlling the average temperature of three thermocouples (type K stainless-steel sheathed thermocouples have provided suitable), symmetrically disposed and in contact with, but not welded to, the heater element (see Figure 2). 1,0 mm to 1,6 mm outside diameter sheathed (unearthed) thermocouples with an unexposed hot junction may be used. The heater shall be capable of producing heat fluxes on the surface of the specimen of up to 75 kW/m². The heat flux shall be uniform within the central 50 mm × 50 mm area of the exposed specimen surface to within ±2 % for an irradiance of 50 kW/m².

The cone heater shall be provided with a removable radiation shield to protect immediately the specimen from heat prior to the start of the test.

6.3 Heat flux controller

The heat flux control system shall maintain the average temperature of the heater element steady to within ±2 °C.

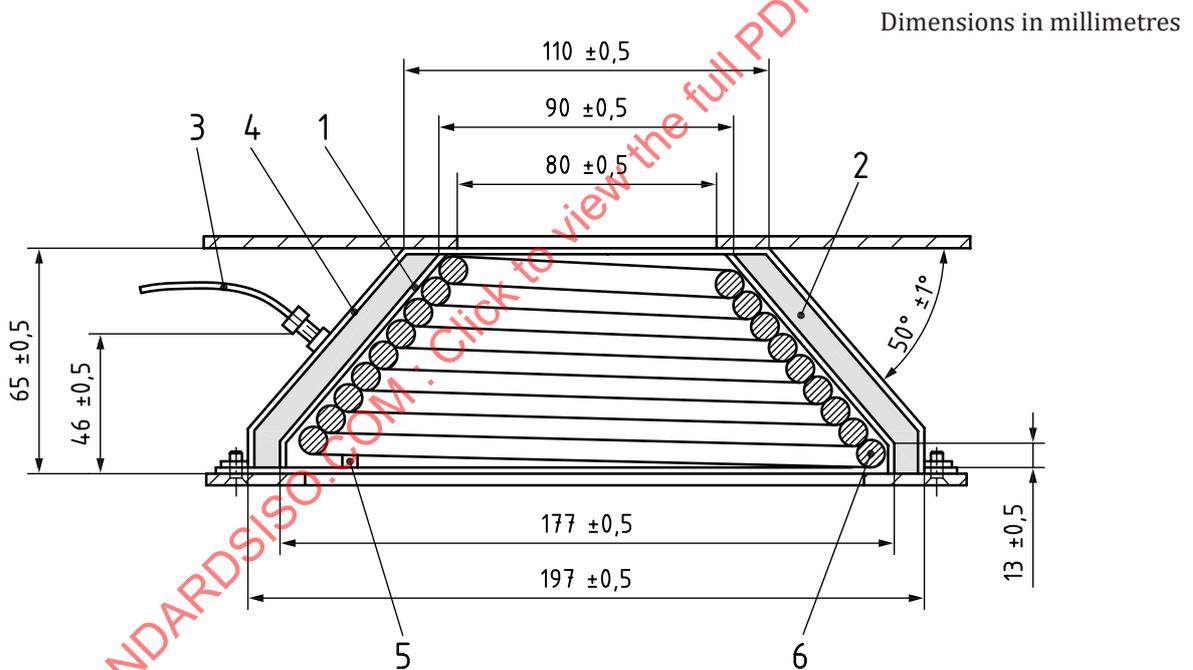

- Key**
- 1 inner shell
 - 2 refractory-fibre packing
 - 3 thermocouple
 - 4 outer shell
 - 5 spacer block
 - 6 heating element

Figure 2 — Cross-sectional view through heater

6.4 Chimney and thermopiles

A circular cross-section chimney 600 mm \pm 2 mm long and 115 mm \pm 2 mm internal diameter constructed from 1 mm-thick stainless steel shall be used to house the thermopiles. This shall be fixed on top of the top-plate of the cone heater. The axis of the chimney shall coincide with the axis of the cone heater.

Each thermopile shall consist of four 1,6 mm \pm 0,2 mm outside diameter type K sheathed thermocouples. The tips of the thermocouples shall be fixed 17 mm from the centreline of the chimney. The four thermocouples shall be connected in series and the two ends shall be connected to the data collection system.

A thermopile shall be housed within the chimney at a height of 550 mm above the cone top-plate and the chimney penetration points shall be equally distributed about the circumference of the chimney.

Another thermopile shall be housed 275 mm above the cone top-plate and the chimney penetration points are equally distributed across, about the circumference of the chimney.

The arrangement of the chimney and thermopiles is shown in [Figure 1](#).

Both thermopiles shall be calibrated individually according to [Clause 9](#).

6.5 Specimen holder

The specimen holder is shown in [Figure 3](#).

The specimen holder shall have the shape of a square pan with an opening of (106 \pm 1) mm \times (106 \pm 1) mm and a depth of 25 mm. The holder shall be constructed from stainless steel with a thickness of (2,4 \pm 0,15) mm. It shall include a handle to facilitate insertion and removal and a mechanism to ensure central location of the specimen under the heater and proper alignment with the weighing device. The distance between the bottom surface of the cone heater and the top of the specimen shall be adjusted to 25 mm, except when testing dimensionally unstable materials, in which case, the distance shall be adjusted to 60 mm \pm 1 mm. All tests shall be conducted with the retainer frame shown in [Figure 4](#). Details of specimen and specimen holder preparation are given in [8.3](#).

6.6 Retainer frame

The frame shall be constructed of stainless steel with a thickness of (1,9 \pm 0,1) mm in the shape of a box with an inside dimension of each side (111 \pm 1) mm and a height of (54 \pm 1) mm. The opening for the specimen face shall be (94,0 \pm 0,5) mm² as shown in [Figure 4](#). The retainer frame shall have an appropriate means to secure it to the specimen holder with a specimen in position.

Dimensions in millimetres


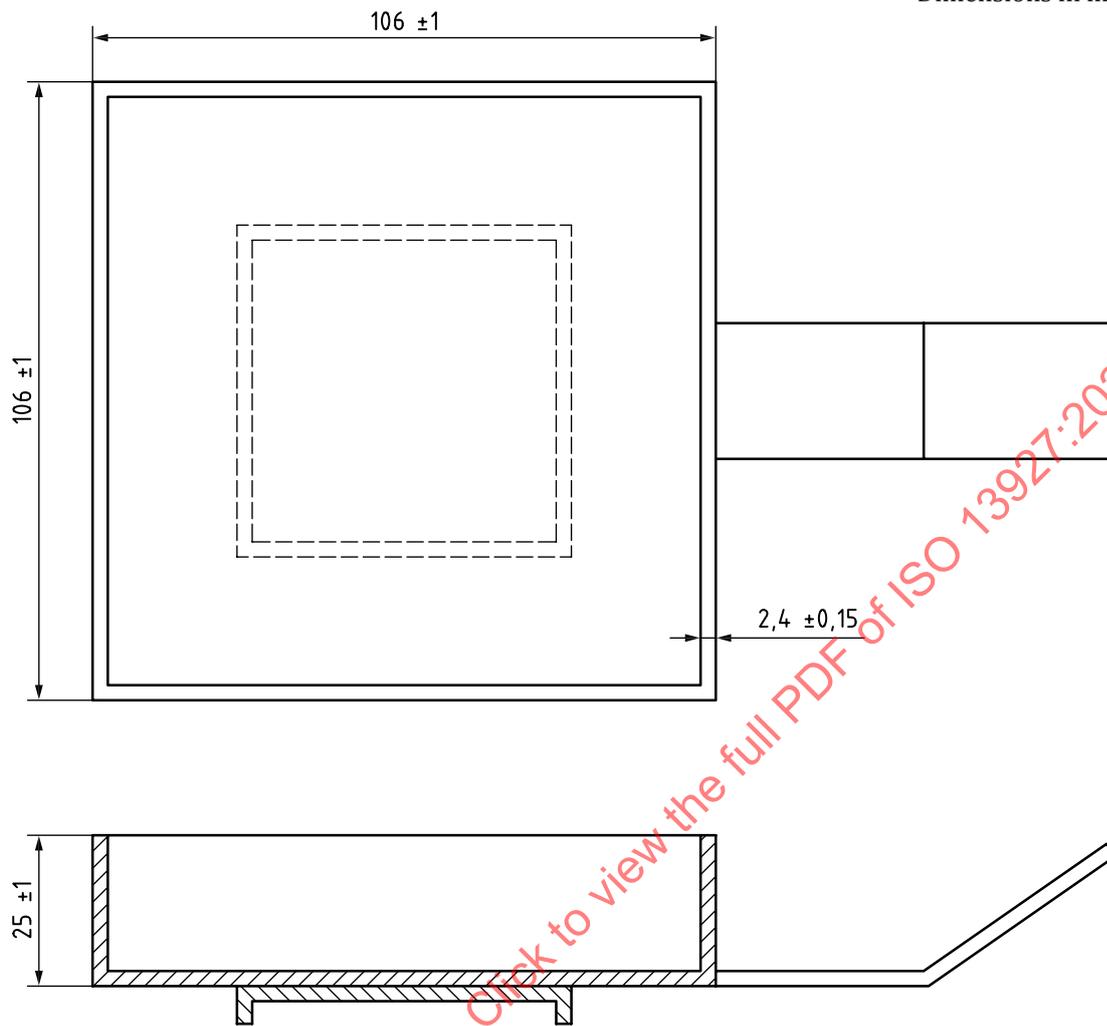


Figure 3 — Specimen holder

Dimensions in millimetres

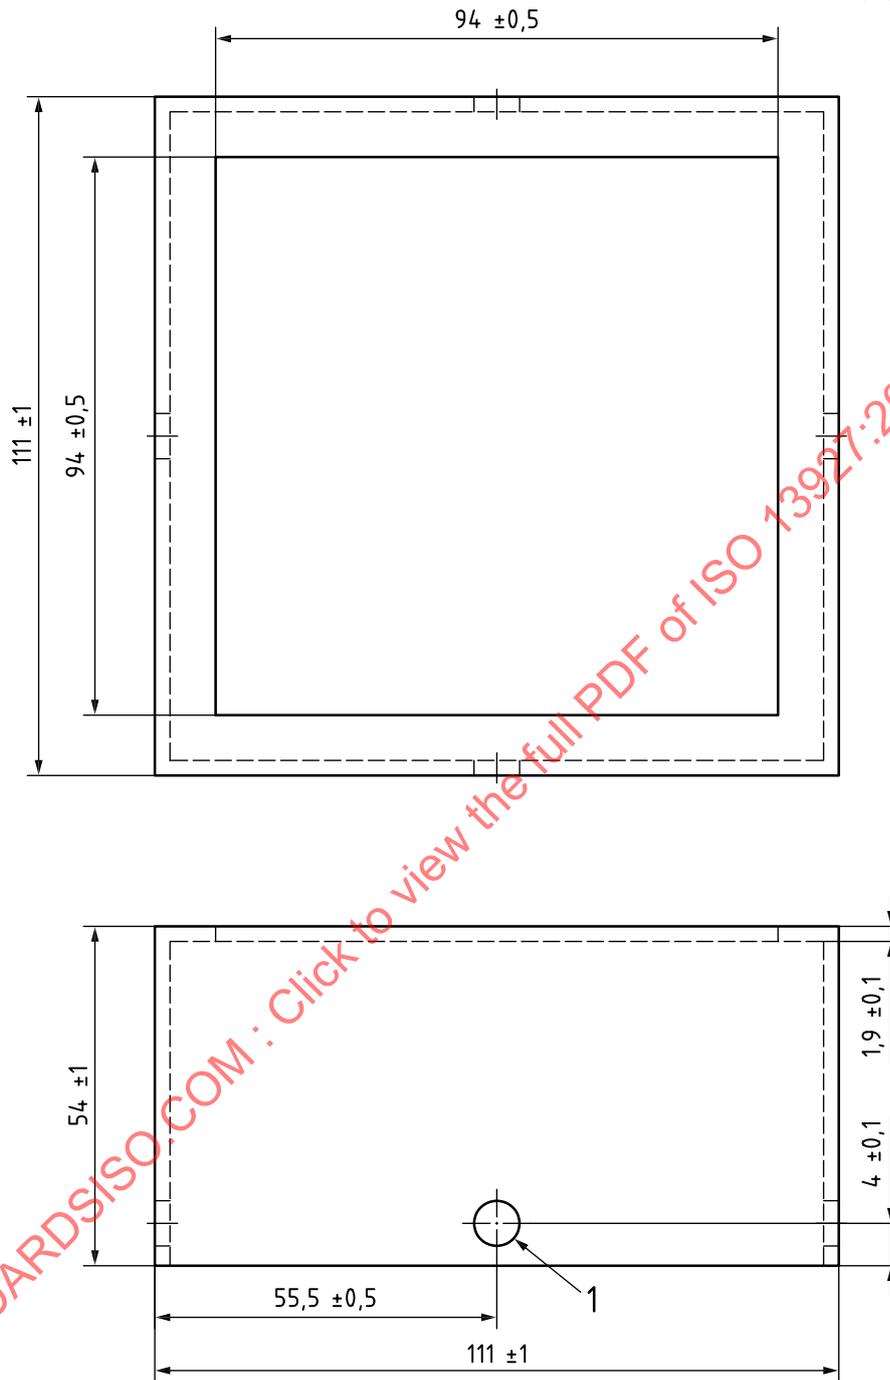

Key

- 1 tapped holes in four places (M3 or 10×32 recommended)

Figure 4 — Retainer frame

6.7 Fume extraction system

The apparatus shall be used under a hood or in a fume cupboard with adequate ventilation to remove safely combustion products from the laboratory.

6.8 Ignition circuit

Specimen ignition shall be accomplished by a spark plug powered by a 10 kV transformer or a 10 kV spark generator capable of continuous sparking. The spark electrodes shall have a gap of $3 \text{ mm} \pm 0,5 \text{ mm}$. If a transformer is used, it shall be of a type specifically designed for spark ignition use. The transformer shall have an isolated (unearthed) secondary to minimize interference with the data transmission lines. The electrode length and location of the spark plug shall be such that the spark gap is located $13 \text{ mm} \pm 2 \text{ mm}$ above the centre of the specimen in the horizontal orientation.

6.9 Ignition timer

The timer shall be capable of recording elapsed time to the nearest second and accurate to within 1 s in 1 h.

6.10 Heat flux meter

The heat flux meter shall be of the Schmidt-Boelter (thermopile) type with a design range of up to about 100 kW/m^2 . The target receiving radiation, and possibly to a small extent convection, shall be flat and circular of approximately 12,5 mm in diameter and coated with a durable matt black finish of surface emissivity $\varepsilon = 0,95 \pm 0,05$. The target shall be water-cooled, but care shall be taken that this does not cause water condensation on the target surface of the meter.

Radiation shall not pass through any window before reaching the target. The instrument shall be robust, simple to set up and use, and stable in calibration. The instrument shall also have an accuracy of within $\pm 3 \%$ and a repeatability of within 0,5 %.

The calibration of the heat flux meter shall be checked whenever recalibration of the apparatus is carried out, as described in [Annex A](#) or ISO 14934-3.

6.11 Calibration burner


The calibration burner shall consist of a square pan with a top opening of $(100_{-2}^{+0}) \text{ mm} \times (100_{-2}^{+0}) \text{ mm}$, constructed from stainless steel of thickness $2,4 \text{ mm} \pm 0,1 \text{ mm}$, and filled with sand. The burner shall have a handle to facilitate insertion and removal, and a mechanism to ensure central location of the burner under the heater and proper alignment with the weighing device. The burner shall be designed so that a metered supply of methane of at least 99,5 % purity can be introduced through a tube in the side wall as shown in [Figure 5](#). The flowmeter used to monitor the methane flow shall be one of the following: a rotameter, a dry-test meter, a wet-test meter, or an electronic mass flow controller.

The distance between the bottom surface of the cone heater and the top of the calibration burner shall be adjusted to 25 mm.

6.12 Data collection system

This system shall record the output from thermopile and the load cell (optional). It shall have an accuracy of 0,01 % of the full-scale output of the load cell (if used) and shall be capable of recording data every 5 s or less for at least 1 h and measuring temperature to a resolution of 0,5 °C.

Dimensions in millimetres

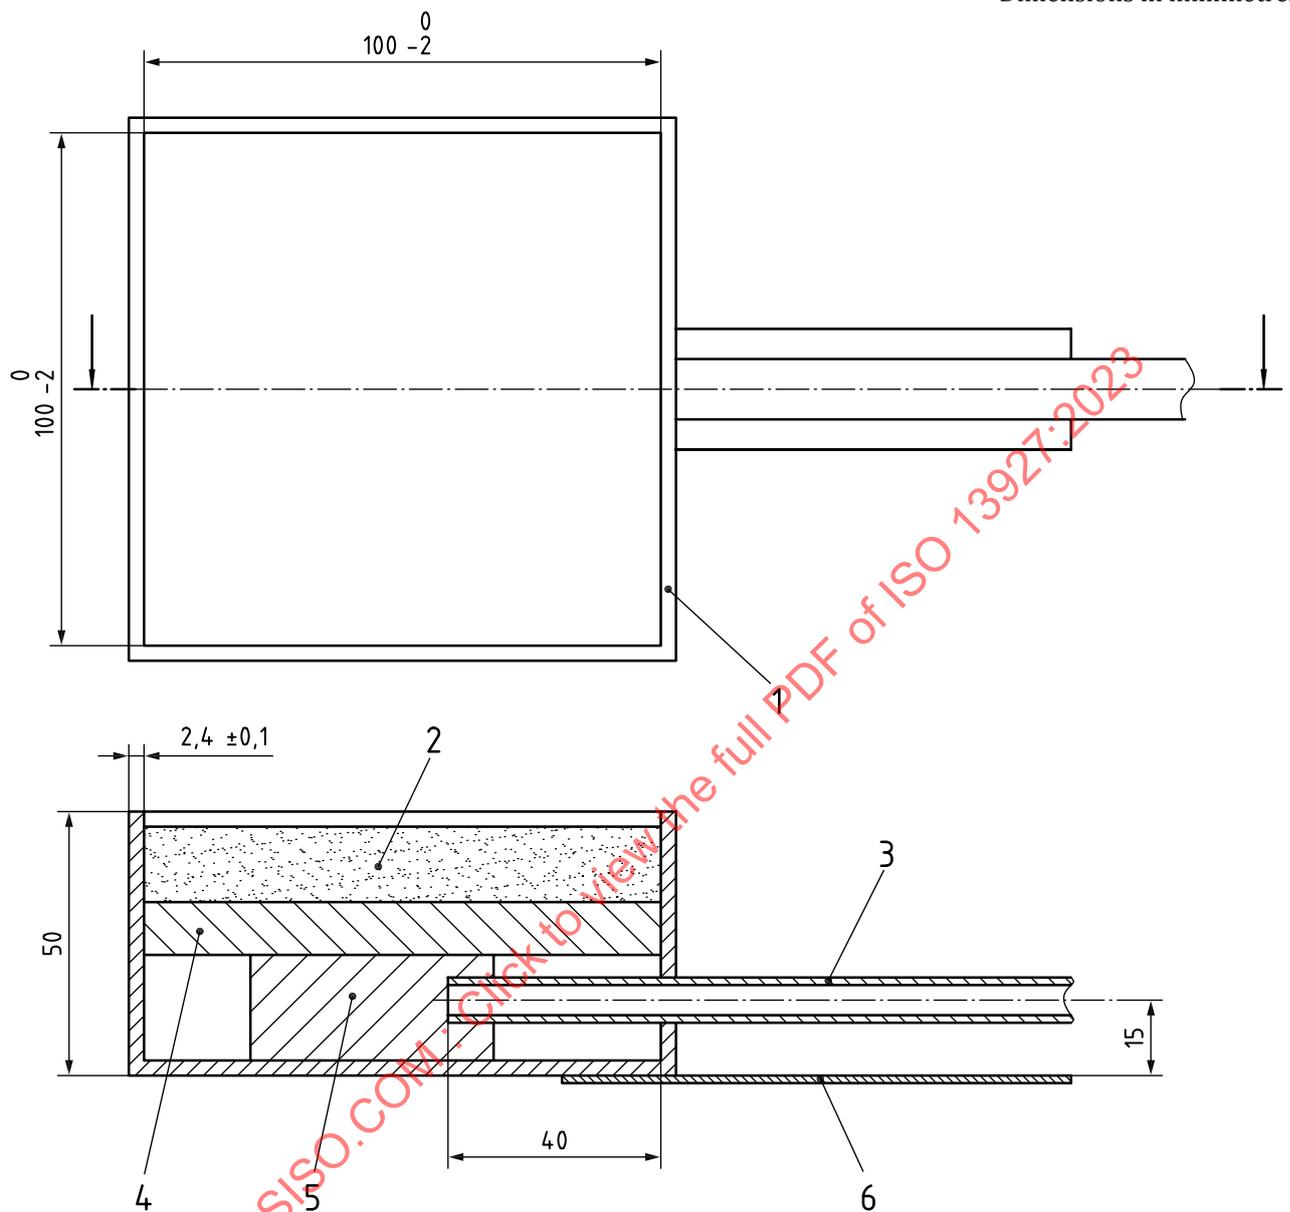**Key**

- 1 square stainless-steel pan
- 2 sand, grain size approximately 1 mm to 2 mm
- 3 tube, inner diameter 8 mm
- 4 ceramic-fibre blanket, 100 mm × 100 mm × 12 mm, density approximately 100 kg/m³
- 5 ceramic-fibre blanket, 50 mm × 50 mm × 22 mm, density approximately 100 kg/m³
- 6 handle

Figure 5 — Typical calibration burner design

7 Suitability of a product for testing

7.1 Surface characteristics

A product having one of the following properties is suitable for testing:

- a) an essentially flat exposed surface;
- b) an irregular surface whose irregularity is evenly distributed over the exposed surface, provided that
 - 1) at least 50 % of the surface of a representative 100 mm² area lies within a depth of 10 mm from a plane taken across the highest points on the exposed surface, or
 - 2) for surfaces containing cracks, fissures, or holes not exceeding 8 mm in width or 10 mm in depth, the total area of such cracks, fissures, or holes at the surface does not exceed 30 % of a representative 100 mm² area of the exposed surface.

When an exposed surface does not meet the requirements of either a) or b), the product shall be tested in a modified form, conforming as nearly as possible to the requirements given above. The test report shall then state that the product has been tested in a modified form and clearly describe the modification.

7.2 Asymmetrical products

A product submitted for this test can have faces which differ or can contain laminations of different materials arranged in a different order in relation to the two faces. If either of the faces can be exposed in use within a room, cavity, or void, then both faces shall be tested.

7.3 Thin materials

This test method can prove unsuitable for excessively thin products since insufficient data will be collected for the calculation of mass loss rates (optional) or thermopile output. For some materials, reducing the data collection interval on any logging system used to 1 s or increasing chart recorder speeds will help to generate more data.

7.4 Composite specimens

The test method is suitable for composite specimens provided they are prepared as specified in [8.3](#).

7.5 Dimensionally unstable materials

This test method is not suitable for materials that change their dimensions substantially when exposed to the cone heater radiation, for example, materials that intumesce or shrink away from the cone radiator because the heat flux on the surface of the specimen at the time of ignition can differ significantly from that which is set initially.

Specimens that intumesce shall be tested by increasing the separation between the bottom side of the cone heater and the specimen surface to 60 mm to accommodate the intumescence. Calibrate the heater at this new separation. Specimens that intumesce so much that when tested at this increased range, they still contact the spark plug or the underside of the cone heater prior to ignition which can only be tested if one of the following methods are employed.

Other dimensionally unstable products, for example, products that warp or shrink during testing, shall be restrained against excessive movement. This shall be accomplished with four tie wires as described below. Metal wires of (1,0 ± 0,1) mm diameter and at least 350 mm long shall be used. The sample shall be prepared in the standard way as described in [Clause 8](#). A tie wire is then looped around the sample holder and retainer frame assembly so that it is parallel to and approximately 20 mm away from one of the four sides of the assembly. The ends of the wires are twisted together such that the wire is pulled

firmly against the retainer frame. Excess wire is trimmed from the twisted section before testing. The three remaining wires shall be fitted around the specimen holder and retainer frame assembly in a similar manner parallel to the three remaining sides.

Materials that distort so extensively that they cannot be held by four wires shall be tested using the fine wire grid used in ISO 5660-1. This is made of $(0,8 \pm 0,1)$ mm steel wire with a spacing between wires of (20 ± 2) mm and is shown in [Figure 6](#).

Materials that intumesce in a fluid phase, such that molten materials overflow the retainer frame or seep between the retainer frame and the specimen holder, and hence invalidate the test, shall be tested without the retainer frame and shall be housed in 0,1 mm thick aluminium tray wrappings ([8.3.1](#)) which extends 10 mm above the top edge of the test specimen.

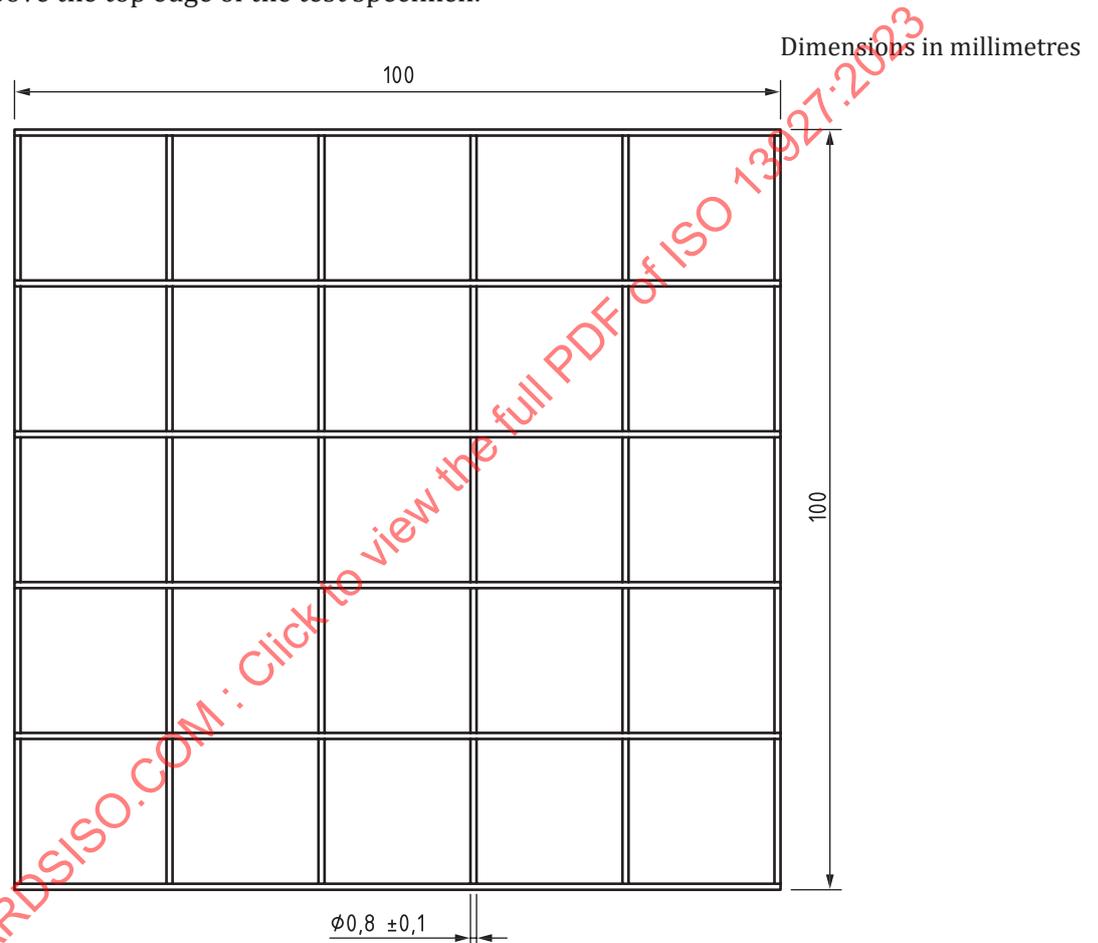


Figure 6 — Wire grid for use with dimensionally unstable materials

7.6 Materials that require testing under compression

Materials, such as fibres, which need to be both physically restrained or compressed to be tested at installed densities, shall be tested in a suitable specimen test cage (see [Figure 7](#)) which provides appropriate artificial boundaries to enable the materials to be tested ([8.3.2](#)). The specimen test cage is made of a steel wire cage constructed from $(1,0 \pm 0,1)$ mm steel wire with (9 ± 1) mm spacing (see [8.3.3](#)).

8 Specimen construction and preparation

8.1 Specimens

8.1.1 Unless otherwise specified, three specimens shall be tested at each level of heat flux selected and for each different exposed surface.

8.1.2 The specimens shall be representative of the product and shall be square with sides measuring (100_{-2}^{+0}) mm.

8.1.3 Products with a normal thickness of 50 mm or less shall be tested using their full thickness.

8.1.4 For products with a normal thickness of greater than 50 mm, the requisite specimens shall be obtained by cutting away the unexposed face to reduce the thickness to (50_{-3}^0) mm.

8.1.5 When cutting specimens from products with irregular surfaces, the highest point on the surface shall be arranged to occur at the centre of the specimen.

8.1.6 Assemblies shall be tested as specified in [8.1.3](#) or [8.1.4](#) as appropriate.

Where thin materials or composites are used in the fabrication of an assembly, the presence of air or an air gap or the nature of any underlying construction can significantly affect the ignition and burning characteristics of the exposed surface. It is important to note that the influence of the underlying layers be understood and taken care of to ensure that the test result obtained on any assembly is relevant to its use in practice.

When the product is a material or composite that would normally be attached to a well-defined substrate, it shall be tested in conjunction with that substrate using the recommended fixing technique, for example, bonded with the appropriate adhesive or fixed mechanically. In the absence of a unique or well-defined substrate, an appropriate substrate for testing shall be selected in accordance with ISO 14697.

8.1.7 Products that are thinner than 6 mm shall be tested with a substrate representative of end-use conditions, such that the total specimen thickness is 6 mm or more. In the case of specimens of less than 6 mm thickness that would be used with an air space adjacent to the unexposed face, the specimens shall be mounted so that there is an air space of at least 12 mm between the unexposed face and the refractory-fibre blanket.

NOTE Air gap can be achieved by the use of a metal spacer frame.

8.2 Conditioning of specimens

Before the test, specimens shall be conditioned to constant mass at a temperature of $23\text{ °C} \pm 2\text{ °C}$ and a relative humidity of $(50 \pm 5)\%$ in accordance with ISO 291.

NOTE Constant mass is considered to be reached when two successive weighing operations, carried out at an interval of 24 h, do not differ by more than 0,1 % of the mass of the test specimen or 0,1 g whichever is the greater.

Materials such as polyamide, which require more than 1 week of conditioning to reach equilibrium, shall be conditioned at a temperature of $23\text{ °C} \pm 2\text{ °C}$ and a relative humidity of $(50 \pm 5)\%$ for not less than one week, and the length of the conditioning period shall be stated in the test report.

8.3 Preparation

8.3.1 Specimen wrapping

A conditioned specimen shall be wrapped in a single layer of aluminium foil of 0,025 mm to 0,04 mm thickness with the shiny side of the foil towards the specimen covering the unexposed surfaces. Composite specimens shall then be exposed in a manner typical of the end-use condition, for example, if used with an air gap (see [8.1.6](#)), an air gap shall be included behind the specimen within the aluminium foil.

The aluminium foil shall be pre-cut to a size to cover the bottom and sides of the specimen and extend 3 mm or more beyond the upper surface of the specimen. The specimen shall be placed in the middle of the foil and the bottom and sides shall be wrapped. The excess foil above the top surface shall be cut if necessary, so that it does not extend more than 3 mm above the top surface of the specimen. The excess foil at the corners shall be folded around the corners to form a seal around the top surface of the specimen. After wrapping, the wrapped specimen shall be placed in the specimen holder and covered by a retainer frame. No aluminium foil shall be visible after the procedure is completed.

For soft specimens, a dummy specimen having the same thickness as the specimen to be tested may be used to pre-shape the aluminium foil.

8.3.2 Specimen preparation

All test specimens (other than those that intumesce in a fluid phase or those that require testing under compressing in specimen cages as in [8.3.3](#)) shall be tested with the retainer frame shown in [Figure 4](#). The following steps shall be taken to prepare the specimen for testing:

- a) put the retainer frame on a flat surface facing downwards;
- b) insert a foil-wrapped specimen in the frame with the exposed surface facing down;
- c) put layers of ceramic-fibre blanket (nominal thickness 13 mm and nominal density 65 kg/m³) on top of the specimen until two layers extend above the rim of the frame;
- d) fit the specimen holder into the frame on top of the ceramic fibre and press down;
- e) tighten the screw through the bottom of the frame and turn the assembly around.

8.3.3 Preparing specimens of materials that require testing under compression

- a) Construct the specimen test cage as shown in [Figure 7](#) by forming a 241 mm × 101 mm sheet of steel mesh constructed from (1,0 ± 0,1) mm steel wire with (9 ± 1) mm separation around a solid template 10 mm × 100 mm × 100 mm.
- b) Remove the template, and then, pack the test material into the specimen cage, such that the density is that which is used in the installed use.
- c) Test the specimen as described in [8.3.1](#), but do not use the retainer frame.

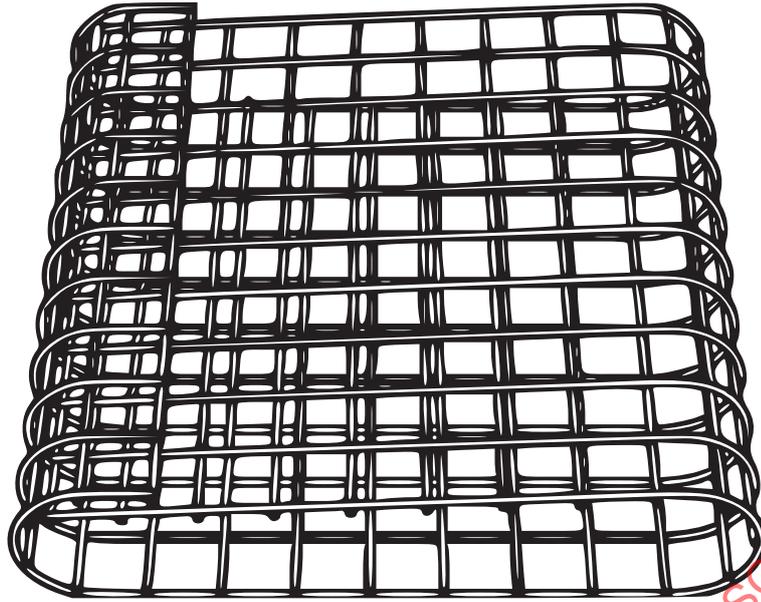


Figure 7 — Specimen test cage for materials requiring testing under compression

9 Calibration

9.1 Heater calibration

Adjust the temperature controller so that the cone heater produces the required heat flux as measured by the heat flux meter at the start of each test day or when changing to a new heat flux.

No specimen or specimen holder shall be used when the heat flux meter is inserted into the calibration position equivalent to the centre of the test specimen surface. Operate the cone heater for at least 10 min and ensure that the temperature controller is within its proportional band before beginning this calibration.

9.2 Thermopile calibration

9.2.1 General

The thermopile shall be calibrated initially at each test heat flux using the procedure given in [9.2.2](#). Thereafter, it shall be checked at the operating heat flux before each day's work. An example of thermopile calibration is given in [Annex D](#).

9.2.2 Initial calibration

The calibration burner described in [6.10](#) and either a data-logging system or a chart recorder shall be used for recording the thermopile output. The calibration shall be undertaken at each heat flux level used for testing. Set the radiators at the set heat flux and allow the system to stabilize. Place the calibration burner in position and introduce methane at a flow rate corresponding to 5 kW based on the net heat of combustion of methane ($50,0 \times 10^3$ kJ/kg)^{[3][4]} using a pre-calibrated flowmeter. Record the stabilized output from the thermopile and repeat the above procedure for methane flow rates equivalent to 4 kW, 3 kW, 2 kW, 1 kW, 0,75 kW and 0,5 kW (other heat level can be used). [Table 1](#) shows mass flow rate (g/min) and volume flow rate (l/min) at 1 atm and 293 K of methane for each relevant heat release rate. Plot a calibration graph of thermopile output versus the heat input from [Table 1](#). An example of such plot is given in [Annex D](#).

Table 1 — Methane flow rate calibration

Heat release rate kW	Methane mass flow rate g/min	Methane flow rate at 293 K l/min
0,50	0,60	0,90
0,75	0,90	1,35
1,00	1,20	1,80
2,00	2,40	3,60
3,00	3,60	5,40
4,00	4,80	7,19
5,00	6,00	8,99

9.2.3 Daily calibration

At the beginning of each working day or when the operating heat flux is changed, the thermopile output shall be checked with a methane flow rate corresponding to 3 kW. If this lies within $\pm 5\%$ of that which is shown in the initial calibration, testing can proceed. If it does not, the thermopile shall be checked for correct positioning and if this is not in error, then the system shall be recalibrated in accordance with 9.2.2. If the thermopile is not correctly positioned, reposition and recalibrate.

10 Test procedure

10.1 General precautions

WARNING — So that suitable precautions are taken to safeguard health, the attention of all concerned in fire tests is drawn to the possibility that toxic or harmful gases can evolve during exposure of test specimens.

The test procedures involve high temperatures and combustion processes. Therefore, hazards can exist for burns, ignition of extraneous objects, or clothing. The operator shall use protective gloves for insertion and removal of test specimens. Neither the cone heater nor the associated fixtures shall be touched while hot, except with the use of protective gloves. Care shall be taken to never touch the spark igniter which carries a substantial potential (10 kV). The apparatus shall be placed under a suitable fume extraction system. This extraction system shall be checked for proper operation before testing and shall discharge into a building extraction system with adequate capacity. The possibility of the violent ejection of hot, molten material, or sharp fragments from some kind of specimen when irradiated cannot be totally discounted and it is therefore essential that eye protection be worn.

10.2 Initial preparation

10.2.1 Turn on the power to the cone heater and the extractor fan.

Do not turn the power to the load cell on and off on a daily basis.

10.2.2 Perform the calibration procedure specified in 9.2.3.

If a load cell is used, put a thermal screen on top of the cell (an empty specimen holder with refractory blanket may be used during warm-up and between tests to avoid excessive heat transmission to the load cell).

10.2.3 Position the spark igniter in the correct location.

10.3 Procedure

10.3.1 When ready to test, remove the empty specimen holder if one has been placed on top of the load cell (see [10.3.7](#)).

10.3.2 Place the specimen in position and start the collection of mass loss (optional) and thermopile output data (the holder shall be at room temperature initially). If a computerized data collection system is used, the data collection intervals shall be 5 s or less.

10.3.3 Move the spark plug in place, turn on the power so that the spark plug is sparking continuously, and at the same time, start the ignition timer.

10.3.4 Record the time at which flashing or transitory flaming occurs. If sustained flaming occurs, record the time and remove the spark igniter. If the flames go out less than 15 min after t_{ig} , re-insert the spark igniter within 5 s of extinguishment and turn on the spark. Leave the spark igniter in position until sustained flaming resumes or until the 15 min post t_{ig} period has elapsed. Report all these events in the test report.

10.3.5 Collect all thermopile and mass loss data (optional):

- a) either until 2 min after flaming or other signs of combustion have ceased, or
- b) if the specimen does not ignite, until 10 min have elapsed (in this case, remove and discard the specimen unless it is showing signs of heat evolution).

Whichever occurs first, observe and record physical changes to the specimen such as melting, swelling, and cracking.

10.3.6 Remove the specimen and specimen holder.

10.3.7 Replace with an empty specimen holder.

10.3.8 Test three specimens in this way and report as described in [Clause 12](#).

10.3.9 Use the calibration graph of heat release against thermopile output produced as described in [9.2.2](#) to calculate all heat release data quoted in the test report.

NOTE The test data have limited validity if the specimen melts sufficiently to overflow from the specimen holder if explosive spalling occurs or if the specimen swells excessively and touches the spark igniter or the heater baseplate.

11 Precision

The precision of this test method is not known because interlaboratory data are not available at the time of publication.

12 Test report

The test report shall be as comprehensive as possible and shall include any observations made during the test and comments on any difficulties experienced during testing. The units for all measurements shall be clearly stated in the test report.

The following essential information shall be given in the report:

- a) name and address of the test laboratory;

- b) name and address of the person/organization requesting the test;
- c) name and address of the manufacturer/supplier of the material tested;
- d) date of the test;
- e) operator;
- f) trade name of the material tested and the specimen identification code or number;
- g) composition or generic identification of the material tested;
- h) specimen thickness, expressed in millimetres, and specimen mass, expressed in grams [with composites and assemblies, the nominal thickness and density of each of the components shall be given together with the apparent (overall) density of the whole];
- i) colour of the specimens;
- j) details of specimen preparation by the test laboratory;
- k) details of specimen mounting including any special mounting procedures used (e.g. for intumescent materials) and details of the face tested;
- l) heat flux produced by the heater, expressed in kilowatts per square metre, and the flow rate of the extraction system, expressed in cubic metres per second;
- m) number of replicate specimens tested under the same conditions [this will normally be three (see [8.1.1](#)), except for exploratory testing];
- n) time to sustain flaming, expressed in seconds;
NOTE Method of calculation of effective critical heat flux for ignition is given in [Annex E](#) for information.
- o) test duration, i.e. the time between the start of the test and the end as defined in [10.3.5](#), expressed in seconds;
- p) values, expressed in kilowatts per square metre, of the heat release rate per unit area at 180 s after ignition \dot{q}''_{180} , and at 300 s after ignition \dot{q}''_{300} , and the maximum heat release rate per unit area reached \dot{q}''_{\max} (see [10.3.9](#));
- q) average, for all replicate determinations, of the values reported in items n) and o);
- r) any additional observations such as transitory flaming or flashing;
- s) mass loss results in accordance with [C.4](#) (optional);
- t) details of any difficulties encountered in testing.

Annex A (normative)

Calibration of the heat flux meter

The calibration of the heat flux meter shall be checked whenever recalibration of the apparatus is carried out in comparison with two instruments of the same type as the working heat flux meter and of similar range held as reference standards and not used for any other purpose.

One of the heat flux meter reference standards shall be fully calibrated against a primary reference standard instrument at yearly intervals. This meter shall be used to calibrate the heater temperature controller. It shall also be positioned at a location equivalent to the centre of the specimen face during this calibration.

The inter-comparison of working and reference standard heat flux meters required above shall be made using the conical heater with each heat flux meter mounted in turn in the calibration position with care being taken to allow the whole apparatus to attain thermal equilibrium. Alternatively, an apparatus specially built for comparative purposes may be used (e.g. that specified in BS 6809).

NOTE The use of two reference standards rather than one provides a greater safeguard against change in sensitivity of the reference instruments.

STANDARDSISO.COM : Click to view the full PDF of ISO 13927:2023

Annex B (informative)

Guidance notes for operators

B.1 General

This annex aims to provide the operator carrying out the test and the user of the test results with background information on the method, the apparatus, and the data obtained.

B.2 Heat release rate measurements

The test method does not prescribe the heat flux levels, nor whether external ignition is to be used. These should be determined separately for each product to be assessed. For given applications and products, a comparison with full-scale fires is generally necessary to determine the time period over which heat release is to be calculated.

For exploratory testing, it is recommended that the spark igniter and a heat flux of 35 kW/m² be used initially. In the absence of further specifications from the person/organization ordering the test, testing at 25 kW/m², 35 kW/m², and 50 kW/m² are recommended. The results obtained can then suggest whether additional testing at different heat flux levels is desirable.

The test results might not be statistically significant unless the heat flux used (10 kW/m²) is substantially higher than the minimum heat flux level needed for sustained flaming to occur for that specimen.

B.3 Back face conditions

The heat losses through the back face of the specimen can have an influence on the area burning rate near the end of the burning time. For reproducible measurements, the loss through the back face should be standardized and this is achieved by using a layer of insulating material.