
INTERNATIONAL STANDARD



1432

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION • МЕЖДУНАРОДНАЯ ОРГАНИЗАЦИЯ ПО СТАНДАРТИЗАЦИИ • ORGANISATION INTERNATIONALE DE NORMALISATION

Rubber, vulcanized — Determination of stiffness at low temperature (Gehman test)

Caoutchouc vulcanisé — Détermination de la rigidité à basse température (essai Gehman)

First edition — 1976-10-15

STANDARDSISO.COM : Click to view the full PDF of ISO 1432:1976

UDC 678.4/.7.063 : 678.01 : 539.414

Ref. No. ISO 1432-1976 (E)

Descriptors : rubber, vulcanized rubber, tests, low temperature tests, stiffness tests.

FOREWORD

ISO (the International Organization for Standardization) is a worldwide federation of national standards institutes (ISO member bodies). The work of developing International Standards is carried out through ISO technical committees. Every member body interested in a subject for which a technical committee has been set up has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work.

Draft International Standards adopted by the technical committees are circulated to the member bodies for approval before their acceptance as International Standards by the ISO Council.

Prior to 1972, the results of the work of the technical committees were published as ISO Recommendations; these documents are in the process of being transformed into International Standards. As part of this process, Technical Committee ISO/TC 45, *Rubber and rubber products*, has reviewed ISO Recommendation R 1432-1971 and found it technically suitable for transformation. International Standard ISO 1432 therefore replaces ISO Recommendation R 1432-1971, to which it is technically identical.

ISO Recommendation R 1432 had been approved by the member bodies of the following countries :

Australia	Greece	Poland
Austria	Hungary	Spain
Brazil	India	Sweden
Canada	Iran	Switzerland
Colombia	Israel	Thailand
Czechoslovakia	Italy	Turkey
Egypt, Arab Rep. of	Korea, Rep. of	United Kingdom
France	Netherlands	U.S.A.
Germany	New Zealand	U.S.S.R.

No member body had expressed disapproval of the Recommendation.

No member body disapproved the transformation of the Recommendation into an International Standard.

Rubber, vulcanized – Determination of stiffness at low temperature (Gehman test)

1 SCOPE AND FIELD OF APPLICATION

This International Standard specifies a static procedure, known as the Gehman test, for determining the relative stiffness characteristics of vulcanized rubbers over a temperature range from room temperature to approximately -70°C .

2 APPARATUS¹⁾

2.1 Torsion apparatus, as shown in the figure. It consists of a torsion head (A), capable of being turned 180° in a plane normal to the torsion wire (B). The top of the wire is fastened to the torsion head through a loosely fitting sleeve (C). The bottom of the wire is fastened to the test piece clamp stud (D) by means of a screw connector (E). A pointer (F) and a movable protactor (G) are provided to permit convenient and exact adjustment of the zero point. The torsion apparatus is clamped to a supporting stand (H). It is advantageous to make the vertical portion of the stand from material of poor thermal conductivity. The base of the stand shall be of stainless steel or other corrosion-resistant material.

2.2 Torsion wires (B), made of tempered spring wire, of length 65 ± 8 mm, and having torsional constants of 0,70, 2,81 and 11,24 mJ/rad of twist.

The 2,81 mJ/rad wire shall be considered the standard wire.

2.3 Test piece rack (I), made of material of poor thermal conductivity, for holding the test piece (J) in a vertical position in the heat transfer medium. The rack shall be constructed to hold several test pieces²⁾. The rack is clamped to the stand (H).

Two clamps shall be provided for holding each test piece. The bottom clamp (K) shall be a fixed part of the test piece rack. The top clamp (L) acts as an extension of the test piece and shall not touch the rack³⁾. The top clamp is secured to a stud (D) which in turn is connected to the screw connector (E).

2.4 Temperature-measuring device, capable of measuring the temperature to within 1°C over the range from approximately -70°C to $+30^{\circ}\text{C}$. Copper-constantan thermocouples, used in conjunction with a potentiometer, are highly satisfactory.

The sensitive element shall be positioned between two test pieces, equidistant from the top and bottom respectively.

2.5 Heat-transfer media, which may be liquid or gaseous. Any material which remains fluid at the test temperature and which will not effect the materials being tested may be used. Among the liquids that have been found suitable for use at low temperatures are acetone, methanol, ethanol, butanol, silicone fluid and *n*-hexane. Carbon dioxide or air are commonly used gaseous media.

Vapours of liquid nitrogen are useful for testing at very low temperatures.

It should be noted that stiffness measurements in gaseous media may not give in each case the same results as the measurements made in liquid media.

2.6 Temperature control, for controlling the temperature of the heat-transfer medium within $\pm 1,0^{\circ}\text{C}$.

2.7 Tank, for liquid heat-transfer media, or **test chamber** for gaseous media.

2.8 Stirrer, for liquids, or **fan** or **blower** for air, which ensures thorough circulation of the heat-transfer medium.

2.9 Stop-watch, or other timing device, calibrated in seconds.

1) The apparatus and its use are described in "Low temperature characteristics of elastomers" S. D. Gehman, D. E. Woodford and C. S. Wilkinson, *Ind. and Eng. Chem.*, Vol. 39, Sept. 1947, p 1108.

2) Racks providing space for five or ten test pieces are commonly used.

3) Clearance between the top of the test piece rack and the test piece clamp stud is ensured by inserting thin spacers between the two. Slotted laminated plastics of thickness about 1,3 mm and width about 12 mm have been found satisfactory. At low temperatures the test pieces stiffen in position and the spacers may be removed without losing the clearance.

3 TEST PIECE

3.1 Preparation of test piece

The test piece shall be $40 \pm 2,5$ mm, $3 \pm 0,2$ mm, and $2 \pm 0,2$ mm. It shall be moulded or cut with a suitable die from a vulcanized sheet of suitable thickness.

3.2 Conditioning of test piece

3.2.1 The minimum time between vulcanization and testing shall be 16 h.


For non-product tests, the maximum time between vulcanization and testing shall be 4 weeks and, for evaluations intended to be comparable, the tests should be carried out, as far as possible, after the same time-interval.

For product tests, whenever possible, the time between vulcanization and testing should not exceed 3 months. In other cases, tests shall be made within 2 months of the date of receipt by the customer of the product.

3.2.2 Samples and test pieces shall be protected from light as completely as possible during the interval between vulcanization and testing.

3.2.3 Prepared test pieces shall be conditioned immediately before testing for a minimum of 3 h at a standard laboratory temperature, the same temperature being used throughout any one test or series of tests intended to be comparable.

STANDARDSISO.COM : Click to view the full PDF of ISO 1432-1976

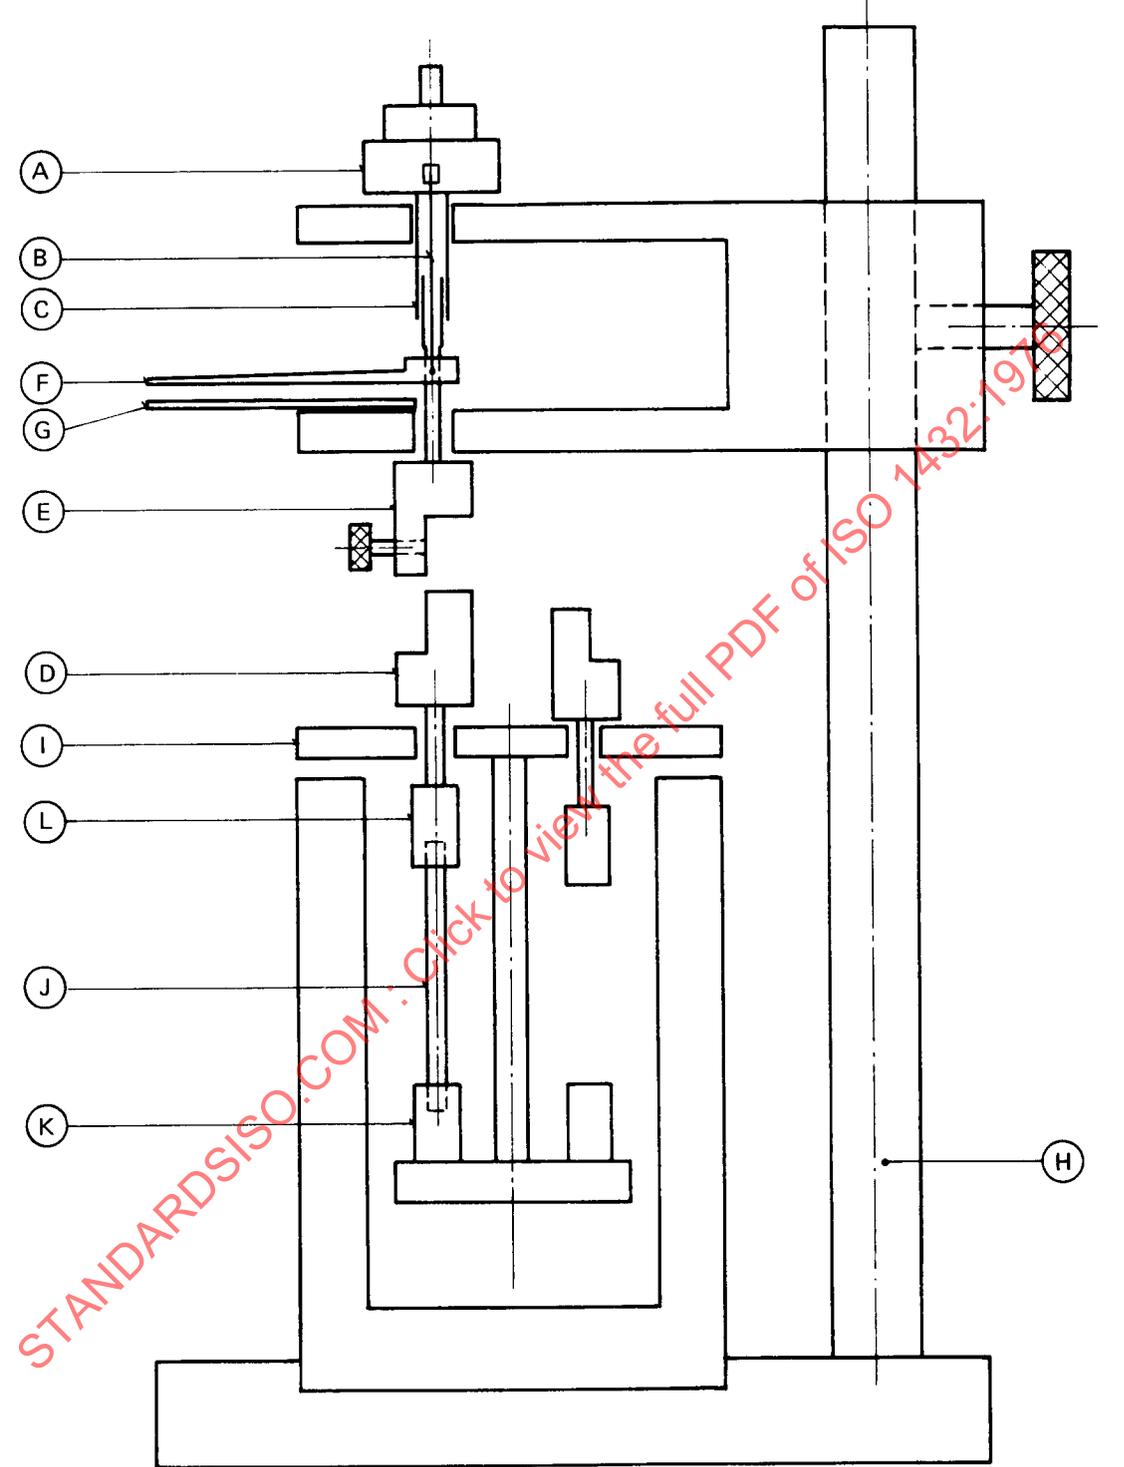

- | | | |
|------------------|------------------------|------------------|
| (A) Torsion head | (E) Screw connector | (I) Rack |
| (B) Torsion wire | (F) Pointer | (J) Test piece |
| (C) Sleeve | (G) Movable protractor | (K) Bottom clamp |
| (D) Clamp stud | (H) Supporting stand | (L) Top clamp |

FIGURE – Apparatus for determination of stiffness characteristics

4 PROCEDURE

4.1 Calibration of torsion wire

Insert one end of the torsion wire (B) in a vertical position, in a fixed clamp, and attach the lower end of the wire at the exact longitudinal centre of a rod of known dimensions and mass. (It is suggested that the length of the rod be 200 to 250 mm and the diameter about 6,4 mm.)

Twist the rod through an angle of not more than 90° and then release it. Allow it to oscillate freely in a horizontal plane and note the time, in seconds, for 20 oscillations. (An oscillation includes the swing from one extreme to the other and return.)

The mass moment of inertia I of the rod is given, in kilogram millimetres squared, by the formula

$$I = \frac{m L^2}{12}$$

where

m is the mass, in kilograms, of the rod;

L is the length, in millimetres, of the rod.

The torsional constant (i.e. the restoring torque) λ of the wire is given, in millijoules per radian of twist, by the formula

$$\lambda = \frac{\pi^2 I}{250 T^2}$$

where

I is the mass moment of inertia, in kilogram millimetres squared, of the rod;

T is the period of one oscillation, in seconds.

The torsion wires shall calibrate within ± 3 % of their specified torsional constants.

4.2 Mounting of test piece

Clamp each test piece used in such a manner that 25 ± 3 mm of the test piece is free between the clamps. The test piece clamp stud (D) shall be located with respect to a reference point on the rack (I) in such a position that the specimen is under zero torque.

4.3 Stiffness measurements in liquid media

Place the rack (I) containing the test pieces in the liquid bath with a minimum of 25 mm of liquid covering the test pieces. Then adjust the temperature of the bath to 25 °C. Connect one of the test pieces to the torsion head (A) by means of the screw connector (E) and the standard wire.

Take care when attaching the screw connector to the test piece clamp stud (D) not to move the stud from the zero torque position. The position head (A) shall also remain in the zero position while the connector is being fastened to the stud. The spacer which provides clearance between the test piece rack and the test piece clamp stud need not be used for measurements made at room temperature.

Adjust the pointer reading to zero by rotating the protractor scale (G). Then turn the torsion head quickly but smoothly through 180° and record the pointer reading after 10 s as indicated by the timer (2.9). If the reading at 25 °C does not fall in the range of 120 to 170°, the standard torsion wire is not suitable for testing the test piece. Test pieces producing twists of more than 170° shall be tested with a wire having a torsional constant of 0,70 mJ/rad of twist. Test pieces producing twists of less than 120° shall be tested with a wire having a torsional constant of 11,24 mJ/rad of twist.

Return the torsion head to its initial position and disconnect the test piece.

Then move the test piece rack to bring the next test piece into position for measurement¹⁾.

Measure all the test pieces in the rack at 25 °C.

Insert the spacers between the test piece rack and the test piece clamp studs. Remove the test pieces from the liquid bath and adjust the temperature of the liquid to the lowest temperature desired. Replace the test pieces in the bath and maintain them at this temperature for approximately 15 min. After this, remove one spacer and measure one test piece as was done at 25 °C²⁾. Return the spacer to its original position after the test piece has been tested. Measure all the test pieces in the rack in this way, taking care that the measurement of each test piece lasts approximately 2 min.

Then increase the bath temperature by 5 °C intervals, making each increase in approximately 5 min. Carry out the stiffness measurements after conditioning the test piece for 5 min at each temperature. Continue the tests until a temperature is reached at which the angular twist is within 5 to 10° of the twist at 25 °C.

4.4 Stiffness measurements in gaseous media

Procedures in air or carbon dioxide differ from those with liquid media only in that cooling is effected with the test pieces in the medium and that the length of the conditioning period is different.

With the test pieces in the test chamber (2.7), adjust the temperature of the chamber to the lowest temperature desired in approximately 30 min. After this temperature has been maintained constant for 10 min, carry out the measurements as for the liquid media, testing each test piece in 2 min.

1) Apparatus is now in use in which the rack is stationary while the torsion head is movable and can be positioned over the several test pieces in turn.

2) Movement of the spacer often tends to alter the pointer position with respect to the protractor; therefore, adjust the pointer to zero after removing the spacer.