
**Optics and optical instruments — Test
methods for telescopic systems —**

Part 7:

Test methods for limit of resolution

*Optique et instruments d'optique — Méthodes d'essai pour systèmes
télescopiques —*

Partie 7: Méthodes d'essai pour limite de résolution

STANDARDSISO.COM : Click to view the full PDF of ISO 14490-7:2005



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 14490-7:2005

© ISO 2005

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword.....	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Method of determination of the limit of resolution	1
4.1 General	1
4.2 Test equipment	1
4.3 Preparation and carrying out of measurements	3
4.4 Determination of results	3
5 Test report	3
Annex A (informative) Dimensions of a bar-type test target for determination of the limit of resolution of telescopic systems	4
Bibliography	9

STANDARDSISO.COM : Click to view the full PDF of ISO 14490-7:2005

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 14490-7 was prepared by Technical Committee ISO/TC 172, *Optics and photonics*, Subcommittee SC 4, *Telescopic systems*.

ISO 14490 consists of the following parts, under the general title *Optics and optical instruments — Test methods for telescopic systems*:

- *Part 1: Test methods for basic characteristics*
- *Part 2: Test methods for binocular systems*
- *Part 3: Test methods for telescopic sights*
- *Part 4: Test methods for astronomical telescopes*
- *Part 5: Test methods for transmittance*
- *Part 6: Test methods for veiling glare index*
- *Part 7: Test methods for limit of resolution*

Introduction

There are various characteristics which are relevant for overall image quality of telescopic systems and observational telescopic instruments. Two important characteristics are the limit of resolution and the optical transfer function.

The present part of ISO 14490 specifies the test method for the determination of the limit of resolution of telescopic systems and observational telescopic instruments. Optical transfer function measurement as applied to telescopic systems is specified in ISO 9336-3 (see bibliography).

Besides the limit of resolution and the optical transfer function, further characteristics are relevant for an assessment of the image quality; the most important of them are

- secondary spectrum (dispersive aberrations);
- distortion;
- vignetting;
- colour matching.

The secondary spectrum of the test specimen can produce colour fringes surrounding observed objects (especially at high-contrast edges) which can look like coloured neon tube light.

The distortion of the perceived image might be of barrel or pincushion type. The pincushion type is considered to give a more naturalistic impression of the observed object when swivelling the test specimen.

Vignetting can lead to a perceivable intensity degradation from the centre to the edge of the field of view.

Colour matching is the accuracy of the colour rendition of an object observed with the test specimen. Any colour deviation might be due to the lens material or to coatings.

Optics and optical instruments — Test methods for telescopic systems —

Part 7: Test methods for limit of resolution

1 Scope

This part of ISO 14490 specifies the test methods for the determination of the limit of resolution of telescopic systems and observational telescopic instruments.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 14132-1:2002, *Optics and optical instruments — Vocabulary for telescopic systems — Part 1: General terms and alphabetical indexes of terms in ISO 14132*

ISO 14490-1:2005, *Optics and optical instruments — Test methods for telescopic systems — Part 1: Test methods for basic characteristics*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 14132-1 apply.

4 Method of determination of the limit of resolution

4.1 General

The limit of resolution of a telescopic system is the minimum angular distance between centrelines of two adjacent bright (or dark) bars of the bar-type resolution test target whose direction can be detected when viewing through the test specimen.

4.2 Test equipment

The limit of resolution of telescopic systems shall be determined with the test arrangement shown in Figure 1.

The bar-type resolution test target has contrast

$$K = \frac{\tau_{tr} - \tau_{op}}{\tau_{tr} + \tau_{op}} \geq 0,9 \tag{1}$$

where

τ_{tr} is the transmittance of a translucent part of the resolution test target;

τ_{op} is the transmittance of an opaque part of the resolution test target.

It shall be placed at the focal plane of the collimator lens.

For systems that require the limit of resolution to be measured with a focus setting other than infinity, the position of the resolution test target with respect to the collimator lens shall be adjusted in order to obtain its image at the specified distance from the test specimen.


The bar-type resolution test target is a glass plate bearing a picture that consists of bright bars having different widths on a dark background.

The dimensions of one acceptable design of bar-type resolution test target are given in Annex A.

The resolution test target shall be illuminated uniformly ($\pm 5\%$) by means of a light source with a correlated colour temperature of 5 000 K to 6 000 K, condenser and diffuser for non-dazzling observation conditions. The illuminance of the resolution test target shall be optimum for observation of its image.

The diameter of the collimator lens shall at least exceed 1,2 times the diameter of the entrance pupil of the test specimen. The focal length of the collimator lens shall be at least 5 times that of the objective of the test specimen.

The magnification of the auxiliary telescope shall not reduce the diameter of the exit pupil of the whole system below 0,8 mm.

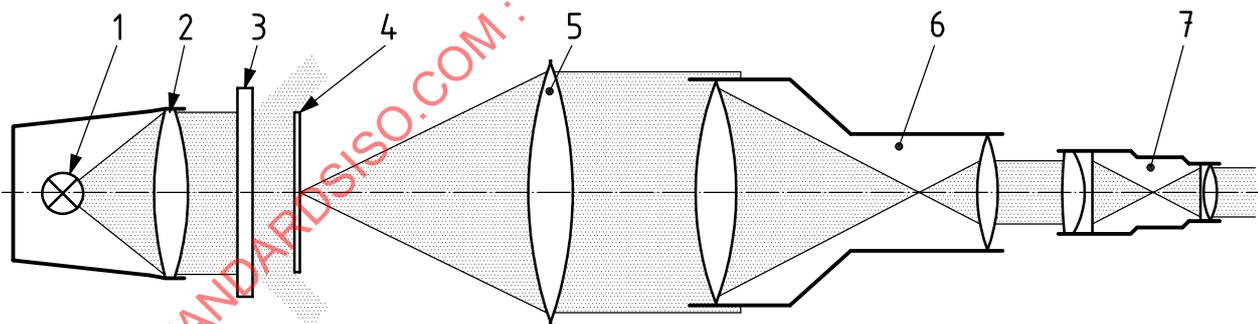

Key

- | | |
|-----------------------------------|-----------------------|
| 1 light source | 5 collimator lens |
| 2 condenser | 6 test specimen |
| 3 diffuser | 7 auxiliary telescope |
| 4 bar-type resolution test target | |

^a The auxiliary telescope should not be used if the angular limit of resolution behind the eyepiece of the test specimen is worse than 2' to 3' and the diameter of the exit pupil is below 1 mm.

Figure 1 — Test arrangement for measurement of the limit of resolution (schematic)

4.3 Preparation and carrying out of measurements

Eliminate all possible stray light and vibration from the test set-up.

Check the cleanliness of the optical surfaces of the lenses of the test specimen, the collimator lens, the condenser, and the auxiliary telescope. No traces of lubricants, fingerprints, moisture, or dust are allowed.

Select the size number of the resolution test target according to the focal length of the collimator lens and the limit of resolution of the test specimen (for instance, see Table A.2).

If an auxiliary telescope is used, adjust its eyepiece according to the observer's eye to allow sharp viewing of the telescope reticle. The auxiliary telescope and the eye of the observer shall not limit the assessment of the resolution. After that, focus the auxiliary telescope on the image of the resolution test target which is located in the focal plane of the collimator lens.

Focus the test specimen on the image of the resolution test target; then position the test specimen and the auxiliary telescope coaxially with the collimator lens.

Set the eyepiece of the test specimen in a position which enables sharp viewing of the reticle of the test specimen through the auxiliary telescope. If no reticle is provided, adjust the eyepiece to zero dioptres.

Determine the limit of resolution of the test specimen in the centre of the field of view.

During observation through the eyepiece of the auxiliary telescope, the maximum sharpness of bars of all patterns in one group of the resolution test target shall be obtained by means of refocusing the test specimen. If no focusing is available in the test specimen, the maximum sharpness of bars of the resolution test target shall be obtained by refocusing the auxiliary telescope.

During successive viewing of images of certain groups of the resolution test target having different spatial frequencies, a group of the resolution test target shall be found which enables easy detection of all four bar directions. This shall be achieved without refocusing for the different bar directions. This group shall be located in the centre of the field of view of the test specimen.

4.4 Determination of results

From the size number of the resolution test target group that enables the detection of all four pattern directions, determine the bar width b .

Calculate the angular distance φ , in seconds of angle, between the centrelines of adjacent dark (or bright) bars of each resolution test target group according to the equation

$$\varphi = \frac{2b}{f'_k} \times 206\,265 \quad (2)$$

where

b is the bar width in mm;

f'_k is the focal length of the collimator lens in mm;

206 265 is the number of arc seconds/radian.

5 Test report


A test report shall be presented and shall include the general information specified in Clause 13 of ISO 14490-1:2005, the result of the test as specified in 4.4 above and information on the test target used for the test.

Annex A
(informative)

Dimensions of a bar-type test target for determination of the limit of resolution of telescopic systems

A.1 Resolution test target layout

The resolution test target consists of 25 groups, as shown in Figure A.1, and two pairs of parallel, equally spaced marks. The distance between the centres of the marks that defines the size of the test target is called the test target base.

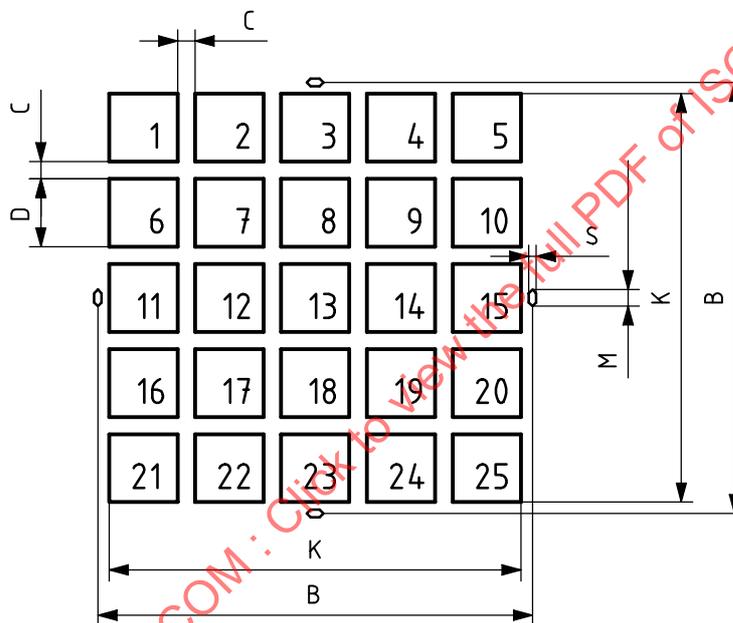

Dimensions of resolution test targets are given in Table A.1.


Figure A.1 — Resolution test target layout

A.2 Layout of groups of resolution test target

Each group of the resolution test target consists of four patterns formed by five bars each. The bars have equal lengths and widths and are arranged as shown in Figure A.2. The intervals between adjacent bars are equal to the bar width.

A.3 Dimensions

Dimensions of resolution test targets should be in accordance with Table A.1.

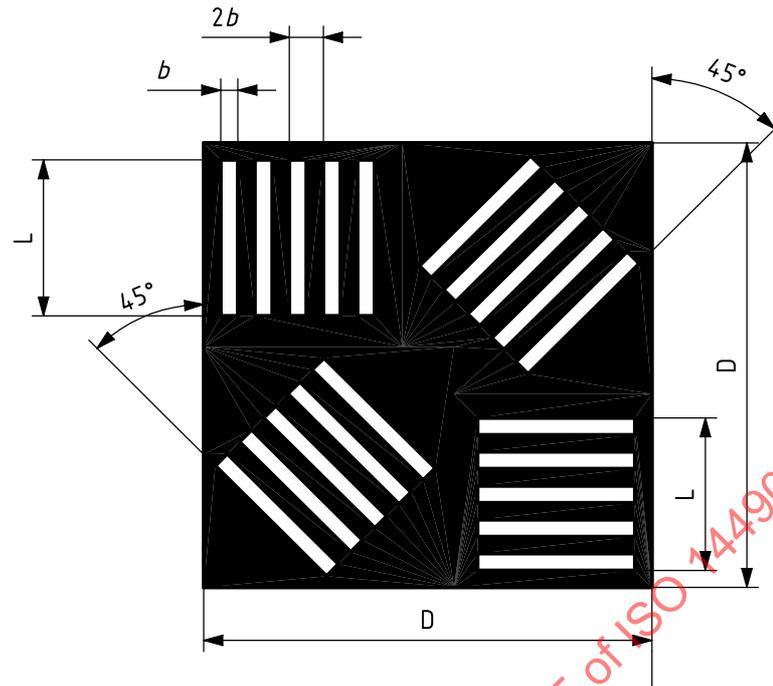

Dimensions of resolution test targets are given in Table A.1.

Figure A.2 — A group of the resolution test target

A.4 Bar width

The bar width b in the resolution test target shall decrease from the group No.1 to the group No.25 in accordance with the geometric progression having the base $2^{-1/12} = 0,94$.

NOTE For dimensions, see Table A.1.

A.5 Number of bars

The number N of bars per millimetre for any test target group number should be determined by division of 1 000 μm by the total width of a dark plus a bright bar ($2b$) in μm .

Table A.1 — Dimensions of resolution test targets

Dimensions in millimetres

Designation ^a	Test target number					
	1	2	3	4	5	6
B	1,2	2,4	4,8	9,6	19,2	38,4
D	0,2	0,4	0,9	1,7	3,5	7,0
C	0,01	0,02	0,04	0,08	0,16	0,32
K	1,1	2,3	4,5	9,1	18,2	36,4
M	0,05	0,1	0,2	0,4	0,8	1,6
S	0,005	0,01	0,02	0,04	0,08	0,16
L	0,09	0,18	0,36	0,72	1,44	2,88

^a See Figures A.1 and A.2.

A.6 Angular distance between centrelines of adjacent bars

The angular distance φ , in seconds of angle, between the centrelines of adjacent dark (or bright) bars of each resolution test target group is calculated in accordance with Equation 2 (see 4.4).

The values of the angular distance φ which depend on the focal length of the collimator objective f'_k and the number of bars N for the test target specified in this annex are given in Table A.2.

Table A.2 — Values of the angular distance φ for the test target specified in A.1 to A.5

Numbers of target groups for a test target number						Bar width b	Bars N	Angular distance φ between the middles of adjacent bars for a given collimator focal length f'_k in seconds						
Test target number						μm	bars/mm	f'_k mm						
1	2	3	4	5	6			600	1 000	1 200	1 600	2 500	3 000	5 000
25	—	—	—	—	—	2,5	200	1,72	1,03	0,88	0,64	0,41	0,34	0,20
24	—	—	—	—	—	2,6	190	1,82	1,09	0,91	0,68	0,44	0,36	0,22
23	—	—	—	—	—	2,8	180	1,93	1,16	0,96	0,72	0,46	0,38	0,23
22	—	—	—	—	—	3,0	170	2,04	1,23	1,02	0,76	0,49	0,40	0,25
21	—	—	—	—	—	3,1	160	2,16	1,30	1,08	0,81	0,52	0,43	0,26
20	—	—	—	—	—	3,3	150	2,29	1,38	1,15	0,86	0,55	0,46	0,28
19	—	—	—	—	—	3,5	140	2,43	1,46	1,22	0,91	0,58	0,49	0,29
18	—	—	—	—	—	3,7	130	2,58	1,54	1,29	0,96	0,62	0,51	0,31
17	—	—	—	—	—	4,0	125	2,73	1,63	1,37	1,02	0,65	0,54	0,33
16	—	—	—	—	—	4,2	120	2,89	1,73	1,45	1,08	0,70	0,57	0,35
15	—	—	—	—	—	4,5	110	3,06	1,83	1,53	1,15	0,74	0,61	0,37
14	—	—	—	—	—	4,7	105	3,24	1,94	1,62	1,22	0,78	0,65	0,38
13	25	—	—	—	—	5,0	100	3,44	2,06	1,72	1,29	0,82	0,69	0,41
12	24	—	—	—	—	5,3	95	3,64	2,18	1,82	1,36	0,87	0,73	0,44
11	23	—	—	—	—	5,6	90	3,86	2,31	1,93	1,44	0,92	0,77	0,46
10	22	—	—	—	—	5,9	85	4,08	2,45	2,04	1,52	0,98	0,82	0,49
9	21	—	—	—	—	6,3	80	4,33	2,60	2,16	1,62	1,04	0,87	0,52
8	20	—	—	—	—	6,7	75	4,58	2,76	2,29	1,72	1,10	0,92	0,55
7	19	—	—	—	—	7,1	70	4,86	2,92	2,43	1,82	1,16	0,97	0,58
6	18	—	—	—	—	7,5	65	5,16	3,08	2,58	1,92	1,24	1,02	0,62
5	17	—	—	—	—	7,9	63	5,46	3,26	2,73	2,04	1,32	1,08	0,66
4	16	—	—	—	—	8,4	60	5,78	3,46	2,90	2,16	1,40	1,14	0,70
3	15	—	—	—	—	8,9	56	6,12	3,65	3,06	2,30	1,48	1,22	0,74
2	14	—	—	—	—	9,4	53	6,48	3,88	3,24	2,44	1,56	1,30	0,78
1	13	25	—	—	—	10,0	50	6,88	4,12	3,44	2,58	1,64	1,38	0,82