

---

---

**Plastics — Determination of haze for  
transparent materials**

*Plastiques — Détermination du trouble des matériaux transparents*

STANDARDSISO.COM : Click to view the full PDF of ISO 14782:2021



STANDARDSISO.COM : Click to view the full PDF of ISO 14782:2021



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
Foreword.....	iv
<b>1</b> <b>Scope</b> .....	<b>1</b>
<b>2</b> <b>Normative references</b> .....	<b>1</b>
<b>3</b> <b>Terms and definitions</b> .....	<b>1</b>
<b>4</b> <b>Principle</b> .....	<b>1</b>
<b>5</b> <b>Apparatus</b> .....	<b>2</b>
<b>6</b> <b>Specimens</b> .....	<b>3</b>
<b>7</b> <b>Conditioning</b> .....	<b>4</b>
<b>8</b> <b>Procedure</b> .....	<b>4</b>
<b>9</b> <b>Expression of results</b> .....	<b>4</b>
<b>10</b> <b>Precision</b> .....	<b>5</b>
<b>11</b> <b>Test report</b> .....	<b>6</b>
<b>Bibliography</b> .....	<b>7</b>

STANDARDSISO.COM : Click to view the full PDF of ISO 14782:2021

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*.

This second edition cancels and replaces the first edition (ISO 14782:1999), which has been technically revised. It also incorporates the Technical Corrigendum ISO 14782:1999/Cor 1:2005.

The main changes compared to the previous edition are as follows:

- [Formula \(1\)](#) in [Clause 9](#) has been corrected;
- the document has been editorially revised.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

# Plastics — Determination of haze for transparent materials

## 1 Scope

This document specifies a method for the measurement of haze, an optical property resulting from wide-angle scattering of light, in transparent and substantially colourless plastics. This method is applicable to the measurement of haze values of less than 40 %.

**NOTE** The haze of abraded or matted transparent plastics can be measured, but the value obtained can be erroneously lower than the true value due to light scattering within a narrow angle.

## 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 472, *Plastics — Vocabulary*

ISO 291, *Plastics — Standard atmospheres for conditioning and testing*

ISO/CIE 11664-1, *Colorimetry — Part 1: CIE standard colorimetric observers*

ISO 11664-2, *Colorimetry — Part 2: CIE standard illuminants*

ISO 13468-1, *Plastics — Determination of the total luminous transmittance of transparent materials — Part 1: Single-beam instrument*

CIE PUBLICATION No. 15, *Colorimetry*

## 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 472 and ISO 13468-1 apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at <https://www.iso.org/obp>


— IEC Electropedia: available at <https://www.electropedia.org/>

## 4 Principle

Haze is determined using an integrating sphere the efficiency of which is held constant by compensation.

## 5 Apparatus

5.1 The apparatus shall consist of a stabilized light source, an associated optical system, an integrating sphere with ports, and a photometer comprising a photodetector, signal processor and display unit or recorder (see [Figure 1](#)).

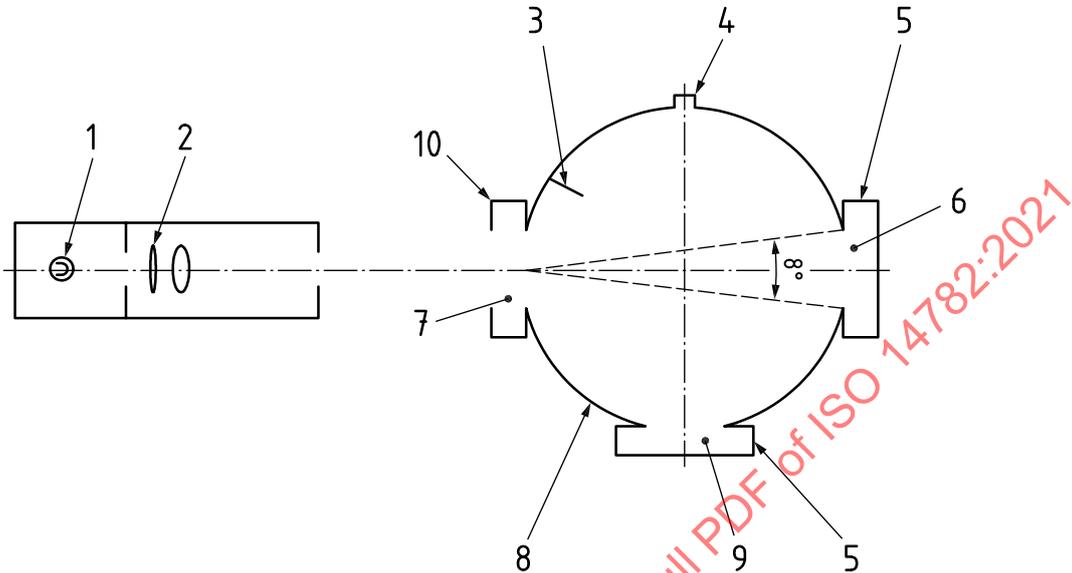

### Key

- |   |               |    |                    |
|---|---------------|----|--------------------|
| 1 | lamp          | 6  | exit port          |
| 2 | lens          | 7  | entrance port      |
| 3 | baffle        | 8  | integrating sphere |
| 4 | photodetector | 9  | compensation port  |
| 5 | light trap    | 10 | specimen holder    |

**Figure 1 — Schematic arrangement of the apparatus**

5.2 The light source and the photometer shall be used in conjunction with a filter to provide an output corresponding to the photopic standard luminous efficiency  $V(\bar{\epsilon})$  (as defined in ISO/CIE 11664-1), which is identical to the colour-matching function  $\bar{y}(\bar{\epsilon})$  specified in ISO/CIE 11664-1 under CIE standard illuminant  $D_{65}$  as specified in ISO 11664-2. The output of the photodetector shall be proportional to the incident flux, to within 1 % of the incident flux, over the range used.

The spectral and photometric characteristics of the light source and photometer shall be kept constant during measurements.

5.3 The light source and its associated optical system shall produce a parallel light beam, no ray of which makes an angle of more than 0,05 rad ( $3^\circ$ ) with the beam axis. This beam shall not be vignetted at either port of the integrating sphere.

5.4 The design of the instrument shall be such that the reading is zero in the absence of the light beam.

5.5 The integrating sphere used to collect the transmitted light may be of any diameter (but preferably no less than 150 mm in order to be able to accommodate large specimens), as long as the total port area does not exceed 3,0 % of the internal reflecting area of the sphere.

**5.6** The integrating sphere shall have an entrance port, an exit port, a compensation port and a photodetector port (see [Figure 1](#)). The entrance and exit ports shall be centred on the same great circle of the sphere, and there shall be an angle of  $(3,14 \pm 0,03)$  rad  $[(180 \pm 2)^\circ]$  between the centres of the ports. The exit port shall subtend an angle of  $(0,140 \pm 0,002)$  rad  $[(8 \pm 0,1)^\circ]$  at the centre of the entrance port. The exit and compensation ports shall have the same size. The entrance and compensation ports and the photodetector shall not lie on the same great circle of the sphere. The compensation port shall be positioned at an angle of less than 1,57 rad ( $90^\circ$ ) from the entrance port.

NOTE The compensation port is used to compensate for changes in the efficiency of the integrating sphere, which depends on the area of the inner surface, the number of ports and the way they are covered.

**5.7** When the beam is unobstructed by a specimen, its cross-section at the exit port shall be approximately circular, sharply defined and concentric with the exit port, leaving round it an annulus which subtends an angle of  $(0,023 \pm 0,002)$  rad  $[(1,3 \pm 0,1)^\circ]$  at the centre of the entrance port.

It is important to verify whether the unobstructed-beam diameter and centering at the exit port are maintained, especially if the source aperture and focus are changed.

NOTE The tolerance of  $\pm 0,002$  rad ( $\pm 0,1^\circ$ ) stated for the angle subtended by the annulus corresponds to an uncertainty of  $\pm 0,6$  % in a haze reading. This is relevant to the assessment of the precision of this test method.

**5.8** The position of the photodetector on the integrating sphere shall be at an angle of  $(1,57 \pm 0,26)$  rad  $[(90 \pm 15)^\circ]$  to the entrance port. The photodetector shall be fitted with baffles to prevent light from the specimen falling directly on it.

Light traps shall be provided for the exit and compensation ports to absorb the beam completely when no specimen is present, or the instrument design shall obviate the need for light traps for the exit and compensation ports.

**5.9** The tristimulus value  $Y_{10}$ , measured in accordance with CIE Publication No.15, of the surfaces of the interior of the integrating sphere, the baffles and the white reference (a working reference normally provided by the instrument manufacturer) shall be 90 % or more and shall not vary by more than  $\pm 3$  %. When direct measurement of the reflectance of the inner surface of the integrating sphere is difficult, the measurement may be made on a surface prepared from the same material in the same condition as the inner surface.

**5.10** The specimen holder shall be designed to hold the specimen rigidly in a plane perpendicular, to within  $\pm 2^\circ$ , to the light beam and as close as possible to the integrating sphere in order to ensure that all the light passing through the specimen, including scattered light, is collected. The holder shall also be designed so that flexible specimens such as film are kept flat.

It is recommended that thin, flexible film be held round the edge in a double-ring clamp or stuck to the holder by means of double-sided adhesive tape. Double-sided adhesive tape can also be used for thicker specimens which will not fit in the double-ring clamp. The use of a vacuum pump and a vacuum plate to mount the specimen on the holder is also recommended.

## 6 Specimens

**6.1** Cut specimens from films, sheets or injection- or compression-moulded articles.

**6.2** Specimens shall be free of dust, grease, adhesive from protective materials, scratches, blemishes and other defects, including visibly discernible internal voids and foreign bodies.

**6.3** Specimens shall be sufficiently large to cover either the entrance port or, if required, the compensation port of the integrating sphere. A disc of 50 mm diameter or a square with a side of the same length is suggested.

6.4 Unless otherwise specified, prepare three specimens of each sample of a given material.

## 7 Conditioning

7.1 When conditioning is required, condition the specimens in accordance with ISO 291 at  $(23 \pm 2)$  °C and  $(50 \pm 10)$  % relative humidity for no less than 40 h prior to the test.

7.2 When conditioning is required, place the test apparatus in an atmosphere maintained at  $(23 \pm 2)$  °C and  $(50 \pm 10)$  % relative humidity.

## 8 Procedure

8.1 Allow the apparatus sufficient time to reach thermal equilibrium before the measurements are made.

8.2 Mount a specimen in the specimen holder.

8.3 Make the four measurements given in [Table 1](#).

8.4 Measure the thickness of the specimen in three places to an accuracy of 0,02 mm for sheets and 1 µm for films.

8.5 Carry out the procedure on each of the three specimens in turn.

**Table 1 — Measurements**

	Entrance port	Exit port	Compensation port
$\tau_1$		White reference	Light trap <sup>a</sup>
$\tau_2$	Specimen	White reference	Light trap
$\tau_3$		Light trap	White reference
$\tau_4$	Specimen	Light trap	White reference
<sup>a</sup> See note to <a href="#">Clause 9</a> .			

## 9 Expression of results

Calculate the haze, in percent, using [Formula \(1\)](#):

$$H = [(\tau_4/\tau_2) - (\tau_3/\tau_1)] \quad (1)$$

where

$H$  is the haze;

$\tau_1$  is the intensity of the incident light;

$\tau_2$  is the intensity of all the light transmitted by the specimen;

$\tau_3$  is the intensity of the light scattered by the instrument;

$\tau_4$  is the intensity of the light scattered by the instrument and the specimen.

NOTE Haze can also be calculated as the ratio of the diffuse transmittance  $\tau_d$  to the total luminous transmittance  $\tau_t$ .

To obtain an accurate value of the total luminous transmittance, however, it is necessary, when using a single-beam instrument as in this document, to place a specimen over the compensation port when measuring  $\tau_1$  (as specified in ISO 13468-1), in order to compensate for the change in efficiency. Alternatively, an accurate value of the luminous transmittance can be obtained by using a calibrated reference standard to correct the value measured. However, in practice it is sufficient to use the value of  $\tau_1$  obtained by placing a light trap over the compensation port instead of a specimen since this makes little difference to the haze value obtained.

An accurate value of the diffuse transmittance  $\tau_d$  can be obtained from the equation  $\tau_d = [\tau_4 - \tau_3(\tau_2/\tau_1)]/\tau_1$ , using the accurate value of  $\tau_1$  obtained above.

## 10 Precision

An interlaboratory trial was conducted to determine the precision of the method. The haze of eight samples was measured by seven laboratories. The data were analysed in 1994 according to ISO 5725-1, ISO 5725-2 and ISO 5725-3.

The test results are given in [Table 2](#).

One outlier was detected using Grubb's test and was excluded.

**Table 2 — Interlaboratory trial data**

Values in percent

Test sample	Haze	Within-laboratory reproducibility <sup>a</sup> standard deviation $s_{R_w}$	Reproducibility <sup>b</sup> standard deviation $s_R$	Outlier
PMMA	0,30	0,028	0,051	0
PMMA-HI (1)	0,40	0,027	0,078	0
PMMA-HI (2)	0,95	0,032	0,050	0
ABS, transparent (1)	2,88	0,17	0,30	0
ABS, transparent (2)	11,7	0,68	1,25	0
PMMA, matted	31,0	0,19	1,50	0
PE	38,2	0,68	1,14	1
PET/PE	41,8	1,52	2,02	0

<sup>a</sup> The within-laboratory reproducibility is the precision when the test results are obtained with the same method on identical material in the same laboratory, but the operator, the equipment and/or the time of measurement are different.

<sup>b</sup> The reproducibility is the precision when the test results are obtained with the same method on identical test material in different laboratories with different operators using different equipment and expressed as a reproducibility standard deviation.