

First edition  
1999-05-15

Corrected version  
2003-07-15

---

---

**Determination of the ultimate aerobic  
biodegradability of plastic materials in an  
aqueous medium — Method by measuring  
the oxygen demand in a closed  
respirometer**

*Évaluation de la biodégradabilité aérobie ultime des matériaux plastiques  
en milieu aqueux — Méthode par détermination de la demande en oxygène  
dans un respiromètre fermé*



Reference number  
ISO 14851:1999(E)

**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 14851:1999

© ISO 1999

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 14851 was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*.

Annexes A to G of this International Standard are for information only.

This corrected version of ISO 14851:1999 incorporates the following corrections:

- in Clause 2, the year of publication of ISO 9408 has been inserted and the footnote deleted;
- the remaining footnotes have been renumbered;
- in Annex C, errors in the key to Figure C.1 have been corrected and minor improvements made to the figure itself;
- in the Bibliography, references [1] and [2] have been updated.

STANDARDSISO.COM : Click to view the full PDF of ISO 14851:1999

## Introduction

With the increasing use of plastics, their recovery and disposal have become a major issue. As a first priority, recovery should be promoted. Complete recovery of plastics, however, is difficult. For example, plastic litter, which comes mainly from consumers, is difficult to recover completely. Additional examples of plastics which are difficult to recover are fishing tackle, agricultural mulches and water-soluble polymers. These plastic materials tend to leak from closed waste-management cycles into the environment. Biodegradable plastics are now emerging as one of the options available to solve such environmental problems. Plastic materials, such as products or packaging, which are sent to composting facilities should be potentially biodegradable. Therefore it is very important to determine the potential biodegradability of such materials and to obtain an indication of their biodegradability in natural environments.

STANDARDSISO.COM : Click to view the full PDF of ISO 14851:1999

# Determination of the ultimate aerobic biodegradability of plastic materials in an aqueous medium — Method by measuring the oxygen demand in a closed respirometer

**WARNING** — Sewage, activated sludge, soil and compost may contain potentially pathogenic organisms. Therefore appropriate precautions should be taken when handling them. Toxic test compounds and those whose properties are unknown should be handled with care.

## 1 Scope

This International Standard specifies a method, by measuring the oxygen demand in a closed respirometer, for the determination of the degree of aerobic biodegradability of plastic materials, including those containing formulation additives. The test material is exposed in an aqueous medium under laboratory conditions to an inoculum from activated sludge, compost or soil.

If an unadapted activated sludge is used as the inoculum, the test simulates the biodegradation processes which occur in a natural aqueous environment; if a mixed or pre-exposed inoculum is used, the method can be used to investigate the potential biodegradability of a test material.

The conditions used in this International Standard do not necessarily correspond to the optimum conditions allowing maximum biodegradation to occur, but the standard is designed to determine the potential biodegradability of plastic materials or give an indication of their biodegradability in natural environments.

The method enables the assessment of the biodegradability to be improved by calculating a carbon balance (optional, see annex E).

The method applies to the following materials:

- Natural and/or synthetic polymers, copolymers or mixtures thereof.
- Plastic materials which contain additives such as plasticizers, colorants or other compounds.
- Water-soluble polymers.
- Materials which, under the test conditions, do not inhibit the microorganisms present in the inoculum. Inhibitory effects can be determined using an inhibition control or by another appropriate method (see e.g. ISO 8192<sup>[3]</sup>). If the test material is inhibitory to the inoculum, a lower test concentration, another inoculum or a pre-exposed inoculum can be used.

## 2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 8245:1999, *Water quality — Guidelines for the determination of total organic carbon (TOC) and dissolved organic carbon (DOC)*.

ISO 9408:1999, *Water quality — Evaluation of ultimate aerobic biodegradability of organic compounds in aqueous medium by determination of oxygen demand in a closed respirometer*.

ISO 10634:1995, *Water quality — Guidance for the preparation and treatment of poorly water-soluble organic compounds for the subsequent evaluation of their biodegradability in an aqueous medium*.

ISO/TR 15462:1997, *Water quality — Selection of tests for biodegradability*.

### 3 Definitions

For the purposes of this International Standard, the following definitions apply:

#### 3.1

##### **ultimate aerobic biodegradation**

the breakdown of an organic compound by microorganisms in the presence of oxygen into carbon dioxide, water and mineral salts of any other elements present (mineralization) plus new biomass

#### 3.2

##### **activated sludge**

biomass produced in the aerobic treatment of waste water by the growth of bacteria and other microorganisms in the presence of dissolved oxygen

#### 3.3

##### **concentration of suspended solids in an activated sludge**

the amount of solids obtained by filtration or centrifugation of a known volume of activated sludge and drying at about 105 °C to constant mass

#### 3.4

##### **biochemical oxygen demand**

##### **BOD**

the mass concentration of the dissolved oxygen consumed under specified conditions by the aerobic biological oxidation of a chemical compound or organic matter in water, expressed as milligrams of oxygen uptake per milligram or gram of test compound

#### 3.5

##### **theoretical oxygen demand**

##### **ThOD**

the theoretical maximum amount of oxygen required to oxidize a chemical compound completely, calculated from the molecular formula, expressed as milligrams of oxygen uptake per milligram or gram of test compound

#### 3.6

##### **total organic carbon**

##### **TOC**

all the carbon present in organic matter which is dissolved or suspended in water

#### 3.7

##### **dissolved organic carbon**

##### **DOC**

that part of the organic carbon in water which cannot be removed by specified phase separation, for example by centrifugation at 40 000 m·s<sup>-2</sup> for 15 min or by membrane filtration using membranes with pores of 0,2 µm to 0,45 µm diameter

### 3.8

#### **lag phase**

the time, measured in days, from the start of a test until adaptation and/or selection of the degrading microorganisms is achieved and the degree of biodegradation of a chemical compound or organic matter has increased to about 10 % of the maximum level of biodegradation

### 3.9

#### **maximum level of biodegradation**

the degree of biodegradation, measured in per cent, of a chemical compound or organic matter in a test, above which no further biodegradation takes place during the test

### 3.10

#### **biodegradation phase**

the time, measured in days, from the end of the lag phase of a test until about 90 % of the maximum level of biodegradation has been reached

### 3.11

#### **plateau phase**

the time, measured in days, from the end of the biodegradation phase until the end of a test

### 3.12

#### **pre-exposure**

the pre-incubation of an inoculum in the presence of the chemical compound or organic matter under test, with the aim of enhancing the ability of the inoculum to biodegrade the test material by adaptation and/or selection of the microorganisms

### 3.13

#### **pre-conditioning**

the pre-incubation of an inoculum under the conditions of the subsequent test in the absence of the chemical compound or organic matter under test, with the aim of improving the test by acclimatization of the microorganisms to the test conditions

## 4 Principle

The biodegradability of a plastic material is determined using aerobic microorganisms in an aqueous system. The test mixture contains an inorganic medium, the organic test material (the sole source of carbon and energy) with a concentration between 100 mg/l and 2 000 mg/l of organic carbon, and activated sludge or a suspension of active soil or compost as the inoculum. The mixture is stirred in closed flasks in a respirometer for a period not exceeding 6 months. The carbon dioxide evolved is absorbed in a suitable absorber in the headspace of the flasks. The consumption of oxygen (BOD) is determined, for example by measuring the amount of oxygen required to maintain a constant volume of gas in the respirometer flasks, or by measuring the change in volume or pressure (or a combination of the two) either automatically or manually. An example of a respirometer is given in annex C. Alternatively, the two-phase closed-bottle version described in ISO 10708<sup>[4]</sup> may be used (see annex D).

The level of biodegradation is determined by comparing the BOD with the theoretical amount (ThOD) and expressed in per cent. The influence of possible nitrification processes on the BOD have to be considered. The test result is the maximum level of biodegradation determined from the plateau phase of the biodegradation curve. Optionally, a carbon balance may be calculated to give additional information on the biodegradation (see annex E).

Unlike ISO 9408, which is used for a variety of organic compounds, this International Standard is specially designed for the determination of the biodegradability of plastic materials. The special requirements necessary affect the choice of the inoculum and the test medium, and there is the possibility of improving the evaluation of the biodegradability by calculating a carbon balance.

## 5 Test environment

Incubation shall take place in the dark or in diffuse light in an enclosure which is free from vapours inhibitory to microorganisms and which is maintained at a constant temperature, preferably between 20 °C and 25 °C, to an accuracy of  $\pm 1$  °C, or at any other appropriate temperature depending on the inoculum used and the environment to be assessed.

NOTE With a compost inoculum, higher temperatures may be appropriate.

## 6 Reagents

Use only reagents of recognized analytical grade.

**6.1 Distilled or deionized water**, free of toxic substances (copper in particular) and containing less than 2 mg/l of DOC.

### 6.2 Test medium.

Depending on the purpose of the test, different test media may be used. For example, if simulating a natural environment use the standard test medium (6.2.1). If a test material is used at higher concentrations, use the optimized test medium (6.2.2) with higher buffering capacity and nutrient concentrations.

#### 6.2.1 Standard test medium

##### 6.2.1.1 Solution A

Dissolve

anhydrous potassium dihydrogen phosphate ( $\text{KH}_2\text{PO}_4$ )	8,5 g
anhydrous dipotassium hydrogen phosphate ( $\text{K}_2\text{HPO}_4$ )	21,75 g
disodium hydrogen phosphate dihydrate ( $\text{Na}_2\text{HPO}_4 \cdot 2\text{H}_2\text{O}$ )	33,4 g
ammonium chloride ( $\text{NH}_4\text{Cl}$ )	0,5 g

in water (6.1) and make up to 1 000 ml.

NOTE The correct composition of the solution can be checked by measuring the pH, which should be 7,4.

##### 6.2.1.2 Solution B

Dissolve 22,5 g of magnesium sulfate heptahydrate ( $\text{MgSO}_4 \cdot 7\text{H}_2\text{O}$ ) in water (6.1) and make up to 1 000 ml.

##### 6.2.1.3 Solution C

Dissolve 36,4 g of calcium chloride dihydrate ( $\text{CaCl}_2 \cdot 2\text{H}_2\text{O}$ ) in water (6.1) and make up to 1 000 ml.

##### 6.2.1.4 Solution D

Dissolve 0,25 g of iron(III) chloride hexahydrate ( $\text{FeCl}_3 \cdot 6\text{H}_2\text{O}$ ) in water (6.1) and make up to 1 000 ml.

Prepare this solution freshly before use to avoid precipitation, or add a drop of concentrated hydrochloric acid (HCl) or a drop of 0,4 g/l aqueous solution of ethylenediaminetetraacetic acid (EDTA).

##### 6.2.1.5 Preparation

To prepare 1 litre of test medium, add, to about 500 ml of water (6.1),

- 10 ml of solution A;
- 1 ml of each of solutions B to D.

Make up to 1 000 ml with water (6.1).

### 6.2.2 Optimized test medium

This optimized medium is highly buffered and contains more inorganic nutrients. This is necessary to keep the pH constant in the system during the test, even at high concentrations of the test material. The medium contains about 2400 mg/l of phosphorus and 50 mg/l of nitrogen and is therefore suitable for concentrations in the test material of up to 2000 mg/l of organic carbon. If higher test-material concentrations are used, increase the nitrogen content to keep the C:N ratio at about 40:1.

#### 6.2.2.1 Solution A

Dissolve

anhydrous potassium dihydrogen phosphate ( $\text{KH}_2\text{PO}_4$ )	37,5 g
disodium hydrogen phosphate dihydrate ( $\text{Na}_2\text{HPO}_4 \cdot 2\text{H}_2\text{O}$ )	87,3 g
ammonium chloride ( $\text{NH}_4\text{Cl}$ )	2,0 g

in water (6.1) and make up to 1 000 ml.

#### 6.2.2.2 Solution B

Dissolve 22,5 g of magnesium sulfate heptahydrate ( $\text{MgSO}_4 \cdot 7\text{H}_2\text{O}$ ) in water (6.1) and make up to 1 000 ml.

#### 6.2.2.3 Solution C

Dissolve 36,4 g of calcium chloride dihydrate ( $\text{CaCl}_2 \cdot 2\text{H}_2\text{O}$ ) in water (6.1) and make up to 1 000 ml.

#### 6.2.2.4 Solution D

Dissolve 0,25 g of iron(III) chloride hexahydrate ( $\text{FeCl}_3 \cdot 6\text{H}_2\text{O}$ ) in water (6.1) and make up to 1 000 ml (see second paragraph of 6.2.1.4).

#### 6.2.2.5 Solution E (trace-element solution, optional)

Dissolve in 10 ml of aqueous HCl solution (25 %, 7,7 mol/l), in the following sequence:

70 mg of  $\text{ZnCl}_2$ , 100 mg of  $\text{MnCl}_2 \cdot 4\text{H}_2\text{O}$ , 6 mg of  $\text{H}_3\text{BO}_3$ , 190 mg of  $\text{CoCl}_2 \cdot 6\text{H}_2\text{O}$ , 3 mg of  $\text{CuCl}_2 \cdot 2\text{H}_2\text{O}$ , 240 mg of  $\text{NiCl}_2 \cdot 6\text{H}_2\text{O}$ , 36 mg of  $\text{Na}_2\text{MoO}_4 \cdot 2\text{H}_2\text{O}$ , 33 mg of  $\text{Na}_2\text{WO}_4 \cdot 2\text{H}_2\text{O}$  and 26 mg of  $\text{Na}_2\text{SeO}_3 \cdot 5\text{H}_2\text{O}$

and make up to 1 000 ml with water (6.1).

#### 6.2.2.6 Solution F (vitamin solution, optional)

Dissolve in 100 ml of water (6.1) 0,6 mg of biotine, 2,0 mg of niacinamide, 2,0 mg of *p*-aminobenzoate, 1,0 mg of pantothenic acid, 10,0 mg of pyridoxal hydrochloride, 5,0 mg of cyanocobalamine, 2,0 mg of folic acid, 5,0 mg of riboflavin, 5,0 mg of DL-thioctic acid and 1,0 mg of thiamine dichloride or use a solution of 15 mg of yeast extract in 100 ml of water (6.1). Filter the solution for sterilization using membrane filters (see 7.4).

NOTE Solutions E and F are optional and are not required if a sufficient concentration of the inoculum is used, e.g. activated sludge, soil or compost. It is recommended that 1 ml portions be prepared and kept refrigerated until use.

### 6.2.2.7 Preparation

To prepare 1 litre of test medium, add, to about 800 ml of water (6.1),

- 100 ml of solution A;
- 1 ml of each of solutions B to D and, optionally, E and F.

Make up to 1 000 ml with water (6.1) and measure the pH.

NOTE The correct composition of the test medium can be checked by measuring the pH, which should be  $7,0 \pm 0,2$ .

### 6.3 Pyrophosphate solution.

Dissolve 2,66 g of anhydrous sodium pyrophosphate ( $\text{Na}_4\text{P}_2\text{O}_7$ ) in water (6.1) and make up to 1 000 ml.

**6.4 Carbon dioxide absorber**, preferably soda lime pellets or another suitable absorbant.

## 7 Apparatus

Ensure that all glassware is thoroughly cleaned and, in particular, free from organic or toxic matter.

Required is usual laboratory equipment, plus the following:

**7.1 Closed respirometer**, including test vessels (glass flasks) fitted with stirrers and all other necessary equipment, and located in a constant-temperature room or in a thermostatted apparatus (e.g. water-bath). For an example, see annex C.

NOTE Any respirometer able to determine with sufficient accuracy the biochemical oxygen demand is suitable, preferably an apparatus which measures and replaces automatically and continuously the oxygen consumed so that no oxygen deficiency and no inhibition of the microbial activity occurs during the degradation process. Instead of an ordinary respirometer, the two-phase closed-bottle version may be used (see annex D).

**7.2 Analytical equipment for measuring total organic carbon (TOC) and dissolved organic carbon (DOC)** (see ISO 8245).

**7.3 Analytical equipment for measuring nitrate and nitrite concentrations.**

NOTE A qualitative test is recommended first to decide if any nitrification has occurred. If there is evidence of nitrate/nitrite in the medium, a quantitative determination using a suitable method (for example ion chromatography) is required.

**7.4 Centrifuge, or filtration device** with membrane filters (0,45  $\mu\text{m}$  pore size) which neither adsorb nor release organic carbon significantly.

**7.5 Analytical balance** (usual laboratory equipment).

**7.6 pH meter** (usual laboratory equipment).

## 8 Procedure

### 8.1 Test material

The test material shall be of known mass and contain sufficient carbon to yield a BOD that can be adequately measured by the respirometer used. Calculate from the chemical formula or determine by elemental analysis the ThOD (see annex A) and the TOC (using e.g. ISO 8245). Use a test-material concentration of at least 100 mg/l, corresponding to a ThOD of about 170 mg/l or a TOC of about 60 mg/l. Use lower concentrations only if the sensitivity of the respirometer is adequate. The maximum amount of test material is limited by the oxygen supply to the respirometer and the test medium used. When using the optimized test medium (6.2.2), the test-material

concentration shall be such that the TOC does not exceed about 2000 mg/l, i.e. a C:N ratio of about 40:1. If higher concentrations are to be tested, increase the amount of nitrogen in the test medium.

NOTE 1 If biodegradation processes in natural environments are to be simulated, the use of the standard medium and a test-material concentration of 100 mg/l are recommended.

NOTE 2 The test material should preferably be used in powder form, but it may also be introduced as films, pieces, fragments or shaped articles. The form and shape of the test material may influence its biodegradability. Similar shapes should preferably be used if different kinds of plastic material are to be compared. If the test material is used in the form of a powder, particles of known, narrow size distribution should be used. A particle-size distribution with the maximum at 250 µm diameter is recommended. Also, the size of the test equipment used may depend on the form of the test material. It should be ascertained that no substantial mechanical aberrations occur due to the test conditions, for example due to the type of stirring mechanism used. Processing of the test material (e.g. the use of powder in the case of composites) should not influence significantly the degradation behaviour of the material. Optionally, record the hydrogen, oxygen, nitrogen, phosphorus and sulfur contents and the molecular mass of a polymeric test material, using for example liquid exclusion chromatography (see e.g. ASTM D 3536-91<sup>[1]</sup> or any other applicable standard method). Preferably, plastic materials without additives such as plasticizers should be tested. When the material does contain such additives, information on their biodegradability will be needed to assess the biodegradability of the polymeric material itself.

For details on how to handle poorly water-soluble compounds, see ISO 10634.

## 8.2 Reference material

Use aniline and/or a well defined biodegradable polymer (for example microcrystalline cellulose powder, ashless cellulose filters or poly-β-hydroxybutyrate) as a reference material. If possible, the TOC, form and size should be comparable to that of the test material.

As a negative control, a non-biodegradable polymer (e.g. polyethylene) in the same form as the test material can optionally be used.

## 8.3 Preparation of the inoculum

Activated sludge from a sewage-treatment plant treating predominantly domestic sewage is a suitable source of the inoculum. It is obtained from an active aerobic environment and is available over a wide geographical area in which a broad range of plastic materials has to be tested. Alternatively, soil and/or compost suspensions can be used for inoculation, as with some plastic materials the activity of fungi is important for biodegradation. When biodegradation in a specific waste-treatment system is to be determined, collect the inoculum from that environment.

The inoculum can be prepared from the sources described in 8.3.1 and 8.3.2, or from a mixture of these sources in order to obtain a varied and concentrated microbial flora with sufficient biodegradation activity. If the endogenous respiration of the inoculum is too high, stabilize the inoculum by aeration before use. Harmonize the test temperature with the inoculum used (see note to clause 5).

NOTE It may be useful to determine the colony-forming units (cfu) of the inoculum used. The test mixture should preferably contain about  $10^{-6}$  cfu/ml.

### 8.3.1 Inoculum from wastewater-treatment plants

Take a sample of activated sludge collected from a well-operated sewage-treatment plant or a laboratory plant handling predominantly domestic sewage. Mix well, keep the sample under aerobic conditions and use preferably on the day of collection (at least within 72 h).

Before use, determine the concentration of suspended solids (use e.g. ISO 11923<sup>[5]</sup>). If necessary, concentrate the sludge by settling so that the volume of sludge added to the test assay is minimal. Add a suitable volume to obtain suspended solids in the range 30 mg/l to 1000 mg/l in the final mixture.

NOTE 1 When biodegradation processes in a natural environment are to be simulated or when a carbon balance determination (see annex E) is to be carried out, an inoculum concentration of 30 mg/l suspended solids is recommended. As solid matter can interfere with the carbon balance determination, the following procedure for preparing the inoculum is recommended. Take 500 ml of the activated sludge and homogenize for 2 min at medium speed in a blender or in a suitable high-speed mixer. Allow to settle until the supernatant liquid contains no significant amounts of suspended matter, but in any case for at least 30 min. Decant a sufficient volume of the supernatant liquid and add it to the test flasks to obtain a concentration of 1 % (V/V) to 5 % (V/V) in the test medium. Avoid carrying over sludge particles.

NOTE 2 An inoculum may be pre-conditioned, but normally no pre-exposed inoculum should be used, especially in the case of standard tests simulating biodegradation behaviour in natural environments. Depending on the purpose of the test, a pre-exposed inoculum may also be used, provided this is clearly stated in the test report (e.g. per cent biodegradation =  $x$  %, using pre-exposed inocula) and the method of pre-exposure detailed in the test report. Pre-exposed inocula can be obtained from suitable laboratory biodegradation tests (see ISO/TR 15462) conducted under a variety of conditions or from samples collected from locations where relevant environmental conditions exist (e.g. contaminated areas or industrial treatment plants).

### 8.3.2 Inoculum from soil and/or compost

Suspend 10 g of non-sterile, fertile soil or compost from a composting plant treating predominantly organic waste in 100 ml of the test medium (6.2.1 or 6.2.2) or in a pyrophosphate solution (6.3) which is commonly used in soil microbiology. Allow to settle for about 30 min. Decant and filter the supernatant liquid through a coarse porous filter and add the inoculum to the test flasks to obtain a concentration of 1 % (V/V) to 5 % (V/V) in the test medium. Higher amounts of inoculum can be used if necessary, but this may cause problems in establishing carbon balances. The use of compost can increase the number of fungi in the test flasks and improve the biodegradation of plastic materials. In this case, indicate the state of the compost used in the test report (e.g. mature compost, compost from the hot phase at about 50 °C).

When a higher inoculum concentration is needed, suspend a higher amount of soil or compost in the test medium and dilute to an appropriate concentration for inoculation.

### 8.4 Test

Provide a number of flasks, so that the test includes at least the following:

- a) Two test flasks for the test material (symbol  $F_T$ ).
- b) Two flasks for the blank (symbol  $F_B$ ).
- c) One flask for checking the inoculum activity using a reference material (symbol  $F_C$ ).

And, if required:

- d) One flask for checking for possible abiotic degradation or non-biological change in the test material such as by hydrolysis (symbol  $F_S$ ). The test solution in  $F_S$  shall be sterilized, for example by autoclaving or by the addition of a suitable inorganic toxic compound to prevent microbial activity. Use, for example, 5 ml/l of a solution containing 10 g/l of mercury(II) chloride ( $HgCl_2$ ). Add the same amount of the toxic substance during the test if required.
- e) One flask as a negative control (symbol  $F_N$ ) using a non-biodegradable polymeric substance (e.g. polyethylene) in the same form as the test material.
- f) One flask for checking the possible inhibiting effect of the test material on microbial activity (symbol  $F_I$ ). Take care that the ratio of carbon in the test and reference material to nitrogen in the medium is at least about C:N = 40:1. Add nitrogen if required.

Add appropriate amounts of the test medium (6.2) and the inoculum (see 8.3) to the test flasks as indicated in table 1.

Measure the pH in the flasks and adjust to 7 if necessary. Add carbon dioxide absorber (6.4) to the absorber compartments of the respirometer (see annex C). Add the test material (see 8.1), the reference material and the material for the negative control (see 8.2) to the respective flasks as indicated in table 1. If a carbon balance is to be run (see annex E), remove a known sufficient volume of the inoculated test medium from each flask or from additional separate flasks for DOC and biomass determination at the beginning and the end of the incubation period. Consider the removed volume when adjusting the final volume or when calculating the test results.

Place the flasks in a constant-temperature environment (see clause 5) and allow all vessels to reach the desired temperature. Make any necessary connections, seal the flasks, place them in the respirometer and start the stirrer. Take the necessary readings on the manometers (if manual) and verify that the recorder of oxygen consumption is

functioning properly (automatic respirometer). As an alternative, the two-phase closed-bottle version described in annex D may be used.

**Table 1 — Final distribution of test and reference materials**

Flask	Test material	Reference material	Inoculum
F <sub>T</sub> Test	+	–	+
F <sub>T</sub> Test	+	–	+
F <sub>B</sub> Blank	–	–	+
F <sub>B</sub> Blank	–	–	+
F <sub>C</sub> Inoculum check	–	+	+
F <sub>S</sub> Abiotic degradation check (optional)	+	–	–
F <sub>I</sub> Inhibition control (optional)	+	+	+
F <sub>N</sub> Negative control (optional)	–	+	+

When a constant level of BOD is attained (plateau phase reached) and no further biodegradation is expected, the test is considered to be completed. The maximum test period is 6 months. In the case of long test durations, special attention must be paid to the technical system (e.g. tightness of the test vessels and connections).

At the end of the test, measure the pH and determine the concentrations of nitrate and nitrite immediately in flasks F<sub>T</sub> (see note), or take suitably preserved samples. Use the values to correct the calculated degree of biodegradation for nitrification (see annex B).

NOTE Allylthiourea can only inhibit nitrification during short incubation periods, as it is biodegradable. Therefore addition of allylthiourea to prevent nitrification is not recommended. Experience shows, however, that with low inoculum concentrations [about 1 % (v/v)] nitrification will not occur, even during long incubation periods, when no inhibitor is used.

## 9 Calculation and expression of results

### 9.1 Calculation

Read the oxygen consumption values for each flask, using the method given by the manufacturer for the appropriate type of respirometer. Calculate the specific biochemical oxygen demand (BOD<sub>S</sub>) of the test material as the difference between oxygen consumption in the test flasks F<sub>T</sub> and the blanks F<sub>B</sub> divided by the concentration of the test material, using equation (1):

$$BOD_S = \frac{BOD_t - BOD_{Bt}}{\rho_{TC}} \quad \dots (1)$$

where

BOD<sub>S</sub> is the specific BOD, in milligrams per gram of test material;

BOD<sub>t</sub> is the BOD of the flasks F<sub>T</sub> containing test material at time *t*, in milligrams per litre;

BOD<sub>Bt</sub> is the BOD of the blank F<sub>B</sub> at time *t*, in milligrams per litre;

ρ<sub>TC</sub> is the concentration of the test material in the reaction mixture of flask F<sub>T</sub>, in milligrams per litre.

Calculate the percentage biodegradation  $D_t$  as the ratio of the specific biochemical oxygen demand to the theoretical oxygen demand (ThOD, in milligrams per gram of test material), using equation (2):

$$D_t = \frac{\text{BOD}_S}{\text{ThOD}} \times 100 \quad \dots (2)$$

Calculate in the same way the BOD and percentage biodegradation of the reference material  $F_C$  and, if included, the abiotic degradation check  $F_S$ , the inhibition control  $F_I$  and the negative control  $F_N$ .

NOTE For calculation of the ThOD, see annex A. If significant concentrations of nitrite and nitrate are determined, consider the oxygen demand due to nitrification (see annex B). If a carbon balance is to be calculated, use information given in annex E.

## 9.2 Expression and interpretation of results

Compile a table of the BOD values measured and the percentages of biodegradation for each measurement interval and each test flask. For each vessel, plot a BOD curve and a biodegradation curve in per cent as a function of time. If comparable results are obtained for the duplicate flasks, a mean curve may be plotted.

The maximum level of biodegradation determined as the mean value of the plateau phase of the biodegradation curve or the highest value, e.g. when the curve decreases or, further on, slowly increases in the plateau phase, characterizes the degree of biodegradation of the test material. If a carbon balance has been determined, the result of this determination characterizes the total degree of biodegradation.

The wettability and the shape of the test material may influence the result obtained, and hence the test procedure may be limited to comparing plastic materials of similar chemical structure.

Information on the toxicity of the test material may be useful in the interpretation of test results showing a low biodegradability.

## 10 Validity of results

The test is considered valid if

- the degree of biodegradation of the reference material (inoculum check  $F_C$ ) is > 60 % at the end of the test;
- the BOD of the blank  $F_B$  at the end of the test does not exceed an upper limiting value obtained by experience (this value depends on the amount of inoculum and is, for example, in the case of 30 mg/l dry matter, about 60 mg/l as interlaboratory tests have shown).

If in flask  $F_I$  (inhibition check, if included) the percentage biodegradation is < 25 % and no significant degradation of the test material is observed, it can be assumed that the test material is inhibitory.

If in flask  $F_S$  (abiotic degradation check, if included) a significant amount (> 10 %) of BOD is observed, abiotic degradation processes may have taken place.

If flask  $F_N$  (negative control) was included, no significant amount of BOD shall be observed.

If these criteria are not fulfilled, repeat the test using another pre-conditioned or pre-exposed inoculum.

## 11 Test report

The test report shall contain at least the following information:

- a reference to this International Standard;
- all information necessary to identify the test and reference materials, including their TOC, ThOD, chemical composition and formula (if known), shape, form and amount/concentration in the samples tested;

- c) the main test parameters, including test volume, test medium used, incubation temperature and final pH;
- d) the source and amount of the inoculum used, including details of any pre-exposure and the state of the compost used;
- e) the analytical techniques used, including the principle of the respirometer and the TOC and nitrate/nitrite determinations;
- f) all the test results obtained for the test and reference materials (in tabular and graphical form), including the measured BOD, the percentage biodegradation values, the respective curves of these parameters against time and the nitrate/nitrite concentrations;
- g) the duration of the lag phase, biodegradation phase and maximum level of degradation, as well as the total test duration;

and, optionally, if run or determined:

- h) the results of the abiotic degradation check  $F_S$ , the inhibition control  $F_I$  and the negative control  $F_N$ ;
- i) the results of the carbon balance determination, including for example:
  - 1) the amount of carbon in the test material oxidized to carbon dioxide, estimated from the degree of biodegradation based on the BOD,
  - 2) the increase in DOC in the test medium during the incubation period due to water-soluble substances,
  - 3) the increase in organic carbon in the biomass during the test,
  - 4) the carbon content of the residual polymers at the end of the test,
  - 5) the sum of all the carbon measured, expressed as a percentage of the carbon introduced as the test material;
- j) the colony-forming units (cfu/ml) in the inoculated test mixtures;
- k) any other relevant data (e.g. initial molecular mass of the sample, molecular mass of the residual polymer).

STANDARDSISO.COM : Click to view the full PDF of ISO 14851:1999

## Annex A (informative)

### Theoretical oxygen demand (ThOD)

#### A.1 Calculation of the ThOD

The theoretical oxygen demand (ThOD) of a substance  $C_cH_hCl_{cl}N_nS_sP_pNa_{na}O_o$  of relative molecular mass  $M_r$  can be calculated, if the elemental composition is known or can be determined by elemental analysis, using the equation

$$\text{ThOD} = \frac{16 [2c + 0,5(h - cl - 3n) + 3s + 2,5p + 0,5na - o]}{M_r}$$

This calculation assumes that carbon is converted to  $CO_2$ , hydrogen to  $H_2O$ , phosphorus to  $P_2O_5$ , sulfur to an oxidation state of +6 and halogens eliminated as hydrogen halides. The oxidation of N, P and S has to be checked by analysis. The calculation also assumes that nitrogen is released as ammonium. For the influence of nitrification, see annex B.

Express the ThOD in milligrams per gram of substance or in milligrams per milligram of substance.

#### A.2 Example: Poly( $\beta$ -hydroxybutyric acid) (PHB)

Summary formula<sup>1)</sup>:  $C_4H_6O_2$ ,  $c = 4$ ,  $h = 6$ ,  $o = 2$ ; relative molecular mass  $M_r = 86$ .

$$\text{ThOD} = \frac{16 [2 \times 4 + 0,5 \times 6 - 2]}{86}$$

$$\text{ThOD} = 1,6744 \text{ mg/mg PHB} = 1674,4 \text{ mg/g PHB}$$

#### A.3 Example: Blend of polyethylene/starch/glycerol

Component	Formula	ThOD mg/g	Amount of component		ThOD mg/flask
			%	mg/flask	
Polyethylene	$(C_2H_4)_n$	3400	50	500	1700
Starch	$(C_6H_{10}O_5)_n$	1190	40	400	476
Glycerol	$C_3H_8O_3$	1200	10	100	120
Total blend			100	1000	2296

<sup>1)</sup> PHB is a polymer consisting of the  $\beta$ -hydroxybutyrate monomer. For polymerization (ester formation), water is removed, so that the summary formula for PHB is equivalent to that of the monomer minus one  $H_2O$ , which is eliminated in the chemical reaction.

## Annex B (informative)

### Correction of BOD values for interference by nitrification

#### B.1 Influence of nitrification

BOD values can be influenced by nitrification. They have to be corrected if serious errors are to be avoided in the calculation of degrees of biodegradation based on the oxidation of the carbon in a nitrogen-containing test material. Errors in the case of nitrogen-free substances are normally negligible, because the oxidation of the ammonium in the medium is taken into account by the subtraction of the blank.

Ammonium salts and nitrogen-containing test compounds can be oxidized to nitrite or nitrate during the incubation period of a biodegradation test. Since the reactions are sequential (carried out by different bacterial species), it is possible for the nitrite concentration to increase or decrease. In the latter case, an equivalent concentration of nitrate is formed. The chemical reactions follow equations (B.1) to (B.3):



Overall:



From these equations, it can be concluded that

- for the oxidation of 2 moles (28 g) of ammonia nitrogen (added as  $\text{NH}_4\text{Cl}$  with the inorganic medium) to nitrite, 3 moles (96 g) of oxygen ( $\text{BOD}_{\text{NO}_2}$ ) are needed, resulting in a factor of 3,43 (96/28) mg of oxygen demand per mg of nitrogen;
- for the oxidation of 2 moles (28 g) of ammonia nitrogen to nitrate, 4 moles (128 g) of oxygen ( $\text{BOD}_{\text{NO}_3}$ ) are needed, resulting in a factor of 4,57 (128/28) mg of oxygen demand per mg of nitrogen.

The amount of nitrification can be determined by measuring the nitrate and nitrite concentrations at the end of the test in the medium in flasks  $F_T$ . A qualitative test is recommended first to decide if any nitrification has occurred. If there is evidence of nitrate or nitrite, a quantitative determination is required.

The part of the BOD deriving from nitrogen oxidation at the end of the test,  $\text{BOD}_N$ , is calculated, in milligrams per litre, using equation (B.4):

$$\text{BOD}_N = (\rho_{\text{NO}_3} \times 4,57) + (\rho_{\text{NO}_2} \times 3,43) \quad \dots \text{(B.4)}$$

where

- $\rho_{\text{NO}_3}$  is the measured concentration of nitrate nitrogen in flasks  $F_T$  at the end of the test, in milligrams per litre;
- $\rho_{\text{NO}_2}$  is the measured concentration of nitrite nitrogen in flasks  $F_T$  at the end of the test, in milligrams per litre;
- 4,57 is the factor for the oxygen demand for the formation of nitrate;
- 3,43 is the factor for the oxygen demand for the formation of nitrite.

The part of the BOD deriving from carbon oxidation at the end of the test,  $BOD_C$ , is calculated, in milligrams per litre, using equation (B.5):

$$BOD_C = BOD_G - BOD_N - BOD_{Bf} \quad \dots (B.5)$$

where

$BOD_G$  is the measured BOD of flasks  $F_T$  at the end of the test, in milligrams per litre;

$BOD_{Bf}$  is the BOD of the blank  $F_B$  at the end of the test, in milligrams per litre.

$BOD_C$  corresponds to  $BOD_t$  and is used for calculating  $BOD_S$  and  $D_t$  [see equations (1) and (2) in 9.1].

## B.2 Example

Test substance *p*-aminobenzoic acid 2-ethylhexyl ester at a concentration of 100 mg/l in  $F_T$ .


ThOD	239 mg/l
Measured $BOD_t$ at the end of the test	199 mg/l
Measured blank $BOD_{Bf}$	8 mg/l
$D_t$ without correction for nitrification	80 %
Nitrate at the end of the test 15 mg/l	$\rho_{NO_3} = 3,5$ mg/l
Nitrite at the end of the test 1 mg/l	$\rho_{NO_2} = 0,3$ mg/l
$BOD_N$ at the end of the test	17 mg/l
$BOD_C$	174 mg/l
$D_t$ corrected for nitrification	73 %

STANDARDSISO.COM : Click to view the full PDF of ISO 14851:1999

## Annex C (informative)

### Principle of a closed manometric respirometer

The respirometer is set up in a temperature-controlled environment (e.g. a water bath) and contains test vessels each fitted with a magnetic stirrer rod and a container in the headspace for a CO<sub>2</sub> absorber, a coulometric oxygen production unit, a manometer, magnetic stirrers for each vessel, and an external monitoring device and recorder (printer, plotter or computer). The test vessels are filled to about one-third of their volume with the test mixture. Continuous stirring guarantees an equilibrium of oxygen between the aqueous and the gaseous phase. If biodegradation takes place, the microorganisms consume oxygen and produce carbon dioxide which is totally absorbed. The total pressure in the vessels decreases. The pressure drop is detected by the manometer and used to initiate the electrolytic generation of oxygen. When the original pressure is re-established, electrolysis is stopped and the quantity of electricity used, which is proportional to the oxygen consumption, is continuously measured and utilized to indicate the oxygen consumption, in mg/l BOD, on the recorder.

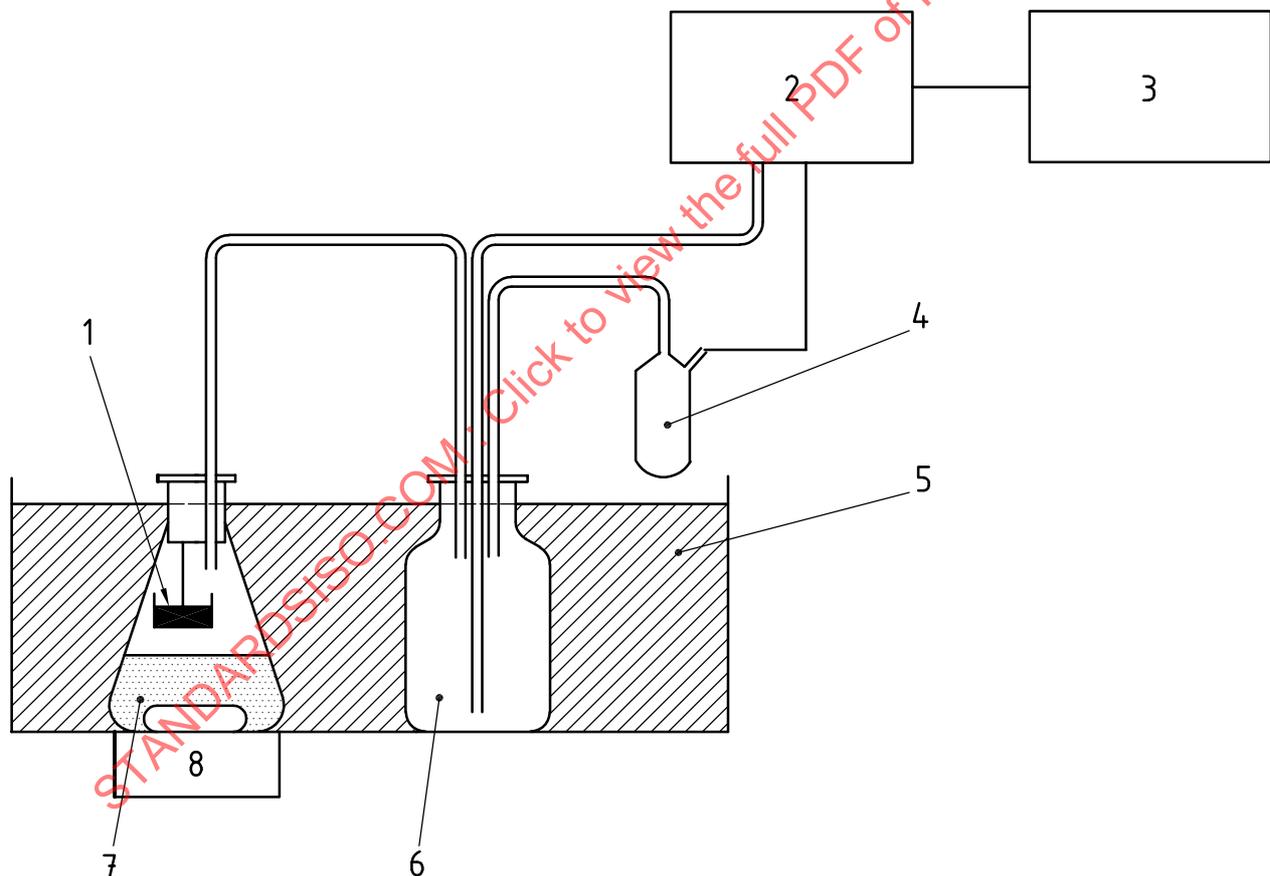

#### Key

- 1 CO<sub>2</sub> absorber
- 2 Monitor
- 3 Printer, plotter or computer
- 4 Manometer
- 5 Water bath
- 6 Oxygen-producing unit
- 7 Test flask
- 8 Stirrer

Figure C.1 — Schematic drawing of a manometric respirometer

## Annex D (informative)

### Two-phase closed-bottle version of the respirometric test

#### D.1 Principle

This version can be used as an alternative, e.g. if no respirometer is available. The inoculated medium and the test and reference materials are shaken or stirred at 20 °C to 25 °C in closed bottles containing known volumes of aqueous medium and air to assure steady-state oxygen partitioning between the aqueous and the gas phase. The biodegradation is followed by means of regular measurements of the dissolved-oxygen concentration in the aqueous phase. The total oxygen uptake in the test flasks is calculated from the difference in the measured dissolved-oxygen concentrations in the blank and test flasks divided by the oxygen saturation value under normal conditions and multiplied by the total oxygen content originally present in the aqueous and gas phases. Biodegradability is calculated as the total oxygen uptake divided by the theoretical oxygen demand (ThOD) and expressed as a percentage.

#### D.2 Special apparatus

**D.2.1 Incubation bottles:** gas-tight bottles, e.g. narrow-necked flasks with volumes of 200 ml to 300 ml and with suitable stoppers (e.g. ground-glass stoppers, butyl-rubber stoppers or screw caps), providing shielding from the light (e.g. made of brown glass). Stopper clamps are recommended. Mark each bottle with waterproof markings. If oxygen electrodes with mounted stirrers are not used, provide the bottles with a magnetic stirrer with a PTFE-coated stirrer bar. Either use bottles of standard volume such that the standard deviation from the mean volume for the batch of bottles is less than 1 ml or measure and record the volumes of individual, numbered bottles with an accuracy of 1 ml. Carefully grease the stoppers of the bottles with inert silicone grease to assure proper closing and easy removal.

**D.2.2 Oxygen electrode,** preferably with a mounted stirrer, capable of measuring in the range 0 to 10 mg/l to an accuracy of 1 %. The steady state should be reached within about 1,5 min. Mount the electrode e.g. in an inert stopper which makes a leakproof fit in the ground-glass neck of the incubation bottle or use a technique to measure the oxygen concentration in a circular bypass.

**D.2.3 Magnetic stirrer or shaking device.**

#### D.3 Procedure

Set up the incubation bottles as described in 8.4, but with three of each of bottles  $F_T$ ,  $F_B$  and  $F_C$ . Place a stirrer bar in each bottle if they are to be stirred rather than shaken. Prepare sufficient test medium, preferably the standard test medium (6.2.1), to perform the complete test. To guarantee a sufficient supply of nutrients, increase the amount of ammonium chloride in solution A (6.2.1.1) by a factor of three to 1,5 g/l. Inoculate the medium in accordance with 8.3, preferably using activated sludge at a concentration of 30 mg/l of suspended solids, mix well and add the mixture to the bottles. Add a volume equal to two-thirds of the volume of the bottle (e.g. 200 ml of liquid to 300 ml bottles). Place the bottles on the shaking device or stir them, and incubate at 20 °C to 25 °C for one week. During this time, the bacteria will use their reserve material and the inoculum will be stabilized. Then aerate the bottles with the help of water-saturated compressed air and an air diffuser for about 15 min. Measure the initial oxygen concentration. Add to the relevant bottles the test or reference material as specified in 8.1 and 8.2. The maximum test material concentration in this test should correspond to 150 mg/l ThOD which corresponds to about 90 mg/l TOC. Stopper all bottles tightly and continue the incubation.

After incubation periods of one week, or more frequently, determine the concentration of dissolved oxygen in each bottle. Maintain the bottles at the incubation temperature kept at a constant value ( $\pm 0,5$  °C) during the measurements. Calibrate accurately the oxygen electrode in accordance with the manufacturer's instructions. For oxygen measurements, take each bottle successively and shake vigorously by hand for about 30 s. Place the bottle on a stirrer, without stirring. Remove the stopper and immediately put the oxygen electrode through the neck of the bottle so that the electrode stopper effectively closes the bottle and the electrode tip is well below the liquid surface. Start the stirrer at such a speed that oxygen measurements are possible but no vortex is formed. Use the same stirrer speed throughout a set of measurements and electrode calibrations. Record the oxygen value when it is stable, which should be reached in about 2 min. Use for the calculation of the test result only those bottles in which the oxygen concentration was  $> 1,5$  mg/l. Alternatively, other appropriate techniques for measuring the dissolved-oxygen concentration in the aqueous phase can be used, such as an oxygen electrode positioned in a closed circular bypass.

Then measure the pH in each bottle and record it. If the pH is below 6,0, adjust to about 7,5 with 0,1 mol/l to 0,5 mol/l sodium hydroxide solution. If the pH is above 8,0, adjust to about 7,5 with 0,1 mol/l to 0,5 mol/l hydrochloric acid solution. Finally, aerate the medium in each bottle with an air-diffuser for 15 min and measure the oxygen concentration again as described previously. Re-stopper the bottles, put them on the shaker and continue the incubation. Correct the measured BOD values at the end of the test for nitrification (see 8.4 and annex B).

#### D.4 Calculation of results

Determine the relative oxygen uptake  $U_r$  measured in the aqueous phase in each bottle, using equation (D.1)

$$U_r = \frac{C_{Bt} - C_t}{C_s} \quad \dots (D.1)$$

where

$C_{Bt}$  is the mean value, in milligrams per litre, of the dissolved-oxygen concentration in the blank bottles after incubation, at time  $t$ ;

$C_t$  is the dissolved-oxygen concentration, in milligrams per litre, in each test bottle after incubation, at time  $t$ ;

$C_s$  is the saturation value, in milligrams per litre, for dissolved oxygen.

Use as the saturation value  $C_s$  a mean value measured after each aeration or re-aeration of the blank and test bottles. The theoretical value at standard atmospheric pressure (1013 hPa) and 20 °C is 9,08 mg/l.

Determine, using equation (D.2), the total oxygen capacity  $O_c$  (mg/bottle) of a bottle from the maximum oxygen content in the gas phase and the oxygen content in the aqueous phase at standard pressure and 20 °C:

$$O_c = (0,28 \times V_g) + (0,009 \times V_l) \quad \dots (D.2)$$

where

0,28 is the oxygen content of normal air, in milligrams per millilitre;

$V_g$  is the volume of gas in an incubation bottle, in millilitres;

0,009 is the oxygen content of saturated water, in milligrams per millilitre;

$V_l$  is the volume of liquid in an incubation bottle, in millilitres.

Normally,  $V_l$  will be constant in a test series, except if samples for analysis are taken, but  $V_g$  may differ depending on the test bottles used. If the differences between the individual bottles are small, a constant  $O_c$  may be used. If the differences are significant (e.g.  $> 2$  ml for bottles with a volume of 200 ml),  $O_c$  should be calculated for each bottle. If  $V_l$  decreases according to the volume of the sample taken,  $V_g$  increases proportionately.

Then calculate the oxygen uptake BOD (mg/bottle) from equation (D.3):

$$\text{BOD} = U_r \times O_c \quad \dots \text{(D.3)}$$

Sum the oxygen uptake  $\Sigma\text{BOD}$  (mg/bottle) for all ( $n$ ) incubation periods using equation (D.4) to obtain the BOD at the end of the test.

$$\Sigma\text{BOD} = \text{BOD}_1 + \text{BOD}_2 + \dots \text{BOD}_n \quad \dots \text{(D.4)}$$

Finally, calculate the percentage biodegradation as described in 9.1.

Use appropriate formulae to determine the abiotic elimination, as well as the biodegradation of the reference material and the inhibition control.

STANDARDSISO.COM : Click to view the full PDF of ISO 14851:1999