
**Petroleum and related products —
Determination of spray ignition
characteristics of fire-resistant
fluids —**

**Part 2:
Spray test — Stabilised flame heat
release method**

*Produits pétroliers et produits connexes — Détermination
des caractéristiques d'inflammation des fluides difficilement
inflammables en jet pulvérisé —*

*Partie 2: Essai de pulvérisation — Méthode par dégagement de
chaleur d'une flamme stabilisée*



STANDARDSISO.COM : Click to view the full PDF of ISO 15029-2:2018



COPYRIGHT PROTECTED DOCUMENT

© ISO 2018

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	2
5 Reagents and materials	2
6 Apparatus	3
7 Sampling and sample preparation	11
8 Apparatus preparation	11
9 Procedure	12
9.1 Measurements at a propane flow rate of 0,13 Nm ³ /h	12
9.2 Measurements at a propane flow rate of 0,4 Nm ³ /h	13
9.3 Rejection of test data	13
9.4 Repeat testing	13
9.5 Number of tests	14
9.5.1 General	14
9.5.2 Calculation	14
9.5.3 Marginal values	14
9.5.4 Conclusion	14
10 Calculations	15
10.1 Ignitability factor	15
10.1.1 At propane flow rate of 0,13 Nm ³ /h	15
10.1.2 At propane flow rate of 0,4 Nm ³ /h	15
10.2 Flame length index	15
10.2.1 At propane flow rate of 0,13 Nm ³ /h	15
10.2.2 At propane flow rate of 0,4 Nm ³ /h	15
10.3 Smoke density	16
11 Expression of results	16
11.1 Individual results	16
11.2 Ranking system	16
12 Precision	16
13 Test report	16
Annex A (normative) Verification of propane pressure and flow rate	17
Annex B (normative) Verification of propane flame characteristics	18
Annex C (normative) Test apparatus calibration	23
Annex D (informative) Fire-resistant classification scheme	25
Annex E (informative) Examples of pro-forma for test results	26
Bibliography	29

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established, has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 28, *Petroleum and related products, fuels and lubricants from natural or synthetic sources*.

This first edition of ISO 15029-2 cancels and replaces ISO/TS 15029-2:2012 which has been technically revised. Definitions and some procedural steps have been further clarified based on comments received from the market. This method has now largely superseded the older procedure in ISO 15029-1 in specifications and fluid development. Unlike ISO 15029-1, this document is a method that can rank fluids in terms of their spray flammability and as several test rigs are available, is capable of the generation of some precision data.

A list of all parts in the ISO 15029 series can be found on the ISO website.

Petroleum and related products — Determination of spray ignition characteristics of fire-resistant fluids —

Part 2:

Spray test — Stabilised flame heat release method

WARNING — Use of this document can involve hazardous materials, operations and equipment. This document does not purport to address all of the safety problems associated with its use. It is the responsibility of users of this standard to ensure appropriate measures to safeguard the health and safety of personnel prior to application of the standard, and to determine the applicability of any other restrictions.

1 Scope

This document specifies a method by which the fire hazards of pressurised sprays of fire-resistant fluids can be compared. Two sizes of propane flame are used to ignite and stabilise combustion of an air-atomised release of fluid. Measurements related to the rate of heat release, length of flame and density of smoke give quantitative information on the fire behaviour of the fluid.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3170, *Petroleum liquids — Manual sampling*

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*

ISO 9162, *Petroleum products — Fuels (class F) — Liquefied petroleum gases — Specifications*

IEC 60584-1, *Thermocouples — Part 1: EMF specifications and tolerances*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

3.1

stabilised spray flame

point at which the rate of energy release, flame length and other combustion properties, are steady as a function of time, so that sensible time-averaged values can be calculated

3.2

flame length

distance in millimetres from the vertical centre line of the gas burner to the furthest downstream point reached by the visible flame

3.3

flame length index

function of the flame length and propane flow rate corrected to the nearest integer

3.4

ignitability factor

function of heat release at a specific propane flow rate corrected to the nearest integer

3.5

smoke density

function of smoke opacity in the flue pipe measured before and after introduction of the test fluid

Note 1 to entry: See ISO 5659-2:2017, 3.8.

4 Principle

A pre-conditioned flow of the test fluid is delivered to a test chamber through a twin-fluid atomiser. Compressed air, supplied to the nozzle at a controlled rate, is used to produce an atomised spray, which is exposed to a defined flame of a gas burner present throughout the test. As a result of heat input at a steady rate from the gas flame, a stabilised spray flame (3.1) is produced so that combustion properties, such as the rate of energy release, flame length, (3.2) and smoke production (3.5) are sufficiently steady over time to allow time-averaged values to be measured.

Temperatures are measured both at the entry to the combustion chamber and in the exhaust, with the burner operating first without, and then with, release of the test fluid. The flame length (3.2) and smoke opacity of the exhaust can be measured. Calculations of functions, such as flame length index (3.3) ignitability factor (3.4) and smoke density (3.5) are made from these measurements. A system for ranking the performance of fire-resistant fluids based upon these measurements and computed performance indices is proposed.

5 Reagents and materials

- 5.1 **Propane**, high purity (minimum 98 %) grade, conforming to the requirements of ISO 9162.
- 5.2 **Nitrogen**, oxygen-free, commercial grade.
- 5.3 **Compressed air**.
- 5.4 **Water**, conforming to the requirements of grade 3 of ISO 3696:1987.
- 5.5 **Mono ethylene glycol**, laboratory grade (98 % purity).
- 5.6 A solvent compatible with the tested fluid, laboratory grade.

6 Apparatus

6.1 Test installation

6.1.1 General

The major components of the installation are described in [6.1.2](#) to [6.1.6](#).

[Figure 1](#) gives a general layout of the test installation.


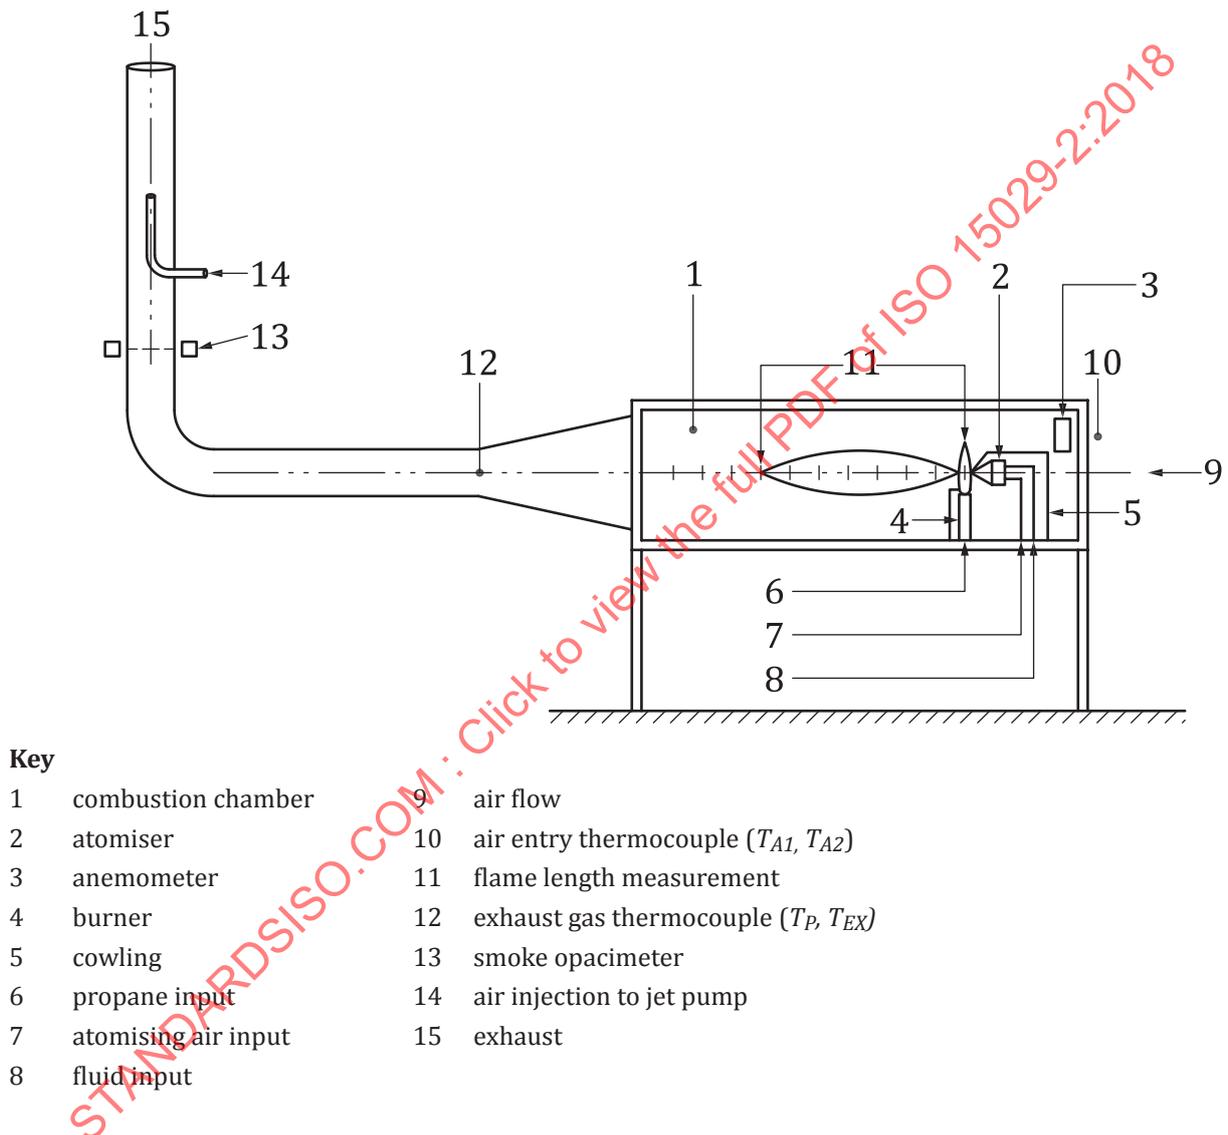


Figure 1 — General view of installation

Figure 2 shows a schematic diagram of a suggested layout of the test equipment detailing the different input streams to the combustion chamber and exhaust duct. In this Figure A, B and C respectively refer to the propane, air and fluid delivery streams.

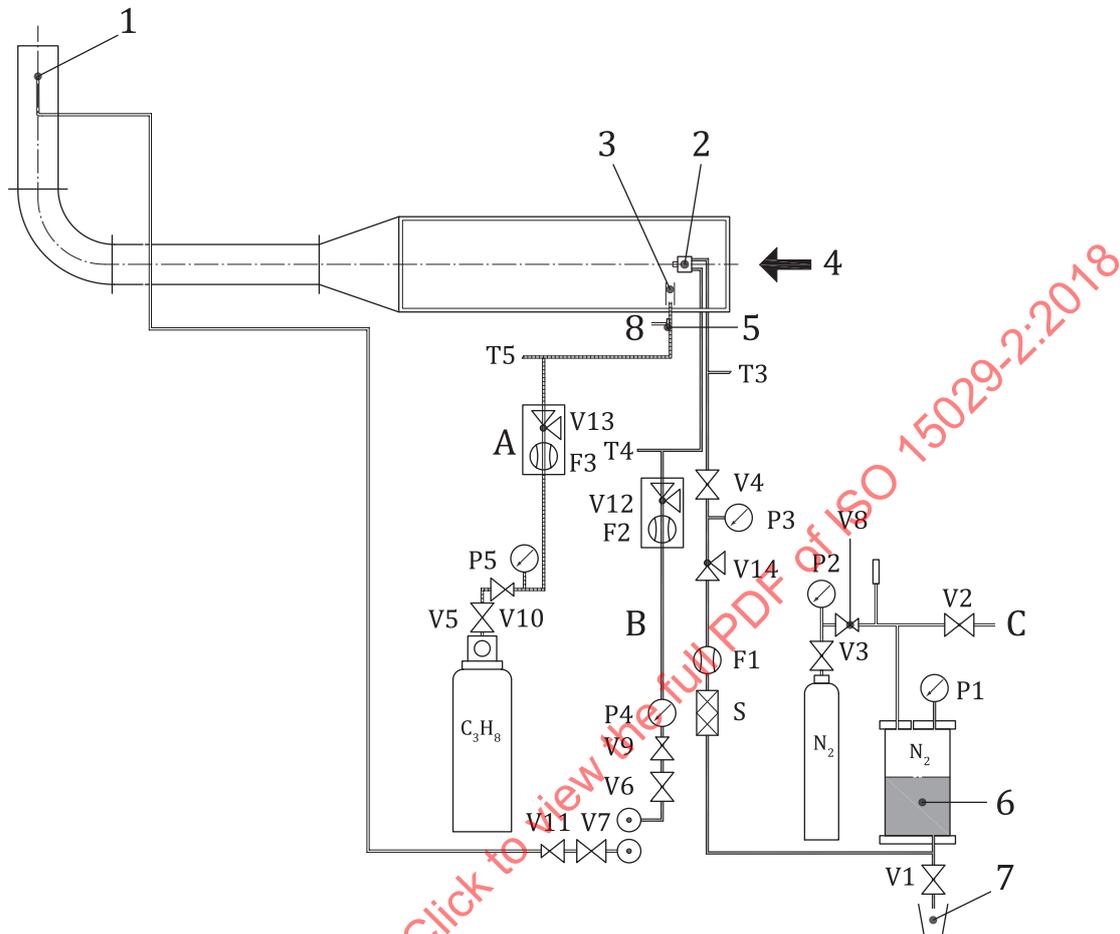


Key

1	jet pump	P1	pressure gauge 0 MPa to 2,5 MPa
2	atomiser	P2	pressure gauge 0 MPa to 27,6 MPa
3	pilot burner	P3	pressure gauge 0 MPa to 2,5 MPa
4	induced air input 1,3 m/s to 1,5 m/s	P4	pressure gauge 0 MPa to 0,6 MPa
5	mixing chamber	P5	pressure gauge 0 MPa to 0,2 MPa
6	test fluid 13 °C to 25 °C	F1	liquid flow meter 90 ml/min ± 0,5 ml/min
7	drain	F2	variable area flow meter or equivalent 0,4 Nm ³ /h to 3,0 Nm ³ /h
8	air in	F3	variable area flow meter or equivalent 0,1 Nm ³ /h to 0,5 Nm ³ /h
T3	fluid thermocouple	V1-7	shut-off valves
T4	atomising air thermocouple	V8-V11	pressure regulators
T5	propane gas thermocouple	V12-V14	flow control valves
S	fluid filter		

Figure 2 — Schematic diagram of suggested test rig layout

6.1.2 Combustion chamber

This shall be fabricated from steel sheet, 8 mm thick, of square cross-section with internal dimensions of $(2\,000 \pm 5)$ mm \times (490 ± 5) mm \times (490 ± 5) mm. The inner and outer surfaces shall be painted with black heat-resistant paint. A clear window of heat-resistant glass, 8,5 mm thick, shall be located in one side of the chamber. The glass shall be $(1\,920 \pm 10)$ mm \times (525 ± 10) mm providing an open area of the window of $(1\,880 \pm 10)$ mm \times (480 ± 10) mm. The window is hinged from below to allow access to the chamber. The window shall be clamped shut during use and sealed with mineral fibre tape to avoid ingress of air (see Figure 3).

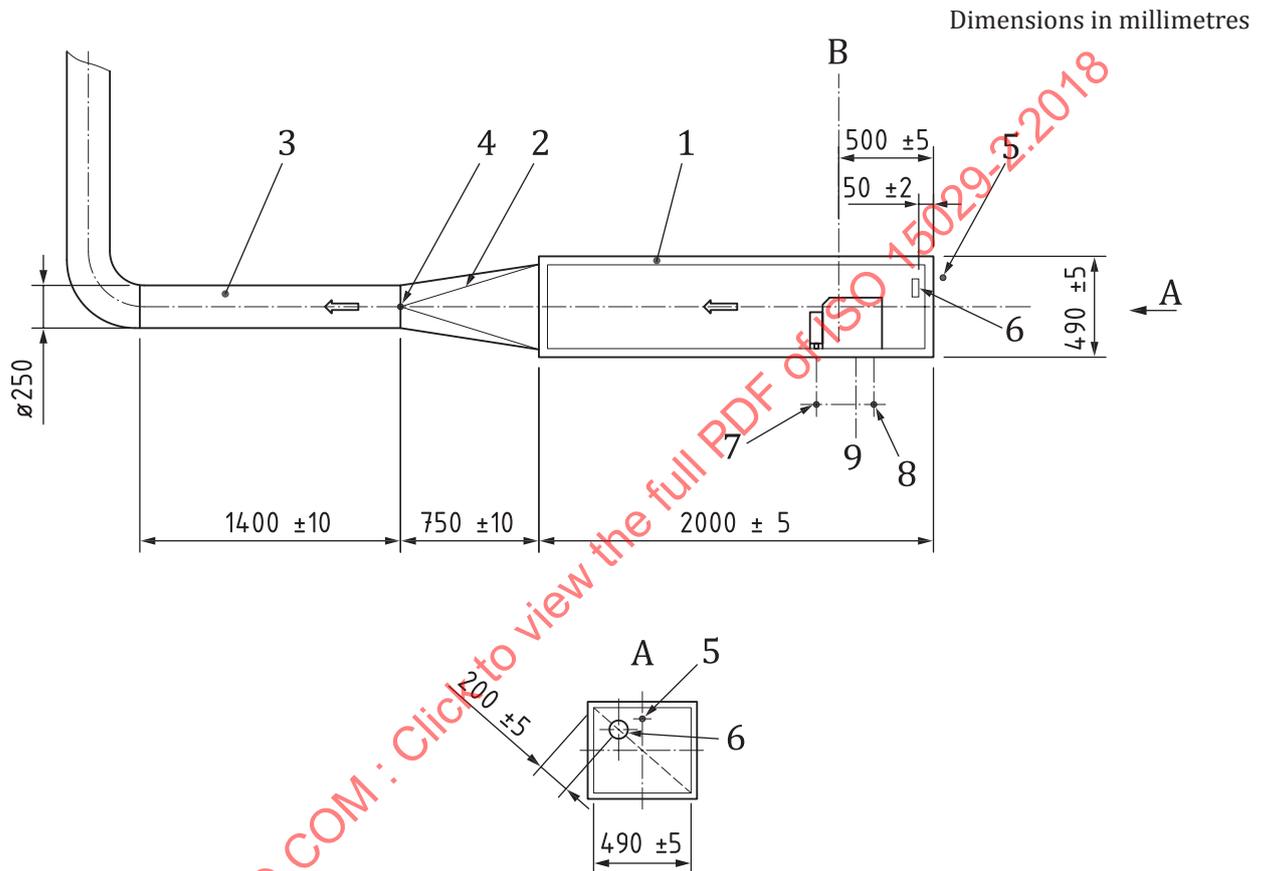

Key

1	combustion chamber	6	anemometer
2	contraction	7	propane gas thermocouple
3	flue pipe	8	atomising air thermocouple
4	exhaust gas thermocouple	9	fluid inlet pipe
5	ambient air thermocouple	B	end of fluid delivery nozzle

Figure 3 — Combustion chamber and exhaust system

6.1.3 Extraction system

The combustion chamber exit (Figure 3) shall be connected to a contraction fabricated from steel sheet 1 mm thick, providing a transition from the square to a circular cross-section with an internal diameter of $250 \text{ mm} \pm 4 \text{ mm}$. This contraction, $750 \text{ mm} \pm 10 \text{ mm}$ long, connected to a horizontal section of flue pipe $1\,400 \text{ mm} \pm 10 \text{ mm}$ in length that in turn may be connected to further exhaust ducting or a clearing system that shall be designed to provide stable conditions in the combustion chamber during a test.

The air flow, through the chamber, is produced by a jet pump mounted in the exhaust duct producing an air velocity of $1,4 \text{ m/s} \pm 0,1 \text{ m/s}$ measured $50 \text{ mm} \pm 2 \text{ mm}$ inside the open end of the combustion chamber inlet, and $200 \text{ mm} \pm 5 \text{ mm}$ along the entry plane diagonal from one upper corner of the test chamber (Figure 3). The temperature of the air entering the chamber shall be sufficiently constant within the range $10 \text{ }^\circ\text{C}$ to $25 \text{ }^\circ\text{C}$, such that the temperature variation over a period of 30 s shall not exceed $1 \text{ }^\circ\text{C}$. The relative humidity of the air shall lie between 40 % and 80 %.

6.1.4 Spray delivery system

6.1.4.1 Reservoir

The test fluid shall be contained in a steel reservoir of minimum capacity 3 l, designed for an internal pressure of 2,5 MPa at $20 \text{ }^\circ\text{C}$. The flow of fluid from the reservoir is provided by means of pressurised nitrogen (5.2) supplied to the upper part of the reservoir, with a valve situated in the nitrogen supply pipe. Means shall be provided to permit complete drainage of the system.

6.1.4.2 Test fluid delivery

The fluid volume flow rate can be measured with a suitable flowmeter and controlled to $90 \text{ ml/min} \pm 0,5 \text{ ml/min}$ by means of a needle valve or other equivalent device. The fluid temperature is maintained between $10 \text{ }^\circ\text{C}$ and $25 \text{ }^\circ\text{C}$, and measured by a thermocouple located immediately before the fluid nozzle. The fluid is delivered to the atomiser¹⁾ through nylon and/or steel piping with an internal diameter of $7,5 \text{ mm} \pm 2,5 \text{ mm}$, rated at 2 MPa and the flowmeter shall be located $350 \text{ mm} \pm 150 \text{ mm}$ downstream of the valve. A standard oil filter can be incorporated in the line.

6.1.4.3 Compressed air

Compressed air shall be supplied via a suitable mesh filter to remove droplets and particulates, at a steady flow rate of $1,92 \text{ Nm}^3/\text{h} \pm 0,05 \text{ Nm}^3/\text{h}$ at a pressure of 0,2 MPa. The flow rate shall be measured with a variable area flowmeter or other equivalent device having a range of $0,4 \text{ Nm}^3/\text{h}$ to $3,0 \text{ Nm}^3/\text{h}$, located $3\ 500 \text{ mm} \pm 500 \text{ mm}$ before the spray jet at a pressure of 0,2 MPa, and controlled by a valve installed downstream of the flowmeter. The temperature of the atomising air shall be between $10 \text{ }^\circ\text{C}$ and $25 \text{ }^\circ\text{C}$.

6.1.5 Burner system

6.1.5.1 System design

The gas burner, constructed of brass and illustrated in Figure 4, provides a continuous ignition source using propane (5.1) pre-mixed with air. It incorporates a nozzle, drilled to a diameter of 0,68 mm, and two mixing chambers, the whole mounted rigidly on to a steel base plate of 6 mm thickness (see Figure 5). The exit of the 26 mm internal diameter mixing chamber shall be $143 \text{ mm} \pm 1 \text{ mm}$ below the centre line of the atomiser, and a distance of $42,5 \text{ mm} \pm 1 \text{ mm}$ downstream of the atomiser orifice. If required, the burner can be manufactured from the illustration given in Figure 5.

Propane, at a minimum pressure of 0,25 MPa, shall be supplied through $4\ 000 \text{ mm} \pm 1\ 000 \text{ mm}$ of flexible tubing of $6 \text{ mm} \pm 2 \text{ mm}$ bore, to an assembly of a pressure gauge, flowmeter and valve. Further flexible and/or metal tubing, $2\ 500 \text{ mm} \pm 500 \text{ mm}$ in length and of a minimum bore of 6 mm, is installed between the valve in the assembly and the gas burner.

At a controlled pressure of 0,2 MPa, the propane flow rate shall be either $0,13 \text{ Nm}^3/\text{h} \pm 0,005 \text{ Nm}^3/\text{h}$, or $0,40 \text{ Nm}^3/\text{h} \pm 0,005 \text{ Nm}^3/\text{h}$, depending upon specific test requirements. The flow rate shall be measured with a variable area flowmeter having a range of $0,10 \text{ Nm}^3/\text{h}$ to $0,50 \text{ Nm}^3/\text{h}$ and of suitable resolution. The temperature of the propane on entering the burner shall be between $10 \text{ }^\circ\text{C}$ and $25 \text{ }^\circ\text{C}$.


1) Body type B1/4JB-BSS with SU12-22 manufactured by Spraying Systems Company (<http://www.spray.com>) is an example of a suitable product available commercially. This information is for the convenience of users of this part of ISO 15029 and does not constitute an endorsement by ISO of this product.

6.1.5.2 System verification

Upon installation the system shall be verified for conformity to the standard design. [Annexes A](#) and [B](#) describe protocols for checking the control systems and flame characteristics. This should be done at least annually or if it is suspected that the burner characteristics have changed. The burner may be checked by sampling the flame temperature at a few selected locations and comparing the measurements with the standard values given in [Annex B](#). The flame characteristics can be adjusted by positioning of the regulation collar in relation to the burner air inlet port ([Figure 4](#)).

STANDARDSISO.COM : Click to view the full PDF of ISO 15029-2:2018

Dimensions in millimetres

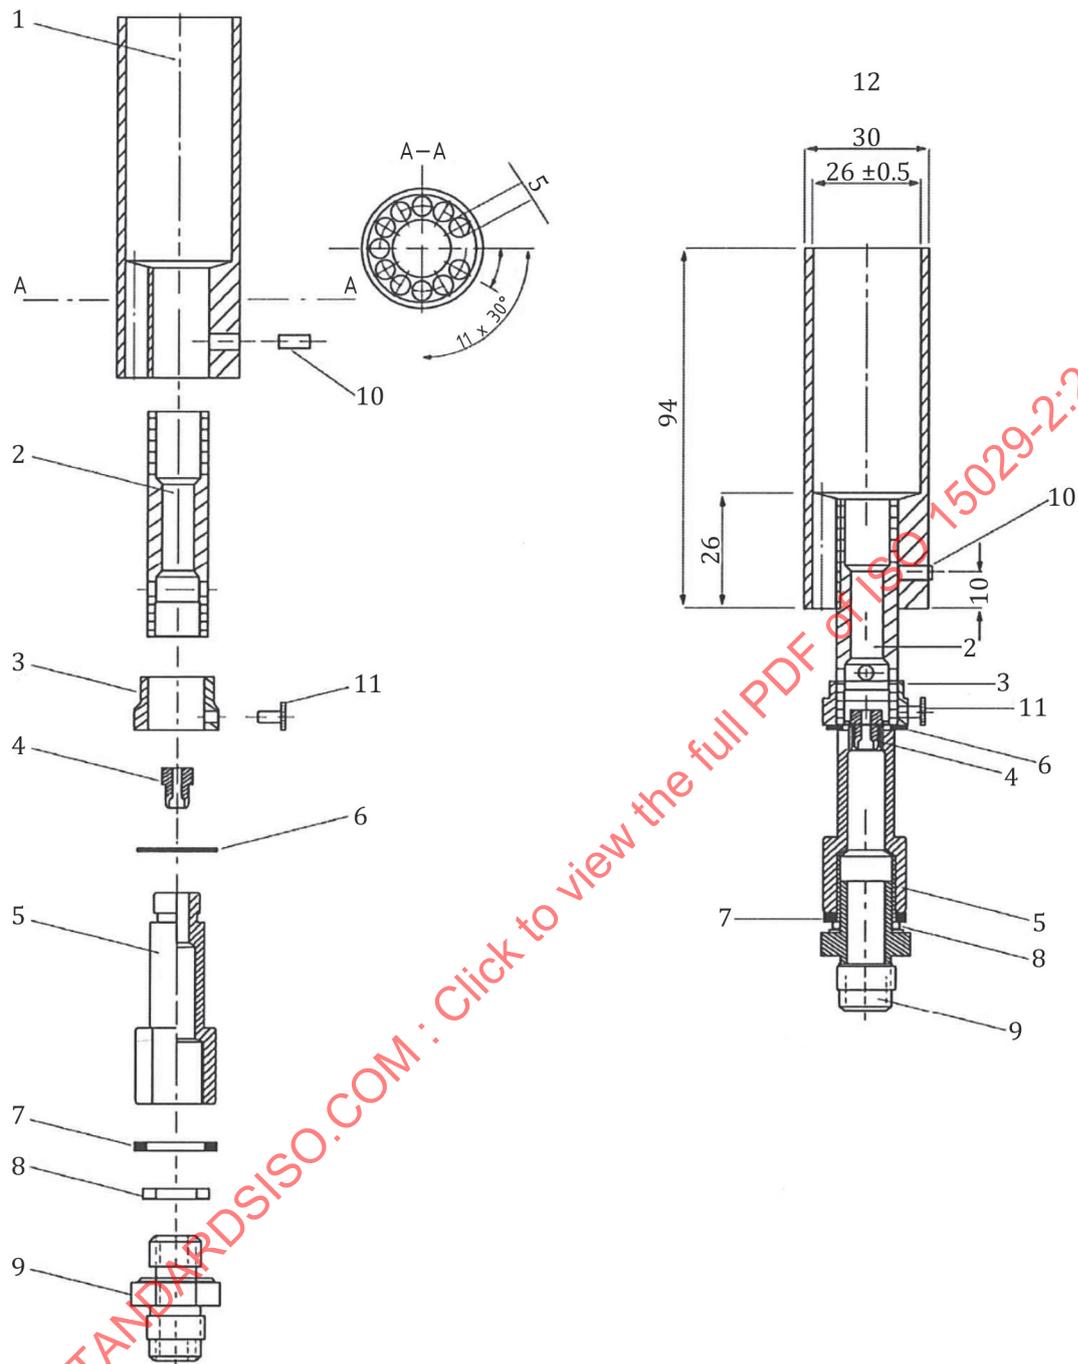

Key

- | | | | | | |
|---|-------------------|---|------------------------------------|----|-----------------------|
| 1 | mixing chamber 1 | 5 | nozzle holder with flash-back unit | 9 | straight male adaptor |
| 2 | mixing chamber 2 | 6 | washer | 10 | locking screw |
| 3 | regulation collar | 7 | washer | 11 | locking screw |
| 4 | burner nozzle | 8 | sealing ring | 12 | completed assembly |

Figure 4 — Propane burner


6.1.6 Burner and atomiser mounting

6.1.6.1 Mounting

The atomiser and burner assembly, on the steel base plate, is protected by a cowling fabricated from 1 mm thick sheet steel bent into the form shown in Figure 5, with a height of $300 \text{ mm} \pm 1 \text{ mm}$, overall width of $97 \text{ mm} \pm 1 \text{ mm}$, and overall length of $255 \text{ mm} \pm 1 \text{ mm}$. The burner shall also be protected from the surrounding air flow by a cylindrical cowling of $87 \text{ mm} \pm 1 \text{ mm}$ diameter, containing a vertical slot with an external opening of $61 \text{ mm} \pm 2 \text{ mm}$ on its upstream face. Three threaded supports provide a means of elevation of this cowling, with its upper part at a distance of $37 \text{ mm} \pm 2 \text{ mm}$ from the horizontal plane passing through the atomiser axis.

6.1.6.2 Placement

The base plate is positioned on the floor of the combustion chamber with the atomiser orifice $500 \text{ mm} \pm 5 \text{ mm}$ downstream of the combustion chamber inlet orifice. Connections through the base plate and combustion chamber floor shall be provided for the supply of air, propane and test fluid to the burner and atomiser as appropriate.

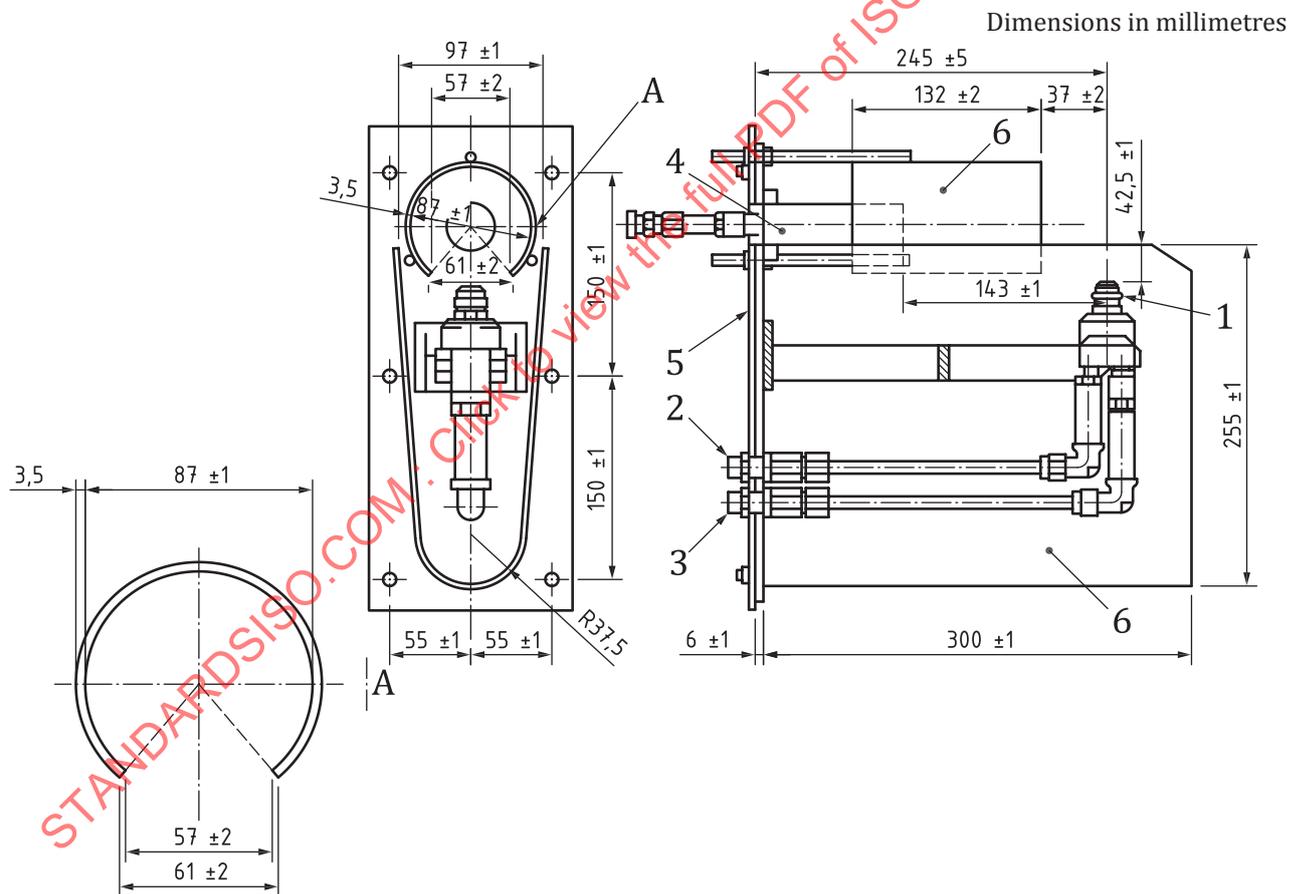

Key

- | | | | |
|---|--------------|---|----------------|
| 1 | spray nozzle | 4 | propane burner |
| 2 | fluid supply | 5 | base plate |
| 3 | air supply | 6 | cowling |

Figure 5 — Atomiser and burner system

6.2 Instrumentation

6.2.1 Temperature sensors

Five T-type Cu-CuNi thermocouples with an outer diameter of 1,5 mm, conforming to the requirements of IEC 60584-1, or temperature measurement devices of equivalent precision and accuracy, are positioned as illustrated in [Figure 2](#). The third thermocouple is positioned in the test fluid reservoir with at least 50 mm of sheath completely immersed in the fluid, and not in contact with the vessel wall. All the thermocouples shall be used with 0 °C reference junctions, in accordance with IEC 60584-1. Measurement accuracy shall be $\pm 0,5$ °C over the range 15 °C to 200 °C, and the temperature resolution shall be 0,1 °C.

The accuracy of the test result is highly dependent upon the accurate positioning, particularly in the vertical of the exhaust gas thermocouple. This shall be located with an accuracy of $\pm 0,5$ mm and checked before the commencement of each new series of tests.

Where a computer is used, both this and the data acquisition system shall be capable of calculating averages of at least 100 values of each temperature measured over 120 s. Where manual data collection is employed digital temperature readouts should be used with an accuracy of $\pm 0,1$ °C.

6.2.2 Anemometer

The air flow velocity in the combustion chamber is measured using a rotating vane anemometer with a vane diameter of $95 \text{ mm} \pm 30 \text{ mm}$ located as illustrated in [Figure 2](#) (including section A).

6.2.3 Humidity sensors

The relative humidity of the incoming air used in each test series shall be measured and recorded at the beginning and end of each day of testing.

6.2.4 Flame length scale

A linear scale of at least 1 m in length, with a resolution of no greater than 10 mm, shall be attached to the combustion chamber side window.

6.2.5 Smoke meter

A white light obscuration smoke opacity meter, using an illuminated beam of $20 \text{ mm} \pm 5 \text{ mm}$ diameter, is mounted $625 \text{ mm} \pm 125 \text{ mm}$ downstream of the contraction in the flue pipe. The arrangement shall not reduce light transmission by soot deposits by more than 5 %²⁾.

6.2.6 Calibration of instruments

6.2.6.1 Temperature sensors: all the temperature sensors shall be calibrated in accordance with relevant standards and appropriate corrections shall be applied to observed readings.

6.2.6.2 Smoke meter: the output of the smoke meter shall be calibrated before and after using at least three neutral density filters inserted in the light beam, giving 25 %, 50 % and 75 % light obscuration use. Observed readings shall be corrected for deviations in linearity.

6.2.6.3 Other meters: flowmeters and the anemometer shall be calibrated according to the manufacturer's recommendations or at least annually by means traceable to a relevant standard, and the appropriate corrections made to observed readings.

2) A suitable instrument is the DIN 50055 White Light Smoke Measurement System manufactured by Fire Testing Technology of East Grinstead, UK. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO. Equivalent products may be used if they can be shown to lead to the same results.

6.2.6.4 Humidity sensor: the relative humidity sensor should be calibrated according to the manufacturer's recommendations and appropriate corrections shall be applied to all observed readings.

6.2.6.5 Test apparatus: prior to each new series of tests, the entire test apparatus shall be calibrated for ignitability factor by the procedure described in [Annex C](#) and corrected values used for reporting, as described in [10.1](#). It is important that any changes in the measured ignitability factor values obtained with the calibration fluids be investigated to ensure that the test apparatus has not been subject to modification and conforms to the requirements of this document.

If calibration test values differ significantly from those previously obtained, then the calibration of individual components (e.g. flowmeters) shall be examined.

7 Sampling and sample preparation

7.1 Unless otherwise specified, samples of at least 5 l shall be obtained in accordance with the procedures described in ISO 3170.

7.2 Store samples in sealed containers at a temperature between 10 °C to 30 °C under clean and dry conditions. After removing a sample immediately re-seal the container to minimise any moisture loss or gain.

7.3 Mix the sample by shaking or stirring and examine for clarity and contamination before transferring the test portion to the conditioning beaker. If phase separation and/or particulate are observed, discard the sample.

7.4 For water-based fluids, such as those in categories HFAE or HFAS (as classified in ISO 6743-4), prepare the concentrate with water ([5.4](#)) within 1 h of the start of the test.

8 Apparatus preparation

8.1 Turn off the propane supply and thoroughly clean the apparatus in preparation for each test, in the manner described in [8.2](#) to [8.6](#).

8.2 Remove any traces of previous sample by draining the reservoir, pipework and flowmeter by means of disconnecting orifices at the various lowest points. Re-connect these orifices.

8.3 Clean the internal surfaces of the reservoir with 500 ml of solvent appropriate to the sample previously used.

8.4 Open the valve in the fluid supply circuit and pressurise the reservoir with nitrogen. Allow at least 250 ml of liquid to be expelled through the atomiser. Close the valve and de-pressurise. Drain the fluid/solvent at the atomiser orifice. Repeat the procedure given in [8.2](#).

8.5 Remove any further traces of solvent in the apparatus by evaporation or careful wiping with a lint-free cloth.

8.6 Place 500 ml of the new test fluid in the reservoir and repeat the procedure given in [8.4](#). If the new fluid is in the same category and quality as that last tested, repeat this operation twice. If the new fluid is a different category or quality, repeat the operation at least three times.

9 Procedure

9.1 Measurements at a propane flow rate of 0,13 Nm³/h

9.1.1 Place 1 500 ml of sample into a 2 000 ml glass beaker and heat or cool as appropriate to the test temperature (10 °C to 25 °C), stirring to maintain homogeneity.

When the fluid is supplied as a concentrate it should first be diluted with distilled or deionised water as recommended by the manufacturer or supplier and 1 500 ml of the diluted fluid placed in the reservoir.

9.1.2 Pour the test portion into the reservoir of the apparatus and pressurise the reservoir to the pressure established for the specified flow rate. Pass fluid through the atomiser, without atomising air, combustion chamber air or burner propane, until at least 200 ml of fluid has been collected at the atomiser exit. Check that the flow has been steady, that there are no air bubbles in the delivery and that the fluid is free of contaminant. Initial releases will be carried out to establish the pressure required to provide the specified flow. This will normally be about 1 MPa, the flow can be adjusted using the needle valve.

9.1.3 The fluid delivery rate at the nozzle should be checked by collecting fluid in a suitably graduated container over a measured time; the volume and time for collection taking into account the accuracy required. If necessary, adjust the flow control valve until the flow rate is within the specified limits. Initial releases will be carried out to establish the pressure required to provide the specified flow. This will normally be about 1 MPa, the flow can be adjusted using the needle valve.

9.1.4 In order to ensure test parameters are within the specified limits, measure and record fluid temperature, air inlet temperature and atmospheric humidity.

9.1.5 Set the air flow rate through the combustion chamber to obtain an air velocity of 1,4 m/s ± 0,1 m/s. Record the value and also the ambient relative humidity.

9.1.6 Ignite the propane burner and adjust the propane flow rate to 0,130 Nm³/h ± 0,005 Nm³/h.

9.1.7 Adjust the atomising air to a flow rate of 1,92 Nm³/h ± 0,05 Nm³/h.

9.1.8 Measure and record the light obscuration from the smoke meter under steady conditions before the test fluid is introduced into the chamber, V_0 , as the average of at least four readings taken over a period of 60 s.

9.1.9 With the glass window of the combustion chamber closed, and sealed, allow conditions to stabilise to a point at which the temperature of the exhaust gases at the chamber exit T_P and the temperature of the air at the chamber inlet, T_{AI} , vary by no more than 1 °C over a period of 30 s. Record these values to the nearest 0,1 °C, taking the average of at least four values over a 60 s period.

9.1.10 Pass test fluid to the atomiser at the specified flow rate of 90 ml/min ± 0,5 ml/min and measure the new exhaust temperature, T_{EX} , at intervals of approximately 5 s, until the average of at least five values over a period of 30 s is within 2,5 % of the average of at least five values taken in a consecutive period of 30 s.

9.1.11 With conditions steady, take measurements of the temperature at the chamber inlet, T_{A2} , and the new exhaust temperature, T_{EX} , as the average of at least 10 measurements of each taken over a period of 120 s.

9.1.12 If required, measure and record the flame length, L_A , as the average of at least 10 measurements taken over a period of 120 s of steady conditions. In the case of a fluctuating flame, the length shall be the furthest distance reached downstream instantaneously.

9.1.13 If required, measure the light obscuration from the smoke meter with the fluid test fluid flowing as the average of at least four readings taken over the same period of 60 s and record as V_1 .

9.1.14 Calculate the ignitability factor, RI , as outlined in [Clause 10](#).

9.1.15 If required, calculate the flame length index, RL as outlined in [Clause 10](#).

9.1.16 If required, calculate the smoke density, D as outlined in [Clause 10](#).

9.1.17 If, during a test, the fluid has been found to have an ignitability factor above 50, or a flame length of less than 100 mm, at a propane flow rate of $0,13 \text{ Nm}^3/\text{h}$, it is necessary to carry out the test at a higher propane flow rate, as described in [9.2.1](#) and to report these results.

IMPORTANT — The fluid flow rate can vary during the test as the equipment (and fluid) temperatures increase. It is therefore necessary to check the flow rate after every four determinations and, if outside the limit, then repeat the test runs as appropriate.

9.2 Measurements at a propane flow rate of $0,4 \text{ Nm}^3/\text{h}$

9.2.1 The test conditions shall be established as indicated in [9.1.1](#) to [9.1.7](#) with the exception that the propane flow rate shall now be adjusted to $0,400 \text{ Nm}^3/\text{h} \pm 0,005 \text{ Nm}^3/\text{h}$.

9.2.2 Carry out the procedure described in [9.1.8](#) to [9.1.16](#) at the new propane flow rate.

9.3 Rejection of test data

A test run shall be discontinued if, during the procedure any of the test conditions are not satisfied, as defined below:

- a) the temperature at the combustion chamber inlet is constant to within $\pm 1 \text{ }^\circ\text{C}$;
- b) the atomising air flow rate is constant at $1,92 \text{ Nm}^3/\text{h} \pm 0,05 \text{ Nm}^3/\text{h}$;
- c) the propane flow rate is constant at either $0,130 \text{ Nm}^3/\text{h} \pm 0,005 \text{ Nm}^3/\text{h}$ or $0,400 \text{ Nm}^3/\text{h} \pm 0,005 \text{ Nm}^3/\text{h}$;
- d) the test fluid flow rate is constant at $90 \text{ ml}/\text{min} \pm 0,5 \text{ ml}/\text{min}$;
- e) the air velocity through the combustion chamber is constant at $1,4 \text{ m}/\text{s} \pm 0,1 \text{ m}/\text{s}$;
- f) the relative humidity of the air is 40 % to 80 %;
- g) the temperature of the test fluid is $10 \text{ }^\circ\text{C}$ to $25 \text{ }^\circ\text{C}$;
- h) the temperature of the atomising air at the nozzle, and of the propane, is $10 \text{ }^\circ\text{C}$ to $25 \text{ }^\circ\text{C}$.

Testing may be resumed as soon as the conditions meet the above limits.

9.4 Repeat testing

The relatively large number of measurements required to obtain the test results are best recorded on proforma result sheets, which may also allow space for any calculation required. Examples of pro-forma are in [Annex E](#).

9.5 Number of tests

9.5.1 General

The minimum number of test determinations is set upon the basis of obtaining an ignitability factor, RI , which is the most sensitive property being measured, within some defined limits of accuracy. The minimum level of accuracy set is that the average of N individual RI measurements lies within 5 % of the true mean value obtained from an infinite sample size, with 67 % confidence.

9.5.2 Calculation

Assuming a normal distribution of measurements, the number of tests required to satisfy the condition specified in 9.5.1 is given by the equation:

$$400S_N^2/N RI_N \leq 1,0 \quad (1)$$

where

N is the number of tests;

RI_N is the average of N tests;

S_N is the variance, defined by [Formula \(2\)](#).

$$S_N^2 = \sum (RI_i - RI_N)^2 / (N - 1) \quad (2)$$

where RI_i is the i th measurement of ignitability factor.

The percentage error, δ , in the mean, RI_N , of N measurements of RI , is given by the equation:

$$\delta = 100S_N / RI_N N^{0,5} \quad (3)$$

Where the ignitability factor is found to be within 5 % of a grade boundary, a sufficient number of tests are required to derive a mean value of RI which is accurate to within one integer. This requires:

$$N \geq S_N^2 \quad (4)$$

Tests shall be repeated until this calculation is satisfied by repeating the procedure from [9.1.7](#).

9.5.3 Marginal values

When an average value of RI , obtained at a propane flow rate of 0,13 Nm³/h, lies between 35 and 60, and more than $N/2$ of these tests give individual values greater than 50, that fluid shall be re-tested at the higher propane flow rate of 0,4 Nm³/h, and the low propane flow rate results discarded. If less than $N/2$ tests at the low propane flow rate give individual values greater than 50, then all the values are included in the calculation of average RI .

If the average of these values is greater than or equal to 50, then this fluid shall be re-tested at the higher flow rate. If a fluid, tested at the low propane flow rate, gives an average value of equal to or above 50, but re-tested at the higher propane flow rate, gives an average value of below 50, the value of RI for that fluid shall be taken as 50.

9.5.4 Conclusion

On the basis of the above considerations, the minimum number of tests required at a specified propane flow rate is eight.

10 Calculations

10.1 Ignitability factor

10.1.1 At propane flow rate of 0,13 Nm³/h

Calculate the uncorrected ignitability factor, RI_W , at the low propane flow rate from the following equation:

$$RI_W = 500(T_p - T_{A1}) / [7(T_{EX} - T_{A2})] \quad (5)$$

where

T_p is the averaged exhaust temperature without release of the test fluid, expressed in degrees Celsius;

T_{A1} is the averaged air temperature at the chamber inlet without release of the test fluid, expressed in degrees Celsius;

T_{EX} is the averaged exhaust temperature with release of the test fluid, expressed in degrees Celsius;

T_{A2} is the averaged air temperature at the chamber inlet with release of the test fluid, expressed in degrees Celsius.

Correct RI_W to obtain RI from the low propane flow rate calibration curve developed by the method described in [Annex C](#), and in accordance with [6.2.6.5](#).

10.1.2 At propane flow rate of 0,4 Nm³/h

Calculate the uncorrected ignitability factor, RI_X , at the high propane flow rate from the following equation:

$$RI_X = [100(T_p - T_{A1}) / (T_{EX} - T_{A2})] + 30 \quad (6)$$

Correct RI_X to obtain RI from the high propane flow rate calibration curve developed by the method described in [Annex C](#), and in accordance with [6.2.6.5](#).

10.2 Flame length index

10.2.1 At propane flow rate of 0,13 Nm³/h

Calculate the flame length index, RL_W , from the measured flame length at the low propane volumetric flow rate, L_A , in mm, from the following equation:

$$RL_W = 5\,000 / L_A \quad (7)$$

10.2.2 At propane flow rate of 0,4 Nm³/h

Calculate the flame length index, RL_X , from the measured flame length at the high propane volumetric flow rate, L_B , in mm, from the following equation:

$$RL_X = (6\,250 / L_B) + 37,5 \quad (8)$$

10.3 Smoke density

Calculate the smoke density, D , defined by the equation:

$$D = \lg(V_0/V_1) \quad (9)$$

where

V_0 is the light obscuration expressed as a percentage obtained from the meter before test fluid flow;

V_1 is the light obscuration expressed as a percentage obtained from the meter during test fluid flow.

11 Expression of results

11.1 Individual results

Round the ignitability factor, RI , and the flame length index, RL , to the nearest integer, with values of exactly 0,5 being rounded up.

Round the smoke density, D , to the nearest 0,001.

Test results shall be expressed as numerical values of RI , RL and D .

11.2 Ranking system

The results may also be classified in terms of an alphabetical ranking scheme.

One suggested scheme given within [Annex D](#). This scheme may be modified as further test experience is obtained. In this scheme, the primary reference is the ignitability factor, RI , with flame length index, RL , and smoke density, D , being secondary factors.

The spray ignition characteristics may therefore be reported in the manner shown in [Table D.1](#), with letter categories corresponding to the numerical results obtained in the tests.

12 Precision

No precision is yet available for this method due to the small number of test rigs in regular use. Until this situation changes, each laboratory shall report RI values along with the results for ignitability for the calibration fluids given in [Table C.1](#).

13 Test report

The test report shall contain at least the following information:

- a) a reference to this document, i.e. ISO 15029-2;
- b) the type and complete identification of the product tested, including any dilution of concentrate, if appropriate;
- c) the result of the test (see [Clauses 11](#) and [12](#));
- d) the conditions under which each test run was carried out and any deviation, by agreement or otherwise, from the procedure specified;
- e) the date of the test.

Annex A (normative)

Verification of propane pressure and flow rate

A.1 Apparatus

A.1.1 Pressure gauge

A calibrated digital or analogue gauge, with a minimum range of 20 kPa to 500 kPa, and with an accuracy of ± 5 kPa or better over the range 200 kPa to 400 kPa.

A.1.2 Flowmeter

A calibrated flowmeter, or flowmeters, with a resolution of $0,005 \text{ Nm}^3/\text{h}$ or better over the range $0,1 \text{ Nm}^3/\text{h}$ to $0,5 \text{ Nm}^3/\text{h}$.

The procedure is intended to check the burner. Thus the circuit comprises the propane cylinder, a regulator, a valve and a flowmeter. The circuit used in the rig for carrying out the test should not be used.

A.2 Procedure

A.2.1 Measurement

At a distance of no more than 3 m from the propane burner, and at a point beyond which there are no restrictions or sharp bends in the supply line, insert the pressure gauge (A.1.1) and immediately downstream of it, the flowmeter (A.1.2). Supply propane from a source via a variable regulator until the pressure at the gauge is steady for at least 10 s. Read the pressure and flow under steady conditions. Increase the pressure and repeat the readings. Take pressure and flow readings, and at least four pressures between 40 kPa and 200 kPa.

A.2.2 Verification

Table A.1 gives the standard pressure/flow curve points for propane supply. Fit the readings obtained in accordance with A.2.1 on to this curve and compare the values. For satisfactory performance, the measured flow rate shall be within $\pm 0,01 \text{ Nm}^3/\text{h}$ of the corresponding point on the curve.

Table A.1 — Propane pressure and flow-rate calibration curve

Gauge pressure, MPa	40	50	70	100	150	200
Flow rate, Nm³/h	0,164	0,184	0,222	0,261	0,333	0,400


Annex B (normative)

Verification of propane flame characteristics

B.1 Apparatus

B.1.1 General

Figure B.1 illustrates a general view of the positioning of the thermocouple in the combustion chamber for temperature measurement of the burner flame. Measurements are carried out with the inner and outer cowlings in place, but with the front window of the combustion chamber fully open to allow access and adjustment to the traverse system.

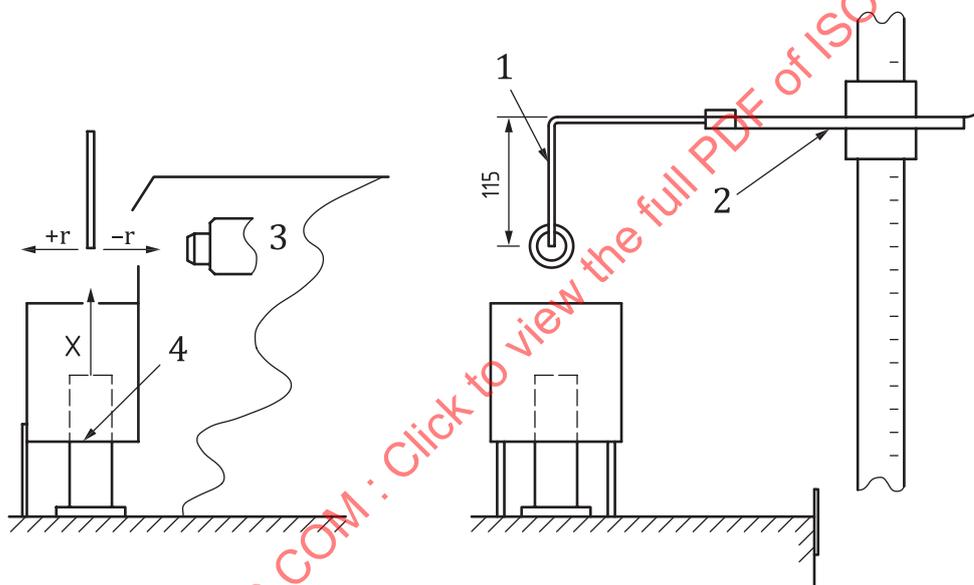

Key

- 1 K-type thermocouple
- 2 traversing system
- 3 atomiser
- 4 gas nozzle

Figure B.1 — General arrangement of flame temperature measurement

B.1.2 Temperature sensor

K-type 3 mm stainless steel sheathed thermocouple, bent through 90° at a distance of 115 mm ± 5 mm from the sensing tip.

B.1.3 Traverse system

A suitable stand and clamp shall hold the thermocouple with the 115 mm straight section aligned at ± 5° to the vertical. The stand shall have both vertical and horizontal linear scales for the measurement of the spatial position of the thermocouple tip.

B.1.4 Insulation board

A ceramic fibre insulating board, 7 mm \pm 1 mm in thickness and with a minimum size of 300 mm \times 300 mm, shall be fitted to the inner upper surface of the combustion chamber during testing. It shall be held in place by supports that do not interfere with the flame characteristics or the free movement of the thermocouple in the traverse system.

B.2 Flame temperature measurements

B.2.1 Axial temperatures

Adjust the propane flow rate to either the low (0,13 Nm³/h) or high (0,4 Nm³/h) rate and light the burner. Position the tip of the thermocouple at a distance of $x = 0$, corresponding to the exit orifice plane of the gas nozzle, and within ± 2 mm of the orifice centre line. Measure and record this temperature. Move the thermocouple upwards in the same vertical plane and repeat the temperature measurements at 10 mm intervals up to a distance of 200 mm above the nozzle. Repeat the procedure for the second propane flow rate.

B.2.2 Radial temperatures

Position the thermocouple at a distance of 143 mm \pm 1 mm above the gas nozzle exit orifice and traverse 40 mm in a horizontal plane towards the atomiser.

Light the burner, adjust the propane flow to either the low or the high rate, and measure and record the temperature.

Move the thermocouple horizontally away from the atomiser and repeat the temperature measurements at 5 mm intervals across the flame width until a position of 60 mm on the other side of the flame centre line is reached. Repeat the procedure for the second propane flow rate.

B.3 Verification

B.3.1 Standard values

[Tables B.1](#) and [B.2](#) give the standard values for axial and radial temperature measurements under the conditions of test. These are illustrated as curves in [Figures B.2](#) and [B.3](#). The distances in [Figure B.3](#) are measured from the burner with negative values towards the spray nozzle/atomiser.

B.3.2 Conformity values

B.3.2.1 Axial tests: the burner shall be deemed to conform to the standard burner if, at each measurement position, the measured temperature is within ± 50 °C of the standard temperature.

B.3.2.2 Radial tests: the burner shall be deemed to conform to the standard burner if, at each measurement position, the measured temperature is within ± 40 °C of the standard value, within the range -30 mm to 30 mm for the low propane flow rate, and -40 mm to 50 mm for the high propane flow rate.


Table B.1 — Propane burner temperature distribution

Distance from burner exit mm	Axial direction	
	Temperature at low propane flow rate °C	Temperature at high propane flow rate °C
0	861	550
10	869	568
20	871	567
30	874	580
40	872	611
50	864	629
60	866	675
70	861	718
80	860	762
90	858	817
100	852	852
110	862	880
120	870	905
130	884	927
140	890	938
150	891	946
160	904	960
170	901	971
180	888	977
190	875	980
200	854	988
210	802	994
220	796	996

Table B.2 — Propane burner temperature distribution


Distance from burner centre line mm	Radial direction	
	Temperature at low propane flow rate °C	Temperature at high propane flow rate °C
-40	88	310
-35	95	435
-30	125	540
-25	228	718
-20	430	820
-15	570	948
-10	800	975
-5	900	986
0	905	970
5	900	950
10	920	970
15	820	1 006
20	650	1 000
25	460	918
30	273	778
35	145	593
40	103	455
45	—	318
50	—	234
55	—	150
60	—	121

STANDARDSISO.COM : Click to view the full PDF of ISO 15029-2:2018

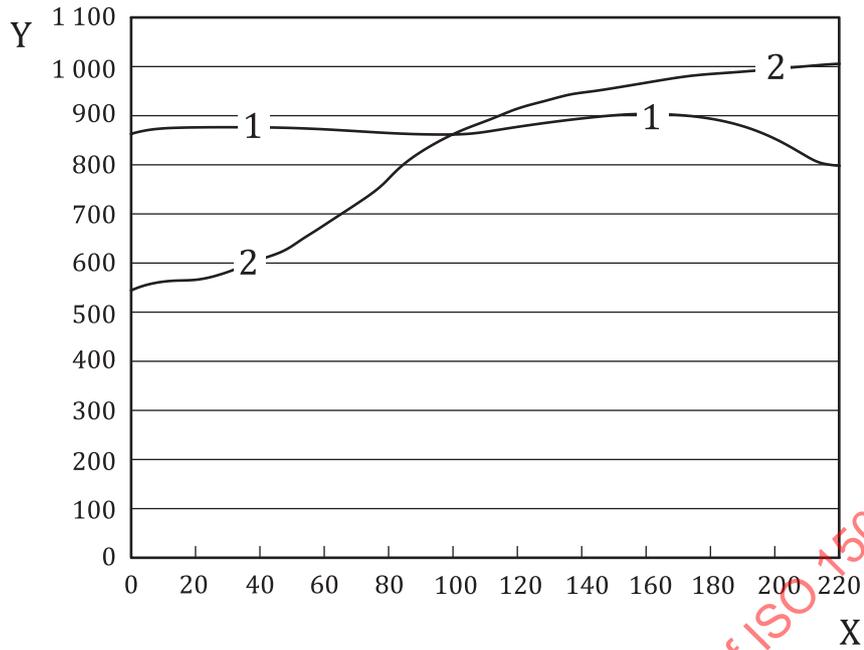

Key
 1 low propane flow
 2 high propane flow
 X distance, in mm
 Y temperature, in °C

Figure B.2 — Axial temperature distribution of propane flame

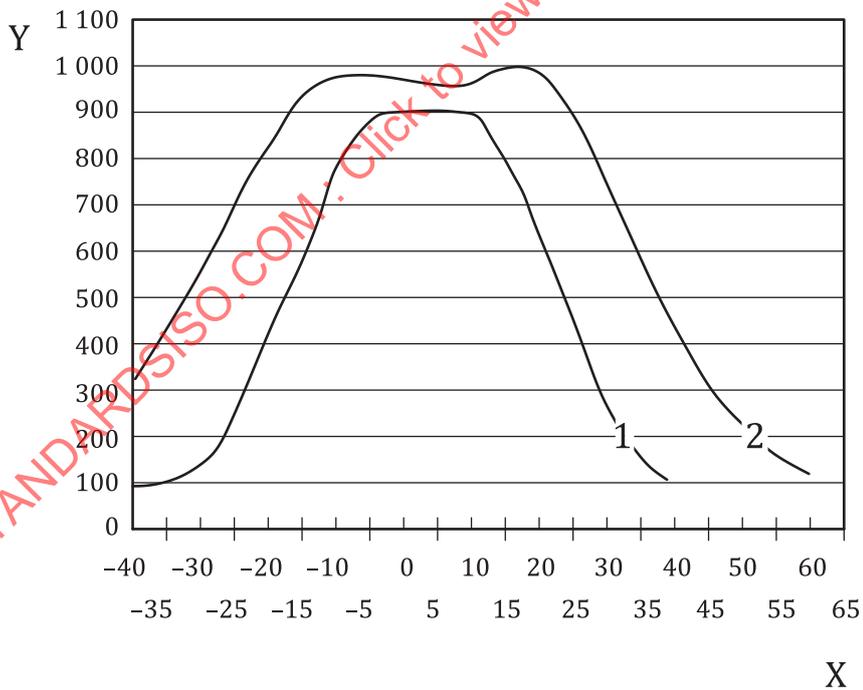

Key
 1 low propane flow
 2 high propane flow
 X distance towards atomiser, in mm
 Y temperature, in °C

Figure B.3 — Radial temperature distribution of propane flame

Annex C (normative)

Test apparatus calibration

C.1 Calibration fluids

Prepare a series of calibration fluids (CF₀ to CF₉₀) by volumetric mixing of mono ethylene glycol (5.5) with water (5.4).

Table C.1 gives the composition of this series. In Table C.1, % (V/V) is used to represent the volume fraction of a material.

Table C.1 — Calibration fluid composition and ignitability factor

Fluid designation	Ethylene glycol % (V/V)	Water % (V/V)	Standard ignitability factor
CF ₀	100	0	17,1
CF ₁₅	85	15	23,8
CF ₂₀	80	20	34,2
CF ₂₅	75	25	45,6
CF ₃₀	70	30	59,7
CF ₄₀	60	40	64,0
CF ₄₅	55	45	71,8
CF ₅₀	50	50	81,0
CF ₆₀	40	60	90,8
CF ₇₅	25	75	108,5
CF ₉₀	10	90	125,0

C.2 Testing

Carry out the procedure given in 9.1 at the low propane flow rate on fluids CF₀, CF₁₅, CF₂₀ and CF₂₅ and the procedure given in 9.2, at the high propane flow rate for the other fluids in the series, omitting the measurements of flame length and smoke density. Calculate the average uncorrected ignitability factor (RI_W or RI_X) on each fluid from a minimum of eight tests. Further tests shall be carried out if the accuracy does not conform to within 5 % of the mean value (see 9.5). Irrespective of the actual measured value of ignitability factor, do not re-test the fluids at the other propane flow rate. Table C.1 gives "standard" ignitability factor values for each calibration fluid.

C.3 Calibration

For the measured ignitability factors, RI_W for the low propane flow rate and RI_X for the high propane flow rate, solve the quadratic equations below to obtain coefficients a , b , c , d and e , using a 'least-squares' fit to obtain the mean values. Plot these mean values against the standard values given in Table C.1.

For low propane flow rate and $RI < 50$: $RI = aRI_W + bRI_W^2$

For high propane flow rate and $RI \geq 50$: $RI = c + dRI_X + eRI_X^2$