
**Hydraulic fluid power — Determination of
the fluid-borne noise characteristics of
components and systems —**

Part 3:
Measurement of hydraulic impedance

*Transmissions hydrauliques — Évaluation des caractéristiques du bruit
liquidien des composants et systèmes —*

Partie 3: Mesurage de l'impédance hydraulique

STANDARDSISO.COM : Click to view the full PDF of ISO 15086-3:2008



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 15086-3:2008



COPYRIGHT PROTECTED DOCUMENT

© ISO 2008

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword.....	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions.....	1
4 Symbols	3
5 Test conditions and accuracy of instrumentation	4
5.1 Test conditions (permissible variations).....	4
5.2 Instrumentation precision.....	4
6 Measurement of the impedance of a single-port passive component.....	5
6.1 Local impedance — Measurement principle.....	5
6.2 Hydraulic impedance.....	5
6.3 Factors influencing the accuracy of the impedance measurement	7
6.4 Measurement of local impedance	9
7 Measurement of the admittance matrix and impedance matrix of a two-port passive hydraulic component.....	13
7.1 Definitions and principles of measurement of the admittance matrix and impedance matrix of a two-port passive hydraulic component	13
8 Test report	22
8.1 General.....	22
8.2 General information.....	22
8.3 Test data	22
9 Identification statement (Reference to this part of ISO 15086)	23
Bibliography	24

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 15086-3 was prepared by Technical Committee ISO/TC 131, *Fluid power systems*, Subcommittee SC 8, *Product testing*.

ISO 15086 consists of the following parts, under the general title *Hydraulic fluid power — Determination of the fluid-borne noise characteristics of components and systems*:

- *Part 1: Introduction*
- *Part 2: Measurement of the speed of sound in a fluid in a pipe*
- *Part 3: Measurement of hydraulic impedance*

Introduction

In hydraulic fluid power systems, power is transmitted and controlled through a liquid under pressure within a closed circuit. During the process of converting mechanical power into fluid power, fluid-borne noise (flow fluctuations and pressure fluctuations) is generated, which in turn leads to structure-borne noise and airborne noise. The transmission of fluid-borne noise is influenced by the impedance of the components installed in the hydraulic circuit.

This part of ISO 15086 adopts the concepts of ISO 15086-1 which describe the basis for the methods of measurement that make it possible to determine the characteristics of fluid-borne noise emitted or transmitted by hydraulic transmission systems.

Clause 6 of this part of ISO 15086 describes the method for measuring the hydraulic impedance of a single-port component (local hydraulic impedance) and Clause 7 describes the method for measuring the hydraulic impedance matrix of a two-port hydraulic component.

STANDARDSISO.COM : Click to view the full PDF of ISO 15086-3:2008

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 15086-3:2008

Hydraulic fluid power — Determination of the fluid-borne noise characteristics of components and systems —

Part 3: Measurement of hydraulic impedance

1 Scope

This part of ISO 15086 describes the procedure for the determination of the impedance characteristics of hydraulic components, by means of measurements from pressure transducers mounted in a pipe.

This part of ISO 15086 is applicable to passive components, irrespective of size, operating under steady-state conditions, over a frequency range from 10 Hz to 3 kHz.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1000, *SI units and recommendations for the use of their multiples and of certain other units*

ISO 5598, *Fluid power systems and components — Vocabulary*

ISO 1219-1, *Fluid power systems and components — Graphic symbols and circuit diagrams — Part 1: Graphic symbols for conventional use and data-processing applications*

ISO 15086-1:2001, *Hydraulic fluid power — Determination of the fluid-borne noise characteristics of components and systems — Part 1: Introduction*

ISO 15086-2: 2000, *Hydraulic fluid power — Determination of the fluid-borne noise characteristics of components and systems — Part 2: Measurement of the speed of sound in a fluid in a pipe*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 5598 and the following apply.

3.1

flow ripple

fluctuating component of flow rate in hydraulic fluid

3.2

pressure ripple

fluctuating component of pressure in hydraulic fluid

3.3 wide-band pulse generator
hydraulic component generating a periodic flow ripple and consequently pressure ripple in a circuit, or an hydraulic component generating a pressure ripple and, consequently, a flow ripple in a circuit

3.4 fundamental frequency
lowest frequency of pressure ripple (or flow ripple) considered in a theoretical analysis or measured by an instrument

EXAMPLE An hydraulic pump or motor with a shaft frequency of N revolutions per second can be taken to have a fundamental frequency of N Hz. Alternatively, for a pump or motor with k displacement elements, the fundamental frequency can be taken to be Nk Hz, provided that the measured behaviour does not deviate significantly from cycle to cycle.

3.5 harmonic
sinusoidal component of a signal that occurs at an integer multiple of the fundamental frequency

NOTE An harmonic can be represented by its amplitude and phase, or by its real and imaginary parts.

3.6 impedance
ratio of the pressure ripple to the flow ripple occurring at a given point in a hydraulic system and at a given frequency

3.7 admittance
reciprocal of impedance

3.8 characteristic impedance
(of a pipeline) impedance of an infinitely long pipeline of constant cross-sectional area

3.9 hydro-acoustic energy
fluctuating part of the energy in a liquid

3.10 wide-band noise
hydro-acoustic energy distributed over the frequency spectrum

3.11 port-to-port symmetry
property of a two-port component in which the wave propagation characteristics remain the same when the port connections to the circuit are reversed

4 Symbols

The symbols used in this part of ISO 15086 are defined as shown in Table 1.

Table 1 — Symbols

Symbol	Description	Unit
A_e	Complex coefficient (term of admittance matrix between transducer PT3 and component 0)	$\text{m}^3 \cdot \text{s}^{-1} \cdot \text{Pa}^{-1}$
A_x	Complex coefficient (term of admittance matrix between transducers PT _x and PT3)	$\text{m}^3 \cdot \text{s}^{-1} \cdot \text{Pa}^{-1}$
A_{xy}	Terms of admittance matrix (for x and y equal to 1 or 2)	$\text{m}^3 \cdot \text{s}^{-1} \cdot \text{Pa}^{-1}$
B_e	Complex coefficient (term of admittance matrix between transducer PT3 and component 0)	$\text{m}^3 \cdot \text{s}^{-1} \cdot \text{Pa}^{-1}$
B_x	Complex coefficient (term of admittance matrix between transducers PT _x and PT3)	$\text{m}^3 \cdot \text{s}^{-1} \cdot \text{Pa}^{-1}$
c	Speed of sound in the fluid	$\text{m} \cdot \text{s}^{-1}$
f_{\min}	Minimum frequency	Hz
f_{\max}	Maximum frequency	Hz
H_{x3}	Transfer function between pressure ripples P_x and P_3	—
L	Distance between transducers	m
p_m	Mean test pressure	MPa
P_e	Fourier transform of pressure ripple at upstream port of component	Pa
P_s	Fourier transform of pressure ripple at downstream port of component	Pa
P_x	Fourier transform of pressure ripple at location x , where x is the number of the pressure transducer, equal to 1, 2 or 3, corresponding to PT1, PT2 or PT3, respectively	Pa
P_1, P_2 and P_3	Fourier transform of pressure ripple at the location of pressure transducer 1 (PT1), pressure transducer 2 (PT2) and pressure transducer 3 (PT3), respectively	Pa
$Q_{e \rightarrow 0}$	Fourier transform of flow ripple into upstream port of component (0)	$\text{m}^3 \cdot \text{s}^{-1}$
$Q_{s \rightarrow 0}$	Fourier transform of flow ripple into downstream port of component (0)	$\text{m}^3 \cdot \text{s}^{-1}$
x	Number of the pressure transducer, equal to 1, 2 or 3, corresponding to PT1, PT2 or PT3, respectively	—
Z_e	Impedance	
ν	Kinematic viscosity	cSt (1 cSt = $10^{-6} \cdot \text{m}^2 \cdot \text{s}^{-1}$)
θ	Phase of harmonic component (pressure or flow ripple, as appropriate)	degree (°)
$d\theta$	Phase precision of the Fourier analyser	degree (°)

Units used in this part of ISO 15086 are in accordance with ISO 1000.

Graphical symbols are in accordance with ISO 1219-1 unless otherwise stated.

5 Test conditions and accuracy of instrumentation

5.1 Test conditions (permissible variations)

5.1.1 General

The required operating conditions shall be maintained throughout each test within the limits specified in Table 2.

Table 2 — Permissible variations in test conditions

Test parameter	Permissible variation
Mean flow	± 2 %
Mean pressure	± 2 %
Temperature	± 2 °C

5.1.2 Fluid temperature

The temperature of the fluid shall be that measured at the measuring pipe inlet.

5.1.3 Fluid density and viscosity

The density and viscosity of the fluid shall be known to an accuracy within the limits specified in Table 3.

Table 3 — Required accuracy of fluid property data

Property	Required accuracy %
Density	± 2
Viscosity	± 5

5.1.4 Mean fluid pressure

The mean fluid pressure of the fluid shall be that measured at the measuring pipe inlet.

5.1.5 Mean flow measurement

The mean flow measurement shall be measured downstream of the measuring pipe (e.g. in cases where the mean flow influences the terms of the admittance or impedance matrix).

5.2 Instrumentation precision

5.2.1 Steady-state accuracy class

The accuracy required shall be in accordance with the values given in ISO 15086-1:2001, Annex A.

5.2.2 Dynamic-state accuracy class

The accuracy required shall be in accordance with the values given in ISO 15086-1:2001, Annex B.

6 Measurement of the impedance of a single-port passive component

6.1 Local impedance — Measurement principle

The hydraulic impedance, $Z_{e\rightarrow 0}$, of a component with a single-port connection is defined by Equation (1) and shown diagrammatically in Figure 1:

$$Z_{e\rightarrow 0} = \frac{P_e}{Q_{e\rightarrow 0}} \quad (1)$$


where

P_e is the Fourier transform of the pressure ripple at the component inlet;

$Q_{e\rightarrow 0}$ is the Fourier transform of the flow ripple entering the component and regarded as positive when entering the 0 component.

In the high-frequency ranges (> 10 Hz), no convenient systems exist to measure the flow $Q_{e\rightarrow 0}$.

To enable a pulsating flow to be inferred, this test method requires the use of a rigid hydraulic pipe fitted with dynamic pressure transducers having a sufficiently high bandwidth and with the distances between the transducers selected according to the frequency range of interest.

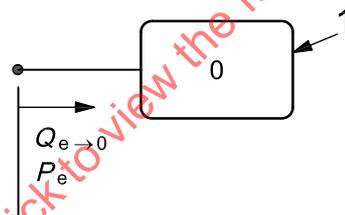

Key

1 component 0

Figure 1 — Key parameters in the measurement of impedance of a single-port component

6.2 Hydraulic impedance

6.2.1 Measurement principle


Figure 2 illustrates the principle for measuring the impedance, Z_e , at the inlet of the single-port component (0).

NOTE It is important to remember that a passive component is not itself a generator of hydro-acoustic energy.

Three dynamic pressure transducers (PT1 to PT3) are connected to the rigid pipe constituting the flow-ripple measuring pipe at transducer PT3.

It is assumed that appropriate technical measures have been taken to ensure that the speed of sound in the fluid between PT1 and PT3 is uniform. This requires that the mean temperature of the fluid in the measuring pipe be uniform to within 2 °C along its length.

The speed of the sound in the measuring pipes can be determined by means of the three pressure transducers, PT1 to PT3, in accordance with the algorithm described in ISO 15086-2.

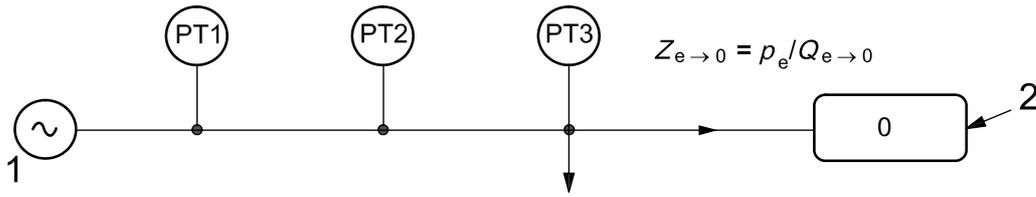

Key

- 1 pulse generator
- 2 component 0
- PT1, PT2, PT3 location of pressure transducers 1, 2 and 3, respectively

Figure 2 — Principle of measuring the impedance of a single port component

6.2.2 Simplified algorithm for determining the component of the local hydraulic impedance

The flow being determined at the upstream port of component (0) is $Q_{3 \rightarrow 0}$.

A_x and B_x are the elements of the admittance matrix describing the pipe between PT x and PT3 where x is 1 or 2 depending on the transducers selected to determine the flows.

A_e and B_e are the elements of the admittance matrix describing the pipe between the inlet of the single-port component (0) and PT3.

By referring to ISO 15086-1, which provides the basic definitions, the algebraic relationships shown in Equations (2) to (5) are obtained.

$$Q_{3 \rightarrow 0} = -Q_{3 \rightarrow x} = -(A_x P_3 + B_x P_x) \tag{2}$$

$$Q_{e \rightarrow 0} = -\frac{A_e Q_{3 \rightarrow 0}}{B_e} + (A_e^2 - B_e^2) P_3 \tag{3}$$

$$P_e = \frac{Q_{3 \rightarrow 0}}{B_e} - \frac{A_e P_3}{B_e} \tag{4}$$

$$Z_{e \rightarrow 0} = \frac{P_e}{Q_{e \rightarrow 0}} \tag{5}$$

$$= \frac{Q_{3 \rightarrow 0} A_e P_3}{(A_e^2 - B_e^2) P_3 - A_e Q_{3 \rightarrow 0}}$$

$$= \frac{-(A_x P_3 + B_x P_x) - A_e P_3}{(A_e^2 - B_e^2) P_3 + A_e (A_x P_3 + B_x P_x)}$$

Equation (6) for the measurement of the component hydraulic impedance, $Z_{e \rightarrow 0}$, is derived by dividing the numerator and the denominator of Equation (5) by P_3 :

$$Z_{e \rightarrow 0} = \frac{-A_x - A_e - B_x \frac{P_x}{P_3}}{A_e^2 - B_e^2 + A_e A_x + A_e B_x \frac{P_x}{P_3}} \tag{6}$$

where x is equal to 1 or 2 according to the frequency ranges being measured.

The transfer function, P_x/P_3 , can be directly measured by a suitable frequency-response analyser, but due account shall be taken of the pressure-transducer calibration (see 6.3.3).

6.3 Factors influencing the accuracy of the impedance measurement

6.3.1 General

The various factors influencing the accuracy of the impedance measurement and the precautions to take as a result are described in 6.3.2.

6.3.2 Pulse generator

It is necessary to have a device that is capable of producing a strong pressure ripple with a frequency and an amplitude stable over the required frequency range. Suitable devices are

- a) a piston pump or other pump with a broad-band pressure ripple,
- b) a specially designed rotary valve that produces regular flow ripples,
- c) an electrodynamic vibrator and actuator,
- d) a high-frequency response servovalve,
- e) a piezoelectric actuator.

Items c) to e) can be excited using a swept-sinusoid, a periodic broad-band waveform or a random signal.

6.3.3 Pressure transfer function measured by the PT_x/PT_3 pressure transducers and the calibration correction

An accurate measurement of the P_x/P_3 transfer function requires an initial calibration of the PT_x/PT_3 transducers.

Calibration shall be undertaken using the technique described in ISO 15086-2:2000, 8.5.

The transducers shall be calibrated under environmental conditions identical to those pertaining for the impedance measurement (e.g. the same mean fluid pressure and same fluid temperature).

Settings of the analyser during calibration shall be identical to those during the impedance measurements (e.g. the same measurement range, window shape, analysis band, signal averaging).

The coherence function obtained when measuring the transfer functions by means of the Fourier analyser is an excellent indication of the validity of the measurements when the signal-to-noise ratio of the transducers is adequate.

The pressure-excitation source level shall be such that the coherence function of the transfer functions measured is greater than 0,95. By averaging a sufficiently large number of spectra, it can be possible to improve the coherence for frequencies where the excitation is low.

The transfer-function measurements taken when measuring the impedances shall be corrected through the use of the calibration transfer functions (see ISO 15086-2:2000, 8.5).

6.3.4 Numerical value of terms A and B of the pipe section admittance matrix used for the indirect determination of the pulsed flows

6.3.4.1 General

The admittance matrix terms A and B depend on five factors:

- a) transducer spacing;
- b) measuring pipe internal diameter;
- c) speed of sound in the fluid in the measuring pipe;
- d) fluid kinematic viscosity;
- e) fluid density.

6.3.4.2 Transducer spacing

6.3.4.2.1 General

The distances between the transducers shall be suitable for the range of analysis frequencies selected and for the upper and lower limits of this analysis band. Generally, one single spacing value is inadequate for carrying out a measurement over a wide frequency range.

At high frequencies, the limitation is due to the fact that the analysis becomes indeterminate when the distance between transducers is equal to half of the wavelength of the pressure ripples.

At very low frequencies, the limitation is due to the fact that the amplitude ratio approaches unity and the phase shift between the transducers approaches zero. The analysis becomes inaccurate when the phase shift between the transducers is less than 10 times the accuracy of the analyser's phase measurement capability.

The distances between the transducers should be measured with an accuracy of ± 1 mm.

6.3.4.2.2 Practical rules for establishing the transducer spacing

Firstly, using Equation (7), determine the distance, L , for an upper frequency limit, f_{\max} , where L is the distance between the transducers selected to measure the impedance between PT1 and PT3 or between PT2 and PT3.

$$L \leq \frac{0,95 \cdot c}{2 \cdot f_{\max}} \tag{7}$$

EXAMPLE 1 Substituting $f_{\max} = 1\,600$ Hz and $c = 1\,300$ m s⁻¹ into Equation (7) gives

$$L \leq \frac{0,95 \cdot 1\,300 \text{ m} \cdot \text{s}^{-1}}{2 \cdot (1\,600 \text{ Hz})}$$

$$L \leq 0,386 \text{ m}$$

With the distance, L , established, the lower limit of the frequency measurement, f_{\min} , can be estimated using Equation (8):

$$f_{\min} = f_{\max} \cdot \frac{d\theta \cdot 10}{180} \tag{8}$$

EXAMPLE 2 If $d\theta$ of the analyser is $0,5^\circ$, then Equation (8) gives

$$f_{\min} = \frac{1600 \cdot (0,5) \cdot 10}{180} \approx 44 \text{ Hz}$$

Thus a spacing of 0,386 m allows the correct transfer function measurement in a frequency range between an f_{\min} equal to 44 Hz and an f_{\max} equal to 1 600 Hz.

The distance between transducer PT3 and the upstream port of component (0) shall be between 0,1 L and 0,2 L .

6.3.4.3 Speed of sound in the fluid in the measuring pipe

The speed of sound is used in the determination of the admittance matrix terms describing the measuring pipes.

This parameter depends on the temperature and mean pressure of the fluid flowing in the measuring pipes; these parameters shall, therefore, be set according to the desired test conditions and maintained within the limits specified in Table 2 during the measurements.

6.3.4.4 Density of the fluid circulating in the measuring pipes

The density is used in the determination of the admittance matrix terms describing the measuring pipes.

This parameter depends on the temperature and mean pressure of the fluid flowing in the measuring pipes; these parameters shall, therefore, be set according to the desired test conditions and maintained within the limits specified in Table 2 during the measurements.

6.4 Measurement of local impedance

6.4.1 Test circuit


6.4.1.1 Simplified circuit

A simplified test circuit suitable for measuring the hydraulic impedance of a single-port component is shown in Figure 3.

The test circuit is comprised of the following components:

- a) hydraulic pump and electric motor, to ensure that the mean flow and mean pressure of the component being tested are supplied; the pump shall be protected by means of a safety valve;
- b) connecting hose, to connect the pump outlet to the test circuit; if the pump generates a pressure-ripple level much greater than the pulse generator, it can be necessary to reduce the pressure-ripple level at the pump outlet by means of this hose or another attenuating system; otherwise, the pressure-ripple level of the pump can saturate the dynamic pressure transducers PT1 to PT3, or can prevent accurate measurement of the harmonics of the pressure ripple from the pulse generator (see 6.4.1.2);
- c) rigid pipe, in which the pressure transducers are mounted as shown in Figure 3, with the distance between the transducers suited to the band of frequencies used;
- d) three pressure transducers (PT1 to PT3) arranged on rigid pipes upstream and downstream of the component (preferably miniature flush-membrane-type piezoelectric transducers), used to determine the pressure ripple and flow ripple in the pipes and the speed of sound in the test fluid;
- e) pulse generator, capable of generating pulses in the selected frequency band with an adequate level to obtain the correct signal-to-noise ratio (see 6.3.2);

- f) adjustable restrictor, to allow adjustment of the mean pressure, p_m , downstream of the test circuit controlled by the pressure gauge;
- g) cooler (heat exchanger), to ensure temperature regulation of the test fluid controlled by the thermometer;
- h) optional mean flowmeter for use in case the mean flow rate in the component under test influences its hydro-acoustic characteristics;
- i) component under test;
- j) precision transducer or pressure gauge used to monitor the mean pressure during the test.

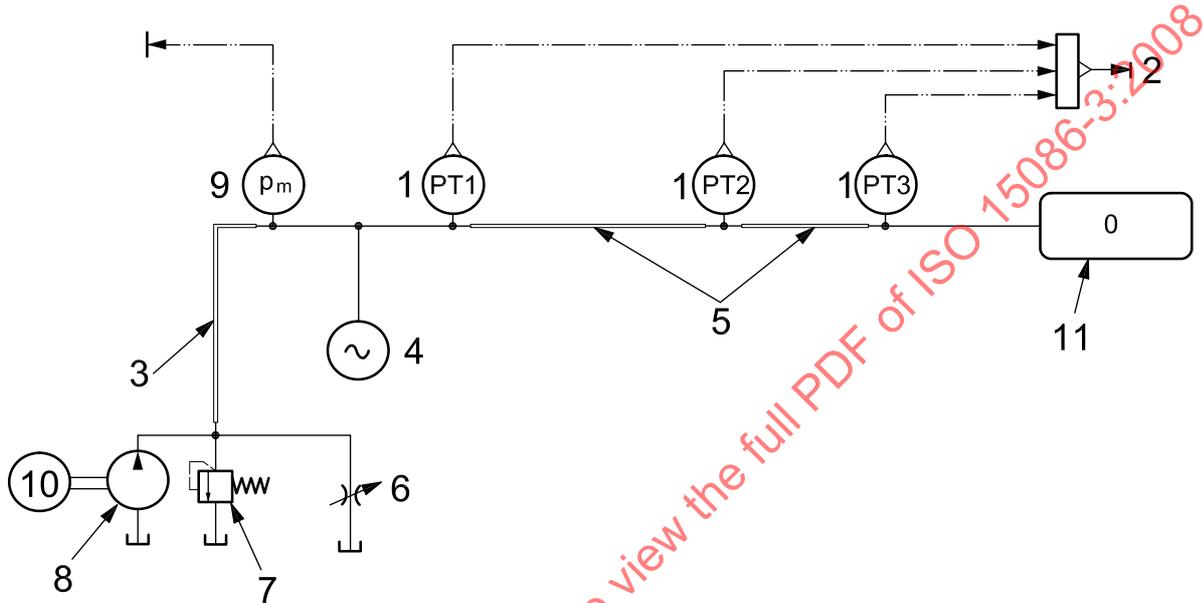

Key

- | | | | |
|---|---|----|---------------------|
| 1 | pressure transducers | 7 | relief valve |
| 2 | Fourier analyser | 8 | pump |
| 3 | flexible hose and small-diameter metal pipe | 9 | mean pressure gauge |
| 4 | pulse generator | 10 | electric motor |
| 5 | metal pipes of the same diameter | 11 | component 0 |
| 6 | adjustable restrictor | | |

Figure 3 — Simplified test circuit for measuring the impedance of a single port component

6.4.1.2 Isolation of pump pressure ripple

Transmission to the pressure transducers of the pressure ripple produced by the pump should be minimized. This can be achieved by using a flexible hose at least 1 m long, followed by a small-diameter rigid pipe, (typically 0,5 to 0,75 times the diameter of the tube), at least 1 m long.

6.4.2 Test procedure

6.4.2.1 Calibration of the miniature pressure transducers PT1 to PT3

Before taking the measurements, calibrate the pressure transducers (see ISO 15086-2:2000, 8.5) in order to obtain the calibration transfer functions.

6.4.2.2 Adjustment and preliminary operations prior to measuring the impedance

Before carrying out the calibration operation described in 6.4.2.1, steps 6.4.2.2 a) to e) shall be performed.

- a) Place the flush-mounted diaphragm pressure transducers in the measuring pipe.
- b) Purge the circuit.
- c) Adjust the mean test pressure, p_m , by means of the adjustable restrictor.
- d) Ensure that the excitation level of the pulse generator is adequate to obtain the correct transfer functions (acceptable coherence criterion $> 0,95$).
- e) If the pump generates a pressure ripple level much greater than the pulse generator, it can be necessary to reduce the pressure-ripple level at the pump outlet by means of a hose or other attenuating system. Otherwise, the pressure-ripple level of the pump can saturate the dynamic pressure transducers PT1 to PT3, or can prevent accurate measurement of the harmonics of the pressure ripple from the pulse generator.

6.4.2.3 Measurement procedure

For each mean pressure required, capture the inter-transducer transfer functions by signal averaging using a multi-channel analyser allowing the simultaneous acquisition of the output from the three pressure transducers and their transfer function relative to one of the other transducers.

6.4.2.4 Processing of measurements taken

6.4.2.4.1 Determination of the speed of sound in the measuring pipes

Determine the speed of sound in the fluid in accordance with the procedure described in ISO 15086-2, using the measurements from the three pressure transducers PT1 to PT3.

Use the value of the speed of sound, c , to determine the values of the terms A_x and B_x of the pipe sections between transducers PT1 and PT3 and between PT2 and PT3.

6.4.2.4.2 Determination of the impedance of the component connected to the measuring point PT3

Carry out the following using the procedure described in 6.3.

- a) Select the pairs of transducers (PT1 and PT3) or (PT2 and PT3) suitable for the analysis band at the selected frequency.
- b) Use the value of the speed of sound, c , as determined in 6.4.2.4.1 to calculate A_1 , B_1 or A_2 , B_2 and A_e , B_e in accordance with the relationships defined in ISO 15086-1:2001, 5.3.
- c) Calculate the transfer functions H_{13} and H_{23} , corrected according to the calibration transfer function.
- d) Calculate the inlet hydraulic impedance of the component (at the location of PT3) using Equation (9):

$$Z_{e \rightarrow 0} = \frac{-A_x - A_e - B_x H_{x3}}{A_e^2 - B_e^2 + A_e A_x + A_e B_x H_{x3}} \quad (9)$$

where x is either 1 or 2;


- e) Repeat steps a) through d) for all frequencies at which the impedance is determined.

6.4.2.5 Presentation of results

The hydraulic impedance measurements shall be presented in the form of curves as a function of frequency.

Because the impedance, Z_e , is a complex variable, it is necessary to describe this variable by its real and imaginary parts or by its amplitude and phase.

Examples of representative impedance curves are shown in Figure 4.

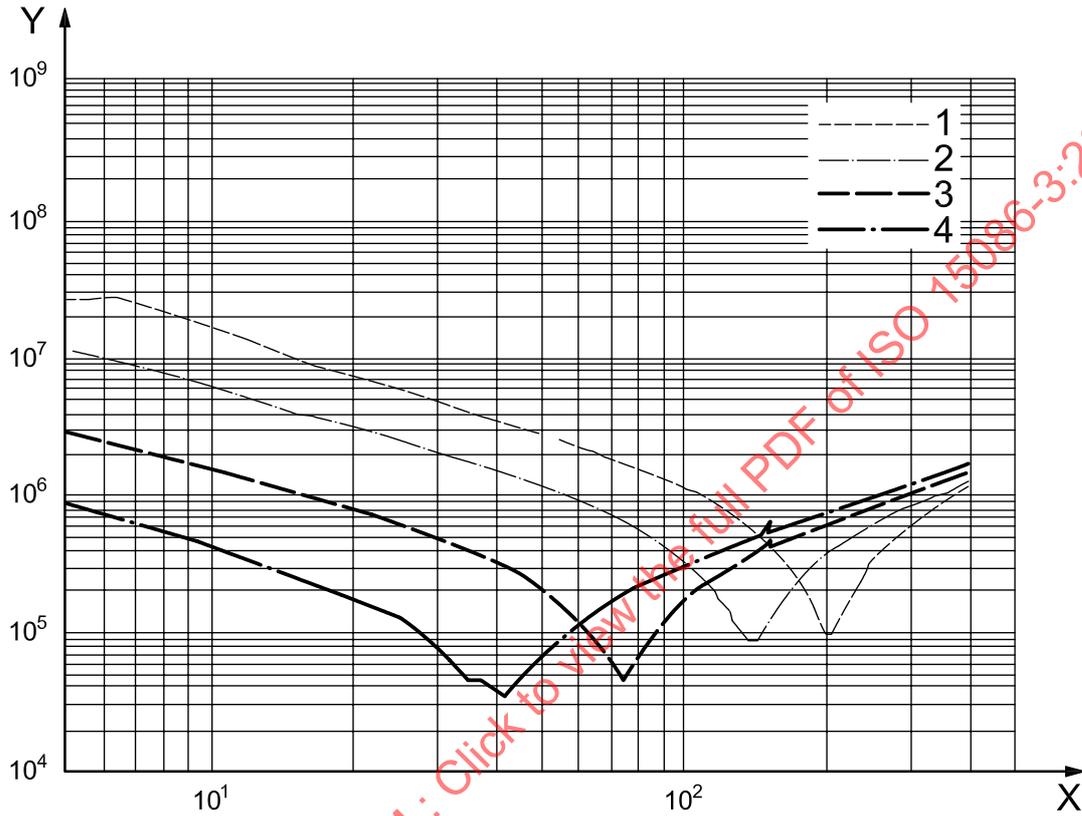


Key

- X frequency, expressed in hertz
- Y amplitude of complex impedance, Z_e , expressed in pascal-seconds per cubic metre (Pa s m^{-3})
- 1 curve for $p_m = 4 \text{ MPa}$ (40 bar)
- 2 curve for $p_m = 2 \text{ MPa}$ (20 bar)
- 3 curve for $p_m = 1 \text{ MPa}$ (10 bar)
- 4 curve for $p_m = 0,5 \text{ MPa}$ (5 bar)

a) Amplitude versus frequency

Figure 4 (continued)

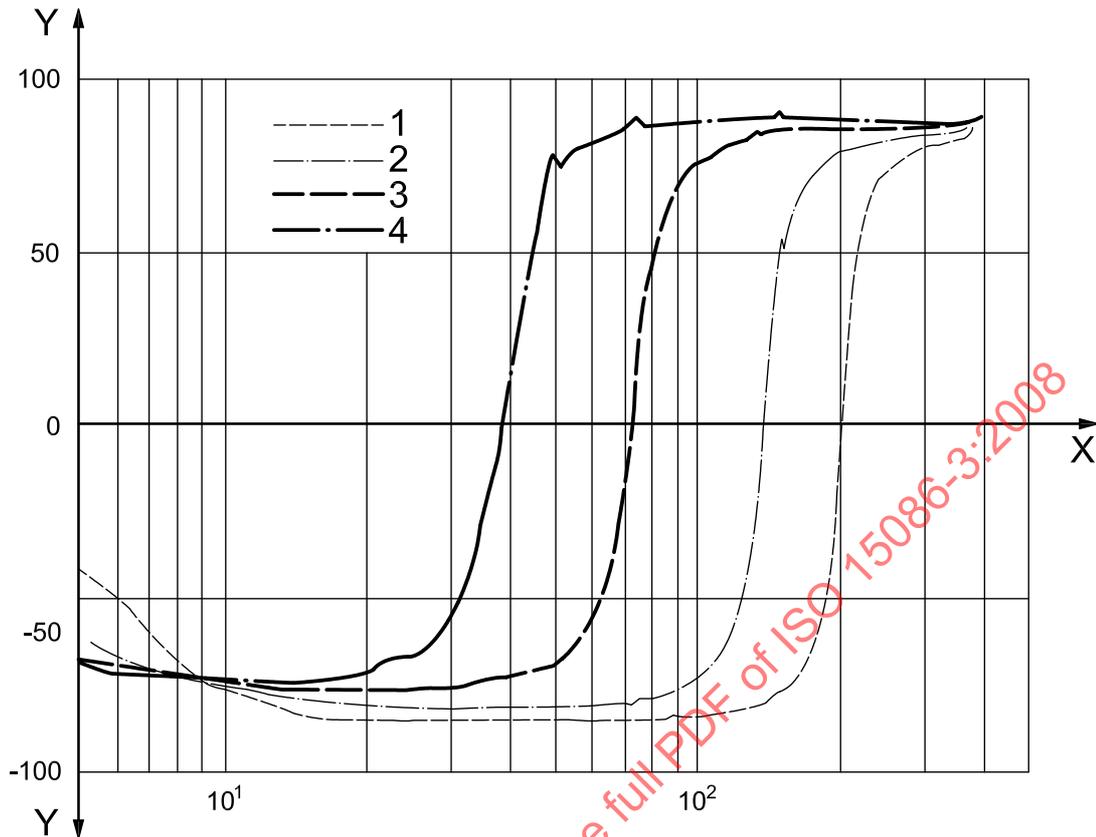**Key**

- X frequency, expressed in hertz
 Y phase of complex impedance, Z_e , expressed in degrees
 1 curve for $p_m = 4$ MPa (40 bar)
 2 curve for $p_m = 2$ MPa (20 bar)
 3 curve for $p_m = 1$ MPa (10 bar)
 4 curve for $p_m = 0,5$ MPa (5 bar)

b) Phase angle versus frequency

Figure 4 — Impedance of a hydraulic accumulator at four mean pressures


7 Measurement of the admittance matrix and impedance matrix of a two-port passive hydraulic component

7.1 Definitions and principles of measurement of the admittance matrix and impedance matrix of a two-port passive hydraulic component

7.1.1 General

Figure 5 is a schematic diagram of a two-port passive hydraulic connecting component with pressure ripples and flow ripples (P_1, Q_1) and (P_2, Q_2), respectively, at ports 1 and 2.

NOTE It is important to remember that a passive component is not itself a generator of hydro-acoustic energy.

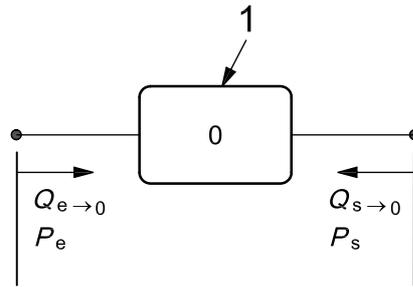

Key

- 1 component 0

Figure 5 — Key parameters for the measurement of admittance matrix and impedance matrix of a two port component

The hydraulic admittance matrix of the component as shown in Figure 5 can be written as shown in Equation (10):


$$\begin{bmatrix} Q_{1 \to 0} \\ Q_{2 \to 0} \end{bmatrix} = \begin{bmatrix} A_{11} & A_{12} \\ A_{21} & A_{22} \end{bmatrix} \cdot \begin{bmatrix} P_e \\ P_s \end{bmatrix} \tag{10}$$

where A_{xy} are the terms of the passive component hydraulic admittance matrix.

It should be remembered that the hydraulic admittance is the inverse of the hydraulic impedance.

7.1.2 Principle of the method of measuring the admittance matrix

The inlet and outlet of the component being measured are connected to pipes fitted with dynamic pressure transducers, making it possible to measure indirectly the pressure ripples P_e and P_s and the flow ripples $Q_{e \to 0}$ and $Q_{s \to 0}$ (see Figure 6).

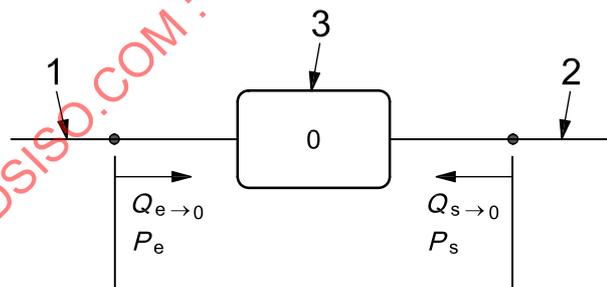


Key

- 1 pipe in which the pressure ripple, P_e , and the flow ripple, $Q_{e \to 0}$, are measured
- 2 pipe in which the pressure ripple, P_s , and the flow ripple, $Q_{s \to 0}$, are measured
- 3 component 0

Figure 6 — Principle of measuring the admittance matrix of a two port component

Measurement of the admittance matrix consists of determining the values of the matrix terms A_{11} , A_{12} , A_{21} and A_{22} of the hydraulic component under consideration.

Figure 7 shows a more detailed diagram of the test circuit.

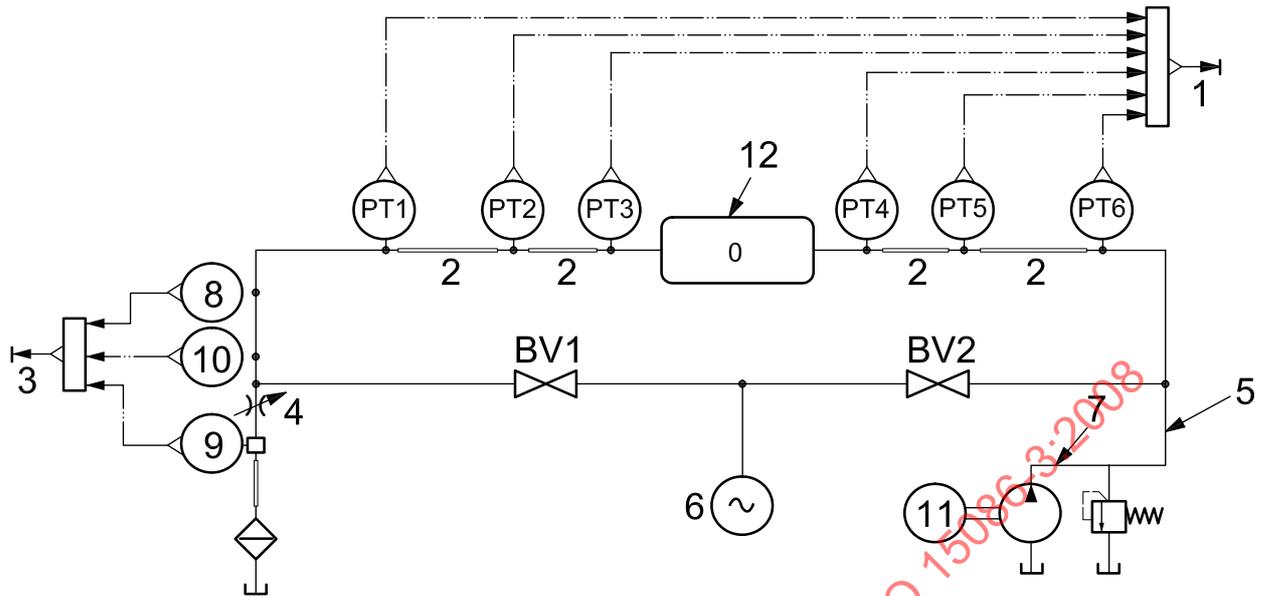

Key

1	Fourier analyser	8	pressure transducer to measure mean pressure
2	rigid pipes of the same diameter	9	flowmeter to measure mean flow
3	mean parameters	10	thermometer
4	adjustable restrictor	11	electric motor
5	small-diameter pipe	12	component 0
6	pulse generator	BV1, BV2	ball valves
7	flexible hose	PT1 to PT6	pressure transducers

Figure 7 — Circuit for transfer matrix measurement of a two port component

The main elements of the test circuit are the following.

- An hydraulic pump ensures that the mean flow and mean pressure of the component being tested are supplied. The pump shall be protected by means of a safety valve.
- A connecting hose connects the pump outlet to the test circuit. If the pump generates a pressure-ripple level much greater than the pulse generator, it can be necessary to reduce the pressure-ripple level at the pump outlet by means of a hose or other attenuating system. Otherwise, the pressure-ripple level of the pump can saturate the dynamic pressure transducers PT1 to PT6, or can prevent accurate measurement of the harmonics of the pressure ripple from the pulse generator.
- The two pairs of rigid pipes all have the identical internal diameter. The pressure transducers are mounted in these pipes, with the distance between the transducers suited to the band of frequencies used and, for each pair of pipes, the same distances between the transducers and the component.
- Six pressure transducers (PT1 to PT6) are arranged on rigid pipes upstream and downstream of the component (preferably miniature flush-membrane-type piezoelectric transducers) and used to determine the pressure ripple and flow ripple in the rigid pipes and the speed of sound in the test fluid.
- A pulse generator, which can be connected to either the upstream pipe or the downstream pipe by means of the isolating valves BV1 and BV2, shall be capable of generating pulses in the selected frequency band with an adequate level to obtain the correct signal-to-noise ratio.
- An adjustable restrictor allows the adjustment of the mean pressure, p_m , downstream of the test circuit controlled by the pressure gauge.

- g) A cooler (heat exchanger) ensures the regulation of the temperature, T_m , of the test fluid controlled by the thermometer.
- h) An optional mean flowmeter can be used in case the mean flow rate, q_m , in the component under test influences its hydro-acoustic characteristics.

Solution for the four terms A_{11} , A_{12} , A_{21} and A_{22} of the admittance matrix of the test component requires a system of at least four equations. This necessitates that tests be performed under two separate conditions. For test condition 1, the pulse generator is connected, by means of valves BV1 and BV2, upstream of the measuring pipes and for test condition 2 the pulse generator is connected, again by means of valves BV1 and BV2, downstream of the measuring pipes.

7.1.3 Algorithm for determining the admittance matrix of a two-port, passive component for identical dimensions of upstream and downstream pipes

The upstream and downstream pipes shall be of the same internal diameter and have identical distances between transducers suited to the frequency bands selected where


- a) L_{23} is the distance between PT2 and PT3,
- b) L_{13} is the distance between PT1 and PT3,
- c) L_{45} is the distance between PT4 and PT5,
- d) L_{46} is the distance between PT4 and PT6,
- e) L_{23} is equal to L_{45} ,
- f) L_{13} is equal to L_{46} .

The values of the distances L_{23} and L_{13} shall meet the requirements of 6.3.4.2 commensurate with the upper and lower limits of the analysis frequencies.

Determination of the speed of sound in the fluid is necessary to calculate the values of the terms of the admittance matrix A and B of the measuring pipes.

The three upstream transducers PT1, PT2 and PT3 or PT4, PT5 and PT6 allow a determination of the speed of sound in the fluid upstream and downstream of the component in accordance with the requirements of ISO 15086-2.

On the basis of the two different test conditions illustrated in Figure 8, the algorithm for resolving the equation system in 7.1.3.2 c) makes it possible to calculate the admittance matrix terms of the test component.

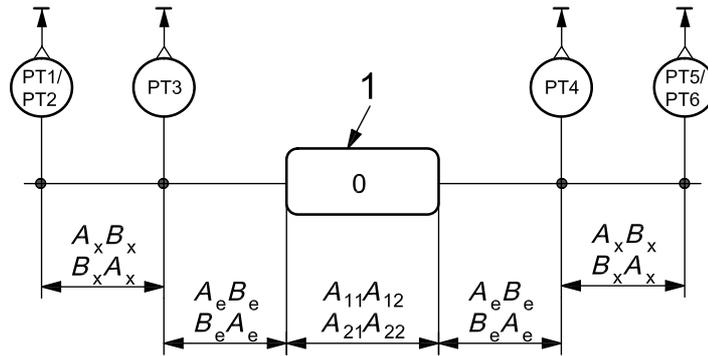
Key

- 1 component for which the matrix is being determined
 PT1 to PT6 positions for pressure transducers 1 to 6, respectively, test condition 1

Figure 8 — Key parameters for the two test conditions
7.1.3.1 Determination of the speed of sound in the measuring pipes

Determine the speed of sound in the fluid in the upstream line in accordance with the procedure described in ISO 15086-2, using the measurements from the three pressure transducers PT1 to PT3. Also use the same procedure to determine the speed of sound in the downstream line using the measurements from the three pressure transducers PT4 to PT6.

Determine the mean speed of sound as the mean of the speeds of sound in the upstream and downstream lines.

7.1.3.2 Determination of the admittance matrix of the component

- Select the pairs of transducers (PT1 and PT3, PT4 and PT 6) or (PT2 and PT3, PT4 and PT5) suitable for the analysis band at the selected frequency.
- Use the value of the mean speed of sound as determined in 7.1.3.1 to determine the values of the terms A_1 , B_1 or A_2 , B_2 and A_e , B_e according to the relationships defined in ISO 15086-1:2001, 5.3.
- Calculate the temporary variables X , Y and Z for test condition 1 as given in Equations (11) to (13) and the temporary variables X' , Y' and Z' for test condition 2 according to Equations (14) to (16) for either $x = 1$ and $y = 6$, or $x = 2$ and $y = 5$:

$$X = \frac{Q_{e \rightarrow 0}}{P_e} = - \left[\frac{(A_e^2 - B_e^2 + A_e A_x) + A_e B_x H_{x3}}{A_x + A_e + B_x H_{x3}} \right] \quad (11)$$

where

$Q_{e \rightarrow 0}$ is the ripple flow rate entering the inlet port of the component for test condition 1;

P_e is the pressure ripple at the inlet port of the component for test condition 1;

$$H_{x3} = \frac{P_x}{P_3}$$

where P_x and P_3 are the pressure ripples present in the upstream measuring pipe for test condition 1.

$$Y = \frac{Q_{s \rightarrow 0}}{P_e} = - \left[\frac{(A_e^2 - B_e^2 + A_e A_x) H_{43} + A_e B_x H_{y3}}{(A_x + A_e) H_{43} + B_x H_{x3}} \right] \quad (12)$$

where

$Q_{s \rightarrow 0}$ is the flow ripple entering the outlet port of the component for test condition 1;

$$H_{43} = \frac{P_4}{P_3}$$

where P_4 is the pressure ripple present in the downstream measuring pipe for test condition 1;

$$H_{y3} = \frac{P_y}{P_3}$$

where P_y is the pressure ripple present in the downstream measuring pipe for test condition 1.

$$Z = \frac{P_s}{P_e} = - \left[\frac{(A_x + A_e) H_{43} + B_x H_{y3}}{A_x + A_e + B_x H_{x3}} \right] \quad (13)$$

where

P_s is the pressure ripple at the outlet port of the component for test condition 1,

NOTE In Figure 7, for test condition 1, BV1 is open and BV2 is closed.

$$X' = \frac{Q'_{e \rightarrow 0}}{P'_e} = - \left[\frac{(A_e^2 - B_e^2 + A_e A_x) + A_e B_x H'_{x3}}{A_x + A_e + B_x H'_{x3}} \right] \quad (14)$$

where

$Q'_{e \rightarrow 0}$ is the flow ripple entering the inlet port of the component for test condition 2;

P'_e is the pressure ripple at the inlet port of the component for test condition 2;

$$H'_{x3} = \frac{P'_x}{P'_3}$$

where P'_x and P'_3 are the pressure ripples present in the upstream and downstream measuring pipes, respectively, for test condition 2.

$$Y' = \frac{Q'_{s \rightarrow 0}}{P'_e} = - \left[\frac{(A_e^2 - B_e^2 + A_e A_x) H'_{43} + A_e B_x H'_{y3}}{(A_x + A_e) H'_{43} + B_x H'_{x3}} \right] \quad (15)$$

where

$Q'_{s \rightarrow 0}$ is the ripple flow rate entering the outlet port of the component for test condition 2;

$$H'_{43} = \frac{P'_4}{P'_3}$$

where P'_3 and P'_4 are the pressure ripples present in the upstream and downstream measuring pipes, respectively, for test condition 2;

$$H'_{y3} = \frac{P'_y}{P'_3}$$

where P'_y is the pressure ripple present in the downstream measuring pipe for test condition 2.

$$Z' = \frac{P'_s}{P'_e} = - \left[\frac{(A_x + A_e)H'_{43} + B_x H'_{y3}}{A_x + A_e + B_x H'_{x3}} \right] \quad (16)$$

where

P'_s is the pressure ripple at the outlet port of the component for test condition 2.

NOTE In Figure 7, for test condition 2, BV1 is closed and BV2 is open.

d) Calculate the terms of the admittance matrices as given in Equations (17) to (20).

$$A_{11} = \frac{XZ' + X'Z}{Z - Z'} \quad (17)$$

$$A_{12} = \frac{X - X'}{Z - Z'} \quad (18)$$

$$A_{21} = \frac{YZ' + YZ'}{Z - Z'} \quad (19)$$

$$A_{22} = \frac{Y - Y'}{Z - Z'} \quad (20)$$

e) Repeat steps a) through d) for all frequencies at which the impedance is determined.

7.1.4 Measurement result presentation

7.1.4.1 Admittance matrices

The terms A_{11} , A_{12} , A_{21} and A_{22} are complex variables and are therefore represented as a real and imaginary part or amplitude and phase.

An example of a representative curve of the terms of a rigid piping matrix is shown in Figure 9.