
**Surface active agents —
Determination of polyethylene glycol
content in nonionic ethoxylated
surfactants — HPLC method**

Agents de surface tensioactifs — Dosage de la teneur en polyéthylène glycol dans les surfactants éthoxylés non ioniques — Méthode par CLHP

STANDARDSISO.COM : Click to view the full PDF of ISO 16560:2015



STANDARDSISO.COM : Click to view the full PDF of ISO 16560:2015



COPYRIGHT PROTECTED DOCUMENT

© ISO 2015

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
5 Reagents	1
6 Apparatus	2
7 Sampling	2
7.1 Preparation of the test sample.....	2
7.2 Preparation of test solutions.....	2
8 Procedure	3
8.1 Apparatus settings.....	3
8.2 Calibration.....	3
8.2.1 Preparation of calibration solutions.....	3
8.2.2 Calibration curve.....	4
8.3 Determination.....	4
9 Expression of results	5
10 Precision	5
10.1 Repeatability.....	5
10.2 Reproducibility.....	5
11 Test report	5
Annex A (informative) Results of interlaboratory tests for fatty alcohol ethoxylate	6

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT), see the following URL: [Foreword — Supplementary information](#).

The committee responsible for this document is ISO/TC 91, *Surface active agents*.

Introduction

This International Standard was developed based on EN 12582.

STANDARDSISO.COM : Click to view the full PDF of ISO 16560:2015

STANDARDSISO.COM : Click to view the full PDF of ISO 16560:2015

Surface active agents — Determination of polyethylene glycol content in nonionic ethoxylated surfactants — HPLC method

1 Scope

This International Standard specifies a method for the determination of the polyethylene glycol (PEG) content in aromatic and aliphatic non-ionic surface active agents of the type $R-(O-C_2H_4)_n OH$; where n is the mean ethylene oxide (EO) value. It is applicable to all ethoxylated products soluble in methanol or methanol/water mixture. This method applies to PEG concentrations as mass fraction greater than or equal to 0,1 %. This International Standard is not applicable to PEG whose molar mass is lower than 400 g/mol. Monomeric ethylene glycol, diethylene glycol, triethylene glycol, and glycerol are not detected.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 607, *Surface active agents and detergents — Methods of sample division*

ISO 5725-2, *Accuracy (trueness and precision) measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

polyethylene glycol content

amount of polyethylene glycol, expressed as a percentage by mass, calculated from the calibration curve in accordance with this International Standard

4 Principle

Polyethylene glycol is separated from the polyethoxylated surface active agents by means of reversed phase liquid chromatography. In this process PEG is eluted in the first minutes while the non-ionic surface active agents are retarded. Evaporative light scattering detector (ELSD) or charged aerosol detector (CAD) does not detect volatile materials such as the sample solvent; interferences with the PEG peak are limited. The sample is dissolved in an 80/20 (V/V) mixture of methanol/water or in another methanol/water mixture to obtain a clear solution. A portion of the sample solution is then analysed by high performance liquid chromatography (HPLC). Quantification of PEG content is achieved by external calibration with PEG molar mass equal to 1 000 g/mol.

5 Reagents

During the analysis, use only reagents of recognized analytical grade and the water used shall conform to grade 3 in accordance with ISO 3696.

5.1 Polyethylene glycol, with molar mass of 1 000 g/mol, gel permeation chromatography (GPC) grade.

ISO 16560:2015(E)

5.2 **Methanol**, HPLC grade, filtered before use with filter unit (6.5).

5.3 **Water**, HPLC grade, filtered before use with filter unit (6.5).

5.4 **Helium gas**, chromatography grade, for degassing eluent.

5.5 **Nitrogen or air**, dry, and without dust.

5.6 **Mobile phase**, either of the following:

- a) 80/20 (V/V) mixture of methanol and water;
- b) methanol.

6 Apparatus

Ordinary laboratory apparatus and glassware with the following.

6.1 **HPLC unit**, equipped with gradient pump.

6.2 **Evaporative light scattering detector (ELSD), or charged aerosol detector (CAD).**

6.3 **Chromatography column**, octadecyl C18 bonded phase silica gel; 5 µm; 250 mm length and 4,6 mm internal diameter.

6.4 **Data logger/plotter**, capable of recording and displaying the chromatographic peak area.

6.5 **Filter unit**, for solvent (0,45 µm).

7 Sampling

7.1 Preparation of the test sample

Prepare and store the test sample in accordance with ISO 607.

7.2 Preparation of test solutions

Weigh, to the nearest 0,1 mg, the test sample mass given in [Table 1](#) for the expected PEG content into a 100 ml volumetric flask. Fill to the mark with the mobile phase [[5.6 a](#)] or other suitable mixture of methanol/water and dissolve to obtain a clear solution. If necessary, filter through 0,45 µm filter unit.

Table 1

Expected PEG content, %	Sample mass, g ^a
<0,1	>1
0,1 to 2	1
2 to 5	0,5
5 to 10	0,25
10 to 25	0,1
^a Sample mass can be adjusted depending on the detector sensitivity.	

8 Procedure

8.1 Apparatus settings

Set the HPLC unit according to the following conditions.

8.1.1 Gradient

- a) t = 0 min 0 % methanol [5.6 b]);
- b) t = 6 min 0 % methanol [5.6 b]);
- c) t = 7 min 100 % methanol [5.6 b]);
- d) t = 30 min 100 % methanol [5.6 b]);
- e) t = 35 min 0 % methanol [5.6 b)].

NOTE Going from mobile phase [5.6 a)] to mobile phase [5.6 b)] is done in order to elute the ethoxylated products more rapidly.

8.1.2 Flow rate: 1,0 ml/min.

8.1.3 Temperature: room temperature.

8.1.4 Injection volume: 20 µl.

8.1.5 Detector: evaporative light scattering detector (ELSD), or charged aerosol detector (CAD).

Optimize the working conditions, depending on the apparatus in use and the physical parameters.

8.2 Calibration

8.2.1 Preparation of calibration solutions

Weigh, to the nearest 0,1 mg, 0,1 g of polyethylene glycol (PEG 1 000) (5.1) into a 100 ml volumetric flask, dissolve with the mobile phase [5.6 a)] and make up to the mark. Quantitatively transfer 1,0 ml, 5,0 ml, 10 ml, 25 ml of this solution each into 100 ml volumetric flasks and make up to the volume with the mobile phase. The concentrations of PEG in these solutions respectively are 0,01 g/l, 0,05 g/l, 0,1 g/l, 0,25 g/l. Mix the solution thoroughly. If necessary, filter through a 0,45 µm filter unit.

NOTE Mass of polyethylene glycol can be adjusted depending on the detector sensitivity.

8.2.2 Calibration curve

Analyse, at least twice, calibration solutions prepared in 8.2.1, in accordance with the chromatographic conditions given in 8.1. Construct a graph: log of peak area (y-axis) versus log PEG weight in 100 ml (x-axis) and draw a calibration curve.

NOTE For ELSD, calibration curves give similar results when molar masses of PEG are less than or equal to 4 000, and curve shift is observed when the molar mass of PEG is greater than 4 000. For CAD, calibration curves give similar results when molar masses of PEG are less than or equal to 10 000, and curve shift is observed when the molar mass of PEG is greater than 10 000.

8.3 Determination

Take the test solution as prepared in 7.2 and carry out the analysis in accordance with the chromatographic conditions given in 8.1. Typical chromatograms are shown in Figure 1 and Figure 2.

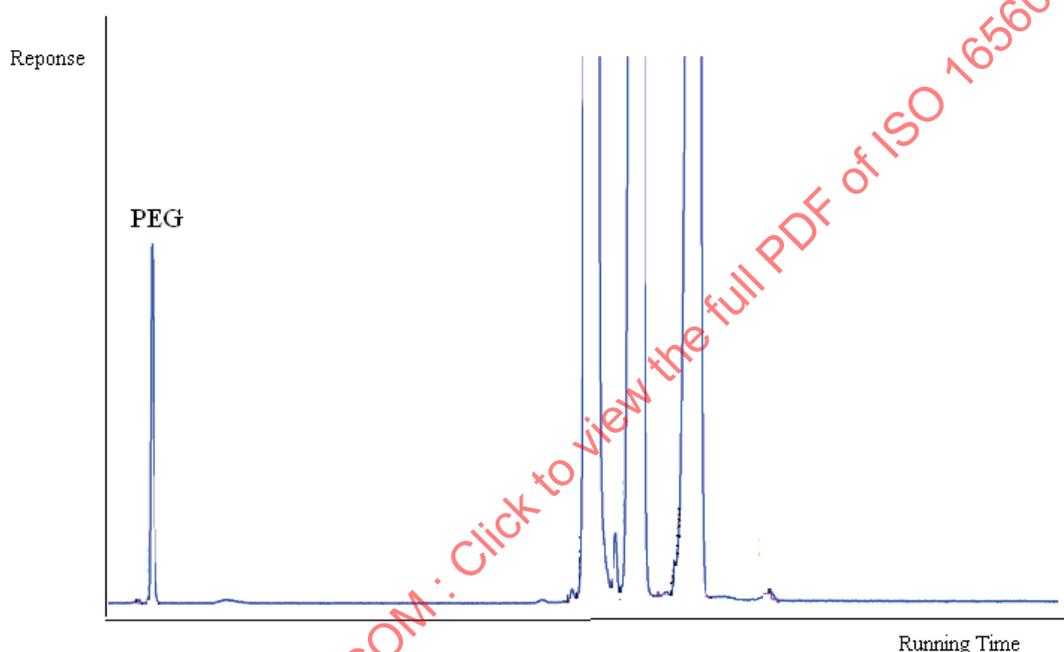


Figure 1 — Chromatogram of fatty alcohol ethoxylate (near 3 EO) by ELSD

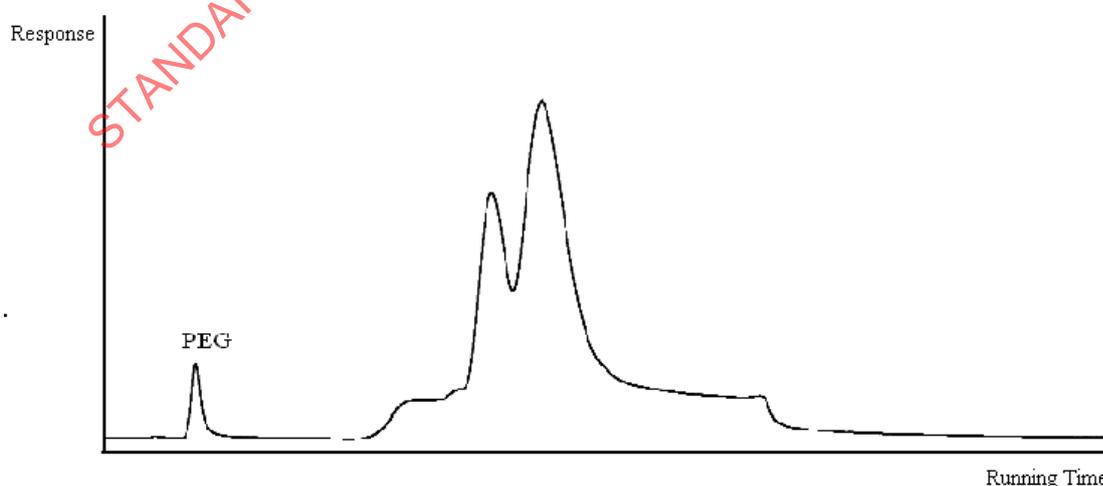


Figure 2 — Chromatogram of fatty alcohol ethoxylate (near 25EO) by CAD

NOTE In this reversed phase HPLC method, polyethylene glycol elutes quickly in the first minutes, in only one peak. When the molar mass distribution of PEG is large, it is possible to observe several peaks or shoulders corresponding to different molar masses of PEG. Sum the peak areas of the chromatogram corresponding to PEG.

9 Expression of results

Use the calibration curve in [8.2.2](#) to obtain the PEG mass corresponding to the area given by the integrator. Express the PEG content as mass fraction in percent as follows:

$$\text{PEG, \%} = \frac{m \times 100}{m_0} \quad (1)$$

where

m_0 is the mass of sample to be analysed ([7.2](#)), in grams;

m is the mass of PEG determined by means of the calibration curve, in grams.

10 Precision

10.1 Repeatability

The absolute difference between the results of two determinations carried out simultaneously or in rapid succession by the same operator on the same sample using the same equipment according to ISO 5725-2 shall not be greater than 0,2 % with a probability of 95 %.

Results of an interlaboratory test carried out in accordance with ISO 5725-2 are given in [Annex A](#).

10.2 Reproducibility

The absolute difference between two results obtained in different laboratories on the same sample according to ISO 5725-2 shall not be greater than 0,8 % with a probability of 95 %.

Results of an interlaboratory test carried out in accordance with ISO 5725-2 are given in [Annex A](#).

11 Test report

The test report shall include the following information:

- a) all information necessary for the complete identification of the sample;
- b) a reference to this International Standard, i.e. ISO 16560;
- c) the results with their units (see [Clause 9](#));
- d) room temperature for each liquid chromatographic determination and all information about ELSD or CAD;
- e) details of any operations not specified in this International Standard or in the International Standards to which reference is made, and any operations regarded as optional, as well as any incidents likely to have affected the results.