
**Fine ceramics (advanced ceramics,
advanced technical ceramics) —
Thermophysical properties of ceramic
composites — Determination of
thermal expansion**

*Céramiques techniques — Propriétés thermophysiques des composites
céramiques — Détermination de la dilatation thermique*

STANDARDSISO.COM : Click to view the full PDF of ISO 17139:2014



STANDARDSISO.COM : Click to view the full PDF of ISO 17139:2014



COPYRIGHT PROTECTED DOCUMENT

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	2
4.1 General.....	2
4.2 Direct measurement.....	2
4.3 Differential method.....	2
5 Apparatus	2
5.1 Construction materials.....	2
5.2 Heating and cooling device.....	2
5.3 Temperature measurement.....	2
5.4 Test piece mounting.....	2
5.5 System for measuring and recording the thermal expansion.....	3
5.6 Test piece measurement.....	3
6 Specimens	3
6.1 Test pieces.....	3
6.2 Reference pieces.....	3
6.3 Dimensions.....	3
7 Procedure	4
8 Calculations	5
8.1 Direct measurement.....	5
8.2 Differential method.....	5
9 Test report	6
Annex A (normative) Direct measurement apparatus	9
Annex B (normative) Differential type measurement apparatus	11
Bibliography	12

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 206, *Fine ceramics*.

Fine ceramics (advanced ceramics, advanced technical ceramics) — Thermophysical properties of ceramic composites — Determination of thermal expansion

1 Scope

This International Standard describes methods for the determination of linear thermal expansion characteristics of ceramic matrix composite materials up to 2 300 K, and is applicable to 1D, 2D, and nD materials.

The method describes general principles of construction, calibration, and operation of the equipment.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

IEC 60584-1, *Thermocouples — Part 1: Reference tables*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

linear thermal expansion

positive or negative change in one dimension that occurs when a material is subjected to a change in temperature

3.2

linear thermal expansion coefficient at temperature T

derivative of the length L with respect to temperature at the temperature T , divided by the length at temperature T

$$\alpha_T = \frac{1}{L} \left(\frac{dL}{dT} \right)$$

3.3

mean linear thermal expansion coefficient between temperatures T_1 and T_2

linear thermal expansion between temperatures T_1 and T_2 divided by the temperature increment T_1 to T_2 and the length at temperature T_1

$$\alpha(T_1, T_2) = \frac{L(T_2) - L(T_1)}{L(T_1)} \times \frac{1}{(T_2 - T_1)}$$

3.4

representative volume element

RVE

minimum volume which is representative of the material considered

4 Principle

4.1 General

A test piece is heated and subsequently cooled, either at a specified uniform rate or using defined temperature increments. Its change of length and its temperature are measured continuously, or at regular frequent intervals during the imposed temperature cycle.

One of two methods can be used to determine the linear thermal expansion coefficient, either by direct measurement or by a differential method.

4.2 Direct measurement

In this method, the variation in length of the test piece is measured directly. It is necessary to know the change in dimensions of the test piece support system by previous calibration.

The test piece is placed in a specimen holder and is made to contact a displacement transducer by using a push rod, made of the same material as the holder. This assembly is put in a furnace. The differential expansion between the test piece and the test piece holder is measured during the increase and the decrease in temperature.

The apparatus is shown in [Figure 1](#).

4.3 Differential method

This method consists of measuring the changes in length between a reference piece ([6.2](#)) and the test piece. It is not therefore necessary to know the change in dimensions of the test piece support system.

The apparatus is shown in [Figure 2](#).

5 Apparatus

5.1 Construction materials

The test piece holder and the push rod shall be made from thermomechanically stable materials of the same type, which shall be chemically inert and thermally compatible with the test piece material under the environmental conditions of the test.

NOTE For temperatures above 1 400 °C, it is necessary to employ a vacuum or inert gas atmosphere, with a non-oxide material appropriate for the test environment, such as a grade of dense graphite.

5.2 Heating and cooling device

Furnace, capable of working in a controlled atmosphere when required, and of controlling the temperature of the test piece to within 1 % of its mean temperature, expressed in K.

5.3 Temperature measurement

Thermocouples, in accordance with IEC 60584-1, subject to the upper temperature requirements and environmental consideration, except for tungsten-rhenium couples which may be used at higher temperatures but are not covered by IEC 60584-1, should be individually calibrated. For temperature in excess of 2 000 K, infrared detectors or any suitable device may be used.

5.4 Test piece mounting

The device used shall allow free axial movement of the test piece and of the reference piece in case of differential measurement. The mechanical environment shall minimize stresses. For vertical

measurement apparatus, the test pieces shall be free standing and mechanically stable on the end-plate. For measuring apparatus which is horizontal or inclined to the horizontal, the sideways movement or twist of the test piece shall be restricted, without any restriction of axial movement, by a suitable arrangement.

5.5 System for measuring and recording the thermal expansion

System, capable of measuring displacements to an accuracy better than 0,1 μm . The system shall allow recording of the test piece temperature and the displacement simultaneously. The system for measuring of displacements shall be periodically calibrated in accordance with [Annex A](#) for direct measurement or [Annex B](#) for differential measurement.

5.6 Test piece measurement

Device for measuring the test piece dimensions, with an accuracy better than 0,05 mm (e.g. micrometer in accordance with ISO 3611 or callipers in accordance with ISO 6906).

6 Specimens

6.1 Test pieces

The dimensions of the test pieces depend on the type of apparatus used. For differential measurements, the test piece and the reference piece ([6.2](#)) shall have the same length L_0 (see [Table 1](#)).

The test piece shall be cut in such a way that the axis of desired measurement is related to the principal fibre orientations in accordance with agreement between parties to the measurement.

The end-faces of the length of the test piece shall be plane, parallel to each other, and perpendicular to the long axis.

6.2 Reference pieces

Reference materials shall be chosen so that their properties are as close as possible to the properties of the material to be tested. The reference piece shall have a volume of the same order and, if possible, shall have the same dimensions as the test piece (see [Table 1](#)).

For measurement at high temperature (over 2 000 K) under inert atmosphere, reference materials generally used are either tungsten or highly purified graphite. Reference materials shall be procured from a certified laboratory.

6.3 Dimensions

See [Table 1](#).

Table 1 — Recommended test piece dimensions

Dimensions in millimetres

	Material with small RVE (3.4) such as 1D or 2D	Material with large RVE (3.4) such as nD (n ≥ 3)	Tolerances
L_0 , total length	30	70	±0,2
B, width	7	Depending on material and equipment	—
h, thickness	Depending on material and equipment	Depending on material and equipment	Depending on material and equipment
ϕ , diameter	-	30	—
Parallelism	±0,01	±0,01	—

A test piece volume of a minimum of 5 RVE (3.4) is recommended.

The shape and dimensions of the test piece depend on the structure of reinforcement. In the case of material such as 3D, a large test piece is often necessary when the representative volume element is important.

For nD (n ≥ 3) composites with large RVE, thick beam specimens or cylinders with diameter ϕ are recommended.

If dimensions different from the recommended ones are used, specimen volume shall be larger than 5 RVE. Tolerances: dimensions: ±0,2 - Parallelism: ±0,05.

7 Procedure

In order to simplify calibration procedures, test pieces and reference pieces of the same length should be used. If reference and test pieces have different lengths, then it is necessary to take into account a base line shift. In this case, refer to EN 821-1.

- Measure the original length of the test piece at room temperature with devices (5.6).
The accuracy shall be better than
 - 0,05 mm for length of 10 mm and above, and
 - 0,02 mm for length lower than 10 mm.
- Make sure that the equipment has been calibrated for the type of material prior to the test, according to the procedure described in Annex A for direct measurement [determination of S and $\bar{\alpha}(A)$], and in Annex B for differential measurement (S and δ).
- Introduce the test piece in test system and provide a good contact between the push rod and the test piece. The force to apply on the specimen depends on the test system and material, but values lower than 1 N are generally sufficient.
- Proceed with heating or cooling at a rate of between 1 K/min and 5 K/min, ensuring a fairly constant temperature gradient along the test piece. If the temperature is changed by steps, the hold temperature shall be maintained until the length of the test piece shows no change for at least 5 min before the measure.
- Record temperature T and displacement Δx .

In case of large test pieces, a stepwise temperature rise is recommended.

The mean linear thermal expansion coefficient shall be calculated as the average from the results of tests on three test pieces.

Push rod for test should not have any reaction with the test piece and the reference.

8 Calculations

8.1 Direct measurement

Calculate the change in length, Δl , of a length of the sample holder material equal to the original test piece length L_0 , from Formula (1):

$$\Delta l = L_0 \bar{\alpha}_A (T_2 - T_1) \quad (1)$$

using the calculated value of Δl , the change in length of ΔL of the specimen is obtained from the measured displacement $S\Delta x$:

$$\Delta L = S\Delta x + \Delta l \quad (2)$$

Calculate the mean linear thermal expansion coefficient of the test piece material from Formula (3):

$$\bar{\alpha} = \frac{\Delta L}{L_0 (T_2 - T_1)} \quad (3)$$

where

- $\bar{\alpha}$ is the mean linear thermal expansion coefficient of the test piece material, in K⁻¹;
- $\bar{\alpha}_A$ is the mean linear thermal expansion coefficient correction for the apparatus over the temperature range used. It is determined from calibration (see [Annex A](#));
- L_0 is the initial length of the test piece at room temperature, in mm;
- Δx is the recorded displacement (in mm, volt, etc.) over the temperature range;
- S is the measurement sensitivity of the displacement recording system;
- Δl is the change in length of the sample holder material, in mm;
- ΔL is the change in length of the test piece, in mm;
- $T_2 - T_1$ is the temperature interval in K for which the change in length is measured.

A curve of $\frac{\Delta L}{L_0}$ versus T may be constructed.

8.2 Differential method

Calculate the mean linear thermal expansion coefficient of the test piece material from Formula (4):

$$\bar{\alpha} = \frac{S\Delta x - \delta}{L_0 (T_2 - T_1)} + \bar{\alpha}(R) \times \frac{L(R)}{L_0} \quad (4)$$

where

- δ is the baseline correction over the temperature range, which is introduced because of the possibility of unequal response from the two pushrods;
- $L(R)$ is the initial reference piece length at room temperature, in mm;
- $\bar{\alpha}(R)$ is the mean linear thermal expansion coefficient of the reference piece, in K⁻¹.


Other terms are as in [8.1](#).

9 Test report

The results shall be reported in accordance with ISO/IEC 17025 and the test report shall include the following information:

- a) the name of the testing establishment;
- b) the date of the test; a unique identification of the report and on each page, the name and address of the customer, and a signatory of the report;
- c) a reference to this International Standard, i.e. "Determined in accordance with ISO 17139";
- d) general description of the method used, i.e. Direct or Differential (see [Clause 4](#));
- e) method of calibration;
- f) description of the test piece: dimensions, preparation method, orientation, mass, volume;
- g) thermal cycle(s), number of hold periods, time at hold periods, and temperature interval between holds;
- h) maximum temperature testing;
- i) testing atmosphere;
- j) hysteresis between the heating and cooling cycle for materials which show a repeatable behaviour;
- k) indication of the thermal cycles carried out on the test piece prior to the measurement;
- l) table of the mean linear thermal expansion coefficient at the temperature required;
- m) any features identifiable as phase changes or softening under load of the measuring device;
- n) all other relevant information and all incidents that can affect the results, including comments on the test or test results.


STANDARDSISO.COM : Click to view the full PDF of ISO 17139:2014

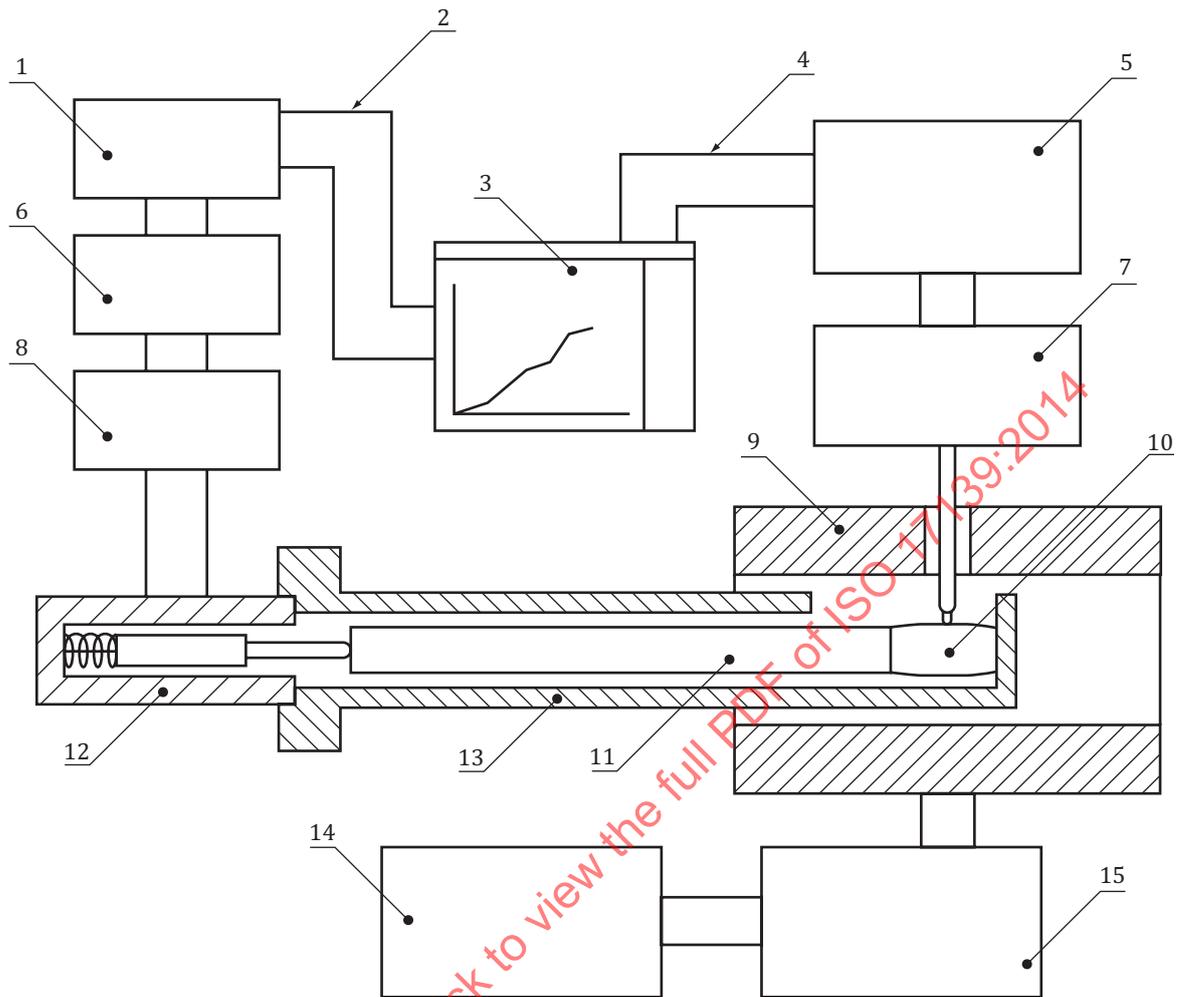

Key

- | | | | |
|---|---------------------|----|---|
| 1 | expansion ranging | 9 | furnace |
| 2 | y-axis | 10 | sample |
| 3 | X-Y recorder | 11 | push rod |
| 4 | x-axis | 12 | linear variable differential transformer (LVDT) |
| 5 | temperature ranging | 13 | sample holder |
| 6 | correction factor | 14 | programmer |
| 7 | 0 °C reference | 15 | furnace power control |
| 8 | expansion amplifier | | |

Figure 1 — Schematic of a direct measurement system

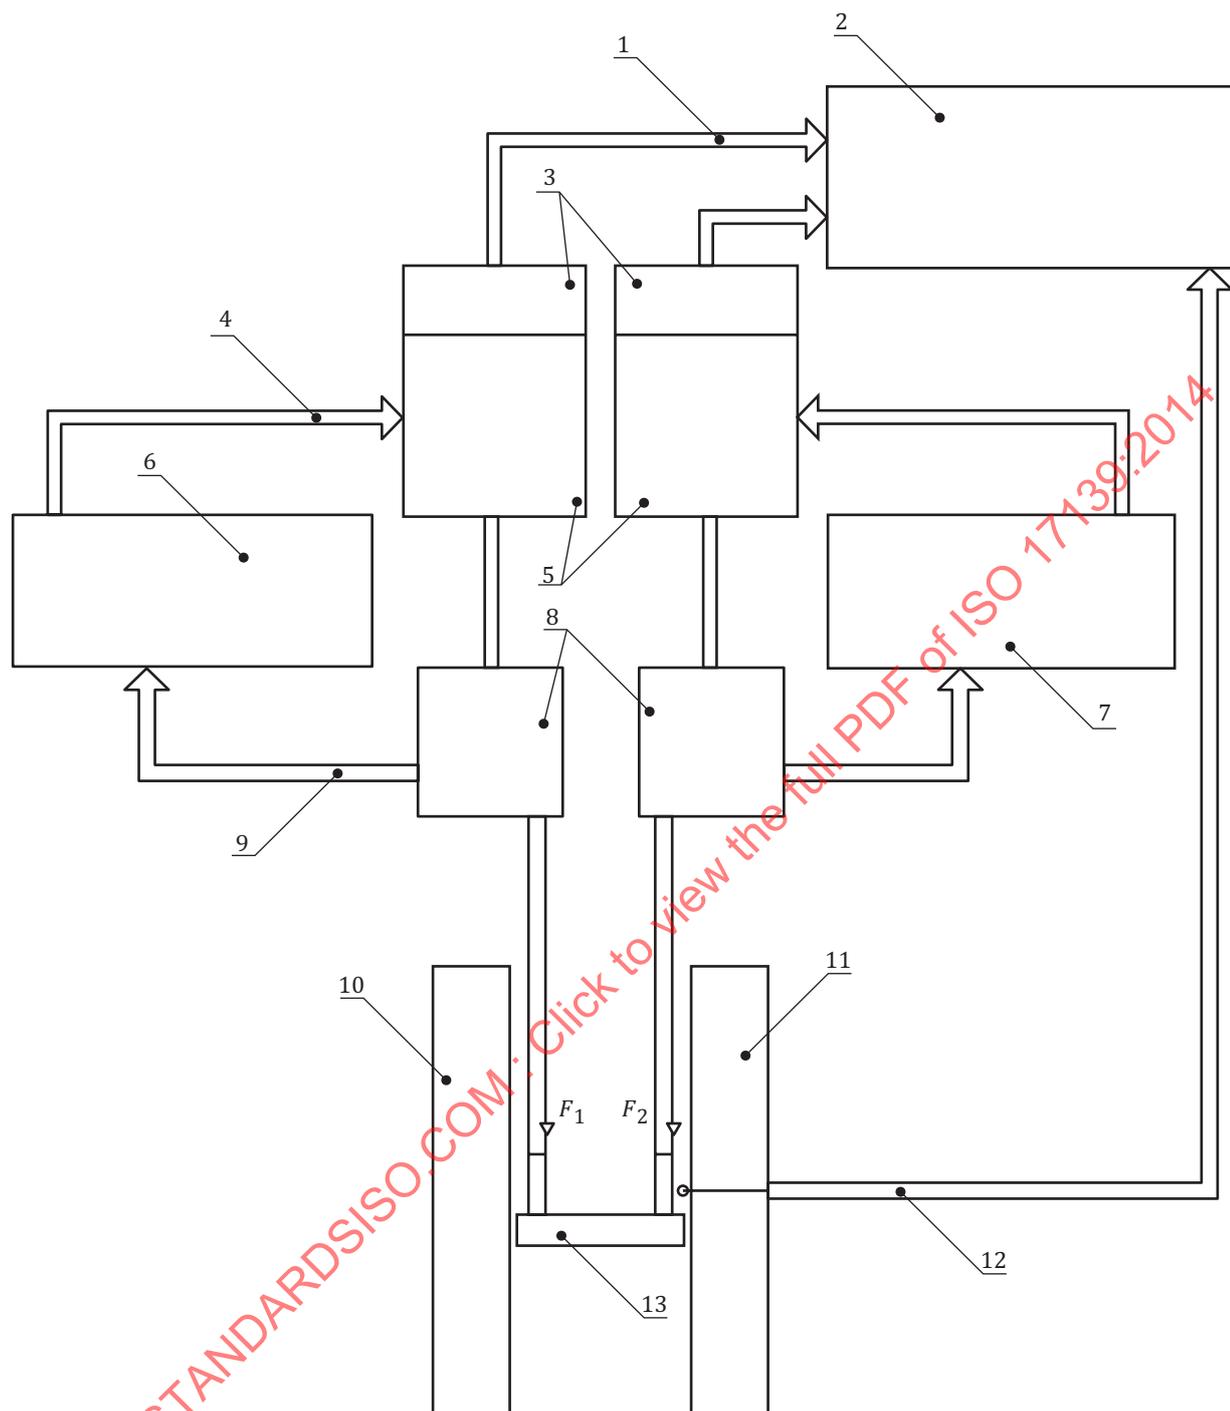

Key

- | | |
|---|----------------------------|
| 1 displacement measurement | 8 strength transducer |
| 2 data treatment (analog or digital) | 9 strength measurement |
| 3 encoders | 10 sample |
| 4 displacement signal | 11 reference |
| 5 displacement modules | 12 temperature measurement |
| 6 control in order to have $F_1 = C_1$ ($C_1 =$ adjustable constant) | 13 furnace |
| 7 control in order to have $F_2 = C_2$ ($C_2 =$ adjustable constant) | |

Figure 2 — Schematic of a differential measurement system

Annex A (normative)

Direct measurement apparatus

A.1 Determination of measurement sensitivity

The sensitivity of the measurement device, S , requires to be calibrated if it is not based on a direct-reading dial gauge or micrometer. This can be done either by using direct mechanical movement produced by using a certified micrometer of sufficient accuracy, or by use of two certified thermal expansion reference materials as test pieces.

Calibration tests shall be made for mechanical movement in both directions, and then the mean value of sensitivity taken. Calibration should take place in the same environment and at the same heating rate as the measurements on the test piece. Any nonlinearity shall be reported, and the apparatus shall be calibrated over the same range of displacement as that to be used for any series of tests.

NOTE This procedure applies to linear displacement transducer measuring devices in particular.

When two certified thermal expansion reference materials are available, the sensitivity is determined using Formula (A.1):

$$\bar{\alpha} = \frac{S\Delta x}{L_0\Delta T} + \bar{\alpha}_A \quad (\text{A.1})$$

for the two materials:

$$\bar{\alpha}_1 = \frac{S\Delta x_1}{L_0\Delta T} + \bar{\alpha}_A \quad (\text{A.2})$$

$$\bar{\alpha}_2 = \frac{S\Delta x_2}{L_0\Delta T} + \bar{\alpha}_A \quad (\text{A.3})$$

and by subtracting:

$$S = \frac{(\bar{\alpha}_1 - \bar{\alpha}_2)L_0\Delta T}{\Delta x_1 - \Delta x_2} \quad (\text{A.4})$$

where

$\bar{\alpha}_1$ and $\bar{\alpha}_2$ are the mean thermal expansion coefficients of the two reference materials over the temperature range ΔT ;

L_0 is the initial length, in mm, of the two reference pieces at room temperature;

$\Delta x_1, \Delta x_2$ are the recorded displacements (in mm, volts...) over the temperature range ΔT ;

ΔT is the temperature interval for which the changes in length are measured;

S is the measured sensitivity of the displacement recording system;

$\bar{\alpha}_A$ is the mean thermal expansion coefficient correction for the apparatus.

A.2 Determination of $\bar{\alpha}_A$

$$\bar{\alpha}_A = \bar{\alpha}(R) - \frac{S\Delta x}{L_0\Delta T} \quad (\text{A.5})$$

where

- $\bar{\alpha}_A$ is the mean linear thermal expansion coefficient correction for the apparatus over the temperature range used;
- $\bar{\alpha}(R)$ is the mean linear thermal expansion coefficient of the reference piece material;
- Δx is the recorded displacement (in mm, volts, etc.) over the temperature range ΔT ;
- S is the measurement sensitivity of the displacement recording system;
- L_0 is the initial length of the test piece, in mm;
- ΔT is the temperature range, in K, over which the change in length is measured.

The mean linear thermal expansion coefficient $\bar{\alpha}_A$ is obtained by using a certified reference material of similar thermal expansion to that of the material of the test piece holder and the push rod, and carrying out measurement in accordance with the procedure given in [Clause 7](#). The value of $\bar{\alpha}_A$ is obtained by inserting calibrated and experimental data for the reference material in Formula (A.5).

The calibrated reference piece is certified by approved organizations. The dimensions of the test piece to be measured and of the reference piece are identical within machining tolerances.

The physical properties of the material to be measured and the reference material (thermal expansion coefficient, thermal conductivity, emissivity) should be as close as possible. Measurements on the reference material and on the specimen should be performed under identical experimental conditions: type of environment, measuring kinetics, material for the specimen holder, temperature measurement device.