
**Fine ceramics (advanced ceramics,
advanced technical ceramics) —
Test method for air-purification
performance of semiconducting
photocatalytic materials under indoor
lighting environment —**

**Part 5:
Removal of methyl mercaptan**

STANDARDSISO.COM : Click to view the full PDF of ISO 17168-5:2018



STANDARDSISO.COM : Click to view the full PDF of ISO 17168-5:2018



COPYRIGHT PROTECTED DOCUMENT

© ISO 2018

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Symbols	2
5 Principle	2
6 Apparatus	2
6.1 Test equipment	2
6.2 Test gas supply	3
6.3 Photoreactor	3
6.4 Light source	6
6.5 UV sharp cut-off filter	6
6.6 Analytical system	6
7 Test piece	7
8 Procedure	7
8.1 General aspects	7
8.2 Pretreatment of the test piece	8
8.3 Pollutant removal test	8
9 Calculation	9
10 Test method for test pieces with lower performance	10
11 Test report	10
Bibliography	11

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 206, *Fine ceramics*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

Photocatalyst is a substance that performs decomposition and removal of contaminants, self-cleaning, antifogging, deodorization and antibacterial actions under photoirradiation. Its application has expanded considerably in recent years. The application of photocatalysts for indoor spaces has increasingly been sought as a solution to indoor environmental problems. Since conventional photocatalysts are responsive only to ultraviolet light, studies have been made to develop an indoor-light-active photocatalyst that makes effective use of indoor light, which room lights mainly emit, and thus demonstrates high photocatalytic performance indoors. The development has recently led to the commercialization of various indoor-light-active photocatalytic products, and there has been demand for the establishment of test methods to evaluate the performance of this type of photocatalyst.

This document, with ISO 22197-1 and ISO 22197-2 as the basis, is intended to provide a testing method to determine the performance of indoor-light-active photocatalytic materials with regards to the removal of methyl mercaptan, enabling swift distribution of photocatalytic products and thus contributing to a safe and clean environment.

STANDARDSISO.COM : Click to view the full PDF of ISO 17168-5:2018

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 17168-5:2018

Fine ceramics (advanced ceramics, advanced technical ceramics) — Test method for air-purification performance of semiconducting photocatalytic materials under indoor lighting environment —

Part 5: Removal of methyl mercaptan

1 Scope

This document specifies a test method for the determination of the air-purification performance, with regards to removal of methyl mercaptan, of materials that contain a photocatalyst or have photocatalytic films on the surface, usually made from semiconducting metal oxides such as titanium dioxide or other ceramic materials, by continuous exposure of a test piece to the model air pollutant under illumination with indoor light.

This document is intended for use with different kinds of materials, such as construction materials in flat sheet, board or plate shape, which are the basic forms of materials for various applications. This document also applies to materials in honeycomb form, and to plastic or paper materials containing ceramic microcrystals and composites. This document does not apply to powder or granular photocatalytic materials.

This test method is usually applicable to photocatalytic materials produced for air purification. This method is not suitable for the determination of other performance attributes of photocatalytic materials, i.e. decomposition of water contaminants, self-cleaning, antifogging and antibacterial actions.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 6145-7, *Gas analysis — Preparation of calibration gas mixtures using dynamic volumetric methods — Part 7: Thermal mass-flow controllers*

ISO 14605, *Fine ceramics (advanced ceramics, advanced technical ceramics) — Light source for testing semiconducting photocatalytic materials used under indoor lighting environment*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

ISO 17168-1, *Fine-ceramics (advanced ceramics, advanced technical ceramics) — Test method for air-purification performance of semiconducting photocatalytic materials under indoor lighting environment — Part 1: Removal of nitric oxide*

ISO 80000-1, *Quantities and units — Part 1: General*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 17168-1 apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

4 Symbols

f	air-flow rate of test gas converted into that at the standard state (0 °C, 101,3 kPa) (l/min)
ϕ_M	methyl mercaptan volume fraction at the reactor exit ($\mu\text{l/l}$)
ϕ_{M0}	supply volume fraction of methyl mercaptan ($\mu\text{l/l}$)
n_M	removal quantity, by test piece, of methyl mercaptan (μmol)
R_M	removal percentage, by test piece, of methyl mercaptan (%)


5 Principle

This document deals with the development, comparison, quality assurance, characterization, reliability and design data generation of photocatalytic materials^[1]. The method described is intended to obtain the air-purification performance of photocatalytic materials by exposing a test piece to model polluted air under illumination by indoor light. Methyl mercaptan (methanethiol, CH_3SH) is chosen as a typical malodorous substance^[2]. The test piece, placed in a flow-type photoreactor, is activated by indoor-light illumination, and adsorbs and oxidizes gas-phase methyl mercaptan. The air-purification performance is determined from the amount of the net removal of methyl mercaptan and removal rate of methyl mercaptan. The simple adsorption and desorption of CH_3SH by the test piece (not due to photocatalysis) is evaluated by tests in the dark. However, this document cannot be applied to test pieces which do not give a stable concentration of methyl mercaptan in the designated test time. The photocatalytic activity may depend on physical and chemical properties of pollutants, mainly due to the adsorption process involved. For a better evaluation of air purification performance of photocatalytic materials, it is recommended that one or more suitable test methods are combined, as provided in other parts of the ISO 17168 series.

6 Apparatus

6.1 Test equipment

The test equipment enables a photocatalytic material to be examined for its pollutant-removal capability by supplying the test gas continuously, while providing photoirradiation to activate the photocatalyst. It is the same as that used in the test method for the removal of nitric oxide (see ISO 17168-1) and consists of a test gas supply, a photoreactor, a light source, a UV sharp cut-off filter and pollutant measurement equipment. Since low concentrations of pollutants are to be tested, the system shall be constructed with materials of low adsorption and resistant to ultraviolet (UV) radiation, for example acrylic resin, stainless steel, glass and fluorocarbon polymers. An example of a test system is shown in [Figure 1](#).

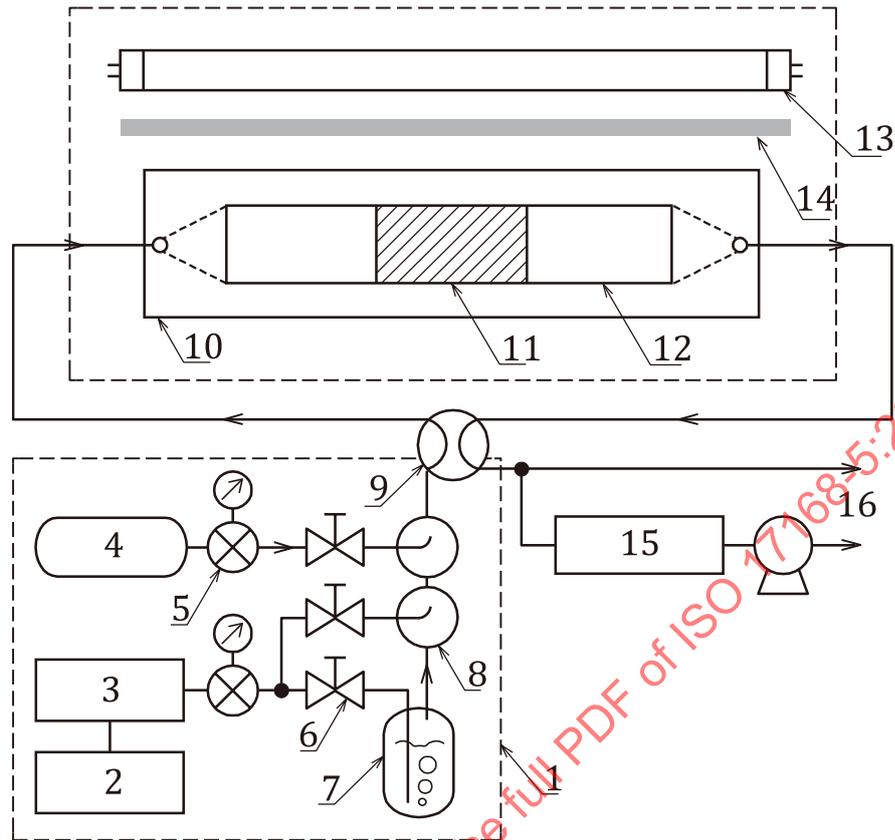

Key

- | | |
|-----------------------------------|----------------------------|
| 1 test gas supply | 9 four-way valve |
| 2 air compressor | 10 photoreactor |
| 3 air-purification system | 11 test piece |
| 4 standard gas (pollutant) | 12 airtight optical window |
| 5 pressure regulator with a gauge | 13 light source |
| 6 mass-flow controller | 14 sharp cut-off filter |
| 7 humidifier | 15 analyser |
| 8 gas mixer | 16 vent |

Figure 1 — A schematic of the testing equipment

6.2 Test gas supply


The test gas supply provides air polluted with model contaminant at a predetermined concentration, temperature and humidity, and supplies it continuously to the photoreactor. It consists of flow regulators, a humidifier, gas mixers and so on. The flow rate of each gas should be within 5,0 % of the designated value, which is easily attained by using thermal mass-flow controllers with knowledge of temperature and gas type at calibration in accordance with ISO 6145-7. The expression of gas flow rate in this document is that converted to the standard state (0 °C, 101,3 kPa). Typical capacities of flow controller for pollutant gas, dry air and wet air are 50, 1 000 and 1 000 ml/min, respectively. The standard methyl mercaptan gas in a cylinder, normally balanced with nitrogen, shall have a volume fraction of 100 µl/l to 1 000 µl/l.

6.3 Photoreactor



The photoreactor holds a planar test piece within a 50-mm wide trough, with its surface parallel to an airtight optical window for photoirradiation. The reactor shall be fabricated from materials that adsorb

little test gas and withstand irradiation of near-UV light. The test piece shall be separated from the window by a $5,0 \text{ mm} \pm 0,5 \text{ mm}$ thick air layer. The test gas shall pass only through the space between the test piece and the window. This gap shall be accurately set up according to the thickness of the test piece, for example by using height-adjusting plates with different thicknesses, as shown in [Figure 2 a\)](#). When a filter-type material is tested, an alternative type of test-piece holder shall be used, which holds the test piece while allowing the test gas to pass through the cells of the filter under illumination [[Figure 2 b\)](#)]. Quartz or borosilicate glass that absorbs minimal light at wavelengths longer than 300 nm should be used for the window.

STANDARDSISO.COM : Click to view the full PDF of ISO 17168-5:2018

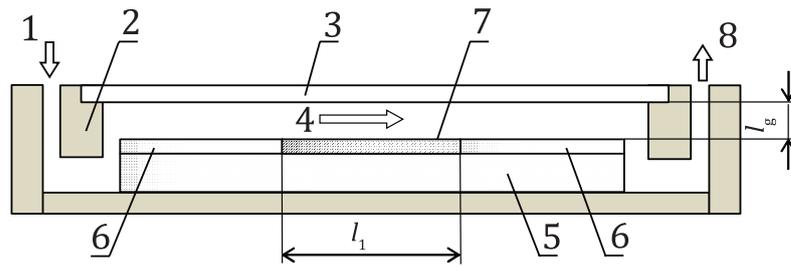

a) For flat test pieces

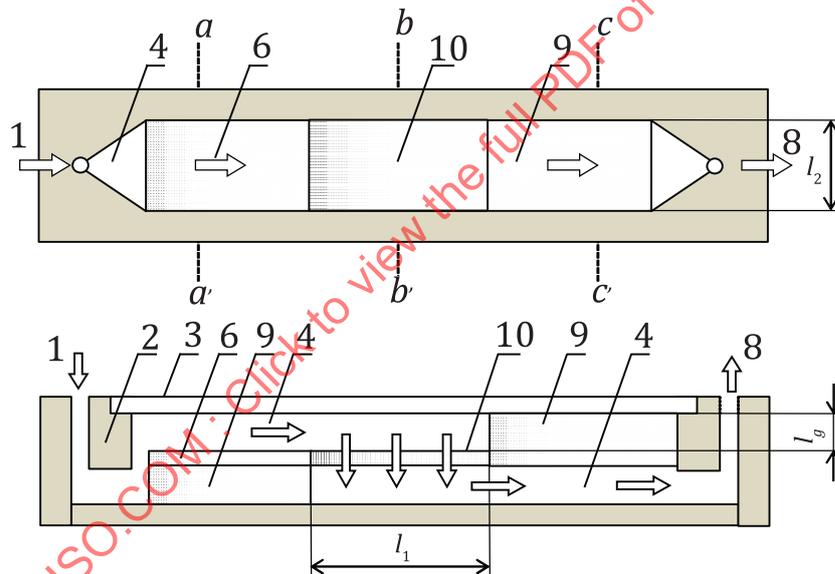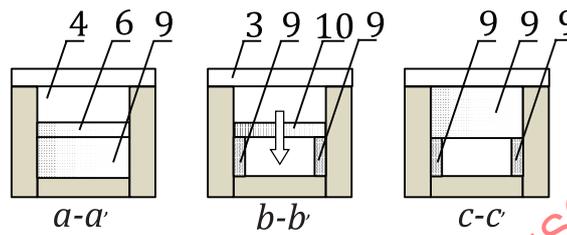

b) For filter-type test pieces

Test piece length l_1	Test piece width l_2	Air layer thickness l_g
$99,0 \pm 1,0$ mm	$49,0 \pm 1,0$ mm	$5,0 \pm 0,5$ mm

Key

- | | |
|---------------------------|-----------------------------|
| 1 test gas inlet | 6 auxiliary plate |
| 2 baffle | 7 test piece (flat-type) |
| 3 airtight optical window | 8 test gas outlet |
| 4 flow channel | 9 test piece holder |
| 5 height-adjusting plate | 10 test piece (filter-type) |

Figure 2 — Cross-sectional views of photoreactor

6.4 Light source


A cool white harophosphate fluorescent lamp and a UV sharp cut-off filter as specified in ISO 14605 shall be used. The test piece shall be illuminated uniformly through the window by the light source. When testing honeycomb-form photocatalysts, the light source shall illuminate one face of the test piece. A light source that requires warming up shall be equipped with a shutter. The distance between the light source and the reactor shall be adjusted so that the illuminance at the test piece surface is $6\,000\text{ lx} \pm 300\text{ lx}$. The illuminance along the length of the test piece shall also be constant within $\pm 5\%$. The illuminance shall be measured with an illuminance meter which conforms to ISO 14605. The reactor and light source shall be shielded from external light. The parts around the light source, such as luminaire and shielding device, shall have small reflectance, or flat spectral reflectance over the wavelength range of indoor light.

6.5 UV sharp cut-off filter

The UV sharp cut-off filter shall remove a small amount of UV light radiated from the light source. The transmittance of the UV sharp cut-off filter shall be less than 0,1 % (wavelength $< 365\text{ nm}$), less than 1 % (at 380 nm) and higher than 80 % ($400\text{ nm} < \text{wavelength} < 780\text{ nm}$), and the wavelength where the transmittance is half of the average transmittance between 400 nm and 780 nm is located at $390\text{ nm} \pm 5\text{ nm}$.

6.6 Analytical system

The concentration of methyl mercaptan shall be determined by gas chromatography. Either packed column or capillary column can be used as long as it can separate methyl mercaptan from related organic compounds. The detection shall be made by either flame ionization detector (FID) or flame photometric detector (FPD). The test gas is sampled with a gas-tight syringe. However, use of a six-way valve is recommended for reproducible and automatic sampling. The flow diagram when a six-way valve is used is shown in [Figure 3](#). A small sampling pump continuously ventilates the metering tube with the test gas. The pump is stopped when the test gas is sampled by switching the six-way valve. The volume of the metering tube is typically 0,5 ml, but it shall be determined by the sensitivity of the analytical system.

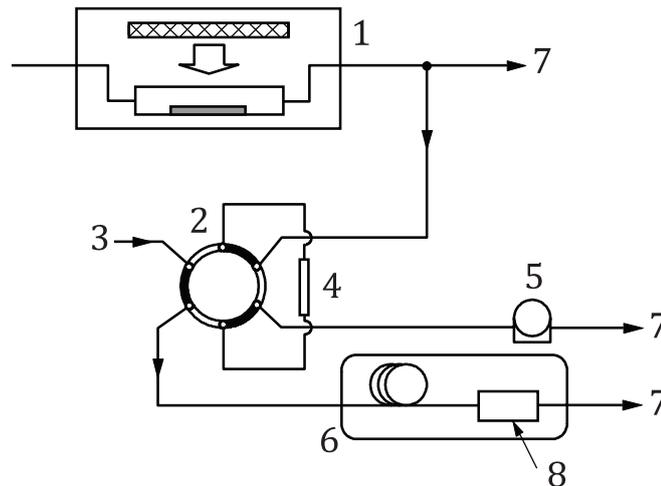**Key**

- 1 photoreactor
- 2 six-way valve
- 3 carrier gas
- 4 metering tube
- 5 sampling pump
- 6 gas chromatograph
- 7 vent
- 8 FID

Figure 3 — Gas sampling system


7 Test piece

The test piece shall be a flat material or a honeycomb filter $49,0 \text{ mm} \pm 1,0 \text{ mm}$ wide and $99,0 \text{ mm} \pm 1,0 \text{ mm}$ long. It may be cut to these dimensions from a larger bulk material or coated sheet, or may be specially prepared for the test by coating a pre-cut substrate. The thickness of the test piece shall ideally be less than 5 mm, in order to minimize the contribution from the side faces. If thicker test pieces are to be tested, the side faces shall be sealed with an inert material before testing. The honeycomb test piece shall not be thicker than 20 mm.

8 Procedure

8.1 General aspects

The test procedure consists of pre-treatment of a test piece, adsorption process in the dark, and measurements of removal of methyl mercaptan under photoirradiation. An example of concentration change of methyl mercaptan during the test is shown in [Figure 4](#). Some test pieces may not give accurate removal of methyl mercaptan due to lower photocatalytic activity. In this case, loading of methyl mercaptan per test piece can be reduced following the procedure in [Clause 10](#).

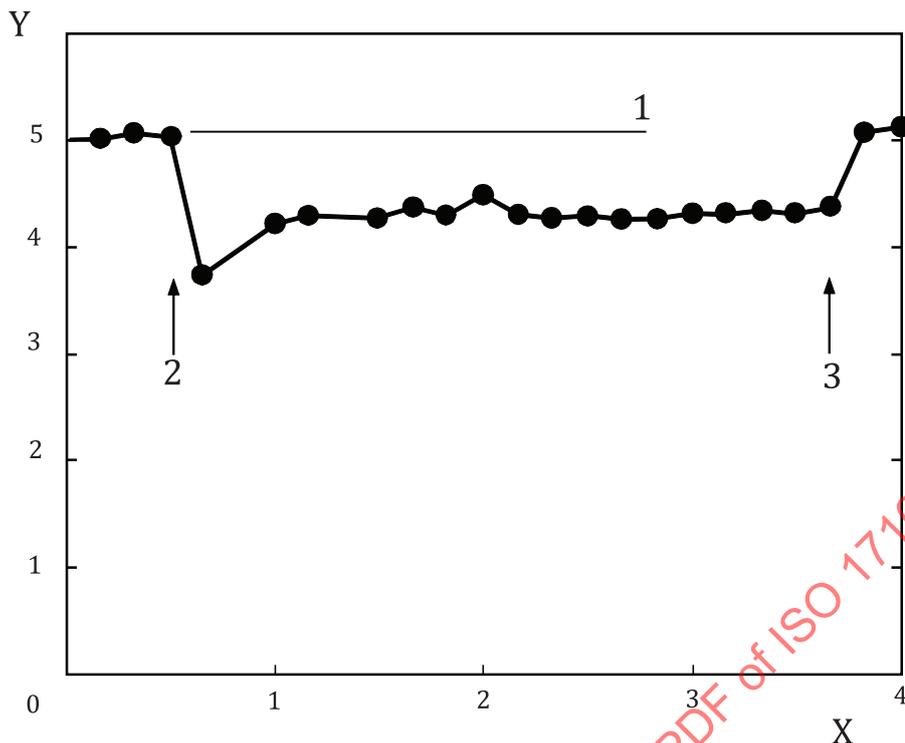**Key**

- 1 feed level
- 2 lights on
- 3 lights off
- X time (h)
- Y methyl mercaptan concentration (µl/l)

Figure 4 — Examples of methyl mercaptan concentration measurement

8.2 Pretreatment of the test piece

8.2.1 The test piece shall normally be pretreated as specified in 8.2.2 and 8.2.3 in this order. When it is anticipated that the test piece has hydrophobic contamination, 8.2.3 may be followed by 8.2.2. The procedure in 8.2.2 can be omitted if it causes damage to the test piece. If the test pieces are not to be tested immediately after this pretreatment, they shall be kept in an airtight container.

8.2.2 Immerse the test piece in deionized water for 2 h or more, remove it and air-dry at room temperature. The test piece may be dried by heating within a temperature range that does not cause physical and chemical changes to the test piece (maximum 120 °C). Dryness is confirmed when a constant mass is reached. The method of drying and any observations, such as the appearance of sediment in the wash water, shall be recorded.

8.2.3 Irradiate the test piece with an ultraviolet lamp for at least 12 h (up to 24 h) to decompose residual organic matter on the test piece. The UV irradiance at the sample surface shall be high enough to secure complete decomposition of organic matter (10 W/m² – 20 W/m²).

8.3 Pollutant removal test

8.3.1 Adjust the test gas supply beforehand so that it can stably supply the test gas containing 5,0 µl/l ± 0,25 µl/l of methyl mercaptan and 1,56 % ± 0,08 % of volume fraction of water vapour at