

---

---

**Petroleum and related products —  
Preparation of a test portion of high-  
boiling liquids for the determination of  
water content — Nitrogen purge method**

*Pétrole et produits connexes — Préparation d'une prise d'essai de  
liquides à haut point d'ébullition en vue du dosage de l'eau — Méthode  
par purge à l'azote*

STANDARDSISO.COM : Click to view the PDF file ISO 20764:2003



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 20764:2003

© ISO 2003

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 20764 was prepared by Technical Committee ISO/TC 28, *Petroleum products and lubricants*.

STANDARDSISO.COM : Click to view the full PDF of ISO 20764:2003



# Petroleum and related products — Preparation of a test portion of high-boiling liquids for the determination of water content — Nitrogen purge method

**WARNING** — The use of this International Standard may involve hazardous materials, operations and equipment. This International Standard does not purport to address all of the safety problems associated with its use. It is the responsibility of the user of this International Standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.

## 1 Scope

This International Standard specifies two procedures for the preparation of test portions from petroleum and related products boiling above 200 °C, which can then be used for the determination of total water content within the range of 3 mg/kg to 1 000 mg/kg. The method is applicable to unused and used lubricating oils, non-aqueous hydraulic fluids and high-boiling solvents. The test portions generated by these procedures are suitable for standard Karl Fischer water-content determinations, such as those described in ISO 6296 (see [1] in the Bibliography) and ISO 12937 (see [2] in the Bibliography).

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 383:1976, *Laboratory glassware — Interchangeable conical ground joints*

ISO 3170:—<sup>1)</sup>, *Petroleum liquids — Manual sampling*

## 3 Principle

### 3.1 Atmospheric pressure

The water is driven out of a weighed portion of the material under test by a nitrogen purge at 120 °C. It is then condensed in methanol (4.2) held in a titration vessel (5.4) at approximately –77 °C. The resulting water/methanol solution is immediately available for the determination of water content by Karl Fischer titration.

### 3.2 Reduced pressure

For used lubricating oils and high-boiling materials with high-water retaining characteristics, the water is driven out of a weighed portion by a nitrogen purge at 60 °C under an absolute pressure of 0,30 kPa to 0,65 kPa. It is collected and titrated in the same manner as the test portion in 3.1.

---

1) To be published. (Revision of ISO 3170:1988)

## 4 Reagents and materials

**4.1 Nitrogen**, of pure grade, containing less than 500 mg/kg of oxygen. The source shall be regulated to a low pressure that gives agitation without vortex at a flow rate of 3 l/h. It shall be dried through a drying agent upstream of the wash-bottle inlet.

NOTE The maximum water-content target of the nitrogen is 1 µg/l.

**4.2 Methanol**, of commercial grade, dried to a water content of not more than 100 mg/kg. Dried methanol shall be continuously protected by a drying tube containing a suitable drying agent.

**4.3 Solid carbon dioxide**

**4.4 Cooling medium**: commercial grade of methanol, ethanol or acetone.

## 5 Apparatus

### 5.1 General

The layout of the extraction apparatus is illustrated in Figure 1, with details of the titration vessel and inserts shown in Figures 2, 3 and 4. The major components are described in 5.2 to 5.5.

Ground-glass joints from different sources may have one of two diameter-to-length ratios. For the purposes of this International Standard, either is suitable, and for some applications, the diameter itself can be one of two. However, it is critical that the male and female parts of each joint are from the same series to avoid recession or protuberance.

NOTE In Europe, ground-glass joints normally come from a series known as "k = 6" as described in ISO 383, whereas in North America, the series generally used is "k = 8". For joints specified in the figures in this International Standard, these result in joints with dimensions of 14,5/23 and 14,5/30, respectively.

**5.2 Heating bath**, consisting of a liquid bath of sufficient capacity to hold the wash bottle (5.3), and capable of being controlled at temperatures of  $60\text{ }^{\circ}\text{C} \pm 1\text{ }^{\circ}\text{C}$  and  $120\text{ }^{\circ}\text{C} \pm 1\text{ }^{\circ}\text{C}$ .

**5.3 Wash bottle**, made of a borosilicate glass, of inside diameter 55 mm and insert, with a graduation line at 250 ml, as illustrated in Figure 1.


**5.4 Titration vessel**, consisting of a borosilicate glass three-necked flask as shown in Figure 2, fitted with inserts as shown in Figures 1, 3 and 4. Figure 4 is illustrative only, as the design will depend upon the Karl Fischer detection system used for the final analysis.

**5.5 Cooling vessel**, consisting of a Dewar flask or similar, of sufficient capacity to hold the titration vessel (5.4) surrounded by cooling medium (4.4), and with access to allow the addition of solid carbon dioxide (4.3). A temperature-controlled bath containing cooling medium at  $-77\text{ }^{\circ}\text{C} \pm 3\text{ }^{\circ}\text{C}$  is suitable.

**5.6 Vacuum source**, a pump or other source of vacuum, capable of maintaining an absolute pressure of 0,3 kPa to 0,65 kPa for a minimum period of 90 min.

**5.7 Analytical balance**, of minimum capacity 500 g, capable of weighing to the nearest 0,01 g.


**5.8 Flowmeter**, capable of reading the nitrogen flow of  $3\text{ l/h} \pm 0,3\text{ l/h}$ .

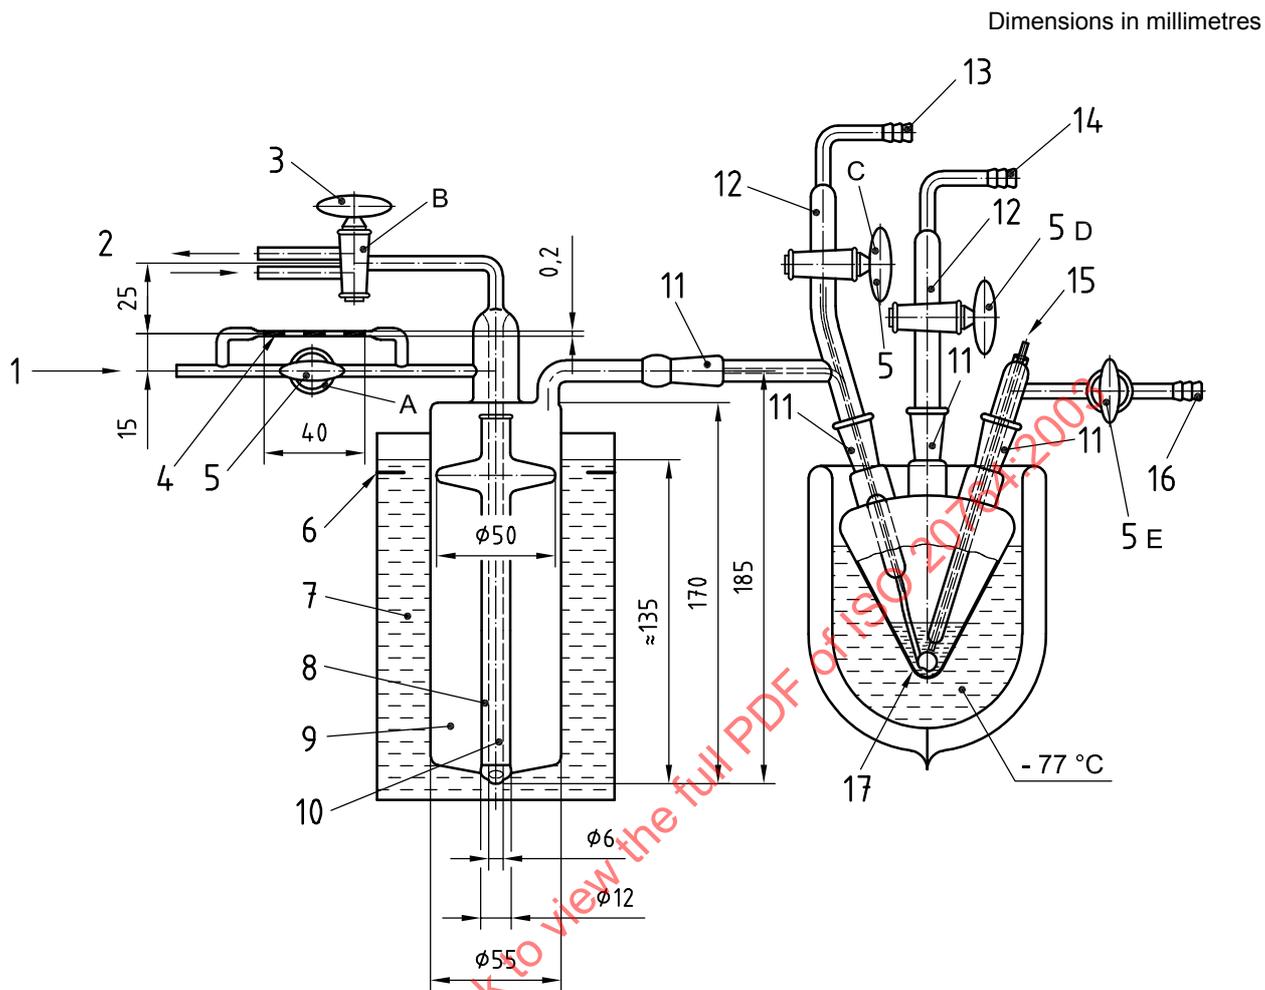

**Key**

- |                                       |                                     |
|---------------------------------------|-------------------------------------|
| 1 nitrogen in                         | 10 filling tube                     |
| 2 test portion                        | 11 ground-glass sockets/cones       |
| 3 two-way cock B                      | 12 0,1 to 0,2 bore tube             |
| 4 vacuum capillary                    | 13 methanol connection              |
| 5 one-way cocks A, C, D and E         | 14 Karl Fischer solution connection |
| 6 graduation line at $\approx$ 250 ml | 15 Karl Fischer detector connection |
| 7 heating bath                        | 16 vacuum pump connection           |
| 8 riser tube                          | 17 titration vessel                 |
| 9 graduated wash bottle               |                                     |

**Figure 1 — Layout of apparatus**

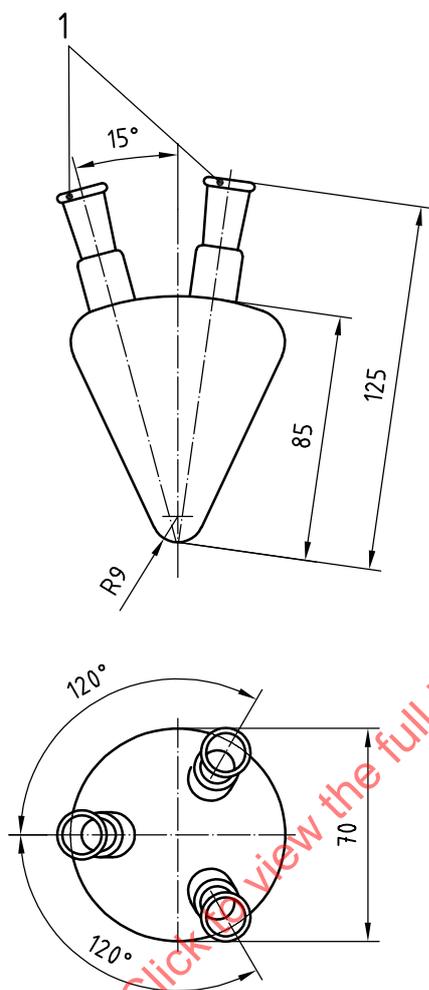


**Key**

- 1 ground-glass sockets

**Figure 2 — Titration vessel**


Dimensions in millimetres

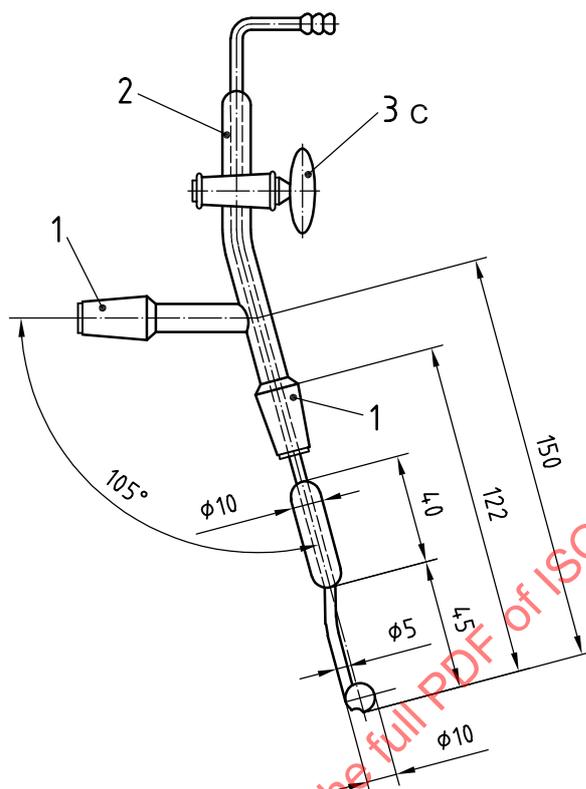

**Key**

- 1 ground-glass sockets/cones
- 2 0,1 to 0,2 bore tube
- 3 one-way cock C

**Figure 3 — Methanol and water vapour insert**

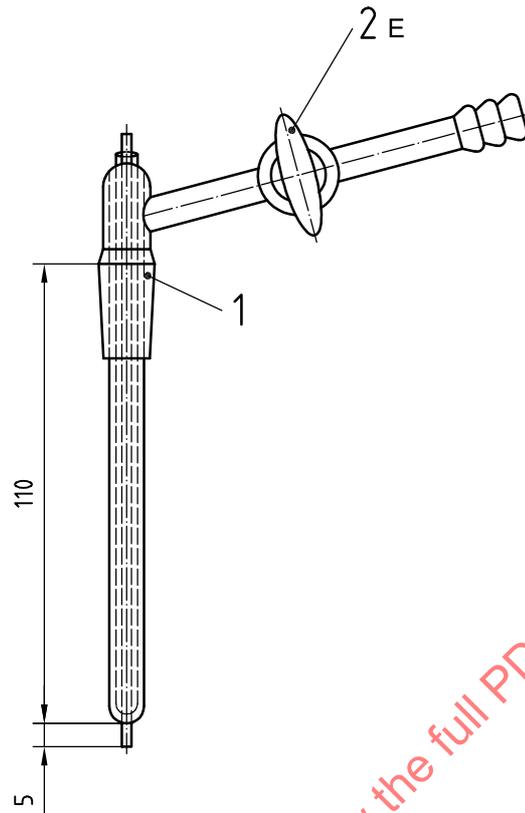**Key**

- 1 ground-glass sockets/cones
- 2 one-way cock E

**Figure 4** — Vacuum and detector insert**6 Samples and sampling**

- 6.1** Unless otherwise specified, samples shall be obtained by the procedures described in ISO 3170.
- 6.2** The laboratory samples shall be drawn into absolutely dry dark-glass containers fitted with ground-glass stoppers. The stoppers shall be made airtight by the application of a suitable water-resistant sealing medium.
- 6.3** Samples shall be withdrawn directly into the sample containers with the container immersed in the bulk. The stoppers shall not be removed until immersion is complete. No subsequent compositing of samples is allowed.

If alternative sample containers are all that are available, maximum precautions shall be taken to prevent ingress of moist air during and following sampling, without the risk of removing water from the sample.

- 6.4** In general, the start of test-portion preparation shall immediately follow sampling, and the maximum time difference shall be 1 h. If a longer period has elapsed, note and report the time difference.

## 7 Procedure

### 7.1 General

**7.1.1** Assemble the apparatus and add 3 ml to 5 ml of dried methanol (4.2) to the titration vessel. Adjust the nitrogen flow to  $3 \text{ l/h} \pm 0,3 \text{ l/h}$  and obtain a reading of the blank mass of water for the reagents, using the technique described in 7.2.4, over a period of  $15 \text{ min} \pm 2 \text{ min}$ , with the temperature of the dried methanol at  $0 \text{ }^\circ\text{C}$  to  $20 \text{ }^\circ\text{C}$ .

**7.1.2** Weigh the wash bottle (5.3) without the top and riser tube, to the nearest 0,01 g. Add a quantity of the laboratory sample by nitrogen displacement of 180 ml to 220 ml, and reweigh to the nearest 0,01 g.

**NOTE** The volume chosen is to ensure that, at no time during the procedure, the liquid level rises above the graduated mark on the wash bottle. For samples expected to have water contents in excess of 50 mg/kg, the volume may be reduced to 100 ml.

**7.1.3** Immediately assemble the apparatus and ensure that all joints are sealed.

**7.1.4** Adjust the temperature of the cooling medium (4.4) to  $-77 \text{ }^\circ\text{C} \pm 3 \text{ }^\circ\text{C}$  (approximately the saturated liquid temperature of solid carbon dioxide) and start the nitrogen flow (see 7.3.2).

**7.1.5** Switch on the heating bath (5.2) and adjust to the temperature specified in 7.2 or 7.3.

### 7.2 Atmospheric pressure

**7.2.1** Raise the temperature in the heating bath to  $120 \text{ }^\circ\text{C} \pm 1 \text{ }^\circ\text{C}$ .

**7.2.2** Maintain this temperature, with the nitrogen flow at  $3,0 \text{ l/h} \pm 0,3 \text{ l/h}$  for  $60 \text{ min} \pm 5 \text{ min}$ .

**7.2.3** At the end of this period, remove the cooling vessel (5.5) from the titration vessel (5.4) and allow the methanol/water mixture to rise to a temperature within the range of  $0 \text{ }^\circ\text{C}$  to  $20 \text{ }^\circ\text{C}$ .

**7.2.4** Determine the mass of water in the methanol/water mixture by potentiometric or coulometric titration, with the nitrogen still flowing to stir the mixture.

### 7.3 Reduced pressure

**7.3.1** Raise the temperature in the heating bath to  $60 \text{ }^\circ\text{C} \pm 1 \text{ }^\circ\text{C}$ .

**7.3.2** Adjust the vacuum to 0,30 kPa to 0,65 kPa absolute pressure, at the same time reducing the nitrogen flow rate. As soon as vacuum is applied, ensure that Cock C and Cock D in Figure 1 are closed.

The nitrogen flow rate should be very low, but positive, as the vacuum is established to minimize the risk of the material in the wash bottle foaming as it is degassed. A flow rate of 2 to 3 gas bubbles (50  $\mu\text{l}$ ) per second is recommended, and is achieved either by the use of the vacuum-capillary bypass shown in Figure 1, or by a suitable control valve.

**7.3.3** Maintain the temperature of the heating bath at  $60 \text{ }^\circ\text{C} \pm 1 \text{ }^\circ\text{C}$ , with the liquid in the cooling medium at  $-77 \text{ }^\circ\text{C} \pm 3 \text{ }^\circ\text{C}$ , and the vacuum at 0,30 kPa to 0,65 kPa for  $90 \text{ min} \pm 5 \text{ min}$ .

**7.3.4** At the end of this period, adjust the pressure back to atmospheric, increase the nitrogen flow, and follow the procedures described in 7.2.3 and 7.2.4.