

INTERNATIONAL  
STANDARD

ISO  
21422

IDF 242:2018

First edition  
2018-09

Corrected version  
2021-03

---

---

**Milk, milk products, infant  
formula and adult nutritionals —  
Determination of chloride —  
Potentiometric titration method**

*Lait, produits laitiers, formules infantiles et produits nutritionnels  
pour adultes — Détermination de la teneur en chlorures — Méthode  
par titrage potentiométrique*

STANDARDSISO.COM : Click to view the full PDF of ISO 21422:2018



Reference numbers  
ISO 21422:2018(E)  
IDF 242:2018:2018(E)

© ISO and IDF 2018

STANDARDSISO.COM : Click to view the full PDF of ISO 21422:2018



**COPYRIGHT PROTECTED DOCUMENT**

© ISO and IDF 2018

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11

Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

International Dairy Federation  
Silver Building • Bd Auguste Reyers 70/B  
B-1030 Brussels  
Phone: +32 2 325 67 40  
Fax: +32 2 325 67 41  
Email: [info@fil-idf.org](mailto:info@fil-idf.org)  
Website: [www.fil-idf.org](http://www.fil-idf.org)

# Contents

	Page
Foreword .....	iv
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>1</b>
<b>5 Reagents</b> .....	<b>1</b>
<b>6 Preparation of solutions</b> .....	<b>2</b>
<b>7 Apparatus</b> .....	<b>3</b>
<b>8 Sample preparation</b> .....	<b>4</b>
8.1 Powders, for milk, milk products and infant formula .....	4
8.2 Cheese, for hard or rinded cheese .....	4
8.3 Butter .....	4
<b>9 Extraction</b> .....	<b>4</b>
9.1 Cheese .....	4
9.2 Butter .....	5
9.3 Milk, milk products, infant formula and adult nutritional products .....	5
9.4 Procedure .....	5
<b>10 Instrument operating conditions</b> .....	<b>5</b>
10.1 Check and maintenance of the combined silver electrode .....	5
10.2 Titration .....	5
10.3 Determination of very low amounts of chloride .....	6
10.4 Blank test .....	6
<b>11 System suitability test</b> .....	<b>6</b>
<b>12 Calculations</b> .....	<b>6</b>
<b>13 Precision</b> .....	<b>7</b>
13.1 General .....	7
13.2 Repeatability .....	7
13.3 Reproducibility .....	8
<b>14 Test report</b> .....	<b>9</b>
<b>Annex A (informative) Examples of titration end point determination</b> .....	<b>10</b>
<b>Annex B (informative) Precision data</b> .....	<b>12</b>
<b>Annex C (informative) Comparison of results between sample extraction with and without additional protein precipitation</b> .....	<b>14</b>
<b>Bibliography</b> .....	<b>16</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products* and the International Dairy Federation (IDF). It is being published jointly by ISO and IDF and separately by AOAC INTERNATIONAL. The method described in this International Standard is equivalent to the AOAC Official Method 2016.03: Chloride in Milk, Milk Products, Whey Powder, Infant Formula and Adult Nutritionals Potentiometric titration.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

This corrected version of ISO 21422 | FIL 242:2018 incorporates the following corrections:

- in [5.1](#), the sentence has been revised to "[...] less than 0,056 mS/cm (more than 18 M $\Omega$ ) [...]";
- in [Clause 12](#), the description of " $V_1$ " in [Formulae \(1\)](#) and [\(2\)](#) has been revised to " $V_1$  is the volume of 0,1 mol/l or 0,025 mol/l AgNO<sub>3</sub> solution [...]".

**IDF (the International Dairy Federation)** is a non-profit private sector organization representing the interests of various stakeholders in dairying at the global level. IDF members are organized in National Committees, which are national associations composed of representatives of dairy-related national interest groups including dairy farmers, dairy processing industry, dairy suppliers, academics and governments/food control authorities.

ISO and IDF collaborate closely on all matters of standardization relating to methods of analysis and sampling for milk and milk products. Since 2001, ISO and IDF jointly publish their International Standards using the logos and reference numbers of both organizations.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. IDF shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

This document was prepared by the IDF Standing Committee on Analytical Methods for Composition and ISO Technical Committee ISO/TC 34, Food products, Subcommittee SC 5, Milk and milk products. It is being published jointly by ISO and IDF.

The work was carried out by the ISO/IDF Project Group C39 of the Standing Committee on Analytical Methods for Composition under the aegis of its project leader, Mr E. Konings (CH).

STANDARDSISO.COM : Click to view the full PDF of ISO 21422:2018

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 21422:2018

# Milk, milk products, infant formula and adult nutritionals — Determination of chloride — Potentiometric titration method

## 1 Scope

This document specifies a method for the determination of chloride in milk, milk products, infant formula and adult nutritionals by potentiometry<sup>[1][2][3][4]</sup> with an analytical range of 0,35 mg chloride/100 g to 711,6 mg chloride/100 g product, or ready-to-feed products.

## 2 Normative references

There are no normative references in this document.

## 3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

## 4 Principle

Chloride is extracted from samples by mixing in warm water, or directly from ready-to-feed (RTF) products. After (optional) precipitation of proteins, chloride ions are titrated with standardized  $\text{AgNO}_3$  solution potentiometrically, using a silver electrode to detect the end point.

## 5 Reagents

**5.1 Water**, purified, less than 0,056 mS/cm (more than 18 M $\Omega$ ) (EMD Millipore<sup>1)</sup> Corp., Billerica, MA, USA, or equivalent).

**5.2 Sodium chloride** ( $\text{NaCl}$ ), purity  $\geq 99,5$  %, certified reference material for titrimetry, Sigma Aldrich #71387<sup>1)</sup> or equivalent.

**5.3 Silver nitrate** ( $\text{AgNO}_3$ ), meeting analytical specification of European Pharmacopoeia (Ph. Eur), British Pharmacopoeia (BP), United States Pharmacopoeia (USP), assay 99,8 % to 100,5 %, Sigma-Aldrich 10220<sup>1)</sup>, or equivalent.

**5.4 Potassium ferrocyanide trihydrate** ( $\text{K}_4\text{Fe}(\text{CN})_6 \cdot 3\text{H}_2\text{O}$ ), puriss. p.a., American Chemical Society (ACS) reagent, reagent Ph. Eur.,  $\geq 99$  %, Sigma-Aldrich # 31524<sup>1)</sup> or equivalent.

1) This is an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO or IDF of the product named. Equivalent products may be used if they can be shown to lead to the same results.

**5.5 Zinc acetate dihydrate** ( $\text{Zn}(\text{CH}_3\text{COO})_2 \cdot 2\text{H}_2\text{O}$ ), ACS reagent puriss p.a.,  $\geq 99,0\%$ , Sigma Aldrich # 96459<sup>1)</sup> or equivalent.

**5.6 Nitric acid** ( $\text{HNO}_3$ ), minimum 65 % p.a., Merck #100452<sup>1)</sup> or equivalent.

**5.7 Standardized  $\text{AgNO}_3$  solution**, substance concentration  $c = 0,1$  mol/l, Titripur® Reag. Ph. Eur. Reag. USP. # 1,09081,1000 or EM3214-1, or ready-to-use standardized titrant prepared according to GB/T 601<sup>[5]1)</sup>, or equivalent.

**5.8 NaCl standard solution**,  $c = 0,1000$  mol/l, Alfa Aesar<sup>1)</sup>, # 35616, (Ward Hill, MA, USA), or equivalent.

**5.9 Glacial acetic acid, 100 %**, p.a., MERCK, # 100063<sup>1)</sup> or equivalent.

**5.10 Potassium nitrate**, ( $\text{KNO}_3$ ), p.a., MERCK, # 105063<sup>1)</sup> or equivalent.

**5.11 Acetone.**

**5.12 Dimethylpolysiloxane**, defoaming agent, Sigma-Aldrich, #DMPS2C<sup>1)</sup> or equivalent.

## 6 Preparation of solutions

### 6.1 Standardized $\text{AgNO}_3$ solution, $c = 0,1$ mol/l.

If ready-to-use  $\text{AgNO}_3$  (5.7) standard solution is not available, weigh  $16,989\ 0\ \text{g} \pm 0,000\ 5\ \text{g}$   $\text{AgNO}_3$  (5.3) previously dried for 2 h at  $120\ ^\circ\text{C} \pm 2\ ^\circ\text{C}$ . Dissolve in water (5.1) and make up to the mark in a 1 000 ml volumetric flask. Store in a brown reagent bottle.

After preparation, check the titre by titration of 5,0 ml with exactly 0,1 mol/l NaCl solution. For either commercial or in-house solution verify the titre on a regular basis. Store the standardized  $\text{AgNO}_3$  solution so it is protected from light for up to two months.

### 6.2 NaCl solution, $c = 0,1$ mol/l.

If ready-to-use NaCl (5.8) standard solution is not available, weigh  $5,844\ 0\ \text{g} \pm 0,000\ 5\ \text{g}$  NaCl (5.2), previously dried for 2 h at  $110\ ^\circ\text{C} \pm 2\ ^\circ\text{C}$ . Dissolve in water (5.1) and make up to the mark in a 1 000 ml volumetric flask. This solution is stable for up to one month.

### 6.3 Precipitating solution (Carrez) I.

Weigh 106 g potassium ferrocyanide trihydrate (5.4), and transfer into a 1 000 ml volumetric flask. Dissolve with an appropriate amount of water (5.1). Make up to the mark using water (5.1). Mix well.

### 6.4 Precipitating solution (Carrez) II.

Weigh 220 g zinc acetate dihydrate (5.5) and transfer into a 1 000 ml volumetric flask. Dissolve in an appropriate amount of water (5.1) and add 30 ml glacial acetic acid (5.9). Make up to the mark with water (5.1). Mix well.

### 6.5 $\text{HNO}_3$ solution, $c = 4$ mol/l.

Carefully add 100 ml concentrated  $\text{HNO}_3$  (5.6) to 300 ml water (5.1). Mix well.

In accordance with the autosampler/titrator manufacturer's instructions, this may be used as the wash solution (e.g. acetone, nitric acid solution or other).

#### 6.6 AgNO<sub>3</sub> solution, $c = 0,025 \text{ mol/l}$ (optional).

Pipet 25 ml AgNO<sub>3</sub> solution, 0,1 mol/l (5.7 or 6.1) into a 100 ml volumetric flask. Make up to the mark with water (5.1). Prepare freshly before use. Then check the titre by titration of 25 ml against 0,025 mol/l NaCl solution.

#### 6.7 NaCl solution, $c = 0,025 \text{ mol/l}$ (optional).

Pipet 25 ml NaCl solution, 0,1 mol/l (5.8 or 6.2) into a 100 ml volumetric flask. Make up to the mark with water (5.1). Prepare freshly before use.

#### 6.8 KNO<sub>3</sub> solution, $c = 1 \text{ mol/l}$ .

Weigh 10,11 g KNO<sub>3</sub> (5.10) into a 100 ml volumetric flask. Add about 80 ml of water (5.1) and place it in an ultrasonic cleaner (7.13) until completely dissolved. Cool down to room temperature and make up to the mark with water (5.1). Filter using a disposable syringe with a 0,45 µm membrane filter (7.14) before use.

### 7 Apparatus

Usual laboratory equipment and, in particular, the following.

7.1 **Analytical balances**, precision 0,01 mg and 0,1 mg.

7.2 **Centrifuge**, table-top with rotor for 50 ml conical tubes, capable of operating at 4 °C and  $\geq 12\,000g$ .

7.3 **Centrifuge tubes**, 50 ml, conical, polypropylene.

7.4 **Pipettes**, 1 ml, 10 ml, 20 ml, 50 ml and 100 ml, volumetric or automatic, Class A in accordance with ISO 1042<sup>[6]</sup>.

7.5 **One-mark volumetric flasks**, 50 ml, 100 ml, 500 ml, and 1 000 ml, Class A in accordance with ISO 1042<sup>[6]</sup>.

7.6 **Graduated cylinders**, 25 ml, 100 ml and 500 ml, glass.

7.7 **Autosampler beaker**, e.g. 120 ml, depending on the titrator used.

7.8 **pH-meter or mV-meter**, with a scale covering  $\pm 700 \text{ mV}$ .

7.9 **Automatic titrator**, autosampler, motorized piston burette, with remote-control dispensing and filling, or glass burette 20 ml or 25 ml.

Mettler T50, Roundo Tower autosampler, MettlerLabX 3.1 software or Metrohm 862 Compact Titrosampler, 800 Dosino, 10 ml Exchange Unit, or equivalent. Alternatively, a semi-automated titrator (e.g. MetrohmTitrand 905/907, with MetrohmTiamo™ software<sup>2)</sup> or equivalent or a manual titrator (using a burette with a readability of 0,01 ml) may be used.

7.10 **Combined ring silver electrode**, e.g. Mettler DM 141 or DMi145-SC, Metrohm Ag Titrode 6.0430.100<sup>2)</sup> or equivalent. Alternatively, a silver electrode with reference electrode may be used.

2) These are examples of suitable products available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO or IDF of the products named. Equivalent products may be used if they can be shown to lead to the same results.

7.11 **Magnetic stirrer.**

7.12 **Water bath.**

7.13 **Ultrasonic cleaner.**

7.14 **Disposable syringe**, 3 ml, with handspike and 0,45 µm disposable syringe filter.

7.15 **Blender**, capable to hold and blend 100 ml volume.

## 8 Sample preparation

### 8.1 Powders, for milk, milk products and infant formula

Mix well to ensure that the sample is homogeneous, Reconstitute powder samples by dissolving 25 g sample in 200 ml warm water of 40 °C.

### 8.2 Cheese, for hard or rinded cheese

Prior to analysis, remove the rind or smear or mouldy surface layer of the cheese in such a way as to provide a sample representative of the cheese as it is usually consumed. Grind or grate the sample by means of an appropriate device. Mix the ground or grated mass quickly, and if possible grind or grate a second time and again mix thoroughly. If the sample cannot be ground or grated, mix it thoroughly by intensive stirring and kneading.

Transfer the sample to an airtight container to await analysis, which should be carried out as soon as possible after grinding. If delay is unavoidable, take all precautions to ensure proper preservation of the sample and to prevent condensation of moisture on the inside surface of the container. The storage temperature should be 10 °C to 12 °C.

### 8.3 Butter

If the sample is visibly inhomogeneous, or if the history of the sample (age, storage conditions) is such that inhomogeneity is expected, homogenize the sample as follows.

Warm the sample in the original unopened container, which should be from one-half to two-thirds full, to a temperature at which the sample will be soft enough to facilitate thorough mixing to a homogeneous state (either by a mechanical shaker or by hand). Take care that the mixing temperature does not exceed 30 °C.

Cool the sample to ambient temperature with constant mixing until cooling is complete. As soon as possible thereafter, open the sample container and stir briefly (no longer than 10 s) with a suitable device, for example a spoon or spatula, before weighing.

## 9 Extraction

### 9.1 Cheese

Weigh 2 g to 5 g of the prepared sample (8.2) into the titration vessel. For processed cheese, weigh 2,5 g. Add 30 ml of water (5.1) at about 55 °C. Suspend the sample using a blender (7.15). Rinse the blender with approximately 10 ml of water, collecting the rinsing in the titration vessel. Add 2 ml to 3 ml of the HNO<sub>3</sub> solution of  $c = 4 \text{ mol/l}$  (6.5). Proceed with 9.4.4.

## 9.2 Butter

Weigh 2 g to 4 g of the prepared sample (8.3) into the titration vessel. For salted butter, weigh 2,5 g. Carefully add 100 ml of boiling water and heat to boiling to suspend the test portion. Cool the obtained suspension to below 55 °C. Proceed with 9.4.4.

## 9.3 Milk, milk products, infant formula and adult nutritional products

Proceed with 9.4.3 unless it is determined that additional protein precipitation is required to achieve acceptable performance. Protein precipitation is accomplished by following 9.4.1 to 9.4.2.

NOTE Validation data from the collaborative trial for infant formula and adult nutritional products (Annex B) showed no difference in results for samples treated with and without additional protein precipitation. See Annex C.

## 9.4 Procedure

9.4.1 Weigh an appropriate well mixed aliquot of RTF product or reconstituted powder (8.1) (e.g. 25 g accurate to 1 mg) into a 50 ml centrifuge tube. For samples with a high chloride content, weigh a smaller test portion (e.g. 5 g of RTF or reconstituted powder).

Transfer 2,5 ml precipitating solution I (6.3) and 2,5 ml precipitating solution II (6.4) into the tube. Dilute to 50 ml with water. Mix well. If foam impacts the constant volume, add one or two drops of defoaming agent (5.12).

9.4.2 Centrifuge at 12 000g for 5 min at 4 °C. Then equilibrate to room temperature.

9.4.3 Accurately transfer either 10 ml supernatant from steps 9.4.1 to 9.4.2 or weigh an appropriate aliquot of RTF or reconstituted powder (8.1) (e.g. 25 g ± 1 g accurately weighed to 1 mg). For samples with a high chloride content, weigh a smaller test portion (e.g. 5 g ± 1 g of RTF or reconstituted or powder) into a 120 ml sample beaker or autosampler cup.

Add 5 ml HNO<sub>3</sub> solution (6.5) and 50 ml of water before titration. Add a magnetic stirring bar (if the titrator does not have a built-in rod stirrer). Place the autosampler cup or beaker onto a magnetic stirrer and stir until dissolved or finely suspended.

9.4.4 The pH of the test solution shall be below 1,5. In case of any doubt, check by means of a pH-meter and, if necessary, add a little more HNO<sub>3</sub> solution (6.5).

## 10 Instrument operating conditions

### 10.1 Check and maintenance of the combined silver electrode

Rinse the electrode with deionized water and wipe before use. Renew the electrolyte  $c = 1 \text{ mol/l KNO}_3$  (6.8) periodically as per the manufacturer's recommendations. If fat sticks to the electrodes during a series of analyses, then remove it by briefly immersing the electrode in acetone (5.11). Store the silver electrode in KNO<sub>3</sub> solution (6.8) after appropriate cleaning.

NOTE Instead of the combined silver electrode, separate silver and reference electrodes can be used.

### 10.2 Titration

Connect the combined silver electrode to the titration apparatus, according to the manufacturer's instructions. Ensure that the titration vessels are correctly placed on the autosampler and that there are sufficient reagents, both HNO<sub>3</sub> solution (6.5), if added automatically, and standardized AgNO<sub>3</sub> solution (6.1). If no autosampler is available, place the sample solutions manually under the titration equipment.

Put the wash solution (6.5) in the washing position if an autosampler is used. Ensure that the volume of wash solution is adequate.

Under continuous stirring and without touching the electrode, titrate the sample solution automatically with standardized AgNO<sub>3</sub> solution (6.1), up to the end potential. See Annex A for an example. The consumption of standardized AgNO<sub>3</sub> solution (6.1) should be recorded automatically and can be read from the titrator software, or documented in the titrator operating records.

For manual titration using a burette (7.9), add standardized AgNO<sub>3</sub> solution (6.1) until the end potential has nearly been met. Continue to titrate slowly until the end point is reached as observed on the meter with two small (about 0,05 ml) additions of standardized AgNO<sub>3</sub> solution (6.1).

### 10.3 Determination of very low amounts of chloride

When determining low chloride (e.g. < (10 to 20) mg/100 g) concentrations, such as in desalted whey powder, for greater precision a 0,025 mol/l standardized AgNO<sub>3</sub> solution (6.6) should be used for the titration.

### 10.4 Blank test

To determine the reagent background content of chloride, perform a blank test using reagents and substituting water (5.1) for the sample portion. The titrant consumption of the blank test obtained at the end point shall be less than 0,05 ml while using the standardized AgNO<sub>3</sub> solution (5.7 or 6.1) and 0,2 ml when using the 0,025 mol/l standardized AgNO<sub>3</sub> solution (6.6). Otherwise, check the reagents and water involved in the procedures, and perform the blank test again until the criteria is achieved.

## 11 System suitability test

Prior to use, transfer 5 ml of NaCl solution (5.8 or 6.2) into a 120 ml sample beaker. If 0,025 mol/l AgNO<sub>3</sub> titrant is required, use 1 ml NaCl solution. Add 5 ml HNO<sub>3</sub> solution (6.5) and 50 ml water. Place the wash solution (6.5) in the washing position of the autosampler. Titrate using an automatic, semi-automatic or manual titrator. Carry out in triplicate.

Calculate the concentration of the AgNO<sub>3</sub> solution according to Clause 12. The difference between the calculated concentration and the certified value should be within 0,5 %. If it is outside the acceptance value, check the experimental procedures and titration system. If the issue is not resolved, then use fresh standardized AgNO<sub>3</sub>. If fresh standardized AgNO<sub>3</sub> does not provide an acceptable result, replace the electrolyte of the electrode and check the operating condition of the dosing unit.

## 12 Calculations

Calculate the concentration of AgNO<sub>3</sub>,  $c_{\text{snc}}$ , in mol/l, for system suitability verification and report to four decimal places.

If using the prepared NaCl solution (6.2), use Formula (1):

$$c_{\text{snc}} = \frac{m_1}{5,844 \times V_1 \times 10} \quad (1)$$

where

$m_1$  is the mass of NaCl in 5 ml or 1 ml of NaCl solution (6.2), in mg;

$V_1$  is the volume of 0,1 mol/l or 0,025 mol/l  $\text{AgNO}_3$  solution consumed at titration end point, in ml;

5,844 is the NaCl mass, in mg, corresponding to 1 ml of 0,1 mol/l  $\text{AgNO}_3$ ;

10 is the mass conversion from titre to the concentration of titrant.

Or, if using a commercially available standard grade 0,10 mol/l NaCl solution (5.8), use Formula (2):

$$c_{\text{snc}} = \frac{0,1 \times V_3}{V_1} \quad (2)$$

where

$V_3$  is the volume of purchased standard grade 0,10 mol/l NaCl added, in ml;

$V_1$  is the volume of 0,1 mol/l or 0,025 mol/l  $\text{AgNO}_3$  solution consumed at titration end point, in ml.

Calculate the chloride mass fraction,  $w_{\text{cl}}$ , in mg/100 g in the sample and report to three significant digits, using Formula (3):

$$w_{\text{cl}} = \frac{35,45 \times c \times (V_2 - V_0) \times f \times 100}{m} \quad (3)$$

where

$m$  is the sample mass, in g;

$c$  is the certified concentration of  $\text{AgNO}_3$  titrant [0,100 0 mol/l or standardized concentration Formula (1)];

$V_2$  is the volume of  $\text{AgNO}_3$  solution consumed at titration end point, in ml;

$V_0$  is the volume of  $\text{AgNO}_3$  solution consumed at titration end point for blank (10.4), in ml;

$f$  is the dilution factor for preparation of reconstituted powder, RTF or concentrate; for samples requiring the protein precipitation step (9.4.1 to 9.4.2), an additional factor (e.g. for 25 g sample  $f = 2$ ) is needed;

35,45 is the chloride mass, in mg, corresponding to 1 ml of 1 mol/l  $\text{AgNO}_3$ ;

100 is the mass conversion to mg/100 g.

## 13 Precision

### 13.1 General

Details of the interlaboratory test of the precision of the method are summarized in Annex B. The values derived from the interlaboratory test may not be applicable to analyte concentration ranges and/or matrices other than those given in Annex B.

### 13.2 Repeatability

The absolute difference between two single test results found on identical test material by one operator using the same apparatus within the shortest feasible time interval will exceed the repeatability limit  $r$  in not more than 5 % of the cases.

The values for chloride are given in [Table 1](#).

**Table 1 — Repeatability values for chloride**

Mean $\bar{x}$ (mg/100 g)	Repeatability limit, $r$ [ $r = 2,8 \times s_r$ ], mg/100 g	Matrix
385,5	6,30	Adult nutritional powder low fat
162,6	4,76	Adult nutritional RTF high fat
154,2	8,37	Adult nutritional RTF high protein
701,1	14,03	SRM 1849a
478,6	11,68	Toddler formula powder milk based
42,4	1,12	Infant formula RTF milk based
510,3	15,93	Infant formula powder soy based
413,7	20,38	Infant formula powder milk based
330,4	10,36	Infant formula powder FOS/GOS based
386,1	7,92	Infant formula powder part hyd soy based
380,2	6,55	Infant formula powder part hyd milk based
357,3	9,97	Infant formula powder milk based
443,6	5,49	Child formula powder milk based
372,54	8,62	Infant elemental powder
35,41	3,11	Adult nutritional RTF high fat – placebo
40,2	1,26	Adult nutritional RTF high protein – placebo
32,4	11,20	Child formula powder milk based – placebo
22,5	0,92	Infant formula RTF milk based – placebo
358,9	5,26	Infant elemental powder – placebo
375,5	17,67	Butter
562,2	23,66	Cheese
169,5	6,10	Whey protein concentrate
711,6	11,12	Whole milk powder
95,3	3,64	Whole milk
281,3	5,35	Whey powder

### 13.3 Reproducibility

The absolute difference between two single test results found on identical test material reported by different laboratories with different operators using different equipment, will exceed the reproducibility limit  $R$  in not more than 5 % of the cases.

The values for chloride are given in [Table 2](#)

**Table 2 — Reproducibility values for chloride**

Mean $\bar{x}$ , mg/100 g	Reproducibility limit, $R$ [ $R = 2,8 \times s_R$ ], mg/100 g	Matrix
385,5	37,35	Adult nutritional powder low fat
162,6	11,59	Adult nutritional RTF high fat
154,2	13,02	Adult nutritional RTF high protein
701,1	47,99	SRM 1849a
478,6	50,32	Toddler formula powder milk based
42,4	2,77	Infant formula RTF milk based

Table 2 (continued)

Mean $\bar{x}$ , mg/100 g	Reproducibility limit, $R$ [ $R = 2,8 \times s_R$ ], mg/100 g	Matrix
510,3	28,67	Infant formula powder soy based
413,7	40,46	Infant formula powder milk based
330,4	23,52	Infant formula powder FOS/GOS based
386,1	44,16	Infant formula powder part hyd soy based
380,2	24,16	Infant formula powder part hyd milk based
357,3	36,68	Infant formula powder milk based
443,6	44,24	Child formula powder milk based
372,54	40,66	Infant elemental powder
35,41	7,14	Adult nutritional RTF high fat - placebo
40,2	4,37	Adult nutritional RTF high protein - placebo
32,4	18,90	Child formula powder milk based - placebo
22,5	2,21	Infant formula RTF milk based - placebo
358,9	22,48	Infant elemental powder - placebo
375,5	36,48	Butter
562,2	44,07	Cheese
169,5	18,28	Whey protein concentrate
711,6	51,30	Whole milk powder
95,3	7,25	Whole milk
281,3	28,11	Whey powder


## 14 Test report

The test report shall at least include the following information:

- all information necessary for the identification of the sample (type of sample, origin and designation of the sample);
- a reference to this document, i.e. ISO 21422 | IDF 242;
- the date and type of sampling procedure (if known);
- the date of receipt;
- the date of test;
- the test results and the units in which they have been expressed;
- any operations not specified in the method or regarded as optional, which might have affected the results.

## Annex A (informative)


### Examples of titration end point determination

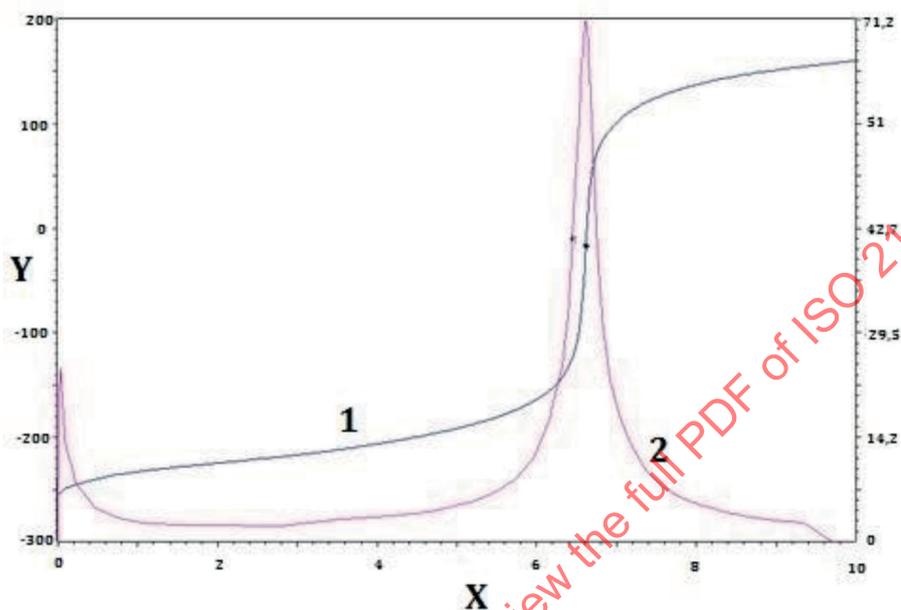

#### Key

- X volume of consumption of the standardized  $\text{AgNO}_3$  titrant during titration, in ml
- Y voltage of Ag electrode detected during titration, in mV
- 1 titration curve
- 2 first derivative of the titration curve drawn by voltage of electrode versus volume of titrant consumption

**Figure A.1 — Automatic titration end point recognition using dynamic titration (DET U) mode on Methohm Titrand 905**

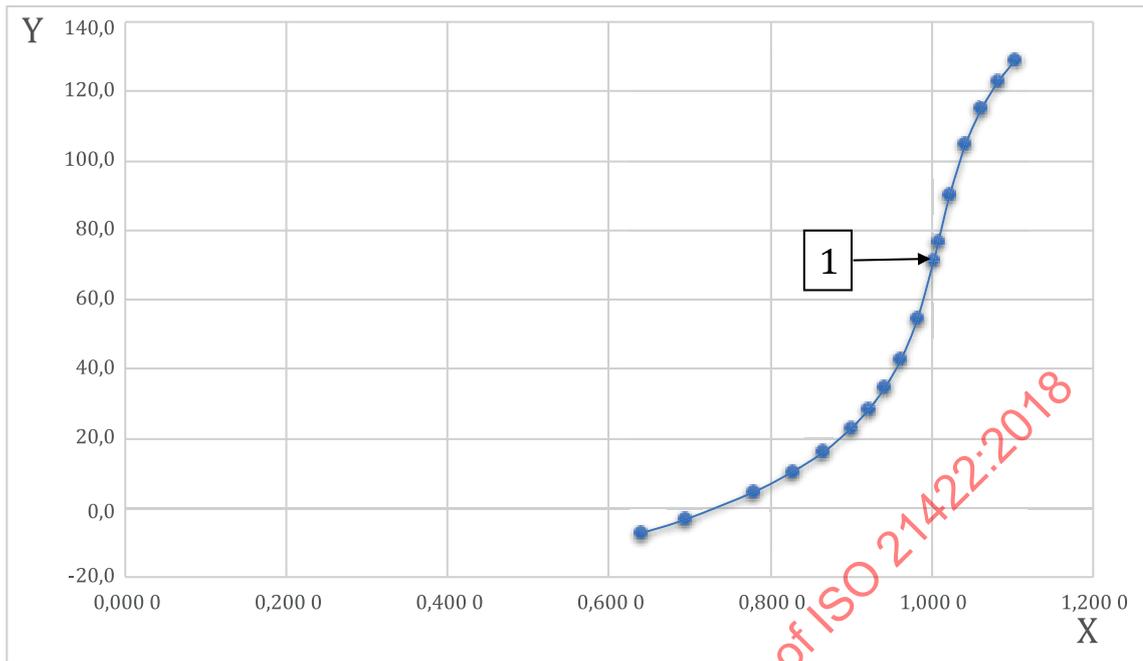

Volume ml	Increment ml	Signal mV	Change mV	1 <sup>st</sup> deriv. mV/ml	Time s	Temp. °C
0,640 5	0,098 5	-7,2	7,1	77,21	59	25,0
0,695 5	0,055 0	-3,2	4,0	92,25	64	25,0
0,779 0	0,083 5	4,6	7,8	125,68	74	25,0
0,827 5	0,048 5	10,5	5,9	158,57	81	25,0
0,865 5	0,038 0	16,1	5,6	201,91	88	25,0
0,900 0	0,034 5	23,0	6,9	269,55	96	25,0
0,922 0	0,022 0	28,5	5,5	336,34	102	25,0
0,942 0	0,020 0	34,8	6,3	404,52	109	25,0
0,962 0	0,020 0	43,0	8,2	533,58	116	25,0
0,982 0	0,020 0	54,5	11,5	677,59	124	25,0
1,002 0	0,020 0	71,2	16,7	779,28	131	25,0
1,007 7		76,6		781,17		
1,022 0	0,020 0	90,2	19,0	755,93	138	25,0
1,042 0	0,020 0	105,0	14,6	636,30	144	25,0
1,062 0	0,020 0	115,2	10,2	487,45	149	25,0
1,082 0	0,020 0	122,8	7,6	376,97	154	25,0
1,103 5	0,021 5	129,1	6,3	307,43	160	25,0

**Key**

- X volume, in ml
- Y signal, in mV
- 1 titration end point

**Figure A.2 — Example of a titration curve from Mettler autotitrator**

## Annex B (informative)

### Precision data

The data given in [Table B.1](#) were obtained in an international interlaboratory study organized in 2016, in accordance with ISO 5725-2<sup>[2]</sup> and the AOAC-IUPAC harmonized protocol for collaborative study procedures, to access precision characteristics of a method of analysis<sup>[8]</sup>. The study was performed based on requirements given in Reference <sup>[9]</sup>.

**Table B.1 — Precision data for chloride**

Sample	Number of laboratories retained after eliminating outliers	Number of outliers (laboratories)	Number of accepted results	Mean value, $\bar{x}$	Repeatability standard deviation, $s_r$	Reproducibility standard deviation, $s_R$	RSD <sub>r</sub>	RSD <sub>R</sub>	Hor-Rat
				mg/100 g	mg/100 g	mg/100 g	% <sup>a</sup>	% <sup>b</sup>	
Adult nutritional powder low fat	16	0	16	385,5	2,25	13,34	0,58	3,46	0,75
Adult nutritional RTF high fat	16	6	10	162,6	1,7	4,14	1,05	2,54	0,48
Adult nutritional RTF high protein	16	0	16	154,2	2,99	4,65	1,94	3,01	0,57
SRM 1849a	16	0	16	701,1	5,01	17,14	0,72	2,44	0,58
Toddler formula powder milk based	16	0	16	478,6	4,17	17,97	0,87	3,76	0,84
Infant formula RTF milk based	16	1	15	42,4	0,40	0,99	0,94	1,21	0,36
Infant formula powder soy based	16	2	14	510,3	5,69	10,24	1,12	2,01	0,45
Infant formula powder milk based	16	1	15	413,7	7,28	14,45	1,76	3,49	0,76
Infant formula powder FOS/GOS based	16	1	15	330,4	3,7	8,4	1,12	2,54	0,54
Infant formula powder part hyd soy based	16	1	15	386,1	2,83	15,77	0,73	4,08	0,88
Infant formula powder part hyd milk based	16	2	14	380,2	2,34	8,63	0,61	2,27	0,49
<sup>a</sup> Relative standard deviation of repeatability. <sup>b</sup> Relative standard deviation of reproducibility. <sup>c</sup> Expired liquid samples possibly spoiled/separated.									

Table B.1 (continued)

Sample	Number of laboratories retained after eliminating outliers	Number of outliers (laboratories)	Number of accepted results	Mean value, $\bar{x}$	Repeatability standard deviation, $s_r$	Reproducibility standard deviation, $s_R$	RSD <sub>r</sub>	RSD <sub>R</sub>	Hor-Rat
				mg/100 g	mg/100 g	mg/100 g	% <sup>a</sup>	% <sup>b</sup>	
Infant formula powder milk based	16	3	13	357,3	3,56	13,10	1,00	3,67	0,78
Child formula powder milk based	16	0	16	443,6	1,96	15,8	0,44	3,56	0,79
Infant elemental powder	16	0	16	372,54	3,08	14,52	0,83	3,9	0,84
Adult nutritional RTF high fat – placebo	16	8	8	35,41	1,11	2,55	3,14 <sup>c</sup>	7,21 <sup>c</sup>	1,09
Adult nutritional RTF high protein – placebo	16	5	11	40,2	0,45	1,56	1,12	3,89	0,60
Child formula powder milk based – placebo	16	5	11	32,4	4,0	6,75	12,4 <sup>c</sup>	20,8 <sup>c</sup>	3,11
Infant formula RTF milk based – placebo	16	0	16	22,5	0,33	0,79	1,49	3,5	0,49
Infant elemental powder – placebo	16	0	16	358,9	1,88	8,03	0,52	2,24	0,48
Butter	13	1	12	375,5	6,31	13,03	1,68	3,47	0,75
Cheese	13	1	12	562,2	8,45	15,74	1,5	2,8	0,64
Whey protein concentrate	13	3	10	169,5	2,18	6,53	1,28	3,85	0,74
Whole milk powder	13	0	13	711,6	3,97	18,32	0,56	2,57	0,61
Whole milk	12	1	11	95,3	1,30	2,59	1,37	2,72	0,48
Whey powder	12	3	9	281,3	1,91	10,04	0,68	3,57	0,74
Requirements according to Reference [9]:							≤ 2 %	≤ 4 %	
<sup>a</sup> Relative standard deviation of repeatability. <sup>b</sup> Relative standard deviation of reproducibility. <sup>c</sup> Expired liquid samples possibly spoiled/separated.									