

First edition
2008-12-15

Corrected version
2009-02-15

**Plastics — Determination of thermal
conductivity and thermal diffusivity —
Part 2:
Transient plane heat source (hot disc)
method**

*Plastiques — Détermination de la conductivité thermique et de la
diffusivité thermique —*

Partie 2: Méthode de la source plane transitoire (disque chaud)

STANDARDSISO.COM : Click to view the full PDF of ISO 22007-2:2008



Reference number
ISO 22007-2:2008(E)

© ISO 2008

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 22007-2:2008



COPYRIGHT PROTECTED DOCUMENT

© ISO 2008

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	2
4 Principle	3
5 Apparatus	3
6 Test specimens	5
6.1 Bulk specimens	5
6.2 Anisotropic bulk specimens	6
6.3 Slab specimens	6
6.4 Thin-film specimens	6
7 Procedure	7
8 Calculation of thermal properties	9
8.1 Bulk specimens	9
8.2 Anisotropic bulk specimens	12
8.3 Slab specimens	13
8.4 Thin-film specimens	14
9 Calibration and verification	14
9.1 Calibration of apparatus	14
9.2 Verification of apparatus	14
10 Precision and bias	15
11 Test report	16
Bibliography	17

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 22007-2 was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*.

ISO 22007 consists of the following parts, under the general title *Plastics — Determination of thermal conductivity and thermal diffusivity*:

- *Part 1: General principles*
- *Part 2: Transient plane heat source (hot disc) method*
- *Part 3: Temperature wave analysis method*
- *Part 4: Laser flash method*

In this corrected version of ISO 22007-2:2008, Figure 3 has been amended to remove a horizontal line running between ΔU and the earth connection.

Introduction

A significant increase in the development and application of new and improved materials for broad ranges of physical, chemical, biological and medical applications has necessitated better performance data from methods of measurement of thermal-transport properties. The introduction of alternative methods that are relatively simple, fast and of good precision would be of great benefit to the scientific and engineering communities [1].

A number of measurement techniques described as contact transient methods have been developed and several have been commercialized. These are being widely used and are suitable for testing many types of material. In some cases, they can be used to measure several properties separately or simultaneously [2],[3].

A further advantage of some of these methods is that it has become possible to measure the true bulk properties of a material. This feature stems from the possibility of eliminating the influence of the thermal contact resistance (see 8.1.1) that is present at the interface between the probe and the specimen surfaces [1],[3],[4],[5],[6].

STANDARDSISO.COM : Click to view the full PDF of ISO 22007-2:2008

STANDARDSISO.COM : Click to view the full PDF of ISO 22007-2:2008

Plastics — Determination of thermal conductivity and thermal diffusivity —

Part 2: Transient plane heat source (hot disc) method

1 Scope

1.1 This part of ISO 22007 specifies a method for the determination of the thermal conductivity and thermal diffusivity, and hence the specific heat capacity per unit volume, of plastics. The experimental arrangement can be designed to match different specimen sizes. Measurements can be made in gaseous and vacuum environments at a range of temperatures and pressures.

1.2 This method is suitable for testing homogeneous and isotropic materials, as well as anisotropic materials with a uniaxial structure. In general, the method is suitable for materials having values of thermal conductivity, λ , in the approximate range $0,01 \text{ W}\cdot\text{m}^{-1}\cdot\text{K}^{-1} < \lambda < 500 \text{ W}\cdot\text{m}^{-1}\cdot\text{K}^{-1}$ and values of thermal diffusivity, α , in the range $5 \times 10^{-8} \text{ m}^2\cdot\text{s}^{-1} \leq \alpha \leq 10^{-4} \text{ m}^2\cdot\text{s}^{-1}$, and for temperatures, T , in the approximate range $50 \text{ K} < T < 1\,000 \text{ K}$.

NOTE The specific heat capacity per unit volume, C , can be obtained by dividing the thermal conductivity, λ , by the thermal diffusivity, α , i.e. $C = \lambda/\alpha$, and is in the approximate range $0,2 \text{ MJ}\cdot\text{m}^{-3}\cdot\text{K}^{-1} < C < 5 \text{ MJ}\cdot\text{m}^{-3}\cdot\text{K}^{-1}$. It is also referred to as the volumetric heat capacity.

1.3 The thermal-transport properties of liquids can also be determined, provided care is taken to minimize thermal convection.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 472, *Plastics — Vocabulary*

ISO 22007-1, *Plastics — Determination of thermal conductivity and thermal diffusivity — Part 1: General principles*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 472 and ISO 22007-1 and the following apply.

3.1 penetration depth

Δp_{pen}
measure of how far into the specimen, in the direction of heat flow, a heat wave has travelled

NOTE 1 For this method, the penetration depth is given by

$$\Delta p_{\text{pen}} = \kappa \sqrt{\alpha \cdot t_{\text{tot}}}$$

where

t_{tot} is the total measurement time for the transient recording;

α is the thermal diffusivity of the specimen material;

κ is a constant dependent on the sensitivity of the temperature recordings.

NOTE 2 It is expressed in metres (m).

3.2 probing depth

Δp_{prob}
measure of how far into the specimen, in the direction of heat flow, a heat wave has travelled during the time window used for calculation

NOTE 1 The probing depth is given by

$$\Delta p_{\text{prob}} = \kappa \sqrt{\alpha \cdot t_{\text{max}}}$$

where t_{max} is the maximum time of the time window used for calculating the thermal-transport properties.

NOTE 2 It is expressed in metres (m).

NOTE 3 A typical value in hot-disc measurements is $\kappa = 2$, which is assumed throughout this document.

3.3 sensitivity coefficient

β_q
coefficient defined by the equation

$$\beta_q = q \frac{\partial [\Delta T(t)]}{\partial q}$$

where

q is the thermal conductivity, λ , the thermal diffusivity, α , or the volumetric specific heat capacity, C ;

$\Delta T(t)$ is the mean temperature increase of the probe

NOTE 1 Different sensitivity coefficients are defined for thermal conductivity, thermal diffusivity and specific heat per unit volume [8].

NOTE 2 To define the time window that is used to determine both the thermal conductivity and diffusivity from one single experiment, the theory of sensitivity coefficients is used. Through this theory, which deals with a large number of experiments and considers the constants, q , as variables, it has been established that

$$0,30 \leq t_{\max} \cdot \alpha / r^2 \leq 1,0$$

where r is the mean radius of the outermost spiral of the probe.

Assuming $\kappa = 2$, this expression can be rewritten as


$$1,1r \leq \Delta p_{\text{prob}} \leq 2,0r$$

4 Principle

A specimen containing an embedded hot-disc probe of negligible heat capacity is allowed to equilibrate at a given temperature. A heat pulse in the form of a stepwise function is produced by an electrical current through the probe to generate a dynamic temperature field within the specimen. The increase in the temperature of the probe is measured as a function of time. The probe operates as a temperature sensor unified with a heat source (i.e. a self-heated sensor). The response is then analysed in accordance with the model developed for the specific probe and the assumed boundary conditions.

5 Apparatus

5.1 A schematic diagram of the apparatus is shown in Figure 1.

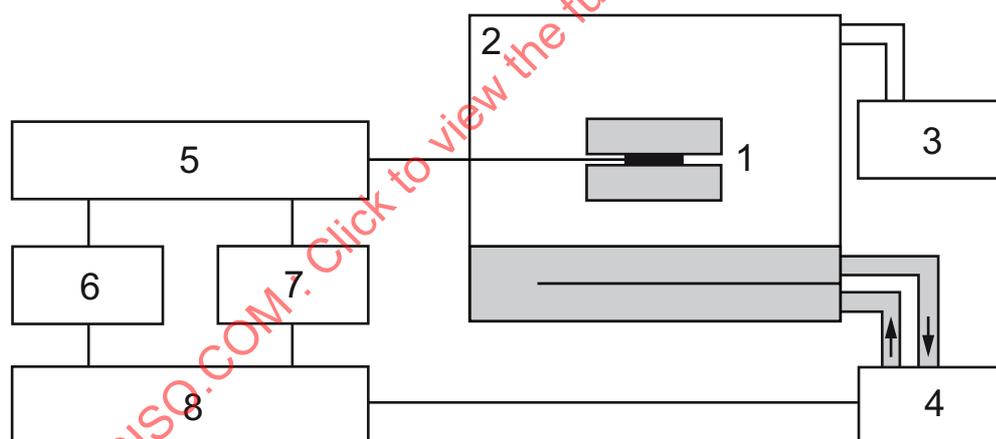

Key

1 specimen with probe	5 bridge circuit
2 chamber	6 voltmeter
3 vacuum pump	7 voltage source
4 thermostat	8 personal computer

Figure 1 — Basic layout of the apparatus

5.2 A typical hot-disc probe is shown in Figure 2. Convenient probes can be designed with diameters from 4 mm to 100 mm, depending on the specimen size and the thermal-transport properties of the material to be tested. The probe is constructed as a bifilar spiral etched out of a $(10 \pm 2) \mu\text{m}$ thick metal foil and covered on both sides by thin (from $7 \mu\text{m}$ to $100 \mu\text{m}$) insulating film. It is recommended that nickel or molybdenum be used as the heater/temperature-sensing metal foil due to their relatively high temperature coefficient of electrical resistivity and stability over a wide temperature range. It is recommended that polyimide, mica, aluminum nitride or aluminum oxide be used as the insulating film, depending on the ultimate temperature of use. The arms of the bifilar spiral forming an essentially circular probe shall have a width of $(0,20 \pm 0,03) \text{ mm}$ for probes with an overall diameter of 15 mm or less and a width of $(0,35 \pm 0,05) \text{ mm}$ for probes of larger diameter. The distance between the edges of the arms shall be the same as the width of the arms.

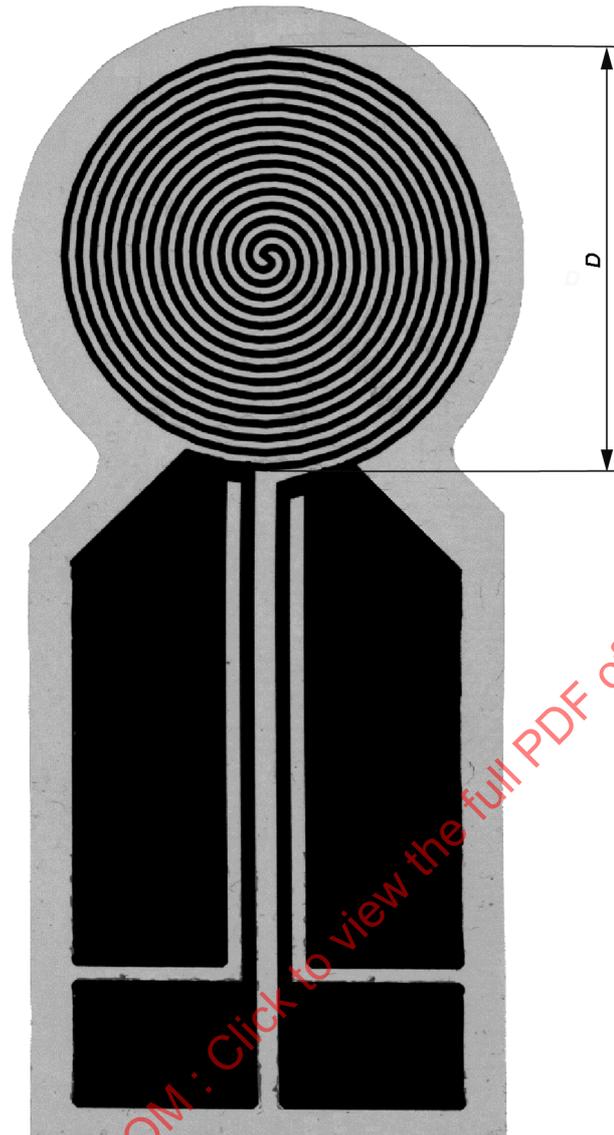
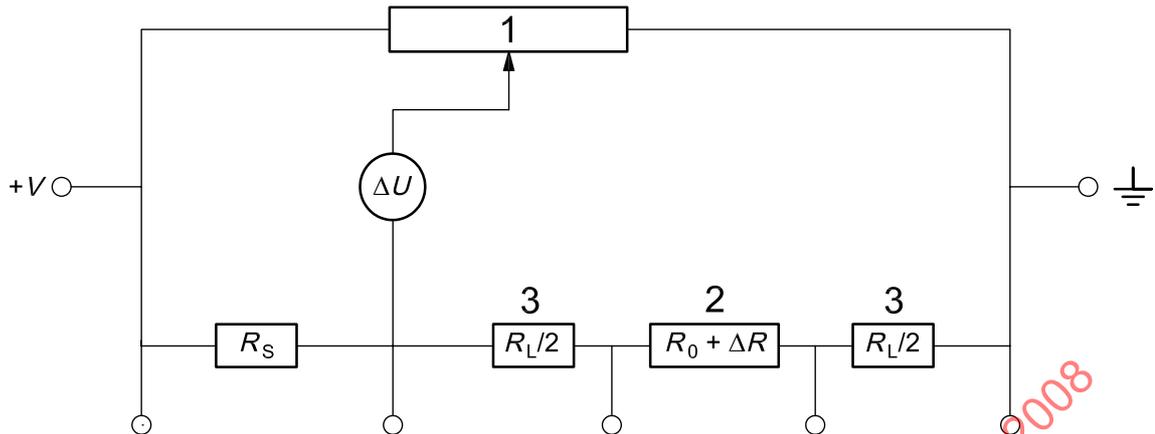


Figure 2 — Probe with bifilar spiral as heating/sensing element

(Sensor diameters, D , from 4 mm to 100 mm can be used, depending on available specimen size)

5.3 An electrical bridge shall be used to record the transient increase in resistance of the probe. Through the bridge, which is initially balanced, the successive increases in resistance of the probe shall be followed by recording the imbalance of the bridge with a sensitive voltmeter (see Figure 3). With this arrangement, the probe is placed in series with a resistor which shall be designed in such a way that its resistance is kept strictly constant throughout the transient. These two components are combined with a precision potentiometer, the resistance of which shall be about 100 times larger than the sum of the resistances of the probe and the series resistor. The bridge shall be connected to a power supply which can supply 20 V and a current of up to 1 A. The digital voltmeter by which the difference voltages are recorded shall have a resolution corresponding to 6,5 digits at an integration time of 1 power line cycle. The resistance of the series resistor, R_S , shall be close to the initial resistance of the probe with its leads, $R_0 + R_L$, in order to keep the power output of the probe as constant as possible during the measurement.

**Key**

- 1 potentiometer
- 2 probe
- 3 probe leads

Figure 3 — Diagram of bridge for recording the resistance increase of the probe

R_S is the series resistance, R_L is the total resistance of the probe leads, R_0 is the resistance of the probe before initiating the transient heating, ΔR is the increase in resistance of the probe during the transient heating and ΔU is the voltage imbalance created by the increase in the resistance of the probe.

NOTE This experimental arrangement allows the determination of temperature deviations from the iterated straight line (see treatment of experimental data in 8.1) down to or better than 50 μK .

5.4 A constant-temperature environment controlled to $\pm 0,1 \text{ K}$ or better for the duration of a measurement shall be established. The chamber need only be evacuated when working with slab specimens (see 6.3).

6 Test specimens

6.1 Bulk specimens

6.1.1 For bulk specimens, the requirement for specimen thickness depends on the thermal properties of the material from which the specimen is made. The expression for the probing depth contains the diffusivity, which is not known prior to the measurement. This means that the probing depth has to be calculated after an initial experiment has been completed. If, with this new information, the probing depth is outside the limits given in 8.1.3, the test shall be repeated, with an adjusted total measurement time, until the required conditions are fulfilled.

The shape of the specimen can be cylindrical, square or rectangular. Machining to a certain shape is not necessary, as long as a flat surface (see 6.1.4) of each of the two specimen halves faces the sensor and the requirements on the sensor size given in 8.1.3 are fulfilled.

6.1.2 The thickness of the specimen shall be at least 20 times the characteristic length of the components making up the material or of any inhomogeneity in the material, e.g. the average diameter of the particles if the specimen is a powder.

6.1.3 The specimen dimensions shall be chosen to minimize the effect that its outer surfaces will have on the measurement. The specimen size shall be such that the distance from any part of the bifilar spiral of the hot-disc probe to any part of the outside boundary of the specimen is larger than the overall mean radius of the bifilar spiral (see 5.2). An increase in this distance beyond the size of the diameter of the spiral does not improve the accuracy of the results.

6.1.4 Specimen surfaces which are in contact with the sensor shall be plane and smooth. The specimen halves shall be clamped on to both sides of the hot-disc probe.

NOTE Heat sink contact paste is not recommended since:

- a) it is difficult to obtain a sufficiently thin layer of paste which will actually improve the thermal contact;
- b) the paste obviously increases the heat capacity of the insulating layer and delays the development of the constant temperature difference between the sensing material and the specimen surface;
- c) it is difficult to obtain exactly the same thickness of paste on both sides of the probe and achieve a strictly symmetrical flow of heat from the heating/sensing material through the insulation into the two specimen halves.

6.1.5 For liquids, suitable containment vessels with adequate seals are necessary and air bubbles and evaporation shall be avoided.

Storage and conditioning of the liquid may affect its properties, e.g. by absorption of water or gas. It may be necessary to pretreat the specimen prior to testing, e.g. by degassing. However, pretreatment procedures shall not be used when they could detrimentally affect the material to be tested, e.g. through degradation.

6.1.6 For materials with which significant dimensional changes may occur, e.g. when making measurements over large temperature ranges, due to thermal expansion, a change of state, a phase transition or other causes, care shall be taken to ensure that, when placing the hot-disc probe in contact with the specimen, the applied load does not affect the properties of the specimen.

With soft materials, the clamping pressure shall not compress the specimen and thus change its thermal-transport properties.

6.1.7 The specimen shall be conditioned in accordance with the standard specification which applies to the type of material and its particular use.

6.2 Anisotropic bulk specimens

6.2.1 If a material is anisotropic, specimens shall be cut (or otherwise prepared) so that the probe can be oriented in the main directions (e.g. the fibre directions in reinforced plastics, the main directions in layered structures or the principal axes in crystals)^{[4],[7]}. The hot-disc method is limited to materials in which the thermal properties along two of the orthogonal and principal axes are the same, but are different from those along the third axis.

6.2.2 The size of anisotropic specimens shall be chosen so that the requirements of 8.1.3 are fulfilled along the principal axes.

6.3 Slab specimens

The so-called slab method is used with sheet-formed specimens extending in two dimensions, but with a limited and well-defined thickness in the range from 1 mm to 10 mm^[9]. The slab specimen thickness shall be known to an accuracy of 0,01 mm. When two equally thick slabs of a material are clamped around a probe and thermally insulated on the outer sides, it is possible to measure the thermal conductivity and diffusivity of such specimens. The condition related to the probing depth (see 3.2) has to be fulfilled in the plane of the probe but not in the through-thickness direction. This method is particularly suited to studies of materials having thermal conductivities higher than $10 \text{ W}\cdot\text{m}^{-1}\cdot\text{K}^{-1}$ but can also be used for materials with thermal conductivities as low as $1 \text{ W}\cdot\text{m}^{-1}\cdot\text{K}^{-1}$, provided good thermal insulation of the slabs can be arranged (for instance by performing the measurements in a vacuum).

6.4 Thin-film specimens

The so-called thin-film method is used with specimens such as paper, textiles, polymer films or deposited thin-film layers (such as ceramic coatings) with thicknesses ranging from 0,01 mm to 1,0 mm^[10]. The thickness of thin-film specimens (placed on both sides of the probe) shall be known to an accuracy of $\pm 1 \mu\text{m}$.

NOTE 1 When making a measurement on a material with a high thermal conductivity, the temperature undergoes a rapid increase at the very beginning of the transient followed by a much more gradual increase. The insulating layer, between which the sensing spiral is sandwiched, causes this rapid increase. It has been shown both experimentally and in computer simulations that the temperature difference across the insulating layer becomes constant within a very short time and remains constant throughout the measurement. The reason is that the total power output, the area of the sensing material and the thickness of the insulating layer are constant in the test.

If thin films of a material are placed between the probe and a high-conductivity background material (in the form of an "infinite" solid), it is possible to measure the thermal conductivity of the film material, provided that the thermal conductivity of the insulating layer with which the probe is covered has been determined in a separate experiment [10].

NOTE 2 It might be necessary to make measurements on films of different thicknesses or with different clamping pressures to eliminate mathematically the influence of thermal contact resistances.

The thermal conductivity of the background material shall be at least 10 times greater than that of the thin-film material.

In order to simulate better a plane heat source when testing thin films, a probe similar to the one depicted in Figure 2 shall be used. However, the circular strips should preferably have a width of 0,8 mm and the openings between the strips should only be 0,2 mm. When using a probe with thermal insulation on both sides of the bifilar spiral, an initial test to determine the effective thermal conductivity of the insulation and the adhesive holding the probe together shall be carried out.

7 Procedure

7.1 Place the probe between the plane surfaces of two specimen halves of the material whose thermal properties are to be determined.

Clamp or assemble the specimen/probe assembly securely in the test rig.

NOTE 1 When studying liquids, the probe is simply dipped into the liquid, often with an arrangement to keep the probe flat.

NOTE 2 The total temperature increase in the specimen is normally less than 2 K. This means that the thermodynamic state of the material under test hardly changes during the measurement process and the thermal properties can thus be ascribed to the equilibrium temperature attained prior to the test.

7.2 Assemble the complete system in a constant-temperature chamber and allow it to attain temperature stability as defined in 5.4.

7.3 Balance the electrical bridge prior to the test. For a sensor with an initial resistance between 1 Ω and 50 Ω , the voltage for balancing the bridge shall be selected such that the current does not exceed 1 mA.

7.4 Apply the heat pulse and record the temperature during a predetermined measuring time. Use values provided in Table 1 as an initial guide for the power output and the measurement time.

NOTE In general, a lower power output is preferred in order to minimize the perturbation of the system. However, it should be noted that the sensitivity of the temperature recording increases when the power output (and consequently the current) is higher, which is the case when studying materials with high thermal conductivity. For this reason, it is possible to obtain good precision in measurements on such materials even with temperature increases of only a fraction of a degree.

7.5 The voltage imbalance is determined and recorded at appropriate time intervals over the duration of the measurement time. It is recommended that the frequency of data acquisition be such that at least 100 data points are collected during the measurement time. If the method is used to measure the thermal-transport properties of liquids, the measurement time shall be limited to 1 s so that thermal convection in the liquid does not perturb the measurement.

Table 1 — Summary of recommended experimental parameters for a range of materials with different thermal conductivities

	Metal alloy	Dense ceramic	Steel	Ceramic	Polymer	Insulating material
Thermal conductivity [W/(m·K)]	170	40	14	1,5	0,19	0,028
Thermal diffusivity (mm ² /s)	69	11	3,7	0,96	0,11	0,75
Temperature increase (K)	0,3	0,5	1,0	0,8	1,3	2,5
Probe radius (mm)	15	6,4	6,4	6,4	6,4	15
Specimen thickness (mm)	30	10	10	10	15	30
Specimen diameter (mm)	90	40	40	40	40	90
Measurement time (s)	5	10	10	40	160	160
Power output (W)	4	3	2	0,5	0,25	0,1

7.6 The resolution of the equipment shall be better than 0,001 K.

7.7 Calculate the temperature increase from the voltage readings, $\Delta U(t)$, using the following equation:

$$\Delta T(t) = (R_S + R_L + R_0) \Delta U(t) [J_0 R_S - \Delta U(t)]^{-1} (a R_0)^{-1} \quad (1)$$

where

R_L is the total resistance of the leads;

R_S is the series resistance (see 5.3);

R_0 is the initial resistance of the probe;

a is the temperature coefficient of resistance (TCR) of the probe;

J_0 is the current through the sensor at the start of the transient — this current can easily be determined by measuring the voltage across the bridge at the end of the transient before the heating current is turned off and dividing by $(R_S + R_L + R_0)$ [1].

7.8 Change the test temperature successively to cover the desired temperatures for the specimen, making sure that temperature equilibrium is reached at each temperature.

Multiple measurements under the same experimental conditions should preferably be undertaken. At least three are recommended at the same temperature. Each consecutive measurement should be made after the system has stabilized at the initially chosen temperature. The time to reach thermal equilibrium will vary depending on specimen size, form and thermal properties.

Upon completion of the test at the highest temperature, it is recommended that a repeat measurement be made after cooling to one or more lower temperatures. This makes it possible to detect any degradation in the specimen properties that may have occurred due to exposure to elevated temperatures.

7.9 The thermal conductivity shall be reported along with the conditions under which it was measured such as temperature and pressure. Compositional variation of the material and its direction and orientation in the specimen shall be reported whenever a material is not homogeneous or isotropic.

8 Calculation of thermal properties

8.1 Bulk specimens

8.1.1 For small increases in the temperature of the probe, we have

$$R(t) = R_0 [1 + a \cdot \Delta T(t)] \quad (2)$$

where

$\Delta T(t)$ (= $T(t) - T_0$) is the mean temperature increase of the probe;

R_0 is the initial resistance of the probe at temperature T_0 ;

a is the temperature coefficient of resistance (TCR) of the probe.

The temperature increase can be seen as consisting of two parts. One part represents the temperature difference across the intercalated insulating layer and the other part the temperature increase of the specimen surface during the transient measurement. This can be expressed as

$$\Delta T(t) = \Delta T_i(t) + \Delta T_s(t) \quad (3)$$

where

$\Delta T_i(t)$ is the increase in temperature over the insulating layers of the probe;

$\Delta T_s(t)$ is the increase in the temperature of the specimen surface.

With the assumption that the bifilar probe can be approximated by a number of concentric and equally spaced circular line sources, the solution of the thermal conductivity equation (see Reference [1]) is given by

$$\Delta T_s(\tau) = P_0 (\pi^{3/2} r \lambda)^{-1} D(\tau) \quad (4)$$

where

P_0 is the power output of the probe;

r is the radius of the outermost ring source;

λ is the thermal conductivity of the specimen material;

τ is defined as

$$\tau = (t/\theta)^{1/2} \quad (5)$$

where $\theta = r^2 l \alpha$;

$D(\tau)$ is the dimensionless specific time function, defined as

$$D(\tau) = [m(m+1)]^{-2} \int_0^\tau \sigma^{-2} \left[\sum_{l=1}^m l \sum_{k=1}^m k \exp\left(\frac{-(l^2 + k^2)}{4m^2 \sigma^2}\right) I_0\left(\frac{lk}{2m^2 \sigma^2}\right) \right] d\sigma \quad (6)$$

in which

m is the number of concentric ring sources;

σ is the integration variable;

I_0 is a modified Bessel function.

Typical values of $D(\tau)$ are given in Figure 5.

A time correction, t_c , shall be introduced because of unavoidable hardware and software delays. This means that the development of the full power output of the sensor may not coincide exactly with the time $t = 0$, and a time correction shall be introduced accordingly. This is accomplished by replacing τ by τ_c in Equation (5), where

$$\tau_c = [(t - t_c)/\theta]^{1/2} \quad (7)$$

Typical time corrections are a fraction of a second and shall not be larger than 0,5 % of the total measurement time.

NOTE 1 $\Delta T_i(t)$ becomes constant after a short time provided the insulating layer is thin and the power output is constant. The time it takes to approach this constant value is determined by the relaxation time, δ^2/α_i , where δ is the thickness of the insulating layer and α_i is the thermal diffusivity of the layer. For a typical insulated probe, the relaxation time is less than 10 ms and the time required to reach a constant temperature difference is less than 100 ms.

NOTE 2 The possibility of determining the thermal contact resistance experimentally via the initial temperature difference, $\Delta T_i(t)$, enables the true bulk properties of the specimen material to be determined.


NOTE 3 If the thermal diffusivity and time correction are known (see 8.1.2), there is a linear relationship between the temperature increase, $\Delta T_s(t)$, and $D(\tau)$ [see Figure 4 b) where, in the example given, $\Delta T_i = 0,6566$ and $\Delta T_s(t) = 1,894D(\tau)$].

8.1.2 The calculation of thermal conductivity and diffusivity starts with an iteration procedure with the diffusivity, α , and the time correction, t_c , as optimization variables. Through iteration, a linear relationship between $\Delta T_s(t)$ and $D(\tau)$ is established (by a least-squares fitting procedure) and the diffusivity and time correction are obtained from the final step of the iteration procedure. Finally, λ is determined from the slope of this line [see Equations (4) and (5)].


8.1.3 The initial time window selected for the analysis may result in experimental points deviating from a straight line [see Figure 4 b)]. By removing deviating data points, a correct time window is obtained for the analysis. The graph of residuals [see Figure 4 c)] displays clearly the deviating points.

As the specimen is of limited size, its boundaries might, after some time, affect the temperature increase. This deviation will become apparent in the graph of residuals [see Figure 4 c)] and, if there are deviating points at the end of the transient, these shall also be deleted.

NOTE In view of the statistical nature of the expression used for the probing depth (see 3.2), it can be stated that the probing depth will have to be larger than the radius but less than the diameter of the bifilar spiral of the probe in order to determine both the thermal conductivity and the thermal diffusivity from one single transient recording.

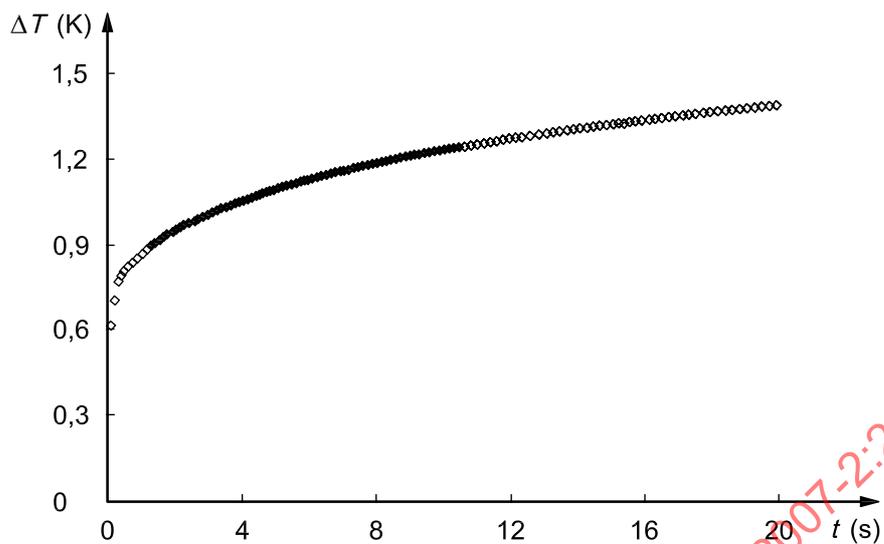

a) Temperature increase versus time

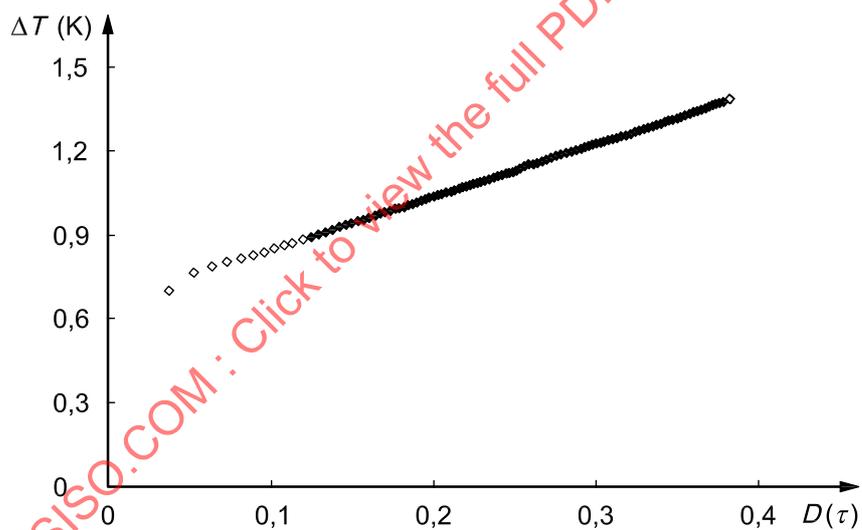


$$\Delta T = 1,894D(\tau) + 0,6566$$

$$R^2 = 0,99999913$$

b) Temperature increase versus $D(\tau)$

Figure 4 (continued)

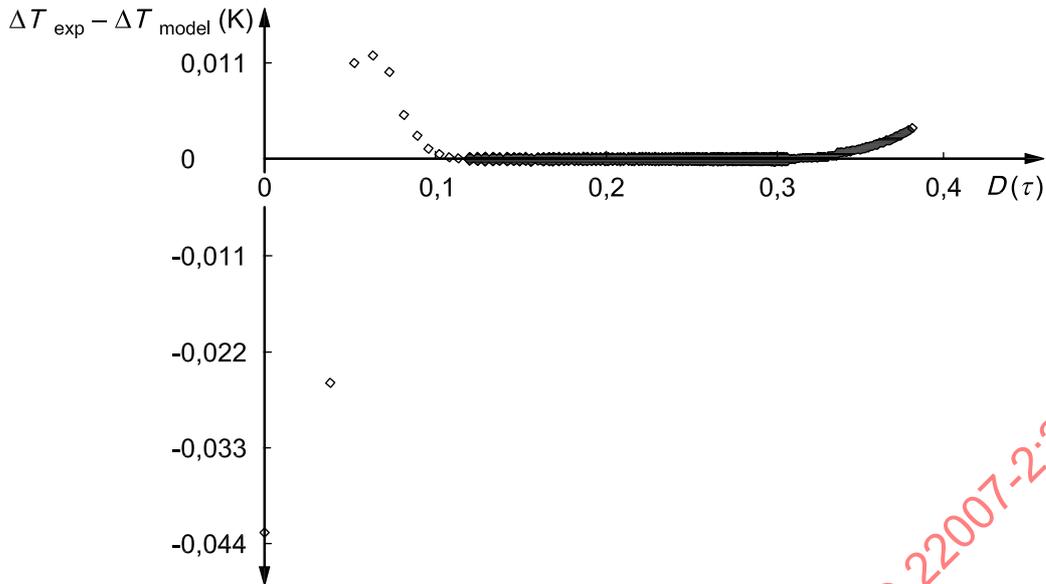

c) Temperature residuals versus $D(\tau)$

(The model fitting has been performed on the solid black points. The mean deviation of these points from the fitted straight line is 30 μ K.)

Key

- $D(\tau)$ specific time function
- R^2 correlation coefficient
- t time
- ΔT temperature increase
- $\Delta T_{\text{exp}} - \Delta T_{\text{model}}$ temperature residual

Figure 4 — Various temperature increase/time plots

8.2 Anisotropic bulk specimens

For anisotropic materials, a separate determination of specific heat and density is required since the specific heat capacity per unit volume is necessary to calculate the thermal properties. If the properties along the a - and b -axes are the same, but different from those along the c -axis, and if the plane of the probe is mapped out by the a - and b -axes, the following expression for the temperature increase applies:

$$\Delta T_s(\tau_a) = P_0 \left[\pi^{3/2} r (\lambda_a \lambda_c)^{1/2} \right]^{-1} D(\tau_a) \tag{8}$$

where

λ_a is the thermal conductivity along the a -axis;

λ_c is the thermal conductivity along the c -axis;

$$\tau_a = (t/\theta_a)^{1/2} \tag{9}$$

where $\theta_a = r^2/\alpha_a$.

An iteration — similar to the one presented in 8.1 — will give the thermal diffusivity, α_a , along the a -axis. If the specific heat capacity per unit volume, C , is known, then

$$\lambda_a = C \cdot \alpha_a \tag{10}$$

From the slope of the line corresponding to Equation (8), λ_c can be obtained since λ_a is known from Equation (10). Finally, the thermal diffusivity along the c -axis can be calculated from the standard relationship.

It is consequently possible to obtain the thermal conductivity and the thermal diffusivity in the principal directions in a uniaxial material from one single transient measurement, provided the specific heat capacity and density are known. (The heat capacity per unit volume is the product of the specific heat capacity and the density.)

8.3 Slab specimens

When solving the thermal-conductivity equation, the mathematical “method of images” has been used, with the assumption that no heat loss occurs from the upper and lower faces or the edges of the specimen. The temperature increase can then be expressed as

$$\Delta T_s(\tau) = P_0 \left(\pi^{3/2} r \lambda \right)^{-1} E(\tau) \quad (11)$$

where

$$E(\tau) = [m(m+1)]^{-2} \int_0^\tau \sigma^{-2} \left[\sum_{l=1}^m l \sum_{k=1}^m k \exp\left(\frac{-(l^2+k^2)}{4m^2\sigma^2}\right) I_0\left(\frac{lk}{2m^2\sigma^2}\right) \right] \left\{ 1 + 2 \sum_{i=1}^\infty \exp\left[-\frac{i^2}{\sigma^2} \left(\frac{h}{r}\right)^2\right] \right\} d\sigma; \quad (12)$$

h is the thickness of each of the two slabs;

σ is the integration variable.

Making the measurement in a vacuum or in still air normally fulfils the condition that the heat loss from the upper and lower faces and the edges of the specimen must be negligible. Figure 5 depicts $D(\tau)$ and examples of $E(\tau)$ functions.

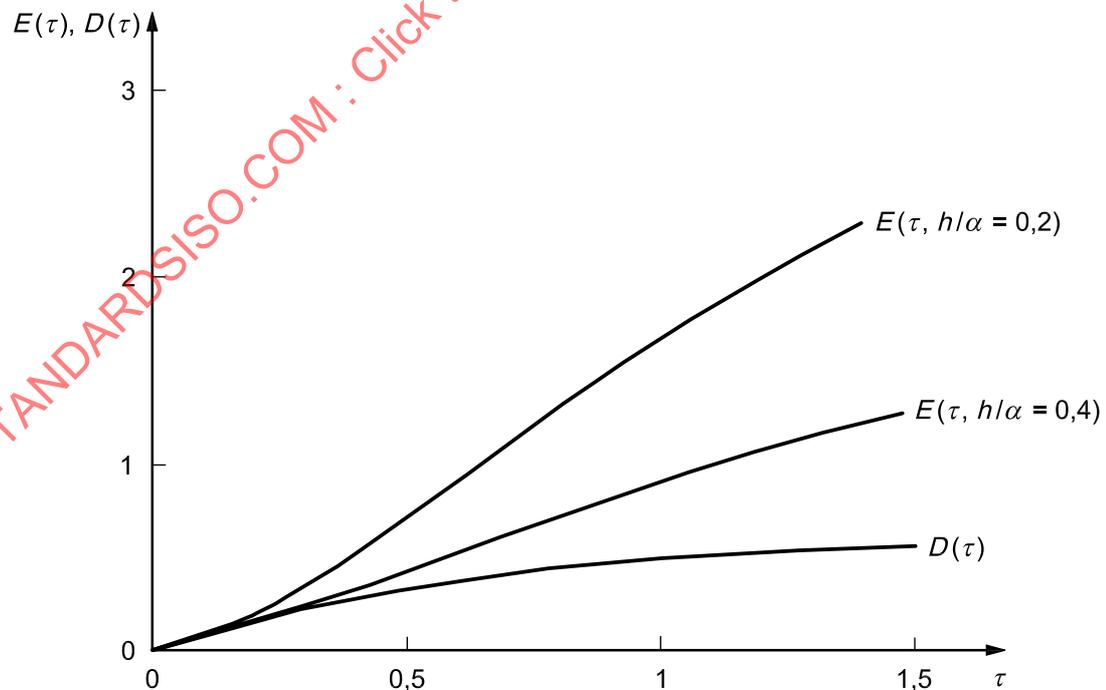


Figure 5 — $D(\tau)$ and $E(\tau)$ functions plotted for values of τ up to 1,5
(In all three cases, it has been assumed that the number of concentric ring sources is 10.)