

INTERNATIONAL
STANDARD

ISO
24681

First edition
2023-05

Ships and marine technology — Fibre-reinforced plastic gratings

STANDARDSISO.COM : Click to view the full PDF of ISO 24681:2023



Reference number
ISO 24681:2023(E)

© ISO 2023

STANDARDSISO.COM : Click to view the full PDF of ISO 24681:2023



COPYRIGHT PROTECTED DOCUMENT

© ISO 2023

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword.....	iv
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Classification.....	2
4.1 Types.....	2
4.1.1 General.....	2
4.1.2 Moulded grating.....	2
4.1.3 Pultruded grating.....	3
4.1.4 Other type gratings.....	3
5 Technical requirements.....	3
5.1 Appearance.....	3
5.2 Load-bearing capacity.....	4
5.3 Corrosion resistance.....	4
5.4 Skid resistance.....	4
5.5 Flame spread characteristics.....	4
5.6 Smoke and toxicity.....	4
5.7 Anti-electrostatic property.....	4
5.8 Fire integrity.....	5
5.9 UV resistance.....	5
5.10 Asbestos-free requirement.....	5
6 Inspection and test methods.....	5
6.1 Appearance.....	5
6.2 Load-bearing capacity test.....	5
6.3 Corrosion resistance.....	5
6.4 Skid resistance.....	5
6.5 Flame spread characteristics.....	6
6.6 Smoke and toxicity.....	6
6.7 Anti-electrostatic property.....	6
6.8 Fire integrity.....	6
6.9 UV resistance.....	6
7 Marking, packing and transportation.....	6
7.1 Marking.....	6
7.2 Packing.....	6
7.3 Transportation.....	6
Annex A (normative) Load-bearing capacity test (three-point bending method).....	7
Annex B (normative) FRP grating fire integrity test.....	10
Annex C (informative) FRP grating application guideline.....	12
Bibliography.....	14

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 8, *Ships and marine technology*, Subcommittee SC 8, *Ship design*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Ships and marine technology — Fibre-reinforced plastic gratings

1 Scope

This document specifies the structure, technical requirements and test methods of gratings for fibre-reinforced plastics (FRP) in the marine industry. It also defines terms related to FRP gratings.

This document is applicable to the design, manufacture and inspection of self-support FRP gratings used for pedestrian pathways and platforms on ships or offshore platforms.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 4892-3:2016, *Plastics — Methods of exposure to laboratory light sources — Part 3: Fluorescent UV lamps*

ISO 9227, *Corrosion tests in artificial atmospheres — Salt spray tests*

ISO 14125, *Fibre-reinforced plastic composites — Determination of flexural properties*

IMO, *International Code for Application of Fire Test Procedures (FTP Code)*, 2010

IMO, *International Convention for the Safety of Life at Sea (SOLAS)*, 1974 and amendment

ASTM D2047, *Test method for static coefficient of friction of polish-coated flooring surfaces as measured by the James machine*

ASTM E84, *Standard test method for surface burning characteristics of building materials*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

3.1

fibre reinforced plastic

FRP

composite material made of resin reinforced with fibre

Note 1 to entry: Glass fibres are widely used as reinforced fibre.

3.2

skid resistance

property of the trafficked surface which limits the relative movement between the contact patch of pedestrian footwear or a vehicle tyre and the surface

4 Classification

4.1 Types

4.1.1 General

Fibre reinforced plastic (FRP) grating is a kind of composite panel material with a certain aperture ratio, which is based on thermosetting resin and reinforced with fibreglass roving, and processed by special technology. The raw materials shall meet recognized standards and be specified in the technical specification, so as to ensure its continuous and stable performance.

FRP gratings are generally divided into two types, moulded or pultruded FRP gratings. For typical examples, see [Figure 1](#) and [Figure 2](#).

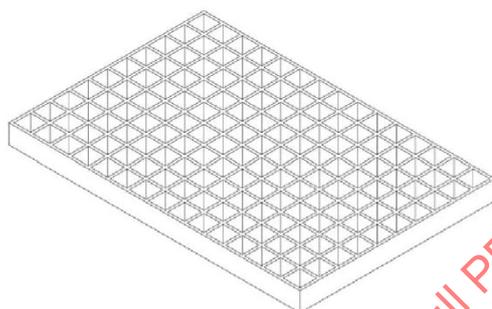


Figure 1 — Moulded grating

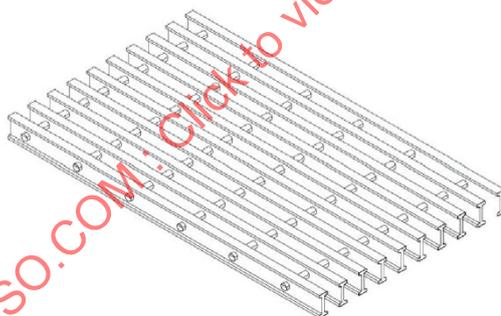


Figure 2 — Pultruded grating

4.1.2 Moulded grating

Moulded FRP gratings are produced by the open mould process in which thermosetting resin and dry glass fibre are placed in the mould in cross directions. After filling the mould with the designated amount of material, the resin is allowed to cure in the open mould. Moulded grating is usually manufactured in square mesh or rectangular mesh configurations. Square mesh moulded grating has nearly equal strength in longitudinal and transverse directions. Rectangular mesh has better strength along longitudinal direction. For the common mesh configuration, see [Table 1](#).

Table 1 — Common moulded FRP grating configuration

Dimensions in millimetres

Mesh size	Height	Web thickness Bottom thickness / top thickness
25,4 × 25,4	50	6/8
38,1 × 38,1	25	5/6,35
38,1 × 38,1	30	5/6,6
38,1 × 38,1	38	5/7
38,1 × 38,1	50	5,8/8,5
38,1 × 38,1	50	9/11,5
38,1 × 38,1	63	5,8/9
38,1 × 38,1	63	9/12
50,7 × 50,7	50	5,8/8,3
25,4 × 50,8	50	9/11,5
25,4 × 152,4	38	5/7
38,1 × 101,6	38	5/7
38,1 × 152,4	50	7/9

NOTE Moulded FRP gratings are in general with inverted trapezoidal web section. The bottom thickness is smallest depending on the mould. The top thickness is greater depending on the height.

4.1.3 Pultruded grating

Pultruded grating consists of longitudinal bearing bars secured in position by transverse bars. The reinforced fibre is impregnated by thermosetting resin and pultruded to make shaped bearing bar under compression and heat. The bearing bar profile is generally “I” or “T” shaped. The product has high strength along bearing bars direction and is suitable for large span use. Common specifications are shown in [Table 2](#).

Table 2 — Common pultruded FRP grating configuration

Dimensions in millimetres

Bearing bar	Width	Space	Height
I	15	10/15/23	25/30/38
T	25,4	12,7/25,4	50,8

NOTE The common transverse securing bar is arranged in 152,4 mm interval.

4.1.4 Other type gratings

Authorities are responsible for confirming other types of gratings of occupied areas for workers or machinery.

5 Technical requirements

5.1 Appearance

5.1.1 FRP grating shall be smooth and flat, with no obvious stratification, burr, crack, fibre exposure and impurities.

5.1.2 No pores larger than 3 mm in diameter are allowed. The number of pores between 1 mm and 3 mm in any 300 mm × 300 mm area shall not exceed 10.

5.1.3 The warpage shall be not more than 2,5 mm/m along bearing bar direction and not more than 5 mm/m in other directions.

5.2 Load-bearing capacity

5.2.1 The flexural strength of the FRP grating panel shall be not less than 345 MPa.

5.2.2 No crack, stratification or other destructive damage shall be observed when the FRP grating is subject to 1,5 times design load.

5.2.3 The design load of the FRP grating used in pedestrian pathways and platform of ship shall be 4 kN/m² uniform load or equivalent. The design load may be other than specified if it is dedicated for a certain load condition. The grating deflection in the middle point of span shall not be greater than 1/120 of the span under design load, and the maximum deflection shall not exceed 9 mm.

5.2.4 For FRP grating used as steps of stair ladders, 2 kN concentrated load applied at the middle of step shall also be considered. The deflection of the middle point of the tread shall not be greater than 1/200 of its span, and the maximum deflection shall not exceed 6 mm.

5.3 Corrosion resistance

FRP grating should have good corrosion resistance. Gratings used for exposed area or ballast tanks shall be designed with good resistance to sea water and high salt fog conditions. After the salt spray test, the load-bearing capacity shall meet the requirements of [5.2.1](#).

5.4 Skid resistance

FRP gratings should have good skid resistance. The average coefficient of friction of upper surface shall be not less than 0,75 for dry weather conditions.

5.5 Flame spread characteristics

When FRP grating is required to have low flame spread characteristics, the product shall be tested in accordance with the test for surface flammability specified in IMO FTP Code 2010, Annex 1, Part 5. The result shall meet the requirements for ceiling, bulkhead, or shall be in accordance with other equivalent standards such as ASTM E84, which specifies a flame spread index (FSI) of ≤ 25 .

5.6 Smoke and toxicity

When the FRP grating is required to not produce excessive quantities of smoke and toxic products or to not give rise to toxic hazards at high temperature, it shall be tested in accordance with the smoke and toxicity test specified in IMO FTP Code 2010, Annex 1. The result shall meet the requirements for ceiling, bulkhead, or shall be in accordance with other equivalent standards such as ASTM E84, which specifies a smoke development index (SDI) of ≤ 450 .

5.7 Anti-electrostatic property

FRP grating used in hazardous areas (as defined by IEC 61892-7) shall be of anti-electrostatic property, and their surface shall be conductive to avoid static accumulation. The resistance value shall not be greater than $10^5 \Omega$ for any 1 m range of any two points on the surface of the grating. The electrical conductivity shall not degrade due to slight wear on the surface and the static shall be transferable to the metal frame by means of securing fixture or other effective means. The grounding resistance at any point of the grating surface shall not be greater than $10^6 \Omega$.

5.8 Fire integrity

5.8.1 When fire integrity is required to be maintained for the pedestrian pathways and platform, the self-support FRP grating shall pass the fire integrity test level 1 (L1) or level 2 (L2), as specified in [Annex B](#).

5.8.2 The FRP grating without fire integrity requirements and not subject to fire resistance test shall be classed as level 0 (L0). L0 FRP grating may be used on a steel deck, operation platform, cargo hold access, void space and other areas.

5.8.3 For design and application of FRP grating, refer to [Annex C](#).

5.9 UV resistance

When used in weather exposed areas, the FRP grating should be UV resistant to avoid damage to its structural strength due to long-term weather exposure.

5.10 Asbestos-free requirement

The FRP grating shall meet the asbestos-free requirement of IMO, SOLAS, 1974, chapter II-1.

6 Inspection and test methods

6.1 Appearance

6.1.1 Appearance and pores shall be subject to visual inspection.

6.1.2 The warpage of the grating shall be measured. Place the grating face up horizontally on a flat surface and draw a straight line in the direction of extension and width. Measure the distance between the midpoint of the line and the top of the grating to check the degree of warping.

6.2 Load-bearing capacity test

6.2.1 The flexural strength of the FRP grating shall be tested in accordance with ISO 14125.

6.2.2 Load-bearing capacity of the FRP grating shall be tested in accordance with [Annex A](#). Loading force shall be increased evenly to design load. Deflection under groups of typical Span-Load shall be recorded including deflection under maximum span and applied design load.

6.2.3 When loading to 1,5 times design load, examine whether there are cracks, delamination phenomena on the grating.

6.3 Corrosion resistance

The corrosion resistance of FRP grating test shall be conducted in accordance with ISO 9227. The endurance test time shall be 720 h.

6.4 Skid resistance

The skid resistance of FRP grating test shall be conducted in accordance with ASTM D2047.

6.5 Flame spread characteristics

Flame spread characteristics shall be tested in accordance with the test for surface flammability specified in the IMO FTP Code, Annex 1, Part 5, or in accordance with equivalent standards such as ASTM E84.

6.6 Smoke and toxicity

Smoke and toxicity testing shall be conducted in accordance with the IMO FTP Code, Annex 1, Part 2, or in accordance with equivalent standards such as ASTM E84.

6.7 Anti-electrostatic property

A calibrated resistance measuring instrument shall be used to measure the resistance of two points of space which are 1 m apart. At least 3 groups shall be measured and no value shall exceed $10^5 \Omega$.

6.8 Fire integrity

The fire integrity of FRP grating shall be tested in accordance with [Annex B](#).

6.9 UV resistance

The FRP grating shall be subject to the accelerated weathering test for at least 720 h in accordance with ISO 4892-3:2016, Table 1 (Method A). No damage such as fracture, crack, blister, delamination or fibre exposure shall be found.

7 Marking, packing and transportation

7.1 Marking

7.1.1 FRP gratings that pass fire integrity test shall be marked with "L1" or "L2" in a prominent location. FRP gratings that are not subject to fire integrity tests shall be marked with "L0" in a prominent location.

7.1.2 FRP gratings that pass UV resistance tests shall be marked with "UV" in a prominent location.

7.2 Packing

7.2.1 FRP grating shall be packed with cardboard on the edge and tied properly.

7.2.2 Each FRP grating packing shall display handling instructions and transportation notice.

7.3 Transportation

7.3.1 The FRP grating shall be placed on a flat panel and safely secured on a vehicle.

7.3.2 It is not permitted to throw the grating during handling.

Annex A (normative)

Load-bearing capacity test (three-point bending method)

A.1 Test principle

Apply a linear load to the FRP grating for the three-point bending test. The load-bearing capacity is determined by measuring the deflection at the mid-point of the span under the corresponding load.

A.2 Test equipment

A.2.1 The test should be carried out on the universal material testing machine or a self-designed testing device. The loading capacity of the testing machine (or device) shall be more than 25 % higher than the required specimen test load.

A.2.2 The load measurement shall be accurate to 1 %.

A.2.3 Equipment for deflection measurement shall be accurate to 0,01 mm.

A.3 Specimen preparation

A.3.1 The length of the grating specimen shall be determined by [Formula \(A.1\)](#):

$$C \geq A + 150 \tag{A.1}$$

where

A is the test span, expressed in millimetres (mm);

NOTE Typical test spans can be: 300 mm, 450 mm, 600 mm, 750 mm, 900 mm, 1 050 mm, 1 200 mm and 1 500 mm.

C is the specimen length, expressed in millimetres.

A.3.2 Specimen width should be about 300 mm and shall include at least 6 bearing bars.


A.3.3 Each set of specimens shall not be less than 3 pieces.

A.4 Test conditions and equipment

A.4.1 The laboratory standard environmental conditions are ambient environment temperature $23\text{ °C} \pm 2\text{ °C}$ and relative humidity $50\% \pm 5\%$. If the laboratory standard environmental conditions are not available, other laboratories close to environmental standards should be selected.

A.4.2 The support and loading bars for test equipment should be smooth steel round bars of 310 mm long and 25 mm diameter, and the steel bars shall be properly fixed and shall not deform or rotate under load. The test load shall be applied at the middle of the transverse bar relative to support bar, as shown in [Figure A.1](#).

A.4.3 When the span length is less than 914 mm, the load speed is 6,35 mm/min, if not, the load speed is 12,7 mm/min.

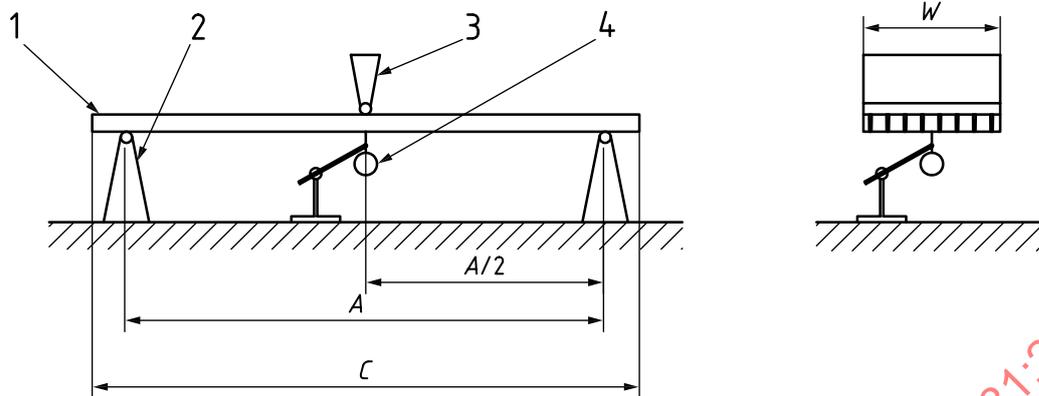

Key

- 1 FRP specimen
- 2 support
- 3 test load
- 4 deflection gauge
- A test span
- W specimen width
- C specimen length

Figure A.1 — Test equipment schematic diagram

A.5 Test procedure

A.5.1 The test load shall be determined by [Formula \(A.2\)](#):

$$P = (A \times W \times P_U) / 1,6 \tag{A.2}$$

where

- P* is the test load, expressed in kilonewtons (kN);
- P_U* is uniform load, expressed in kilonewtons (kN/m²);
- W* is the specimen nominal width, expressed in metres (m), $W = n/N$;
- n* is the number of bearing bars of the specimen;
- N* is the number of bearing bars per metre width (for example, when the centre-to centre spacing of support bars is 38 mm, $N = 27/m$; when the centre-to-centre spacing of support bars is 50 mm, $N = 21/m$).

A.5.2 The equipment for deflection measurement shall be correctly installed. When applying a 50 N initial load to the pultruded grating and a 100 N initial load to the moulded grating, examine and adjust the specimen and equipment for deflection measurement to put the whole system in a normal condition, then reset the load and deflection records to neutral.

A.5.3 The load shall be applied evenly up to the design load, and the maximum deflection shall be recorded.

A.5.4 When continuous loading is up to 1,5 times the design load, examine whether there are cracks or delamination phenomena on the grating.

STANDARDSISO.COM : Click to view the full PDF of ISO 24681:2023

Annex B (normative)

FRP grating fire integrity test

B.1 Specimen preparation

B.1.1 The grating specimen length is the maximum span permitted plus 200 mm, but not less than 1 300 mm.

B.1.2 The specimen width is about 300 mm and contains at least 6 bearing bars.

B.1.3 The specimen should be placed in the standard environmental conditions (temperature $23\text{ °C} \pm 2\text{ °C}$ and relative humidity $50\% \pm 5\%$) for 24 h. If the conditions are not available, they can also be placed in a drying oven for 24 h.

B.1.4 For fire integrity level 2 (L2), at least two specimens shall be prepared for each test. The specimens shall be numbered as specimen 1 and specimen 2, respectively.

B.1.5 For fire integrity level 1 (L1), at least four specimens shall be prepared for each test. The specimens shall be numbered as specimen 1, specimen 2, specimen 3, and specimen 4, respectively.

B.1.6 Specimen shall be taken from a random grating.

B.2 Test conditions and equipment

B.2.1 The tests shall be carried out in laboratories which are recognized by the relevant authorities.

B.2.2 The test shall be conducted in a test furnace that meets the requirements of standard fire test specified in the FTP code. The test shall also be conducted in accordance with the standard time-temperature curve determined by [Formula \(B.1\)](#), as defined by ISO 834-1:

$$T = 345 \log_{10} (8t + 1) + 20 \quad (\text{B.1})$$

where

T is the average furnace temperature (°C);

t is the time (min).

B.3 Test procedure

B.3.1 The specimen shall be placed horizontally in the test furnace according to the maximum support span, and the centre of the specimen shall be sufficiently far from the bottom of the furnace to ensure that the specimen will not touch the bottom during the whole test. When specimen 1 and specimen 2 are tested at the same time, sufficient spacing shall be kept to ensure that they do not affect each other during the test.

B.3.2 Specimen 1 shall be loaded 360 N at the span centre before the test starts, and the load should be a weight with a bottom surface of 300 mm × 300 mm. Other specimens are not loaded.

B.3.3 Start the test in accordance with the standard time-temperature curve specified in [Formula \(B.1\)](#). The test shall be carried out for 60 min. The average furnace temperature shall be recorded during the test at the following regular intervals:

- at 5 min, when the average furnace temperature is 576 °C and shall not vary more than ±15 %;
- at 10 min, when the average furnace temperature is 679 °C and shall not vary more than ±15 %;
- at 15 min, when the average furnace temperature is 738 °C and shall not vary more than ±10 %;
- at 30 min, the average furnace temperature is 841 °C and shall not vary more than ±5 %;
- at 60 min, the average furnace temperature is 945 °C and shall not vary more than ±2,5 %.

B.3.4 Record the time when the deflection of specimen 1 exceeds a distance that equals to 1/10 of the unsupported span length. The time shall be recorded within 6 s after the accident. Observe whether specimen 2 (or specimens 3, 4) collapse during the test.

B.3.5 Specimen 2 (or specimens 3, 4) shall be cooled naturally to room temperature in calm air.

B.3.6 After the furnace test, specimen 2 (or specimens 3, 4) test shall be loaded evenly to the design load in accordance with [Annex A](#) and the load shall be kept for 15 min.

B.3.7 Specimens 2, 3 and 4 that have passed the tests specified in [B.3.4](#) and [B.3.6](#) shall be supported and reinforced according to the maximum span. A shot bag is dropped from the height of 2 000 mm on each specimen. The minimum mass of the shot bag is 40 kg, and the impact point is the midpoint of the span.

B.3.8 Specimens 2, 3 and 4 that have passed the test specified in [B.3.7](#) shall be loaded again in accordance with [Annex A](#) and the load shall be kept for 15 min.

B.4 Acceptance criteria

The FRP grating passes the L2 fire integrity test if specimen 1 does not deform more than 1/10 of the span, or the time is over 15 min in the test described in [B.3.4](#), and specimen 2 does not collapse in the furnace test and during the subsequent load test described in [B.3.6](#).

The FRP grating passes the L1 fire integrity test if specimen 1 does not deform to more than 1/10 of the span or the time is over 15 min in the test described in [B.3.4](#), and specimens 2, 3, 4 do not collapse in the furnace test, and during the subsequent load tests described in [B.3.6](#), [B.3.7](#) and [B.3.8](#).

Annex C (informative)

FRP grating application guideline

The user of this guideline should ensure that the specifications are met when choosing the grating. [Table C.1](#) shows an FRP grating application matrix on ships or offshore platforms.

Table C.1 — FRP grating application matrix

Location	Service	Fire integrity	Flame spread characteristics	Smoke and toxicity
Machinery spaces of category A	All personnel access ladders, platforms or similar	L1	0	0
Other machinery spaces, cargo holds, cargo pump rooms	Personnel access ladders, platforms which may be used for escape, fire fighting, emergency operation or rescue	L2	0	—
	Personnel access ladders, platforms other than those described above	L0	0	—
Cargo tanks, fuel oil tanks	All personnel access ladders, platforms or similar	L0	—	0 ^[1]
Ballast water tanks, cofferdams, double bottoms, pipe tunnels, etc.	All personnel access ladders, platforms or similar	L0	—	—
Accommodation, service and control spaces	All personnel access ladders, platforms or similar	Not permitted	Not permitted	Not permitted
Lifeboat embarkation or temporary safe refuge stations	Platform or escape access to such area	L2	0	0

Key

L1, L2 FRP gratings which pass the fire integrity test.

L0 FRP gratings which are not subject to fire integrity test.

0 FRP gratings of low flame spreads or which would not produce excessive quantities of smoke and toxic products.

— No requirements or not applicable.

FRP gratings should be able to be used at ambient temperature from $-45\text{ }^{\circ}\text{C}$ to $55\text{ }^{\circ}\text{C}$.

FRP grating shall be anti-static when the location or area is defined as a hazardous area (see IEC 60092-502, IEC 61892-7:2007 or other applicable rules). FRP gratings used in such hazardous areas shall be of anti-static property in the above matrix.

As for the use of FRP grating in liquefied natural gas/liquefied petroleum gas storage tanks, although it is not necessary to use the grating at low temperature, the manufacturer shall prove that the grating is suitable for the desired purpose, and the surface is not affected by the low temperature cargo (liquefied natural gas/ liquefied petroleum gas).

When the FRP grating is used in fuel oil tanks or other oil, and chemical storage tank, the manufacturer shall prove that the grating is suitable for the desired purpose. The performance shall not degrade or contaminate the carried cargo.

Although the fire integrity of grating can be maintained after a fire, it is recommended that the grating is replaced after a significant fire, unless it is tested by the manufacturer and competent authority.