

---

---

**Plastics — Determination of total  
luminous transmittance and  
reflectance**

*Plastiques — Détermination de la transmission lumineuse totale et de  
la réflectance*

STANDARDSISO.COM : Click to view the full PDF of ISO 26723:2020



STANDARDSISO.COM : Click to view the full PDF of ISO 26723:2020



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Fax: +41 22 749 09 47  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
Foreword.....	iv
Introduction.....	v
<b>1 Scope.....</b>	<b>1</b>
<b>2 Normative references.....</b>	<b>1</b>
<b>3 Terms and definitions.....</b>	<b>1</b>
<b>4 Principle.....</b>	<b>1</b>
<b>5 Apparatus.....</b>	<b>2</b>
<b>6 Specimen.....</b>	<b>3</b>
<b>7 Conditioning.....</b>	<b>4</b>
<b>8 Procedure.....</b>	<b>4</b>
<b>9 Calculation procedure.....</b>	<b>5</b>
<b>10 Precision.....</b>	<b>5</b>
<b>11 Expression of results.....</b>	<b>5</b>
<b>12 Test report.....</b>	<b>6</b>
<b>Annex A (informative) Measurement examples of total luminous transmittance and total luminous reflectance.....</b>	<b>7</b>
<b>Annex B (informative) Derivation of formulae.....</b>	<b>10</b>
<b>Bibliography.....</b>	<b>11</b>

STANDARDSISO.COM : Click to view the full PDF of ISO 26723:2020

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

## Introduction

This document specifies not only the total luminous transmittance of colourless and transparent plastics that have been covered by ISO 13468-1, but also specifies the transmittance of translucent materials such as opal sheets and the reflectance of materials such as translucent and/or opaque sheets or films.

STANDARDSISO.COM : Click to view the full PDF of ISO 26723:2020

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 26723:2020

# Plastics — Determination of total luminous transmittance and reflectance

## 1 Scope

This document specifies the determination of total luminous transmittance and total luminous reflectance on clear, translucent or opaque plastics. Specimen shapes include moulded plaque or discs, films and sheets.

Fluorescent plastics and chromatic colour plastics are not covered by this document.

NOTE The scope of ISO 13468-1 shows that ISO 13468-1 covers planar transparent and substantially colourless plastics. The method in this document provide the way to trap diffused light and covers to measure translucent and opaque plastics.

## 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 291, *Plastics — Standard atmospheres for conditioning and testing*

ISO/CIE 11664-1, *Colorimetry — Part 1: CIE standard colorimetric observers*

ISO 11664-2, *Colorimetry — Part 2: CIE standard illuminants*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at <https://www.iso.org/obp>

— IEC Electropedia: available at <http://www.electropedia.org/>

### 3.1

#### total luminous transmittance

$\tau_t$

ratio of the transmitted luminous flux to the incident luminous flux when a collimated beam of light passes through a specimen

### 3.2

#### total luminous reflectance

$\rho_t$

ratio of the reflected luminous flux to the incident luminous flux when a collimated beam of light reflected on a specimen

## 4 Principle

When evaluating the total luminous transmittance of light diffusing material, the scattered light will go toward the edge of the specimen by its light diffusing property. This method intends to collect scattered

light from the edge of the specimen toward inside of the integrating sphere. This method is suitable for not only light diffusing materials but also clear materials.

This method can also evaluate total luminous reflectance of clear, translucent or opaque materials.

NOTE When evaluating the specimen which has almost zero absorption of light such as PMMA milky white, sum of total luminous transmittance and total luminous reflectance will be 100 % or around.

## 5 Apparatus

5.1 The apparatus shall consist of a stabilized light source, an associated optical system, an integrating sphere with ports, and a photometer comprising a photo-detector, signal processor and display unit or recorder (see [Figure 1](#)).

5.2 The light source and the photometer shall be used in conjunction with a filter to provide an output corresponding to the photopic standard luminous efficiency  $V(\lambda)$  (as defined in ISO/CIE 11664-1), which is identical to the colour-matching function  $\bar{y}(\lambda)$  specified in ISO/CIE 11664-1 under CIE standard illuminant D65 as specified in ISO 11664-2. The output of the photodetector shall be proportional to the incident flux, to within 1 % of the incident flux, over the range used. The spectral and photometric characteristics of the light source and photometer shall be kept constant during measurements.

5.3 The total port area (sum of area of the port a, b, c and d) shall not exceed 4,0 % of the internal reflecting area of the sphere. It is desirable for the diameter of integrating sphere to be not less than 150 mm to be big enough for a specimen to pull together the scatter light to the thickness direction of the specimen enough.

5.4 Ports a, b and c shall be centred on the same great circle of the sphere. The angle between line ac and line bc shall be 14°. Where the line ac means the line which links the centre of port c to the centre of port a, and the line bc means the line which links the centre of port b to the centre of port c. Port d shall not be in the great circle on the sphere with port a, b and c.


5.5 The light source and its associated optical system shall produce a collimated light beam, no ray of which makes an angle of more than 0,05 rad (3°) with the beam axis. The centre of light flux shall be matched up precisely with the centre of the port a. The cross-section of light flux shall be circular and have sharp image. The diameter of light flux at the port a shall be 0,5 to 0,6 times of specimen, excluding evaluation of reflectance for opaque specimen.

5.6 The white reference which is attached on the port c shall have the even high reflectance for all wavelengths of the visible ray. Barium sulfate and Polytetrafluoroethylene (PTFE) are suitable. The inner wall of the integrating sphere shall have a coating applied that has the same reflectance as a white reference.

5.7 The light trap which is attached on the port b or port c shall absorb light completely when port b or port c doesn't have specimen nor white reference attached.

5.8 When the specimen has higher haze and higher thickness, specimen shape shall be circular and loaded with specimen holder specified on the [Figure 3](#). The inner surface of specimen holder shall have metallic luster. Because the specimen holder can collect scattering light which go toward the edge of the specimen.

5.9 The photometer is attached on the port d. The photometer shall be fitted with baffles to prevent light falling on it directly from the specimen.

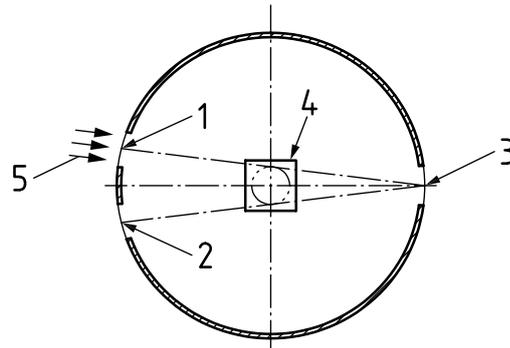

**Key**

- 1 port a
- 2 port b
- 3 port c
- 4 port d: photometer
- 5 incident light


**Figure 1 — Apparatus (integrating sphere and ports)**

## 6 Specimen

6.1 Specimen shall be machined from film, sheet, injection moulded article or compression moulded article. Specimen shall be flat. The thickness of specimen shall be original thickness.

6.2 There are two types of the specimen.

6.2.1 For the test without specimen holder, see [Figure 2](#).



**Key**


- 1 specimen
- 2 inner surface of integrating sphere

**Figure 2 — Specimen without specimen holder**

Diameter of the specimen shall be the range from 1,7 to 2,0 times of the diameter of the port.

This type covers the specimen which has thinner thickness than 10 % of the diameter of the port, or lower Haze than 30 %.

6.2.2 For the test with specimen holder, see [Figure 3](#).



**Key**

- 1 specimen
- 2 inner surface of integrating sphere
- 3 specimen holder
- 4 metallic surface

**Figure 3 — Specimen with specimen holder**

If the thickness of specimen is thicker than 10 % of the diameter of the port and the haze of the specimen is more than 30 %, specimen shall be set in the specimen holder. Edge of the specimen shall be painted with white paint which does not affect the specimen. The specimen shall be attached tightly to the inner surface of the specimen holder. The scattering light which goes toward the edge will go toward the inside of integrating sphere by the specimen holder and white paint.

6.3 Specimens shall be free of defects, dust, grease, adhesive from protecting materials, scratches and blemishes, and shall be free from visibly distinct internal voids and particles.

6.4 Three specimens shall be taken from each sample of a given material unless otherwise specified.

**7 Conditioning**

7.1 Prior to the test, condition the specimens in accordance with ISO 291, at 23 °C ± 2 °C and (50 ± 10) % relative humidity, unless otherwise specified in the applicable material specification, for a length of time dependent on the specimen thickness and material such that the specimens reach thermal equilibrium.

NOTE 16 h is usually sufficient for specimens less than 0,025 mm thick. For thicker material, more than 40 h can be used.

7.2 Set up the apparatus in an atmosphere maintained at 23 °C ± 2 °C and (50 ± 10) % relative humidity.

**8 Procedure**

Total luminous transmittance and reflectance shall be evaluated by the following procedure.

- a) Put the white reference on the port b and port c, and adjust the standard incident light ( $\tau_1$ ) as the instrument reading is 100.
- b) At the status of a), put the specimen on port a and read the instrument reading as transmitting light flux ( $\tau_2$ ).
- c) Then maintain the white reference on the port c, and put the light trap on the port b instead of white reference. Then, read the instrument reading as incident light flux in the light trap ( $\tau_3$ ).

- d) Then put the white reference on port b instead of the specimen, and put the specimen on port c instead of white reference. Then, read the instrument reading as reflection light flux ( $\tau_4$ ). On this procedure, specimen shall be covered by light trap or black felt unless otherwise the specimen is opaque.

**Table 1 — Conditions of evaluations of luminous transmittance and reflectance**

	Port a	Port b	Port c	Port d
Procedure a)	Vacant	White reference	White reference	photometer
Procedure b)	Specimen	White reference	White reference	photometer
Procedure c)	Vacant	Light trap	White reference	photometer
Procedure d)	Vacant	White reference	Specimen with light trap	photometer

## 9 Calculation procedure

Total luminous reflectance and total luminous transmittance are derived by [Formulae \(1\)](#) and [\(2\)](#).

$$\rho_t = \frac{\tau_4}{\tau_1 - (\tau_1 - \tau_3) \left(1 - \frac{\tau_4}{\tau_1}\right)} \times 100 \quad (1)$$

$$\tau_t = \frac{\tau_2}{2\tau_1 - \tau_3 - (\tau_1 - \tau_3) \left(1 - \frac{\rho_t}{100}\right)} \times 100 \quad (2)$$

where

$\tau_t$  is the total luminous transmittance (%);

$\rho_t$  is the total luminous reflectance (%);

$\tau_1$  is the standard incident light;

$\tau_2$  is the transmitting light flux;

$\tau_3$  is the incident light flux in the light trap;

$\tau_4$  is the reflection light flux.

NOTE See [Annex B](#) for derivations of [Formulae \(1\)](#) and [\(2\)](#).

## 10 Precision

Interlaboratory trials based on ISO 5725-2 have not been achieved at the time of publication. Measurements example of total luminous transmittance and total luminous reflectance are shown in [Table A.1](#), [Annex A](#).

## 11 Expression of results

Total luminous transmittance and total luminous reflectance shall be calculated to a decimal one column, and shall be expressed in accordance with following example.

EXAMPLE  $\tau_t = 60,2$  (%),  $\rho_t = 39,5$  (%)

## 12 Test report

The test report shall include at least the following:

- a) a reference to this document, i.e. ISO 26723:2020;
- b) name, type, thickness, size and shape of specimens;
- c) evaluation type (transmittance, reflectance or both);
- d) light incident surface if the surface property or appearance is different between two faces;
- e) average evaluation results of three specimens;
- f) model number and manufacturer of the equipment;
- g) other noticed issue which is out of the scope of this document;
- h) evaluation date.

STANDARDSISO.COM : Click to view the full PDF of ISO 26723:2020

## Annex A (informative)

### Measurement examples of total luminous transmittance and total luminous reflectance

#### A.1 Characteristics of this method

If light diffusing materials, like translucent plastics used for the cover of lighting fixture, are evaluated with ISO 13468-1, evaluating results are often shown lower than actual performance because of efficiency of the integrating sphere or edge-loss (edge-loss: light flux which scatter away from the edge of the specimen.) This document aims to maximize efficiency of the integrating sphere and minimizing edge-loss.

The efficiency of the integrating sphere is better as the opening ratio of the integrating sphere (the ratio of the opening area to the area inside the integrating sphere) is smaller.

Practically, integrating spheres with diameters of 150 mm to 300 mm are available and used.

The magnitude of edge-loss depends on specimen size, specimen thickness, optical properties (transmittance and diffusing property) and the diameter of incident light flux. Edge-loss will be smaller when the specimen size is bigger or specimen thickness is thinner, if the diameter of incident light flux is fixed.

Edge-loss is the phenomenon that incident light scatter from the edge of the specimen through diffusing and transmitting in the inside of the specimen. So, edge-loss will be higher when the specimen has higher transmittance and/or higher diffusibility. Hence, edge-loss will be smaller when the diameter of the incident light flux is smaller, because the distance from incident light to the edge of the specimen will be longer, and the amount of light which reaches the edge of the specimen from incident light will decrease.

## A.2 Measurement examples of total luminous transmittance and total luminous reflectance

Table A.1 — Measurement examples of total luminous transmittance and total luminous reflectance

Material	Colour	Thickness mm	Total luminous transmittance	Total luminous reflectance	$(\tau_t + \rho_t)$ %
			$\tau_t$ %	$\rho_t$ %	
PMMA	Clear	3	92,6	7,4	100,0
PMMA	White	2	9,8	89,4	99,2
PMMA	Milky white (High transmittance A)	5	71,6	26,8	98,4
PMMA	Milky white (High transmittance B)	2	75,2	27,7	102,9
PMMA	Milky white (Middle transmittance A)	5	56,0	42,6	98,6
PMMA	Milky white (Middle transmittance B)	5	41,7	57,7	99,4
PMMA	Milky white (Low transmittance A)	5	22,9	78,1	101,0
PMMA	Milky white (Low transmittance B)	3	30,4	70,9	101,3
PC	Milky white (Low transmittance)	2	34,8	59,5	94,3
PC	Milky white (Low transmittance)	5	30,3	61,0	91,3
PVC	Milky white (Middle transmittance)	2	54,4	44,4	98,8
PVC	Milky white (Middle transmittance)	3	47,9	47,4	95,3
PVC	Milky white (Middle transmittance)	5	41,5	47,1	88,6
Film 1	Translucent	23 <sup>a</sup>	89,8	8,4	98,2
Film 2	Translucent	35 <sup>a</sup>	73,8	24,6	98,4

<sup>a</sup> Expressed in  $\mu\text{m}$ .

## A.3 Measurement examples of the difference between ISO 13468-1 and this document

Measurement examples of the difference between ISO 13468-1 and this document are shown below [Table A.2](#).

For clear specimen and relatively thinner milky white PMMA (2 mm thickness or around), measurement results are similar between these two methods. But for thicker milky white specimen (6mm thickness or around), difference of measurement results between these two methods tend to increase. Especially, for high transmittance milky white specimen is easy affected from edge-loss, because incident light is easy to reach the edge of the specimen.