

---

**INTERNATIONAL STANDARD**



**3405**

---

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION • МЕЖДУНАРОДНАЯ ОРГАНИЗАЦИЯ ПО СТАНДАРТИЗАЦИИ • ORGANISATION INTERNATIONALE DE NORMALISATION

---

**Petroleum products — Determination of distillation characteristics**

*Produits pétroliers — Détermination des caractéristiques de distillation*

**First edition — 1975-02-15**

STANDARDSISO.COM : Click to view the full PDF of ISO 3405:1975

---

**UDC 665.6/.7 : 536.423**

**Ref. No. ISO 3405-1975 (E)**

**Descriptors :** petroleum products, tests, test equipment, distillation, characteristics.

Price based on 13 pages

## FOREWORD

ISO (the International Organization for Standardization) is a worldwide federation of national standards institutes (ISO Member Bodies). The work of developing International Standards is carried out through ISO Technical Committees. Every Member Body interested in a subject for which a Technical Committee has been set up has the right to be represented on that Committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work.

Draft International Standards adopted by the Technical Committees are circulated to the Member Bodies for approval before their acceptance as International Standards by the ISO Council.

International Standard ISO 3405 was drawn up by Technical Committee ISO/TC 28, *Petroleum products*, and circulated to the Member Bodies in November 1973.

It has been approved by the Member Bodies of the following countries :

Australia	Hungary	Romania
Austria	India	South Africa, Rep. of
Belgium	Iran	Spain
Bulgaria	Ireland	Sweden
Canada	Israel	Thailand
Chile	Korea, Rep. of	Turkey
Czechoslovakia	Mexico	United Kingdom
Egypt, Arab Rep. of	Netherlands	U.S.A.
France	Poland	U.S.S.R.
Germany	Portugal	Yugoslavia

No Member Body expressed disapproval of the document.

# Petroleum products — Determination of distillation characteristics

## 1 SCOPE AND FIELD OF APPLICATION

This International Standard specifies a procedure for determination of the distillation characteristics of motor gasolines, aviation gasolines, aviation turbine fuels, special boiling point spirits, naphthas, white spirit, kerosine, gas oils, distillate fuel oils, and similar petroleum products.

NOTE — For the distillation of aviation turbine fuels and other products of such wide boiling range that the low distillation thermometer specified in Group 3 of table 1 is inadequate, this method may be applied by substituting the high distillation thermometer, together with the other test conditions specified in Group 3 (see 8.3).

## 2 DEFINITIONS

**2.1 initial boiling point** : Temperature noted (corrected if required) at the moment when the first drop of condensate falls from the tip of the condenser during a distillation carried out under standardized conditions.

**2.2 end point; final boiling point** : Maximum temperature noted (corrected if required) during the final phase of a distillation carried out under standardized conditions.

**2.3 dry point** : Temperature noted (corrected if required) at the moment of vaporization of the last drop of liquid at the bottom of a flask during a distillation carried out under standardized conditions.

NOTE — The end point (final boiling point), rather than the dry point, is intended for general use. The dry point may be reported in connection with special purpose naphthas, such as those used in the paint industry. Moreover, it should be substituted for the end point (final boiling point) whenever the sample is of such a nature that the precision of the end point (final boiling point) cannot consistently meet the criteria given in clause 9.

**2.4 decomposition point** : Thermometer reading which coincides with the first indications of thermal decomposition of the liquid in the flask.

NOTE — Characteristic indications of thermal decomposition are an evolution of fumes and erratic thermometer readings which usually show a decided decrease after any attempt has been made to adjust the heat.

**2.5 volume recovered** : The volume, in millilitres, of condensate observed in the receiving graduated cylinder at a temperature which is read simultaneously with the volume.

**2.6 percentage recovered** : The maximum per cent recovered, as observed in accordance with 7.7.

**2.7 total percentage recovered** : The combined percentage recovered and residue in the flask, as observed in accordance with 7.8.

**2.8 percentage loss** : 100 minus the total percentage recovered.

**2.9 percentage residue** : The total percentage recovered minus the percentage recovered, or the volume of residue, in millilitres, if measured directly.

**2.10 percentage evaporated** : The sum of the percentage recovered and the percentage loss.

## 3 PRINCIPLE

A 100 ml test portion is distilled under prescribed conditions which are appropriate to the nature of the product (see table 1). Systematic observations of thermometer readings and volumes of condensate are made and the results are calculated from these data.

TABLE 1 — Test conditions

	Group 1	Group 2	Group 3	Group 4
<b>Sample characteristics</b>				
Vapour pressure at 37,8 °C (ISO 3007)	≥ 0,65 bar	< 0,65 bar	< 0,65 bar	< 0,65 bar
<b>Distillation :</b>				
— initial boiling point <sup>1)</sup>	.....	.....	≤ 100 °C	> 100 °C
— end point	≤ 250 °C	≤ 250 °C	> 250 °C	> 250 °C
<b>Preparation of apparatus</b>				
Distillation thermometer (see 4.8)	Low temperature range	Low temperature range	Low temperature range	High temperature range
Diameter of hole in flask support	50 mm	50 mm	50 mm	50 mm
<b>Temperature at start of test :</b>				
— flask and thermometer	13 to 18 °C	13 to 18 °C	13 to 18 °C	≤ ambient
— flask support and shield	≤ ambient	≤ ambient	≤ ambient	.....
— graduated cylinder and 100 ml charge	13 to 18 °C	13 to 18 °C	13 to 18 °C	13 °C to ambient
Flask (see 4.1)	125 ml	125 ml	125 ml	125 ml
<b>Conditions during test procedure</b>				
Temperature of condenser bath	0 to 1 °C	0 to 4 °C	0 to 4 °C	0 to 60 °C <sup>2)</sup>
Temperature of medium around graduated cylinder	13 to 18 °C	13 to 18 °C	13 to 18 °C	within ± 3 °C of temperature of distillation charge
Time from first application of heat to initial boiling point	5 to 10 min	5 to 10 min	5 to 10 min	5 to 15 min
Time from initial boiling point to 5 % recovered	60 to 75 s	60 to 75 s	.....	.....
Uniform average rate of condensation from 5 % recovered to 5 ml residue in flask	4 to 5 ml/min			
Time from 5 ml residue to end point	3 to 5 min	3 to 5 min	≤ 5 min	≤ 5 min

1) As determined under all test conditions of the group concerned.

2) The proper condenser bath temperature will depend upon the wax content of the sample and of its distillation fractions. The minimum temperature which permits satisfactory operation should be used.

#### 4 APPARATUS

Typical assemblies of the apparatus are shown in figures 2 and 3.

NOTE — Limited data have been obtained which indicate that certain types of automatic distillation apparatus are capable of giving test results which correspond in level and precision with those obtained by the manual procedures of this method, when the apparatus has been calibrated according to the manufacturer's instructions. When carrying out determinations in accordance with this International Standard, such automatic apparatus may only be used by agreement between the parties to the test, and provided the type of apparatus is mentioned in the test report.

##### 4.1 Distillation flask

Flasks shall be of heat-resistant glass and constructed to the dimensions and tolerances shown in figure 1.

##### 4.2 Condenser and cooling bath

Typical types of condenser and cooling bath are illustrated in figures 2 and 3. Other types of apparatus may be used, provided the test results obtained by their use are such as to satisfy the precision criteria of clause 9.

4.2.1 The condenser shall be made of seamless brass tubing, 560 mm in length. It shall be 14 mm in outside diameter and shall have a wall thickness of 0,8 to 0,9 mm.

4.2.2 The condenser shall be set so that approximately 390 mm of the tube will be in contact with the cooling medium, with about 50 mm outside the cooling bath at the upper end, and about 114 mm outside at the lower end. The portion of tube projecting at the upper end shall be set at an angle of 75° to the vertical. The portion of the tube

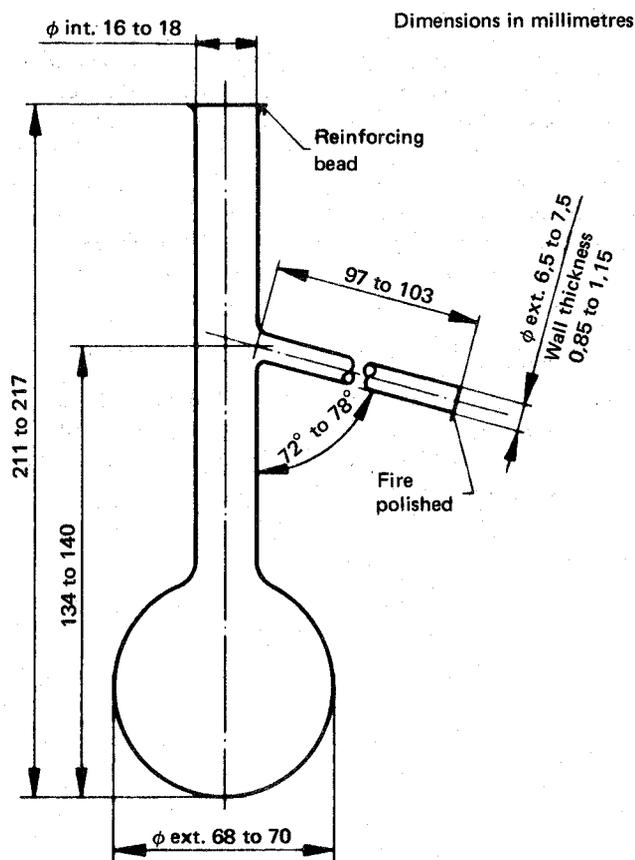


FIGURE 1 — Distillation flask

inside the cooling bath may be either straight or bent in any suitable continuous smooth curve. The average gradient shall be 0,26 mm per linear millimetre of condenser tube (equivalent to an angle of  $15^\circ$ ), and no section of the immersed portion of the condenser tube shall have a gradient less than 0,24 mm nor more than 0,28 mm per linear millimetre of condenser tube. The projecting lower portion of the condenser tube shall be curved downward for a length of 76 mm and slightly backward so as to ensure contact with the wall of the receiving graduated cylinder at a point approximately 25 to 32 mm below the top of the graduated cylinder when it is in position to receive the distillate. The lower end of the condenser tube shall be cut off at an acute angle so that the tip may be brought into contact with the wall of the graduated cylinder.

**4.2.3** The capacity of the cooling bath shall be not less than 5,5 l of cooling medium. The arrangement of the tube in the cooling bath shall be such that its centre line is not less than 32 mm below the plane of the top of the bath at its point of entrance and not less than 19 mm above the floor of the bath at its exit.

**4.2.4** Clearances between the condenser tube and the walls of the bath shall be at least 13 mm except for the sections adjacent to the points of entrance and exit. Multiple tube installations are permissible, provided they conform to the dimensional requirements (4.2.2 and 4.2.3) and the capacity of the bath is not less than 5,5 l per tube.

### 4.3 Metal shield or enclosure for flask

**4.3.1 Type 1 shield** (figure 2) is 480 mm high, 280 mm long, and 200 mm wide, made of sheet metal of approximately 0,8 mm thickness. It shall have a door on one narrow side, and two openings 25 mm in diameter, equally spaced in each of the two narrow sides, with a slot cut in one side for the vapour tube. The centres of these four openings shall be 215 mm below the top of the shield. There shall be three holes of approximately 13 mm in each of the four sides with their centres 25 mm above the base of the shield.

**4.3.2 Type 2 shield** (figure 3) is 440 mm high, 200 mm long, and 200 mm wide, made of sheet metal of approximately 0,8 mm thickness and with a window on the front side. The open bottom of the shield shall be spaced approximately 50 mm from the base of the unit. The rear of the shield shall have an elliptical hole for the vapour tube. A flask-adjusting knob shall be located in front of the shield for adjusting the flask support. If an electric heater (figure 3) is used, it shall be fitted with a stepless heat control unit with an indicating dial. The heater and heat controller shall be built into the lower part of the shield; the remaining portion of the shield above the flask support board (4.5.2) shall be the same as that used for the gas burner; the lower portion, however, may be omitted and the heater, control unit and upper part of the shield supported in any convenient manner.

### 4.4 Heat source

**4.4.1 Gas burner** (figure 2), so constructed that sufficient heat from the available gas can be obtained to distil the product at the specified rate. A sensitive regulating valve and gas-pressure governor to give complete control of heating may be provided.

**4.4.2 Electric heater** (figure 3) may be used instead of a gas burner, provided it is capable of distilling the product at the specified rate. Heater units of low heat retention, adjustable from 0 to 1 000 W, have been found satisfactory.

### 4.5 Flask support

**4.5.1 Type 1 for use with gas burner** (figure 2). A ring support of the ordinary laboratory type, 100 mm or larger in diameter, supported on a stand inside the shield, or a platform adjustable from the outside of the shield, may be used.

**4.5.1.1** Two ceramic or hard asbestos boards, 3 to 6 mm in thickness, shall rest upon the ring or the platform, whichever is used. The board immediately above the ring or platform shall have a central opening 76 to 100 mm in diameter and outside line dimensions slightly smaller than the inside boundaries of the shield.

4.5.1.2 The second or flask support board shall be slightly smaller in outside dimensions than the first board and shall have a central opening of 50 mm in diameter. It shall be 3 to 6 mm in thickness at the centre-hole rim. This flask support board may be moved slightly in accordance with the directions for placing the distillation flask, and direct heat shall be applied to the flask only through the opening in this board.

4.5.2 Type 2 for use with electric heater (figure 3). The top of the electric heater shall consist of a ceramic or hard asbestos flask support board with a central opening of 50 mm in diameter. It shall be 3 to 6 mm in thickness at the centre-hole rim. Provision shall be made for moving the heater unit, with its top, in order to place the distillation flask so that direct heat will be applied to the flask only through the opening in the flask support board.

#### 4.6 Graduated cylinder

The graduated cylinder shall have a capacity of 100 ml and be graduated at intervals of 1 ml. The shape of the base is optional but it shall be such that the receiver does not topple when placed empty on a surface inclined at an angle of 15° to the horizontal.

Construction details and tolerances for the graduated cylinder are shown in figure 4. The use of a Crow receiver is permitted provided that the vertical dimension and the scale length are as shown in the figure.

#### 4.7 Cooling bath for cylinder

An optional cooling bath (see note to 6.7) such as a clear glass or plastics tall-form beaker of sufficient height to allow the graduated cylinder to be immersed up to the 100 ml graduation line in a cooling liquid.

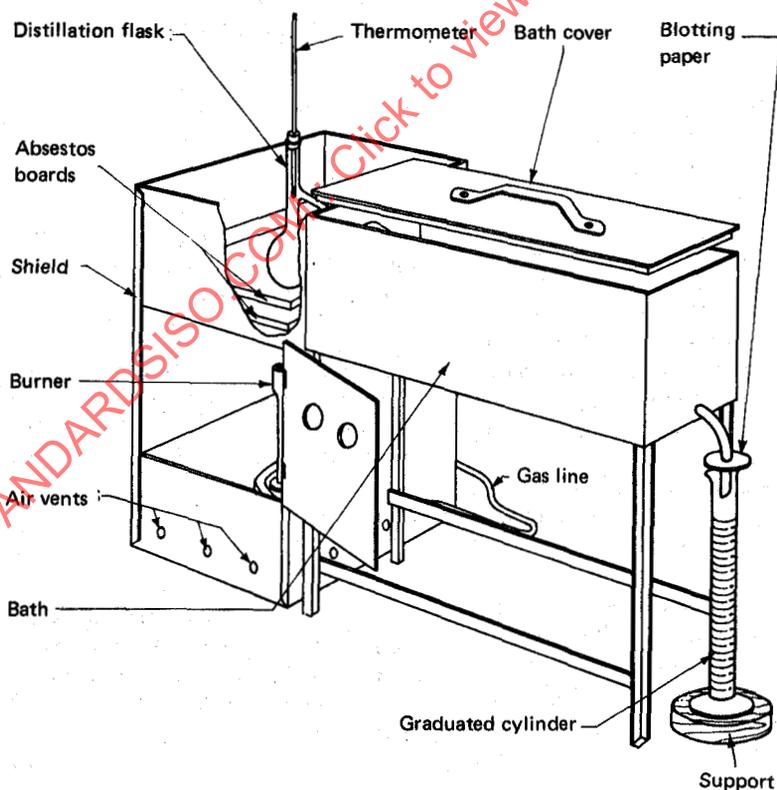


FIGURE 2 – Apparatus assembly using gas burner

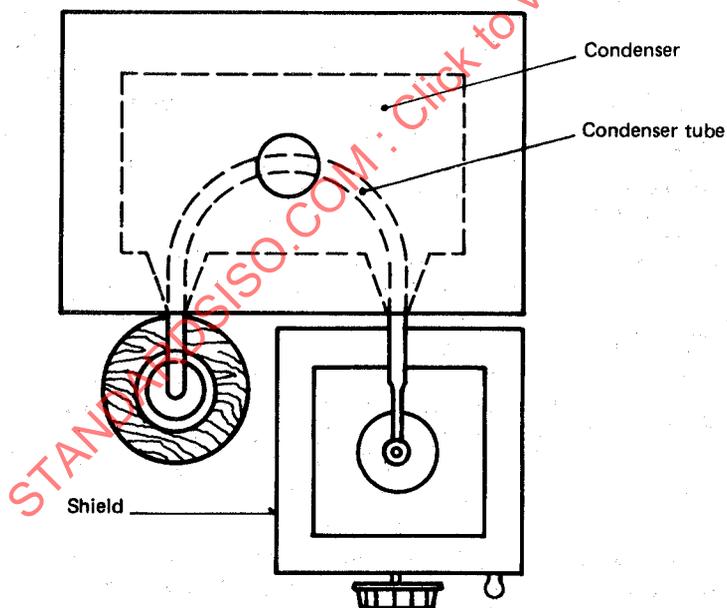
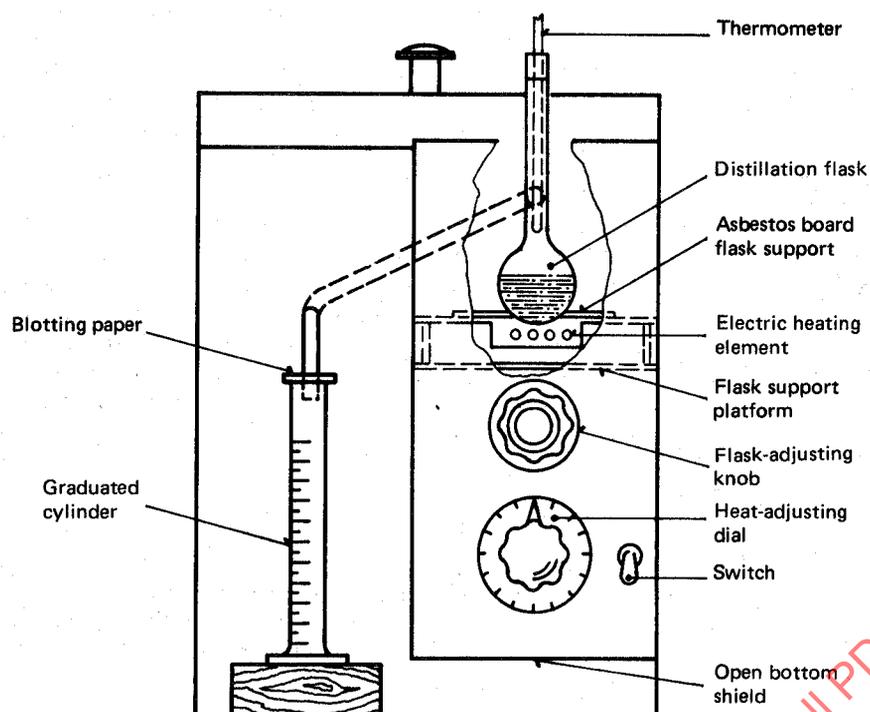


FIGURE 3 — Apparatus assembly using electric heater

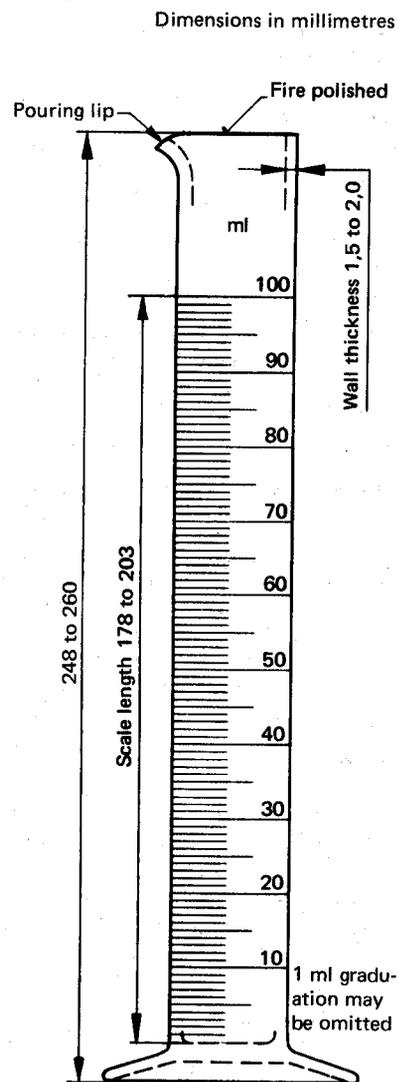


FIGURE 4 — Graduated cylinder  
100 ml in 1 ml graduations  
Tolerance  $\pm 1,0$  ml

4.8 Thermometer<sup>1)</sup>

The thermometer shall be of the mercury-in-glass type, nitrogen filled, graduated on the stem, enamel backed, and shall conform to the following requirements :

Application	Low temperature range	High temperature range
Range	- 2 to + 300 °C	- 2 to + 400 °C <sup>2)</sup>
Subdivisions	1 °C	1 °C
Immersion	total	total
Overall length	381 to 391 mm	381 to 391 mm
Stem diameter	6 to 7 mm	6 to 7 mm
Bulb shape	cylindrical	cylindrical
Bulb length	10 to 15 mm	10 to 15 mm
Bulb diameter	5 to 6 mm	5 to 6 mm
Distance from bottom of bulb to 0 °C line	100 to 110 mm	25 to 45 mm
Distance from bottom of bulb to 300 °C line	333 to 354 mm	-
Distance from bottom of bulb to 400 °C line	-	333 to 354 mm
Longer lines at each	5 °C	5 °C
Figured at each	10 °C	10 °C
Scale error, max.	0,5 °C, up to 300 °C	1,0 °C, up to 370 °C
Maximum line width	0,23 mm	0,23 mm
Expansion chamber	-	required <sup>3)</sup>
Heat stability	see note	see note

NOTE — Thermometers should be artificially aged by means of a suitable heat treatment before graduation in order to secure stability of zero. This treatment should be such that after the procedure described below, the maximum error is within the limits specified.

Heat the thermometer to a temperature corresponding to its highest scale line and keep it at this temperature for 5 min. Allow the thermometer to cool, either naturally in still air, or slowly in the test bath at a reproducible rate to 20° above ambient temperature or to 50 °C, whichever is the lower, then determine the error at a selected reference point. If natural cooling in air is used the error should be determined within 1 h. Heat the thermometer again to a temperature equal to its highest scale line and keep it at this temperature for 24 h, allow it to cool to one of the two temperatures referred to above, at the same rate as in the first part of the test, and redetermine the error under the same conditions as before.

5 SAMPLING

5.1 In the case of a product having a Reid vapour pressure of 0,65 bar or higher, cool the sample bottle to 13 to 18 °C. Collect the sample in the previously cooled bottle, preferably by immersing the bottle in the liquid, where possible, and discarding the first filling. Where immersion is

not possible, draw off the sample into the previously cooled bottle in such a manner that agitation is kept to a minimum. Close the bottle immediately with a tight-fitting stopper, and place it in an ice bath or refrigerator capable of maintaining the sample at a temperature not exceeding 15 °C.

5.2 Samples of materials that visibly contain water are not suitable for testing. If the sample is not dry, and the expected initial boiling point is below 66 °C, obtain for the test another sample which is free from suspended water. If the expected initial boiling point is above 66 °C, shake the sample with anhydrous sodium sulphate or other suitable drying agent and separate it from the drying agent by decanting.

6 PREPARATION OF APPARATUS

6.1 Refer to table 1 and select the thermometer which is required for the sample to be tested. Bring the respective temperatures of the flask, thermometer, graduated cylinder, flask support, and shield to their required values for starting the test.

6.2 Fill the condenser box to cover the condenser tube with any non-flammable coolant such as chopped ice, water, brine, or ethylene glycol solution which is suitable for the temperature specified in table 1. If chopped ice is used, add sufficient water to cover the condenser tube. If necessary, make suitable provision, such as circulation, stirring, or air blowing, so as to maintain the required condenser bath temperature throughout the test. Similarly, make any necessary provision so that the temperature of the bath around the graduated cylinder will remain within the limits specified in table 1.

6.3 Remove any residual liquid in the condenser tube by swabbing with a piece of soft, lint-free cloth attached to a cord or copper wire.

6.4 Bring the temperature of the sample within the range prescribed in table 1. Measure 100 ml of the sample in the graduated cylinder and transfer it as completely as practicable to the distillation flask, taking care that none of the liquid flows into the vapour tube.

6.5 Fit the thermometer, provided with a snug-fitting, well-rolled cork, tightly into the neck of the flask so that the bulb is centred in the neck and the lower end of the capillary is level with the highest point on the bottom of the inner wall of the vapour tube.

1) Thermometers ASTM 7C and 8C, and IP 5C and 6C are suitable.

2) Under certain test conditions, the bulb of the thermometer may be 28 °C above the temperature indicated by the thermometer, and at an indicated temperature of 371 °C the temperature of the bulb is approaching a critical range in the glass. If a thermometer is used at an indicated temperature above 371 °C it should not be re-used without checking the ice point.

3) An expansion chamber is provided for relief of gas pressure to avoid distortion of the bulb at higher temperatures. It is not for the purpose of joining mercury separations. Under no circumstances should the thermometer be heated above the highest temperature reading.

**6.6** Place the flask containing the charge in its support and make a tight connection with the condenser tube by means of a cork through which the vapour tube has been passed. Adjust the flask so that it is in a vertical position and so that the vapour tube extends into the condenser tube for a distance of 25 to 50 mm.

**6.7** Place the graduated cylinder that was used to measure the charge, without drying, into its bath under the lower end of the condenser tube so that the end of the condenser tube is centred in the graduated cylinder and extends into it for a distance of at least 25 mm but not below the 100 ml mark. Cover the graduated cylinder closely with a piece of blotting paper, or similar material, suitably weighted, which has been cut to fit the condenser tube snugly. Maintain the level of the bath around the graduated cylinder so that it is at least as high as the 100 ml mark.

NOTE — If the temperature of the air surrounding the cylinder does not meet the requirements of table 1 a cooling bath (4.7) should be used and the cylinder immersed so that the liquid covers the 100 ml graduation line.

**6.8** Record the prevailing barometric pressure, and proceed at once with the distillation, as specified in clause 7.

## 7 PROCEDURE

**7.1** Apply heat to the distillation flask and its contents. Regulate the heating at this stage so that the time interval between the first application of heat and the initial boiling point is within the limits prescribed in table 1.

**7.2** Immediately after observing the initial boiling point, move the graduated cylinder so that the tip of the condenser touches its inner wall. Continue to regulate the heating so that the rate of condensation into the graduated cylinder is uniform and within the limits prescribed in table 1. Repeat any distillation which did not meet the conditions prescribed in table 1.

**7.3** In the interval between the initial boiling point and the end of the distillation, observe and record whatever data are necessary for the calculation and reporting of the results of the test as prescribed in clause 8. These observed data may include thermometer readings at prescribed percentages recovered, or percentages recovered at prescribed thermometer readings, or both. Record all volumes in the graduated cylinder to the nearest 0,5 ml and all thermometer readings to the nearest 0,5 °C.

**7.4** If either a thermometer reading of 370 °C or a decomposition point is observed, discontinue the heating and proceed as directed in 7.7. Otherwise, proceed as directed in 7.5.

**7.5** When the volume of residual liquid in the flask is approximately 5 ml, make a final adjustment of the heat, if necessary, so that the time from the 5 ml of liquid residue in the flask to the end point (final boiling point) meets the

requirement given in table 1. If this condition is not satisfied, repeat the test, with appropriate modification of the final heat adjustment.

**7.6** Observe and record the end point (final boiling point) or dry point, or both, as required, and discontinue the heating. At the end point (final boiling point), observe if all the liquid has evaporated from the bottom of the flask. If not include a note of this fact in the report as prescribed in clause 8.

**7.7** While the condenser tube continues to drain into the graduated cylinder, observe the volume of condensate at 2 min intervals until two successive observations agree. Measure this volume accurately, and record it, to the nearest 0,5 ml, as percentage recovered. If the distillation was previously discontinued under the conditions given in 7.4, deduct the percentage recovered from 100, report this difference as percentage residue and loss, and omit the procedure given in 7.8 and 7.9.

**7.8** After the flask has cooled, pour its contents into the condensate in the graduated cylinder and allow to drain until no appreciable increase in the volume of liquid in the graduated cylinder is observed. Record this volume to the nearest 0,5 ml as total percentage recovered.

NOTE — As an alternative procedure, drain the cooled liquid remaining in the flask into a small cylinder graduated in 0,1 ml, and observe its volume. Add this observed volume to the percentage recovered, in order to obtain total percentage recovered.

**7.9** Deduct the total percentage recovered from 100 to obtain the percentage loss.

## 8 EXPRESSION OF RESULTS

**8.1** For each test, calculate and report whatever data are required by the specification involved, or as customarily established for the sample under test.

In cases in which no specific data requirements have been indicated, record the initial boiling point, the end point (final boiling point) or dry point, or both, and thermometer readings at 5 % and 95 % recovered and at each multiple of 10 % recovered from 10 to 90, inclusive.

**8.2** Report all percentages to the nearest 0,5, all thermometer readings to the nearest 0,5 °C, and the barometric pressure to the nearest 0,5 mbar.

**8.3** When testing aviation turbine fuels and similar products, pertinent thermometer graduations may be obscured by the cork. To provide the desired data, the distillation of a new test portion according to Group 3 of table 1 may have to be performed. In such cases the test report should identify such substituted data. If, by agreement, reporting these data is waived, this shall be mentioned in the test report.

8.4 If the report is to be based on thermometer readings corrected to 1 013 mbar barometric pressure (see note), obtain the correction to be applied to each thermometer reading by means of the Sydney Young equation as given below, or by the use of table 2. After applying the corrections and rounding each result to the nearest 0,5 °C, use the corrected thermometer readings in all further calculations and reporting.

$$C = 0,000\ 090 (1\ 013 - p) (273 + t)$$

where

*C* is the correction to be added algebraically to the observed thermometer reading (convenient approximations of these corrections are given in table 2);

*p* is the barometric pressure, in millibars, prevailing at the time of the test;

*t* is the observed thermometer reading, in degrees Celsius.

NOTE — Thermometer readings, when given in product definitions or specifications, or both, should be based on 1 013 mbar atmospheric pressure. Observed thermometer readings should be corrected to 1 013 mbar pressure when comparing test data or judging compliance with specifications, or both. If the results are not required for comparison with other data corrected to 1 013 mbar, or if the test is being carried out to check compliance with a specification which does not call for the data to be corrected to 1 013 mbar, the application of the barometric corrections shall be optional. When reporting data, state whether the corrections have or have not been applied.

8.5 After barometric corrections of the thermometer readings have been made, if required, the following data require no further calculation prior to reporting: initial boiling point, dry point, end point (final boiling point), decomposition point, percentage recovered, total percentage recovered, and all pairs of corresponding values involving percentages recovered and thermometer readings. Percentage loss and percentage residue are calculated in accordance with their respective definitions as set forth in 2.8 and 2.9.

8.6 It is advisable to base the report on relationships between thermometer readings and percentages evaporated in any case in which the sample is a gasoline, or any other product classed under Group 1 in table 1, or in which the percentage loss is greater than 2,0. Otherwise, the report may be based on relationships between thermometer readings and percentages evaporated or recovered.

Every report must indicate clearly which basis has been used.

8.7 To report percentages evaporated at prescribed thermometer readings, add the percentage loss to each of the observed percentages recovered at the prescribed thermometer readings, and report these results as the respective percentages evaporated.

TABLE 2 — Approximate corrected thermometer readings

Temperature range	Correction <sup>1)</sup> per 10 mbar difference in pressure
°C	°C
10 to 30	0,26
30 to 50	0,29
50 to 70	0,30
70 to 90	0,32
90 to 110	0,34
110 to 130	0,35
130 to 150	0,38
150 to 170	0,39
170 to 190	0,41
190 to 210	0,43
210 to 230	0,44
230 to 250	0,46
250 to 270	0,48
270 to 290	0,50
290 to 310	0,52
310 to 330	0,53
330 to 350	0,56
350 to 370	0,57
370 to 390	0,59
390 to 410	0,60

1) To be added if the barometric pressure is below 1 013 mbar; to be subtracted if the barometric pressure is above 1 013 mbar.

8.8 To report thermometer readings at prescribed percentages evaporated, use either of the two following procedures, and indicate in the test report whether the graphical procedure or the arithmetical procedure has been used.

8.8.1 Graphical procedure

Using graph paper with uniform subdivisions, plot each thermometer reading (corrected for barometric pressure, if required) against its corresponding percentage recovered. Plot the initial boiling point at 0% recovered. Draw a smooth curve connecting the points. For each prescribed percentage evaporated, deduct the percentage loss, in order to obtain the corresponding percentage recovered, and read from the graph the thermometer reading which this percentage recovered indicates (see note). Values obtained by graphical interpolation procedures are affected by the care with which the plot is made.

NOTE — See the annex for a numerical example illustrating the graphical procedure.

**8.8.2 Arithmetical procedure**

Deduct the distillation loss from each prescribed percentage evaporated in order to obtain the corresponding percentage recovered (see notes 1 and 2). Calculate each required thermometer reading as follows :

$$T = T_L + \frac{(T_H - T_L)(R - R_L)}{(R_H - R_L)}$$

where

*T* is the thermometer reading at the prescribed percentage evaporated;

*R* is the percentage recovered corresponding to the prescribed percentage evaporated;

*R<sub>H</sub>* is the percentage recovered adjacent to, and higher than *R*, at which a thermometer reading *T<sub>H</sub>* was noted;

*R<sub>L</sub>* is the percentage recovered adjacent to, and lower than *R*, at which a thermometer reading *T<sub>L</sub>* was noted.

**NOTES**

1 Values obtained by the arithmetical procedure are affected by the extent to which the distillation graph is non-linear. Intervals between successive data points must, at any stage of the test, be at least as narrow as indicated in the second paragraph of 8.1. In no case shall a calculation be made which involves extrapolation.

2 See the annex for a numerical example illustrating the arithmetical procedure.

**8.9** If a specification includes a maximum percentage loss or a minimum percentage recovered, or both, the actual loss shall be corrected to 1 013 mbar atmospheric pressure, according to the equation given below. The corresponding corrected percentage recovered is computed on the basis that it is greater than the actual recovery by the same amount as the corrected loss is less than the actual loss. Either or both of these corrected data shall be so designated and included in the test report, for the purpose of judging compliance with specifications.

$$\text{Corrected loss} = AL + B$$

where

*L* is the percentage loss as calculated from test data;

*A* and *B* are numerical constants, the values of which depend upon the barometric pressure. The values for these constants at different pressures are listed in table 3.

**9 PRECISION**

The precision of the method, as determined by statistical examination of interlaboratory test results, is as follows :

**9.1 Repeatability**

The difference between successive test results, obtained by the same operator with the same apparatus under constant operating conditions on identical test material, will in the

**TABLE 3 — Values of the constants *A* and *B* used in obtaining corrected distillation loss**

Observed barometric pressure	<i>A</i>	<i>B</i>
mbar		
747	0,231	0,384
760	0,240	0,380
773	0,250	0,375
787	0,261	0,369
800	0,273	0,363
813	0,286	0,357
826	0,300	0,350
840	0,316	0,342
853	0,333	0,333
866	0,353	0,323
880	0,375	0,312
893	0,400	0,300
906	0,428	0,286
920	0,461	0,269
933	0,500	0,250
946	0,545	0,227
960	0,600	0,200
973	0,667	0,166
986	0,750	0,125
1 000	0,857	0,071
1 013	1,000	0,000

long run, in the normal and correct operation of the test method, exceed the value obtained by the use of the nomogram in figure 5 only in one case in twenty.

**9.2 Reproducibility**

The difference between two single and independent results, obtained by different operators working in different laboratories on identical test material, will in the long run, in the normal and correct operation of the test method, exceed the value obtained by the use of the nomogram in figure 5 only in one case in twenty.

**9.3** To facilitate the use of figure 5 the rate of change in thermometer reading in degrees Celsius per the percentage evaporated or recovered (see note), at any point between the initial boiling point and the end point (final boiling point) or dry point, should be assumed to be the same as the average rate between two data points which are equidistant above and below the point in question. The span from the point in question to either of the other data points should not represent more than 10 % evaporated or recovered in any case, nor more than 5 % if the point in question is not included in the 10 to 90 % range. For the initial boiling point, end point (final boiling point), or dry

point, the rate of change should be assumed to be the same as the average rate over an interval, not to exceed 5 % evaporated or recovered, between the extreme point and the next data point above or below it.

NOTE — The "rate of change in thermometer reading" referred to above is calculated from the expression

$$\frac{\Delta t}{R_2 - R_1}$$

where

$\Delta t$  is the rise in temperature during the distillation interval;

$R_1$  is the percentage evaporated (recovered) at the beginning of the interval;

$R_2$  is the percentage evaporated (recovered) at the end of the interval.

9.4 In figure 5 it will be noted that the left and right marginal scales, representing the rate of change in thermometer reading, are identical. This is to facilitate the establishing of a horizontal line across the chart and at the required level, which may be done in any convenient manner. Noting the point where this line intersects the appropriate precision scale, the zone in which such intersection falls indicates the expected repeatability or reproducibility.

STANDARDSISO.COM : Click to view the full PDF of ISO 3405:1975