
**Iron ores for blast furnace
feedstocks — Determination of the
reducibility by the rate of reduction
index**

*Minerais de fer pour charges de hauts fourneaux — Détermination de
la réductibilité à partir de la vitesse de réduction*

STANDARDSISO.COM : Click to view the full PDF of ISO 4695:2015



STANDARDSISO.COM : Click to view the full PDF of ISO 4695:2015



COPYRIGHT PROTECTED DOCUMENT

© ISO 2015, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
5 Sampling, sample preparation and preparation of test portions	1
5.1 Sampling and sample preparation.....	1
5.2 Preparation of test portions.....	2
6 Apparatus	2
6.1 General.....	2
7 Test conditions	3
7.1 General.....	3
7.2 Reducing gas.....	3
7.2.1 Composition.....	3
7.2.2 Purity.....	3
7.2.3 Flow rate.....	3
7.3 Heating and cooling gas.....	3
7.4 Temperature of the test portion.....	3
8 Procedure	4
8.1 Number of determinations for the test.....	4
8.2 Chemical analysis.....	4
8.3 Reduction.....	4
9 Expression of results	5
9.1 Calculation of the reducibility index.....	5
9.2 Repeatability and acceptance of test results.....	5
10 Test report	6
11 Verification	6
Annex A (normative) Flowsheet of the procedure for the acceptance of test results	10
Annex B (informative) Derivation of equation for reducibility	11

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 102, *Iron ore and direct reduced iron*, Subcommittee SC 3, *Physical testing*.

This fourth edition cancels and replaces the third edition (ISO 4695:2007), of which it constitutes a minor revision to contemplate the outcomes of the studies on mass definition, as well as minor editorial improvements.

Introduction

This International Standard concerns one of a number of physical test methods that have been developed to measure various physical parameters and to evaluate the behaviour of iron ores, including reducibility, disintegration, crushing strength, apparent density, etc. This method was developed to provide a uniform procedure, validated by collaborative testing, to facilitate comparisons of tests made in different laboratories.

The results of this test have to be considered in conjunction with other tests used to evaluate the quality of iron ores as feedstocks for blast furnace processes.

This International Standard can be used to provide test results as part of a production quality control system, as a basis of a contract, or as part of a research project.

STANDARDSISO.COM : Click to view the full PDF of ISO 4695:2015

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 4695:2015

Iron ores for blast furnace feedstocks — Determination of the reducibility by the rate of reduction index

CAUTION — This International Standard can involve hazardous operations and equipment. This International Standard does not purport to address all of the safety issues associated with its use. It is the responsibility of the user of this International Standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to its use.

1 Scope

This International Standard specifies a method to provide a relative measure for evaluating the extent to and ease with which oxygen can be removed from iron ores, when reduced under conditions resembling those prevailing in the reduction zone of a blast furnace.

This International Standard is applicable to lump ores, sinters and hot-bonded pellets.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 2597-1, *Iron ores — Determination of total iron content — Part 1: Titrimetric method after tin(II) chloride reduction*

ISO 2597-2, *Iron ores — Determination of total iron content — Part 2: Titrimetric methods after titanium(III) chloride reduction*

ISO 3082, *Iron ores — Sampling and sample preparation procedures*

ISO 9035, *Iron ores — Determination of acid-soluble iron(II) content — Titrimetric method*

ISO 11323, *Iron ore and direct reduced iron — Vocabulary*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 11323 apply.

4 Principle

The test portion is isothermally reduced in a fixed bed, at 950 °C, using a reducing gas consisting of CO and N₂, and the mass loss of the test portion is recorded continuously or at specified time intervals until its degree of reduction reaches 65 %. The rate of reduction is calculated at the oxygen/iron ratio of 0,9.

5 Sampling, sample preparation and preparation of test portions

5.1 Sampling and sample preparation

Sampling of a lot and preparation of a test sample shall be in accordance with ISO 3082.

The size range for pellets, sinters and lump ores shall be -12,5 mm + 10,0 mm.

A test sample of at least 2,5 kg, on a dry basis, of the sized material shall be obtained.

Oven-dry the test sample to constant mass at $105\text{ °C} \pm 5\text{ °C}$ and cool it to room temperature before preparation of the test portions.

NOTE Constant mass is achieved when the difference in mass between two subsequent measurements becomes less than 0,05 % of the initial mass of the test sample.

5.2 Preparation of test portions

Collect each test portion by taking ore particles at random.

NOTE Manual methods of division recommended in ISO 3082, such as riffing, can be applied to obtain the test portions.

At least five test portions, each of approximately 500 g (\pm the mass of one particle) shall be prepared from the test sample: four test portions for testing and one for chemical analysis.

Weigh the test portions to the nearest 1 g and register the mass of each test portion on its recipient label.

6 Apparatus

6.1 General

The test apparatus shall comprise the following:

- a) ordinary laboratory equipment, such as an oven, hand tools, a time-control device and safety equipment;
- b) reduction tube assembly;
- c) furnace, equipped with a balance for permitting the mass loss of the test portion to be read at any time during the test;
- d) system to supply the gases and regulate the flow rates;
- e) weighing device.

[Figure 1](#) shows an example of the test apparatus.

6.2 Reduction tube, made of non-scaling, heat-resistant metal to withstand temperatures higher than 950 °C and resistant to deformation. The internal diameter shall be $75\text{ mm} \pm 1\text{ mm}$. A removable perforated plate, made of non-scaling, heat-resistant metal to withstand temperatures higher than 950 °C , shall be mounted in the reduction tube to support the test portion and to ensure uniform gas flow through it. The perforated plate shall be 4 mm thick, with its diameter 1 mm less than the internal diameter of the tube. The holes in the plate shall be 2 mm to 3 mm in diameter at a pitch centre distance of 4 mm to 5 mm.

[Figure 2](#) shows an example of a reduction tube.

6.3 Furnace, having a heating capacity and temperature control able to maintain the entire test portion, as well as the gas entering the bed, at $950\text{ °C} \pm 10\text{ °C}$.

6.4 Balance, capable of weighing the reduction tube assembly, including the test portion, to an accuracy of 1 g. The balance shall have an appropriate device to suspend the reduction tube assembly.

6.5 Gas-supply system, capable of supplying the gases and regulating gas flow rates. It shall be ensured that a frictionless connection between the gas-supply system and the reduction tube does not affect the weight loss determination during reduction.

6.6 Weighing device, capable of weighing the test sample and test portions to an accuracy of 1 g.

7 Test conditions

7.1 General

Volumes and flow rates of gases used are as measured at a reference temperature of 0 °C and at a reference atmospheric pressure of 101,325 kPa (1,013 25 bar).

7.2 Reducing gas

7.2.1 Composition

The reducing gas shall consist of

CO 40,0 % ± 0,5 % (volume fraction)

N₂ 60,0 % ± 0,5 % (volume fraction)

7.2.2 Purity

Impurities in the reducing gas shall not exceed the following:

H₂ 0,2 % (volume fraction)

CO₂ 0,2 % (volume fraction)

O₂ 0,1 % (volume fraction)

H₂O 0,2 % (volume fraction)

7.2.3 Flow rate

The flow rate of the reducing gas, during the entire reducing period, shall be maintained at 50 L/min ± 0,5 L/min.

7.3 Heating and cooling gas

Nitrogen (N₂) shall be used as the heating and cooling gas. Impurities shall not exceed 0,1 % (volume fraction).

The flow rate of N₂ shall be maintained at 25 L/min until the test portion reaches 950 °C, and at 50 L/min during the temperature-equilibration period. During cooling, it shall be maintained at 5 L/min.

7.4 Temperature of the test portion

The temperature of the entire test portion shall be maintained at 950 °C ± 10 °C during the entire reducing period and, as such, the reducing gas shall be preheated before entering the test portion.

8 Procedure

8.1 Number of determinations for the test

Carry out the test as many times as required by the procedure in [Annex A](#).

8.2 Chemical analysis

Take, at random, one of the test portions prepared in [5.2](#) and use it for the determination of the iron(II) oxide content (w_1) in accordance with ISO 9035 and the total iron content (w_2) in accordance with ISO 2597-1 or ISO 2597-2.

8.3 Reduction

Take, at random, another portion prepared in [5.2](#) and record its mass (m_0). Place it in the reduction tube ([6.2](#)) and level its surface.

NOTE In order to achieve a more uniform gas flow, a double-layer bed of porcelain balls sized between 10,0 mm and 12,5 mm can be placed between the perforated plate and the test portion.

Close the top of the reduction tube. Connect the thermocouple, ensuring that its tip is in the centre of the test portion, as shown in [Figure 1](#).

Insert the reduction tube into the furnace ([6.3](#)) and suspend it centrally from the balance ([6.4](#)) ensuring that there is no contact with the furnace wall or heating elements.

Connect the gas-supply system ([6.5](#)).

Pass a flow of N_2 through the test portion at a rate of 25 L/min and commence heating. When the temperature of the test portion approaches 950 °C, increase the flow rate to 50 L/min. Continue heating while maintaining the flow of N_2 , until the balance reading is constant and the temperature is constant at 950 °C ± 10 °C for 15 min.

DANGER — Carbon monoxide and the reducing gas, which contains carbon monoxide, are toxic and therefore hazardous. Testing shall be carried out in a well-ventilated area or under a hood. Precautions should be taken for the safety of the operator, in accordance with the safety codes of each country.

Tare the balance, start the time control device and immediately introduce the reducing gas at a flow rate of 50 L/min ± 0,5 L/min to replace the N_2 . Record the mass loss of the test portion (Δm_t) at least every 3 min for the first 15 min and thereafter at 10 min intervals.

Calculate the degree of reduction, R_t , relative to the iron(III) state, after t min, as follows:

$$R_t = \left(\frac{0,111w_1}{0,430w_2} + \frac{\Delta m_t}{m_0 \times 0,430w_2} \times 100 \right) \times 100 \quad (1)$$

where

m_0 is the mass, in grams, of the test portion;

Δm_t is the mass loss, in grams, of the test portion after reduction time t ;

w_1 is the iron(II) oxide content, as a percentage by mass, of the test sample prior to the test, determined in accordance with ISO 9035; it is calculated from the iron(II) content by multiplying it by the oxide conversion factor $FeO/Fe(II) = 1,286$.

w_2 is the total iron content, as a percentage by mass, of the test portion prior to the test, determined in accordance with ISO 2597-1 or ISO 2597-2.

When the degree of reduction reaches 65 %, turn off the power and stop the flow of the reducing gas. If after 4 h, 65 % of oxygen loss has not been achieved, the reduction can be stopped. Introduce N₂ at a flow rate of 5 L/min for 5 min or more to purge the reducing gas from the tube.

9 Expression of results

9.1 Calculation of the reducibility index $\left(\frac{dR}{dt}\right)$ (O / Fe = 0,9)

Prepare the reduction curve by plotting the degree of reduction R_t against time t .

Read off, from the reduction curve the time, in minutes, to attain degrees of reduction of 30 % and 60 %.

The reducibility index, expressed as the rate of reduction at the atomic ratio of O/Fe of 0,9¹⁾ in %/min, is calculated from Formula (2)²⁾:

$$\frac{dR}{dt}(\text{O / Fe} = 0,9) = \frac{33,6}{t_{60} - t_{30}} \quad (2)$$

where

t_{30} is the time, in minutes, to attain a degree of reduction of 30 %;

t_{60} is the time, in minutes, to attain a degree of reduction of 60 %;

33,6 is a constant.

Record the result to two decimal places.

NOTE If a degree of reduction of 60 % is not attained in the test, lower values can be accommodated by Formula (3):

$$\frac{dR}{dt}(\text{O / Fe} = 0,9) = \frac{k}{t_y - t_{30}} \quad (3)$$

where

t_y is the time, in minutes, to attain a degree of reduction of y %;

k is a constant depending on y .

If $y = 50$ %, then the value of $k = 20,2$.

If $y = 55$ %, then the value of $k = 26,5$.

9.2 Repeatability and acceptance of test results

Follow the procedure in [Annex A](#) by using the repeatability values given in [Table 1](#). The results shall be reported to two decimal places.

1) The atomic ratio O/Fe = 0,9 means a 40 % degree of reduction.

2) The derivation of the equation is given in [Annex B](#).

Table 1 — Repeatability (r)

Type of iron ore	r %/min
Pellets	$0,07 \times \overline{dR/dt}$
Sinter	0,17
Lump ore	0,10

NOTE $\overline{dR/dt}$ is the mean value of dR/dt results.

10 Test report

The test report shall include the following information:

- a reference to this International Standard, i.e. ISO 4695:2015;
- all details necessary for the identification of the sample;
- the name and address of the test laboratory;
- the date of the test;
- the date of the test report;
- the signature of the person responsible for the test;
- the details of any operation and any test conditions not specified in this International Standard or regarded as optional, as well as any incident which may have had an influence on the results;
- the reducibility index, dR/dt (O/Fe = 0,9);
- the total iron and iron(II) contents of the test portion before reduction;
- the reduction curve, if specified at the time of ordering.

11 Verification

Regular checking of the apparatus is essential to ensure test result reliability. The frequency of checking is a matter for each laboratory to determine.

The conditions of the following items shall be checked.


- weighing device;
- reduction tube;
- temperature control and measurement devices;
- balance;
- gas flow meters;
- purity of gases;
- recording system;

— time-control device.

It is recommended that internal reference material be prepared and used periodically to check test repeatability.

Appropriate records of verification activities shall be maintained.

STANDARDSISO.COM : Click to view the full PDF of ISO 4695:2015

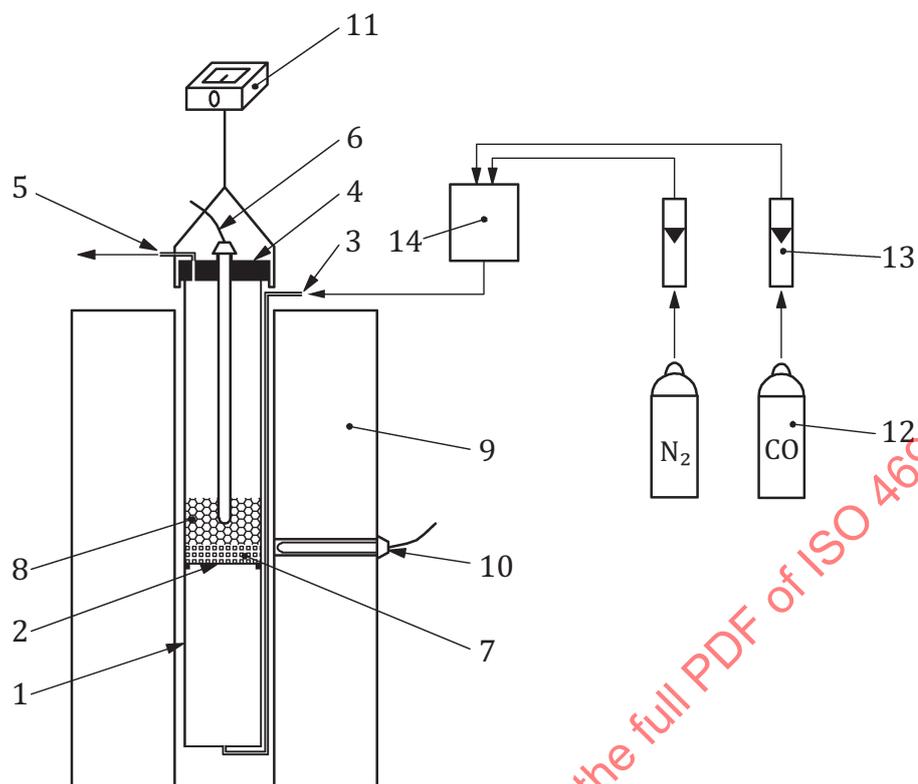

Key

Reduction tube

- 1 reduction tube
- 2 perforated plate
- 3 gas inlet
- 4 lid
- 5 gas outlet
- 6 thermocouple for measuring the reduction temperature
- 7 porcelain ball layer
- 8 test portion

Furnace


- 9 electrically heated furnace
- 10 thermocouple for temperature regulation of furnace
- 11 balance

Gas supply system

- 12 gas cylinder
- 13 gas flow meters
- 14 mixing vessel

Figure 1 — Example of test apparatus (schematic diagram)

Dimensions in millimetres

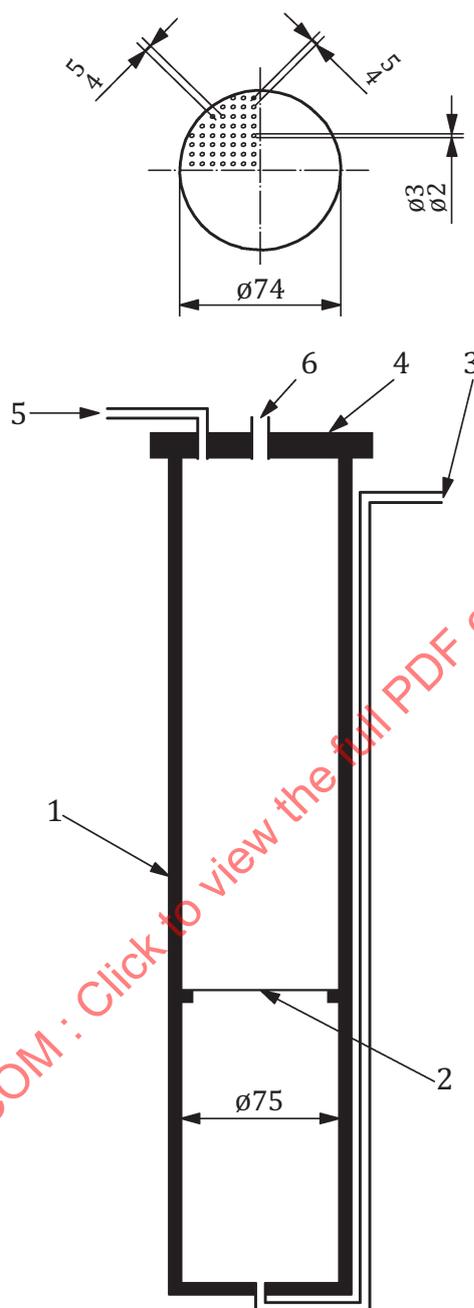**Key**


- 1 reduction tube
- 2 perforated plate
- 3 opening for gas inlet
- 4 lid
- 5 opening for gas outlet
- 6 opening for thermocouple insertion

NOTE Dimensions not specified in [Clause 6](#) are shown for information only.

Figure 2 — Example of reduction tube (schematic diagram)

Annex A (normative)

Flowsheet of the procedure for the acceptance of test results

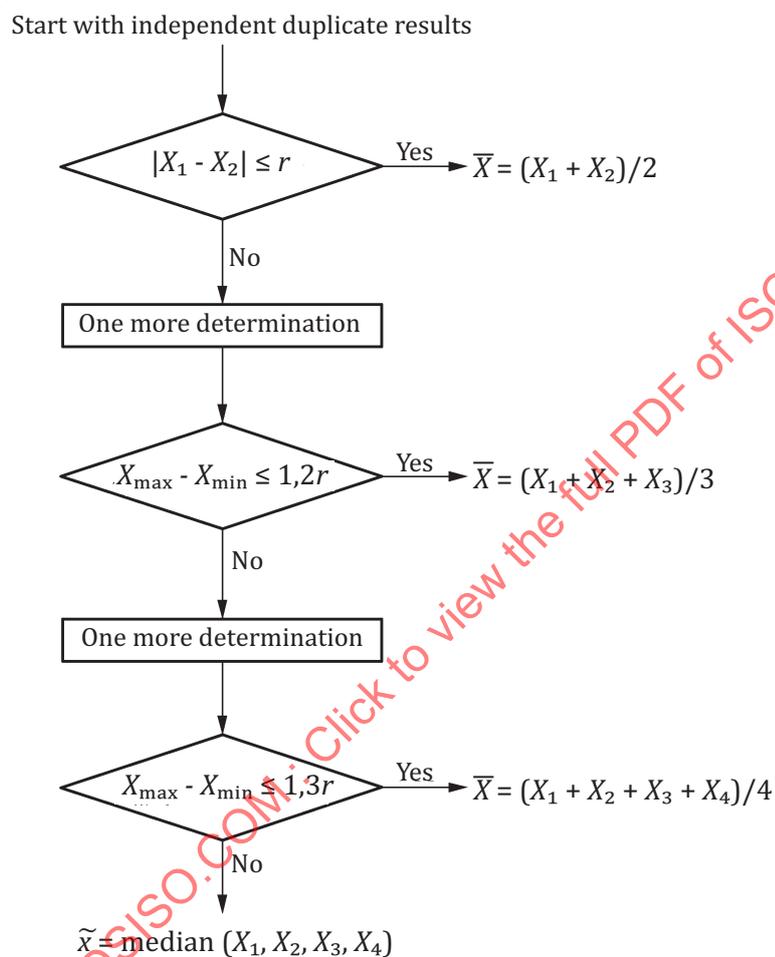

NOTE For r , see [Table 1](#).

Figure A.1 — Flowsheet of the procedure for the acceptance of test results