

INTERNATIONAL STANDARD

ISO 5145

Second edition
2004-04-15

AMENDMENT 1
2006-07-01

Cylinder valve outlets for gases and gas mixtures — Selection and dimensioning

AMENDMENT 1: Cylinder valve outlets for gases for medical use

Raccords de sortie de robinets de bouteilles à gaz et mélanges de gaz — Choix et dimensionnement

AMENDEMENT 1: Raccords de sortie de robinets de bouteilles à gaz à usage médical

STANDARDSISO.COM : Click to view the full PDF of ISO 5145:2004/Amd 1:2006



Reference number
ISO 5145:2004/Amd.1:2006(E)

© ISO 2006

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 5145:2004/Amd 1:2006

© ISO 2006

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

Amendment 1 to ISO 5145:2004 was prepared by Technical Committee ISO/TC 58, *Gas cylinders*, Subcommittee SC 2, *Cylinder fittings*.

Introduction

This amendment to ISO 5145:2004 is intended to indicate how to determine with the help of a flowchart the cylinder valve outlets for gases for medical use. Six examples are given to explain the flowchart.

STANDARDSISO.COM : Click to view the full PDF of ISO 5145:2004/Amd 1:2006

Cylinder valve outlets for gases and gas mixtures — Selection and dimensioning

AMENDMENT 1: Cylinder valve outlets for gases for medical use

Add the following annex after Annex C:

Annex D (informative)

Cylinder valve outlets for gases for medical use

D.1 Scope

This annex gives examples of how to allocate cylinder valve outlets in the case of gases for medical use to ensure patient safety. Such gases are treated differently depending on whether they are gases for inhalation or for other purposes. Allocation is based on the pharmacological and therapeutic properties of the gases and not physical aspects such as pressure.

D.2 Definitions

The following definitions apply.

D.2.1 Gas for medical use

Any gas or mixture of gases intended to be administered to patients for therapeutic, diagnostic or prophylactic purposes, with or without pharmacological action, or to be used for surgical tools. It covers both medicinal and medical gases.

D.2.2 Medicinal gas

Any gas or mixture of gases intended to be administered to patients for therapeutic, diagnostic or prophylactic purposes using pharmacological action and classified as a medicinal product, e.g. according to Article 1.2 of Directive 2001/83/EC of the European Parliament and of the Council of 6 November 2001 on the community code relating to medicinal products for human use.

D.2.3 Gas for inhalation

Medicinal gas intended for introduction into the body through respiration. The gas is administered alone directly or after mixing at the point of use with oxygen or air.

D.2.4 Medicinal gas mixture containing oxygen

Gas mixture in which the oxygen content is taken into account in order to limit the duration of the inhalation under standard atmospheric conditions, for example binary mixtures (from nitrogen, helium, nitrous oxide, carbon dioxide) or ternary mixtures or more used e.g. for lung function testing (LFT). Medicinal gas mixtures containing oxygen can be classified as follows.

- Hypoxic mixtures (mixtures with lower than normal O₂ content): gas with O₂ < 20 %¹⁾ for short-term inhalation.
- Hyperoxic mixtures (mixtures with greater than normal O₂ content): gas with O₂ > 23,5 % for continuous inhalation.
- Normoxic mixtures (mixtures with normal O₂ content): 20 %¹⁾ ≤ O₂ ≤ 23,5 % for continuous inhalation.

D.2.5 Analytical gas

Gas which is used for analysis calibration or for the purpose of supplying energy (flame, oven, etc.) and other similar purposes (for example, gas chromatography, atomic absorption spectrophotometer) in biological or pharmaceutical research laboratories.

D.2.6 Breathable gas

Gas which supports life to be used in breathing or diving apparatus in a non-standard atmospheric medium such as water, at high altitude, in space or in a confined or polluted medium, but not for therapeutic, diagnostic or prophylactic uses. For example, air, oxygen and gas mixtures (nitrogen/oxygen, helium/oxygen, nitrogen/helium/oxygen, etc.) with normal or greater than normal oxygen content.

D.3 Rules of safety

In hospitals, the simultaneous presence of medicinal, medical, analytical and industrial gas cylinders increases the risk of occurrence of serious safety issues for the patient. The following requirements apply.

- Staff involved in the administration of gases for medical use shall be appropriately trained to ensure that the correct gas is used.
- The different gases and gas mixtures shall be easily identified and stored in separate areas.
- Labelling and colour coding of the gas cylinder shall be checked before use.
- As a general rule, cylinders containing non-breathable gases for industrial or medical use shall not be fitted with the same valve outlet connection as those medical gases used for breathing. This then preserves the integrity of the gas-specific safety system (designed to prevent the delivery of non-breathing or hypoxic gas mixtures) and thus protects against the possibility of inadvertently connecting such gases to breathing medical device delivery systems.

1) 19,5 % for some national pharmacopoeia.

D.4 Rules for outlet allocation

A number of valve outlets have already been allocated for the commonly used gases for medical use. The allocation of valve outlets from the limited possibilities comes from risk analysis, mainly asphyxia in the case of connection with gases with lower than 20 %²⁾ oxygen content resulting from the simultaneous presence of industrial gases and gases for medical use in hospitals, and also the presence in gas mixtures of components limiting the duration of inhalation.

Where there is no specific allocation to a given gas or gas mixture, the following rules may be applied:

- For oxygen-enriched ternary or higher gas mixtures intended for inhalation without a specific valve outlet allocation, Figure D.1 allows the valve outlet allocation to be determined as a function of the type of gas according to Table D.1.
- For other gases or gas mixtures, the shared valve outlet assigned to an FTSC gas group according to Tables 2 and 3 may be proposed, e.g. No. 4 (see Table 4) for all inert gases and gas mixtures of FTSC code 0150 (except inert gases and gas mixtures that have a specific valve outlet such as N₂, He, NO/N₂ (100 ppm < NO < 1 000 ppm) or 1050).

Table D.1 lists the maximum thresholds for the components used in oxygen-enriched premixed gases for short-term and continuous inhalation under standard atmospheric conditions.

Figure D.1 is a logical flowchart for the selection of valve outlets for gases for medical use.

Table D.1 — Maximum thresholds for the components used in oxygen-enriched premixed gases for short-term and continuous inhalation in standard atmospheric conditions

Component	LC 50 ^a	Medical use	Recommended maximum volume fraction for continuous inhalation
N ₂ O	—	Anaesthesia or analgesia if 50/50	80 %
CO	3 760 ppm	LFT premixture	0,4 %
CO ₂	—	LFT premixture	7 %
NO	115 ppm	Neonatal intensive care In premixture with N ₂	0,1 %
C ₂ H ₂	—	LFT premixture	0,4 %
H ₂	—	Gut function testing in premixture with air Gas for calibration	Not applicable
CH ₄	—	LFT premixture	0,4 %

^a LC 50 is the concentration of gas in air that will kill 50 % of test subjects.

2) 19,5 % for some national pharmacopoeia.

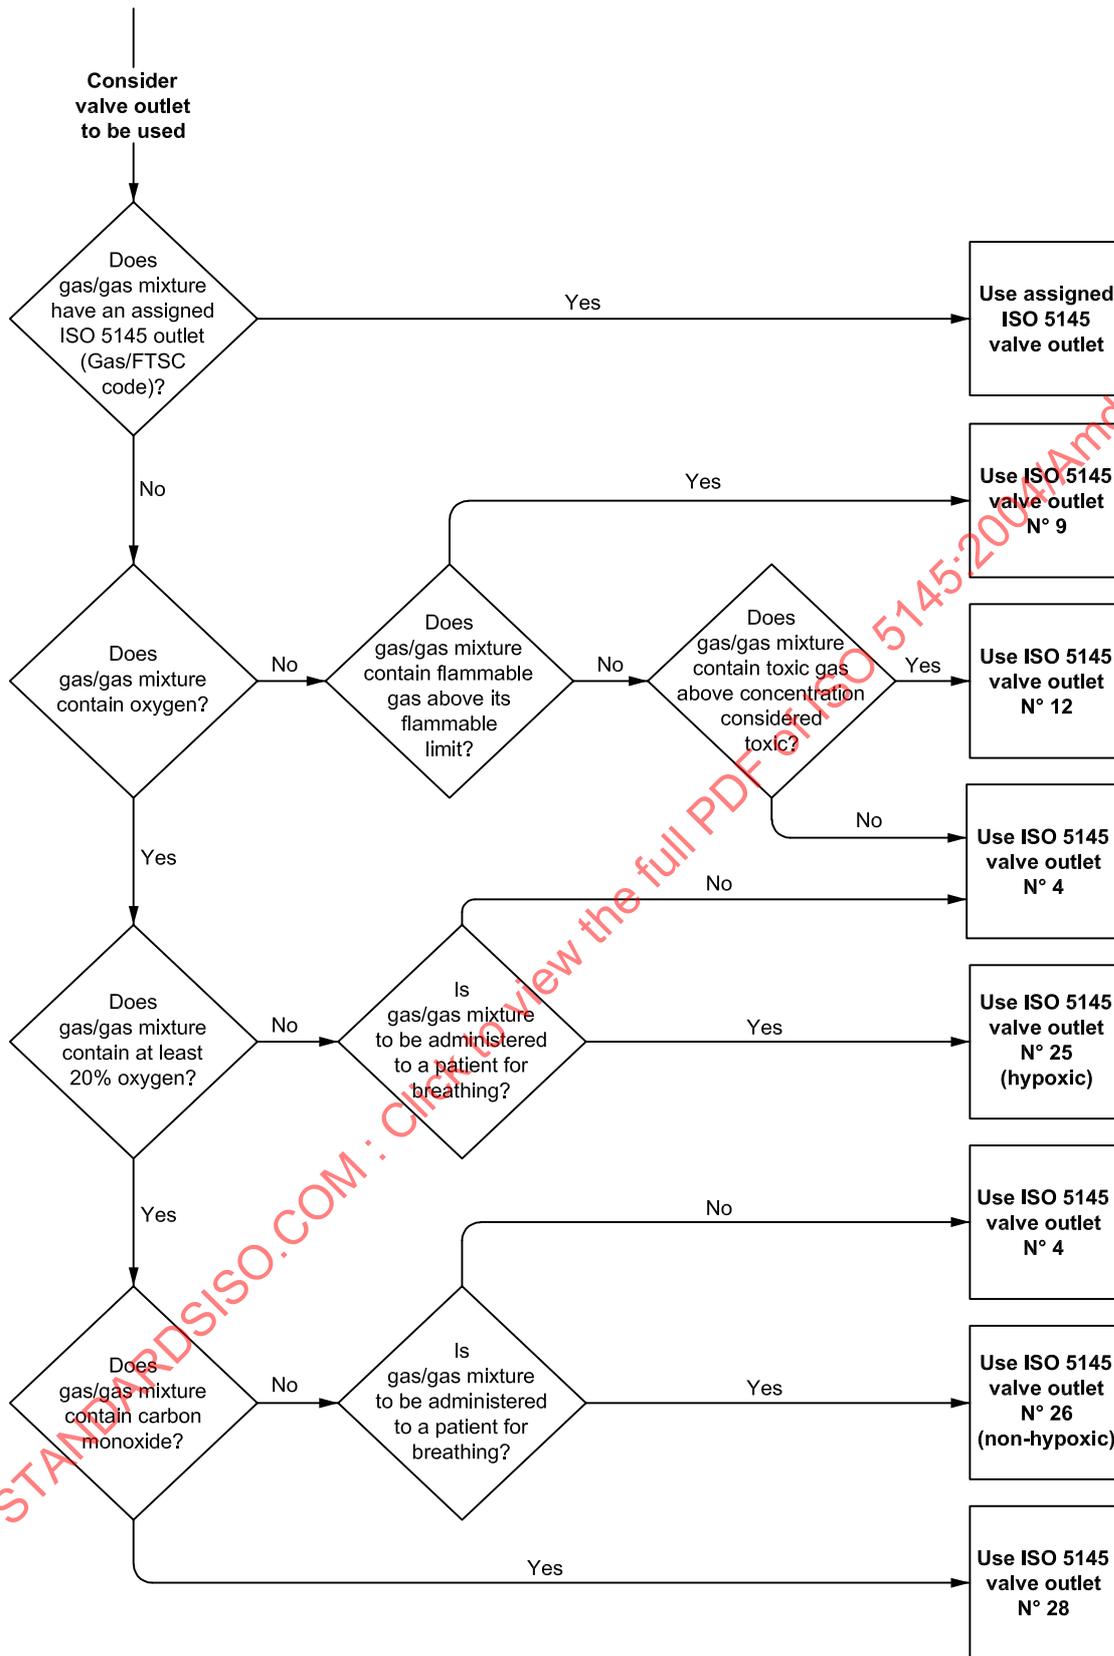


Figure D.1 — Flowchart for the selection of valve outlets for gases for medical use

D.5 Examples of valve outlets selected with the help of Figure D.1

D.5.1 Example 1: anaerobic cellular culture (not for breathing)

Typical mixture composition: 10 % H₂, 5 % CO₂, balance N₂.

Does gas or gas mixture have an assigned outlet (gas/FTSC code)?	No
Does gas contain oxygen?	No
Does gas contain a flammable component above its flammable limit?	Yes
Outlet allocation	Outlet 9

D.5.2 Example 2: toxic hypoxic gas/gas mixture

Typical composition: 100 % nitric oxide (NO).

Does gas or gas mixture have an assigned outlet (gas/FTSC code)?	No
Does gas contain oxygen?	No
Does gas contain a flammable component above its flammable limit?	No
Does gas contain component above its critical concentration where it is considered toxic?	Yes
Outlet allocation	Outlet 12

D.5.3 Example 3: hypoxic lung function test mixture (with no flammable components)

Typical mixture composition: 4 % CO₂, 16 % O₂, balance N₂.

Does gas or gas mixture have an assigned outlet (gas/FTSC code)?	No
Does gas contain oxygen?	Yes
Is oxygen content at least 20 %?	No
Is gas to be administered for breathing?	Yes
Outlet allocation	Outlet 25

D.5.4 Example 4: non-hypoxic lung function test mixture (with no flammable components)

Typical mixture composition: 9 % He, 35 % O₂, balance N₂.

Does gas or gas mixture have an assigned outlet (gas/FTSC code)?	No
Does gas contain oxygen?	Yes
Is oxygen content at least 20 %?	Yes
Does gas contain carbon monoxide?	No
Is gas to be administered for breathing?	Yes
Outlet allocation	Outlet 26 (non hypoxic)