

INTERNATIONAL
STANDARD

ISO
5347-9

First edition
1993-12-15

**Methods for the calibration of vibration
and shock pick-ups —**

Part 9:

Secondary vibration calibration by comparison
of phase angles

Méthodes pour l'étalonnage de capteurs de vibrations et de chocs —

*Partie 9: Étalonnage secondaire de vibrations par comparaison des angles
de phase*



Reference number
ISO 5347-9:1993(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 5347-9 was prepared by Technical Committee ISO/TC 108, *Mechanical vibration and shock*, Sub-Committee SC 3, *Use and calibration of vibration and shock measuring instruments*.

ISO 5347 consists of the following parts, under the general title *Methods for the calibration of vibration and shock pick-ups*:

- Part 0: *Basic concepts*
- Part 1: *Primary vibration calibration by laser interferometry*
- Part 2: *Primary shock calibration by light cutting*
- Part 3: *Secondary vibration calibration*
- Part 4: *Secondary shock calibration*
- Part 5: *Calibration by Earth's gravitation*
- Part 6: *Primary vibration calibration at low frequencies*
- Part 7: *Primary calibration by centrifuge*
- Part 8: *Primary calibration by dual centrifuge*

© ISO 1993

All rights reserved. No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case Postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

- Part 9: Secondary vibration calibration by comparison of phase angles
- Part 10: Primary calibration by high-impact shocks
- Part 11: Testing of transverse vibration sensitivity
- Part 12: Testing of transverse shock sensitivity
- Part 13: Testing of base strain sensitivity
- Part 14: Resonance frequency testing of undamped accelerometers on a steel block
- Part 15: Testing of acoustic sensitivity
- Part 16: Testing of mounting torque sensitivity
- Part 17: Testing of fixed temperature sensitivity
- Part 18: Testing of transient temperature sensitivity
- Part 19: Testing of magnetic field sensitivity
- Part 20: Primary vibration calibration by the reciprocity method

Annex A forms an integral part of this part of ISO 5347.

STANDARDSISO.COM : Click to view the full PDF of ISO 5347-9:1993

STANDARDSISO.COM : Click to view the full PDF of ISO 5347-9:1993

Methods for the calibration of vibration and shock pick-ups —

Part 9:

Secondary vibration calibration by comparison of phase angles

1 Scope

ISO 5347 comprises a series of documents dealing with methods for the calibration of vibration and shock pick-ups.

This part of ISO 5347 lays down detailed specifications for the instrumentation and procedure to be used for comparison phase angle vibration calibration. It applies to rectilinear and working pick-ups.

The limits of uncertainty applicable are $\pm 3\%$ of reading.

2 Apparatus

2.1 Equipment capable of maintaining room temperature at $23\text{ }^{\circ}\text{C} \pm 3\text{ }^{\circ}\text{C}$.

2.2 Primary standard accelerometer, calibrated together with amplifier, uncertainty maximum $\pm 1^{\circ}$.

2.3 Oscillator, having the following characteristics:

- uncertainty for frequency: maximum $\pm 1\%$ of reading;
- frequency stability: better than 1% of reading over the measurement period.

2.4 Power amplifier/vibrator combination, having the following characteristics:

- total distortion: 5% max.;

- transverse, bending and rocking acceleration: 20% max. of the acceleration in the intended direction at frequencies used;

- hum and noise: 40 dB min. below reading.

2.5 Phase-measuring instrumentation, having the following characteristics:

- frequency range: 20 Hz to $5\ 000\text{ Hz}$;
- phase range: 0 to 90° ;
- uncertainty specified: $\pm 1^{\circ}$.

2.6 Oscilloscope, for checking the waveform of the pick-up signal with a frequency range from 5 Hz to $5\ 000\text{ Hz}$.

3 Preferred frequencies

Six frequencies, in hertz, equally covering the range, shall be chosen from the following series:

20; 40; 80; 160; 315; 630; 1 250; 2 500; 5 000.

Values chosen shall be the same as for the standard accelerometer calibration values.

The reference amplitude level of the primary standard accelerometer shall be chosen.

4 Method

Mount the primary standard accelerometer and the pick-up to be calibrated back-to-back on the vibrator head. The test set-up shall be as shown in figure 1.

Measure the phase angle difference between the two pick-ups.

The results shall be reported as phase angle as a function of frequency.

When the calibration results are reported, the total uncertainty of the calibration and the corresponding confidence level, calculated in accordance with annex A, shall also be reported.

A confidence level of 95 % shall be used.

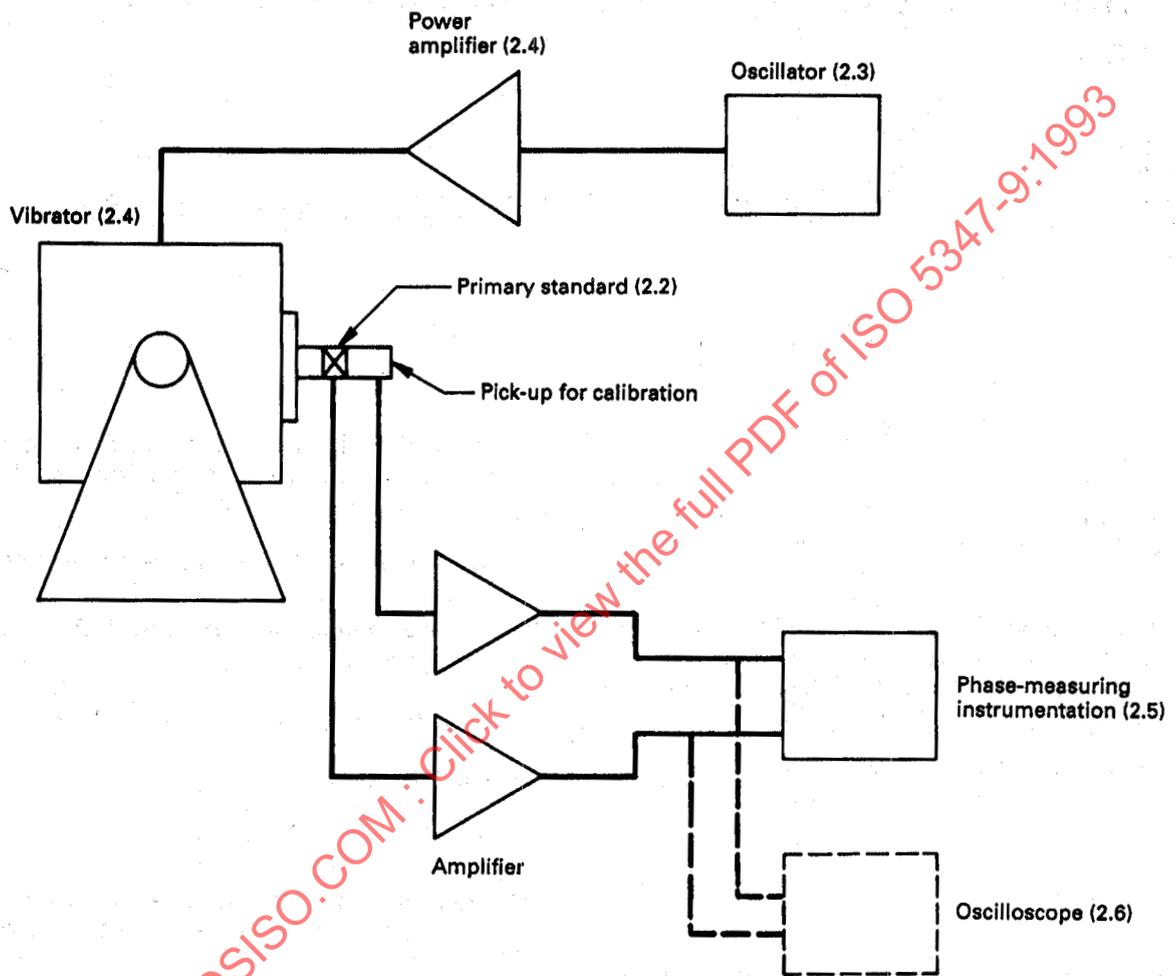


Figure 1 — Measuring system for comparison phase calibration method