

---

---

**Plastics — Determination of dynamic  
mechanical properties —**

**Part 2:  
Torsion-pendulum method**

*Plastiques — Détermination des propriétés mécaniques  
dynamiques —*

*Partie 2: Méthode au pendule de torsion*

STANDARDSISO.COM : Click to view the full PDF of ISO 6721-2:2019



STANDARDSISO.COM : Click to view the full PDF of ISO 6721-2:2019



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2019

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Fax: +41 22 749 09 47  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
Foreword .....	iv
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>1</b>
<b>5 Test apparatus</b> .....	<b>3</b>
5.1 Pendulum .....	3
5.2 Inertial element .....	3
5.2.1 General .....	3
5.2.2 Method A (see <a href="#">Figure 1</a> ) .....	3
5.2.3 Method B (see <a href="#">Figure 2</a> ) .....	3
5.3 Clamps .....	3
5.4 Oscillation-inducing device .....	4
5.5 Oscillation-frequency and oscillation-amplitude recording equipment .....	4
5.6 Temperature-controlled chamber .....	4
5.7 Gas supply .....	4
5.8 Temperature-measurement device .....	4
5.9 Devices for measuring test-specimen dimensions .....	4
<b>6 Test specimens</b> .....	<b>4</b>
6.1 General .....	4
6.2 Shape and dimensions .....	4
6.3 Preparation .....	5
<b>7 Number of specimens</b> .....	<b>5</b>
<b>8 Conditioning</b> .....	<b>5</b>
<b>9 Procedure</b> .....	<b>5</b>
9.1 Test atmosphere .....	5
9.2 Measurement of specimen cross-section .....	5
9.3 Mounting the test specimens .....	5
9.4 Varying the temperature .....	5
9.5 Performing the test .....	5
<b>10 Expression of results</b> .....	<b>6</b>
10.1 Symbols and correction factors .....	6
10.2 Calculation of logarithmic decrement, $\Delta$ .....	7
10.3 Calculation of torsional storage modulus, $G'_{to}$ .....	8
10.4 Calculation of torsional loss modulus, $G''_{to}$ .....	8
<b>11 Precision</b> .....	<b>9</b>
<b>12 Test report</b> .....	<b>9</b>
<b>Annex A (normative) Influence of longitudinal force, <math>W</math></b> .....	<b>10</b>
<b>Annex B (informative) Damping correction factor, <math>F_d</math></b> .....	<b>11</b>
<b>Annex C (informative) Dimensional correction factor, <math>F_c</math></b> .....	<b>12</b>
<b>Bibliography</b> .....	<b>13</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*.

This third edition cancels and replaces the second edition (ISO 6721-2:2008), which has been technically revised. The main changes compared to the previous edition are as follows:

- the document has been revised editorially;
- normative references have been changed to undated.

A list of all parts in the ISO 6721 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

# Plastics — Determination of dynamic mechanical properties —

## Part 2: Torsion-pendulum method

### 1 Scope

This document specifies two methods (A and B) for determining the linear dynamic mechanical properties of plastics, i.e. the storage and loss components of the torsional modulus, as a function of temperature, for small deformations within the frequency range from 0,1 Hz to 10 Hz.

NOTE The temperature dependence of these properties, measured over a sufficiently broad range of temperatures (for example from  $-50\text{ °C}$  to  $+150\text{ °C}$  for most commercially available plastics), gives information on the transition regions (for example the glass transition and the melting transition) of the polymer. It also provides information concerning the onset of plastic flow.

The two methods described are not applicable to non-symmetrical laminates (see ISO 6721-3). The methods are not suitable for testing rubbers, for which the user is referred to ISO 4664-2.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 6721-1, *Plastics — Determination of dynamic mechanical properties — Part 1: General principles*

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 6721-1 apply.


ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

### 4 Principle

A test specimen of uniform cross-section is gripped by two clamps, one of them fixed and the other connected to a disc, which acts as an inertial element, by a rod. The end of the specimen connected to the disc is excited, together with the disc, to execute freely decaying torsional oscillations. The oscillation mode is that designated IV in ISO 6721-1, and the type of modulus is  $G_{t0}$  as defined in ISO 6721-1.


The inertial element is suspended either from the specimen (method A, see [Figure 1](#)) or from a wire (method B, see [Figure 2](#)). In the latter case, the wire is also part of the elastically oscillating system.

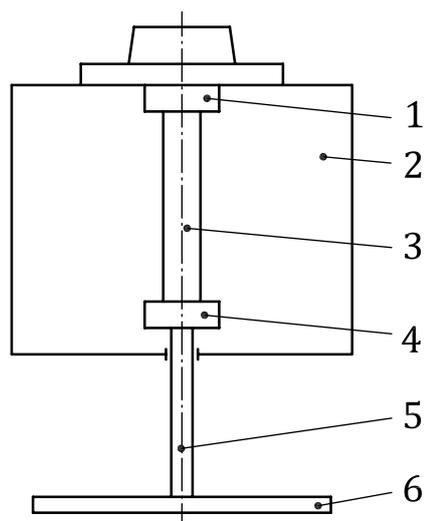

**Key**

- |                                  |                         |
|----------------------------------|-------------------------|
| 1 upper (fixed) clamp            | 4 lower (movable) clamp |
| 2 temperature-controlled chamber | 5 rod                   |
| 3 test specimen                  | 6 inertial element      |

**Figure 1 — Apparatus for method A**

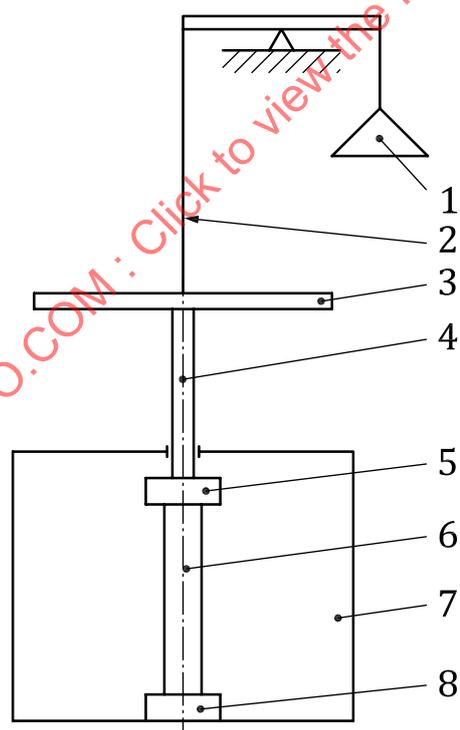

**Key**

- |                    |                                  |
|--------------------|----------------------------------|
| 1 counterweight    | 5 upper (movable) clamp          |
| 2 wire             | 6 test specimen                  |
| 3 inertial element | 7 temperature-controlled chamber |
| 4 rod              | 8 lower (fixed) clamp            |

**Figure 2 — Apparatus for method B**

During a temperature run, the same inertial element can be used throughout the whole run, which results in a frequency decreasing naturally with increasing temperature, or the inertial element can be replaced at intervals by a member of different moment of inertia in order to keep the frequency approximately constant.

During the test, the frequency and the decaying amplitude are measured. From these quantities, the storage component  $G'_{to}$  and loss component  $G''_{to}$  of the torsional complex modulus  $G^*_{to}$  can be calculated.

## 5 Test apparatus

### 5.1 Pendulum

Two types of torsion pendulum are specified for use with this document:

- a) the inertial element is suspended from the test specimen and the lower end of the specimen is excited (method A, [Figure 1](#));
- b) the inertial element is suspended from a wire attached to a counterweight and the upper end of the specimen is excited (method B, [Figure 2](#)).

Both types of pendulum consist of an inertial element, two clamps for gripping the specimen (one of which is connected to the inertial element by a rod) and a temperature-controlled chamber enclosing the specimen and the clamps. For method B, a counterweight and connecting wire are also required.

### 5.2 Inertial element

#### 5.2.1 General

The moment of inertia,  $I$ , of the inertial element, which may be made of aluminium, for instance, shall be selected as a function of the torsional stiffness of the specimen, so that the temperature-dependent natural frequency of the system lies between approximately 0,1 Hz and 10 Hz.

When testing standard specimens (see [6.2](#)), a moment of inertia,  $I$ , of about  $3 \times 10^{-5} \text{ kg}\cdot\text{m}^2$  is recommended if the same inertial element is to be used throughout a run.

NOTE For certain materials, e.g. filled polymers, a value of  $I$  of about  $5 \times 10^{-5} \text{ kg}\cdot\text{m}^2$  can be necessary.

If a constant frequency is desired over a broad temperature range, interchangeable inertial elements with different values of  $I$  may be used, thereby permitting the moment of inertia to be varied in steps of less than 20 %, i.e. the frequency to be corrected in steps of less than 10 %. When testing standard specimens (see [6.2](#)) at a frequency of about 1 Hz, a maximum moment of inertia of about  $3 \times 10^{-3} \text{ kg}\cdot\text{m}^2$  is recommended.

#### 5.2.2 Method A (see [Figure 1](#))

The total mass of the inertial element, the lower clamp and the connecting rod shall be such that the weight,  $W$ , carried by the specimen is not too high [according to [Annex A, Formula \(A.2\)](#)].

#### 5.2.3 Method B (see [Figure 2](#))

The total mass of the inertial element, the upper clamp and the rod must be balanced by a suitable counterweight, so that the longitudinal force,  $W$ , acting on the specimen is minimized [according to [Annex A, Formula \(A.2\)](#)]. The wire supporting these parts is part of the elastically oscillating system.

### 5.3 Clamps

The clamps shall be designed to prevent movement of the portion of the specimens gripped within them. They shall be self-aligning in order to ensure that the specimen axis remains aligned with the axis of

rotation and the test specimen remains adequately secured over the whole temperature range without distortion occurring, thus allowing the free length of the specimen to be accurately determined.

The movable clamp shall be of low mass.

The moment of inertia of the whole system (consisting of the movable clamp, the inertial element and the connecting rod) shall be determined experimentally.

To prevent heat passing from the specimen out of the temperature-controlled chamber and in the opposite direction, the rod connecting the movable clamp and the inertial element shall be thermally non-conducting.

#### 5.4 Oscillation-inducing device

The oscillation-inducing device shall be capable of applying to the pendulum a torsional impulse such that the pendulum oscillates initially through an angle of not more than 1,5° in each direction for normal materials, or not more than 3° in each direction for low-modulus materials (such as elastomers).

#### 5.5 Oscillation-frequency and oscillation-amplitude recording equipment

Optical, electrical or other recording systems may be used provided they have no significant influence on the oscillating system. The entire equipment for measuring frequency and amplitude shall be accurate to  $\pm 1\%$  (within the transition region  $\pm 5\%$ ).

#### 5.6 Temperature-controlled chamber

According to ISO 6721-1.

#### 5.7 Gas supply

According to ISO 6721-1.

#### 5.8 Temperature-measurement device

According to ISO 6721-1.

#### 5.9 Devices for measuring test-specimen dimensions

According to ISO 6721-1.

### 6 Test specimens

#### 6.1 General

According to ISO 6721-1.

#### 6.2 Shape and dimensions

Rectangular test specimens having the following dimensions are recommended:

free length,  $L$ : 40 mm to 120 mm, preferably 50 mm

width,  $b$ : 5 mm to 11 mm, preferably 10 mm

thickness,  $h$ : 0,13 mm to 2 mm, preferably 1 mm

Specimens which are rectangular in cross-section but whose thickness and/or width varies along the main axis of the specimen by more than 3 % of the mean value shall not be used. When comparing different materials, the dimensions of the specimens shall be identical. Specimen dimensions differing from the preferred ones (50 mm × 10 mm × 1 mm) should be chosen to conserve geometric similarity with the preferred specimen shape.

Alternative specimen shapes may be used (e.g. cylindrical or tubular); in such cases, dimensions and tolerances shall be agreed upon by the interested parties.

### 6.3 Preparation

According to ISO 6721-1.

## 7 Number of specimens

According to ISO 6721-1.

## 8 Conditioning

According to ISO 6721-1.

If mechanical conditioning of the specimen is required, the specimen shall be twisted through an angle greater than 5°, but less than 90° in both directions about the torsional-test axis and returned to its normal position.

## 9 Procedure

### 9.1 Test atmosphere

According to ISO 6721-1.

### 9.2 Measurement of specimen cross-section

According to ISO 6721-1.

### 9.3 Mounting the test specimens

Clamp the test specimen between the upper and lower clamps. The longitudinal axis of the test specimen shall coincide with the axis of rotation of the oscillating system. Any misalignment of the specimen will cause lateral oscillations that will interfere with the normal oscillation process.

After clamping the test specimen, measure the distance between the clamps (the free length  $L$ ) to  $\pm 0,5$  %. When setting up the oscillating system in the chamber, check to make sure that the test specimen is not stressed.

After assembling the oscillating system complete with test specimen, and checking its alignment, start the heating or cooling (see [9.4](#)).

### 9.4 Varying the temperature

According to ISO 6721-1.

### 9.5 Performing the test

Start the free oscillations by setting the pendulum ([5.1](#)) in motion using the oscillation-inducing device ([5.4](#)).

Record the oscillation frequency and the oscillation amplitude as it decays.

Check that no amplitude decay is caused either by friction between moving and fixed parts of the apparatus or nonlinear behaviour of the material under test (see ISO 6721-1).

If the frequency is kept fixed during a temperature run, ensure that the inertial element is changed as and when necessary.

## 10 Expression of results

### 10.1 Symbols and correction factors

- b* width, in metres, of a rectangular specimen
- h* thickness, in metres, of a rectangular specimen
- L* free length, in metres, of specimen
- I* moment of inertia, expressed in kilogram metre squared (kg·m<sup>2</sup>), of the inertial element (if appropriate, including the movable clamp and the connecting rod)
- f<sub>d</sub>* frequency, in hertz, of the damped oscillating system
- f<sub>0</sub>* frequency, in hertz, of the pendulum as used in method B, without the specimen
- Λ* logarithmic decrement for damped oscillations of pendulum plus specimen
- Λ<sub>0</sub>* logarithmic decrement for damped oscillations of a method B pendulum, without the specimen
- F<sub>g</sub>* so-called dimensional factor for the specimen, expressed in reciprocal cubic metres (m<sup>-3</sup>)

For specimens with a rectangular cross-section:

$$F_g = 3L / bh^3 F_c \quad (1)$$

where *F<sub>c</sub>* is the so-called dimensional correction factor.

When  $0 \leq h/b \leq 0,6$

$$F_c = 1 - 0,63h/b \quad (2)$$

When  $0,6 \leq h/b \leq 1$

$$F_c = 0,843 / (1 + h^2/b^2) \quad (3)$$

For specimens with a circular cross-section:

$$F_g = 32L / \pi d^4 \quad (4)$$

where *d* is the diameter, in metres, of the specimen.

*F<sub>d</sub>* damping correction factor, given by the formula

$$F_d = 1 - (\Lambda / 2\pi)^2 \quad (5)$$

$G'_{to}$  torsional storage modulus, in pascals, of the specimen

$G''_{to}$  torsional loss modulus, in pascals, of the specimen

NOTE 1 [Formulae \(2\)](#) and [\(3\)](#) are only approximately valid, the maximum error being 0,9 % (see [Annex C](#)).

NOTE 2 The dimensional factor does not include any length corrections to allow for clamping effects. Therefore, only measurements carried out on specimens with the same thickness, width and length ratios will yield accurately comparable results (see ISO 6721-1).

## 10.2 Calculation of logarithmic decrement, $\Lambda$

The logarithmic decrement,  $\Lambda$ , may be calculated using [Formula \(6\)](#):

$$\Lambda = \ln(X_q / X_{q+1}) \quad (6)$$

where  $X_q$  and  $X_{q+1}$  are the amplitudes of two successive oscillations in the same direction (see ISO 6721-1).

To calculate  $\Lambda$  from the amplitudes of any two oscillations  $p$  and  $q$  in the same direction, use [Formula \(7\)](#):

$$\Lambda = \frac{1}{p-q} \ln(X_q / X_p) \quad (7)$$

where

$X_p$  is the amplitude of the  $p$ th oscillation;

$X_q$  is the amplitude of the  $q$ th oscillation.

The [Formula \(8\)](#) shall be used in the case of amplitudes that cannot be recorded on a damped sinusoidal curve with an accurate baseline (see [Figure 3](#)):

$$\Lambda = \ln(X_q^* / X_{q+1}^*) = \frac{1}{p-q} \ln(X_q^* / X_p^*) \quad (8)$$

where  $X_p^*$ ,  $X_q^*$ ,  $X_{q+1}^*$  are the differences between successive positive and negative amplitudes of the oscillation concerned, i.e.  $X_q^* = X_q^+ - X_q^-$ .

NOTE [Formula \(8\)](#) only corrects for a constant shift in the baseline, not for a time-dependent baseline drift. A time-dependent baseline drift can be caused by the non-oscillating part of the relaxation process, following application of the single pulse to start the system oscillating. It can be decreased by using double-pulse starting, with each pulse applied in a different direction.

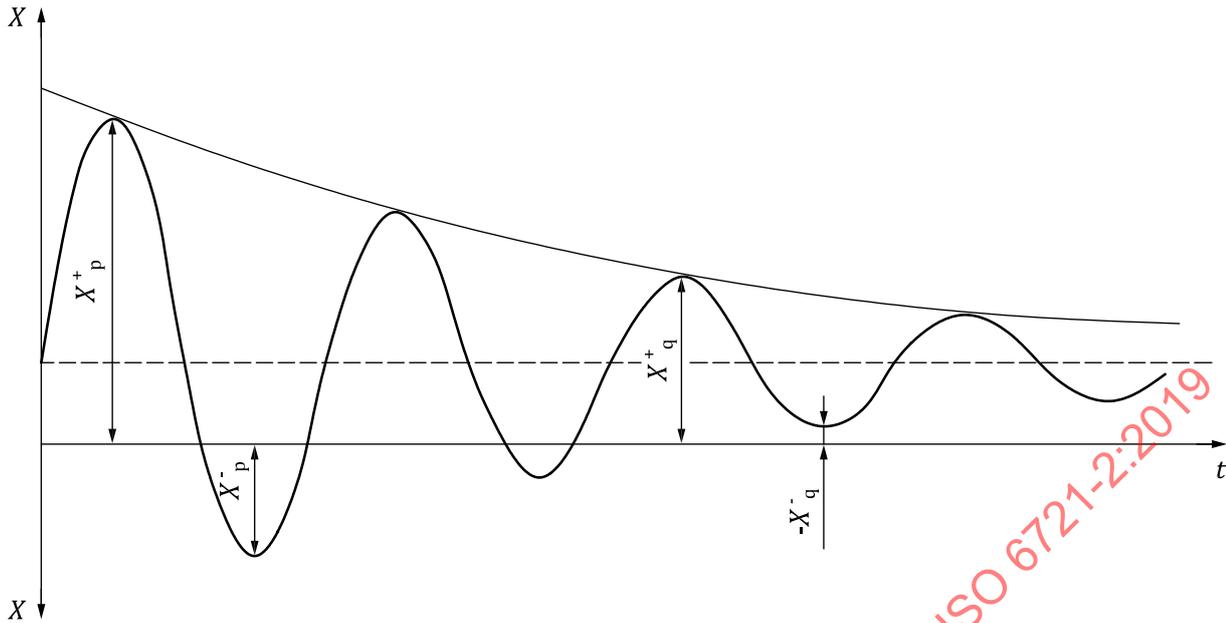


Figure 3 — Amplitude  $X$  versus time  $t$  for damped vibrations showing a baseline shift

### 10.3 Calculation of torsional storage modulus, $G'_{to}$

The torsional storage modulus (see ISO 6721-1) of a test specimen with a rectangular cross-section may be calculated from [Formula \(9\)](#).

$$G'_{to} = 4\pi^2 I (f_d^2 F_d - f_0^2) F_g \quad (9)$$

Assuming a rectangular cross-section with a low  $h/b$  ratio [see [Formulae \(1\)](#) and [\(2\)](#)] and inserting [Formula \(5\)](#), one obtains

$$G'_{to} = 12\pi^2 I f_d^2 \left[ 1 - (\Lambda/2\pi)^2 - (f_0/f_d)^2 \right] \times L / bh^3 F_c \quad (10)$$

$f_0$  being 0 for method A.

For rubber-like materials, high longitudinal forces acting upon the specimen shall be avoided (see [Annex A](#)).

### 10.4 Calculation of torsional loss modulus, $G''_{to}$

The torsional loss modulus  $G''_{to}$  (see ISO 6721-1) may be calculated from [Formula \(11\)](#).

$$G''_{to} = 4\pi I f_d^2 (\Lambda - \Lambda_0) F_g \quad (11)$$

$\Lambda_0$  being 0 for method A.

For method B, if  $\Lambda_0 \ll \Lambda$  and assuming a rectangular cross-section with a low  $h/b$  ratio [see [Formulae \(1\)](#) and [\(2\)](#)] and inserting [Formula \(5\)](#), one obtains

$$G''_{to} = 12\pi I f_d^2 \Lambda L / bh^3 F_c \quad (12)$$

## 11 Precision

The precision of this technique has been determined from the results of interlaboratory tests in which 15 laboratories participated<sup>[7]</sup>. Interlaboratory precision was as follows:

- for  $G'_{to}$  in the glassy region:  $\pm 7\%$ ;
- for  $G'_{to}$  at the glass-transition temperature:  $\pm 30\%$ ;
- for  $G''_{to}$  below the glass-transition temperature:  $\pm 10\%$ .

Utilizing  $G'_{to}$  or  $G''_{to}$ , the glass-transition temperature could be determined to within  $\pm 3^\circ\text{C}$ . The values for intralaboratory precision were about half those for interlaboratory precision.

NOTE The glass-transition temperature was determined from the point of inflexion of the  $\log G'_{to}$  versus temperature curve or from the maximum of the  $G''_{to}$  versus temperature curve associated with the glass transition.

## 12 Test report

The test report shall include the information given in the test report of ISO 6721-1 plus the following:

- a) a reference to this document (i.e. ISO 6721-2), plus the method (i.e. the type of pendulum) used (A or B), e.g. ISO 6721-2B;
- b) if a fixed frequency was used: the frequency chosen and the variation in frequency caused by changing the inertial element;
- c) if the same inertial element was used: the frequency range between the minimum temperature and the maximum temperature;
- d) if method A was used: the mass of the inertial element.

## Annex A (normative)

### Influence of longitudinal force, $W$

A longitudinally superimposed force  $W$  acting on the specimen generates an additional torsional stiffness, resulting in an apparent modulus increase  $\Delta G_W$ . This longitudinal force,  $W$ , is the total weight of all the parts that are suspended from the specimen. Therefore, the appropriate correction is necessary only for the pendulum used in method A, in which the disc, the rod and the lower clamp are suspended from the specimen. For the pendulum used in method B, the counterweight balances the force  $W$  (see [Figures 1](#) and [2](#)).

The modulus correction is given by

$$\Delta G_W = Wb / 4h^3 F_c \quad (\text{A.1})$$

and is subtracted from the value of the storage modulus, calculated from [Formula \(9\)](#). A number of points should be noted with regard to this correction, however:

- It is necessary only for measurements in the rubber elastic region.
- Rubbers show a so-called “primary normal stress difference”, however, which increases in proportion to the square of the shear strain. This effect produces a nonlinear, i.e. non-harmonic, distortion of the vibrations, which can be avoided by restricting measurements to small-amplitude vibrations.
- It is unclear how this effect should be taken into account for the loss modulus  $G''$ , since the basic equations have not been developed for viscoelasticity.

In order to overcome the difficulties listed above, any weight,  $W$ , that generates a modulus correction  $\Delta G_W$  greater than 1 % of the storage modulus  $G'_{to}$  shall be avoided, i.e. the following condition shall be satisfied:

$$W \leq 0,04 G'_{to} h^3 F_c / b \quad (\text{A.2})$$

The moment of inertia of a solid circular inertial element of constant thickness and diameter  $d$  and mass  $m$  is

$$I = md^2 / 8 \quad (\text{A.3})$$

The moment of inertia,  $I$ , and the mass,  $m$ , can therefore be adjusted independently to some extent.