
Anodizing of aluminium and its alloys — Measurement of specular reflectance and specular gloss of anodic oxidation coatings at angles of 20°, 45°, 60° or 85°

Anodisation de l'aluminium et de ses alliages — Mesurage des caractéristiques de réflectivité et de brillant spéculaires des couches anodiques à angle fixe de 20°, 45°, 60° ou 85°

STANDARDSISO.COM : Click to view the full PDF of ISO 7668:2018



STANDARDSISO.COM : Click to view the full PDF of ISO 7668:2018



COPYRIGHT PROTECTED DOCUMENT

© ISO 2018

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	2
5 Apparatus and geometric conditions	2
6 Optical standards	6
6.1 Reference standards	6
6.1.1 Black glass	6
6.1.2 Glass prism (for Method E only)	6
6.2 Working standards	7
6.2.1 Description	7
6.2.2 Zero point check	7
7 Preparation and calibration of apparatus	7
8 Measurement of specular reflectance and specular gloss	8
8.1 General	8
8.2 Measurement of specular reflectance	8
8.3 Measurement of specular gloss	8
9 Expression of results	11
9.1 General	11
9.2 Specular reflectance	11
9.3 Specular gloss	12
10 Test report	12
Annex A (normative) Specular reflectance and specular gloss of black glass	13

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 79, *Light metals and their alloys*, Subcommittee SC 2, *Organic and anodic oxidation coatings on aluminium*.

This third edition cancels and replaces the second edition (ISO 7668:2010), which has been technically revised. The main technical changes are as follows:

- the normative references have been added;
- the definition of specular gloss has been revised;
- the references to CIE spectral luminous efficiency and CIE standard illuminants C and D65 have been added.

Introduction

Specular reflectance and specular gloss are not unique physical properties of a surface. They vary with the angle of measurement, and with the aperture dimensions that define the incident and the reflected beams, such that measurements of these properties are not independent of the apparatus being used.

The specular reflectance of most surfaces increases with the angle of measurement and accounts for the use of reflectometers with various angles as, for example, for painted surfaces. The specular reflectance characteristics of anodized aluminium, however, do not always behave in the normal manner and, because of its property of double reflection, reflected light comes partly from the film surface and partly from the underlying metal. It is advisable to measure the specular reflectance characteristics at 20°, 45°, 60° and 85° to obtain a complete understanding of the specular reflectance properties of the anodized surface, and careful thought should be given to which method or methods are most relevant in any particular situation. The specular reflectance of bright-anodized aluminium with a mirror finish is best measured using 45° or 20° geometry.

STANDARDSISO.COM : Click to view the full PDF of ISO 7668:2018

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 7668:2018

Anodizing of aluminium and its alloys — Measurement of specular reflectance and specular gloss of anodic oxidation coatings at angles of 20°, 45°, 60° or 85°

1 Scope

This document specifies methods for the measurement of specular reflectance and specular gloss of flat samples of anodized aluminium using geometries of 20° (Method A), 45° (Method B), 60° (Method C) and 85° (Method D); and of specular reflectance by an additional 45° method (Method E) employing a narrow acceptance angle.

The methods described are intended mainly for use with clear anodized surfaces. They can be used with colour-anodized aluminium, but only with similar colours.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 7583, *Anodizing of aluminium and its alloys — Terms and definitions*

ISO 11664-1, *Colorimetry — Part 1: CIE standard colorimetric observers*

ISO 11664-2, *Colorimetry — Part 2: CIE standard illuminants*

CIE Publication No. 15, *Colorimetry*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 7583 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

3.1

specular reflectance

ratio of the luminous flux, reflected in the specular direction for a specified source and receptor angle, to the luminous flux of the incident light

Note 1 to entry: Normally expressed as a percentage.

3.2

specular gloss

ratio of the luminous flux, reflected from an object in the specular direction for a specified source and receptor angle, to the luminous flux reflected from glass with a refractive index of 1,567 at a wavelength of 546,1 nm (which is the central wavelength of the spectral luminous efficiency function) in the specular direction

Note 1 to entry: To set the specular gloss scale, polished black glass with a refractive index of 1,567 is assigned the value of 100 for geometries of 20°, 45°, 60° and 85° (see [Table 5](#)). The phenomenon of light reflectance by anodized aluminium is very different to that of black glass and the choice of a black-glass standard is arbitrary and made to allow comparison of different qualities of anodized aluminium.

4 Principle

The specular reflectance and specular gloss of anodized aluminium surfaces are measured under defined conditions using, as required, geometries of 20°, 45°, 60° and 85°.

5 Apparatus and geometric conditions

Usual laboratory apparatus and in particular the following.

5.1 General. Approximate comparisons between surfaces of the same colour can be made, but an accurate measurement requires the combination of light source, photoelectric cell and associated colour filters to give a spectral sensitivity, approximating to the CIE spectral luminous efficiency, $V(\lambda)$, weighted for CIE standard illuminants C or D65. $V(\lambda)$ shall conform to the requirements of ISO 11664-1. CIE standard illuminants C and D65 shall conform to the requirements of CIE 15 and ISO 11664-2.

NOTE Since specular reflection is in general spectrally non-selective, the spectral characteristics of the light source ([5.2](#)) and the receptor ([5.4](#)) do not affect the measurement of normal uncoloured anodized surfaces.

5.2 Polychromatic light source and housing, with a lens that directs a parallel, or very slightly converging, beam of light onto the surface under test.

5.3 Means for locating the specimen surface, in the correct position for measurement.

5.4 Receptor housing containing a lens, a receptor aperture and a photoelectric cell, to receive the cone of reflected light.

5.5 Sensitivity control, for setting the photocell current to any desired value on the instrument scale or digital indicator.

5.6 Receptor meter, capable of giving an indication proportional to the light flux passing the receptor aperture within 1 % of the full-scale reading. Spectral corrections are not usually required (see Note to [5.1](#)).

5.7 Geometric conditions

The incident angle, ε_1 , which is the angle between the axis of the incident beam and the perpendicular to the surface under test, shall have the following values and tolerances:

- for Method A: 20° ± 0,1°;
- for Method B: 45° ± 0,1°;
- for Method C: 60° ± 0,1°;
- for Method D: 85° ± 0,1°;
- for Method E: 45° ± 0,1°.

There shall be no vignetting of rays that lie within the angles specified above.

The axis of the receptor shall, as far as possible, coincide with the mirror image of the axis of the incident beam; the receptor angle, ε_2 , which is the angle between the axis of the receptor and the perpendicular to the surface under test, shall be for all methods such that

$$|\varepsilon_1 - \varepsilon_2| \leq 0,1^\circ$$

With a flat piece of polished glass or other front-surface mirror in the test specimen position, an image of the source shall be formed at the centre of the receptor aperture. The width of the illustrated area of the test specimen shall be not less than 10 mm.

The angular dimensions of the receptor apertures shall be measured from the receptor lenses. The dimensions and tolerances of the sources and receptors shall be as indicated in [Tables 1 and 2](#). [Figures 1, 2 and 3](#) give generalized illustrations of these dimensions. [Table 1](#) gives both angles and corresponding dimensions calculated for lenses of a focal length of 50 mm for Methods A, B, C and D. [Table 2](#) gives the angles and aperture dimensions for Method E. The angles are mandatory and the aperture sizes have been calculated from the corresponding angle, δ , as $2f(\tan \delta/2)$, where f is the focal length of the receptor lens.

Table 1 — Angles and dimensions of source image and receptor apertures for Methods A, B, C and D

Method(s)	Instrument characteristics	In plane of measurement		Perpendicular to plane of measurement	
		Angle δ_1 degrees (°)	Dimension ^a mm	Angle δ_2 degrees (°)	Dimension ^a mm
A, B, C and D	Source image size	0,75($\delta_{1\alpha}$)	0,65	2,5($\delta_{2\alpha}$)	2,18 ^b
	Tolerance	$\pm 0,25$	$\pm 0,22$	$\pm 0,5$	$\pm 0,44$
A	20° Receptor aperture	1,80($\delta_{1\beta}$)	1,57	3,6($\delta_{2\beta}$)	3,14
	Tolerance	$\pm 0,05$	$\pm 0,04$	$\pm 0,1$	$\pm 0,09$
B	45° Receptor aperture	4,4($\delta_{1\beta}$)	3,84	11,7($\delta_{2\beta}$)	10,25
	Tolerance	$\pm 0,1$	$\pm 0,09$	$\pm 0,2$	$\pm 0,17$
C	60° Receptor aperture	4,4($\delta_{1\beta}$)	3,84	11,7($\delta_{2\beta}$)	10,25
	Tolerance	$\pm 0,1$	$\pm 0,09$	$\pm 0,2$	$\pm 0,17$
D	85° Receptor aperture	4,0($\delta_{1\beta}$)	3,49	6,0($\delta_{2\beta}$)	5,24
	Tolerance	$\pm 0,3$	$\pm 0,26$	$\pm 0,3$	$\pm 0,26$


^a Calculated for a focal length of 50 mm. For any other focal length, f , these dimensions shall be multiplied by $f/50$.

^b $0,75^\circ \pm 0,25^\circ$; corresponding to dimensions of $0,65 \text{ mm} \pm 0,22 \text{ mm}$, i.e. the same as those in the plane of measurement, is also recommended.


Table 2 — Angles and dimensions of circular source image and circular receptor aperture for 45° reflectometer of Method E

Instrument characteristics	Angle δ degrees (°)	Dimension ^a mm
Source image size	3,44	1,5
Tolerance	$\pm 0,23$	$\pm 0,1$
45° Receptor aperture	3,44	1,5
Tolerance	$\pm 0,23$	$\pm 0,1$

^a Calculated for focal length of 25,4 mm. For any other focal length, f , the aperture diameter is equal to $2f(\tan \delta/2)$.

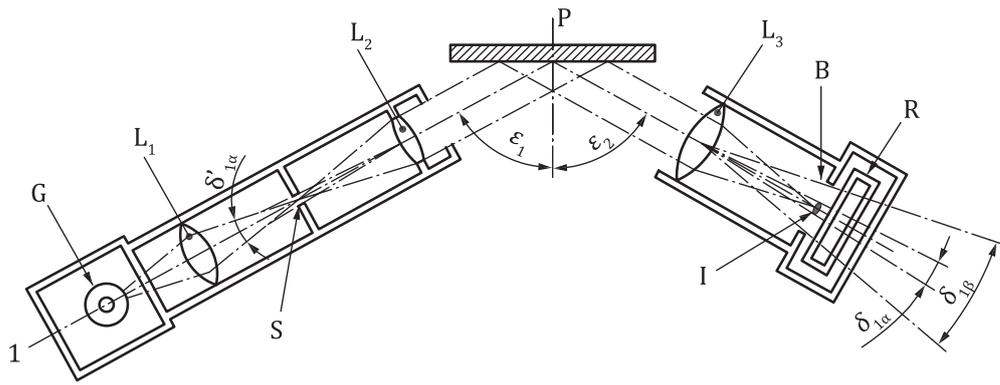

a) In plane of measurement

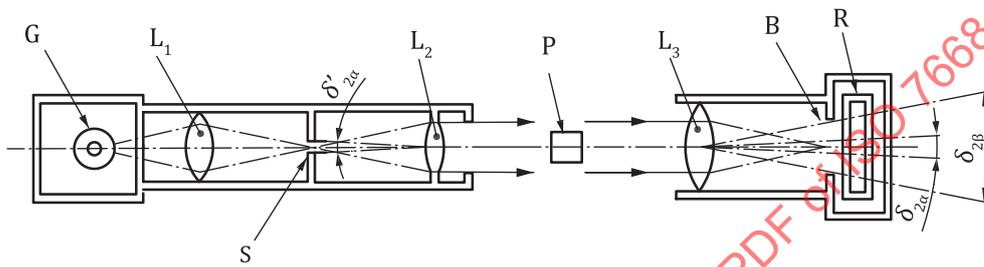


b) Perpendicular to plane of measurement

Key


- | | | | |
|----------------|-----------------------------------|--|--|
| 1 | axis | $\delta_{1\alpha}$ | source image angles (in plane of measurement) |
| G | filament lamp | $\delta_{1\beta}$ | receptor aperture angles (in plane of measurement) |
| L ₁ | condenser lens | $\delta_{2\alpha}$ | source image angles (perpendicular to plane of measurement) |
| L ₂ | collimator lens | $\delta_{2\beta}$ | receptor aperture angles (perpendicular to plane of measurement) |
| L ₃ | receptor lens | $\delta'_{1\alpha} = \delta_{1\alpha}$ and $\delta'_{2\alpha} = \delta_{2\alpha}$ if the focal lengths of L ₂ and L ₃ are the same | |
| S | effective light source (pin note) | ϵ_1 | incident angle |
| P | test surface | ϵ_2 | receptor angle |
| B | receptor field aperture | | |
| I | source image | | |
| R | photoelectric cell | | |

NOTE Angles and dimensions are given in [Table 1](#).

Figure 1 — Schematic arrangement of apparatus showing apertures and source image formation for a collimated-beam-type instrument for Method A (20°), Method B (45°), Method C (60°) and Method D (85°)

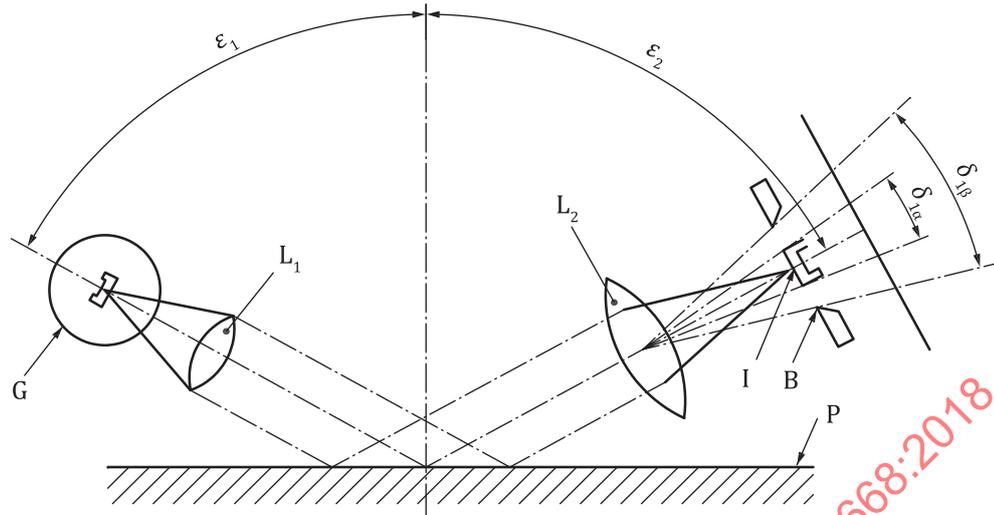

a) In plane of measurement

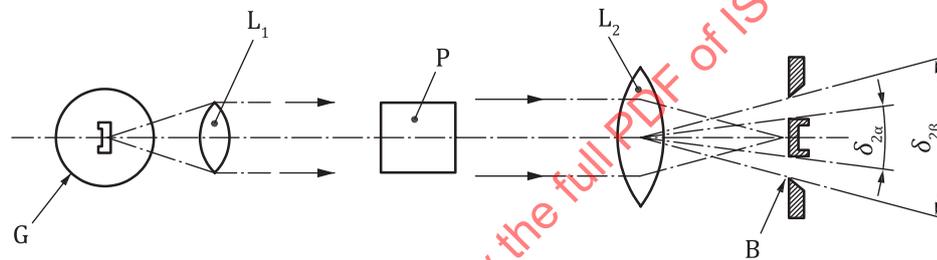


b) Perpendicular to plane of measurement

Key

- | | | | |
|-----------------|-------------------------|---|--------------------------|
| G | filament lamp | $\delta_{1\alpha}$ and $\delta_{2\alpha}$ | source image angles |
| L_1 and L_2 | lenses | $\delta_{1\beta}$ and $\delta_{2\beta}$ | receptor aperture angles |
| P | test surface | ϵ_1 | incident angle |
| B | receptor field aperture | ϵ_2 | receptor angle |
| I | image filament | | |

NOTE Angles and dimensions are given in [Table 1](#).

Figure 2 — Schematic arrangement of apparatus showing apertures and source image formation for a non-collimated-beam type instrument for Method A (20°), Method B (45°), Method C (60°) and Method D (85°)

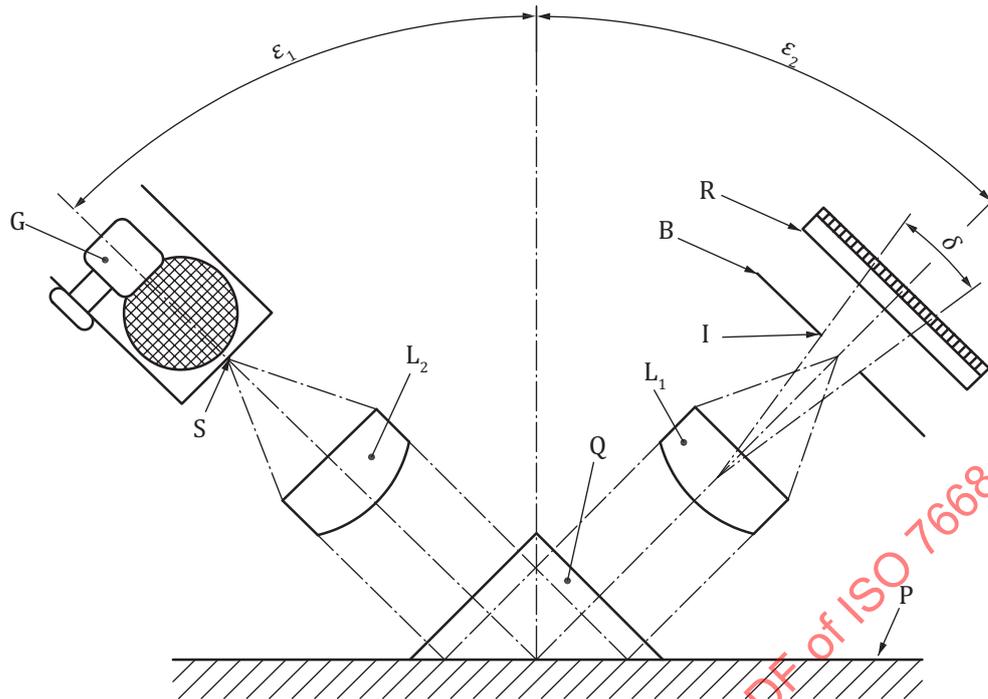

Key

G	lamp with frosted surface	δ	receptor aperture angle
L_1 and L_2	lenses	ϵ_1	incident angle
B	receptor field aperture	ϵ_2	receptor angle
P	test surface	$\epsilon_1 = \epsilon_2 = 45^\circ \pm 0,1^\circ$	
Q	glass prism for calibration		
S	source aperture		
I	source image		
R	photoelectric cell		

NOTE Angles and dimensions are given in [Table 2](#).

Figure 3 — Schematic arrangement of optical system of 45° specular reflectance meter for Method E

6 Optical standards

6.1 Reference standards

6.1.1 Black glass

The primary reference standard shall be made of highly polished black glass of refractive index 1,567 (or clear glass with the back and edges roughened and coated with black paint), the top surface being plane to within two fringes per centimetre as measured by optical interference methods. The effect of the refractive index on specular reflectance and specular gloss values shall be as described in [Annex A](#).

The glass surface shall be kept in a clean condition and free from surface scratches or damage.

6.1.2 Glass prism (for Method E only)

An alternative reference standard, recommended for Method E and suitable only for 45° reflectometers, is provided by the hypotenuse face of a right-angled glass prism, having dimensions

of 25 mm × 25 mm × 35,3 mm and optically worked faces. This uses the principle of total internal reflection for angles greater than the critical angle, but there are losses on entering the prism faces. These can also be calculated from Fresnel's equation (see [A.1](#)) to give the absolute specular reflectance values given in [Table 3](#).

The glass shall be in a perfectly clean condition, maintained free from grease and scratches, and with the hypotenuse face accurately located in the correct plane.

Table 3 — Specular reflectance values for glass prisms

Refractive index	Specular reflectance for 45° angle
	%
1,500	92,16
1,523	91,59
1,567	90,48
1,600	89,63

6.2 Working standards

6.2.1 Description

Working standards shall comprise front-silver-mirrored or anodized aluminium surfaces of uniform appearance and good planarity which have been calibrated against a primary reference standard (see [6.1](#)) for an indicated area and direction of illumination, which shall be clearly marked on the working standard. Working standards shall be checked periodically by comparison with primary reference standards. The working standards shall be uniform and stable. At least two working standards, of different specular reflectance or specular gloss levels, shall be available for each geometry.

6.2.2 Zero point check

A black box or black velvet shall be used for checking the zero point of the display.

7 Preparation and calibration of apparatus

Calibrate the apparatus at the start of every period of operation and during operation at intervals sufficiently frequent to ensure that the instrument response is essentially constant.

Using a primary reference standard, or the higher of two working standards, adjust the instrument reading to the correct or selected value in the upper part of the scale with the sensitivity control ([5.5](#)). If a black-glass standard is used, the instrument shall indicate the relevant specular reflectance value, as indicated in [Table 4](#), for the specular reflectance measurement, or the relevant specular gloss value, as indicated in [Table 5](#), for the specular gloss measurement. If a glass prism is used for Method E, set the reading to the correct value as indicated in [Table 3](#).

Take a second working standard of known specular reflectance or specular gloss for the angle being used, having a value in the lower half of the scale, and make a measurement with the same control settings.

For the specular reflectance measurement, if the reading for the second working standard is within 1 % of its assigned reflectance value it conforms with the proportionality requirement of [5.6](#). For the specular gloss measurement, if the reading for the second working standard in Methods A, B and C is within 1 gloss unit of its assigned value it conforms with the proportionality requirement of [5.6](#). For Method D, the reading for the second working standard with a 60° gloss lower than 10 gloss units shall be within 1 gloss unit of its assigned value. For the second working standard with a 60° gloss higher than 10 gloss units, the reading may be within 2 gloss units of its assigned value.

If there is not conformance with these requirements, the instrument shall be adjusted by the manufacturer, or in accordance with the manufacturer's instructions, and the calibration procedure repeated until the second working standard can be measured with the required accuracy.

NOTE The most common cause of incorrect results is damage or distortion of standards through lack of flatness, presence of dirt, or failure to locate the surface in the correct plane for measurement.

8 Measurement of specular reflectance and specular gloss

8.1 General

Calibrate the instrument as directed in [Clause 7](#) and measure the specular reflectance or specular gloss of the test specimen by placing it in firm contact with the instrument so that the plane of incidence and reflection is parallel to the direction of rolling or machining of the test specimen. Measurement can be carried out in a plane normal to this direction if the anisotropy of the surface under examination is to be assessed.

8.2 Measurement of specular reflectance

For surfaces of low specular reflectance, set the black-glass primary reference standard (see [6.1.1](#)) to read 10 times the relevant specular reflectance value in [Table 4](#) and multiply each reading by 0,1.

For surfaces with a high specular reflectance, set the apparatus to the relevant specular reflectance value specified in [Table 4](#), using a black-glass primary reference standard. Alternatively, in the case of Method E, the reflectometer may be set to the appropriate specular reflectance value specified in [Table 3](#), using a glass prism (see [6.1.2](#)).

NOTE Specular reflectance values which are encountered in practice can cover a very wide range, from 90 % to less than 0,1 %, and only in the case of bright finishes, or with the 85° method, is it practicable to obtain a direct reading of specular reflectance.

8.3 Measurement of specular gloss

Using a black-glass primary reference standard, set the apparatus to the relevant specular gloss value specified in [Table 5](#).

For surfaces with a high specular gloss, in excess of 100 gloss units, set the black-glass primary reference standard at an arbitrary selected value of 0,5 or 0,2 or 0,1 of the specular gloss value in [Table 5](#) and multiply each reading by the corresponding factor (2 or 5 or 10, respectively).

Table 4 — Specular reflectance values for polished black glass

Refractive index <i>n</i>	Angle of incidence			
	20°	45°	60°	85°
1,400	2,800	3,658	7,200	59,832
1,410	2,917	3,791	7,376	60,012
1,420	3,035	3,925	7,552	60,183
1,430	3,155	4,060	7,728	60,345
1,440	3,276	4,196	7,901	60,499
1,450	3,398	4,332	8,074	60,646
1,460	3,522	4,469	8,245	60,786
1,470	3,646	4,607	8,416	60,919
1,480	3,772	4,746	8,584	61,045
1,490	3,899	4,884	8,752	61,166
1,500	4,027	5,024	8,919	61,280
1,510	4,156	5,164	9,084	61,389
1,520	4,285	5,305	9,248	61,492
1,530	4,416	5,446	9,411	61,591
1,540	4,548	5,587	9,573	61,684
1,550	4,681	5,729	9,734	61,773
1,560	4,814	5,871	9,894	61,858
1,567 ^a	4,908 ^a	5,971 ^a	10,006 ^a	61,914 ^a
1,570	4,948	6,014	10,053	61,938
1,580	5,083	6,157	10,211	62,015
1,581	5,102	6,177	10,233	62,025
1,590	5,219	6,299	10,368	62,087
1,600	5,355	6,443	10,524	62,156
1,610	5,493	6,587	10,679	62,221
1,617	5,592	6,691	10,800	62,266
1,620	5,630	6,731	10,833	62,283
1,630	5,769	6,876	10,986	62,342
1,640	5,908	7,020	11,138	62,397
1,648	6,015	7,132	11,255	62,438
1,650	6,048	7,165	11,289	62,449

^a Standard reference sample.

Table 4 (continued)

Refractive index <i>n</i>	Angle of incidence			
	20°	45°	60°	85°
1,660	6,188	7,310	11,440	62,499
1,670	6,329	7,455	11,590	62,545
1,680	6,470	7,601	11,738	62,589
1,690	6,611	7,746	11,886	62,631
1,700	6,754	7,892	12,034	62,697
1,710	6,896	8,038	12,180	62,706
1,720	7,039	8,183	12,325	62,740
1,730	7,183	8,329	12,470	62,772
1,740	7,327	8,475	12,614	62,802
1,750	7,471	8,621	12,758	62,830
1,760	7,615	8,767	12,901	62,856
1,770	7,760	8,914	13,043	62,879
1,780	7,905	9,060	13,184	62,901
1,790	8,051	9,206	13,324	62,921
1,800	8,197	9,352	13,346	62,940

^a Standard reference sample.

Table 5 — Specular gloss values for polished black glass

Refractive index <i>n</i>	Angle of incidence			
	20°	45°	60°	85°
1,400	57,0	61,3	71,9	96,6
1,410	59,4	63,5	73,7	96,9
1,420	61,8	65,7	75,5	97,2
1,430	64,3	68,0	77,2	97,5
1,440	66,7	70,3	79,0	97,6
1,450	69,2	72,6	80,7	98,0
1,460	71,8	74,9	82,4	98,2
1,470	74,3	77,2	84,1	98,4
1,480	76,9	79,5	85,8	98,6
1,490	79,4	81,8	87,5	98,8
1,500	82,0	84,1	89,1	99,0
1,510	84,7	86,5	90,8	99,2
1,520	87,3	88,8	92,4	99,3
1,530	90,0	91,2	94,1	99,5
1,540	92,7	93,6	95,7	99,6

^a Standard reference sample.