
**Anodizing of aluminium and its alloys —
Measurement of reflectance
characteristics of aluminium surfaces
using a goniophotometer or an abridged
goniophotometer**

*Anodisation de l'aluminium et de ses alliages — Mesurage des
caractéristiques de réflectivité des surfaces d'aluminium à l'aide d'un
goniophotomètre normal ou simplifié*

STANDARDSISO.COM : Click to view the full PDF of ISO 7759:2010



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 7759:2010



COPYRIGHT PROTECTED DOCUMENT

© ISO 2010

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle.....	1
5 Apparatus	2
6 Preparation and calibration of apparatus	5
6.1 General conditions	5
6.2 Geometric conditions.....	5
6.3 Spectral conditions	6
6.4 Calibration	6
7 Procedure	6
8 Expression of results	6
8.1 General	6
8.2 Specular reflectance R_s	6
8.3 Distinctness of reflected image R_i	6
8.4 Narrow-angle haze H_n	6
8.5 Wide-angle haze H_w	6
8.6 Diffuseness R_d	7
8.7 Directionality D_h	7
9 Test report.....	7
Annex A (informative) Precision and accuracy of goniophotometers	8
Bibliography.....	9

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 7759 was prepared by Technical Committee ISO/TC 79, *Light metals and their alloys*, Subcommittee SC 2, *Organic and anodic oxidation coatings on aluminium*.

This second edition cancels and replaces the first edition (ISO 7759:1983), which has been technically revised.

STANDARDSISO.COM : Click to view the full PDF of ISO 7759:2010

Introduction

The visual appearance of metallic finishes is important commercially on metals for automotive, architectural, and other uses where these metals undergo special finishing processes to produce the desired appearance. For end-products which use such finished metals, it is important that parts placed together have the same appearance. Specular reflectance is one of the properties measured, but additional measurements are usually required to identify adequately the appearance of any metal surface. In the method described in this International Standard, several important aspects of surface appearance are identified and can be measured. Those surfaces having identical sets of numbers will normally have the same reflectance characteristics and the same appearance (see References [1], [2] and [3]).

STANDARDSISO.COM : Click to view the full PDF of ISO 7759:2010

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 7759:2010

Anodizing of aluminium and its alloys — Measurement of reflectance characteristics of aluminium surfaces using a goniophotometer or an abridged goniophotometer

1 Scope

This International Standard specifies a method for the measurement of the reflectance characteristics of high-gloss anodized aluminium surfaces.

The method described is also suitable for the measurement of the reflectance characteristics of other high-gloss metal surfaces.

The method is not suitable for diffuse-finish metal surfaces and does not measure colour.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

CIE 38:1977, *Radiometric and Photometric Characteristics of Materials and their Measurement*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

goniophotometer

instrument in which specimens can be illuminated at selected angles of incidence and in which the light reflected in different directions can be measured

3.2

abridged goniophotometer

goniophotometer having a fixed angle of incidence and specific fixed direction(s) at which light reflected from the specimen is measured

NOTE The instrument described in this International Standard uses an angle of incidence of 30° and directions for measurement of reflected light of -30° , $-30^\circ \pm 0,3^\circ$, $-30^\circ \pm 2^\circ$, $-30^\circ \pm 5^\circ$, and -45° , although some suitable instruments can be measured only on one side of the 30° angle.

4 Principle

4.1 The visual appearance of an anodized aluminium surface is characterised by means of six different properties (see 4.2 to 4.7) of the reflected light coming from a narrow-source beam incident on the surface at an angle of 30° .

4.2 Specular reflectance, R_s , is measured at 30° to the specimen normal using narrow source and receiver field angles ($0,50^\circ$ wide, maximum in the plane of the angle of reflection).

4.3 Distinctness of reflected image, R_i , is determined from the slightly off-specular reflectance ($R_{30 \pm 0,3}$) measured at $29,7^\circ$ and $30,3^\circ$, the instrument integrating the light received from both of these apertures.

4.4 Narrow-angle haze, H_n , is determined from reflectance measurements taken at angles of 28° or 32° or both, i.e. at 2° away from the specular beam ($R_{30 \pm 2}$).

4.5 Wide-angle haze, H_w , is determined from reflectance measurements taken at angles of 25° or 35° or both, i.e. 5° away from the specular beam ($R_{30 \pm 5}$).

4.6 Diffuseness, R_d , is determined from a reflectance measurement taken at an angle of 45° , i.e. 15° away from the specular beam (R_{45}).

4.7 Directionality, D_n , of the surface, derived from the ratio of two measurements of the narrow-angle haze, H_n , the first taken when the incident light is perpendicular to the direction of the surface texture and the second when the incident light is parallel to the surface texture, i.e. the rolling, extrusion or machining direction.

5 Apparatus


5.1 **Goniophotometer** or **abridged goniophotometer**, see Figures 1 and 2, capable of achieving the specific beam and field angles given in Table 1. The voltage regulation of the instrument shall be set to $\pm 0,01\%$.

NOTE Details of the precision and accuracy of goniophotometers are given in Annex A.

Table 1 — Dimensions of the mirror image of the source-slit, and of the receiver windows measured in the same plane (see Figures 1 and 2)

Values in degrees

Parameter	Source-slit mirror image	Specular receiver window	Distinctness-of-image receiver window	Haze receiver windows		Diffuseness receiver window
Angle of centre of window (measured from perpendicular to specimen surface)	$30,0 \pm 0,4$	$30,0 \pm 0,4$	$30,30 \pm 0,04$ and $29,70 \pm 0,04$	$28,0 \pm 0,4$ and $32,0 \pm 0,4$	$25,0 \pm 0,4$ and $35,0 \pm 0,4$	$45,0 \pm 0,4$
Width (in the plane of the angle of reflection)	$0,44 \pm 0,01$	$0,40 \pm 0,01$	$0,14 \pm 0,01$	$0,4 \pm 0,1$	$0,5 \pm 0,1$	$2,0 \pm 0,2$
Length (across the plane of the angle of reflection)	$5,0 \pm 1,0$	$3,0 \pm 1,0$	$3,0 \pm 1,0$	$3,0 \pm 1,0$	$3,0 \pm 1,0$	$3,0 \pm 1,0$

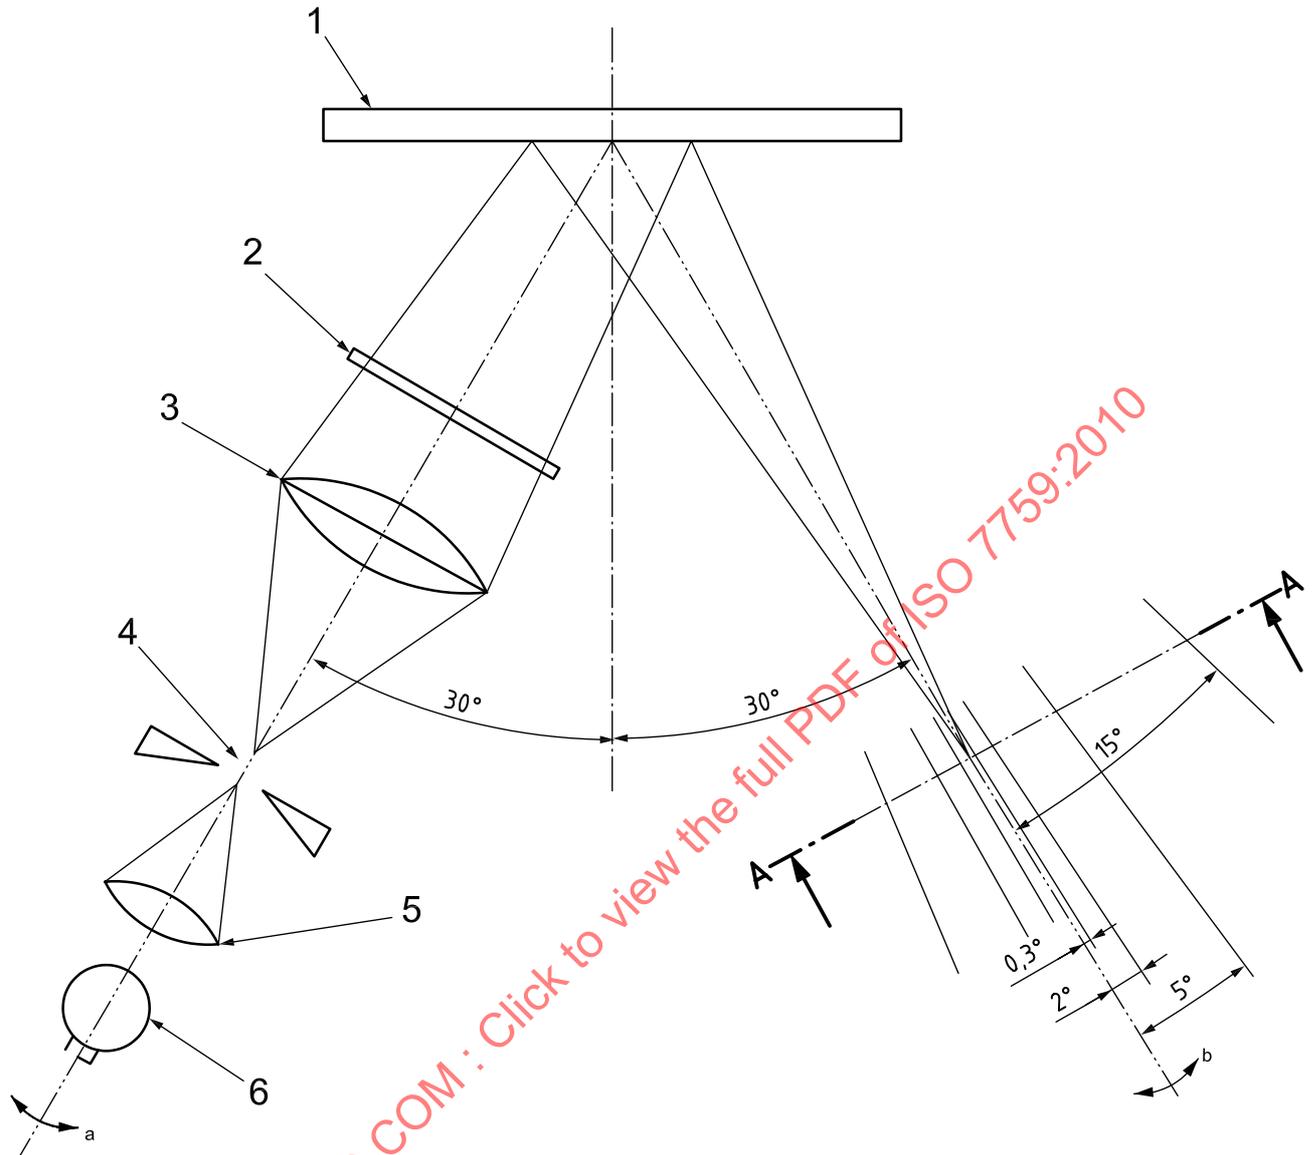


Key

- 1 test piece
- 2 neutral density filter (for high-specularity materials)
- 3 source object lens
- 4 source slit
- 5 condenser lens
- 6 lamp

- a Source-arm centre-line adjustment for maximum peak (optional).
- b Receiver-window array centre-line adjustment for maximum peak (optional).

Figure 1 — Optical diagram of a typical abridged goniophotometer: general geometry of measurement (angles not to scale)

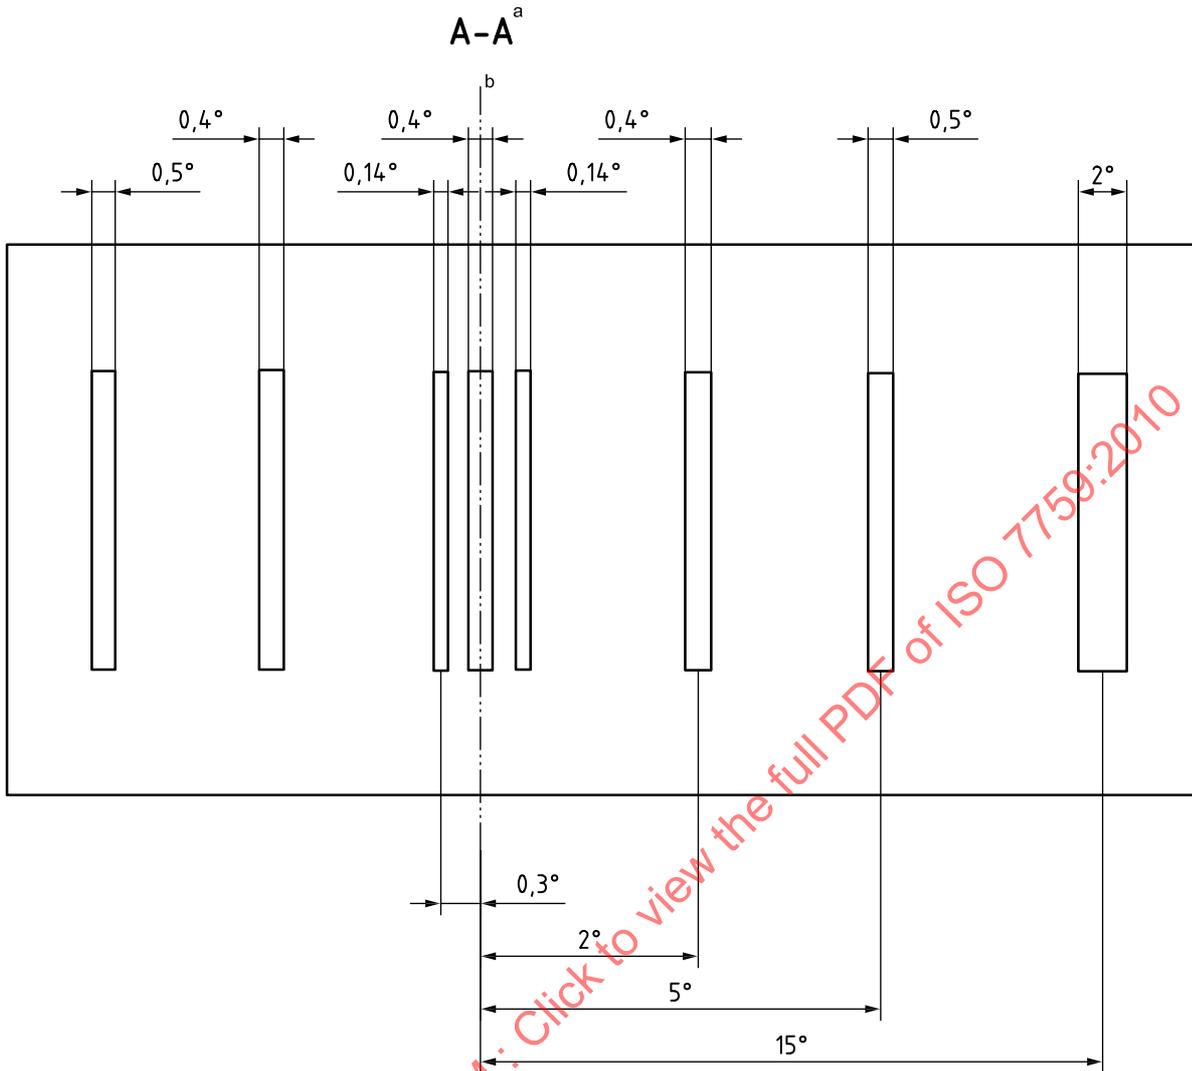

- a Sectional drawing from Figure 1.
- b Centre of reflected beam.

Figure 2 — Optical diagram of a typical abridged goniometer: arrangement of receiver windows (not to scale)

5.2 Rotatable clamp, of the type shown in Figure 3, for flattening and positioning the specimen during measurement.

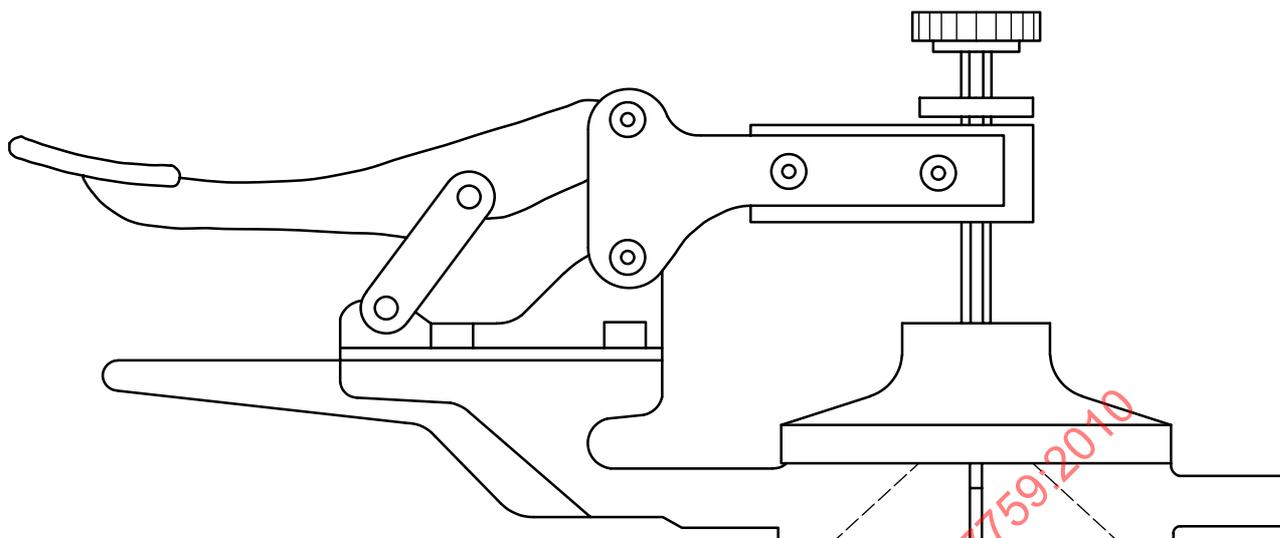


Figure 3 — Rotatable clamp suitable for flattening the test piece and positioning it during measurement

5.3 Reflectance standards

5.3.1 Three calibrated reflectance standards shall be available.

- a) Aluminium evaporated onto plate glass and covered with a protective coating of silicon monoxide, and calibrated for specular reflectance and distinctness of the reflected image. The specular reflectance shall be $85\% \pm 10\%$.
- b) Chromium evaporated onto plate glass and covered with a protective coating of silicon monoxide and calibrated for specular reflectance and distinctness of the reflected image. The specular reflectance shall be $62\% \pm 10\%$.
- c) Reflecting plate with a white diffuse surface from which reflected light has a substantially constant luminance over the angular range of the instrument.

Where the distinctness of the reflected image is being measured, standards intermediate in reflectance and made from anodized aluminium may be useful.

5.3.2 It is essential that standards are kept clean and free from scratches, as well as from contact with contaminating materials. Follow the cleaning method specified by the instrument manufacturer and check standards at regular intervals against reference standards held in reserve.

6 Preparation and calibration of apparatus

6.1 General conditions

Use the instrument (see 5.1) in a clean dry area free from draughts. Switch the instrument on at least 30 min before use.

6.2 Geometric conditions

The direction of incidence shall be 30° . The directions of view shall be opposite to the directions of incidence at angles of -30° , $-30^\circ \pm 0,3^\circ$, $-30^\circ \pm 2^\circ$, $-30^\circ \pm 5^\circ$ and -45° . The angular dimensions of the mirror reflected image of the source-slit in the plane of measurement, and the angular dimensions of the receiver windows in this plane of measurement, shall be as shown in Table 1.

6.3 Spectral conditions

The measurement shall be made using a source of visible light with appropriate filters, such that the spectral product of the light source, spectral filters and spectral response of the light detector shall closely simulate the spectral product of CIE Standard Illuminant C (or D₆₅) and the standard observer function, in accordance with CIE 38:1977.

6.4 Calibration

Adjust the instrument to read the same arbitrary reflectance value for the intensity of light reflected from the diffuse white standard [see 5.3.1 c)] through the specular, distinctness-of-image and haze apertures. Adjust the instrument to read the values of specular reflectance and distinctness of reflected image assigned to the aluminium mirror [see 5.3.1 a)]. If the instrument does not then read the values for the chromium standard [see 5.3.1 b)] within the limits set by the instrument manufacturer, refocus or recalibrate following the manufacturer's instructions.

7 Procedure

Measure the test piece and insert it with the plane of measurement parallel to the longitudinal direction. Clamp the test piece to ensure adequate flatness during observation. To locate the exact longitudinal direction, rotate the clamp (5.2) with the specimen in it to the maximum indication of specular reflectance or distinctness of reflected image, whichever is the more sensitive. After observations in the longitudinal direction, rotate the test piece in the clamp through 90° for the required transverse observations. Measure three separate areas in each direction. Take readings on the reflectance standards (5.3) at frequent intervals and at the end of a series of observations to ensure that the instrument has remained in calibration throughout the operation.

8 Expression of results

8.1 General

Calculate the mean of the three readings on the test piece in both the longitudinal and transverse directions, and for each of the apertures (see Clause 4), using the equations given in 8.2 to 8.7.

8.2 Specular reflectance R_s

$$R_s = R_{30}$$

8.3 Distinctness of reflected image R_i

$$R_i = \left(1 - \frac{R_{30 \pm 0.3}}{R_s} \right) \times 100$$

8.4 Narrow-angle haze H_n

$$H_n = \left(\frac{R_{30 \pm 2}}{R_s} \right) \times 100$$

8.5 Wide-angle haze H_w

$$H_w = \left(\frac{R_{30 \pm 5}}{R_s} \right) \times 100$$