
INTERNATIONAL STANDARD



782

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION • МЕЖДУНАРОДНАЯ ОРГАНИЗАЦИЯ ПО СТАНДАРТИЗАЦИИ • ORGANISATION INTERNATIONALE DE NORMALISATION

Microcopying — Measurement of screen luminance of microfilm readers

Microcopie — Mesurage de la luminance des écrans d'appareils de lecture

First edition — 1975-10-15

STANDARDSISO.COM :: Click to view the full PDF of ISO 782:1975

To become ISO 7565

UDC 778.148 : 535.241.42 : 002

Ref. No. ISO 782-1975 (E)

Descriptors : film readers, microcopies, screens (displays), luminance, measurement.

Price based on 4 pages

FOREWORD

ISO (the International Organization for Standardization) is a worldwide federation of national standards institutes (ISO Member Bodies). The work of developing International Standards is carried out through ISO Technical Committees. Every Member Body interested in a subject for which a Technical Committee has been set up has the right to be represented on that Committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work.

Draft International Standards adopted by the Technical Committees are circulated to the Member Bodies for approval before their acceptance as International Standards by the ISO Council.

Prior to 1972, the results of the work of the Technical Committees were published as ISO Recommendations; these documents are now in the process of being transformed into International Standards. As part of this process, Technical Committee ISO/TC 46 has reviewed ISO Recommendation R 782 and found it technically suitable for transformation. International Standard ISO 782 therefore replaces ISO Recommendation R 782-1968 to which it is technically identical.

ISO Recommendation R 782 was approved by the Member Bodies of the following countries :

Belgium	Greece	Poland
Brazil	Hungary	Portugal
Canada	India	Romania
Chile	Ireland	Sweden
Czechoslovakia	Israel	Switzerland
Denmark	Italy	Spain
Egypt, Arab Rep. of	Japan	United Kingdom
France	Netherlands	U.S.A.
Germany	Norway	

No Member Body expressed disapproval of the Recommendation.

No Member Body disapproved the transformation of ISO/R 782 into an International Standard.

Microcopying — Measurement of screen luminance of microfilm readers

0 INTRODUCTION

The screen luminance of a microfilm reader is an essential factor of eye comfort. However, while certain essential requirements of the human eye as regards luminance can be defined physiologically, it is more difficult to characterize a microcopy reader screen simply by one or more luminance values corresponding to these physiological requirements.

The experts hesitated in particular between two very different methods of measurement of screen luminance. A first method could consist in taking luminance measurements perpendicular to the screen and over its entire surface; a second method could consist in fixing the measuring instrument opposite the centre of the screen and taking the luminance measurements by swivelling the instrument.

In practice, and especially with translucent screens, the results obtained with each of these two methods are fundamentally different. Moreover, the first one is not always practicable, owing to the geometrical layout of the apparatus.

To approximate as closely as possible to the actual conditions of use of the readers, it seemed necessary to combine the two methods by splitting the surface of the screen into separate areas and examining each area according to precisely stated rules.

The width of 21 cm given to these areas was not fixed at random. Physiologically it represents, margins included, the expanse which can normally be scanned by the eye of an observer glancing at a written text.¹⁾

The distance of 33 cm between screen and measuring instrument corresponds to the normal reading distance for a text of the width specified above.

Finally, it was not deemed essential to reproduce the exact conditions of binocular reading because the method adopted covers slanting measurements. While involving a far smaller complication, this feature permits indirect analysis of the differences in luminous perception which may be experienced by the two eyes when observing a single point from different angles.

The proposed method of measurement cannot alone solve the problem of adapting the luminance of microcopy reader screens to the physiological requirements of the human eye. At a later stage, minimal luminance values will have to be determined, as well as the maximal values of the luminance logarithmic differences (see 4.2.1) on one and the same screen.

The results obtained with both opaque and translucent screens are comparable within each category but to a lesser degree from one category to the other.

However, the method will allow comparison of the performance of various readers available on the market and should lead to improved equipment.

1 SCOPE

This International Standard specifies a method of measurement associating with various points of a microcopy reader screen

- a) data representing luminance values and expressing the impression of luminance produced on an observer facing the screen;
- b) data representing luminance logarithmic differences and expressing the impression of luminance uniformity produced on an observer facing the screen.

2 FIELD OF APPLICATION

2.1 This International Standard applies to microfilm reading apparatus having translucent or built-in opaque screens. It does not apply to apparatus using virtual (aerial) images, nor to apparatus in which the conditions of 3.4 and 3.5 cannot be followed. Moreover, this International Standard does not apply to apparatus for reading microcards.

2.2 If the screen is not built into the apparatus, the measurements specified in this International Standard shall be made only on a screen the characteristics and position of which conform to normal conditions of use, as specified by the manufacturer.

1) See ISO 216, *Writing paper and certain classes of printed matter — Trimmed sizes — A and B series*, which standardizes a width of 210 mm for writing paper and some types of printed matter.

2.3 In particular, apparatus known as *office apparatus*, in which the image is formed on a sheet of white paper laid on a table, may be either classed with built-in opaque-screen readers or assessed by measuring the intensity of illumination they can provide, under conditions which have to be agreed by the interested parties. If the method of likening the apparatus to a built-in opaque-screen reader is used, it is the manufacturer's responsibility to supply, in support of performance claims for his apparatus, the sheets of paper which enable them to be verified.

3 METHOD OF MEASUREMENT

3.1 Measuring instrument

Whether the screen be opaque or translucent, the measurements shall be made with a luminance-meter. The angle of acceptance β of the luminance-meter is the angle between the two straight lines EF and EG, E being the point on the screen located in the luminance-meter axis, F and G two points of the luminance-meter aperture (see figure 1).

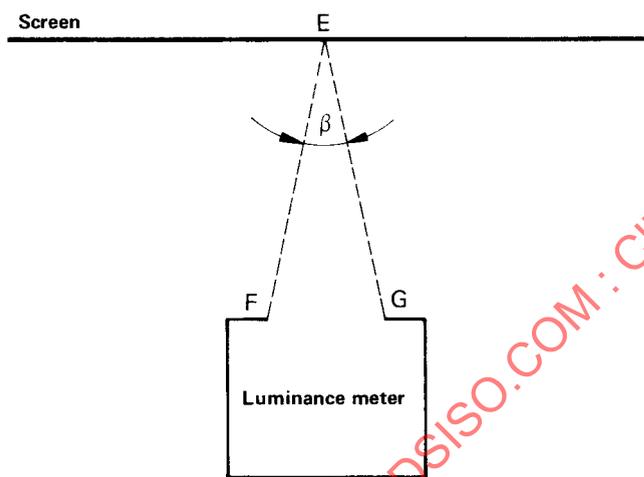


FIGURE 1 — Diagram showing the definition of the angle of acceptance

3.1.1 The angle of acceptance of the luminance-meter should preferably be $2^{\circ} 45'$. If the luminance-meter used has a greater acceptance angle, up to $6^{\circ} 45'$ at most, a possible deviation of 5% from the measurements made shall be allowed for.

3.1.2 The luminance-meter shall be graduated and calibrated in order that the measurements can be expressed in candelas per square metre, or nits. ¹⁾

3.2 Surroundings

The measurements shall be made in complete darkness.

3.3 Screen division into squares

3.3.1 For luminance measurement purposes, the screen shall consist of five areas (see figure 2) as follows:

- a) a central square with 21 cm sides, having a centre O, and four points O₂, O₃, O₄, O₅ marked on the diagonals near the corners at 2,5 cm from each pair of adjacent edges;
- b) four squares with 21 cm sides, having their centres A, B, C, D so arranged that one of the corners of each square is at the meeting point of one of the diagonals of the rectangle circumscribed on the screen (which may have rounded or cut-off corners) with the actual edge of the screen. In each square a point shall be marked at 2,5 cm from two adjacent sides, near the corner located on the screen outline. These four points are designated A₂, B₃, C₄, D₅ by analogy with the positions of the four corresponding points of the central square.

3.3.2 In the case of a very large screen specially intended to be examined at a greater distance (wall projection for instance), a square larger than 21 cm can be accepted while taking into account 3.4.2.

3.3.2.1 Other 21 cm squares may be added in the areas inadequately covered by the above-mentioned squares.

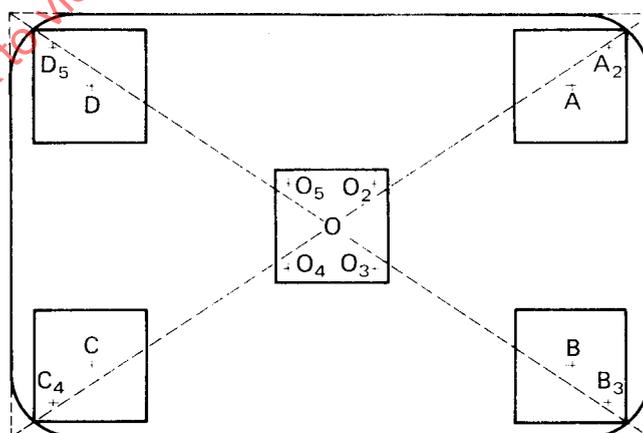


FIGURE 2 — Points on the screen at which the luminance is measured

3.4 Position of luminance-meter during measurements

3.4.1 The luminance-meter shall be placed 33 cm from the screen, on the perpendicular to the screen at the centre of each square successively.

3.4.2 If the screen is very large, a distance from the luminance-meter greater than 33 cm can be agreed upon, taking into account 3.3.2 and preserving unchanged the proportionality ratio between, on the one hand, the

1) The candela per square metre is the SI unit of luminance. A nit-meter is a luminance-meter calibrated directly in candelas per square metre, or nits.

distance of the luminance-meter from the screen and, on the other hand, the sides of the squares and the distances of points such as O_2 and A_2 from the neighbouring sides.

3.5 Points where the luminance is to be measured on the screen

The luminance of the following points or areas of the screen shall be successively measured (see figure 2):

- a) the centre O of the central square, the measurement being made perpendicular to the screen;
- b) the four corners of the central square (see 3.3.1); for this measurement, the luminance-meter, swivelling around the same point of the perpendicular to the screen at point O , is directed towards the points O_2, O_3, O_4, O_5 of the central square;
- c) the four corners of the screen, the luminance-meter being directed, perpendicular to the screen, successively towards the four centres A, B, C, D of the squares (see 3.3.1);
- d) the four ends of the screen diagonals. For the first of these measurements the luminance-meter, swivelling around a point of the perpendicular to the screen at the centre A of the first square (see 3.3.1), is directed towards the point A_2 of the same square. The same measurement is made again, by setting the luminance-meter successively opposite the three other centres B, C, D , perpendicular to the screen and directing it respectively towards the points B_3, C_4, D_5 .

4 EXPRESSION OF RESULTS

4.1 The luminance measured as indicated in 3.5 shall be expressed in candelas per square metre, or nits, and denoted by the symbol of the corresponding point O, A_2 , etc.

4.1.1 The common logarithms of the luminance values shall be calculated and denoted by the symbol of the corresponding point in parentheses $(O), (A_2)$, etc.

4.2 The logarithmic differences of the luminance values of pairs of points shall be calculated as follows :

- a) Express these logarithmic differences for the following pairs of points of the central square:

- $(O) - (O_2)$
- $(O) - (O_3)$
- $(O) - (O_4)$
- $(O) - (O_5)$

- b) Express similarly these logarithmic differences for the pairs of points of the other squares:

- $(A) - (A_2)$
- $(B) - (B_3)$
- $(C) - (C_4)$
- $(D) - (D_5)$

- c) Express also the logarithmic differences between the perpendicular measurements for the following pairs of points:

- $(O) - (A)$
- $(O) - (B)$
- $(O) - (C)$
- $(O) - (D)$

4.2.1 It will be observed that, by adding the differences such as

$$[(O) - (A)] + [(A) - (A_2)]$$

and the three other analogous expressions from 4.2, four values of some importance are obtained:

- $(O) - (A_2)$
- $(O) - (B_3)$
- $(O) - (C_4)$
- $(O) - (D_5)$

4.3 The luminance properties of the screen are thus characterized by

- a) the luminance, in candelas per square metre, or nits, of the centre O of the central square (see 4.1);

- b) the four logarithmic differences referred to in 4.2 a), and the four logarithmic differences referred to in 4.2 b), substantially corresponding to the differences in physiological sensation of the eye looking, while the head remains motionless, at the centre and at a corner of one of the squares defined in 3.3.1;

- c) the four logarithmic differences referred to in 4.2 c), which correspond to the differences in physiological sensation of the eye looking perpendicularly first at the centre of the screen and then at one of the outside points A_2, B_3, C_4, D_5 , obliquely from the positions A, B, C, D .

- d) the four logarithmic differences referred to in 4.2.1 which correspond to the differences in physiological sensation of the eye looking first perpendicularly at the centre of the screen and then at one of the outside corners A_2, B_3, C_4, D_5 , obliquely from the positions A, B, C, D .

5 TEST REPORT

The test report shall include the following particulars:

- a) the type of apparatus tested, opaque or translucent screen; if the former, state whether the screen forms an integral part of the apparatus;

- b) the scale of magnification of the apparatus tested;
- c) the distribution on the screen of 21 cm squares with centres A, B, C, D and of the other points where the measurements were taken, with a dimensioned sketch and guiding letters and subscripts conforming to the indications of figure 2;
- d) the luminance in the centre of the screen (see 4.1); the three series of four logarithmic differences (see 4.2);
- e) all necessary remarks on the measurement conditions or on certain features of the apparatus.

STANDARDSISO.COM : Click to view the full PDF of ISO 782:1975