
**Non-destructive testing — Ultrasonic
testing — Specification for calibration
block No. 2**

*Essais non destructifs — Contrôle par ultrasons — Spécifications
relatives au bloc d'étalonnage n° 2*

STANDARDSISO.COM : Click to view the full PDF of ISO 7963:2022



STANDARDSISO.COM : Click to view the full PDF of ISO 7963:2022



COPYRIGHT PROTECTED DOCUMENT

© ISO 2022

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Manufacture.....	1
4.1 Steel.....	1
4.2 Dimensions.....	1
4.3 Machining, heat treatment and surface finish.....	2
4.4 Reference marks.....	3
5 Methods of use.....	4
5.1 Setting of the time base.....	4
5.1.1 General.....	4
5.1.2 Setting of the time base up to 125 mm steel with a straight-beam probe.....	4
5.1.3 Setting of the time base for 100 mm or 125 mm steel with a miniature angle-beam probe.....	4
5.2 Sensitivity setting and probe checking.....	5
5.2.1 General.....	5
5.2.2 Sensitivity setting with a straight-beam probe.....	5
5.2.3 Miniature angle-beam probes.....	6
6 Declaration of conformity.....	7
Bibliography.....	9

STANDARDSISO.COM : Click to view the full PDF of ISO 7963:2022

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 135, *Non-destructive testing*, Subcommittee SC 3, *Ultrasonic testing* in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 138, *Non-destructive testing*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This third edition cancels and replaces the second edition (ISO 7963:2006), which has been technically revised.

The main changes are as follows:

- document structure aligned with ISO 2400;
- normative references updated;
- wording updated;
- Annex A deleted and the relevant information shifted to the main text;
- [Figures 1, 3 and 6](#) corrected;
- tempering aligned with ISO 2400.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

Calibration block No. 2 is made of steel and may be used for all ultrasonic testing, as calibration block No. 1 described in ISO 2400.

Calibration block No. 2 differs in size and shape from calibration block No.1 but is made from the same material.

Calibration block No. 2 is much smaller and lighter, and its geometry is much simpler than block No 1.

Calibration block No. 2 does not offer as much scope as the larger block No.1; in particular it is not meant to check an ultrasonic instrument completely.

However, calibration block No. 2 makes it possible, during practical testing, to check simply, from time to time, the setting of the time base and the sensitivity of the ultrasonic instrument. Moreover, it is suited to check the beam angle and the probe index point of miniature angle-beam probes.

The International Institute of Welding (IIW) and its members developed the designs of steel calibration blocks in the 1950s and 1960s which were originally indicated as “IIW calibration block 1” and “IIW calibration block 2”. These designs have been adopted widely and they form the basis of many blocks currently available.

The smaller type block is sometimes indicated as “Rompas block” or “miniature angle-beam block (MAB)”, respectively named after the original Dutch designer or the intended use.

Some commercially available blocks look similar to calibration block No. 2, however such blocks are not necessarily according to this document and can have different features, dimensions or materials.

The details of calibration block No. 2, as specified in this document, have been adapted over time.

STANDARDSISO.COM : Click to view the full PDF of ISO 7963:2022

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 7963:2022

Non-destructive testing — Ultrasonic testing — Specification for calibration block No. 2

1 Scope

This document specifies the requirements for the dimensions, material, manufacture and methods of use for calibration block No. 2 for setting and checking ultrasonic test equipment.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 2400, *Non-destructive testing — Ultrasonic testing — Specification for calibration block No. 1*

ISO 5577, *Non-destructive testing — Ultrasonic testing — Vocabulary*

EN 10025-2, *Hot rolled products of structural steels — Part 2: Technical delivery conditions for non-alloy structural steels*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 5577 apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

4 Manufacture

4.1 Steel


Blocks shall be manufactured from steel grade S355J0, specified in EN 10025-2, or from steel of an equivalent grade.

4.2 Dimensions

The dimensions of calibration block No. 2 shall be as shown in [Figure 1](#).

The thickness of the block may be greater than 12,5 mm, for example 20 mm or 25 mm, when using non-miniature probes.

Dimensions in millimetres
Surface roughness in micrometres

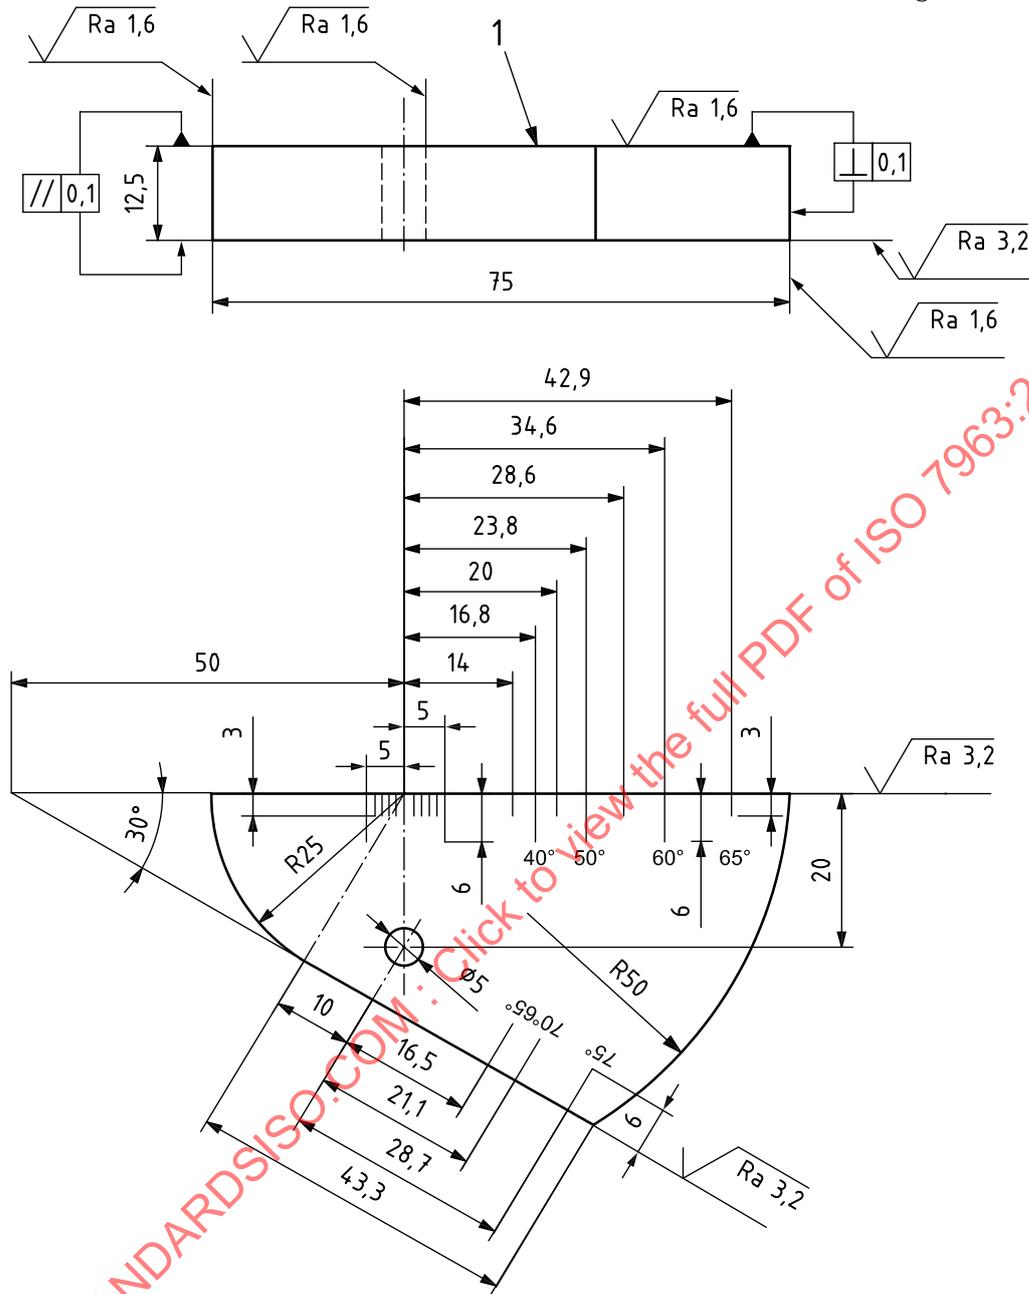

Key

1 reflecting surface

Tolerances, unless otherwise stated: $\pm 0,10$ mm

Height of characters for angle indents: 3 mm

Tolerances on the length of the engraved scale: $\pm 0,5$ mm

NOTE Surface roughness values, *Ra*, are according to ISO 21920-2. Different values for the surface roughness are given because of different functions of the surfaces, e.g. test surface or reflecting surface.

Figure 1 — Calibration block No. 2 — Dimensions of block and scales

4.3 Machining, heat treatment and surface finish

A proof for homogeneity of the material and the determination of the sound velocities in perpendicular directions is only possible on a rectangular block.

Additionally, to determine the sound velocities with the required precision, a thickness larger than 12,5 mm of calibration block No. 2 is needed.

Therefore, it is recommended to manufacture a large rectangular block as for calibration block No. 1 according to ISO 2400 as a semi-finished block.

- a) The block shall be rough-machined to a dimension of 320 mm × 120 mm × 30 mm before heat treatment which shall consist of:
 - 1) austenitizing at 920 °C for 30 min;
 - 2) rapid cooling (quenching) in water;
 - 3) tempering by heating to 650 °C for 3 h;
 - 4) cooling in still air.
- b) At least 2 mm shall be removed from all surfaces after heat treatment.
- c) Prior to final machining, the semi-finished block shall be proven to be free from internal discontinuities.
 - 1) For this purpose, an ultrasonic test shall be carried out after the heat treatment, with a longitudinal wave probe of at least 10 MHz nominal centre frequency and having a transducer size of 10 mm to 15 mm. The block shall be checked on the basis of all four long faces to cover the complete volume.
 - 2) With the probe positioned on the largest face of the block, the instrument gain shall be set to achieve a grain scatter noise of 10 % of the full screen height.
 - 3) No echo from internal imperfections shall have an amplitude greater than that of the grain scatter noise.
- d) Prior to final machining, the velocities of longitudinal and transverse waves shall be determined as specified in ISO 2400.
 - 1) The velocities shall be determined within a maximum permissible error of ±0,2 %, i.e. with an uncertainty of ±6 m/s for transverse waves and ±12 m/s for longitudinal waves.
 - 2) The determined longitudinal wave velocity, v_l , shall be (5 920 ± 30) m/s and the transverse wave velocity, v_t , shall be (3 255 ± 15) m/s.
- e) Then cut this large block into smaller parts to continue with the manufacturing of calibration blocks No. 2.
- f) All external surfaces shall be machined to a R_a value according to [Figure 1](#).
- g) In order to prevent parasitic effects, the depth of the marks of the engraved scale, text and numbers shall be (0,1 ± 0,05) mm.
- h) The length of the marks shall be 6 mm or 3 mm, and the tolerance on the positioning of the marks shall be ±0,2 mm.

4.4 Reference marks

- a) Reference marks as shown in [Figure 1](#) shall be permanent.
- b) Additionally, the block shall be permanently marked with:
 - 1) the manufacturer's name or logo;
 - 2) the reference to this document (i.e. ISO 7963); and

- 3) a unique serial number.

5 Methods of use

5.1 Setting of the time base

5.1.1 General

To set the time base, the leading edge (left side) of successive echoes shall be adjusted to coincide with the appropriate scale markings on the screen of the ultrasonic instrument.


The time of flight of the pulses depends on the velocity of ultrasonic waves in the tested material.

5.1.2 Setting of the time base up to 125 mm steel with a straight-beam probe


The position of the probe on the test surface of the calibration block shall be as indicated in [Figure 2 a\)](#). [Figure 2 b\)](#) is a schematic representation of the screen (A-scan) of the instrument for setting a range of 50 mm steel.

NOTE Depending on the probe and the frequency used, difficulties can arise when setting distances greater than 10 times the thickness of the block.

Dimensions in millimetres

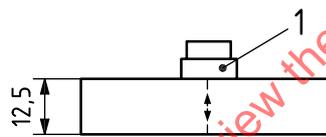

a) Position of a straight-beam probe on calibration block No. 2



b) Schematic representation of the A-scan for setting of a range of 50 mm

Key

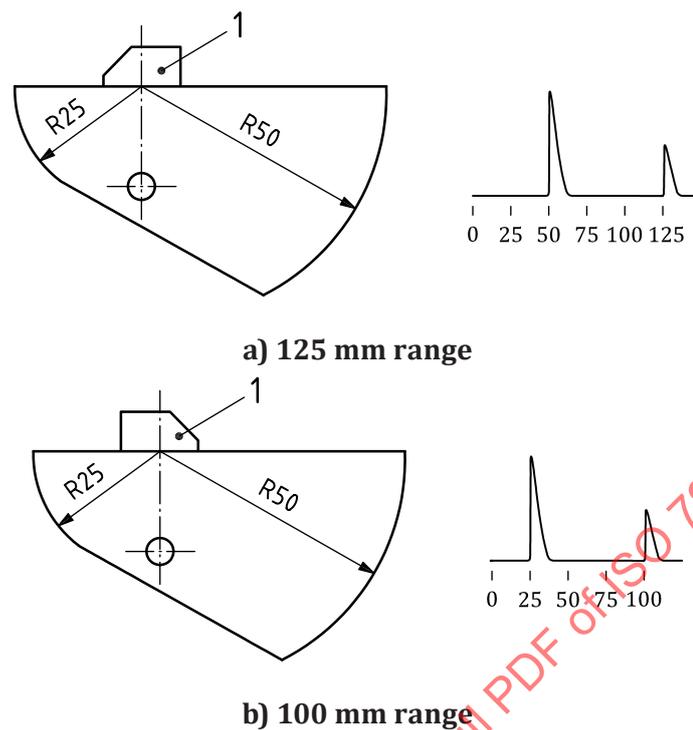
- 1 straight-beam probe

Figure 2 — Setting of the time base for straight-beam probes

5.1.3 Setting of the time base for 100 mm or 125 mm steel with a miniature angle-beam probe

The position of the miniature angle-beam probe on the calibration block shall be as shown in [Figure 3 a\)](#) for a distance of 125 mm and in [Figure 3 b\)](#) for a distance of 100 mm. The screen of the instrument for the setting of these two ranges is shown schematically in [Figures 3 a\)](#) and [3 b\)](#).

Dimensions in millimetres

**Key**

1 angle-beam probe

Figure 3 — Setting of time base for miniature angle-beam probes**5.2 Sensitivity setting and probe checking****5.2.1 General**

When checking probes, the acoustic coupling is an important factor, and when comparing probes, the same coupling medium shall be used.

A large number of factors can influence the sensitivity setting.


The following factors, divided into four main groups, shall be taken into account when setting the sensitivity:

- instrument used, e.g. pulse energy, frequency, pulse shape, gain;
- probe used, e.g. type, size, acoustic impedance, transducer damping, beam shape;
- material to be tested, e.g. surface condition (in connection with coupling), kind of material (its attenuation);
- discontinuities to be detected, e.g. shape, orientation, nature.

5.2.2 Sensitivity setting with a straight-beam probe

The A-scan representing the successive echoes shall be used as a reference for setting sensitivity.

- The probe shall be placed in position "a" as indicated in [Figure 4](#).
- The echo from the 5 mm diameter hole, position "b" in [Figure 4](#) may also be used, with the probe being placed so that the corresponding echo amplitude is at its maximum.

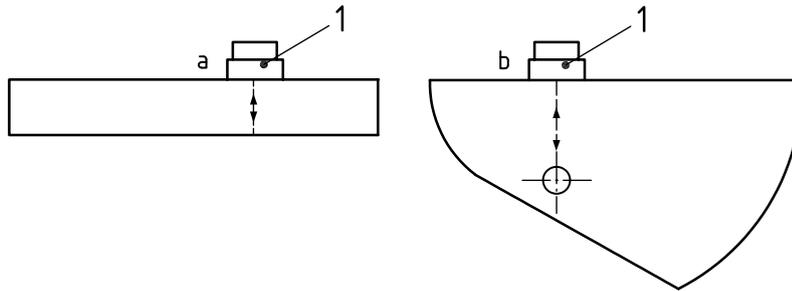

Key


- 1 straight-beam probe
- a probe position using the back wall
- b probe position using the 5 mm diameter hole

Figure 4 — Sensitivity setting for straight-beam probes

5.2.3 Miniature angle-beam probes

5.2.3.1 Sensitivity setting

- a) The maximum echo from the 5 mm diameter hole shall be used as a reference for sensitivity setting (see [Figure 5](#), position "a").

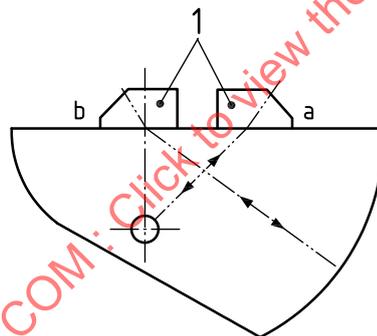

Key

- 1 miniature angle-beam probe
- a, b probe positions

Figure 5 — Sensitivity setting for miniature angle-beam probes

- b) Alternatively, it is possible to make use of the reflections from the cylindrical surfaces of radii 50 mm and 25 mm, respectively.

In this case, there are two possibilities:

- by using a calibrated gain control, the amplitude of the echo from the cylindrical surface is initially set to 80 % of the full screen height and subsequently adjusted to the level desired (see [Figure 5](#), position "b");
- without the use of the calibrated gain control, the successive echoes from the cylindrical surfaces are used for the setting of sensitivity (see [Figure 6](#)).