
**Dentistry — Test methods for rotary
instruments**

Art dentaire — Méthodes d'essai pour instruments rotatifs

STANDARDSISO.COM : Click to view the full PDF of ISO 8325:2004



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 8325:2004

© ISO 2004

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope.....	1
2 Normative references	1
3 Terms and definitions	1
4 Test methods	1
4.1 General	1
4.2 Atmospheric conditions	2
4.3 Measurement instruments	2
5 Measuring of single characteristics of instruments	2
5.1 Shape of the working part	2
5.2 Diameter of the working part	3
5.3 Neck diameter	3
5.4 Dimensions of the shank and the mandrel	4
5.5 Length of the working part	4
5.6 Overall length	4
5.7 Angle of the taper of the working part	5
5.8 Run-out of the working part	5
5.9 Neck strength	7
5.10 Surface roughness	8
Bibliography	9

STANDARDSISO.COM : Click to view the full PDF of ISO 8325:2004

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 8325 was prepared by Technical Committee ISO/TC 106, *Dentistry*, Subcommittee SC 4, *Dental instruments*.

This second edition cancels and replaces the first edition (ISO 8325:1985), which has been technically revised.

STANDARDSISO.COM : Click to view the full PDF of ISO 8325:2004

Introduction

To check the conformity of dental rotary instruments against relevant product standards, it is indispensable to conduct tests on the basis of harmonised test methods in order to achieve comparable test results. In the respective product standards for dental rotary instruments, reference is made to the test methods specified in this International Standard.

STANDARDSISO.COM : Click to view the full PDF of ISO 8325:2004

Dentistry — Test methods for rotary instruments

1 Scope

This International Standard specifies methods for measuring the dimensional characteristics, neck strength and surface roughness of dental rotary instruments, such as burs, cutters, polishers, diamond and abrasive instruments.

This International Standard does not provide test methods for the characteristics of materials used for dental rotary instruments.

NOTE For testing of these characteristics, see the respective product standards.

This International Standard is not applicable to dental root-canal instruments (see ISO 3630-1).

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1797-1, *Dental rotary instruments — Shanks — Part 1: Shanks made of metals*

ISO 1797-2, *Dental rotary instruments — Shanks — Part 2: Shanks made of plastics*

ISO 1942, *Dentistry — Vocabulary*

ISO 3274, *Geometrical Product Specification (GPS) — Surface texture: Profile method — Nominal characteristics of contact (stylus) instruments*

ISO 4288, *Geometrical Product Specification (GPS) — Surface texture: Profile method — Rules and procedures for the assessment of surface texture*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942 apply.

4 Test methods

4.1 General

The test methods specified in this International Standard refer to the main dimensional characteristics of dental rotary instruments. They are demonstrated by describing the measurement procedures for the single characteristics of instruments.

In addition to the test methods specified below, other equivalent methods and test devices exist and may be used, provided they render similar results. In case of dispute, however, the test methods specified in this International Standard become reference.

For evaluation of test results, see the relevant product standard.

4.2 Atmospheric conditions

Tests shall be conducted at room temperature (20 °C to 25 °C).

4.3 Measurement instruments

A list of measurement instruments is provided as follows:

- a) micrometer;
- b) vernier calliper;
- c) dial gauge;
- d) comparator;
- e) toolmaker's microscope, workshop microscope, measuring microscope;
- f) shadowgraph (e.g. profile projector);
- g) ring gauge;
- h) pneumatic gauge;
- i) goniometer;
- j) laser scanner.

Other precision instruments may equally be applicable, and may be used at the discretion of the manufacturer. Measurement instruments with reasonable accuracy shall be chosen in respect to the characteristics of the instruments to be measured.

Lengths and diameters shall be measured and calculated in millimetres, angles in degrees.

5 Measuring of single characteristics of instruments

5.1 Shape of the working part

5.1.1 Measurement instrument

Any suitable instrument of those listed in 4.3 shall be used, having an accuracy of $\leq 0,01$ mm.

The applied measuring force shall not exceed 1,5 N.

5.1.2 Measurement location

The measurement location shall cover the whole representative integral shape of the test piece.

5.1.3 Procedure

Determine the shape of the working part visually or by using an instrument specified in 5.1.1.

Conduct one measurement.

5.2 Diameter of the working part

5.2.1 Measurement instrument

Any suitable instrument of those listed in 4.3 shall be used, having an accuracy of $\leq 0,01$ mm.

The applied measuring force shall not exceed 1,5 N.

In case of dispute, the reference method shall be that using a dial gauge.

5.2.2 Measurement location

The measurement point shall be as follows, unless specified otherwise in the respective product standard:

- a) for cylindrical instruments: the middle of the working part;
- b) for non-cylindrical instruments: the largest diameter of the working part.

5.2.3 Procedure

Measure the diameter of the working part using an instrument as specified in 5.2.1.

Conduct one measurement on the peripheral surface, i.e. on the top surface.

For diamond instruments, conduct three measurements at angles 120° apart on the circumference of the test piece. Lift the blade before rotating the test piece to the next measurement point. Record the three measuring results as d_1 , d_2 and d_3 .

5.2.4 Evaluation of test results for diamond instruments

For diamond instruments, calculate the average diameter by using the following formula:

$$d = \frac{d_1 + d_2 + d_3}{3} \quad (1)$$

where

d_1 is the diameter given by measurement 1;

d_2 is the diameter given by measurement 2;

d_3 is the diameter given by measurement 3.

5.3 Neck diameter

5.3.1 Measurement instrument

Any suitable instrument of those listed in 4.3 shall be used, having an accuracy of 0,01 mm.

If mechanical instruments are used, they shall be equipped with knife-edged tungsten carbide blades of $\leq 0,3$ mm thickness.

The applied measurement force shall not exceed 1,5 N.

5.3.2 Measurement location

The measurement point shall be the smallest diameter just behind the working part, or just behind the collar, where applicable.

5.3.3 Procedure

Measure the neck diameter using an instrument as specified in 5.3.1.

Conduct one measurement.

5.4 Dimensions of the shank and the mandrel

The dimensions of the shank and the mandrel shall be determined in accordance with ISO 1797-1 and ISO 1797-2.

ISO 13295 should also be consulted.

The applied measuring force shall not exceed 1,5 N.

5.5 Length of the working part

5.5.1 Measurement instrument

Any suitable instrument of those listed in 4.3 shall be used, having an accuracy of $\leq 0,01$ mm.

The applied measurement force shall not exceed 1,5 N.

5.5.2 Measurement location

The measurement points shall be the points at the ends of the shortest length of the working part, including, where applicable, the coated neck.

5.5.3 Procedure

Measure the length of the working part using an instrument as specified in 5.5.1.

Conduct one measurement.

5.6 Overall length

5.6.1 Measurement instrument

Any suitable instrument of those listed in 4.3 shall be used, having an accuracy of $\leq 0,01$ mm.

The applied measurement force shall not exceed 1,5 N.

5.6.2 Measurement location

The points for measurement shall be the two ends of the instrument, including tip and shank end.

5.6.3 Procedure

Measure the overall length using an instrument as specified in 5.6.1.

Conduct one measurement.

5.7 Angle of the taper of the working part

5.7.1 Measurement instrument

Any suitable instrument of those listed in 4.3 shall be used, having an accuracy of $\leq 2'$ [equivalent to $(1/30)^\circ$].

The applied measurement force shall not exceed 1,5 N.

5.7.2 Measurement location

The measurement shall be made on the enveloped area of the working part for applying test facilities.

The points of measurement shall be at least two representative points on the surface of the working part of the test piece which are as far apart from each other as possible.

5.7.3 Procedure

Determine the included angle with reference to the baseline (axis) of the test facilities with an instrument as specified in 5.7.1.

Measure the relevant diameters and the length of the taper and, if necessary, calculate the angle of the taper.

Conduct one measurement.

5.8 Run-out of the working part

5.8.1 Holding device and measuring instrument

5.8.1.1 Holding device

The holding device for measuring run-out shall be one of the following:

- a) split V-block with adjustable distances l_1 and l_2 (see Figure 1) for instruments with shanks in accordance with ISO 1797-1;
- b) equivalent device, for example a precision chuck, for instruments with shanks in accordance with ISO 1797-2;
- c) equivalent device for mandrels.

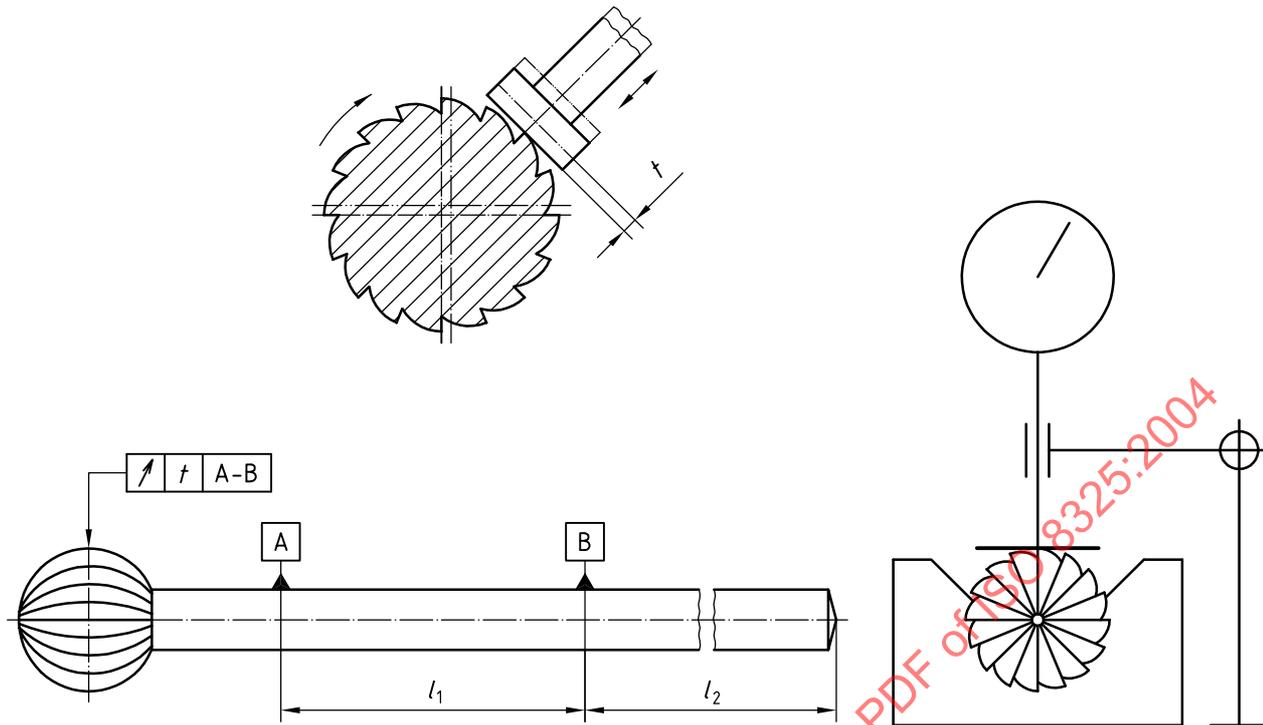


Figure 1 — V-block measuring device

Lengths l_1 and l_2 , which depend on the type of shank and the fitting length of the test piece, shall be in accordance with Table 1.

Table 1 — Dimensions l_1 and l_2

Dimensions in millimetres

Shank type ISO 1797 ^a	Fitting length ISO 1797 ^a	l_1	l_2
1	9	5	3
1	11 and 12	7	3
2	15	10	3
2	30	9	20
3	9	5	2
3	11 and 12	7	2
4	15	10	3
4	30	9	20

^a ISO 1797-1 or ISO 1797-2, as appropriate.

5.8.1.2 Measuring instrument

Any suitable instrument of those listed in 4.3 shall be used, having an accuracy of $\leq 0,01$ mm.

The applied measuring force shall not exceed 0,3 N.