
**Preparation of steel substrates before
application of paints and related
products — Tests for the assessment
of surface cleanliness —**

**Part 6:
Extraction of water soluble
contaminants for analysis (Bresle
method)**

*Préparation des subjectiles d'acier avant application de peintures
et de produits assimilés — Essais pour apprécier la propreté d'une
surface —*

*Partie 6: Extraction des contaminants solubles en vue de l'analyse
(Méthode de Bresle)*



STANDARDSISO.COM : Click to view the full PDF of ISO 8502-6:2020



COPYRIGHT PROTECTED DOCUMENT

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Principle.....	2
5 Apparatus and materials.....	2
6 Procedure.....	3
6.1 Selection of test surface.....	3
6.2 Blank test.....	3
6.3 Extraction by patch or sleeve by injection.....	3
6.4 Extraction by sleeve by pre-filling.....	5
7 Analyses.....	5
8 Test report.....	5
Annex A (normative) Leak test for type testing of adhesive cells (patches and sleeves).....	9
Bibliography.....	11

STANDARDSISO.COM : Click to view the full PDF of ISO 8502-6:2020

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 35, *Paints and varnishes*, Subcommittee SC 12, *Preparation of steel substrates before application of paints and related products*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 139, *Paints and varnishes*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This third edition cancels and replaces the second edition (ISO 8502-6:2006), which has been technically revised.

The main changes compared to the previous edition are as follows:

- inclusion of the sleeve type extraction cells to be used with water extraction;
- specification that only water is used as a solvent for this method.

A list of all parts in the ISO 8502 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

The performance of protective coatings of paint and related products applied to steel is significantly affected by the state of the steel surface immediately prior to painting. The principal factors that are known to influence this performance are:

- a) the presence of rust and mill scale;
- b) the presence of surface contaminants, including salts, dust, oils and greases;
- c) the surface profile.

The ISO 8501 series, ISO 8502 series and ISO 8503 series have been prepared to provide methods of assessing these factors, while ISO 8504 series provides guidance on the preparation methods that are available for cleaning steel substrates, indicating the capabilities of each in attaining specified levels of cleanliness.

These series of International Standards do not contain recommendations for the protective coating systems to be applied to the steel surface. Neither do they contain recommendations for the surface quality requirements for specific situations, even though surface quality can have a direct influence on the choice of protective coating to be applied and on its performance. Such recommendations are found in other documents such as national standards and codes of practice. Users of these International Standards should ensure that the qualities specified are:

- compatible and appropriate both for the environmental conditions to which the steel will be exposed and for the protective coating system to be used;
- within the capability of the cleaning procedure specified.

The four series of International Standards referred to above deal with the following aspects of preparation of steel substrates:

- ISO 8501 covers the visual assessment of surface cleanliness;
- ISO 8502 covers the tests for the assessment of surface cleanliness;
- ISO 8503 covers the surface roughness characteristics of blast-cleaned steel substrates;
- ISO 8504 covers the surface preparation methods.

This document is one of many parts of ISO 8502 that specify tests for the assessment of surface cleanliness. In relation to such tests, there are several methods for the extraction, for analysis, of soluble contaminants on surfaces to be painted. One of these methods is based on the swabbing of comparatively large test surfaces. This technique provides average values of the contamination present, but it might conceal localized concentrations of contaminants. Also, swabbing might not ensure sufficient penetration to dissolve all the deep-seated contamination such as ferrous salts.

There are other methods, however, which use small cells for the liquid used to remove and collect the surface contaminants. The cells are attached to test surfaces where soluble contaminants could be expected, e.g. where pitting has occurred and prevent loss of extraction solution from evaporate. This closed cell technique usually provides more accurate, point values of the contamination present.

This document describes a simple, inexpensive field test using flexible cells in the form of adhesive cells designed to be filled with water. The method was originally developed by a Swedish scientist, Dr. A. Bresle, using one of the cell types included in this document.

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 8502-6:2020

Preparation of steel substrates before application of paints and related products — Tests for the assessment of surface cleanliness —

Part 6:

Extraction of water soluble contaminants for analysis (Bresle method)

1 Scope

This document specifies a method of extracting, for analysis, water soluble contaminants from a surface by use of flexible cells in the form of adhesive patches or sleeves which can be attached to any surface, regardless of its shape (flat or curved) and its orientation (facing in any direction, including downwards).

The method described is suitable for use in the field to determine the presence of water soluble contaminants before painting or a similar treatment.

This document does not cover the subsequent analysis of the contaminants that have been dissolved. Methods of analysis suitable for field use are described in other parts of ISO 8502.

NOTE The extraction method might give a false negative or not take all the water-soluble material off the surface because of: a) Soluble materials hiding in the crevices or under folds of metal; b) Soluble materials under corrosion layers, passivation layers produced by corrosion inhibitors, oil, grease, or other non-visible thin films.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 554, *Standard atmospheres for conditioning and/or testing — Specifications*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 8501-1, *Preparation of steel substrates before application of paints and related products — Visual assessment of surface cleanliness — Part 1: Rust grades and preparation grades of uncoated steel substrates and of steel substrates after overall removal of previous coatings*

ISO 8502-9, *Preparation of steel substrates before application of paints and related products — Tests for the assessment of surface cleanliness — Part 9: Field method for the conductometric determination of water soluble salts*

ISO 8503-2, *Preparation of steel substrates before application of paints and related products — Surface roughness characteristics of blast-cleaned steel substrates — Part 2: Method for the grading of surface profile of abrasive blast-cleaned steel — Comparator procedure*

3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

4 Principle

This document covers two types of cells: adhesive patch and flexible sleeve.

With the first type, an adhesive patch with a central compartment designed to hold a solvent (in this case water) is attached to the surface from which water-soluble contaminants are to be removed. The water is injected into the compartment by means of a syringe, and then sucked back into the syringe. This operation is repeated, and the water is left to dissolve salts on the surface.

With the second type of cell, a sleeve containing water is attached to the surface and the water is left, under some agitation, to dissolve the salts. The water (now containing contaminants dissolved off the test surface) is then transferred to a suitable vessel for analysis.

5 Apparatus and materials

5.1 Adhesive cell

An adhesive cell has a body which is made of ageing-resistant, flexible material with closed pores, (e.g. polyethylene foam, and with a hole punched in the centre. For the adhesive patch, the punched-out material is kept in the hole as reinforcement until the patch is used. With the adhesive sleeve, there is no punched-out material in the hole. The flexibility of the cell shall be sufficient to attach to rough surfaces and to areas with some angularity. For the flexible sleeve, it is essential that the foam adhesive ring maintains an exposed area of known size, 1 000 mm² for the standard S-1000 sleeve. One side of the cell is coated with a thin elastomer film or an extraction sleeve. The other side is coated with adhesive and covered by a removable protective sheet. The hole and the outer edge of the patch may be any shape, e.g. circular, rectangular, elliptical.

The thickness of the adhesive rim shall be 1,5 mm ± 0,3 mm and the width of the adhesive rim between the hole and the outer edge of the patch shall be at least 5 mm. The thickness of the adhesive rim of adhesive sleeves of size S-1000 (see [Table 1](#)) shall be 3 mm ± 0,3 mm and the width at least 7 mm.

Cells with one of the standard compartment sizes specified in [Table 1](#) are called standard cells.

It is essential that the adhesive cell is leak tight. An easily performed leak test for type testing shall be performed according to [Annex A](#). Twelve cells of the same size shall be tested, and at least eight of them shall pass the test. The leak test shall be carried out by an accredited laboratory and the result stated in a test report. For terms and definitions in this context, see ISO/IEC 17000.

The cell should not cause any noticeable variation in the contamination of the extraction liquid. To confirm accuracy, an initial cell blank test shall be required as described in [6.2](#)

Table 1 — Standard cells

Patch size	Compartment area mm ²
A-0155	155 ± 2
A-0310	310 ± 3
A-0625	625 ± 6
A-1250	1 250 ± 13
A-2500	2 500 ± 25

Table 1 (continued)

Sleeve size	Compartment area mm ²
S-1000	1 000 ± 10

5.2 Reusable syringe

max. cylinder volume:	10 ml
max. needle diameter:	1 mm
max. needle length:	50 mm

5.3 Solvent (water), of at least grade 3 purity in accordance with ISO 3696.

NOTE 1 Usually, distilled or de-ionized water of conductivity less than 0,5 mS/m (5 µS/cm) meets this requirement.

NOTE 2 Only water is used in this method. Other acidic solvents are covered in ISO 8502-15.

5.4 Contact thermometer, accurate to 0,5 °C and graduated at 0,5 °C intervals.

5.5 Container, suitable for the analysis to be performed.

6 Procedure

6.1 Selection of test surface

It is important to select test areas where metal loss or pitting is observed, and on or around metal welds, as these are the areas where salts are most prevalently concentrated. Otherwise, choose test areas which are representative of the entire surface.

In case measurements before surface preparation are to be performed, it is recommended to scrape the surface with a metal spatula or knife until bright metal is exposed over at least 50 % of the test area, or replicates the surface condition specified immediately prior to coating.

6.2 Blank test

To check cleanliness of the cells, blank tests shall be performed in advance for each batch.

For the blank test, a piece of clean glass, to which the adhesive patch will adhere, shall be used and water of the same type as to be used for testing. The same procedure as above, 6.3 or 6.4, shall be followed. In case the background interference is significant, the cause shall be investigated and, if possible, eliminated.

In case the background interference introduced by the adhesive cell is significant, reproducible and cannot be eliminated, a blank test shall be performed in parallel to each test and the background subtracted from the field quantitative measurements in order to report a net surface contamination value. If this procedure is followed, it shall be stated in the report.

NOTE For the blank test, 2 patches can be stacked together.

6.3 Extraction by patch or sleeve by injection

6.3.1 Take an adhesive patch, "Bresle patch", or sleeve (5.1) of a suitable size (see Table 1). Remove the protective paper for the patch remove the punched-out material (see Figure 1).

6.3.2 Press the adhesive side of the patch or sleeve against the test surface (see [Figure 2](#) and [Figure 7](#)) in such a way that the minimum amount of air is trapped in the compartment of the patch.

6.3.3 Fill the syringe ([5.2](#)) with water ([5.3](#)) (see [Figure 3](#)).

NOTE The volume of water needed to fill the patch compartment is proportional to the compartment area, and normally amounts to $2,6 \times 10^{-3} \text{ ml/mm}^2 \pm 0,6 \times 10^{-3} \text{ ml/mm}^2$. The volume of water needed to fill the sleeve compartment is proportional to the compartment area, and normally amounts to $10,0 \times 10^{-3} \text{ ml/mm}^2 \pm 1,0 \times 10^{-3} \text{ ml/mm}^2$ (10 ml for S-1000 sleeve).

6.3.4 Insert the syringe needle at an angle of about 30° to the test surface near the outer edge of the patch or sleeve, so that it passes through the adhesive foam body of the patch or sleeve into the compartment formed between the elastomer film and the test surface (see [Figure 4](#)).

6.3.5 If the patch or sleeve is in a position which makes access to the patch compartment difficult, bend the syringe needle as required. Inject the water, ensuring that it wets the whole of the test surface (see [Figure 4](#)).

If necessary to avoid air remaining trapped in the cell compartment, carry out the injection as follows: Inject half of the water. Evacuate the air through the needle by reverse operation of the syringe. Remove the needle from the patch or sleeve. Holding the syringe with the needle pointing upwards, expel the air. Re-insert the needle into the compartment and inject the remainder of the water.

6.3.6 Agitate the solution in the patch or sleeve. Agitation of the water in the patch can be accomplished by sucking the water back into the syringe (see [Figure 5](#)) and re-injecting it at least four times and/or by massaging to create water movement over the test surface. The solution in the flexible sleeve is to be agitated by massaging the sleeve. After a minimum of 10 min extraction time, suck the water back into the syringe (see [Figure 5](#)).

NOTE On unpitted blast-cleaned surfaces, a period of 10 min has been found sufficient as by then more than 90 % of the soluble salts have usually been dissolved.

6.3.7 Transfer the water to a suitable vessel for analysis (see [Figure 6](#)), as per ISO 8502-9.

6.3.8 During steps [6.3.3](#) to [6.3.6](#), it is essential that no water be lost from the cell or syringe, due for instance to inferior-quality materials or improper handling of the materials. If any water is lost, the solution obtained shall be rejected. Some loss of solution during the final transfer of solution, step [6.3.7](#), is acceptable if the extracted volume is not further diluted. When diluted, no more than 5 % of the volume shall be lost.

6.3.9 On completion of step [6.3.7](#), clean and rinse the syringe so that it can be re-used. A bent needle is best left as it is until it becomes necessary to straighten it or bend it further.

NOTE In most cases, approximately 95 % of the soluble surface contaminants can be dissolved by carrying out steps [6.3.3](#) to [6.3.9](#) only once. By repeating these steps with fresh water, almost all of the remaining 5 % can also be dissolved.

6.3.10 Record the volume of water used, V_{extr} , i.e. the total amount of water injected into the extraction cell or the total volume of water used for the analysis as described in ISO 8502-9.

6.3.11 Record the temperature of the steel surface to the nearest $0,5^\circ\text{C}$ using the contact thermometer ([5.4](#)). The temperature shall be over $+5^\circ\text{C}$ to avoid ice on the surface.

6.4 Extraction by sleeve by pre-filling

6.4.1 Take an adhesive sleeve (5.1) of a suitable size (see Table 1). Remove the protective paper and straighten the sleeve.

6.4.2 Prefill the sleeve with the required volume of water (5.3) and adhere the sleeve to the surface without loss of water, see Figure 7.

NOTE The volume of water needed to fill the sleeve compartment is proportional to the compartment area, and normally amounts to $10,0 \times 10^{-3} \text{ ml/mm}^2 \pm 1,0 \times 10^{-3} \text{ ml/mm}^2$.

6.4.3 Position the sleeve such that all water in the sleeve is in contact with the surface.

6.4.4 After a suitable period of time, to be agreed between the interested parties, however a minimum of 10 minutes, let the sleeve hang down in order for the water to flow into the compartment of the sleeve. During this period of time, agitate the sleeve several times by massaging the water on the surface.

6.4.5 Carefully remove the sleeve from the surface. Maintain the water for further analysis.

6.4.6 During steps 6.4.2 to 6.4.4, it is essential that no water be lost from the sleeve, due for instance to inferior-quality materials or improper handling of the materials. If any water is lost, the solution obtained shall be rejected. Some loss of solution during the final transfer of solution, step 6.4.5 is acceptable as long as the remaining volume is sufficient for the analyses to be performed, however no more than 30 % of the volume added.

6.4.7 Record the volume of water used, V_{extr} , i.e. the total amount of water injected into the extraction cell or the total volume of water used for the analysis as described in ISO 8502-9.

6.4.8 Record the temperature of the steel surface to the nearest 0,5 °C using the contact thermometer (5.4). The temperature shall be over +5 °C to avoid ice on the surface.

NOTE In most cases, approximately 95 % of the soluble surface contaminants can be dissolved by carrying out steps 6.4.1 to 6.4.5 only once. By repeating these steps with fresh water, almost all the remaining 5 % can also be dissolved.

7 Analyses

After sampling the solution is analysed as agreed between the interested parties. Suitable methods are conductometric determination of water-soluble salts according to ISO 8502-9 or other methods of chemical analyses.


NOTE Methods of analyses are not covered by this document.

8 Test report


The test report shall contain at least the following information:

- a) a reference to this document, i.e. ISO 8502-6:2020;
- b) the type and size of extraction cell used: patch or sleeve;
- c) the type of water used as solvent;
- d) the total volume of water used for extraction, V_{extr} ;
- e) the total time of contact between the water and substrate;

- f) the temperature during steps [6.3.1](#) to [6.3.11](#) or [6.4.1](#) to [6.4.8](#) of the procedure;
- g) the manufacturer's batch number of the patch or sleeve used;
- h) the date of the test.

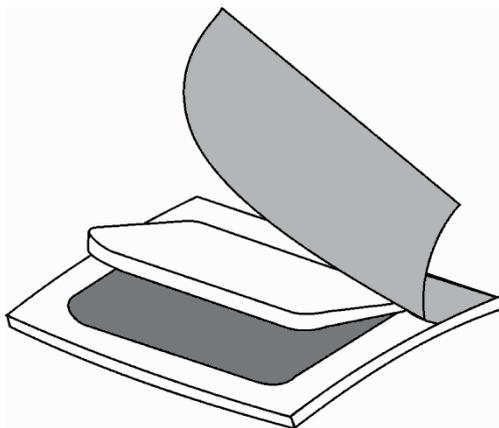

a) Adhesive patch with protective paper and punched-out material

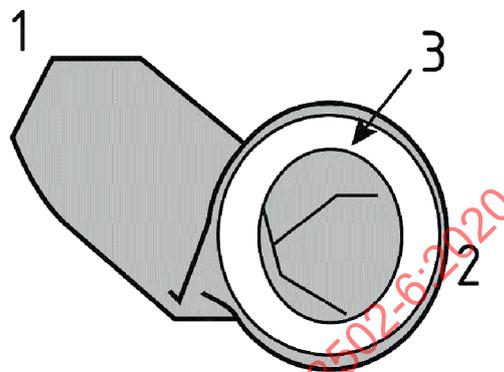

b) Adhesive sleeve

Key

- 1 flexible sleeve-closed end
- 2 flexible sleeve- open end
- 3 adhesive ring with protective paper

Figure 1 — Adhesive patch

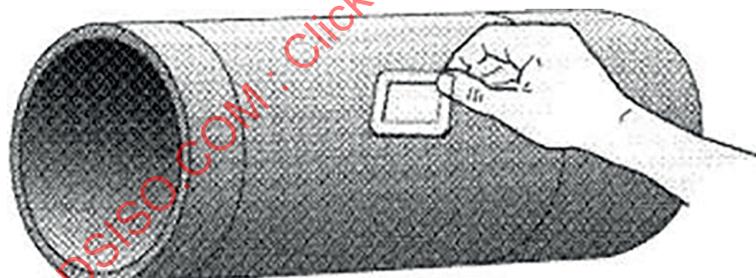


Figure 2 — Adhesive patch being attached to the test surface

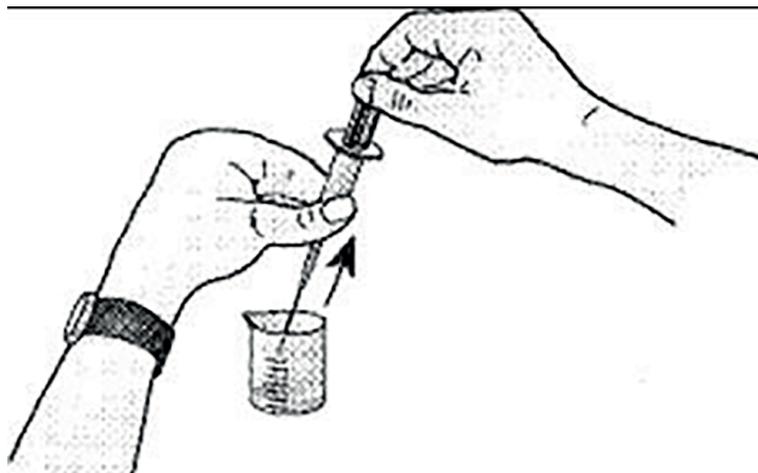


Figure 3 — Syringe being filled with water

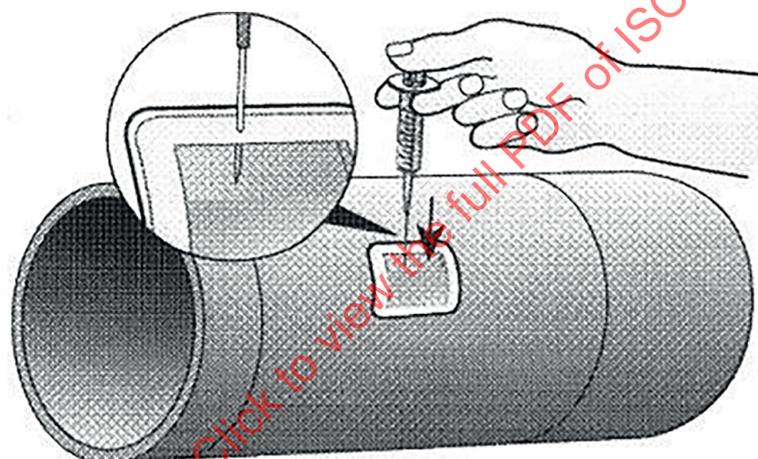


Figure 4 — Water being injected into the compartment in the patch (carefully following the procedure described in [6.3.4](#) and [6.3.5](#))

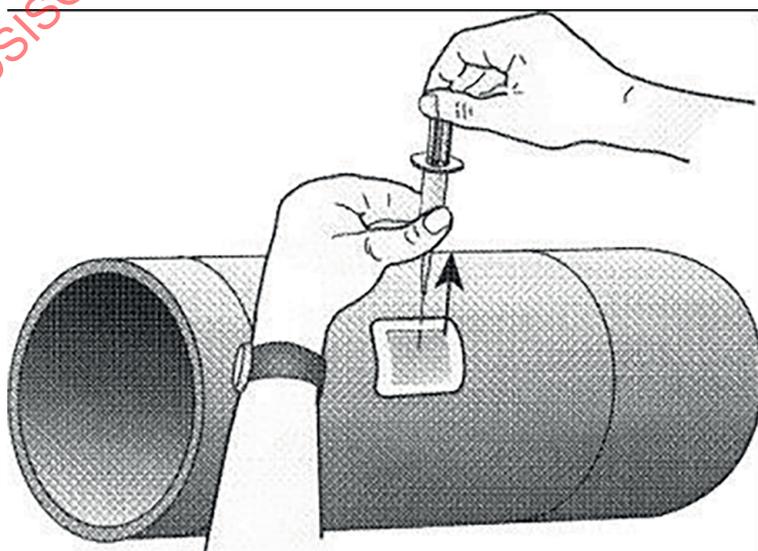


Figure 5 — Water being retrieved from the compartment in the patch

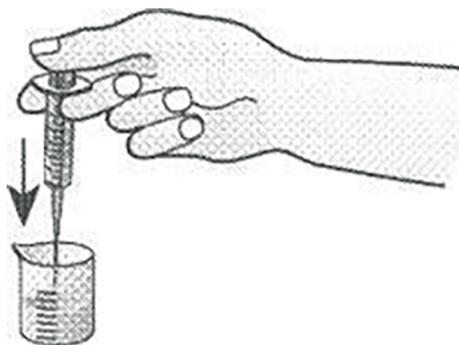


Figure 6 — Water being transferred to a suitable vessel for subsequent analysis

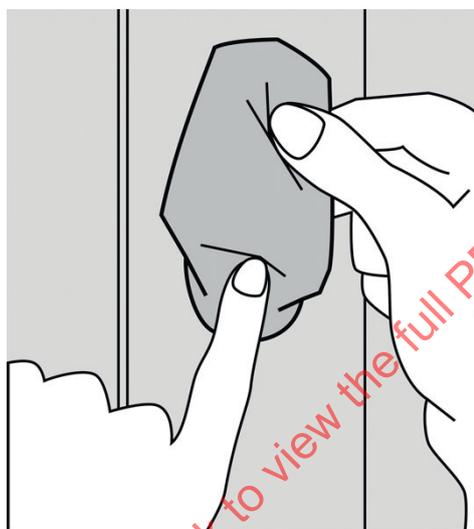


Figure 7 — Flexible sleeve being adhered to a metal surface

STANDARDSISO.COM : Click to view the full PDF of ISO 8502-6:2020