

# INTERNATIONAL STANDARD

**ISO**  
**8536-7**

First edition  
1992-10-01

---

---

## Infusion equipment for medical use —

### Part 7:

Caps made of aluminium-plastics combinations  
for infusion bottles

*Matériel de perfusion à usage médical —*

*Partie 7: Capsules en combinaison aluminium-plastique pour flacons de perfusion*



Reference number  
ISO 8536-7:1992(E)

## Contents

	Page
1 Scope .....	1
2 Normative references .....	1
3 Classification of types .....	1
4 Dimensions and tolerances .....	1
5 Designation .....	2
6 Requirements .....	2
7 Packaging .....	3
8 Marking .....	3

STANDARDSISO.COM : Click to view the full PDF of ISO 8536-7:1992

© ISO 1992

All rights reserved. No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization  
Case Postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 8536-7 was prepared by Technical Committee ISO/TC 76, *Transfusion, infusion and injection equipment for medical use*.

ISO 8536 consists of the following parts, under the general title *Infusion equipment for medical use*:

- Part 1: *Infusion glass bottles*
- Part 2: *Closures for infusion bottles*
- Part 3: *Aluminium caps for infusion bottles*
- Part 4: *Infusion sets for single use*
- Part 5: *Burette type infusion sets*
- Part 6: *Freeze drying closures for infusion bottles*
- Part 7: *Caps made of aluminium-plastics combinations for infusion bottles*

## Introduction

The materials from which infusion glass bottles (including elastomeric closures) are made are suitable primary packaging materials for storing infusion solutions until they are administered. However, in this part of ISO 8536, aluminium caps are not considered as primary packaging materials in direct contact with the infusion solution.

STANDARDSISO.COM : Click to view the full PDF of ISO 8536-7:1992

## Infusion equipment for medical use —

### Part 7:

### Caps made of aluminium-plastics combinations for infusion bottles

#### 1 Scope

This part of ISO 8536 specifies caps made of aluminium-plastics combinations intended for use on infusion bottles as specified in ISO 8536-1.

#### 2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this part of ISO 8536. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this part of ISO 8536 are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 2768-1:1989, *General tolerances — Part 1: Tolerances for linear and angular dimensions without individual tolerance indications.*

ISO 2768-2:1989, *General tolerances — Part 2: Geometrical tolerances for features without individual tolerance indications.*

ISO 8536-1:1991, *Infusion equipment for medical use — Part 1: Infusion glass bottles.*

ISO 8536-3:1992, *Infusion equipment for medical use — Part 3: Aluminium caps for infusion bottles.*

ISO 8872:1988, *Aluminium caps for transfusion, infusion and injection bottles — General requirements and test methods.*

ISO 10985:1992, *Caps made of aluminium-plastics combinations for infusion bottles and injection vials — Requirements and test methods.*

#### 3 Classification of types

Caps shall be classified as follows:

- Type ZB: Aluminium cap with central opening, and plastics component;
- Type ZD: Aluminium cap with complete tear-off tab, and plastics component.

#### 4 Dimensions and tolerances

##### 4.1 Dimensions

All cover versions (flat, ring-shaped or others) of caps shall meet the dimensions given in figure 1 and table 1.

NOTE 1 The configuration of the cap shown in figure 1 is informative only.

##### 4.2 Tolerances

Cap tolerances shall be in accordance with ISO 2768-1 and ISO 2768-2.

Dimensions in millimetres

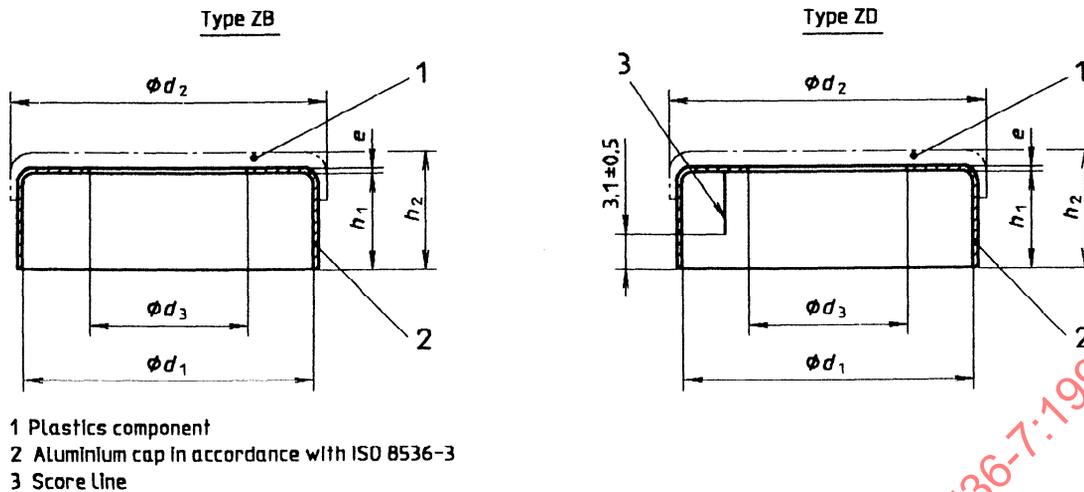


Figure 1 — Configuration of cap

Table 1 — Dimensions of cap

Dimensions in millimetres

Nominal size	$d_1$ $+0,1$ $0$	$d_2$ <sup>1)</sup>		$d_3$ <sup>2)</sup>		$e$ <sup>3)</sup>		$h_1$ $\pm 0,25$	$h_2$ <sup>4)</sup>	
		min.	max.	min.	max.	min.	max.		min.	max.
28	27,9	30,5	31,5	12	17	0,168	0,242	9,2	9	12
32	32,6	35,5	37	15	20			11,9	13	16

1) The diameter  $d_2$  shall be agreed between the manufacturer and user. It shall not differ from the nominal value by more than  $\pm 0,25$  mm. The extreme limits are given without tolerance.

2) After plastics element removal.

3) The thickness  $e$  shall be agreed between the manufacturer and user. It shall not differ from the nominal value by more than  $\pm 0,022$  mm. The extreme limits are given without tolerance.

4) The height  $h_2$  shall be agreed between the manufacturer and user. It shall not differ from the nominal value by more than  $\pm 0,4$  mm. The extreme limits are given without tolerance.

## 5 Designation

Aluminium-plastics caps shall be designated according to type: the designation shall be expressed as the word "cap", the number and part of this International Standard followed by the type letters, followed by the nominal size of the container.

For example a type ZD aluminium-plastics cap of nominal size 32 complying with the requirements laid down in this part of ISO 8536 is designated:

Cap ISO 8536-7 - ZD - 32

## 6 Requirements

### 6.1 General requirements

6.1.1 The requirements for aluminium caps shall be in accordance with ISO 8536-3.

6.1.2 The requirements for plastics components, and the combination between the plastics component and the aluminium cap, shall be in accordance with ISO 10985.

6.1.3 Construction elements which penetrate into the interior space of the aluminium cap shall not interfere with the sealing process.