

# INTERNATIONAL ISO/IEEE STANDARD 11073-10415

Second edition  
2022-12

---

---

## Health informatics — Device interoperability —

### Part 10415: Personal health device communication — Device specialization — Weighing scale

*Informatique de santé — Interopérabilité des dispositifs —*

*Partie 10415: Communication entre dispositifs de santé personnels —  
Spécialisation des dispositifs — Plateau de balance*

STANDARDSISO.COM : Click to view the PDF of ISO/IEEE 11073-10415:2022



Reference number  
ISO/IEEE 11073-10415:2022(E)

© IEEE 2019

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10415:2022



**COPYRIGHT PROTECTED DOCUMENT**

© IEEE 2019

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from IEEE at the address below.

Institute of Electrical and Electronics Engineers, Inc  
3 Park Avenue, New York  
NY 10016-5997, USA

Email: [stds.ipr@ieee.org](mailto:stds.ipr@ieee.org)  
Website: [www.ieee.org](http://www.ieee.org)

Published in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted (see [www.iso.org/directives](http://www.iso.org/directives)).

IEEE Standards documents are developed within the IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (IEEE-SA) Standards Board. The IEEE develops its standards through a consensus development process, approved by the American National Standards Institute, which brings together volunteers representing varied viewpoints and interests to achieve the final product. Volunteers are not necessarily members of the Institute and serve without compensation. While the IEEE administers the process and establishes rules to promote fairness in the consensus development process, the IEEE does not independently evaluate, test, or verify the accuracy of any of the information contained in its standards.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

ISO/IEEE 11073-10415 was prepared by the *IEEE 11073 Standards Committee of the IEEE Engineering in Medicine and Biology Society* (as IEEE Std 11073-10415-2019) and drafted in accordance with its editorial rules. It was adopted, under the "fast-track procedure" defined in the Partner Standards Development Organization cooperation agreement between ISO and IEEE, by Technical Committee ISO/TC 215, *Health informatics*.

This second edition cancels and replaces the first edition (ISO/IEEE 11073-10415:2010), which has been technically revised.

A list of all parts in the ISO/IEEE 11073 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10415:2022

**Health informatics—Personal health device communication**

**Part 10415: Device specialization—  
Weighing scale**

Developed by the

**IEEE 11073™ Standards Committee**  
of the  
**IEEE Engineering in Medicine and Biology Society**

Approved 7 November 2019

**IEEE SA Standards Board**

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10415:2022

**Abstract:** Within the context of the ISO/IEEE 11073 family of standards for device communication, this standard establishes a normative definition of communication between personal telehealth weighing scale devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes) in a manner that enables plug-and-play interoperability. It leverages appropriate portions of existing standards including ISO/IEEE 11073 terminology, information models, application profile standards, and transport standards. It specifies the use of specific term codes, formats, and behaviors in telehealth environments restricting optionality in base frameworks in favor of interoperability. This standard defines a common core of communication functionality for personal telehealth weighing scales.

**Keywords:** IEEE 11073-10415™, medical device communication, personal health devices, weighing scale

---

The Institute of Electrical and Electronics Engineers, Inc.  
3 Park Avenue, New York, NY 10016-5997, USA

Copyright © 2019 by The Institute of Electrical and Electronics Engineers, Inc.  
All rights reserved. Published 23 December 2019. Printed in the United States of America.

IEEE is a registered trademark in the U.S. Patent & Trademark Office, owned by The Institute of Electrical and Electronics Engineers, Incorporated.

PDF: ISBN 978-1-5044-6363-8     STD24007  
Print: ISBN 978-1-5044-6364-5     STDPD24007

*IEEE prohibits discrimination, harassment, and bullying.  
For more information, visit <http://www.ieee.org/web/aboutus/whatis/policies/p9-26.html>.  
No part of this publication may be reproduced in any form, in an electronic retrieval system or otherwise, without the prior written permission of the publisher.*

## Important Notices and Disclaimers Concerning IEEE Standards Documents

IEEE documents are made available for use subject to important notices and legal disclaimers. These notices and disclaimers, or a reference to this page, appear in all standards and may be found under the heading “Important Notices and Disclaimers Concerning IEEE Standards Documents.” They can also be obtained on request from IEEE or viewed at <http://standards.ieee.org/ipr/disclaimers.html>.

## Notice and Disclaimer of Liability Concerning the Use of IEEE Standards Documents

IEEE Standards documents (standards, recommended practices, and guides), both full-use and trial-use, are developed within IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (“IEEE SA”) Standards Board. IEEE (“the Institute”) develops its standards through a consensus development process, approved by the American National Standards Institute (“ANSI”), which brings together volunteers representing varied viewpoints and interests to achieve the final product. IEEE Standards are documents developed through scientific, academic, and industry-based technical working groups. Volunteers in IEEE working groups are not necessarily members of the Institute and participate without compensation from IEEE. While IEEE administers the process and establishes rules to promote fairness in the consensus development process, IEEE does not independently evaluate, test, or verify the accuracy of any of the information or the soundness of any judgments contained in its standards.

IEEE Standards do not guarantee or ensure safety, security, health, or environmental protection, or ensure against interference with or from other devices or networks. Implementers and users of IEEE Standards documents are responsible for determining and complying with all appropriate safety, security, environmental, health, and interference protection practices and all applicable laws and regulations.

IEEE does not warrant or represent the accuracy or content of the material contained in its standards, and expressly disclaims all warranties (express, implied and statutory) not included in this or any other document relating to the standard, including, but not limited to, the warranties of: merchantability; fitness for a particular purpose; non-infringement; and quality, accuracy, effectiveness, currency, or completeness of material. In addition, IEEE disclaims any and all conditions relating to: results; and workmanlike effort. IEEE standards documents are supplied “AS IS” and “WITH ALL FAULTS.”

Use of an IEEE standard is wholly voluntary. The existence of an IEEE standard does not imply that there are no other ways to produce, test, measure, purchase, market, or provide other goods and services related to the scope of the IEEE standard. Furthermore, the viewpoint expressed at the time a standard is approved and issued is subject to change brought about through developments in the state of the art and comments received from users of the standard.

In publishing and making its standards available, IEEE is not suggesting or rendering professional or other services for, or on behalf of, any person or entity nor is IEEE undertaking to perform any duty owed by any other person or entity to another. Any person utilizing any IEEE Standards document, should rely upon his or her own independent judgment in the exercise of reasonable care in any given circumstances or, as appropriate, seek the advice of a competent professional in determining the appropriateness of a given IEEE standard.

IN NO EVENT SHALL IEEE BE LIABLE FOR ANY DIRECT, INDIRECT, INCIDENTAL, SPECIAL, EXEMPLARY, OR CONSEQUENTIAL DAMAGES (INCLUDING, BUT NOT LIMITED TO: PROCUREMENT OF SUBSTITUTE GOODS OR SERVICES; LOSS OF USE, DATA, OR PROFITS; OR BUSINESS INTERRUPTION) HOWEVER CAUSED AND ON ANY THEORY OF LIABILITY, WHETHER IN CONTRACT, STRICT LIABILITY, OR TORT (INCLUDING NEGLIGENCE OR OTHERWISE) ARISING IN ANY WAY OUT OF THE PUBLICATION, USE OF, OR RELIANCE UPON ANY STANDARD, EVEN IF ADVISED OF THE POSSIBILITY OF SUCH DAMAGE AND REGARDLESS OF WHETHER SUCH DAMAGE WAS FORESEEABLE.

## Translations

The IEEE consensus development process involves the review of documents in English only. In the event that an IEEE standard is translated, only the English version published by IEEE should be considered the approved IEEE standard.

## Official statements

A statement, written or oral, that is not processed in accordance with the IEEE SA Standards Board Operations Manual shall not be considered or inferred to be the official position of IEEE or any of its committees and shall not be considered to be, or be relied upon as, a formal position of IEEE. At lectures, symposia, seminars, or educational courses, an individual presenting information on IEEE standards shall make it clear that his or her views should be considered the personal views of that individual rather than the formal position of IEEE.

## Comments on standards

Comments for revision of IEEE Standards documents are welcome from any interested party, regardless of membership affiliation with IEEE. However, IEEE does not provide consulting information or advice pertaining to IEEE Standards documents. Suggestions for changes in documents should be in the form of a proposed change of text, together with appropriate supporting comments. Since IEEE standards represent a consensus of concerned interests, it is important that any responses to comments and questions also receive the concurrence of a balance of interests. For this reason, IEEE and the members of its societies and Standards Coordinating Committees are not able to provide an instant response to comments or questions except in those cases where the matter has previously been addressed. For the same reason, IEEE does not respond to interpretation requests. Any person who would like to participate in revisions to an IEEE standard is welcome to join the relevant IEEE working group.

Comments on standards should be submitted to the following address:

Secretary, IEEE SA Standards Board  
445 Hoes Lane  
Piscataway, NJ 08854 USA

## Laws and regulations

Users of IEEE Standards documents should consult all applicable laws and regulations. Compliance with the provisions of any IEEE Standards document does not imply compliance to any applicable regulatory requirements. Implementers of the standard are responsible for observing or referring to the applicable regulatory requirements. IEEE does not, by the publication of its standards, intend to urge action that is not in compliance with applicable laws, and these documents may not be construed as doing so.

## Copyrights

IEEE draft and approved standards are copyrighted by IEEE under US and international copyright laws. They are made available by IEEE and are adopted for a wide variety of both public and private uses. These include both use, by reference, in laws and regulations, and use in private self-regulation, standardization, and the promotion of engineering practices and methods. By making these documents available for use and adoption by public authorities and private users, IEEE does not waive any rights in copyright to the documents.

## Photocopies

Subject to payment of the appropriate fee, IEEE will grant users a limited, non-exclusive license to photocopy portions of any individual standard for company or organizational internal use or individual, non-commercial use only. To arrange for payment of licensing fees, please contact Copyright Clearance Center, Customer Service, 222 Rosewood Drive, Danvers, MA 01923 USA; +1 978 750 8400. Permission to photocopy portions of any individual standard for educational classroom use can also be obtained through the Copyright Clearance Center.

## Updating of IEEE Standards documents

Users of IEEE Standards documents should be aware that these documents may be superseded at any time by the issuance of new editions or may be amended from time to time through the issuance of amendments, corrigenda, or errata. An official IEEE document at any point in time consists of the current edition of the document together with any amendments, corrigenda, or errata then in effect.

Every IEEE standard is subjected to review at least every 10 years. When a document is more than 10 years old and has not undergone a revision process, it is reasonable to conclude that its contents, although still of some value, do not wholly reflect the present state of the art. Users are cautioned to check to determine that they have the latest edition of any IEEE standard.

In order to determine whether a given document is the current edition and whether it has been amended through the issuance of amendments, corrigenda, or errata, visit IEEE Xplore at <https://ieeexplore.ieee.org> or contact IEEE at the address listed previously. For more information about the IEEE SA or IEEE's standards development process, visit the IEEE SA Website at <http://standards.ieee.org>.

## Errata

Errata, if any, for IEEE standards can be accessed via <https://standards.ieee.org/standard/index.html>. Search for standard number and year of approval to access the web page of the published standard. Errata links are located under the Additional Resources - Details section. Errata are also available in IEEE Xplore: <https://ieeexplore.ieee.org/browse/standards/collection/ieee/>. Users are encouraged to periodically check for errata.

## Patents

Attention is called to the possibility that implementation of this standard may require use of subject matter covered by patent rights. By publication of this standard, no position is taken by the IEEE with respect to the existence or validity of any patent rights in connection therewith. If a patent holder or patent applicant has filed a statement of assurance via an Accepted Letter of Assurance, then the statement is listed on the IEEE SA Website at <https://standards.ieee.org/about/sasb/patcom/patents.html>. Letters of Assurance may indicate whether the Submitter is willing or unwilling to grant licenses under patent rights without compensation or under reasonable rates, with reasonable terms and conditions that are demonstrably free of any unfair discrimination to applicants desiring to obtain such licenses.

Essential Patent Claims may exist for which a Letter of Assurance has not been received. The IEEE is not responsible for identifying Essential Patent Claims for which a license may be required, for conducting inquiries into the legal validity or scope of Patents Claims, or determining whether any licensing terms or conditions provided in connection with submission of a Letter of Assurance, if any, or in any licensing agreements are reasonable or non-discriminatory. Users of this standard are expressly advised that determination of the validity of any patent rights, and the risk of infringement of such rights, is entirely their own responsibility. Further information may be obtained from the IEEE Standards Association.

## Participants

At the time this standard was completed, the Personal Health Devices Working Group had the following membership:

**Daidi Zhong**, *Co-chair*  
**Michael J. Kirwan**, *Co-chair*

Karsten Aalders	James Cheng	Rick Geimer
Charles R. Abbruscato	Peggy Chien	Igor Gejdos
Nabil Abujbara	David Chiu	Ferenc Gerbovics
Maher Abuzaid	Jinyong Choi	Alan Godfrey
James Agnew	Chia-Chin Chong	Nicolae Goga
Haidar Ahmad	Saeed A. Choudhary	Julian Goldman
Manfred Aigner	Jinhan Chung	Raul Gonzalez Gomez
Jorge Alberola	Malcolm Clarke	Chris Gough
Murtaza Ali	John A. Cogan	Channa Gowda
Rolf Ambuehl	John T. Collins	Charles M. Gropper
David Aparisi	Cory Condek	Amit Gupta
Paolo Ariano	Todd H. Cooper	Jeff Guttmacher
Lawrence Arne	David Cornejo	Rasmus Haahr
Diego B. Arquillo	Douglas Coup	Christian Habermann
Serafin Arroyo	Nigel Cox	Michael Hagerty
Muhammad Asim	Hans Crommenacker	Jerry Hahn
Merat Bagha	Tomio Crosley	Robert Hall
Doug Baird	Allen Curtis	Shu Han
David Baker	Ndifor Cyril Fru	Nathaniel Hamming
Anindya Bakshi	Jesús Daniel Trigo	Rickey L. Hampton
Ananth Balasubramanian	Eyal Dassau	Sten Hanke
Sunlee Bang	David Davenport	Aki Harma
M. Jonathan Barkley	Russell Davis	Jordan Hartmann
Gilberto Barrón	Sushil K. Deka	Kai Hassing
David Bean	Ciro de la Vega	Wolfgang Heck
John Bell	Pedro de las-Heras-Quiros	Nathaniel Heintzman
Rudy Belliardi	Jim DeHo Stritto	Charles Henderson
Kathryn M. Bennett	Matthew d'Entremont	Jun-Ho Her
Daniel Bernstein	Kent Dicks	Helen B. Hernandez
George A. Bertos	Hyoungdo Do	Takashi Hibino
Chris Biernacki	Alistair Donaldson	Timothy L. Hirou
Ola Björnsne	Xiaolian Duan	Allen Hobbs
Thomas Blackadar	Brian Dubreuil	Alex Holland
Marc Blanchet	Sourav Dutta	Arto Holopainen
Thomas Bluethner	Jakob Ehrensvarð	Kris Holtzclaw
Douglas P. Bogia	Fredrik Einberg	Xinyi Hong
Xavier Boniface	Michihiro Enokida	Robert Hoy
Shannon Boucoussis	Javier Escayola Calvo	Frank Hsu
Julius Broma	Mark Estes	Anne Huang
Lyle G. Bullock, Jr.	Leonardo Estevez	Sen-Der Huang
Bernard Burg	Roger Feeley	Ron Huby
Chris Burns	Hailing Feng	David Hughes
Anthony Butt	Bosco T. Fernandes	Robert D. Hughes
Jeremy Byford-Rew	Christoph Fischer	Jiyoung Huh
Satya Calloji	Morten Flintrup	Hugh Hunter
Xiaoying Cao	Joseph W. Forler	Hitoshi Ikeda
Carole C. Carey	Russell Foster	Yutaka Ikeda
Craig Carlson	Eric Freudenthal	Philip O. Isaacson
Santiago Carot-Nemesio	Matthias Frohner	Atsushi Ito
Randy W. Carroll	Ken Fuchs	Michael Jaffe
Simon Carter	Jing Gao	Praduman Jain
Seungchul Chae	Qi Gao	Danny Jochelson
Rahul Chauhan	Marcus Garbe	Phaneeth Junga
Wenjuan Chen	John Garguilo	Akiyoshi Kabe

Steve Kahle	Peter Mayhew	Fatemeh Saki
Tomio Kamioka	Jim McCain	Bill Saltzstein
James J. Kang	László Meleg	Benedikt Salzbrunn
Kei Kariya	Alexander Mense	Giovanna Sannino
Andy Kaschl	Behnaz Minaei	Jose A. Santos-Cadenas
Junzo Kashihara	Jinsei Miyazaki	Stefan Sauermann
Kohichi Kashiwagi	Erik Moll	John Sawyer
Ralph Kent	Darr Moore	Guillaume Schatz
Laurie M. Kermes	Carsten Mueglitz	Alois Schloegl
Ikuo Keshi	Piotr Murawski	Paul S. Schluter
Ahmad Kheirandish	Soundharya Nagasubramanian	Lars Schmitt
Junhyung Kim	Jae-Wook Nah	Mark G. Schnell
Minho Kim	Alex Neefus	Richard A. Schrenker
Min-Joon Kim	Trong-Nghia Nguyen-Dobinsky	Antonio Scorpiniti
Taekon Kim	Michael E. Nidd	KwangSeok Seo
Tetsuya Kimura	Tetsu Nishimura	Riccardo Serafin
Alfred Kloos	Jim Niswander	Sid Shaw
Jeongmee Koh	Hongliang Niu	Frank Shen
Jean-Marc Koller	Hiroaki Niwamoto	Min Shih
Fei Kong	Thomas Norgall	Mazen Shihabi
John Koon	Anand Noubade	Redmond Shouldice
Patty Krantz	Yoshiteru Nozoe	Sternly K. Simon
Raymond Krasinski	Abraham Ofek	Marjorie Skubic
Alexander Kraus	Brett Olive	Robert Smith
Ramesh Krishna	BegonyaOtal	Ivan Soh
Geoffrey Kruse	Marco Paleari	Motoki Sone
Falko Kuester	Charles Palmer	Emily Sopensky
Rafael Lajara	Bud Panjwani	Rajagopalan Srinivasan
Shing C. B. Lam	Carl Pantiskas	Andreas Staubert
Pierre Landau	Harry P. Pappas	Nicholas Steblay
Jacchul Lee	Hanna Park	Lars Steubesand
JongMuk Lee	Jong-Tae Park	John (Ivo) Stivoric
Kyong Ho Lee	Myungeun Park	Raymond A. Strickland
Rami Lee	Soojun Park	Chandrasekaran Subramaniam
Sungkee Lee	Phillip E. Pash	Hermann Suominen
Woojae Lee	TongBi Pei	Lee Surprenant
Yonghee Lee	Lucian Pestritu	Ravi Swami
Joe Lenart	Soren Petersen	Ray Sweidan
Kathryn A. Lesh	James Petisce	Jin Tan
Catherine Li	Peter Piction	Yi Tang
Jingli Li	Michael Pliskin	Haruyuyki Tatsumi
Qiong Li	Varshney Prabodh	Isabel Tejero
Xiangchen Li	Jeff Price	John W. Thomas
Zhuofang Li	Harald Prinzhorn	Jonas Tirén
Patrick Lichter	Harry Qiu	Alexandra Todiruta
Jisoon Lim	Arif Rahman	Janet Traub
Joon-Ho Lim	Tanzilur Rahman	Gary Tschautscher
John Lin	Steve Ray	Masato Tsuchid
Hongliang Niu	Phillip Raymond	Ken Tubman
Xiaoming Liu	Terrie Reed	Yoshihiro Uchida
Wei-Jung Lo	Tim Reilly	Akib Uddin
Charles Lowe	Barry Reinhold	Sunil Unadkat
Don Ludolph	Brian Reinhold	Fabio Urbani
Christian Luszick	Melvin I. Reynolds	Philipp Urbauer
Songdong Lv	John G. Rhoads	Laura Vanzago
Bob MacWilliams	Jeffrey S. Robbins	Alpo Väri
Srikanth Madhurbootheswaran	Chris Roberts	Andrei Vasileanu
Miriam L. Makhoul	Moskowitz Robert	Dalimar Velez
Romain Marmot	Scott M. Robertson	Martha Velez
Sandra Martinez	Timothy Robertson	Rudi Voon
Miguel Martínez de	David Rosales	Barry Vornbrock
EspronedcaCámara	Gary Sagiv	Isobel Walker

David Wang  
Jerry P. Wang  
Yao Wang  
Yi Wang  
Steve Warren  
Fujio Watanabe  
Toru Watsuji  
Mike Weng  
Yuefeng Weng

Kathleen Wible  
Paul Williamson  
Jan Wittenber  
Jia-Rong Wu  
Will Wykeham  
Ariton Xhafa  
Qifeng Yan  
Ricky Yang  
Shaoqin Ye  
Melanie S. Yeung

Qiang Yin  
Done-Sik Yoo  
Jianchao Zeng  
Jason Zhang  
Zhiqiang Zhang  
Thomas Zhao  
Jia Zheng  
Miha Zoubek  
Szymon Zyskoter

The following members of the individual Standards Association balloting group voted on this standard. Balloters may have voted for approval, disapproval, or abstention.

Bjoern Andersen  
Lyle G. Bullock, Jr.  
Keith Chow  
Malcolm Clarke  
David Fuschi  
Randall Groves  
Werner Hoelzl

Noriyuki Ikeuchi  
Atsushi Ito  
Raj Jain  
Piotr Karocki  
Raymond Krasinski  
H. Moll

Beth Pumo  
Stefan Schlichting  
Janek Schumann  
Walter Struppler  
Oren Yuen  
Janusz Zalewski  
Daidi Zhong

When the IEEE SA Standards Board approved this standard on 7 November 2019, it had the following membership:

**Gary Hoffman, *Chair***  
**Ted Burse, *Vice Chair***  
**Jean-Philippe Faure, *Past Chair***  
**Konstantinos Karachalios, *Secretary***

Masayuki Ariyoshi  
Stephen D. Dukes  
J. Travis Griffith  
Guido Hiertz  
Christel Hunter  
Joseph L. Koepfinger\*  
Thomas Koshy  
John D. Kulick

David J. Law  
Joseph Levy  
Howard Li  
Xiaohui Liu  
Kevin Lu  
Daleep Mohla  
Andrew Myles

Annette Reilly  
Dorothy Stanley  
Sha Wei  
Phil Wennblom  
Philip Winston  
Howard Wolfman  
Feng Wu  
Jingyi Zhou

\*Member Emeritus

## Introduction

This introduction is not part of IEEE Std 11073-10415-2019, Health informatics—Personal health device communication—Part 10415: Device specialization—Weighing scale.

ISO/IEEE 11073 standards enable communication between medical devices and external computer systems. This document uses the optimized framework created in IEEE Std 11073-20601<sup>a</sup> and describes a specific, interoperable communication approach for weighing scales. These standards align with, and draw on the existing clinically focused standards to provide support for communication of data from clinical or personal health devices.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10415:2022

---

<sup>a</sup> Information on normative references can be found in Clause 2.

**Contents**

1. Overview .....12

    1.1 Scope .....12

    1.2 Purpose .....12

    1.3 Context .....12

    1.4 Word usage .....13

2. Normative references.....13

3. Definitions, acronyms, and abbreviations .....14

    3.1 Definitions .....14

    3.2 Acronyms and abbreviations .....14

4. Introduction to ISO/IEEE 11073 personal health devices .....15

    4.1 General .....15

    4.2 Introduction to IEEE 11073-20601 modeling constructs .....15

    4.3 Compliance with other standards.....16

5. Weighing scale device concepts and modalities .....16

    5.1 General .....16

    5.2 Body weight.....16

    5.3 Body height .....17

    5.4 Body mass index.....17

6. Weighing scale domain information model.....17

    6.1 Overview .....17

    6.2 Class extensions.....17

    6.3 Object instance diagram .....17

    6.4 Types of configuration.....19

    6.5 Medical device system object.....20

    6.6 Numeric objects.....23

    6.7 Real-time sample array objects.....28

    6.8 Enumeration objects .....28

    6.9 PM-store objects.....28

    6.10 Scanner objects.....28

    6.11 Class extension objects.....28

    6.12 Weighing scale information model extensibility rules .....28

7. Weighing scale service model .....29

    7.1 General .....29

    7.2 Object access services.....29

    7.3 Object access event report services .....31

8. Weighing scale communication model.....31

    8.1 Overview .....31

    8.2 Communications characteristics .....31

STANDARDS.PDF.COM Click to view the full PDF of ISO/IEEE 11073-10415:2022

8.3 Association procedure .....	32
8.4 Configuring procedure.....	34
8.5 Operating procedure .....	35
8.6 Time synchronization .....	36
9. Test associations.....	36
9.1 General .....	36
9.2 Behavior with standard configuration.....	36
9.3 Behavior with extended configurations .....	36
10. Conformance .....	37
10.1 Applicability .....	37
10.2 Conformance specification .....	37
10.3 Levels of conformance .....	37
10.4 Implementation conformance statements .....	38
Annex A (informative) Bibliography .....	43
Annex B (normative) Any additional ASN.1 definitions .....	44
Annex C (normative) Allocation of identifiers.....	45
Annex D (informative) Message sequence examples.....	46
Annex E (informative) Protocol data unit examples .....	48
Annex F (informative) Revision history.....	58

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10415:2022

## Health informatics—Personal health device communication

# Part 10415: Device specialization— Weighing scale

### 1. Overview

#### 1.1 Scope

Within the context of the ISO/IEEE 11073 family of standards for device communication, this standard establishes a normative definition of communication between personal telehealth weighing scale devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes) in a manner that enables plug-and-play interoperability. It leverages appropriate portions of existing standards, including ISO/IEEE 11073 terminology, information models, application profile standards, and transport standards. It specifies the use of specific term codes, formats, and behaviors in telehealth environments restricting optionality in base frameworks in favor of interoperability. This standard defines a common core of communication functionality for personal telehealth weighing scales.

#### 1.2 Purpose

This standard addresses a need for an openly defined, independent standard for controlling information exchange to and from personal health devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes). Interoperability is the key to growing the potential market for these devices and to enabling people to be better informed participants in the management of their health.

#### 1.3 Context

See IEEE Std 11073-20601™ for an overview of the environment within which this standard is written.<sup>1</sup>

This document, IEEE Std 11073-10415, defines the device specialization for the weighing scale, being a specific agent type, and it provides a description of the device concepts, its capabilities, and its implementation according to this standard.

This standard is based on IEEE Std 11073-20601, which in turn draws information from both ISO/IEEE 11073-10201:2004 [B7] and ISO/IEEE 11073-20101:2004 [B8].<sup>2</sup> The medical device encoding rules (MDER) used within this standard are fully described in IEEE Std 11073-20601.

<sup>1</sup> Information on normative references can be found in Clause 2.

<sup>2</sup> The numbers in brackets correspond to the numbers of the bibliography in Annex A.

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

This standard defines specialized nomenclature codes that will be collected in future versions of IEEE Std 11073-10101. Between this standard, IEEE Std 11073-10101, IEEE Std 11073-20601, and IEEE Std 11073-104zz, all required nomenclature codes for implementation are documented. New codes may be defined in newer versions/revisions of each of these documents. In the case of a conflict, where one term code has been assigned to two separate semantic concepts with different RefIDs, in general the oldest definition that is in actual use should take precedence. The same policy applies when one RefID has two different code values assigned in different specifications. The resolution of such conflicts will be determined through joint action by the responsible working groups and other stakeholders, and any corrective action published as corrigenda.

NOTE— In this standard, the term *IEEE Std 11073-104zz* is used to refer to the collection of device specialization standards that utilize IEEE Std 11073-20601, where *zz* can be any number from 01 to 99, inclusive.<sup>3</sup>

## 1.4 Word usage

The word *shall* indicates mandatory requirements strictly to be followed in order to conform to the standard and from which no deviation is permitted (shall equals is required to).<sup>4,5</sup>

The word *should* indicates that among several possibilities one is recommended as particularly suitable, without mentioning or excluding others; or that a certain course of action is preferred but not necessarily required (should equals is recommended that).

The word *may* is used to indicate a course of action permissible within the limits of the standard (may equals is permitted to).

The word *can* is used for statements of possibility and capability, whether material, physical, or causal (can equals is able to).

## 2. Normative references

The following referenced documents are indispensable for the application of this document (i.e., they must be understood and used, so that each referenced document is cited in text and its relationship to this document is explained). For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments or corrigenda) applies.

IEEE Std 11073-20601™, Health informatics—Personal health device communication—Part 20601: Application profile—Optimized Exchange Protocol.<sup>6,7</sup>

IEEE Std 11073-10101™, Health informatics—Point-of-care medical device communication—Part 10101: Nomenclature.

See Annex A for all informative material referenced by this standard.

<sup>3</sup> Notes in text, tables, and figures are given for information only and do not contain requirements needed to implement the standard.

<sup>4</sup> The use of the word *must* is deprecated and cannot be used when stating mandatory requirements; *must* is used only to describe unavoidable situations.

<sup>5</sup> The use of *will* is deprecated and cannot be used when stating mandatory requirements; *will* is used only in statements of fact.

<sup>6</sup> The IEEE standards or products referred to in this clause are trademarks of The Institute of Electrical and Electronics Engineers, Inc.

<sup>7</sup> IEEE publications are available from The Institute of Electrical and Electronics Engineers (<http://standards.ieee.org/>).

### 3. Definitions, acronyms, and abbreviations

#### 3.1 Definitions

For the purposes of this standard, the following terms and definitions apply. The *IEEE Standards Dictionary Online* should be referenced for terms not defined in this clause.<sup>8</sup>

**agent:** A node that collects and transmits personal health data to an associated manager.

**class:** In object-oriented modeling, it describes the attributes, methods, and events that objects instantiated from the class utilize.

**compute engine:** *See:* **manager.**

**device:** A physical device implementing either an agent or a manager role.

**handle:** An unsigned 16-bit number that is locally unique and identifies one of the object instances within an agent.

**manager:** A node receiving data from one or more agent systems. Examples of managers include a cellular phone, health appliance, set top box, or a computer system.

**mass:** An intrinsic property of matter that can be measured using the effect of the gravitational field on an object.

**obj-handle:** *See:* **handle.**

**object:** A unit that represents some functionality or item in a device whose properties are described by attributes.

**personal health device:** A device used in personal health applications.

**personal telehealth device:** *See:* **personal health device.**

**weight:** The force that results from the exertion of gravity on an object. The weight is directly proportional to the mass of the object. However, in the health care domain, the term *body weight* is typically used to denote the body mass of a person.

NOTE—The notation about body weight applies also to this standard.

#### 3.2 Acronyms and abbreviations

APDU	application protocol data unit
ASN.1	Abstract Syntax Notation One
BMI	body mass index
DIM	domain information model
EUI-64	extended unique identifier (64 bits)
ICS	implementation conformance statement
MDC	medical device communication
MDER	medical device encoding rules
MDS	medical device system
MOC	managed object class
PHD	personal health device
RT-SA	real-time sample array
VMO	virtual medical object
VMS	virtual medical system

<sup>8</sup> *IEEE Standards Dictionary Online* is available at <http://dictionary.ieee.org>.

## 4. Introduction to ISO/IEEE 11073 personal health devices

### 4.1 General

This standard and the remainder of the series of ISO/IEEE 11073 personal health device (PHD) standards fit in the larger context of the ISO/IEEE 11073 series of standards. The full suite of standards enables agents to interconnect and interoperate with managers and with computerized health-care information systems. See IEEE Std 11073-20601 for a description of the guiding principles for this series of ISO/IEEE 11073 personal health device standards.

IEEE Std 11073-20601 supports the modeling and implementation of an extensive set of personal health devices. This standard defines aspects of the weighing scale device. It describes all aspects necessary to implement the application layer services and data exchange protocol between an ISO/IEEE 11073 PHD weighing scale agent and a manager. This standard defines a subset of the objects and functionality contained in IEEE Std 11073-20601 and extends and adds definitions where appropriate. All new definitions are given in Annex B in Abstract Syntax Notation One (ASN.1) [B9].

All nomenclature codes referenced in this standard are collected in Annex C. Annex C may contain definitions of codes that are used by this standard and that are not yet present in the referenced versions of IEEE Std 11073-10101 and IEEE Std 11073-20601.

### 4.2 Introduction to IEEE 11073-20601 modeling constructs

#### 4.2.1 General

The ISO/IEEE 11073 series of standards, and in particular IEEE Std 11073-20601, is based on an object-oriented systems management paradigm. The overall system model is divided into three principal components: the domain information model (DIM), the service model, and the communication model. See IEEE Std 11073-20601 for a detailed description of the modeling constructs.

#### 4.2.2 Domain information model

The DIM is a hierarchical model that describes an agent as a set of objects. These objects and their attributes represent the elements that control behavior and report on the status of the agent and data that an agent can communicate to a manager. Communication between the agent and the manager is defined by the application protocol in IEEE Std 11073-20601.

#### 4.2.3 Service model

The service model defines the conceptual mechanisms for the data exchange services. Such services are mapped to messages that are exchanged between the agent and the manager. Protocol messages within the ISO/IEEE 11073 series of standards are defined in ASN.1. The messages defined in IEEE Std 11073-20601 can coexist with messages defined in other standard application profiles defined in the ISO/IEEE 11073 series of standards.

#### 4.2.4 Communication model

In general, the communication model supports the topology of one or more agents communicating over logical point-to-point connections to a single manager. For each logical point-to-point connection, the dynamic system behavior is defined by a connection state machine as specified in IEEE Std 11073-20601.

#### 4.2.5 Implementing the models

An agent implementing this standard shall implement all mandatory elements of the information, service, and communication models as well as all conditional elements where the condition is met. The agent should implement the recommended elements, and it may implement any combination of the optional elements. A manager implementing this standard shall utilize at least one of the mandatory, conditional, recommended, or optional elements. In this context, “utilize” means to use the element as part of the primary function of the manager device. For example, a manager whose primary function is to display data would need to display a piece of data in the element in order to utilize it.

#### 4.3 Compliance with other standards

Devices that comply with this standard may also be required to comply with other domain- and device-specific standards that supersede the requirements of this standard with respect to issues including safety, reliability, and risk management. A user of this standard is expected to be familiar with all other such standards that apply and to comply with any higher specifications thus imposed.

Typically, medical devices should comply with the IEC 60601-1 [B2] base standards with respect to electrical and mechanical safety and any device-specific standard as might be defined in the IEC 60601-2 [B3] series of standards. Software aspects may apply through standards such as IEC 62304 [B4]. Devices that comply with this standard implement higher layers of network software and utilize lower layers as appropriate to the application. The requirements on performance of such applications and conformance are defined elsewhere and are outside the scope of this standard. Moreover, the use of any medical equipment is subject to risk assessment and risk management appropriate to the application. Some relevant examples are ISO 14971 [B5] and IEC 80001-1 [B5]. The requirements of such risk assessment, risk management, and conformance are outside the scope of this standard. The applicable versions of the referenced safety related standards may differ per country.

### 5. Weighing scale device concepts and modalities

#### 5.1 General

This clause presents the general concepts of weighing scale devices. In the context of personal health devices in this family of standards, a weighing scale is a device that measures the body weight of a person and, optionally, determines other physiological quantities (e.g., the body mass index or the height of a person). Weighing scale devices considered in this standard are typically placed on the floor with a person stepping on the device to perform a weight measurement, with the result being converted into mass internally of the device.

In the personal health context, the body weight of a person is typically not measured more frequently than twice a day.

Weighing scale devices may use a variety of techniques for measuring body weight. One typical method is to place several strain-gauge load cells under the measurement plane to convert deformation into weight.

#### 5.2 Body weight

The primary data type of a weighing scale device is body weight. It has measurement units of kilograms (kg) or pounds (lb).

### 5.3 Body height

If body mass index reporting is supported, then body height is required. Body height denotes the actual height of the person using a weighing scale device. It has measurement units of centimeters (cm) or inches (in). This observation is typically entered manually.

### 5.4 Body mass index

The body mass index (BMI) is a measure for indicating an overweight or underweight condition of a person and is defined as the individual's body weight, in kilograms, divided by the square of height, in meters (see Garrow and Webster [B1]):

$$\text{BMI} = \frac{\text{body weight [kg]}}{\text{body height squared [m}^2\text{]}}$$

BMI is not measured directly but is derived from body weight and body height. In the case where pounds and inches are used as measurement units instead of kilograms and meters, the BMI may be calculated as follows:

$$\text{BMI} = 703 \times \frac{\text{body weight [lb]}}{\text{body height squared [in}^2\text{]}}$$

Using the value 703 as a conversion factor gives a relative error with respect to using kilograms and meters of less than 0.01%.

## 6. Weighing scale domain information model

### 6.1 Overview

This clause describes the domain information model of the weighing scale.

### 6.2 Class extensions

In this standard, no class extensions are defined with respect to IEEE Std 11073-20601.

### 6.3 Object instance diagram

The object instance diagram of the weighing scale domain information model, defined for the purposes of this standard, is shown in Figure 1.

The objects of the DIM, as shown in Figure 1, are described in 6.4 to 6.12. This includes the medical device system (MDS) object (see 6.5), the numeric objects (see 6.6), the real-time sample array (RT-SA) objects (see 6.7), the enumeration objects (see 6.8), the PM-store objects (see 6.9), and the scanner objects (see 6.10). See 6.11 for rules for extending the weighing scale information model beyond elements as described in this standard. Each clause that describes an object of the weighing scale contains the following information:

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

- The nomenclature code used to identify the class of the object. One example of where this code is used is the configuration event, where the object class is reported for each object. This allows the manager to determine whether the class of the object being specified is a numeric, real-time sample array, enumeration, scanner, or PM-store class.
- The attributes of the object. Each object has attributes that represent and convey information on the physical device and its data sources. Each object has a Handle attribute that identifies the object instance within an agent. Attribute values are accessed and modified using methods such as GET and SET. Attribute types are defined using ASN.1. The ASN.1 definitions for new attribute types specific to this standard are in Annex B, and the ASN.1 definitions for existing attribute types referenced in this standard are in IEEE Std 11073-20601.
- The methods available on the object.
- The potential events generated by the object. Data are sent to the manager using events.
- The available services such as getting or setting attributes.

The attributes for each class are defined in tables that specify the name of the attribute, its value, and its qualifier. The qualifiers mean M — Attribute is Mandatory, C — Attribute is Conditional and depends on the condition stated in the Remark or Value column (if IEEE Std 11073-20601 is referenced, then it contains the conditions), R — Attribute is Recommended, NR — Attribute is Not Recommended, NA — Attribute is Not Allowed and O — Attribute is Optional. Mandatory attributes shall be implemented by the agent. Conditional attributes shall be implemented if the condition applies and may be implemented otherwise. Recommended attributes should be implemented by the agent. Not recommended attributes should not be implemented by the agent. Optional attributes may be implemented by the agent. If any attribute (from the DIM of IEEE Std 11073-20601) is not included in the definition of that object in this standard, it shall not be included in that object by an implementation, unless it is a vendor-specific attribute extended according to 6.12.

An attribute is further qualified as static, dynamic, or observational.

- Static attributes shall not change value during the life of an association.
- Dynamic attributes have a value that may change during the life of an association. The dynamic attribute value should be sent at configuration time and shall be sent at or before the time when the value would be needed for interpreting a reported observation.
- Observational attributes have a value that may change during the life of an association. When a set of observational attribute values are received, these values are combined with the available context information (i.e., all related dynamic and static attribute values) to represent the observation at the observation time.

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

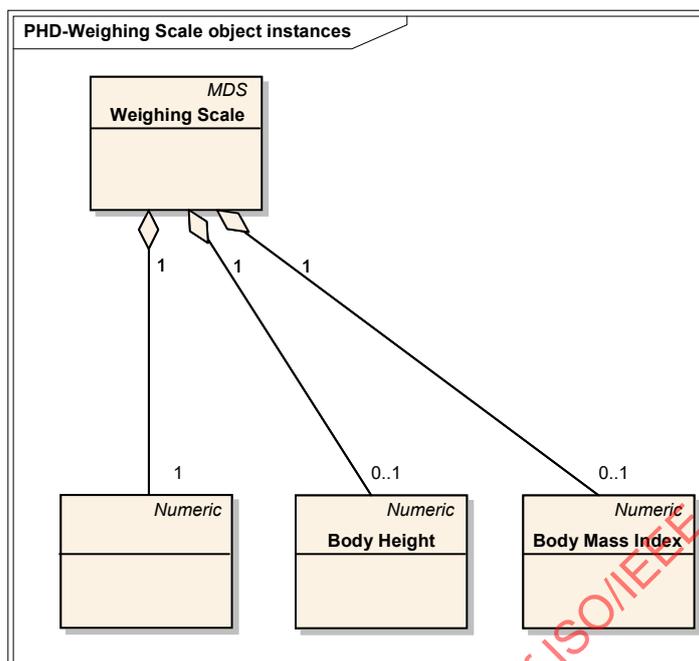


Figure 1—Weighing scale—domain information model

## 6.4 Types of configuration

### 6.4.1 General

As specified in IEEE Std 11073-20601, there are two styles of configuration available. Subclauses 6.4.2 and 6.4.3 briefly introduce standard and extended configurations.

### 6.4.2 Standard configuration

Standard configurations are defined in the IEEE 11073-104zz specializations (such as this standard) and are assigned a well-known identifier (Dev-Configuration-Id). The usage of a standard configuration is negotiated at association time between the agent and the manager. If the manager acknowledges that it recognizes and wants to operate using the configuration, then the agent can send measurements immediately. If the manager does not understand the configuration, the agent provides the configuration prior to transmitting measurement information.

### 6.4.3 Extended configuration

In extended configurations, the configuration of the agent is not predefined in a standard. The agent determines the objects, attributes, and values that are used in a configuration and assigns a configuration identifier. When the agent associates with a manager, it negotiates an acceptable configuration. Typically, the manager does not recognize the configuration of the agent on the first connection, so the manager responds that the agent must send its configuration information as a configuration event report. If, however, the manager already recognizes the configuration, either because it was preloaded in some way or the agent had previously associated with the manager, then the manager responds that the configuration is known and no further configuration information needs to be sent.

6.5 Medical device system object

6.5.1 MDS object attributes

Table 1 summarizes the attributes of the weighing scale MDS object. The nomenclature code to identify the MDS class is MDC\_MOC\_VMS\_MDS\_SIMP.

Table 1—MDS object attributes

Attribute name	Value	Qualifier		
		Extended configuration	Standard configuration (Dev-Configuration-Id = 0x05DC)	Standard configuration (Dev-Configuration-Id = 0x05DD)
Handle	0	M	M	M
System-Type	Attribute not present. See IEEE Std 11073-20601.	C	C	C
System-Model	{“Manufacturer”, “Model”}.	M	M	M
System-Id	Extended unique identifier (64 bits) (EUI-64).	M	M	M
Dev-Configuration-Id	Standard config: 0x05DC (1500) Standard config: 0x05DD (1501). Extended configs: 0x4000–0x7FFF.	M	M	M
Attribute-Value-Map	See IEEE Std 11073-20601.	C	C	C
Production-Specification	See IEEE Std 11073-20601.	O	O	O
Mds-Time-Info	See IEEE Std 11073-20601.	C	C	M
Date-and-Time	See IEEE Std 11073-20601.	C	M	NA
Base-Offset-Time	See IEEE Std 11073-20601.	R	NA	M
Relative-Time	See IEEE Std 11073-20601.	C	NR	NR
HiRes-Relative-Time	See IEEE Std 11073-20601.	C	NR	NR
Date-and-Time-Adjustment	See IEEE Std 11073-20601.	C	C	C
Power-Status	<i>onBattery</i> or <i>onMains</i> .	R	R	R
Battery-Level	See IEEE Std 11073-20601.	R	R	R
Remaining-Battery-Time	See IEEE Std 11073-20601.	R	R	R
Reg-Cert-Data-List	See IEEE Std 11073-20601.	O	O	O
System-Type-Spec-List	{MDC_DEV_SPEC_PROFILE_SCALE, 2}.	M	M	M
Confirm-Timeout	See IEEE Std 11073-20601.	O	O	O

NOTE—See IEEE Std 11073-20601 for information on whether an attribute is static or dynamic.

If a standard configuration is chosen, the timestamp type of MDS shall be consistent with the timestamp type of the metric objects in that standard configuration.

In the response to a Get MDS object command, only implemented attributes and their corresponding values are returned.

See IEEE Std 11073-20601 for descriptive explanations of the individual attributes as well as for information on attribute ID and attribute type.

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

The Dev-Configuration-Id attribute holds a locally unique 16-bit identifier that identifies the device configuration. For a weighing scale agent with extended configuration, this identifier is chosen in the range of extended-config-start to extended-config-end (see IEEE Std 11073-20601) as shown in Table 1.

The agent sends the Dev-Configuration-Id during the Associating state (see 8.3) to identify its configuration for the duration of the association. If the manager already holds the configuration information relating to the Dev-Configuration-Id, it recognizes the Dev-Configuration-Id. Then the Configuring state (see 8.4) is skipped, and the agent and manager enter the Operating state. If the manager does not recognize the Dev-Configuration-Id, the agent and manager enter the Configuring state.

If an agent implements multiple IEEE 11073-104zz specializations, System-Type-Spec-List is a list of type/version pairs, each referencing the respective device specialization and version of that specialization.

### 6.5.2 MDS object methods

Table 2 defines the methods (actions) of the MDS object. These methods are invoked using the Action service. In Table 2, the Subservice type name column defines the name of the method; the Mode column defines whether the method is invoked as an unconfirmed action (i.e., roiv-cmip-action from IEEE Std 11073-20601) or a confirmed action (i.e., roiv-cmip-confirmed-action); the Subservice type (action-type) column defines the nomenclature code to use in the action-type field of an action request and response (see IEEE Std 11073-20601); the Parameters (action-info-args) column defines the associated ASN.1 data structure (see IEEE Std 11073-20601 for ASN.1 definitions) to use in the action message for the action-info-args field of the request; and the Results (action-info-args) column defines the structure to use in the action-info-args of the response.

**Table 2—MDS object methods**

Service	Subservice type name	Mode	Subservice type (action-type)	Parameters (action-info-args)	Results (action-info-args)
ACTION	Set-Time	Confirmed	MDC_ACT_SET_TIME	SetTimeInvoke	—
	Set-Base-Offset-Time	Confirmed	MDC_ACT_SET_BO_TIME	SetBOTimeInvoke	—

— **Set-Time:**

This method allows the manager to set a real-time clock in the agent with the absolute time. The agent indicates whether the Set-Time command is valid using the mds-time-capab-set-clock bit in the Mds-Time-Info attribute (see IEEE Std 11073-20601). Agents with an internal real-time clock (RTC) shall indicate this capability by also setting the mds-time-capab-real-time-clock bit in the Mds-Time-Info attribute.

The Set-Time method can be supported only if the Absolute-Time-Stamp attribute is supported.

— **Set-Base-Offset-Time:**

This method allows the manager to set a real-time clock in the agent with the base time and offset. The agent indicates whether the Set-Base-Offset-Time command is valid using the mds-time-capab-set-clock bit in the Mds-Time-Info attribute (see IEEE Std 11073-20601).

The Set-Base-Offset-Time method can be supported only if the Base-Offset-Time-Stamp attribute is supported.

Agents following only this device specialization and no others shall send event reports (see 6.5.3) using agent-initiated measurement data transmission. Agents following this device specialization as well as others shall send event reports in the appropriate fashion. During the association procedure (see 8.3), DataReqModeCapab shall be set to the appropriate value for the event report style. Implementation of the MDS-Data-Request method/action is not required in this standard and is not shown in Table 2.

6.5.3 MDS object events

Table 3 defines the events that can be sent by the weighing scale MDS object.

Table 3—Weighing scale MDS object events

Service	Subservice type name	Mode	Subservice type (event-type)	Parameters (event-info)	Results (event-reply-info)
EVENT REPORT	MDS-Configuration-Event	Confirmed	MDC_NOTI_CONFIG	ConfigReport	ConfigReportRsp
	MDS-Dynamic-Data-Update-Var	Confirmed	MDC_NOTI_SCAN_RE PORT_VAR	ScanReportInfoVar	—
	MDS-Dynamic-Data-Update-Fixed	Confirmed	MDC_NOTI_SCAN_RE PORT_FIXED	ScanReportInfoFixed	—
	MDS-Dynamic-Data-Update-MP-Var	Confirmed	MDC_NOTI_SCAN_RE PORT_MP_VAR	ScanReportInfoMPVar	—
	MDS-Dynamic-Data-Update-MP-Fixed	Confirmed	MDC_NOTI_SCAN_RE PORT_MP_FIXED	ScanReportInfoMPFixed	—

- **MDS-Configuration-Event:**  
 This event is sent by the weighing scale agent during the configuring procedure if the manager does not already know the configuration of the weighing scale agent from past associations or because the manager has not been implemented to recognize the configuration according to the weighing scale device specialization. The event provides static information about the supported measurement capabilities of the weighing scale agent.
- **MDS-Dynamic-Data-Update-Var:**  
 This event provides dynamic measurement data from the weighing scale agent for the body weight and optionally the body height and BMI numeric object(s). These data are reported using a generic attribute list variable format. The event is sent as an unsolicited message by the agent (i.e., an agent-initiated measurement data transmission). See 8.5.3 for more information on unsolicited event reporting.
- **MDS-Dynamic-Data-Update-Fixed:**  
 This event provides dynamic measurement data from the weighing scale agent for the body weight and optionally the body height and BMI numeric objects. These data are reported in the fixed format defined by the Attribute-Value-Map attribute of the object(s). The event is sent as an unsolicited message by the agent (i.e., an agent-initiated measurement data transmission). See 8.5.3 for more information on unsolicited event reporting.
- **MDS-Dynamic-Data-Update-MP-Var:**  
 This is the same as MDS-Dynamic-Data-Update-Var but allows inclusion of data from multiple people.
- **MDS-Dynamic-Data-Update-MP-Fixed:**  
 This is the same as MDS-Dynamic-Data-Update-Fixed but allows inclusion of data from multiple people.

NOTE— IEEE Std 11073-20601 requires that managers support all of the MDS object events listed above.

## 6.5.4 Other MDS services

### 6.5.4.1 GET service

A weighing scale agent shall support the GET service, which is provided by the MDS object to retrieve the values of all implemented MDS object attributes. The GET service can be invoked only after the manager has confirmed selection of the configuration of the agent.

The manager may request the MDS object attributes of the weighing scale agent; in which case, the manager shall send the “Remote Operation Invoke | Get” message (see roiv-cmip-get in IEEE Std 11073-20601) with the reserved MDS handle value of 0. The weighing scale agent shall report its MDS object attributes to the manager using the “Remote Operation Response | Get” message (see rors-cmip-get in IEEE Std 11073-20601). See Table 4 for a summary of the GET service including some message fields.

**Table 4—Weighing scale MDS object GET service**

Service	Subservice type name	Mode	Subservice type	Parameters	Results
GET	<na>	<implied confirmed>	<na>	GetArgumentSimple = (obj-handle = 0), attribute-id-list <optional>	GetResultSimple = (obj-handle = 0), attribute-list

See 8.5.2 for details on the procedure for getting the MDS object attributes.

### 6.5.4.2 SET service

The weighing scale specialization does not require an implementation to support the MDS object SET service.

## 6.6 Numeric objects

### 6.6.1 General

The weighing scale DIM (see Figure 1) contains one required numeric object for body weight and two optional numeric objects for body height and body mass index. These are described in 6.6.2 to 6.6.4.

Sometimes, the interpretation of one attribute value in an object depends on other attribute values in the same object. For example, Unit-Code and Unit-LabelString provide context for the observed values. Whenever a contextual attribute changes, the agent shall report these changes to the manager using an MDS object event (see 6.5.3) prior to reporting any of the dependent values.

### 6.6.2 Body weight

Table 5 summarizes the attributes of the body weight numeric object. The nomenclature code to identify the numeric class is MDC\_MOC\_VMO\_METRIC\_NU. The body weight numeric object shall be supported by a weighing scale agent.

Table 5—Body weight numeric object attributes

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x05DC)		Standard configuration (Dev-Configuration-Id = 0x05DD)	
	Value	Qual.	Value	Qual.	Value	Qual.
Handle	See IEEE Std 11073-20601.	M	1	M	1	M
Type	MDC_PART_SCADA   MDC_MASS_BODY_ACTUAL.	M	MDC_PART_SCADA   MDC_MASS_BODY_ACTUAL.	M	MDC_PART_SCADA   MDC_MASS_BODY_ACTUAL.	M
Supplemental-Types	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Metric-Spec-Small	mss-avail-intermittent   mss-avail- stored-data   mss-upd-aperiodic   mss-msmt-aperiodic   mss-acc- agent-initiated.	M	mss-avail-intermittent   mss-avail- stored-data   mss-upd-aperiodic   mss- msmt-aperiodic   mss-acc-agent- initiated.	M	mss-avail-intermittent   mss-avail- stored-data   mss-upd-aperiodic   mss- msmt-aperiodic   mss-acc-agent- initiated.	M
Metric-Structure-Small	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Measurement-Status	See IEEE Std 11073-20601.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601.	O
Metric-Id	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Metric-Id-List	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Unit-Code	MDC_DIM_KILO_G or MDC_DIM_LB.	M	MDC_DIM_KILO_G.	M	MDC_DIM_KILO_G.	M
Attribute-Value-Map	See IEEE Std 11073-20601.	C	MDC_ATTR_NU_VAL_OBS_SIMP, then MDC_ATTR_TIME_STAMP_ABS.	M	MDC_ATTR_NU_VAL_OBS_SIMP, then MDC_ATTR_TIME_STAMP_BO.	M
Source-Handle-Reference	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Label-String	See IEEE Std 11073-20601.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601.	O
Unit-LabelString	See IEEE Std 11073-20601.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601.	O	Attribute not initially present. If present, follow IEEE Std 11073-20601.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601.	C	See IEEE Std 11073-20601.	M	Attribute not allowed.	NA
Base-Offset-Time-Stamp	See IEEE Std 11073-20601.	R	Attribute not allowed.	NA	See IEEE Std 11073-20601.	M

Table 5—Body weight numeric object attributes (continued)

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x05DC)		Standard configuration (Dev-Configuration-Id = 0x05DD)	
	Value	Qual.	Value	Qual.	Value	Qual.
Relative-Time-Stamp	See IEEE Std 11073-20601.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Measure-Active-Period	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Simple-Nu-Observed-Value	See IEEE Std 11073-20601.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601 apply.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601. If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601 apply.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Basic-Nu-Observed-Value	See IEEE Std 11073-20601.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601.	C
Compound-Basic-Nu-Observed-Value	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Compound-Nu-Observed-Value	See IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601.	NR
Accuracy	See IEEE Std 11073-20601.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601.	R

NOTE—See IEEE Std 11073-20601 for information on whether an attribute is static or dynamic.

IEEE Std 11073-10415-2019  
 Health Informatics—Personal health device communication  
 Part 10415: Device specialization—Weighing scale

For a weighing scale agent with standard configuration, the AttrValMap structure (see IEEE Std 11073-20601) of the Attribute-Value-Map attribute shall contain the attribute ID and attribute length information of the Simple-Nu-Observed-Value and Absolute-Time-Stamp (or Base-Offset-Time-Stamp) attribute in the same order as indicated in Table 5.

The body weight numeric object does not support any methods, events, or other services.

See IEEE Std 11073-20601 for descriptive explanations on the individual attributes as well as information on attribute ID and attribute type.

**6.6.3 Body height**

Table 6 summarizes the attributes of the body height numeric object. The nomenclature code to identify the numeric class is MDC\_MOC\_VMO\_METRIC\_NU. The body height numeric object may be supported by a weighing scale agent with extended configuration. If the body mass index numeric object is supported, the body height numeric object shall be present. It shall not be present in the standard configuration.

**Table 6—Body height numeric object attributes**

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601.	M
Type	MDC_PART_SCADA   MDC_LEN_BODY_ACTUAL.	M
Supplemental-Types	See IEEE Std 11073-20601.	NR
Metric-Spec-Small	mss-avail-intermittent   mss-avail-stored-data   mss-upd-aperiodic   mss-msmt-aperiodic   mss-acc-agent-initiated   mss-cat-manual.	M
Metric-Structure-Small	See IEEE Std 11073-20601.	NR
Measurement-Status	See IEEE Std 11073-20601.	R
Metric-Id	See IEEE Std 11073-20601.	NR
Metric-Id-List	See IEEE Std 11073-20601.	NR
Metric-Id-Partition	See IEEE Std 11073-20601.	NR
Unit-Code	MDC_DIM_CENTI_M, or MDC_DIM_INCH.	M
Attribute-Value-Map	See IEEE Std 11073-20601.	C
Source-Handle-Reference	See IEEE Std 11073-20601.	NR
Label-String	See IEEE Std 11073-20601.	O
Unit-LabelString	See IEEE Std 11073-20601.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601.	R
Relative-Time-Stamp	See IEEE Std 11073-20601.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601.	NR
Measure-Active-Period	See IEEE Std 11073-20601.	NR
Simple-Nu-Observed-Value	See IEEE Std 11073-20601.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601.	NR
Basic-Nu-Observed-Value	See IEEE Std 11073-20601.	C
Compound-Basic-Nu-Observed-Value	See IEEE Std 11073-20601.	NR
Compound-Nu-Observed-Value	See IEEE Std 11073-20601.	NR
Accuracy	See IEEE Std 11073-20601.	R

NOTE—See IEEE Std 11073-20601 for information on whether an attribute is static or dynamic.

The body height numeric object does not support any methods, events, or other services.

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

See IEEE Std 11073-20601 for descriptive explanations on the individual attributes as well as for information on attribute ID and attribute type.

#### 6.6.4 Body mass index

Table 7 summarizes the attributes of the body mass index numeric object. The nomenclature code to identify the numeric class is MDC\_MOC\_VMO\_METRIC\_NU. The body mass index numeric object may be supported by a weighing scale agent with extended configuration and shall not be present in the standard configuration.

**Table 7—Body mass index numeric object attributes**

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601.	M
Type	MDC_PART_SCADA   MDC_RATIO_MASS_BODY_LEN SQ.	M
Supplemental-Types	See IEEE Std 11073-20601.	NR
Metric-Spec-Small	mss-avail-intermittent   mss-avail-stored-data   mss-upd-aperiodic   mss-msmt-aperiodic   mss-acc-agent-initiated   mss-cat-calculation.	M
Metric-Structure-Small	See IEEE Std 11073-20601.	NR
Measurement-Status	See IEEE Std 11073-20601.	R
Metric-Id	See IEEE Std 11073-20601.	NR
Metric-Id-List	See IEEE Std 11073-20601.	NR
Metric-Id-Partition	See IEEE Std 11073-20601.	NR
Unit-Code	MDC_DIM_KILO_G_PER_M SQ.	M
Attribute-Value-Map	See IEEE Std 11073-20601.	C
Source-Handle-Reference	This attribute shall not be present if Source-Handle-Reference-List is present. If present, the value of this attribute shall be set to the Handle value of the associated body weight object.  This attribute shall be present if the manager-selected version of protocol doesn't support the Source-Handle-Reference-List. See IEEE Std 11073-20601.	C
Source-Handle-Reference-List	The value of this attribute shall be set to the Handle values of the associated body weight object and body height object. If this attribute is used, the Source-Handle-Reference shall not be present. See IEEE Std 11073-20601.	R
Label-String	See IEEE Std 11073-20601.	O
Unit-LabelString	See IEEE Std 11073-20601.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601.	R
Relative-Time-Stamp	See IEEE Std 11073-20601.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601.	NR
Measure-Active-Period	See IEEE Std 11073-20601.	NR
Simple-Nu-Observed-Value	See IEEE Std 11073-20601.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601.	NR
Basic-Nu-Observed-Value	See IEEE Std 11073-20601.	C
Compound-Basic-Nu-Observed-Value	See IEEE Std 11073-20601.	NR
Compound-Nu-Observed-Value	See IEEE Std 11073-20601.	NR
Accuracy	See IEEE Std 11073-20601.	R

NOTE—See IEEE Std 11073-20601 for information on whether an attribute is static or dynamic.

The body mass index numeric object does not support any methods, events, or other services.

See IEEE Std 11073-20601 for descriptive explanations on the individual attributes as well as for information on attribute ID and attribute type.

### 6.7 Real-time sample array objects

Real-time sample array objects are not required by this standard.

### 6.8 Enumeration objects

Enumeration objects are not required by this standard.

### 6.9 PM-store objects

PM-store objects are not required by this standard.

### 6.10 Scanner objects

Scanner objects are not required by this standard.

### 6.11 Class extension objects

In this standard, no class extension objects are defined with respect to IEEE Std 11073-20601.

### 6.12 Weighing scale information model extensibility rules

The weighing scale domain information model of this standard may be extended by including vendor-specific metrics and attributes as required. For example, a vendor might include a body fat measurement in addition to the body weight measurement. Any object or attribute extensions implemented should follow the guidelines of this standard as closely as possible. Such vendor-specific attributes shall be identified by assigning nomenclature codes from the private numbering space (0xF000–0xFFFF) within the corresponding partition as defined in IEEE Std 11073-20601.

A weighing scale agent having a configuration with extensions beyond the standard configuration, as specified in this standard, shall use a configuration ID in the range of IDs reserved for extended configurations (see IEEE Std 11073-20601).

## 7. Weighing scale service model

### 7.1 General

The service model defines the conceptual mechanisms for data exchange services. These services are mapped to messages that are exchanged between the agent and the manager. Protocol messages within the ISO/IEEE 11073 series of standards are defined in ASN.1. See IEEE Std 11073-20601 for a detailed description of the personal health device service model. Subclauses 7.2 and 7.3 define the specifics of object access and event reporting services for a weighing scale agent according to this standard.

### 7.2 Object access services

The object access services of IEEE Std 11073-20601 are used to access the objects defined in the domain information model of the weighing scale.

- GET service: used by the manager to retrieve the values of the agent MDS object attributes. The list of weighing scale MDS object attributes is given in 6.5.4.1.
- SET service: used by the manager to set the values of the agent object attributes. There are no settable attributes defined for a weighing scale agent according to this standard.
- Event report service: used by the agent to send configuration reports and measurement data to the manager. The list of event reports for the weighing scale device specialization is given in 6.5.3.
- Action service: used by the manager to invoke actions (or methods) supported by the agent. An example is Set-Time action, which is used to set a real-time clock with the absolute time at the agent.

Table 8 summarizes the object access services described in this standard.

Table 8—Weighing scale object access services

Service	Subservice type name	Mode	Subservice Type	Parameters	Result	Remarks
GET	<na>	<implied Confirmed >	<na>	GetArgumentSimple = (obj-handle = 0), attribute-id-list <optional>	GetResultSimple = (obj-handle = 0), attribute-list	Allows the manager to retrieve the value of an attribute of an object in the agent.
EVENT REPORT	MDS-Configuration-Event	Confirmed	MDC_NOTI_CONFIG	ConfigReport	ConfigReportRsp	Configuration Report to inform manager of the configuration of the agent.
	MDS-Scan-Report-Var	Confirmed	MDC_NOTI_SCAN_REPORT_VAR	ScanReportInfoVar	—	Data Report to provide dynamic data to manager for some or all of the agent's objects in variable format.
	MDS-Scan-Report-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_FIXED	ScanReportInfoFixed	—	Data Report to provide dynamic data to manager for some or all of the agent's objects in fixed format.
	MDS-Scan-Report-MP-Var	Confirmed	MDC_NOTI_SCAN_REPORT_MP_VAR	ScanReportInfoMPVar	—	This is the same as MDS-Dynamic-Data-Update-Var but allows inclusion of data from multiple people.
	MDS-Scan-Report-MP-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_MP_FIXED	ScanReportInfoMPFixed	—	This is the same as MDS-Dynamic-Data-Update-Fixed but allows inclusion of data from multiple people.
ACTION	Set-Time	Confirmed	MDC_ACT_SET_TIME	SetTimeInvoke	—	Manager method to invoke the agent to set time to requested value.
	Set-Base-Offset-Time	Confirmed	MDC_ACT_SET_BO_TIME	SetBOTimeInvoke	—	Manager method to invoke the agent to set time to requested value.

STANDARDSISO.COM Click to view the full PDF of ISO/IEEE 11073-10415:2022

### 7.3 Object access event report services

The event report service (see Table 8) is used by the agent to report its information (e.g., measurements). Event reports in this standard are a property of the MDS object only. The event reports used in this standard are defined in IEEE Std 11073-20601.

The following conditions apply for a weighing scale agent according to this standard:

- Event reports shall be used in confirmed mode.
- Agent-initiated mode shall be supported for measurement data transmission.

A weighing scale agent, which is designed to operate in an environment where data may be collected from multiple people, may use one of the multiple-person event report styles to transmit all the data from each person in a single event. If this functionality is not required, the agent may use the single-person event report styles, which have reduced overhead.

A manager shall support both single-person and multiple-person event reports. A weighing scale agent may support either one or both single-person and multiple-person event reports. The formats for single- and multiple-person reports are described in IEEE Std 11073-20601.

## 8. Weighing scale communication model

### 8.1 Overview

This clause describes the general communication model and procedures of the weighing scale agent as defined in IEEE Std 11073-20601. Therefore, the respective parts of IEEE Std 11073-20601 are not reproduced; rather the specific choices and restrictions with respect to optional elements (e.g., objects, attributes, and actions) and specific extensions (e.g., nomenclature terms) are specified.

For an illustrative overview of the various message transactions during a typical measurement session, see the sequence diagram for the example use case in Annex D and the corresponding PDU examples in Annex E.

### 8.2 Communications characteristics

In this subclause, limits on the size of an application protocol data unit (APDU) transmitted or to be received by a weighing scale agent are defined. Small limits allow for simple implementations in terms of low cost and complexity.

For a weighing scale agent implementing no other device specialization except this standard, the maximum size of an APDU sent shall be not larger than  $N_{tx}$ . For this standard, it is  $N_{tx} = 896$  octets. An agent according to this definition shall be capable of receiving an APDU up to the size of at least  $N_{rx}$ . For this standard, it is  $N_{rx} = 224$  octets.

For a weighing scale agent implementing multiple functions according to multiple device specializations, the maximum size of an APDU sent shall not be larger than  $N_{tx,i}$ , if this agent implements another device specialization  $i$  with  $N_{tx,i} > N_{tx}$ . Otherwise, the maximum size of an APDU sent shall not be larger than  $N_{tx}$ . An agent according to this definition shall be capable of receiving an APDU up to the size of at least  $N_{rx,i}$  octets if this agent implements another device specialization  $i$  with  $N_{rx,i} > N_{rx}$ . Otherwise, the agent shall be capable of receiving an APDU up to the size of at least  $N_{rx}$ .

In case the APDU size limit does not allow all pending measurements at the agent to be included in a single event report, they shall be sent using multiple event reports. See 8.5.3 for the maximum number of measurements allowed for inclusion in a single event report.

**8.3 Association procedure**

**8.3.1 General**

Unless otherwise stated, the association procedure for a weighing scale agent and manager according to this standard shall be pursued as specified in IEEE Std 11073-20601.

Table 9 lists the valid combinations of protocol version and nomenclature version. In the association procedure, an agent indicating support to a specific protocol version shall indicate support to the corresponding nomenclature version as well. In the association procedure, a manager selecting a specific protocol version shall select the corresponding nomenclature version.

To indicate support for multiple protocol versions, the bit values are combined. For example, if the agent supports protocol-version2, protocol-version3 and protocol-version4, it shall use protocol version bits 0x70000000 and nomenclature-version bits 0xE0000000.

Further valid combinations from future versions of this specification may be used by implementations that comply with those future versions.

**Table 9—Valid combinations of protocol and nomenclature version**

Protocol version	Bit value	Corresponding nomenclature version	Bit value
1	0x80000000	1	0x80000000
2	0x40000000	1	0x80000000
3	0x20000000	2	0x40000000
4	0x10000000	3	0x20000000

**8.3.2 Agent procedure—association request**

In the association request sent by the agent to the manager:

- a) The version of the association procedure used by the agent shall be set to assoc-version1 (i.e., *assoc-version* = 0x80000000).
- b) The DataProtoList structure element of the data protocol identifier shall be set to data-proto-id-20601 (i.e., *data-proto-id* = 0x5079).
- c) The *data-proto-info* field shall contain a PhdAssociationInformation structure that shall contain the following parameter values:
  - 1) The version of the data exchange protocol shall be set to protocol-version4 (i.e., *protocol-version* = 0x10000000). Support for any other version may be indicated by setting additional bits. When protocols lower than protocol-version4 are used, the agent shall use only features in that protocol.
  - 2) At least the MDER shall be supported (i.e., *encoding-rules* = 0x8000).
  - 3) The protocol version bits and nomenclature version bits shall consist of valid combinations of bits as defined in Table 9.
  - 4) The field *functional-units* may have the test association bits set but shall not have any other bits set.

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

- 5) The field *system-type* shall be set to *sys-type-agent* (i.e., *system-type* = 0x00800000).
- 6) The *system-id* field shall be set to the value of the System-Id attribute of the MDS object of the agent. The manager may use this field to determine the identity of the weighing scale with which it is associating and, optionally, to implement a simple access restriction policy.
- 7) The *dev-config-id* field shall be set to the value of the Dev-Configuration-Id attribute of the MDS object of the agent.
- 8) If the agent supports only the weighing scale specialization, then the field indicating the data request modes (*data-req-mode-capab*) supported by the weighing scale agent shall be set to *data-req-supp-init-agent*.
- 9) If the agent supports only the weighing scale specialization, then the *data-req-init-manager-count* field shall be set to 0, and the *data-req-init-agent-count* field shall be set to 1.

### 8.3.3 Manager procedure—association response

In the association response message sent by the manager:

- a) The *result* field shall be set to an appropriate response from those defined in IEEE Std 11073-20601. For example, if all other conditions of the association protocol are satisfied, *accepted* is returned when the manager recognizes the *dev-config-id* of the agent and *accepted-unknown-config* otherwise.
- b) In the DataProtoList structure element, the data protocol identifier shall be set to *data-proto-id-20601* (i.e., *data-proto-id* = 0x5079).
- c) The *data-proto-info* field shall be filled in with a PhdAssociationInformation structure that shall contain the following parameter values:
  - 1) The manager following this specialization shall support *protocol-version4*. The manager may support additional protocol versions and select them if the agent offers them. When protocols lower than *protocol-version4* are used, the manager shall use only features in that protocol.
  - 2) The manager shall respond with a single selected encoding rule that is supported by both agent and manager. The manager shall support at least the MDER.
  - 3) The manager shall select a valid combination of protocol version and nomenclature version as defined in Table 9.
  - 4) The field *functional-units* shall have all bits reset except for those relating to a test association.
  - 5) The field *system-type* shall be set to *sys-type-manager* (i.e., *system-type* = 0x80000000).
  - 6) The *system-id* field shall contain the unique system ID of the manager device, which shall be a valid EUI-64 type identifier.
  - 7) The field *dev-config-id* shall be *manager-config-response* (0).
  - 8) The field *data-req-mode-capab* shall be 0.
  - 9) The field *data-req-init-\*-count* shall be 0.

**8.4 Configuring procedure**

**8.4.1 General**

The agent enters the Configuring state if it receives an association response of accepted-unknown-config. In this case, the configuration procedure as specified in IEEE Std 11073-20601 shall be followed. Subclause 8.4.2 specifies the configuration notification and response messages for a weighing scale agent with standard configuration ID 0x05DD. Normally, a manager would already know the standard configuration. However, standard configuration devices are required to send their configuration, if requested. This covers a case where an agent associates with a manager that does not have preconfigured knowledge of the standard configuration (e.g., due to a version mismatch between agent and manager).

**8.4.2 Weighing scale—standard configuration**

**8.4.2.1 Agent procedure**

The agent performs the configuration procedure using a “Remote Operation Invoke | Confirmed Event Report” message with an MDC\_NOTI\_CONFIG event to send its configuration to the manager (see IEEE Std 11073-20601). The ConfigReport structure is used for the *event-info* field (see Table 3). For a weighing scale agent with standard configuration ID 0x05DD, the format and contents of the configuration notification message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x44	CHOICE.length = 68
0x00 0x42	OCTET STRING.length = 66
0xXX 0xXX	invoke-id (differentiates this message from any other outstanding)
0x01 0x01	CHOICE (Remote Operation Invoke   Confirmed Event Report)
0x00 0x3C	CHOICE.length = 60
0x00 0x00	obj-handle = 0 (MDS object)
0xXX 0xXX 0xXX 0xXX	event-time (set to 0xFFFFFFFF if RelativeTime is not supported)
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x32	event-info.length = 50 (start of ConfigReport)
0x05 0xDD	config-report-id (Dev-Configuration-Id value=1501)
0x00 0x01	config-obj-list.count = 1 Measurement object will be “announced”
0x00 0x2C	config-obj-list.length = 44
0x00 0x06	obj-class = MDC_MOC_VMO_METRIC_NU
0x00 0x01	obj-handle = 1 (→ 1 <sup>st</sup> Measurement is body weight)
0x00 0x04	attributes.count = 4
0x00 0x24	attributes.length = 36
0x09 0x2F	attribute-id = MDC_ATTR_ID_TYPE
0x00 0x04	attribute-value.length = 4
0x00 0x02 0xE1 0x40	MDC_PART_SCADA   MDC_MASS_BODY_ACTUAL
0x0A 0x46	attribute-id = MDC_ATTR_METRIC_SPEC_SMALL
0x00 0x02	attribute-value.length = 2
0xF0 0x40	intermittent, stored data, upd & msmt aperiodic, agent init, measured
0x09 0x96	attribute-id = MDC_ATTR_UNIT_CODE
0x00 0x02	attribute-value.length = 2
0x06 0xC3	MDC_DIM_KILO_G
0x0A 0x55	attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00 0x0C	attribute-value.length = 12
0x00 0x02	AttrValMap.count = 2

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

0x00 0x08	AttrValMap.length = 8
0x0A 0x56 0x00 0x04	MDC_ATTR_NU_VAL_OBS_SIMP   value length = 4
0x0A 0x82 0x00 0x08	MDC_ATTR_TIME_STAMP_BO   value length = 8

Note, at the locations of the message, where the content is not fixed, the value “0xXX” denotes a placeholder and depends on the implementation or on the preceding messaging of the agent.

#### 8.4.2.2 Manager procedure

The manager shall respond to a configuration notification message using a “Remote Operation Response Confirmed Event Report” data message with an MDC\_NOTI\_CONFIG event using the ConfigReportRsp structure for the *event-info* field (see Table 3). As a response to the standard configuration notification message in 8.4.2.1, the format and contents of the manager’s configuration notification response message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x16	CHOICE.length = 22
0x00 0x14	OCTET STRING.length = 20
0xXX 0xXX	invoke-id (differentiates this message from any other outstanding)
0x02 0x01	CHOICE (Remote Operation Response   Confirmed Event Report)
0x00 0x0E	CHOICE.length = 14
0x00 0x00	obj-handle = 0 (MDS object)
0xXX 0xXX 0xXX 0xXX	currentTime
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x04	event-reply-info.length = 4
0x05 0xDD	ConfigReportRsp.config-report-id = 0x05DD
0x00 0x00	ConfigReportRsp.config-result = accepted-config.

Again, the value “0xXX” denotes a placeholder and refers to a fixed location, varying content parts of the message.

## 8.5 Operating procedure

### 8.5.1 General

Measurement data and status information are communicated from the weighing scale agent during the Operating state. If not stated otherwise, the operating procedure for a weighing scale agent of this standard shall be as specified in IEEE Std 11073-20601.

### 8.5.2 GET weighing scale MDS attributes

See Table 4 for a summary of the GET service.

If the manager leaves the attribute-id-list field in the roiv-cmip-get service message empty, the weighing scale agent shall respond with a rors-cmip-get service message in which the attribute-list contains a list with the values of all implemented attributes of the MDS object.

If the manager requests specific MDS object attributes, indicated by the elements in attribute-id-list, then the weighing scale agent shall respond with a rors-cmip-get service message in which the attribute-list contains a list of the values of the requested attributes of the MDS object that are implemented.

### 8.5.3 Measurement data transmission

See Table 3 for a summary of the event report services available for measurement data transfer.

Measurement data transfer for a weighing scale agent of this standard shall always be initiated by the weighing scale (see agent-initiated measurement data transmission in IEEE Std 11073-20601). To limit the amount of data being transported within an APDU, the weighing scale agent shall not include more than 25 temporarily stored measurements in a single event report. If more than 25 pending measurements are available for transmission, they shall be sent using multiple event reports. If multiple measurements are available, up to 25 measurements should be transmitted within a single event report. Alternatively, they may be transmitted using a single event report for each measurement. However, the former strategy is recommended to reduce overall message size and power consumption.

### 8.6 Time synchronization

Time synchronization between a weighing scale agent and a manager may be used to coordinate the clocks used when reporting physiological events. Note that the mechanism for synchronizing an agent to a manager is outside the scope of this standard. If time synchronization is used, then this shall be reported in the Mds-Time-Info attribute of the MDS object.

## 9. Test associations

### 9.1 General

A weighing scale may implement a wide range of behaviors in a test association that enable a manufacturer to test features of a product in a comprehensive manner. It is also possible for a weighing scale to not support test associations at all. This clause defines a simple behavior that simulates the generation of a measurement in the context of a standard device configuration.

### 9.2 Behavior with standard configuration

In order to facilitate automated standardized test processes, a weighing scale that presents the standard configuration ID and enters into a test association should be able to simulate the arrival of measurement data from the device sensors. It should not be necessary for an operator to stimulate the sensors in order for the measurement data to be generated.

After the agent enters the Operating state, it simulates the reception of an event from the sensors representing a body weight measurement of 55 kg. To the extent possible, this measurement is seen only by those components of the agent that understand the test association. When the event is propagated into a numeric object, the test-data bit of the measurement-status attribute shall be set if the measurement-status attribute is supported. An agent is not required to use the measurement-status attribute if it would not normally do so outside of a test association. If body height is supported, it shall be simulated as 172 cm.

The agent should send the events reports for all simulated measures within 30 s of entering the Operating state. The test association is terminated in a manner consistent with the agent's normal behavior for terminating an association.

### 9.3 Behavior with extended configurations

This specification does not define a test association that uses an extended configuration.

## 10. Conformance

### 10.1 Applicability

This standard shall be used in conjunction with IEEE Std 11073-20601.

An implementation or a system can conform to the following elements of this standard:

- Domain information model class hierarchy and object definitions (object attributes, notifications, methods, and data type definitions)
- Nomenclature code values
- Protocol and service models
- Communication service model (association and configuration)

### 10.2 Conformance specification

This standard offers levels of conformance with respect to strict adherence to the standard device and the use of extensions for the following:

- Information model of a specific device
- Use of attributes, value ranges, and access methods

A vendor shall specify the level of conformance for an implementation based on this standard and provide details of the way in which the definitions of this standard and any extensions are applied.

Specifications shall be provided in the form of a set of implementation conformance statements (ICSs) as detailed in 10.4.

Since this standard is used in conjunction with IEEE Std 11073-20601, the ICS should be created for this standard first. The ICS created for IEEE Std 11073-20601 may then refer to the ICS for this standard where applicable.

### 10.3 Levels of conformance

#### 10.3.1 General

This standard defines the following levels of conformance.

#### 10.3.2 Conformance level 1: Base conformance

The application uses elements of the information, service, and communication models (object hierarchy, actions, event reports, and data type definitions) and the nomenclature scheme defined in IEEE Std 11073-20601 and IEEE Std 11073-104zz. All mandatory features defined in the object definition tables and in the ICS tables are implemented. Furthermore, any conditional, recommended, or optional features that are implemented shall follow the requirements in IEEE Std 11073-20601 and IEEE Std 11073-104zz.

**10.3.3 Conformance level 2: Extended nomenclature (ASN.1 and/or IEEE Std 11073-10101)**

Conformance level 2 meets conformance level 1 but also uses or adds extensions in at least one of the information, service, communication, or nomenclature models. These extensions shall conform to nomenclature codes from ASN.1 and/or within the IEEE 11073-10101 framework (0xF000–0xFFFF). These extensions should be defined in ICS tables pointing towards their reference.

**10.4 Implementation conformance statements**

**10.4.1 General format**

The ICSs are provided as an overall conformance statement document that comprises a set of tables in the form given by the templates in the following clauses.

Each ICS table has the following columns:

Index	Feature	Reference	Req/Status	Support	Comment
-------	---------	-----------	------------	---------	---------

The table column headings have the following meaning:


- Index: an identifier (e.g., a tag) of a specific feature.
- Feature: briefly describes the characteristic for which a conformance statement is being made.
- Reference: to the clause/paragraph within this document or an external source for the definition of the feature (may be empty).
- Req/Status: specifies the conformance requirement (e.g., mandatory or recommended)—in some cases, this standard does not specify conformance requirements but requests the status of a particular feature be provided.
- Support: specifies the presence or absence of a feature and any description of the characteristics of the feature in the implementation. This column is to be filled out by the implementer.
- Comment: contains any additional information on the feature. This column is to be filled out by the implementer.

Subclauses 10.4.2 to 10.4.6 specify the format of the specific ICS tables.

**10.4.2 General implementation conformance statement**

The general ICS specifies the versions/revisions that are supported by the implementation and high-level system behavior.

Table 10 shows the general ICSs.

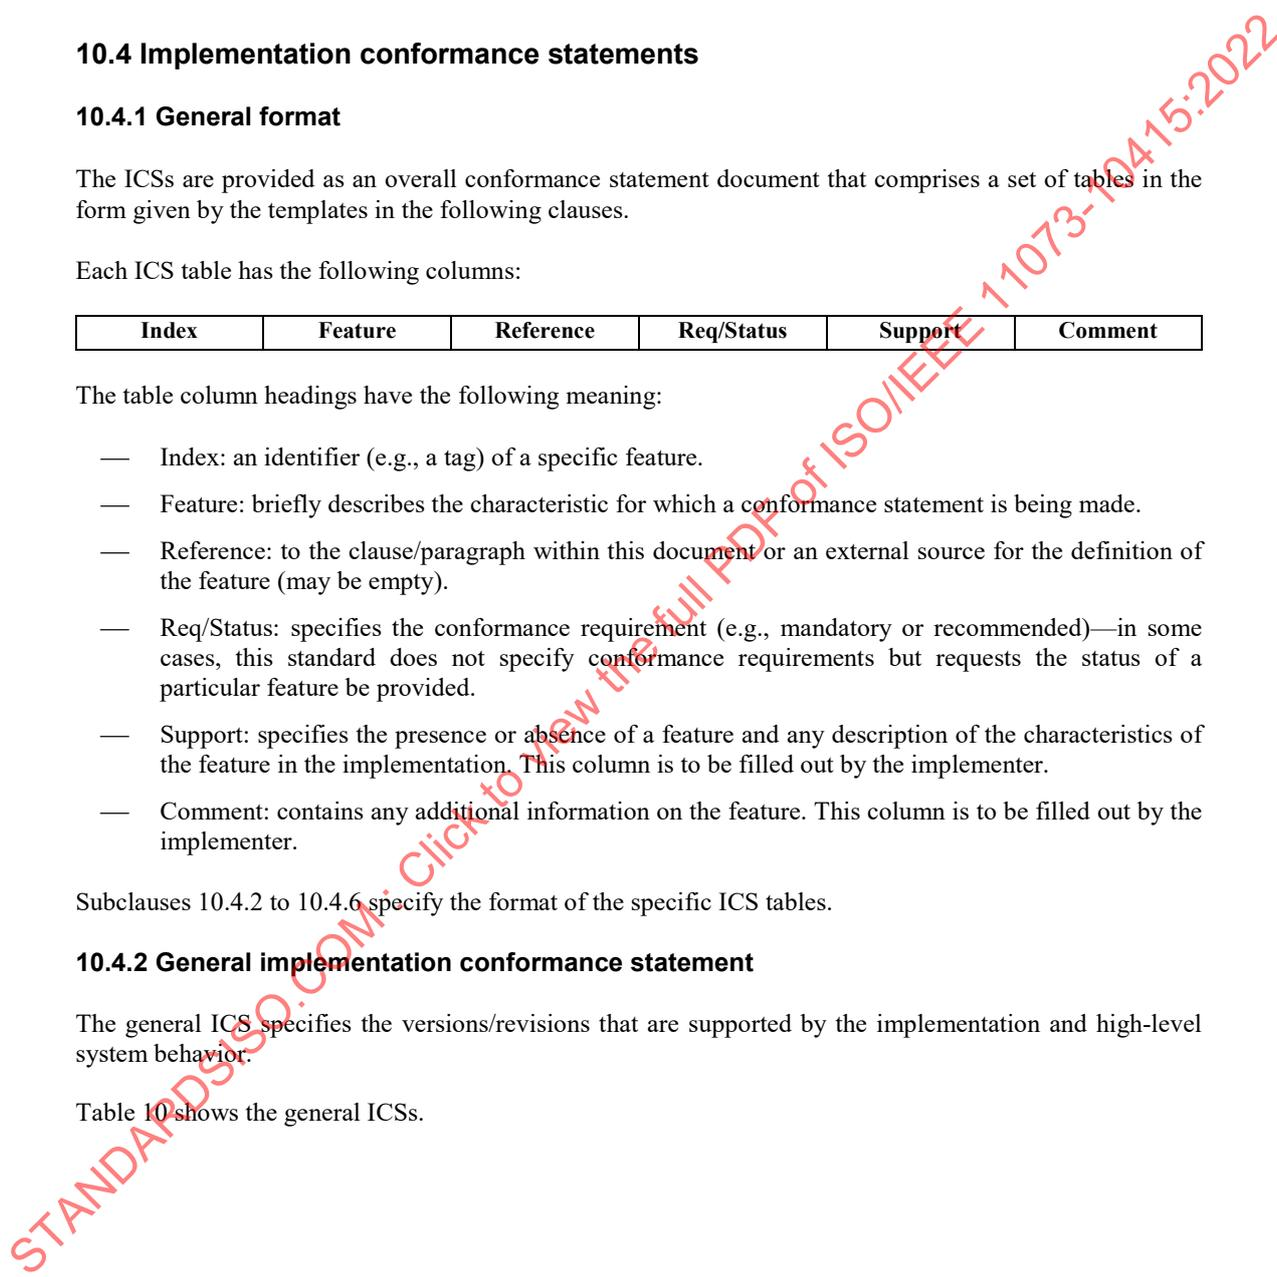

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

Table 10—IEEE 11073-10415 general ICSs table

Index <sup>a</sup>	Feature	Reference	Req./Status	Support	Comment
GEN11073-10415-1	Implementation Description	—	Identification of the device/application. Description of functionality.		
GEN11073-10415-2	Standards followed and their revisions	(standard documents)	(set of existing revisions)	(set of supported revision)	
GEN11073-10415-3	Nomenclature document used and revision	(standard documents)	(set of existing revisions)	(set of supported revisions)	
GEN11073-10415-4	Conformance Adherence - Level 1 -	See 10.3.2	Base conformance declaration that device meets the following IEEE 11073-10415 conformance requirements: a) All mandatory requirements shall be implemented. b) If implemented, conditional, recommended, and optional requirements shall conform to this standard.	Yes/No (No is not expected as No implies that the implementation is non-conformant)	
GEN11073-10415-5	Conformance Adherence - Level 2 -	See 10.3.3	In addition to GEN 11073-10415-4, if the device implements extensions and/or additions, they shall conform to nomenclature codes from ASN.1 and/or IEEE 11073-10101 framework. These extensions should also be defined in ICS tables pointing towards their reference.	Yes/No	
GEN11073-10415-6	Object Containment Tree	See 6.3	Provide Object Containment Diagram showing relations between object instances used by the application. A conforming implementation uses only object relations as defined in the DIM.		
GEN11073-10415-7	Nomenclature document used and revision	(standard documents)	(set of existing revisions)	(set of supported revision)	

**Table 10—IEEE 11073-10415 general ICSs table (continued)**

Index <sup>a</sup>	Feature	Reference	Req./Status	Support	Comment
GEN11073-10415-8	Data Structure Encoding	—	—	description of encoding method(s) for ASN.1 data structures	
GEN11073-10415-9	Use of Private Objects	—	Does the implementation use objects that are not defined in the DIM?	Yes/No (If yes: explain in Table 11)	
GEN11073-10415-10	Use of Private Nomenclature Extensions	—	Does the implementation use private extensions to the nomenclature (i.e., 0xF000–0xFFFF codes from IEEE Std 11073-10101)?  Private Nomenclature extensions are allowed <i>only</i> if the standard nomenclature does not include the specific terms required by the application.	Yes/No  (If yes: explain in Table 14)	
GEN11073-10415-11	11073-20601 Conformance		Provide the conformance report required by the IEEE Std 11073-20601.		

<sup>a</sup> The prefix *GEN11073-10415-* is used for the index in the general ICSs table.

### 10.4.3 DIM MOC implementation conformance statement

The DIM MOC ICS defines which objects are implemented. Information on each object shall be provided as a separate row in the template of Table 11.

**Table 11—Template for DIM MOC ICS table**

Index	Feature	Reference	Req./Status	Support	Comment
MOC-n	Object description	Reference to the clause in the standard or other location where the object is defined.	Implemented	Specify restrictions (e.g., maximum number of supported instances)	

The *n* in the Index column should be the object handle for implementations that have predefined objects. Otherwise the Index column shall simply be a unique number (1..m).

All private objects shall be specified and include either a reference to the definition for the object or, where no publicly available reference is available, the definition of the object should be appended to the conformance statement.

The Support column should indicate any restrictions for the object implementation.

An object containment diagram (class instance diagram) should be provided as part of the DIM MOC ICS.

**10.4.4 MOC attribute implementation conformance statement**

For each supported object as defined in the DIM MOC ICS, a MOC attribute ICS has to be provided that defines which attributes are used/supported by the implementation, including any inherited attributes. Table 12 is a template only.

**Table 12—Template for MOC attribute ICS table**

Index	Feature	Reference	Req./Status	Support	Comment
ATTR-n-x	Attribute Name. Extended attributes shall include the attribute ID also.	Fill in the reference to the ASN.1 structure if the attribute is not defined in this standard.	M = Mandatory / C = Conditional / R = Recommended / O = Optional (as per definition in Attribute Definition Tables)	Implemented? Yes/No Static/Dynamic Specify restrictions (e.g., value ranges). Describe how attribute is accessed (e.g., Get, Set, sent in config event report, sent in a data event report). Describe any specific restrictions.	

All private attributes shall be specified and include reference to the definition for the attribute. Where no publicly available reference is available, the definition of the attribute should be appended to the conformance statement.

The Support column shall specify whether the attribute is implemented; for extension attributes, whether the attribute value is static or dynamic; any value ranges; restrictions on attribute access or availability; as well as any other information.

The n in the Index column refers to the ID of the managed object for which the table is supplied (i.e., the index of the managed object as specified in the MOC ICS). There is one separate table for each supported managed object.

The x in the Index column is a unique serial number (1..m).

NOTE—The attribute definition tables in the standard define a minimum mandatory set of attributes for each object.

**10.4.5 MOC notification implementation conformance statement**

The MOC notification ICS specifies all implemented notifications (typically in the form of the event report service) that are emitted by the agent. Table 13 provides a template for use. One table has to be provided for each object that supports special object notifications. One row of the table shall be used for each notification.

**Table 13—Template for MOC notification ICS table**

Index	Feature	Reference	Req./Status	Support	Comment
NOTI-n-x	Notification Name and Notification ID	Reference to the clause in the standard or other location where the event is defined.		The Support column shall specify how the notification is sent and any restrictions.	

The n in the Index column refers to the ID of the managed object for which the table is supplied (i.e., the index of the managed object as specified in the POC ICS). There is one separate table for each managed object that supports specific object notifications (i.e., events).

The x in the Index column is a unique serial number (1..m).

All private notifications shall be specified and include reference to the definition for the notification. Where no publicly available reference is available, the definition of the notification should be appended to the conformance statement.

**10.4.6 MOC nomenclature conformance statement**

The MOC nomenclature ICS specifies all nonstandard nomenclature codes that are utilized by the agent. Table 14 provides a template for use. One row of the table is to be used for each nomenclature element.

**Table 14—Template for MOC nomenclature ICS table**

Index	Feature	Reference	Req./Status	Support	Comment
NOME-n	Nomenclature Name and Nomenclature value	Reference to the clause in the standard or other location where the nomenclature is defined or used		Describe how the nomenclature is used. Describe any specific restrictions	

The n in the Index column is a unique serial number (1..m).

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10415:2022

IEEE Std 11073-10415-2019  
Health Informatics—Personal health device communication  
Part 10415: Device specialization—Weighing scale

## Annex A

(informative)

### Bibliography

Bibliographical references are resources that provide additional or helpful material but do not need to be understood or used to implement this standard. Reference to these resources is made for informational use only.

[B1] Garrow, J. S., and J. Webster, “Quetelet’s index ( $W/H^2$ ) as a measure of fatness.” *International Journal of Obesity*, vol. 9, pp. 147–153, 1985.

[B2] IEC 60601-1, Ed. 3, Medical electrical equipment—Part 1: General requirements for basic safety and essential performance.<sup>9</sup>

[B3] IEC 60601-2, Medical electrical equipment—Part 2: Particular requirements for the basic safety and essential performance for specific device. (See the entire series of standards, Part 2-1 through Part 2-51.)

[B4] IEC 62304, Medical device software—Software life-cycle processes.

[B5] IEC 80001-1, Application of risk management for IT-networks incorporating medical devices—Part 1: Roles, responsibilities, and activities.

[B6] ISO 14971, Medical devices—Application of risk management to medical devices.<sup>10</sup>

[B7] ISO/IEEE 11073-10201:2004, Health informatics — Point-of-care medical device communication — Part 10201: Domain information model.<sup>11</sup>

[B8] ISO/IEEE 11073-20101:2004, Health informatics — Point-of-care medical device communication — Part 20101: Application profile — Base standard.

[B9] ITU-T Rec. X.680, Information technology — Abstract Syntax Notation One (ASN.1): Specification of basic notation.<sup>12</sup>

<sup>9</sup> IEC publications are available from the International Electrotechnical Commission (<http://www.iec.ch/>).

<sup>10</sup> ISO publications are available from the International Organization for Standardization (<http://www.iso.ch/>).

<sup>11</sup> ISO/IEEE publications are available from the International Organization for Standardization (<http://www.iso.ch/>). ISO/IEC publications are also available in the United States from Global Engineering Documents (<http://global.ihs.com/>). Electronic copies are available in the United States from the American National Standards Institute (<http://www.ansi.org/>).

<sup>12</sup> ITU publications are available from the International Telecommunications Union (<http://www.itu.in/>).

**Annex B**

(normative)

**Any additional ASN.1 definitions**

No additional ASN.1 definitions are defined.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10415:2022

**Annex C**

(normative)

**Allocation of identifiers**

This annex contains the nomenclature codes used in this document and not found in IEEE Std 11073-20601. For those not contained in this annex, the normative definition is found in IEEE Std 11073-20601.


The format used here follows that of IEEE Std 11073-10101.

```

/*****
* From Communication Infrastructure (MDC_PART_INFRA)
*****/
#define MDC_DEV_SPEC_PROFILE_SCALE          4111 /* Weighing scale */

/*****
* From Medical supervisory control and data acquisition (MDC_PART_SCADA)
*****/
#define MDC_MASS_BODY_ACTUAL                57664/* body mass */
#define MDC_LEN_BODY_ACTUAL                57668 /* body length */
#define MDC_RATIO_MASS_BODY_LEN_SQ        57680/*

/*****
* From Dimensions (MDC_PART_DIM)
*****/
#define MDC_DIM_CENTI_M                    1297 /* cm */
#define MDC_DIM_INCH                      1376 /* in */
#define MDC_DIM_KILO_G                    1731 /* kg */
#define MDC_DIM_LB                        1760 /* lb */
#define MDC_DIM_KILO_G_PER_M_SQ          7747 /* kg m-2 */
    
```

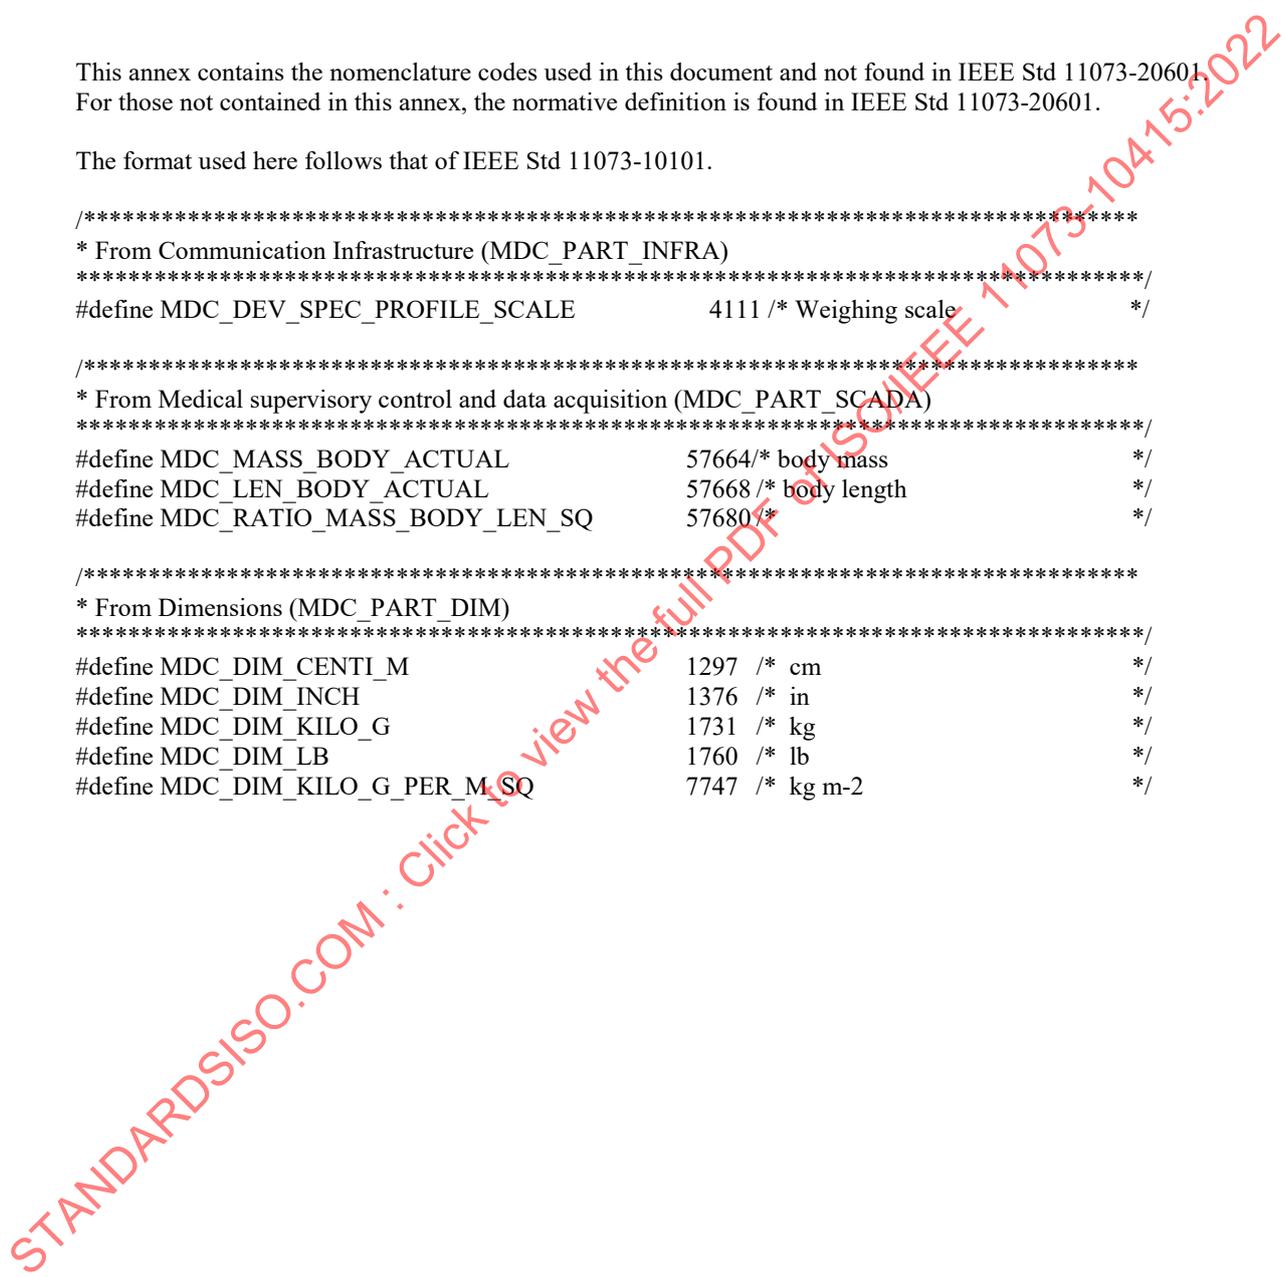

## Annex D

(informative)

### Message sequence examples

Figure D.1 shows a sequence diagram of the messaging procedure corresponding to the following use case. The user of a weighing scale agent intends to connect it to a manager for the first time. The weighing scale is capable of performing body weight and BMI measurements. Thus, it operates as an extended configuration. It is assumed that the person's height has already been manually entered into the weighing scale.

- a) When the user connects the weighing scale, the manager does not yet recognize the agent's configuration and sends a response to the agent's association request with the result *accepted-unknown-config*. See E.2.2.2 and E.2.2.3 for the corresponding PDU examples.
- b) As a consequence of this, the agent negotiates its configuration information to the manager. After getting confirmation from the manager accepting the configuration of the agent, the agent device is ready to send measurements. Both devices enter the Operating state. See E.3.2.2 and E.3.2.3 for the corresponding PDU examples.
- c) Subsequently, the manager requests the MDS object attributes of the agent by sending a data message with the "Remote Operation Invoke | Get" command. Note that the manager may request the MDS object attributes as soon as the agent enters the Associated state, including the Configuring and Operating substates. As a response the agent reports its MDS object attributes to the manager using a data message with the "Remote Operation Response | Get" command. See E.4.2 and E.4.3 for the corresponding PDU examples.
- d) As a next step, the user of the agent device takes a single measurement. The measurement data is transmitted to the manager using a confirmed event report. After having successfully received the measurement data, the manager sends a confirmation to the agent. See E.5.1 and E.5.2 for the corresponding PDU examples. In that particular example, a set of two measurements is transmitted, with the first one being a stored, not yet transmitted, measurement.
- e) The user ends the measurement session (e.g., by pushing a proper button on the device or just by not using the device for a duration longer than a certain time period). As a consequence, the agent disassociates from the manager by sending an association release request. The manager responds with an association release response. See E.6.1 and E.6.2 for the corresponding PDU examples.
- f) When the agent requests to associate to the manager for the next measurement session (e.g., the next day), the result in the manager's response is *accepted*, as it already knows the agent's configuration from the previous measurement session. Both devices transition directly to the Operating state.
- g) Finally, the last two steps shown are similar as in item d) and item e). The user takes a single confirmed measurement followed by releasing the association.

IEEE Std 11073-10415-2019  
 Health Informatics—Personal health device communication  
 Part 10415: Device specialization—Weighing scale

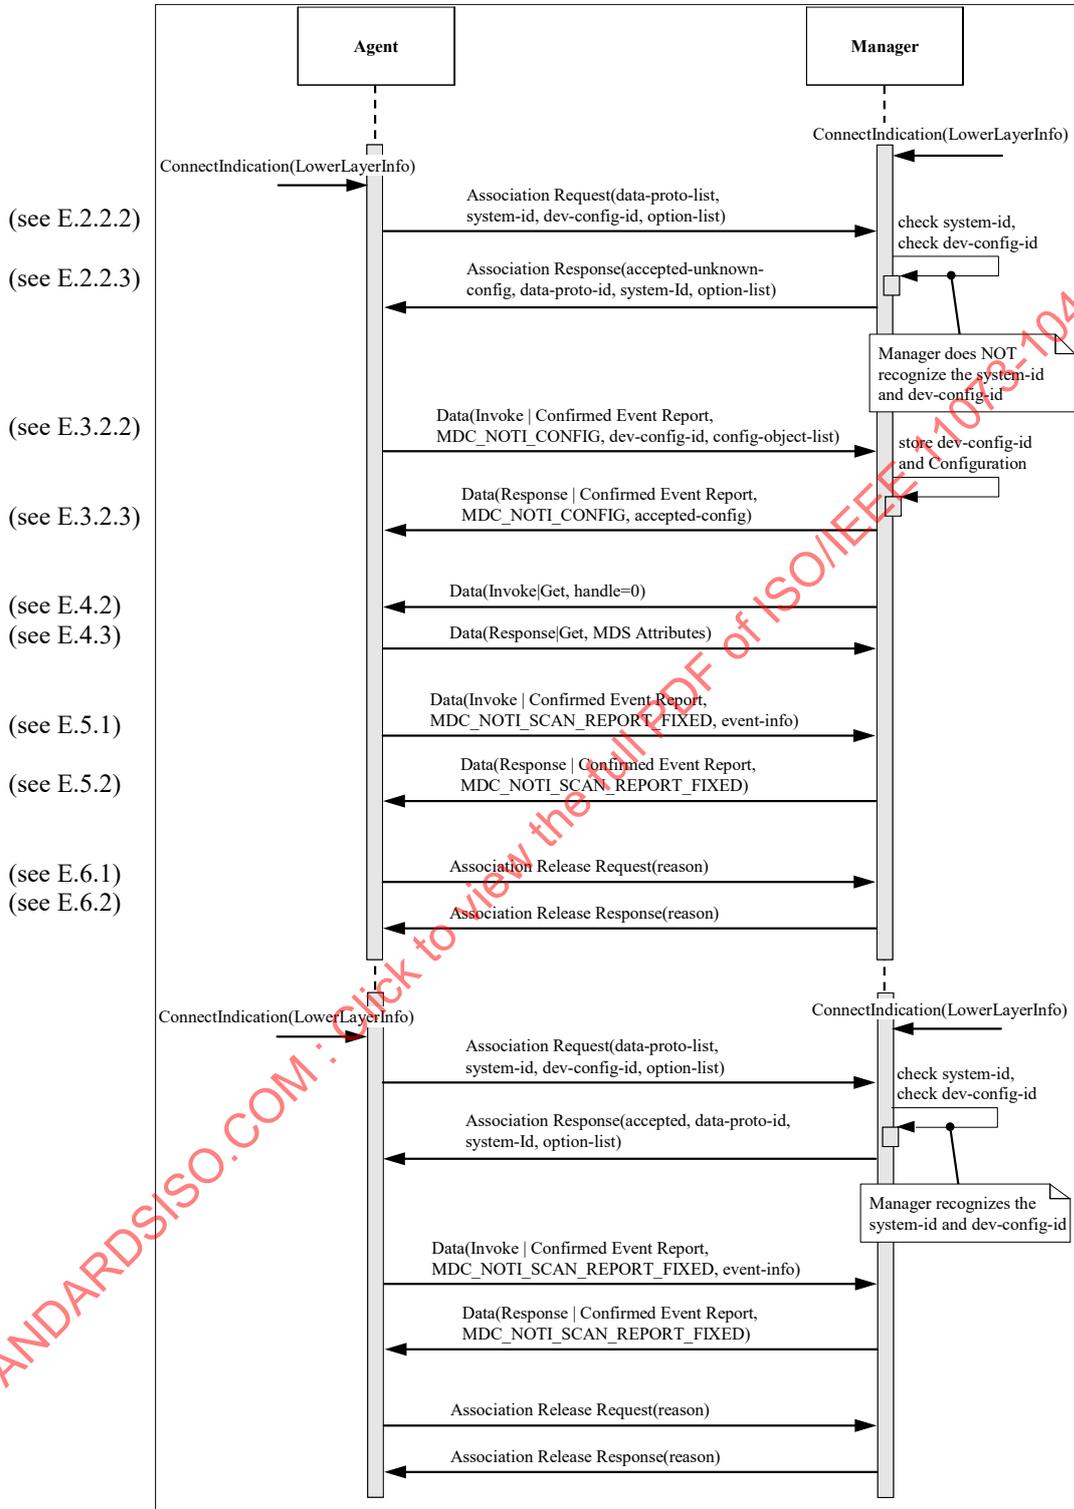


Figure D.1—Sequence diagram for weighing scale example use case