

Second edition
2014-03-01

Corrected version
2014-06-01

**Health informatics — Personal health
device communication —**

Part 10417:

Device specialization: Glucose meter

*Informatique de santé — Communication entre dispositifs de santé
personnels*

Partie 10417: Spécialisation des dispositifs: Glucomètre

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2014



Reference number
ISO/IEEE 11073-10417:2014(E)

© IEEE 2012

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. Neither the ISO Central Secretariat nor IEEE accepts any liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies and IEEE members. In the unlikely event that a problem relating to it is found, please inform the ISO Central Secretariat or IEEE at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2014



COPYRIGHT PROTECTED DOCUMENT

© IEEE 2012

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO or IEEE at the respective address below.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Institute of Electrical and Electronics Engineers, Inc.
3 Park Avenue, New York • NY 10016-5997, USA
E-mail stds.ipr@ieee.org
Web www.ieee.org

ISO version published 2013
Published in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

IEEE Standards documents are developed within the IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (IEEE-SA) Standards Board. The IEEE develops its standards through a consensus development process, approved by the American National Standards Institute, which brings together volunteers representing varied viewpoints and interests to achieve the final product. Volunteers are not necessarily members of the Institute and serve without compensation. While the IEEE administers the process and establishes rules to promote fairness in the consensus development process, the IEEE does not independently evaluate, test, or verify the accuracy of any of the information contained in its standards.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is called to the possibility that implementation of this standard may require the use of subject matter covered by patent rights. By publication of this standard, no position is taken with respect to the existence or validity of any patent rights in connection therewith. ISO/IEEE is not responsible for identifying essential patents or patent claims for which a license may be required, for conducting inquiries into the legal validity or scope of patents or patent claims or determining whether any licensing terms or conditions provided in connection with submission of a Letter of Assurance or a Patent Statement and Licensing Declaration Form, if any, or in any licensing agreements are reasonable or non-discriminatory. Users of this standard are expressly advised that determination of the validity of any patent rights, and the risk of infringement of such rights, is entirely their own responsibility. Further information may be obtained from ISO or the IEEE Standards Association.

This second edition of ISO/IEEE 11073-10417 cancels and replaces the first edition (ISO/IEEE 11073-10417:2010). ISO/IEEE 11073-10417 was prepared by the Substations Committee of the IEEE Power Engineering Society of the IEEE (as IEEE 11073-10417-2011). It was adopted by Technical Committee ISO/TC 215, *Respiratory and anaesthetic equipment*, in parallel with its approval by the ISO member bodies, under the “fast-track procedure” defined in the Partner Standards Development Organization cooperation agreement between ISO and IEEE. IEEE is responsible for the maintenance of this document with participation and input from ISO member bodies.

ISO/IEEE 11073 consists of the following parts, under the general title *Health informatics — Personal health device communication* (text in parentheses gives a variant of subtitle):

- Part 00103: Overview
- Part 10101: (Point-of-care medical device communication) Nomenclature
- Part 10102: (Point-of-care medical device communication) Nomenclature — Annotated ECG
- Part 10103: (Point-of-care medical device communication) — Nomenclature — Implantable device, cardiac
- Part 10201: (Point-of-care medical device communication) Domain information model

ISO/IEEE 11073-10417:2014(E)

- *Part 10404: Device specialization — Pulse oximeter*
- *Part 10406: Device specialization — Basic electrocardiograph (ECG) (1- to 3-lead ECG)*
- *Part 10407: Device specialization — Blood pressure monitor*
- *Part 10408: Device specialization — Thermometer*
- *Part 10415: Device specialization — Weighing scale*
- *Part 10417: Device specialization — Glucose meter*
- *Part 10418: Device specialization — International Normalized Ratio (INR) monitor*
- *Part 10420: Device specialization — Body composition analyzer*
- *Part 10421: Device specialization — Peak expiratory flow monitor (peak flow)*
- *Part 10441: Device specialization — Cardiovascular fitness and activity monitor*
- *Part 10471: Device specialization — Independent living activity hub*
- *Part 10472: Device specialization — Medication monitor*
- *Part 20101: (Point-of-care medical device communication) Application profiles — Base standard*
- *Part 20601: Application profile — Optimized exchange protocol*
- *Part 30200: (Point-of-care medical device communication) Transport profile — Cable connected*
- *Part 30300: (Point-of-care medical device communication) Transport profile — Infrared wireless*
- *Part 30400: (Point-of-care medical device communication) Interface profile — Cabled Ethernet*
- *Part 90101: (Point-of-care medical device communication) Analytical instruments — Point-of-care test*
- *Part 91064: (Standard communication protocol) Computer-assisted electrocardiography*
- *Part 92001: (Medical waveform format) — Encoding rules*

This corrected version of ISO 11073-10417:2014 incorporates the following corrections:

- The text "Authorized licensed use limited to: IEEE Standards Staff and authorized IEEE Sponsor Ballot Participants. Downloaded on May 28,2013 at 14:27:23 UTC from IEEE Xplore. Restrictions apply." has been deleted from the footer.
- On the cover page "First edition" has been replaced by "Second edition" and a sentence giving this revision information has been added in the Foreword.

Health Informatics—Personal health device communication

Part 10417: Device specialization— Glucose meter

IEEE Engineering in Medicine and Biology Society

Sponsored by the
IEEE 11073™ Standards Committee

IEEE
3 Park Avenue
New York, NY 10016-5997
USA

IEEE Std 11073-10417™-2011
(Revision of
IEEE Std 11073-10417-2009)

27 January 2012

STANDARDSISO.COM: Click to view the full PDF of ISO/IEEE 11073-10417:2014

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2014

Health informatics—Personal health device communication

**Part 10417: Device specialization—
Glucose meter**

Sponsor

IEEE 11073™ Standards Committee

of the

IEEE Engineering in Medicine and Biology Society

Approved 7 December 2011

IEEE-SA Standards Board

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2014

Abstract: Within the context of the ISO/IEC 11073 family of standards for device communication, a normative definition of communication between personal telehealth glucose meter devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes) is established by this standard in a manner that enables plug-and-play interoperability. Appropriate portions of existing standards are leveraged, including ISO/IEEE 11073 terminology, information models, application profile standards, and transport standards. The use of specific term codes, formats, and behaviors in telehealth environments restricting optionality in base frameworks in favor of interoperability are specified. A common core of communication functionality for personal telehealth glucose meters is defined in this standard.

Keywords: glucose meter, IEEE 11073-10417, medical device communication, personal health devices

The Institute of Electrical and Electronics Engineers, Inc.
3 Park Avenue, New York, NY 10016-5997, USA

Copyright © 2012 by the Institute of Electrical and Electronics Engineers, Inc.
All rights reserved. Published 27 January 2012. Printed in the United States of America.

IEEE is a registered trademark in the U.S. Patent & Trademark Office, owned by The Institute of Electrical and Electronics Engineers, Incorporated.

PDF: ISBN 978-0-7381-7163-0 **STD97195**
Print: ISBN 978-0-7381-7188-3 **STDPD97195**

IEEE prohibits discrimination, harassment and bullying. For more information, visit <http://www.ieee.org/web/aboutus/whatis/policies/a9-26.html>. No part of this publication may be reproduced in any form, in an electronic retrieval system or otherwise, without the prior written permission of the publisher.

IEEE Standards documents are developed within the IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (IEEE-SA) Standards Board. The IEEE develops its standards through a consensus development process, approved by the American National Standards Institute, which brings together volunteers representing varied viewpoints and interests to achieve the final product. Volunteers are not necessarily members of the Institute and serve without compensation. While the IEEE administers the process and establishes rules to promote fairness in the consensus development process, the IEEE does not independently evaluate, test, or verify the accuracy of any of the information contained in its standards.

Use of an IEEE Standard is wholly voluntary. The IEEE disclaims liability for any personal injury, property or other damage, of any nature whatsoever, whether special, indirect, consequential, or compensatory, directly or indirectly resulting from the publication, use of, or reliance upon this, or any other IEEE Standard document.

The IEEE does not warrant or represent the accuracy or content of the material contained herein, and expressly disclaims any express or implied warranty, including any implied warranty of merchantability or fitness for a specific purpose, or that the use of the material contained herein is free from patent infringement. IEEE Standards documents are supplied **“AS IS.”**

The existence of an IEEE Standard does not imply that there are no other ways to produce, test, measure, purchase, market, or provide other goods and services related to the scope of the IEEE Standard. Furthermore, the viewpoint expressed at the time a standard is approved and issued is subject to change brought about through developments in the state of the art and comments received from users of the standard. Every IEEE Standard is subjected to review at least every five years for revision or reaffirmation. When a document is more than five years old and has not been reaffirmed, it is reasonable to conclude that its contents, although still of some value, do not wholly reflect the present state of the art. Users are cautioned to check to determine that they have the latest edition of any IEEE Standard.

In publishing and making this document available, the IEEE is not suggesting or rendering professional or other services for, or on behalf of, any person or entity. Nor is the IEEE undertaking to perform any duty owed by any other person or entity to another. Any person utilizing this, and any other IEEE Standards document, should rely upon the advice of a competent professional in determining the exercise of reasonable care in any given circumstances.

Interpretations: Occasionally questions may arise regarding the meaning of portions of standards as they relate to specific applications. When the need for interpretations is brought to the attention of IEEE, the Institute will initiate action to prepare appropriate responses. Since IEEE Standards represent a consensus of concerned interests, it is important to ensure that any interpretation has also received the concurrence of a balance of interests. For this reason, IEEE and the members of its societies and Standards Coordinating Committees are not able to provide an instant response to interpretation requests except in those cases where the matter has previously received formal consideration. At lectures, symposia, seminars, or educational courses, an individual presenting information on IEEE standards shall make it clear that his or her views should be considered the personal views of that individual rather than the formal position, explanation, or interpretation of the IEEE.

Comments for revision of IEEE Standards are welcome from any interested party, regardless of membership affiliation with IEEE. Suggestions for changes in documents should be in the form of a proposed change of text, together with appropriate supporting comments. Comments on standards and requests for interpretations should be addressed to:

Secretary, IEEE-SA Standards Board
445 Hoes Lane
Piscataway, NJ 08854-4141
USA

Authorization to photocopy portions of any individual standard for internal or personal use is granted by the Institute of Electrical and Electronics Engineers, Inc., provided that the appropriate fee is paid to Copyright Clearance Center. To arrange for payment of licensing fee, please contact Copyright Clearance Center, Customer Service, 222 Rosewood Drive, Danvers, MA 01923 USA; +1 978 750 8400. Permission to photocopy portions of any individual standard for educational classroom use can also be obtained through the Copyright Clearance Center.

Introduction

This introduction is not part of IEEE Std 11073-10417-2011, Health informatics—Personal health device communication—Part 10417: Device specialization—Glucose meter.

ISO/IEEE 11073 standards enable communication between medical devices and external computer systems. This document uses the optimized framework created in ISO/IEEE 11073-20601:2010^a and describes a specific, interoperable communication approach for glucose meters. These standards align with and draw on the existing clinically focused standards to provide support for communication of data from clinical or personal health devices.

Revision history for IEEE Std 11073-10417

IEEE Std 11073-10417-2009	Initial release of the standard.
IEEE Std 11073-10417-2011	<p>The following changes were implemented in this revision:</p> <ul style="list-style-type: none"> a) In Table 6, the Supplemental-Type attribute was changed from Conditional to Optional. b) In the fourth paragraph of 6.9.1, the first sentence was reworded to specify that the agent init will be disabled when a PM-store is present. c) In the second paragraph of 6.9.1, the use cases associated with agent-init versus manager-init transmission of measurement data were clarified. d) In Annex B, “Numeric class” to “Enumeration class” was corrected. e) A new standard configuration was added, which affects the following: <ul style="list-style-type: none"> 1) New paragraph in 6.4.2. 2) Added a new Control Solution object separate from the Blood Glucose object (6.6.7). 3) Removed MDC_CONC_GLU_CONTROL from the Blood Glucose object’s Type attribute. 4) In 6.6.2, added +/- INFINITY as a way to indicate out-of-range sensor measurements. Also added this to the new Control Solution object in 6.6.7. f) In Table 13, the Semantic-Modality attribute was removed and the Supplemental-Types attribute was added. g) MDC_CONC_GLU_UNDETERMINED_PLASMA and MDC_CONC_GLU_UNDETERMINED_WHOLEBLOOD were added for meters that report plasma or whole blood glucose concentrations taken from an unknown sample source. Also, Table 1 was modified to add the “undetermined” sample source. The new OID was added to the Blood Glucose object extended configuration and the new standard configuration (Table 7). h) The MDC_CTXT_GLU_MEAL_BEDTIME nomenclature code was added to the Context Meal enumeration object. i) The Confirm-Timeout attribute was added, which was missing in Table 22. j) Table 13 was corrected. The recommended Enum-Observed-Value attribute should be Basic-Bit-Str instead of Simple-Bit-Str, as explained in the text following the table. k) In E.5.1, the encoding of Measurement-Active-Period = 1 hour was corrected to be a FLOAT type instead of a UINT-32. l) In C.3, the description of Glucose Context Meal BeforeMeal was corrected and lines were added for Glucose Context Meal Fasting and Glucose Context Meal Bedtime. m) In 8.3.2 and 8.3.3, the protocol-version text was modified to clarify what must be done when multiple protocol versions exist.

^aFor information on references, see Clause 2.

	<p>n) In 8.2, the N_{tx} limitation requirement was modified such that there is a limit for non-PM-store configurations but not for a PM-store configuration. The N_{tx} value of 5120 for non-PM-store configurations is based on an event report that contains 25 measurements of each of the 11 defined objects.</p> <p>o) An additional use case description text to 5.1 was added.</p> <p>p) Title, headers and footers, copyrights, formatting, references, and so on were updated per IEEE Standards publishing guidelines.</p> <p>q) In Table 7 for the Simple-Nu-Observed-Value and Compound-Simple-Nu-Observed-Value, the qualifier to “C” was changed and the text in the Value column was expanded.</p> <p>r) In 6.6.1, the first sentence of the last paragraph was replaced with “For standard configurations the optional attributes are initially not present.”</p> <p>s) Six occurrences of “manager device” to were changed to “manager”.</p>
--	---

Notice to users

Laws and regulations

Users of these documents should consult all applicable laws and regulations. Compliance with the provisions of this standard does not imply compliance to any applicable regulatory requirements. Implementers of the standard are responsible for observing or referring to the applicable regulatory requirements. IEEE does not, by the publication of its standards, intend to urge action that is not in compliance with applicable laws, and these documents may not be construed as doing so.

Copyrights

This document is copyrighted by the IEEE. It is made available for a wide variety of both public and private uses. These include both use, by reference, in laws and regulations, and use in private self-regulation, standardization, and the promotion of engineering practices and methods. By making this document available for use and adoption by public authorities and private users, the IEEE does not waive any rights in copyright to this document.

Updating of IEEE documents

Users of IEEE standards should be aware that these documents may be superseded at any time by the issuance of new editions or may be amended from time to time through the issuance of amendments, corrigenda, or errata. An official IEEE document at any point in time consists of the current edition of the document together with any amendments, corrigenda, or errata then in effect. In order to determine whether a given document is the current edition and whether it has been amended through the issuance of amendments, corrigenda, or errata, visit the IEEE Standards Association web site at <http://ieeexplore.ieee.org/xpl/standards.jsp>, or contact the IEEE at the address listed previously.

For more information about the IEEE Standards Association or the IEEE standards development process, visit the IEEE-SA web site at <http://standards.ieee.org>.

Errata

Errata, if any, for this and all other standards can be accessed at the following URL: <http://standards.ieee.org/findstds/errata/index.html>. Users are encouraged to check this URL for errata periodically.

Interpretations

Current interpretations can be accessed at the following URL:
<http://standards.ieee.org/findstds/interps/index.html>.

Patents

Attention is called to the possibility that implementation of this standard may require use of subject matter covered by patent rights. By publication of this standard, no position is taken by the IEEE with respect to the existence or validity of any patent rights in connection therewith. If a patent holder or patent applicant has filed a statement of assurance via an Accepted Letter of Assurance, then the statement is listed on the IEEE-SA website <http://standards.ieee.org/about/sasb/patcom/patents.html>. Letters of Assurance may indicate whether the Submitter is willing or unwilling to grant licenses under patent rights without compensation or under reasonable rates, with reasonable terms and conditions that are demonstrably free of any unfair discrimination to applicants desiring to obtain such licenses.

Essential Patent Claims may exist for which a Letter of Assurance has not been received. The IEEE is not responsible for identifying Essential Patent Claims for which a license may be required, for conducting inquiries into the legal validity or scope of Patents Claims, or determining whether any licensing terms or conditions provided in connection with submission of a Letter of Assurance, if any, or in any licensing agreements are reasonable or non-discriminatory. Users of this standard are expressly advised that determination of the validity of any patent rights, and the risk of infringement of such rights, is entirely their own responsibility. Further information may be obtained from the IEEE Standards Association.

STANDARDSISO.COM : Click to view the full PDF of IEEE 11075-104-17:2014

Contents

1. Overview	1
1.1 Scope	1
1.2 Purpose	1
1.3 Context	2
2. Normative references.....	2
3. Definitions, acronyms, and abbreviations	3
3.1 Definitions	3
3.2 Acronyms and abbreviations	3
4. Introduction to ISO/IEEE 11073 personal health devices	4
4.1 General	4
4.2 Introduction to IEEE 11073-20601 modeling constructs	4
5. Glucose meter device concepts and modalities	5
5.1 General	5
6. Glucose meter domain information model	6
6.1 Overview	6
6.2 Class extensions.....	6
6.3 Object instance diagram	7
6.4 Types of configuration.....	8
6.5 Medical device system object.....	9
6.6 Numeric objects.....	12
6.7 Real-time sample array objects.....	18
6.8 Enumeration objects	18
6.9 PM-store objects.....	22
6.10 Scanner objects.....	26
6.11 Class extension objects.....	26
6.12 Glucose meter information model extensibility rules	26
7. Glucose meter service model.....	26
7.1 General	26
7.2 Object access services.....	26
7.3 Object access event report services	27
8. Glucose meter communication model	29
8.1 Overview	29
8.2 Communication characteristics.....	29
8.3 Association procedure	29
8.4 Configuring procedure.....	31
8.5 Operating procedure	33
8.6 Time synchronization	34

9. Test associations.....	34
9.1 Behavior with standard configuration.....	35
9.2 Behavior with extended configurations	35
10. Conformance	35
10.1 Applicability	35
10.2 Conformance specification	35
10.3 Levels of conformance	36
10.4 Implementation conformance statements	36
Annex A (informative) Bibliography	41
Annex B (normative) Any additional ASN.1 definitions	42
Annex C (normative) Allocation of identifiers.....	43
Annex D (informative) Message sequence examples.....	46
Annex E (informative) Protocol data unit examples	48
Annex F (informative) IEEE list of participants	58

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2014

Health informatics—Personal health device communication

Part 10417: Device specialization— Glucose meter

IMPORTANT NOTICE: *This standard is not intended to ensure safety, security, health, or environmental protection. Implementers of the standard are responsible for determining appropriate safety, security, environmental, and health practices or regulatory requirements.*

This IEEE document is made available for use subject to important notices and legal disclaimers. These notices and disclaimers appear in all publications containing this document and may be found under the heading “Important Notice” or “Important Notices and Disclaimers Concerning IEEE Documents.” They can also be obtained on request from IEEE or viewed at <http://standards.ieee.org/IPR/disclaimers.html>.

1. Overview

1.1 Scope

Within the context of the ISO/IEEE 11073 family of standards for device communication, this standard establishes a normative definition of communication between personal telehealth glucose meter devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes) in a manner that enables plug-and-play interoperability. It leverages appropriate portions of existing standards, including ISO/IEEE 11073 terminology, information models, application profile standards, and transport standards. It specifies the use of specific term codes, formats, and behaviors in telehealth environments restricting optionality in base frameworks in favor of interoperability. This standard defines a common core of communication functionality for personal telehealth glucose meters.

1.2 Purpose

This standard addresses a need for an openly defined, independent standard for controlling information exchange to and from personal health devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes). Interoperability is the key to growing the potential market for these devices and to enabling people to be better informed participants in the management of their health.

1.3 Context

See IEEE Std 11073-20601aTM-2010¹ for an overview of the environment within which this standard is written.

This standard defines the device specialization for the glucose meter, being a specific agent type, and it provides a description of the device concepts, its capabilities, and its implementation according to this standard.

This standard is based on IEEE Std 11073-20601aTM-2010 and ISO/IEEE 11073-20601:2010, which in turn draw information from both ISO/IEEE 11073-10201:2004 [B3]² and ISO/IEEE 11073-20101:2004 [B4]. The medical device encoding rules (MDERs) used within this standard are fully described in ISO/IEEE 11073-20601:2010.

This standard reproduces relevant portions of the nomenclature found in ISO/IEEE 11073-10101:2004 [B2] and adds new nomenclature codes for the purposes of this standard. Among this standard, ISO/IEEE 11073-20601:2010, and IEEE Std 11073-20601a-2010, all required nomenclature codes for implementation are documented.

NOTE 1—IEEE Std 11073-20601a-2010 is an amendment to ISO/IEEE 11073-20601:2010. It contains new material and corrections and does not copy the content of ISO/IEEE 11073-20601:2010. Throughout this standard, a reference to IEEE Std 11073-20601a-2010 refers to the document that is obtained after applying this new material and corrections to ISO/IEEE 11073-20601:2010.³

NOTE 2—In this standard, ISO/IEEE 11073-104zz is used to refer to the collection of device specialization standards that utilize IEEE Std 11073-20601a-2010, where zz can be any number from 01 to 99, inclusive.

2. Normative references

The following referenced documents are indispensable for the application of this document (i.e., they must be understood and used, so that each referenced document is cited in text and its relationship to this document is explained). For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments or corrigenda) applies.

IEEE Std 11073-20601aTM-2010, Health informatics—Personal health device communication—Application profile—Optimized Exchange Protocol—Amendment 1.^{4,5}

ISO/IEEE 11073-20601:2010, Health informatics—Personal health device communication—Application profile—Optimized Exchange Protocol.⁶

¹ Information on references can be found in Clause 2.

² The numbers in brackets correspond to those of the bibliography in Annex A.

³ Notes in text, tables, and figures are given for information only and do not contain requirements needed to implement the standard.

⁴ The IEEE standards or products referred to in this clause are trademarks of the Institute of Electrical and Electronics Engineers, Inc.

⁵ IEEE publications are available from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, Piscataway, NJ 08854-4141, USA (<http://standards.ieee.org/>).

⁶ ISO/IEEE publications are available from the ISO Central Secretariat, 1, ch. de la Voie-Creuse, Case postale 56, CH-1211, Geneva 20, Switzerland (<http://www.iso.ch/>). ISO/IEEE publications are also available in the United States from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, Piscataway, NJ 08854-4141, USA (<http://standards.ieee.org/>).

3. Definitions, acronyms, and abbreviations

3.1 Definitions

For the purposes of this document, the following terms and definitions apply. The *IEEE Standards Dictionary: Glossary of Terms & Definitions* should be consulted for terms not defined in this clause.⁷

agent: A node that collects and transmits personal health data to an associated manager.

class: In object-oriented modeling, it describes the attributes, methods, and events that objects instantiated from the class utilize.

compute engine: *See: manager.*

device: A term used to refer to a physical apparatus implementing either an agent or a manager role.

glucose meter: A medical device for determining the approximate concentration of glucose in the blood.

handle: An unsigned 16-bit number that is locally unique and identifies one of the object instances within an agent.

manager: A node receiving data from one or more agent systems. Some examples of managers include a cellular phone, health appliance, set top box, or a computer system.

obj-handle: *See: handle.*

object: In object-oriented modeling, a particular instantiation of a class. The instantiation realizes attributes, methods, and events from the class.

personal health device: A device used in personal health applications.

personal telehealth device: *See: personal health device.*

3.2 Acronyms and abbreviations

APDU	application protocol data unit
ASN.1	Abstract Syntax Notation One
AST	alternative site testing
DIM	domain information model
EUI-64	extended unique identifier (64 bits)
HbA1c	hemoglobin bound to glucose (the A1c form)
HCP	health care professional
ICS	implementation conformance statements
ISF	interstitial fluid
MDC	medical device communication
MDER	medical device encoding rules
MDS	medical device system
MOC	managed object class
OID	object identifier
PDU	protocol data unit
PHD	personal health device
VMO	virtual medical object
VMS	virtual medical system

⁷ The *IEEE Standards Dictionary: Glossary of Terms & Definitions* is available at <http://shop.ieee.org/>.

4. Introduction to ISO/IEEE 11073 personal health devices

4.1 General

This standard and the remainder of the series of ISO/IEEE 11073 personal health device (PHD) standards fit in the larger context of the ISO/IEEE 11073 series of standards. The full suite of standards enables agents to interconnect and interoperate with managers and with computerized health-care information systems. See IEEE Std 11073-20601a-2010 for a description of the guiding principles for this series of ISO/IEEE 11073 Personal Health Device standards.

IEEE Std 11073-20601a-2010 supports the modeling and implementation of an extensive set of personal health devices. This standard defines aspects of the glucose meter device. It describes all aspects necessary to implement the application layer services and data exchange protocol between an ISO/IEEE 11073 PHD glucose meter agent and a manager. This standard defines a subset of the objects and functionality contained in IEEE Std 11073-20601a-2010, and it extends and adds definitions where appropriate. All new definitions are given in Annex B in Abstract Syntax Notation One (ASN.1) Nomenclature codes referenced in this standard, which are not defined in IEEE Std 11073-20601a-2010, are normatively defined in Annex C.

4.2 Introduction to IEEE 11073-20601 modeling constructs

4.2.1 General

The ISO/IEEE 11073 series of standards, and in particular IEEE Std 11073-20601a-2010, is based on an object-oriented systems management paradigm. The overall system model is divided into three principal components: the domain information model (DIM), the service model, and the communication model. See IEEE Std 11073-20601a-2010 for a detailed description of the modeling constructs.

4.2.2 Domain information model

The DIM is a hierarchical model that describes an agent as a set of objects. These objects and their attributes represent the elements that control behavior and report on the status of the agent and the data that an agent can communicate to a manager. Communication between the agent and the manager is defined by the application protocol in IEEE Std 11073-20601a-2010.

4.2.3 Service model

The service model defines the conceptual mechanisms for the data exchange services. Such services are mapped to messages that are exchanged between the agent and the manager. Protocol messages within the ISO/IEEE 11073 series of standards are defined in ASN.1. The messages defined in IEEE Std 11073-20601a-2010 can coexist with messages defined in other standard application profiles defined in the ISO/IEEE 11073 series of standards.

4.2.4 Communication model

In general, the communication model supports the topology of one or more agents communicating over logical point-to-point connections to a single manager. For each logical point-to-point connection, the dynamic system behavior is defined by a connection state machine as specified in IEEE Std 11073-20601a-2010.

4.2.5 Implementing the models

An agent implementing this standard shall implement all mandatory elements of the information, service, and communication models as well as all conditional elements where the condition is met. The agent should implement the recommended elements, and it may implement any combination of the optional elements. A manager implementing this standard shall utilize at least one of the mandatory, conditional, recommended, or optional elements. In this context, “utilize” means to use the element as part of the primary function of the manager device. For example, a manager whose primary function is to display data would need to display a piece of data in the element in order to utilize it.

5. Glucose meter device concepts and modalities

5.1 General

This clause presents the general concepts of glucose meters. In the context of personal health devices in this family of standards, a glucose meter is a device that measures the concentration of glucose in the blood. Glucose, or the concentration of blood sugar in the blood, is the primary source of energy for the body’s cells. The glucose level is tightly regulated in the human body and is normally maintained between approximately 70 mg/dL and 150 mg/dL (4 mmol/L and 8 mmol/L). The total amount of glucose in the circulating blood is, therefore, approximately 3.5 g to 7.5 g (assuming an ordinary adult blood volume of 5 L). Glucose levels rise after meals and are usually lowest in the morning, before the first meal of the day.

In a healthy adult male of 75 kg with a blood volume of 5 L, a blood glucose level of 100 mg/dL (5.5 mmol/L) corresponds to a total of approximately 5 g (1/5 oz and equivalent to a commercial sugar packet) of glucose in the blood and approximately 45 g (1.5 oz) in the total body fluid (which includes blood and interstitial fluid) and on average will be approximately 60% of the total body weight in men.

The failure to maintain blood glucose in the normal range leads to conditions of persistently high (hyperglycemia) or low (hypoglycemia) blood sugar. Diabetes mellitus, which is characterized by persistent hyperglycemia from several causes, is the most prominent disease related to the failure to regulate blood sugar. Fructose and galactose are also sugars found in the blood; however, only glucose levels are regulated via insulin and glucagon.

Countries that use the metric system generally use mmol/L. The United States uses mg/dL. To convert blood glucose readings, utilize the following conversions:

Divide the mg/dL by 18 to get mmol/L (or multiply by 0.055)

Multiply the mmol/L by 18 to get mg/dL (or divide by 0.055)

The glucose meters considered in this specialization are typically handheld instruments that require a sample of blood or body fluid to perform the glucose measurement. The glucose concentration measured by various techniques can be classified into different types defined by three elements: sample type, sample source, and concentration reference method. Table 1 shows all the glucose concentration types defined in this standard.

Table 1—Glucose concentration types

Sample type	Sample source	Reference method
Blood	Capillary	Whole blood
		Plasma
	Venous	Whole blood
		Plasma
	Arterial	Whole blood
		Plasma
	Undetermined	Whole blood
		Plasma
Interstitial fluid	N/A	N/A
Control solution	N/A	N/A

NOTE—The blood glucose concentration may be indirectly derived from an interstitial fluid (ISF) sample, which is a common technique used in continuous glucose monitoring. A control solution is normally used for glucose meter quality control.

In addition to glucose measurement, glucose meters generally provide a means for the user to associate information on meals, exercise, and medications with a glucose measurement. Advanced devices may also allow users to customize device settings and to provide additional information related to their diabetes treatment and disease management.

Glucose meters are usually small, portable devices that are carried around by the user so that blood glucose measurements may be taken as needed, whether or not the user is in a network environment where communications with a manager can be established. Hence, measurement data are typically logged within the meter and can be retrieved at a later time, either in whole or in part, when the meter is connected to a manager network. There are two typical use cases for the transfer of measurement data to a manager:

- By the user in a non-health-care environment. A user may connect the meter to a personal manager device such as a personal computer or a portable communications device such as a cell phone. In this case, the user would download the most recent logged measurement data from the meter for near-term trend analysis or for transfer of data to an external electronic health network service. The transfer of data would happen immediately on connection with the manager application and require no initiation by the user. This is a temporary storage model of the meter.
- By a health care professional in an office or clinic environment. The health care professional would download all logged measurement data from the meter for longer term analysis, such as the data logged since the patient's last appointment. The transfer of data would be controlled entirely by the manager application and would not necessarily happen automatically when a connection is established. This is a long-term storage model of the meter.

This standard supports configurations that allow for support of both temporary and long-term storage models.

6. Glucose meter domain information model

6.1 Overview

This clause describes the domain information model of the glucose meter.

6.2 Class extensions

In this standard, no class extensions are defined with respect to IEEE Std 11073-20601a-2010.

6.3 Object instance diagram

The object instance diagram of the glucose meter domain information model, which is defined for the purposes of this standard, is shown in Figure 1.

The objects of the DIM, as shown in Figure 1, are described in 6.5 to 6.11. See 6.5 through 6.11 for descriptions of the different glucose meter objects [e.g., the glucose meter medical device system (MDS) object, the glucose numeric object, and the enumeration object]. See 6.12 for rules for extending the glucose meter information model beyond elements as described in this standard. Each clause that describes an object of the glucose meter contains the following information:

- The nomenclature code used to identify the class of the object. One example where this code is used is the configuration event, where the object class is reported for each object. This allows the manager to determine whether the class of the object being specified is a numeric, real-time sample array, enumeration, scanner, or PM-store class.
- The attributes of the object. Each object has attributes that represent and convey information on the physical device and its data sources. Each object has a Handle attribute that identifies the object instance within an agent. Attribute values are accessed and modified using methods such as GET and SET. Attribute types are defined using an ASN.1. The ASN.1 definitions for new attribute types specific to this standard are in Annex B, and the ASN.1 definitions for existing attribute types referenced in this standard are in IEEE Std 11073-20601a-2010.
- The methods available on the object.
- The potential events generated by the object. The data are sent to the manager using events.
- The available services such as getting or setting attributes.

The attributes for each class are defined in tables that specify the name of the attribute, its value, and its qualifier. The qualifiers mean: M — Attribute is Mandatory, C — Attribute is Conditional and depends on the condition stated in the Remark or Value column (if IEEE Std 11073-20601a-2010 is referenced, then it contains the conditions), R — Attribute is Recommended, NR — Attribute is Not Recommended, and O — Attribute is Optional. Mandatory attributes shall be implemented by an agent. Conditional attributes shall be implemented if the condition applies and may be implemented otherwise. Recommended attributes should be implemented by the agent. Not recommended attributes should not be implemented by the agent. Optional attributes may be implemented on an agent.

The attributes can be either static, dynamic, or observational as specified in IEEE Std 11073-20601a-2010.

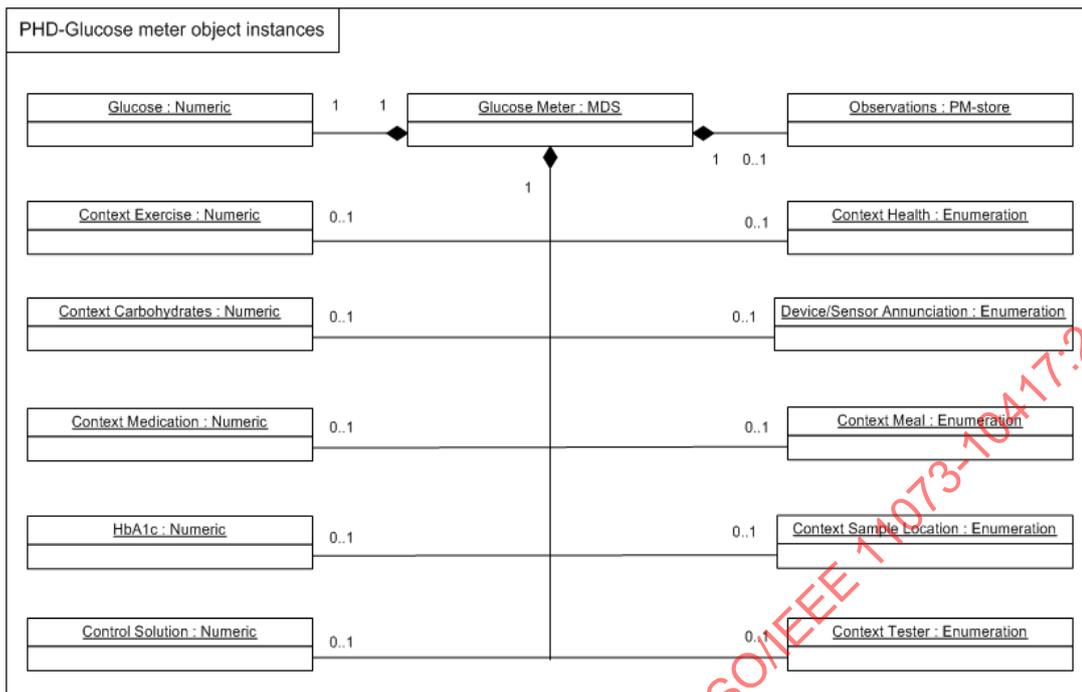


Figure 1—Glucose meter—domain information model

6.4 Types of configuration

6.4.1 General

As specified in IEEE Std 11073-20601a-2010, there are two styles of configuration available. Subclauses 6.4.2 and 6.4.3 briefly introduce standard and extended configurations.

6.4.2 Standard configuration

Standard configurations are defined in the ISO/IEEE 11073-104zz specializations (such as this standard) and are assigned a well-known identifier (Dev-Configuration-Id). The usage of a standard configuration is negotiated at association time between the agent and the manager. If the manager acknowledges that it understands and wants to operate using the configuration, then the agent can begin sending measurements immediately. If the manager does not understand the configuration, the agent provides the configuration prior to transmitting measurement information.

Two standard configurations are defined in this standard. Standard configuration 1700 (0x06A4) contains only a glucose numeric object as defined in 6.6.2. Standard configuration 1701 (0x06A5) contains a glucose numeric object and a control solution numeric object as defined in 6.6.7.

6.4.3 Extended configuration

In extended configurations, the agent’s configuration is not predefined in a standard. The agent determines which objects, attributes, and values will be used in a configuration and assigns a configuration identifier. When the agent associates with a manager, it negotiates an acceptable configuration. Typically, the manager does not recognize the agent’s configuration on the first connection, so the manager responds that the agent needs to send the configuration information as a configuration event report. If, however, the manager already understands the configuration, either because it was preloaded in some way or the agent

had previously associated with the manager, then the manager responds that the configuration is known and no further configuration information needs to be sent.

6.5 Medical device system object

6.5.1 MDS object attributes

Table 2 summarizes the attributes of the glucose meter MDS object. The nomenclature code to identify the MDS object class is MDC_MOC_VMS_MDS_SIMP.

Table 2—MDS object attributes

Attribute name	Value	Qual.
Handle	0	M
System-Type	Attribute not present. See IEEE Std 11073-20601a-2010.	C
System-Type-Spec-List	{MDC_DEV_SPEC_PROFILE_GLUKOSE, 2}.	M
System-Model	{“Manufacturer”, “Model”}	M
System-Id	Extended unique identifier (64 bits) (EUI-64)	M
Dev-Configuration-Id	Standard config: 0x06A4 (1700) Standard config: 0x06A5 (1701) Extended configs: 0x4000–0x7FFF	M
Attribute-Value-Map	See IEEE Std 11073-20601a-2010.	C
Production-Specification	See IEEE Std 11073-20601a-2010.	O
Mds-Time-Info	See IEEE Std 11073-20601a-2010.	C
Date-and-Time	See IEEE Std 11073-20601a-2010.	C
Relative-Time	See IEEE Std 11073-20601a-2010.	C
HiRes-Relative-Time	See IEEE Std 11073-20601a-2010.	C
Date-and-Time-Adjustment	See IEEE Std 11073-20601a-2010.	C
Power-Status	<i>onBattery</i> or <i>onMains</i>	O
Battery-Level	See IEEE Std 11073-20601a-2010.	O
Remaining-Battery-Time	See IEEE Std 11073-20601a-2010.	O
Reg-Cert-Data-List	See IEEE Std 11073-20601a-2010.	O
Confirm-Timeout	See IEEE Std 11073-20601a-2010.	O

NOTE—See IEEE Std 11073-20601a-2010 for information on whether an attribute is static or dynamic.

In the response to a Get MDS object command, only implemented attributes and their corresponding values are returned.

See IEEE Std 11073-20601a-2010 for descriptive explanations of the individual attributes as well as for information on attribute ID and attribute type.

The Dev-Configuration-Id attribute holds a locally unique 16-bit identifier that identifies the device configuration instance. For a glucose meter agent with extended configuration, this identifier is chosen in the range of extended-config-start to extended-config-end (see IEEE Std 11073-20601a-2010) as shown in Table 2.

The agent sends the Dev-Configuration-Id during the Associating state (see 8.3) to identify its configuration for the duration of the association. If the manager already holds the configuration information relating to the Dev-Configuration-Id, it recognizes the Dev-Configuration-Id. Then the Configuring state (8.4) is skipped, and the agent and manager enter the Operating state. If the manager does not recognize the Dev-Configuration-Id, the agent and manager enter the Configuring state.

If an agent implements multiple IEEE 11073-104zz specializations, System-Type-Spec-List is a list of type/version pairs, each referencing the respective device specialization and version of that specialization.

6.5.2 MDS object methods

Table 3 defines the methods (actions) of the glucose meter agent's MDS object. These methods are invoked using the Action service. In Table 3, the Subservice type name column defines the name of the method; the Mode column defines whether the method is invoked as an unconfirmed action (i.e., roiv-cmip-action from IEEE Std 11073-20601a-2010) or a confirmed action (i.e., roiv-cmip-confirmed-action); the Subservice type (action-type) column defines the nomenclature code to use in the action-type field of an action request and response (see IEEE Std 11073-20601a-2010); the Parameters (action-info-args) column defines the associated ASN.1 data structure (see IEEE Std 11073-20601a-2010 for ASN.1 definitions) to use in the action message for the action-info-args field of the request; and the Results (action-info-args) column defines the structure to use in the action-info-args of the response.

Table 3—MDS object methods

Service	Subservice type name	Mode	Subservice type (action-type)	Parameters (action-info-args)	Results (action-info-args)
ACTION	Set-Time	Confirmed	MDC_ACT_SET_TIME	SetTimeInvoke	—

Set-Time

This method allows the manager to set a real-time clock in the agent with the absolute time. The agent indicates whether the Set-Time command is valid using the mds-time-capab-set-clock bit in the Mds-Time-Info attribute (see IEEE Std 11073-20601a-2010).

Agents following only this device specialization and no others shall send event reports using agent-initiated measurement data transmission. Agents following this device specialization as well as others shall send event reports in the appropriate fashion. During the association procedure (see 8.3), data-req-mode-capab shall be set to the appropriate value for the event report style. As a result, the manager shall assume the glucose meter agent does not support any of the MDS-Data-Request features (see IEEE Std 11073-20601a-2010 for additional information). Thus, implementation of the MDS-Data-Request method/action is not required in this standard and is not shown in Table 3.

6.5.3 MDS object events

Table 4 defines the events that can be sent by the glucose meter MDS object.

Table 4—Glucose meter MDS object events

Service	Subservice type name	Mode	Subservice type (event-type)	Parameters (event- info)	Results (event-reply- info)
EVENT REPORT	MDS-Configuration-Event	Confirmed	MDC_NOTI_CONFIG	ConfigReport	ConfigReport Rsp
	MDS-Dynamic-Data-Update-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_FIXED	ScanReportInfoFixed	—
	MDS-Dynamic-Data-Update-Var	Confirmed	MDC_NOTI_SCAN_REPORT_VAR	ScanReportInfoVar	—
	MDS-Dynamic-Data-Update-MP-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_MP_FIXED	ScanReportInfoMP Fixed	—
	MDS-Dynamic-Data-Update-MP-Var	Confirmed	MDC_NOTI_SCAN_REPORT_MP_VAR	ScanReportInfoMP Var	—

— **MDS-Configuration-Event:**

This event is sent by the glucose meter agent during the configuring procedure if the manager does not already know the glucose meter agent's configuration from past associations or because the manager has not been implemented to recognize the configuration according to the glucose meter device specialization. The event provides static information about the supported measurement capabilities of the glucose meter agent.

— **MDS-Dynamic-Data-Update-Var:**

This event provides dynamic measurement data from the glucose meter agent for the glucose numeric object. These data are reported using a generic attribute list variable format. The event is sent as an unsolicited message by the agent (i.e., an agent-initiated measurement data transmission). See 8.5.3 for more information on unsolicited event reporting.

— **MDS-Dynamic-Data-Update-Fixed:**

This event provides dynamic measurement data from the glucose meter agent for the glucose numeric object. These data are reported in the fixed format defined by the Attribute-Value-Map attribute of the object(s). The event is sent as an unsolicited message by the agent (i.e., an agent-initiated measurement data transmission). See 8.5.3 for more information on unsolicited event reporting.

— **MDS-Dynamic-Data-Update-MP-Var:**

This is the same as MDS-Dynamic-Data-Update-Var but allows inclusion of data from multiple people.

— **MDS-Dynamic-Data-Update-MP-Fixed:**

This is the same as MDS-Dynamic-Data-Update-Fixed but allows inclusion of data from multiple people.

NOTE—IEEE Std 11073-20601a-2010 requires that managers support all of the MDS object events listed above.

6.5.4 Other MDS services

6.5.4.1 GET service

A glucose meter agent shall support the GET service, which is provided by the MDS object to retrieve the values of all implemented MDS object attributes. The GET service can be invoked as soon as the glucose meter agent receives the Association Response and moves to the Associated state, including the Operating and Configuring substates.

The manager may request the MDS object attributes of the glucose meter agent; in which case, the manager shall send the “Remote Operation Invoke | Get” message (see roiv-cmip-get in IEEE Std 11073-20601a-2010) with the reserved MDS handle value of 0. The glucose meter agent shall report its MDS object attributes to the manager using the “Remote Operation Response | Get” message (see rors-cmip-get in IEEE Std 11073-20601a-2010). See Table 5 for a summary of the GET service including some message fields.

Table 5—Glucose meter MDS object GET service

Service	Remark	Field	Value	Qual.
roiv-cmip-get	Manager GET service request of agents MDS attributes.	obj-handle	0	M
		attribute-id-list	Dynamic	O
rors-cmip-get	Agent GET service response to GET service request by manager.	obj-handle	0	M
		attribute-list	Dynamic	M

See 8.5.2 for details on the procedure for getting the MDS object attributes.

6.5.4.2 SET service

The glucose meter specialization does not require an implementation to support the MDS object SET service.

6.6 Numeric objects

6.6.1 General

The glucose meter DIM (see Figure 1) contains numeric objects that represent aspects of blood glucose and associated medical context. The nomenclature code to identify the numeric class is MDC_MOC_VMO_METRIC_NU. Table 6 shows attributes that are common to all the numeric types of the glucose meter agent.

Table 6—Common glucose numeric object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601a-2010.	M
Type	Defined in each table below.	M
Supplemental-Types	See IEEE Std 11073-20601a-2010.	NR
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated mss-cat-manual	M
Metric-Structure-Small	See IEEE Std 11073-20601a-2010.	NR
Measurement-Status	See IEEE Std 11073-20601a-2010.	NR
Metric-Id	See IEEE Std 11073-20601a-2010.	C
Metric-Id-List	See IEEE Std 11073-20601a-2010.	NR
Metric-Id-Partition	See IEEE Std 11073-20601a-2010.	NR
Unit-Code	See IEEE Std 11073-20601a-2010.	M
Attribute-Value-Map	See IEEE Std 11073-20601a-2010.	C
Source-Handle-Reference	See IEEE Std 11073-20601a-2010.	NR
Label-String	See IEEE Std 11073-20601a-2010.	O
Unit-LabelString	See IEEE Std 11073-20601a-2010.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	R
Relative-Time-Stamp	See IEEE Std 11073-20601a-2010.	O
HiRes-Time-Stamp	See IEEE Std 11073-20601a-2010.	C
Measure-Active-Period	See IEEE Std 11073-20601a-2010.	C
Simple-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	NR
Basic-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	C
Compound-Basic-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	NR
Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	NR
Compound-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	NR
Accuracy	See IEEE Std 11073-20601a-2010.	R

Subclauses 6.6.2 through 6.6.6 describe the numeric objects that are defined for use in the glucose meter. Each object represents a specific aspect of blood glucose measurement or an associated medical context. The class is denoted by the *Type* attribute. The description of each numeric object defines the data or events it produces, the possible states, and where appropriate, its behavior. The respective tables define the numeric values generated by the agent in response to a change in state.

Sometimes, the interpretation of one attribute value in an object depends on other attribute values in the same object. For example, *Unit-Code* and *Unit-LabelString* provide context for the observed values. Whenever a contextual attribute changes, the agent shall report these changes to the manager using an MDS object event (see 6.5.3) prior to reporting any of the dependent values.

The numeric object does not support any methods, events, or other services.

For standard configurations, the optional attributes are initially not present. See IEEE Std 11073-20601a-2010 for descriptive explanations on the individual attributes as well as for information on attribute ID and attribute type.

6.6.2 Blood glucose

Table 7 summarizes the attributes of the blood glucose numeric object. The blood glucose numeric object shall be supported by a glucose meter agent.

Table 7—Blood glucose numeric object attributes

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x06A4)		Standard configuration (Dev-Configuration-Id = 0x06A5)	
	Value	Qual.	Value	Qual.	Value	Qual.
Handle	See IEEE Std 11073-20601a-2010	M	1	M	1	M
Type	{MDC_PART_SCADA, MDC_CONC_GLU_CAPILLARY_WHOLEBLOOD or MDC_CONC_GLU_CAPILLARY_PLASMA or MDC_CONC_GLU_VENOUS_WHOLEBLOOD or MDC_CONC_GLU_VENOUS_PLASMA or MDC_CONC_GLU_ARTERIAL_WHOLEBLOOD or MDC_CONC_GLU_ARTERIAL_PLASMA or MDC_CONC_GLU_UNDETERMINED_WHOLEBLOOD or MDC_CONC_GLU_UNDETERMINED_PLASMA or MDC_CONC_GLU_ISF}.	M	{MDC_PART_SCADA, MDC_CONC_GLU_CAPILLARY_WHOLEBLOOD}.	M	{MDC_PART_SCADA, MDC_CONC_GLU_UNDETERMINED_PLASMA}.	M
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated. The mss-cat-manual shall only be set if the reading is manually entered.	M	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated.	M	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated.	M
Unit-Code	MDC_DIM_MILLI_G_PER_DL or MDC_DIM_MILLI_MOLE_PERL.	M	MDC_DIM_MILLI_G_PER_DL.	M	MDC_DIM_MILLI_G_PER_DL.	M
Attribute-Value-Map	See IEEE Std 11073-20601a-2010.	C	MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_ABS.	M	MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_ABS.	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	C	If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601a-2010 apply.	C	If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601a-2010 apply.	C

STANDARDS.PDF Click to view the full PDF of ISO/IEEE 11073-10417:2014

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x06A4)		Standard configuration (Dev-Configuration-Id = 0x06A5)	
	Value	Qual.	Value	Qual.	Value	Qual.
Relative-Time-Stamp	See IEEE Std 11073-20601a-2010.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601a-2010.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601a-2010.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601a-2010.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601a-2010.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601a-2010.	C
Measure-Active-Period	See IEEE Std 11073-20601a-2010.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601a-2010.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601a-2010.	NR
Basic-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	C	See IEEE Std 11073-20601a-2010.	M	See IEEE Std 11073-20601a-2010.	M
Simple-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	C	This type of observed value is not allowed because the Basic-Nu-Observed-Value is mandatory, and IEEE Std 11073-20601a-2010 mandates that one and only one type of observed value can be used.	C	This type of observed value is not allowed because the Basic-Nu-Observed-Value is mandatory, and IEEE Std 11073-20601a-2010 mandates that one and only one type of observed value can be used.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	NR	This type of observed value is not allowed because the Basic-Nu-Observed-Value is mandatory, and IEEE Std 11073-20601a-2010 mandates that one and only one type of observed value can be used.	C	This type of observed value is not allowed because the Basic-Nu-Observed-Value is mandatory, and IEEE Std 11073-20601a-2010 mandates that one and only one type of observed value can be used.	C
Accuracy	See IEEE Std 11073-20601a-2010.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601a-2010.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601a-2010.	NR

NOTE—See IEEE Std 11073-20601a-2010 for information on whether an attribute is static or dynamic.

The blood glucose numeric object does not support any methods, events, or other services.

In case a blood glucose measurement needs to be further associated with a meal, sample location, and tester information, the additional Enumeration objects (i.e., context carbohydrates, context sample location, and context tester) can be used. See 6.8 for detail.

In standard configuration 1701 (0x06A5), a glucose measurement that is above the capabilities of the device sensor shall be indicated with an observed value of +INFINITY, and a glucose measurement that is below the capabilities of the device sensor shall be indicated with an observed value of -INFINITY.

6.6.3 Hemoglobin bound to glucose A1c form (HbA1c)

HbA1c, which is also known as A1c or glycated hemoglobin, is used as the long-term measure of blood sugar control. The A1c test measures how many A1c hemoglobin cells (a specific part of red blood cells) have sugar attached to them. Because these cells live for approximately 4 months, this test indicates how well blood sugar has been controlled over the previous few months. The American Diabetes Association [B1] recommends an A1c result of 7% or less to help reduce the risk of long-term complications of diabetes. Table 8 identifies the measured, calculated or manually entered values for recording HbA1c data.

Table 8—HbA1c numeric object attributes

Attribute name	Extended configuration	
	Value	Qual.
Type	{MDC_PART_SCADA, MDC_CONC_HBA1C}.	M
Unit-Code	MDC_DIM_PERCENT.	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	M
Basic-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	M

NOTE—See IEEE Std 11073-20601a-2010 for information on whether an attribute is static or dynamic.

If the HbA1c value is entered manually, the mss-cat-manual bit shall be set in Metric-Spec-Small as well.

6.6.4 Context exercise

The level of exercise undertaken in a period can be important to record to balance food intake and insulin dose. Where there are issues over control of blood glucose, a review of exercise may be helpful in the care and management of the person. Table 9 identifies the values a person can enter on the glucose device to record his or her exercise regimen.

Table 9—Context exercise numeric object attributes

Attribute name	Extended configuration	
	Value	Qual.
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_EXERCISE}.	M
Unit-Code	MDC_DIM_PERCENT.	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	M
Measure-Active-Period	See IEEE Std 11073-20601a-2010—this indicates the duration of exercise.	M
Basic-Nu-Observed-Value	See IEEE Std 11073-20601a-2010—this indicates the intensity of exercise ranging from 0 to 100.	M

NOTE—See IEEE Std 11073-20601a-2010 for information on whether an attribute is static or dynamic.

The context exercise numeric object does not support any methods, events, or other services.

If the Exercise value is entered manually, the mss-cat-manual bit shall be set in Metric-Spec-Small as well.

6.6.5 Context medication

Treatment for diabetes is most effective when the effects of medication on blood glucose levels are monitored. The ability to track medication with a test result can inform a physician as to whether a particular medication or a combination of medicines is effective. Table 10 identifies the values a person can enter on the glucose device to record his or her medication regimen.

Table 10—Context medication numeric object attributes

Attribute name	Extended configuration	
	Value	Qual.
Type	{MDC_PART_PHD_DM, MDC_CTXT_MEDICATION}.	M
Metric-Id	MDC_CTXT_MEDICATION_RAPIDACTING or MDC_CTXT_MEDICATION_SHORTACTING or MDC_CTXT_MEDICATION_INTERMEDIATEACTING or MDC_CTXT_MEDICATION_LONGACTING or MDC_CTXT_MEDICATION_PREMIX.	M
Unit-Code	MDC_DIM_MILLI_G or MDC_DIM_MILLI_L.	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	M
Basic-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	M

NOTE—See IEEE Std 11073-20601a-2010 for information on whether an attribute is static or dynamic.

If the Medication value is entered manually, the mss-cat-manual bit shall be set in Metric-Spec-Small as well.

6.6.6 Context carbohydrates

Recording carbohydrates intake can be an important aid in insulin dose management. Whereas there are issues over control of blood glucose, a review of carbohydrates may be helpful in the care and management of the person. Table 11 enables the person to record the amount of carbohydrates ingested as this can directly affect the level of glucose in the blood.

Table 11—Context carbohydrates numeric object attributes

Attribute name	Extended configuration	
	Value	Qual.
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_CARB}.	M
Metric-Id	MDC_CTXT_GLU_CARB_BREAKFAST or MDC_CTXT_GLU_CARB_LUNCH or MDC_CTXT_GLU_CARB_DINNER or MDC_CTXT_GLU_CARB_SNACK or MDC_CTXT_GLU_CARB_DRINK or MDC_CTXT_GLU_CARB_SUPPER or MDC_CTXT_GLU_CARB_BRUNCH	M
Unit-Code	MDC_DIM_G	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	M
Basic-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	M

NOTE—See IEEE Std 11073-20601a-2010 for information on whether an attribute is static or dynamic.

If the Carbohydrates value is entered manually, the mss-cat-manual bit shall be set in Metric-Spec-Small as well.

6.6.7 Control solution

Table 12 summarizes the attributes of the control solution numeric object. In standard configuration 1701 (0x06A5), the control solution numeric object shall be supported by a glucose meter agent.

Table 12—Control solution numeric object attributes

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x06A5)	
	Value	Qual.	Value	Qual.
Handle	See IEEE Std 11073-20601a-2010.	M	2	M
Type	{MDC_PART_SCADA, MDC_CONC_GLU_CONTROL}	M	{MDC_PART_SCADA, MDC_CONC_GLU_CONTROL}	M
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated	M	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated	M
Unit-Code	MDC_DIM_MILLI_G_PER_DL or MDC_DIM_MILLI_MOLE_PERL	M	MDC_DIM_MILLI_G_PER_DL.	M
Attribute-Value-Map	See IEEE Std 11073-20601a-2010.	C	MDC_ATTR_NUM_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_ABS	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	C	See IEEE Std 11073-20601a-2010.	M
Basic-Nu-Observed-Value	See IEEE Std 11073-20601a-2010.	C	See IEEE Std 11073-20601a-2010.	M

A control solution measurement that is above the capabilities of the device sensor shall be indicated with an observed value of +INFINITY, and a control solution measurement that is below the capabilities of the device sensor shall be indicated with an observed value of –INFINITY.

If a device supports the Context Sample Location enumeration object and reports an MDC_CONC_GLU_CONTROL measurement, then the device shall also report a corresponding MDC_CTXT_GLU_SAMPLELOCATION_CTRLsolution measurement.

6.7 Real-time sample array objects

Real-time sample array objects are not required by this standard.

6.8 Enumeration objects

6.8.1 General

The blood glucose meter uses a number of optional enumeration objects to represent data that are related to blood glucose. The nomenclature code to identify the enumeration class is MDC_MOC_VMO_METRIC_ENUM. The attribute structure shown in Table 13 is common to all enumeration types. Subclauses 6.8.2 through 6.8.6 define the precise definitions for each enumeration type and take precedence.

Table 13—Common glucose enumeration object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601a-2010.	M
Type	Defined in each enumeration table below.	M
Supplemental-Types	See IEEE Std 11073-20601a-2010.	NR
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated mss-cat-manual	M
Metric-Structure-Small	See IEEE Std 11073-20601a-2010.	NR
Measurement-Status	See IEEE Std 11073-20601a-2010.	NR
Metric-Id	See IEEE Std 11073-20601a-2010.	NR
Metric-Id-List	See IEEE Std 11073-20601a-2010.	NR
Metric-Id-Partition	See IEEE Std 11073-20601a-2010.	NR
Unit-Code	See IEEE Std 11073-20601a-2010.	NR
Attribute-Value-Map	See IEEE Std 11073-20601a-2010.	C
Source-Handle-Reference	See IEEE Std 11073-20601a-2010.	NR
Label-String	See IEEE Std 11073-20601a-2010.	O
Unit-LabelString	See IEEE Std 11073-20601a-2010.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	R
Relative-Time-Stamp	See IEEE Std 11073-20601a-2010.	O
HiRes-Time-Stamp	See IEEE Std 11073-20601a-2010.	O
Measure-Active-Period	See IEEE Std 11073-20601a-2010.	O
Enum-Observed-Value-Simple-OID	See IEEE Std 11073-20601a-2010.	O
Enum-Observed-Value-Simple-Bit-Str	See IEEE Std 11073-20601a-2010.	O
Enum-Observed-Value-Basic-Bit-Str	See IEEE Std 11073-20601a-2010.	O
Enum-Observed-Value-Simple-Str	See IEEE Std 11073-20601a-2010.	O
Enum-Observed-Value	See IEEE Std 11073-20601a-2010.	O
Enum-Observed-Value-Partition	See IEEE Std 11073-20601a-2010.	O

Subclauses 6.8.2 through 6.8.6 describe the possible uses of the glucose enumeration object. Each use is an instance of the enumeration class with a particular Type value. The interpretation of associated values is dependent on the Type value. The description of each enumeration object defines all the possible states and, where appropriate, its behavior. The respective tables define the glucose enumeration types generated by the agent in response to a change in state.

The enumeration object does not support any methods, events, or other services. Event reports for these objects are generated by the MDS object.

See IEEE Std 11073-20601a-2010 for descriptive explanations on the individual attributes as well as for information on attribute id and attribute type.

6.8.2 Device and sensor status annunciation

The device and sensor status annunciation object allows glucose meter specific errors to be recorded to track important troubleshooting information for manufacturers. Faulty sensor detection and signal irregularities are closely associated with a glucose meter, applicable to telehealth use cases. An Enumeration object fulfills this need.

An additional Enumeration object containing the running status of the device and sensor assembly is also provided. If this object is to be implemented, then the object identifier (OID)-Type and bit assignments shall be implemented as described in this clause. The nomenclature code to identify the enumeration object class is MDC_MOC_VMO_METRIC_ENUM. Refer to Table 14 for the set of attributes of this object.

This object is instantiated only in extended configurations. A manager should support the interpretation of this object to enable reporting of these occurrences. An agent should support this object to transmit these occurrences.

Table 14—Device and sensor annunciation status attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601a-2010.	M
Type	{MDC_PART_PHD_DM, MDC_GLU_METER_DEV_STATUS}	M
Supplemental-Types	See IEEE Std 11073-20601a-2010.	NR
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored- data mss-upd-aperiodic mss-msmt- aperiodic mss-acc-agent-initiated	M
Metric-Structure-Small	See IEEE Std 11073-20601a-2010.	NR
Measurement-Status	See IEEE Std 11073-20601a-2010.	O
Metric-Id	See IEEE Std 11073-20601a-2010.	NR
Metric-Id-List	See IEEE Std 11073-20601a-2010.	NR
Metric-Id-Partition	See IEEE Std 11073-20601a-2010.	NR
Unit-Code	See IEEE Std 11073-20601a-2010.	NR
Attribute-Value-Map	See IEEE Std 11073-20601a-2010.	C
Source-Handle-Reference	See IEEE Std 11073-20601a-2010.	NR
Label-String	See IEEE Std 11073-20601a-2010.	O
Unit-LabelString	See IEEE Std 11073-20601a-2010.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	C
Relative-Time-Stamp	See IEEE Std 11073-20601a-2010.	C
HiRes-Time-Stamp	See IEEE Std 11073-20601a-2010.	C
Enum-Observed-Value-Simple-OID	See IEEE Std 11073-20601a-2010.	O
Enum-Observed-Value-Simple-Bit-Str	See following text.	NR
Enum-Observed-Value-Basic-Bit-Str	See following text.	R
Enum-Observed-Value-Simple-Str	See IEEE Std 11073-20601a-2010.	NR
Enum-Observed-Value	See following text.	NR
Enum-Observed-Value-Partition	See IEEE Std 11073-20601a-2010.	O

NOTE 1—See IEEE Std 11073-20601a-2010 for information on whether an attribute is static or dynamic.

NOTE 2—See 6.3 for a description of the qualifiers.

An agent explicitly expresses the existence of annunciations by setting the appropriate bits in the Enum-Observed-Value-Basic-Bit-Str attribute, as defined in Table 15. It is recommended to use the Enum-Observed-Value-Basic-Bit-Str attribute as it consumes fewer payload octets than the Enum-Observed-Value-Simple-Bit-Str attribute. The Enum-Observed-Value attribute should not be used, as it unnecessarily complicates the modeling of the object. If a manager supports the interpretation of this object, it shall be able to interpret the entire set of presented conditions. An agent may implement any subset of these same conditions. Note that a manager shall interpret these bits only within the context of this attribute and only within this device specialization as other specializations may use corresponding terms for different purposes.

Table 15—Mapping of device, sensor, and signal status to object Bit-Str attribute

Device or sensor condition	GlucoseDevStat mnemonic
Agent reports that the battery is low and needs replacing.	device-battery-low
Agent reports that the sensor is malfunctioning or faulting.	sensor-malfunction
Agent reports that there is not enough blood/control solution on the strip.	sensor-sample-size-insufficient
Agent reports that the strip was inserted incorrectly.	sensor-strip-insertion
Agent reports that the strip is not the right type for the device.	sensor-strip-type-incorrect
Agent reports that the reading or value is higher than the sensor can process.	sensor-result-too-high
Agent reports that the reading or value is lower than the sensor can process.	sensor-result-too-low
Agent reports that the ambient temperature is too high for a valid test/result.	sensor-temp-too-high
Agent reports that the ambient temperature is too low for a valid test/result.	sensor-temp-too-low
Agent reports that the reading was interrupted or the strip was pulled too soon.	sensor-read-interrupt
A general device fault has occurred in the agent.	device-gen-fault

The specific bit mappings of GlucoseDevStat are defined in Annex B.

6.8.3 Context meal

A blood sugar measurement (or referred to as a reading) may be further associated with information on meal relationship when this measurement is taken. The blood sugar level can be significantly affected by the testing time relative to the meal time. Table 16 defines the meal condition at the time when the blood sugar measurement is taken.

Table 16—Context meal enumeration object attributes

Attribute name	Extended configuration	
	Value	Qual.
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_MEAL}.	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	M
Enum-Observed-Value-Simple-OID	One of the following nomenclature value shall be used: MDC_CTXT_GLU_MEAL_PREPRANDIAL MDC_CTXT_GLU_MEAL_POSTPRANDIAL MDC_CTXT_GLU_MEAL_FASTING MDC_CTXT_GLU_MEAL_BEDTIME. MDC_CTXT_GLU_MEAL_CASUAL.	M

6.8.4 Context sample location

A blood sugar measurement may be further characterized by the blood sample location. Table 17 defines the possible blood locations where the blood sample may be taken.

Table 17—Context sample location enumeration object attributes

Attribute name	Extended configuration	
	Value	Qual.
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_SAMPLELOCATION}	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	M
Enum-Observed-Value-Simple-OID	One of the following nomenclature value shall be used: MDC_CTXT_GLU_SAMPLELOCATION_FINGER MDC_CTXT_GLU_SAMPLELOCATION_AST MDC_CTXT_GLU_SAMPLELOCATION_EARLOBE MDC_CTXT_GLU_SAMPLELOCATION_CTRLsolution	M

6.8.5 Context tester

The precision (or validity) of a blood sugar measurement can be impacted by whom and where the measurement is performed. Table 18 defines the possible cases of testers who may perform the blood sugar measurement.

Table 18—Context tester enumeration object attributes

Attribute name	Extended configuration	
	Value	Qual.
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_TESTER}	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	M
Enum-Observed-Value-Simple-OID	One of the following nomenclature value shall be used: MDC_CTXT_GLU_TESTER_SELF MDC_CTXT_GLU_TESTER_HCP MDC_CTXT_GLU_TESTER_LAB	M

6.8.6 Context health

Stress is an important factor when monitoring blood sugar levels, as excessive stress can cause these levels to rise. Stress hormones such as epinephrine and cortisol are released and, as a result, can significantly raise the blood sugar levels. Table 19 defines the various levels of health a person feels when taking a glucose measurement. Although the state of health is a matter of perception, it enables a dialog between patient and physician to discuss matters that may affect therapy. Minor and major are related to the general health or the level of illness of the person. Menses refers to the female menstrual cycle, and stress refers to physiological or psychological stress. In the event of multiple readings, the most impactful on the result shall be noted.

Table 19—Context health enumeration object attributes

Attribute name	Extended configuration	
	Value	Qual.
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_HEALTH}	M
Absolute-Time-Stamp	See IEEE Std 11073-20601a-2010.	M
Enum-Observed-Value-Simple-OID	One of the following nomenclature value shall be used: MDC_CTXT_GLU_HEALTH_MINOR MDC_CTXT_GLU_HEALTH_MAJOR MDC_CTXT_GLU_HEALTH_MENSES MDC_CTXT_GLU_HEALTH_STRESS MDC_CTXT_GLU_HEALTH_NONE	M

6.9 PM-store objects

6.9.1 General

In the context of personal health devices, glucose meters are highly portable due to their convenient sizes and are normally carried around with users so that blood glucose measurements may be taken as needed. More often than not, blood glucose measurements are taken at a time when out of the network and when manager/agent associations cannot be established. It is also common that a given set of measurements made by glucose meters may need to be uploaded to more than one manager, for example, in the home and at a medical facility.

To support dual usage, an agent may provide two or more configurations. One configuration may use a temporary measurement storage model that uploads the most recent data immediately on association (agent initiated) with little user intervention, such as might be used by a typical home user that uploads measurements frequently to a personal computer or a mobile device such as a cell phone. Another

configuration may use a long-term measurement storage model that uploads data at the request of the manager, such as might be used by the patient’s physician or other health care professionals.

The long-term storage model is realized using PM-stores. Any configuration that does not include a PM-store object utilizes agent-initiated event reports to transmit the observations. The use of temporarily stored data as defined in IEEE Std 11073-20601a-2010 is most useful for small numbers of measurements and is subject to automatic deletion during upload.

Alternatively, in the case where a large number of measurements may be stored or if automatic deletion is to be avoided, a PM-store configuration should be used. Any configuration with a PM-store for persistent storage shall disable agent-initiated transmission and shall enable access to the PM-store transmissions. As a result, this standard describes a mechanism using PM-store to hold measurements for longer durations. The data held in PM-store objects are deleted by user actions via the manager or user interface on the device, and the capacity is limited only by the amount of memory.

6.9.2 Persistent store model

The PM-store model utilizes a PM-segment for each type of object to be persistently stored (see Figure 2). The segment holding glucose readings shall be present if the PM-store is implemented. The other segments are optional and hold observations from the supporting medical context objects that are implemented. Each entry shall include one of the time formats in the segm-entry-header so a manager can correlate entries across the different segments. Entries in the supported medical context PM-segments do not require a correlating result in the GlucoseSeg PM-segment and can therefore be independent of a glucose measurement. This model was selected to reduce the transmission sizes as much as possible. If a particular medical context object is not supported, then the segment is not required to exist. If a person does not enter any data of that type when a reading is taken (e.g., the person does not respond to a prompt for what was eaten recently), then the entry in the PM-segment is not created. The PM-segments that are zero to many in Figure 2 behave this way because of the unknown number of time stamp changes, which are used to determine a common notion of time.

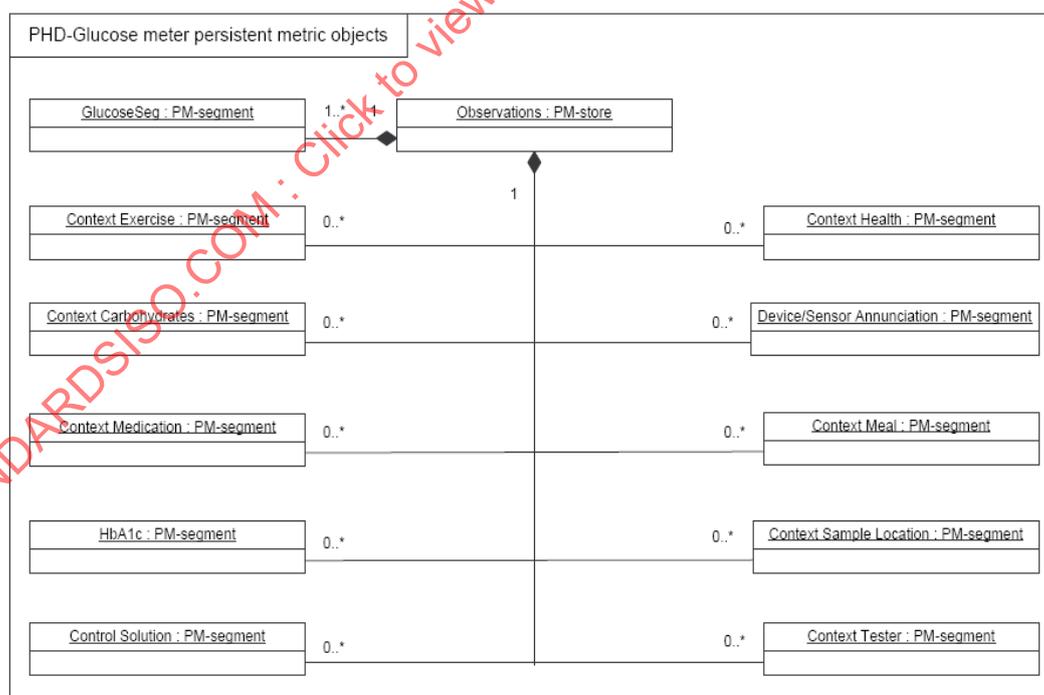


Figure 2—Glucose meter—persistent store model

6.9.3 PM-store object attributes

Table 20 defines the attributes of the PM-store objects that shall be implemented by the agent. The nomenclature code to identify the PM-store objects is MDC_MOC_VMO_PMSTORE.

Table 20—Glucose meter PM-store object attributes

Attribute name	Extended configuration	
	Value	Qual.
Handle	See IEEE Std 11073-20601a-2010.	M
PM-Store-Capab	See IEEE Std 11073-20601a-2010.	M
Store-Sample-Algorithm	See IEEE Std 11073-20601a-2010.	M
Store-Capacity-Count	See IEEE Std 11073-20601a-2010.	M
Store-Usage-Count	See IEEE Std 11073-20601a-2010.	M
Operational-State	See IEEE Std 11073-20601a-2010.	M
PM-Store-Label	See IEEE Std 11073-20601a-2010.	M
Sample-Period	See IEEE Std 11073-20601a-2010.	NR
Number-Of-Segments	Number dependent on context support or time changes.	M
Clear-Timeout	See IEEE Std 11073-20601a-2010.	M

Some considerations when using the PM-Store-Capab are as follows:

- If the agent creates new segments because of time changes as described in the “Comparable time” clause of IEEE Std 11073-20601a-2010, then pmsc-var-no-of-segm shall be set.
- If the agent is recording episodic data in the PM-store, then the pmsc-epi-seg-entries shall be set.
- The remaining bits are agent specific.

6.9.4 PM-store object methods

Table 21 defines the methods of the PM-store objects.

Table 21—Glucose meter PM-store object methods

Service	Subservice type name	Mode	Subservice type (action-type)	Parameters (action-info-args)	Results (action-info-args)
ACTION	Clear-Segments	Confirmed	MDC_ACT_SEG_CLR	SegmSelection	
ACTION	Get-Segment-Info	Confirmed	MDC_ACT_SEG_GET_INFO	SegmSelection	SegmentInfoList
ACTION	Trig-Segment-Data-Xfer	Confirmed	MDC_ACT_SEG_TRIG_XFER	TrigSegmDataXferReq	TrigSegmDataXferRsp

Clear-Segments

This method allows the manager to delete the data currently stored in one or more selected PM-segments. All entries in the selected PM-segments are deleted.

Get-Segment-Info

This method allows the manager to retrieve the PM-segment attributes.

Trig-Segment-Data-Xfer

This method allows the manager to initiate the transfer of the data entries stored in the PM-segment object.

6.9.5 PM-store object events

Table 22 defines the events sent by the PM-store objects.

Table 22—Glucose meter PM-store object events

Service	Subservice type name	Mode	Subservice type (event-type)	Parameters (event-info)	Results (event-reply-info)
EVENT REPORT	Segment-Data-Event	Confirmed	MDC_NOTI_SEGMENT_DATA	SegmentDataEvent	SegmentDataResult

Segment-Data-Event

This event allows the agent to send the data entries stored in the PM-segment object. This event is triggered by the manager using the Trig-Segment-Data-Xfer action.

6.9.6 PM-store object services

6.9.6.1 GET service

The PM-store object supports the GET service to retrieve the values of all PM-store object attributes. The GET service may be invoked as soon as the agent is in the Operating state.

6.9.7 PM-segment objects

Each of the PM-store objects contains a corresponding PM-segment object.

Table 23 defines the attributes of the PM-segment object contained in the PM-store object that represents the stored glucose measurements. The nomenclature code to identify the PM-segment object class is MDC_MOC_PM_SEGMENT.

Table 23—Common PM-segment object attributes

Attribute name	Extended configuration	
	Value	Qual.
Instance Number	See IEEE Std 11073-20601a-2010.	M
PM-Segment-Entry-Map	See IEEE Std 11073-20601a-2010.	M
PM-Seg-Person-Id	See IEEE Std 11073-20601a-2010.	C
Sample-Period	See IEEE Std 11073-20601a-2010.	C
Operational-State	See IEEE Std 11073-20601a-2010.	M
Segment-Label	See IEEE Std 11073-20601a-2010.	M
Segment-Start-Abs-Time	See IEEE Std 11073-20601a-2010.	M
Segment-End-Abs-Time	See IEEE Std 11073-20601a-2010.	M
Segment-Date-and-Time-Adjustment	See IEEE Std 11073-20601a-2010.	C
Segment-Usage-Count	See IEEE Std 11073-20601a-2010.	M
Segment-Statistics	See IEEE Std 11073-20601a-2010.	O
Fixed-Segment-Data	Segment data transferred as an array of entries in a format as specified in the PM-Segment-Entry-Map attribute.	M
Confirm-Timeout	See IEEE Std 11073-20601a-2010.	O
Transfer-Timeout	See IEEE Std 11073-20601a-2010.	M

The Fixed-Segment-Data attribute stores the actual measurements or context logs. When the Fixed-Segment-Data attribute is transmitted, all entries in the event report are formatted according to the PM-Segment-Entry-Map. Each entry stores a single sample point, which may consist of a set of attributes.

6.10 Scanner objects

Scanner objects are not required by this standard.

6.11 Class extension objects

In this standard, no class extension objects are defined with respect to IEEE Std 11073-20601a-2010.

6.12 Glucose meter information model extensibility rules

The glucose meter domain information model of this standard may be extended by including vendor-specific metrics and attributes as required. For example, a vendor might include a cholesterol measurement in addition to the glucose measurement. Any object or attribute extensions implemented should follow the guidelines of this standard as closely as possible.

A glucose meter agent having a configuration with extensions beyond the standard configuration, as specified in this standard, shall use a configuration ID in the range of IDs reserved for extended configurations (see IEEE Std 11073-20601a-2010).

7. Glucose meter service model

7.1 General

The service model defines the conceptual mechanisms for data exchange services. These services are mapped to messages that are exchanged between the agent and the manager. Protocol messages within the ISO/IEEE 11073 series of standards are defined in ASN.1. See IEEE Std 11073-20601a-2010 for a detailed description of the personal health device service model. Subclauses 7.2 and 7.3 define the specifics of object access and event reporting services for a glucose meter agent according to this standard.

7.2 Object access services

The object access services of IEEE Std 11073-20601a-2010 are used to access the objects defined in the domain information model of the glucose device.

The following generic object access services are supported by a glucose meter agent according to this standard:

- GET service: used by the manager to retrieve the values of the agent MDS and PM-store object attributes. The list of glucose meter MDS object attributes is given in 6.5.4.1, and the list of glucose meter PM Store attributes is given in 6.9.3.
- SET service: used by the manager to set the values of the agent object attributes. No settable attributes are defined for a glucose meter agent according to this standard.
- Event report service: used by the agent to send configuration reports and measurement data to the manager. The list of event reports for the glucose meter device specialization is given in 6.5.3.

- Action service: used by the manager to invoke actions (or methods) supported by the agent. An example is Set-Time action, which is used to set a real-time clock with the absolute time at the agent.

Table 24 summarizes the object access services described in this standard.

7.3 Object access event report services

The event report service (see Table 24) is used by the agent to report its information (e.g., measurements). Event reports in this standard are a property of the MDS object only. The event reports used in this standard are defined in IEEE Std 11073-20601a-2010.

The following conditions apply for a glucose meter agent according to this standard:

- Event reports shall be used in confirmed mode.
- Agent-initiated mode shall be supported for measurement data transmission.

A glucose meter agent designed to operate in an environment where data may be collected from multiple people may use one of the multiple-person event report styles to transmit all the data from each person in a single event. If this functionality is not required, the agent may use the single-person event report styles, which have reduced overhead.

A manager shall support both single-person and multiple-person event reports. A glucose meter agent may support either one or both single-person and multiple-person event reports. The formats for single- and multiple-person reports are described in IEEE Std 11073-20601a-2010.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2014

Table 24—Glucose meter object access services

Service	Subservice type name	Mode	Subservice type	Parameters	Result	Remarks
GET	<na>	<implied Confirmed>	<na>	GetArgumentSimple = (obj-handle = 0), attribute-id-list <optional>	GetResultSimple = (obj-handle = 0), attribute-list	Allows the manager to retrieve the value of an attribute of an object in the agent.
	<na>	<implied Confirmed>	<na>	GetArgumentSimple = (obj-handle = <i>handle of PM-Store object</i>), attribute-id-list <optional>	GetResultSimple = (obj-handle = <i>handle of PM-Store object</i>), attribute-list	Allows the manager to retrieve the values of all PM-store object attributes.
EVENT REPORT	MDS-Configuration-Event	Confirmed	MDC_NOTI_CONFIG	ConfigReport	ConfigReportRsp	Configuration Report to inform manager of the agent's configuration.
	MDS-Dynamic-Data-Update-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_FIXED	ScanReportInfoFixed	—	Data Report to provide dynamic data to manager for some or all of the agent's objects in fixed format.
	MDS-Dynamic-Data-Update-Var	Confirmed	MDC_NOTI_SCAN_REPORT_VAR	ScanReportInfoVar	—	Data Report to provide dynamic data to manager for some or all of the agent's objects in variable format.
	MDS-Dynamic-Data-Update-MP-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_MP_FIXED	ScanReportInfoMPFixed	—	This is the same as MDS-Dynamic-Data-Update-Fixed but allows inclusion of data from multiple people.
	MDS-Dynamic-Data-Update-MP-Var	Confirmed	MDC_NOTI_SCAN_REPORT_MP_VAR	ScanReportInfoMPVar	—	This is the same as MDS-Dynamic-Data-Update-Var but allows inclusion of data from multiple people.
ACTION	Set-Time	Confirmed	MDC_ACT_SET_TIME	SetTimeInvoke	—	Manager method to invoke the agent to set time to requested value.
	Clear-Segments	Confirmed	MDC_ACT_SEG_CLR	SegmSelection	—	Allows the manager to clear some or all of the entries contained in PM-segment objects.
	Get-Segment-Info	Confirmed	MDC_ACT_SEG_GET_INFO	SegmSelection	SegmentInfoList	Allows the manager to retrieve information about some or all PM-segment objects.
	Trig-Segment-Data-Xfer	Confirmed	MDC_ACT_SEG_TRIG_XFER	TrigSegmDataXferReq	TrigSegmDataXferRsp	Allows the manager to begin sending segment data.

8. Glucose meter communication model

8.1 Overview

This clause describes the general communication model and procedures of the glucose meter agent as defined in IEEE Std 11073-20601a-2010. Therefore, the respective parts of IEEE Std 11073-20601a-2010 are not reproduced; rather, the specific choices and restrictions with respect to optional elements (e.g., objects, attributes, and actions) and specific extensions (e.g., nomenclature terms) are specified.

For an illustrative overview of the various message transactions during a typical measurement session, see the sequence diagram for the example use case in Annex D and the corresponding protocol data unit (PDU) examples in Annex E.

8.2 Communication characteristics

In this subclause, limits on the size of an application protocol data unit (APDU) transmitted or to be received by a glucose agent are defined. Small limits allow for simple implementations in terms of low cost and complexity.

A glucose agent implementing only this device specialization shall not transmit any APDU larger than N_{tx} and shall be capable of receiving any APDU up to a size of N_{rx} . For this standard, N_{tx} shall be 64 512 octets for implementations supporting persistent metric storage. In the absence of the persistent metric storage capability, N_{tx} shall be 5120 octets. For this standard, N_{rx} shall be 224 octets.

For a glucose agent implementing functions from other device specializations, an upper bound estimation of the APDU sizes brings the following: An agent shall not transmit any APDU larger than the sum of N_{tx} of all the device specializations implemented and shall be capable of receiving any APDU up to the sum of N_{rx} of all the device specializations implemented. If these numbers are higher than the maximum size determined in IEEE Std 11073-20601a-2010, the latter shall be applied.

In case the APDU size limit does not allow for the inclusion of a certain amount of multiple pending measurements at the agent, they shall be sent using multiple event reports. See 8.5.3 for the maximum number of measurements allowed for inclusion in a single event report.

8.3 Association procedure

8.3.1 General

Unless otherwise stated, the association procedure for a glucose meter agent and manager according to this standard shall be pursued as specified in IEEE Std 11073-20601a-2010.

8.3.2 Agent procedure—association request

In the association request sent by the agent to the manager:

- The version of the association procedure used by the agent shall be set to *assoc-version1* (i.e., *assoc-version* = 0x80000000).
- The *DataProtoList* structure element of the data protocol identifier shall be set to *data-proto-id-20601* (i.e., *data-proto-id* = 0x5079).
- The *data-proto-info* field shall contain a *PhdAssociationInformation* structure that shall contain the following parameter values:

- 1) The agent shall support protocol-version1. Support for any other version may be indicated by setting additional bits. When protocols higher than protocol-version1 are used, the agent shall continue to use only features as specified in this standard.
- 2) At least the MDERs shall be supported (i.e., *encoding-rules* = 0x8000).
- 3) The version of the nomenclature used shall be set to nom-version1 (i.e., *nomenclature-version* = 0x80000000).
- 4) The field *functional-units* may have the test association bits set but shall not have any other bits set.
- 5) The field *system-type* shall be set to sys-type-agent (i.e., *system-type* = 0x00800000).
- 6) The *system-id* field shall be set to the value of the System-Id attribute of the MDS object of the agent. The manager may use this field to determine the identity of the glucose meter with which it is associating and, optionally, to implement a simple access restriction policy.
- 7) The *dev-config-id* field shall be set to the value of the Dev-Configuration-Id attribute of the MDS object of the agent.
- 8) If the agent supports only the glucose meter specialization, then the field indicating the data request modes (*data-req-mode-capab*) supported by the glucose meter agent shall be set to *data-req-supp-init-agent*.
- 9) If the agent supports only the glucose meter specialization, then *data-req-init-manager-count* shall be set to zero, and *data-req-init-agent-count* shall be set to 1.

8.3.3 Manager procedure—association response

In the association response message sent by the manager:

- The *result* field shall be set to an appropriate response from those defined in IEEE Std 11073-20601a-2010. For example, if all other conditions of the association protocol are satisfied, *accepted* is returned when the manager recognizes the *dev-config-id* of the agent and *accepted-unknown-config* otherwise.
- In the DataProtoList structure element, the data protocol identifier shall be set to data-proto-id-20601 (i.e., *data-proto-id* = 0x5079).
- The *data-proto-info* field shall be filled in with a PhdAssociationInformation structure that shall contain the following parameter values:
 - 1) The manager following this specialization shall support protocol-version1. The manager may support additional protocol versions and select them if the agent offers them.
 - 2) The manager shall respond with a single selected encoding rule that is supported by both agent and manager. The manager shall support at least the MDERs.
 - 3) The version of the nomenclature used shall be set to nom-version1 (i.e., *nomenclature-version* = 0x80000000).
 - 4) The field *functional-units* shall have all bits reset except for those relating to a test association.
 - 5) The field *system-type* shall be set to sys-type-manager (i.e., *system-type* = 0x80000000).
 - 6) The *system-id* field shall contain the unique system ID of the manager, which shall be a valid EU1-64 type identifier.
 - 7) The field *dev-config-id* shall be manager-config-response (0).
 - 8) The field *data-req-mode-capab* shall be 0.
 - 9) The fields *data-req-init-*-count* shall be 0.

8.4 Configuring procedure

8.4.1 General

The agent enters the Configuring state if it receives an association response of accepted-unknown-config. In this case, the configuration procedure as specified in IEEE Std 11073-20601a-2010 shall be followed. Subclause 8.4.2 specifies the configuration notification and response messages for a glucose meter agent with standard configuration ID 0x06A4 (1700), and 8.4.3 specifies the configuration notification and response messages for a glucose meter agent with standard configuration ID 0x06A5 (1701). Normally, a manager would already know the standard configuration. However, standard configuration devices are required to send their configuration, if requested. This covers a case where an agent associates with a manager that does not have preconfigured knowledge of the standard configuration (e.g., due to a version mismatch between agent and manager).

The agent shall support the GET service for the MDS attributes during the Configuring state.

8.4.2 Glucose meter—standard configuration (0x06A4)

8.4.2.1 Agent procedure

The agent performs the configuration procedure using a “Remote Operation Invoke | Confirmed Event Report” message with an MDC_NOTI_CONFIG event to send its configuration to the manager (see IEEE Std 11073-20601a-2010). The ConfigReport structure is used for the *event-info* field (see Table 4). For a glucose meter agent with standard configuration ID 0x06A4, the format and contents of the configuration notification message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x44	CHOICE.length = 68
0x00 0x42	OCTET STRING.length = 66
0x00 0x02	invoke-id (differentiates this message from any other outstanding)
0x01 0x01	CHOICE(Remote Operation Invoke Confirmed Event Report)
0x00 0x3C	CHOICE.length = 60
0x00 0x00	obj-handle = 0 (MDS object)
0xFF 0xFF 0xFF 0xFF	event-time (set to 0xFFFFFFFF if RelativeTime is not supported)
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x32	event-info.length = 50 (start of ConfigReport)
0x06 0xA4	config-report-id (Dev-Configuration-Id value)
0x00 0x01	config-obj-list.count = 1 Measurement object will be “announced”
0x00 0x2C	config-obj-list.length = 44
0x00 0x06	obj-class = MDC_MOC_VMO_METRIC_NU
0x00 0x01	obj-handle = 1 (→ 1 st Measurement is blood glucose)
0x00 0x04	attributes.count = 4
0x00 0x24	attributes.length = 36
0x09 0x2F	attribute-id = MDC_ATTR_ID_TYPE
0x00 0x04	attribute-value.length = 4
0x00 0x02	MDC_PART_SCADA
0x71 0xB8	MDC_CONC_GLU_CAPILLARY_WHOLEBLOOD
0x0A 0x46	attribute-id = MDC_ATTR_METRIC_SPEC_SMALL

0x00 0x02	attribute-value.length = 2
0xF0 0x40	intermittent, stored data, upd & msmt aperiodic, agent init, measured
0x09 0x96	attribute-id = MDC_ATTR_UNIT_CODE
0x00 0x02	attribute-value.length = 2
0x08 0x52	MDC_DIM_MILLI_G_PER_DL
0x0A 0x55	attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00 0x0C	attribute-value.length = 12
0x00 0x02	AttrValMap.count = 2
0x00 0x08	AttrValMap.length = 8
0x0A 0x4C 0x00 0x02	MDC_ATTR_NU_VAL_OBS_BASIC value length = 2
0x09 0x90 0x00 0x08	MDC_ATTR_TIME_STAMP_ABS value length = 8

8.4.2.2 Manager procedure

The manager shall respond to a configuration notification message using a “Remote Operation Response | Confirmed Event Report” data message with an MDC_NOTI_CONFIG event using the ConfigReportRsp structure for the *event-info* field (see Table 4). As a response to the standard configuration notification message in 8.4.2.1, the format and contents of the manager’s configuration notification response message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x16	CHOICE.length = 22
0x00 0x14	OCTET STRING.length = 20
0x00 0x02	invoke-id (differentiates this message from any other outstanding)
0x02 0x01	CHOICE (Remote Operation Response Confirmed Event Report)
0x00 0x0E	CHOICE.length = 14
0x00 0x00	obj-handle = 0 (MDS object)
0x05 0x14 0xDB 0x12	currentTime
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x04	event-reply-info.length = 4
0x06 0xA4	ConfigReportRsp.config-report-id = 1700
0x00 0x00	ConfigReportRsp.config-result = accepted-config

8.4.3 Glucose meter—standard configuration (0x06A5)

8.4.3.1 Agent procedure

The agent performs the configuration procedure using a “Remote Operation Invoke | Confirmed Event Report” message with an MDC_NOTI_CONFIG event to send its configuration to the manager (see IEEE Std 11073-20601a-2010). The ConfigReport structure is used for the *event-info* field (see Table 4). For a glucose meter agent with standard configuration ID 0x06A5, the format and contents of the configuration notification message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x44	CHOICE.length = 68
0x00 0x42	OCTET STRING.length = 66
0x00 0x02	invoke-id (differentiates this message from any other outstanding)
0x01 0x01	CHOICE (Remote Operation Invoke Confirmed Event Report)
0x00 0x3C	CHOICE.length = 60
0x00 0x00	obj-handle = 0 (MDS object)
0xFF 0xFF 0xFF 0xFF	event-time (set to 0xFFFFFFFF if RelativeTime is not supported)
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x32	event-info.length = 50 (start of ConfigReport)

0x06	0xA5	config-report-id (Dev-Configuration-Id value)		
0x00	0x01	config-obj-list.count = 1 Measurement object will be “announced”		
0x00	0x2C	config-obj-list.length = 44		
0x00	0x06	obj-class = MDC_MOC_VMO_METRIC_NU		
0x00	0x01	obj-handle = 1 (→ 1 st Measurement is blood glucose)		
0x00	0x04	attributes.count = 4		
0x00	0x24	attributes.length = 36		
0x09	0x2F	attribute-id = MDC_ATTR_ID_TYPE		
0x00	0x04	attribute-value.length = 4		
0x00	0x02	MDC_PART_SCADA		
0x72	0x70	MDC_CONC_GLU_UNDETERMINED_PLASMA		
0x0A	0x46	attribute-id = MDC_ATTR_METRIC_SPEC_SMALL		
0x00	0x02	attribute-value.length = 2		
0xF0	0x40	intermittent, stored data, upd & msmt aperiodic, agent init, measured		
0x09	0x96	attribute-id = MDC_ATTR_UNIT_CODE		
0x00	0x02	attribute-value.length = 2		
0x08	0x52	MDC_DIM_MILLI_G_PER_DL		
0x0A	0x55	attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP		
0x00	0x0C	attribute-value.length = 12		
0x00	0x02	AttrValMap.count = 2		
0x00	0x08	AttrValMap.length = 8		
0x0A	0x4C	0x00	0x02	MDC_ATTR_NU_VAL_OBS_BASIC value length = 2
0x09	0x90	0x00	0x08	MDC_ATTR_TIME_STAMP_ABS value length = 8

8.4.3.2 Manager procedure

The manager shall respond to a configuration notification message using a “Remote Operation Response | Confirmed Event Report” data message with an MDC_NOTI_CONFIG event using the ConfigReportRsp structure for the *event-info* field (see Table 4). As a response to the standard configuration notification message in 8.4.3.1, the format and contents of the manager’s configuration notification response message are as follows:

0xE7	0x00	APDU CHOICE Type (PrstApu)		
0x00	0x16	CHOICE.length = 22		
0x00	0x14	OCTET STRING.length = 20		
0x00	0x02	invoke-id (differentiates this message from any other outstanding)		
0x02	0x01	CHOICE (Remote Operation Response Confirmed Event Report)		
0x00	0x0E	CHOICE.length = 14		
0x00	0x00	obj-handle = 0 (MDS object)		
0x05	0x14	0xDB	0x12	currentTime
0x0D	0x1C	event-type = MDC_NOTI_CONFIG		
0x00	0x04	event-reply-info.length = 4		
0x06	0xA5	ConfigReportRsp.config-report-id = 1701		
0x00	0x00	ConfigReportRsp.config-result = accepted-config		

8.5 Operating procedure

8.5.1 General

Measurement data and status information are communicated from the glucose meter agent during the Operating state. If not stated otherwise, the operating procedure for a glucose meter agent of this standard shall be as specified in IEEE Std 11073-20601a-2010.

8.5.2 GET glucose meter MDS and PM-store attributes

The glucose meter shall support the GET service for MDS and PM-store objects (if it has PM-store objects) according to IEEE Std 11073-20601a-2010.

See Table 5 for a summary of the GET service.

If the manager leaves the *attribute-id-list* field in the roiv-cmip-get service message empty, the glucose meter agent shall respond with a rors-cmip-get service message in which the attribute-list contains a list of all implemented attributes of the MDS object. This allows the glucose meter agent to store a predefined transmission template for its response message and to modify just the varying parts at fixed locations before sending.

If the manager requests specific MDS object attributes, indicated by the elements in *attribute-id-list*, and the agent supports this capability, the glucose meter agent shall respond with a rors-cmip-get service message in which the attribute-list contains a list of the requested attributes of the MDS object that are implemented. It is not required for a glucose meter agent to support this capability. If this capability is not implemented, the glucose meter agent shall respond with a “Remote Operation Error Result” (roer) service message (see IEEE Std 11073-20601a-2010) with the error-value field set to no-such-action (9).

8.5.3 Measurement data transmission

See Table 4 and Table 22 for a summary of the event report services available for measurement data transfer.

For temporary store measurement, data transfer for a glucose meter agent of this standard shall always be initiated by the glucose meter (see agent-initiated measurement data transmission in IEEE Std 11073-20601a-2010). To limit the amount of data being transported within an APDU, the glucose meter agent shall not include more than 25 temporarily stored measurements in a single event report. If more than 25 pending measurements are available for transmission, they shall be sent using multiple event reports. If multiple glucose measurements are available, up to 25 measurements should be transmitted within a single event report. Alternatively, they may be transmitted using a single event report for each glucose measurement. However, the former strategy is recommended to reduce overall message size and power consumption.

A glucose meter agent with standard configuration shall use the fixed format data update messages method for transmitting measurement data. A glucose meter agent with extended configuration may use either fixed or variable format data update messages for transmitting measurement data.

For PM-store transfers, the manager inspects the available segments and retrieves all applicable data.

8.6 Time synchronization

Time synchronization may be employed between a glucose meter and a manager to coordinate the clocks used when reporting physiological events. Note that the mechanism for synchronizing an agent to a manager is outside the scope of this standard. If time synchronization is used, then this shall be reported in the Mds-Time-Info attribute of the MDS object.

9. Test associations

A glucose meter may implement a wide range of behaviors in a test association that enable a manufacturer to test features of a product in a comprehensive manner. It is also possible for a glucose meter not to support test associations at all. This clause defines a simple behavior that simulates the generation of a measurement in the context of a standard device configuration.

9.1 Behavior with standard configuration

To facilitate automated standardized test processes, a glucose meter that presents the standard configuration ID and enters into a test association should be able to simulate the arrival of measurement data from the device measurement engine. It should not be necessary for an operator to perform a test for the measurement data to be generated.

After the agent enters the operating state, it simulates the reception of an event from the measurement engine representing a blood glucose measurement of 999 mg/dL. To the extent possible, this measurement is observed only by those components of the agent that understand the test association. When the event is propagated into a numeric object, the test-data bit of the measurement-status attribute shall be set if the measurement-status attribute is supported. An agent is not required to use the measurement-status attribute if it would not normally do so outside of a test association.

The agent should send the events reports for all simulated measures within 30 s of entering the Operating state. The test association is terminated in a manner consistent with the agent's normal behavior for terminating an association.

9.2 Behavior with extended configurations

This specification does not define a test association that uses an extended configuration.

10. Conformance

10.1 Applicability

This standard shall be used in conjunction with IEEE Std 11073-20601a-2010.

An implementation or a system can conform to the following elements of this standard:

- Domain information model class hierarchy and object definitions (object attributes, notifications, methods, and data type definitions)
- Nomenclature code values
- Protocol and service models
- Communication service model (association and configuration)

10.2 Conformance specification

This standard offers levels of conformance with respect to strict adherence to the standard device and the use of extensions for:

- Information model of a specific device
- Use of attributes, value ranges, and access methods

A vendor shall specify the level of conformance for an implementation based on this standard and provide details of the way in which the definitions of this standard and any extensions are applied.

Specifications shall be provided in the form of a set of implementation conformance statements (ICS) as detailed in 10.4.

Because this standard is used in conjunction with IEEE Std 11073-20601a-2010, the ICS should be created for this standard first. The ICS created for IEEE Std 11073-20601a-2010 may then refer to the ICS for this standard where applicable.

10.3 Levels of conformance

10.3.1 General

This standard defines the following levels of conformance.

10.3.2 Conformance level 1: Base conformance

The application uses elements of the information, service, and communication models (object hierarchy, actions, event reports, and data type definitions) and the nomenclature scheme defined in IEEE Std 11073-20601a-2010 and ISO/IEEE 11073-104zz standards. All mandatory features defined in the object definition tables and in the ICS tables are implemented. Furthermore, any conditional, recommended, or optional features that are implemented shall follow the requirements in IEEE Std 11073-20601a-2010 and ISO/IEEE 11073-104zz documents.

10.3.3 Conformance level 2: Extended nomenclature (ASN.1 and/or ISO/IEEE 11073-10101:2004 [B2])

Conformance level 2 meets conformance level 1 but also uses or adds extensions in at least one of the information, service, communication, or nomenclature models. These extensions shall conform to nomenclature codes from ASN.1 and/or within the ISO/IEEE 11073-10101:2004 [B2] framework (0xF000 – 0xFFFF). These extensions should be defined in ICS tables pointing toward their reference.

10.4 Implementation conformance statements

10.4.1 General format

The ICSs are provided as an overall conformance statement document that comprises a set of tables in the form given by the templates in the following clauses.

Each ICS table has the following columns:

Index	Feature	Reference	Req/Status	Support	Comment
-------	---------	-----------	------------	---------	---------

The table column headings have the following meaning:

- Index: an identifier (e.g., a tag) of a specific feature.
- Feature: briefly describes the characteristic for which a conformance statement is being made.
- Reference: to the clause/paragraph within this document or to an external source for the definition of the feature (may be empty).
- Req/Status: specifies the conformance requirement (e.g., mandatory or recommended)—in some cases, this standard does not specify conformance requirements but requests the status of a particular feature be provided.
- Support: specifies the presence or absence of a feature and any description of the characteristics of the feature in the implementation. This column is to be filled out by the implementer.
- Comment: contains any additional information on the feature. This column is to be filled out by the implementer.

Subclauses 10.4.2 to 10.4.6 specify the format of the specific ICS tables.

10.4.2 General implementation conformance statement

The general ICS specifies the versions/revisions that are supported by the implementation and high-level system behavior.

Table 25 shows the general ICSs.

Table 25—11073-10417 general ICS table

Index ^a	Feature	Reference	Req./Status	Support	Comment
GEN 11073-10417-1	Implementation Description	—	Identification of the device/ application. Description of functionality.		
GEN 11073-10417-2	Standards followed and their revisions	(standard documents)	(set of existing revisions)	(set of supported revision)	
GEN 11073-10417-3	Nomenclature document used and revision	(standard documents)	(set of existing revisions)	(set of supported revisions)	
GEN 11073-10417-4	Conformance Adherence - Level 1 -	See 10.3.3	Base conformance declaration that device meets the following IEEE Std 11073-10417 conformance requirements: a) All mandatory requirements shall be implemented. b) If implemented, conditional, recommended, and optional requirements shall conform to standard.	Yes/No (No is not expected as No implies that the implementation is non-conformant)	
GEN 11073-10417-5	Conformance Adherence - Level 2 -	See 6.3	In addition to GEN 11073-10417-4, if the device implements extensions and/or additions, they shall conform to nomenclature codes from ASN.1 and/or 10101 framework. These extensions should also be defined in ICS tables pointing toward their reference.	Yes/No	
GEN 11073-10417-6	Object Containment Tree	See 6.3	Provide Object Containment Diagram showing relations between object instances used by the application. A conforming implementation uses only object relations as defined in the DIM.		
GEN 11073-10417-7	Nomenclature document used and revision	(standard documents)	(set of existing revisions)	(set of supported revision)	

Index ^a	Feature	Reference	Req./Status	Support	Comment
GEN 11073-10417-8	Data Structure Encoding	—	—	Description of encoding method(s) for ASN.1 data structures	
GEN 11073-10417-9	Use of Private Objects	—	Does the implementation use objects that are not defined in the DIM?	Yes/No (If yes: explain in Table 26)	
GEN 11073-10417-10	Use of Private Nomenclature Extensions	—	Does the implementation use private extensions to the nomenclature (i.e., 0xF000-0xFFFF codes from ISO/IEEE 11073-10101:2004 [B2])? Private Nomenclature extensions are <i>only</i> allowed if the standard nomenclature does not include the specific terms required by the application.	Yes/No (If yes: explain in Table 29)	
GEN 11073-10417-11	11073-20601 Conformance		Provide the conformance report required by IEEE Std 11073-20601a-2010.		

^a The prefix GEN11073-10417- is used for the index in the general ICS table.

10.4.3 DIM MOC implementation conformance statement

The DIM MOC ICS defines which objects are implemented. Information on each object shall be provided as a separate row in the template of Table 26.

Table 26—Template for DIM MOC ICS table

Index	Feature	Reference	Req./Status	Support	Comment
MOC- <i>n</i>	Object description	Reference to the clause in the standard or other location where the object is defined.	Implemented	Specify restrictions, e.g., max. number of supported instances	

The *n* in the Index column should be the object handle for implementations that have predefined objects. Otherwise the Index column shall simply be a unique number (1..*m*).

All private objects should be specified and include either a reference to the definition for the object, or where no publicly available reference is available, the definition of the object should be appended to the conformance statement.

The Support column should indicate any restrictions for the object implementation.

An object containment diagram (class instance diagram) should be provided as part of the DIM MOC ICS.

10.4.4 MOC attribute ICS

For each supported object as defined in the DIM MOC ICS, a MOC attribute ICS has to be provided that defines which attributes are used/supported by the implementation, including any inherited attributes. Table 27 is a template only.

Table 27—Template for MOC attribute ICS table

Index	Feature	Reference	Req./Status	Support	Comment
ATTR- <i>n-x</i>	Attribute Name. Extended attributes shall include the Attribute ID also.	Fill in the reference to the ASN.1 structure if the attribute is not defined in this standard.	M = Mandatory / C = Conditional / R = Recommended / O = Optional (as per definition in Attribute Definition Tables)	Implemented? Yes/No Static/Dynamic Specify restrictions (e.g., value ranges). Describe how attribute is accessed (e.g. Get, Set, sent in config event report, sent in a data event report). Describe any specific restrictions.	

All private attributes should be specified and include reference to the definition for the attribute. Where no publicly available reference is available, the definition of the attribute should be appended to the conformance statement.

The Support column shall specify whether the attribute is implemented; for extension attributes, whether the attribute value is static or dynamic; any value ranges; restrictions on attribute access or availability; and any other information.

The *n* in the Index column refers to the ID of the managed object for which the table is supplied (i.e., the index of the managed object as specified in the MOC ICS). There is one separate table for each supported managed object.

The *x* in the Index column is a unique serial number (1..*m*).

NOTE—The attribute definition tables in the standard define a minimum mandatory set of attributes for each object.

10.4.5 MOC notification implementation conformance statement

The MOC notification ICS specifies all implemented notifications (typically in form of the event report service) that are emitted by the agent. Table 28 provides a template for use. One table has to be provided for each object that supports special object notifications.

Table 28—Template for MOC notification ICS table

Index	Feature	Reference	Req./Status	Support	Comment
NOTI- <i>n-x</i>	Notification Name and Notification ID	Reference to the clause in the standard or other location where the event is defined.		The Support column shall specify how the notification is sent and any restrictions.	

The *n* in the Index column refers to the ID of the managed object for which the table is supplied (i.e., the index of the managed object as specified in the POC ICS). There is one separate table for each managed object that supports specific object notifications (i.e., events).

The *x* in the Index column is a unique serial number (1..*m*).

All private notifications should be specified and include reference to the definition for the notification. Where no publicly available reference is available, the definition of the notification should be appended to the conformance statement.

10.4.6 MOC nomenclature conformance statement

The MOC nomenclature ICS specifies all nonstandard nomenclature codes that are utilized by the agent. Table 29 provides a template for use. One row of the table is to be used for each nomenclature element.

Table 29—Template for MOC nomenclature ICS table

Index	Feature	Reference	Req./Status	Support	Comment
NOME- <i>n</i>	Nomenclature Name and Nomenclature value	Reference to the clause in the standard or other location where the nomenclature is defined or used.		Describe how the nomenclature is used. Describe any specific restrictions.	

The *n* in the Index column is a unique serial number (1..*m*).

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2014

Annex A

(informative)

Bibliography

Bibliographical references are resources that provide additional or helpful material but do not need to be understood or used to implement this standard. Reference to these resources is made for informational use only.

[B1] American Diabetes Association, “Standards of medical care in diabetes—2006,” *Diabetes Care*, vol. 29, suppl. 1, Jan. 2006.

[B2] ISO/IEEE 11073-10101:2004, Health informatics—Point-of-care medical device communication—Part 10101: Nomenclature.⁸

[B3] ISO/IEEE 11073-10201:2004, Health informatics—Point-of-care medical device communication—Part 10201: Domain information model.

[B4] ISO/IEEE 11073-20101:2004, Health informatics—Point-of-care medical device communication—Part 20101: Application profile—Base standard.

[B5] ITU-T Rec. X.680-2002, Information technology—Abstract Syntax Notation One (ASN.1): Specification of basic notation.⁹

⁸ ISO/IEEE publications are available from the ISO Central Secretariat, 1, ch. de la Voie-Creuse, Case postale 56, CH-1211, Geneva 20, Switzerland (<http://www.iso.ch/>). ISO/IEEE publications are also available in the United States from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, Piscataway, NJ 08854-4141, USA (<http://standards.ieee.org/>).

⁹ ITU publications are available from the International Telecommunications Union, Place des Nations, 1211 Geneva 20, Switzerland (<http://www.itu.in/>).

Annex B

(normative)

Any additional ASN.1 definitions

B.1 Device and sensor status bit mapping

The threshold extensions to the Enumeration class require the following four ASN.1 structure definitions:

```
GlucoseDevStat ::= BITS-16 {  
    device-battery-low(0),  
    sensor-malfunction(1),  
    sensor-sample-size-insufficient(2),  
    sensor-strip-insertion(3),  
    sensor-strip-type-incorrect(4),  
    sensor-result-too-high(5),  
    sensor-result-too-low(6),  
    sensor-temp-too-high(7),  
    sensor-temp-too-low(8),  
    sensor-read-interrupt(9),  
    device-gen-fault(10)  
}
```

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2014

Annex C

(normative)

Allocation of identifiers

C.1 General

This annex contains the nomenclature codes used in this document and not found in IEEE Std 11073-20601a-2010. For those not contained in this annex, the normative definition is found in IEEE Std 11073-20601a-2010.

C.2 Definitions of terms and codes

The format used here follows that of ISO/IEEE 11073-10101:2004 [B2].

```
/*
* From Medical supervisory control and data acquisition (MDC_PART_SCADA)
*/
#define MDC_CONC_GLU_GEN 28948/* */
#define MDC_CONC_GLU_CAPILLARY_WHOLEBLOOD 29112/* */
#define MDC_CONC_GLU_CAPILLARY_PLASMA 29116/* */
#define MDC_CONC_GLU_VENOUS_WHOLEBLOOD 29120/* */
#define MDC_CONC_GLU_VENOUS_PLASMA 29124/* */
#define MDC_CONC_GLU_ARTERIAL_WHOLEBLOOD 29128/* */
#define MDC_CONC_GLU_ARTERIAL_PLASMA 29132/* */
#define MDC_CONC_GLU_UNDETERMINED_WHOLEBLOOD 29292/* */
#define MDC_CONC_GLU_UNDETERMINED_PLASMA 29296/* */
#define MDC_CONC_GLU_CONTROL 29136/* */
#define MDC_CONC_GLU_ISF 29140/* */
#define MDC_CONC_HBA1C 29148/* */

/*
* From Personal Health Device Disease Management (MDC_PART_PHD_DM)
*/
#define MDC_GLU_METER_DEV_STATUS 29144/* */
#define MDC_CTXT_GLU_EXERCISE 29152/* */
#define MDC_CTXT_GLU_CARB 29156/* */
#define MDC_CTXT_GLU_CARB_BREAKFAST 29160/* */
#define MDC_CTXT_GLU_CARB_LUNCH 29164/* */
#define MDC_CTXT_GLU_CARB_DINNER 29168/* */
#define MDC_CTXT_GLU_CARB_SNACK 29172/* */
#define MDC_CTXT_GLU_CARB_DRINK 29176/* */
#define MDC_CTXT_GLU_CARB_SUPPER 29180/* */
#define MDC_CTXT_GLU_CARB_BRUNCH 29184/* */
#define MDC_CTXT_MEDICATION 29188/* */
#define MDC_CTXT_MEDICATION_RAPIDACTING 29192/* */
#define MDC_CTXT_MEDICATION_SHORTACTING 29196/* */
#define MDC_CTXT_MEDICATION_INTERMEDIATEACTING 29200/* */
#define MDC_CTXT_MEDICATION_LONGACTING 29204/* */
#define MDC_CTXT_MEDICATION_PREMIX 29208/* */
#define MDC_CTXT_GLU_HEALTH 29212/* */
#define MDC_CTXT_GLU_HEALTH_MINOR 29216/* */
```

```
#define MDC_CTXT_GLU_HEALTH_MAJOR          29220/* */
#define MDC_CTXT_GLU_HEALTH_MENSES        29224/* */
#define MDC_CTXT_GLU_HEALTH_STRESS        29228/* */
#define MDC_CTXT_GLU_HEALTH_NONE          29232/* */
#define MDC_CTXT_GLU_SAMPLELOCATION         29236/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_FINGER  29240/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_AST     29244/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_EARLOBE 29248/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_CTRLsolution 29252/* */
#define MDC_CTXT_GLU_MEAL                  29256/* */
#define MDC_CTXT_GLU_MEAL_PREPRANDIAL      29260/* */
#define MDC_CTXT_GLU_MEAL_POSTPRANDIAL     29264/* */
#define MDC_CTXT_GLU_MEAL_FASTING          29268/* */
#define MDC_CTXT_GLU_MEAL_BEDTIME         29300/* */
#define MDC_CTXT_GLU_MEAL_CASUAL           29272/* */
#define MDC_CTXT_GLU_TESTER                29276/* */
#define MDC_CTXT_GLU_TESTER_SELF           29280/* */
#define MDC_CTXT_GLU_TESTER_HCP            29284/* */
#define MDC_CTXT_GLU_TESTER_LAB            29288/* */
```

```
/* From Dimensions (MDC_PART_DIM)
*****
#define MDC_DIM_MILLI_L          1618 /* mL */
#define MDC_DIM_MILLI_G          1746 /* mg */
#define MDC_DIM_MILLI_G_PER_DL   2130 /* mg dL-1 */
#define MDC_DIM_MILLI_MOLE_PER_L 4722 /* mmol L-1 */
#define MDC_DIM_G                1728 /* g */
```

C.3 Systematic derivations of terms and codes

Systematic name	Common term	Acronym	Description/definition	Reference ID	Code
Glucose Concentration ControlSolution	Control Result		Object containing measurement produced from control solution	MDC_CONC_GLU_CONTROL	29136
Glucose Concentration InterstitialFluid	Interstitial Fluid Glucose		Object containing glucose measurement obtained from interstitial fluid	MDC_CONC_GLU_ISF	29140
HbA1c Concentration	HbA1c		Object containing A1c or glycated hemoglobin	MDC_CONC_HBA1C	29148
Status value FunctionalStatus Device	Device Status		Object containing glucose device specific status flags	MDC_GLU_METER_DEV_STATUS	29144
Glucose Context Exercise	Exercise		Object containing contextual information related to the effect of exercise on glucose level	MDC_CTXT_GLU_EXERCISE	29152
Glucose Context Carb	Carbohydrates		Object containing contextual information related to the effect of carbohydrates on glucose level	MDC_CTXT_GLU_CARB	29156
Medication Context	Medication		Object containing contextual information related to the effect of	MDC_CTXT_MEDICATION	29188

Systematic name	Common term	Acronym	Description/definition	Reference ID	Code
			medication on glucose level		
Glucose Context Health	Level of Health		Object containing contextual information related to the effect of health on glucose level	MDC_CTXT_GLU_HEALTH	29212
Glucose Context SampleLocation	Sample Location		Object specifying location of test performed	MDC_CTXT_GLU_SAMPLELOCATION	29236
Glucose Context Samplelocation Alternativesitetest	Alternative Site test of sample location		Object specifying that the location of test performed was from an alternative site on the body	MDC_CTXT_GLU_SAMPLELOCATION_AST	29244
Glucose Context Meal	Meal Relationship		Object containing contextual information related to the effect of food intake on glucose level	MDC_CTXT_GLU_MEAL	29256
Glucose Context Meal BeforeMeal	Pre-Meal Relationship		Object containing contextual information related to the effect of between-meal food intake on glucose level	MDC_CTXT_GLU_MEAL_PREPRANDIAL	29260
Glucose Context Meal AfterMeal	Post-Meal Relationship		Object containing contextual information related to the effect of diet on glucose level	MDC_CTXT_GLU_MEAL_POSTPRANDIAL	29264
Glucose Context Meal Fasting	Fasting Relationship		Object containing contextual information related to the effect of long-term absence of food intake (overnight) on glucose level	MDC_CTXT_GLU_MEAL_FASTING	29268
Glucose Context Meal Bedtime	Bedtime Relationship		Object containing contextual information related to the effect of evening food intake on glucose level	MDC_CTXT_GLU_MEAL_BEDTIME	29300
Glucose Context Tester	Tester		Object containing contextual information related to a third party conducting the test	MDC_CTXT_GLU_TESTER	29276
Glucose Context Tester HealthCareProfessional	Health Care Professional Tester		Object containing contextual information related to a health care professional conducting the test	MDC_CTXT_GLU_TESTER_HCP	29284

Annex D

(informative)

Message sequence examples

Figure D.1 shows a sequence diagram of the messaging procedure corresponding to the following use case. The user of a glucose meter agent device intends to connect it to a manager for the first time. The glucose meter is capable of performing glucose measurements. Thus, it operates as an extended configuration.

- a) When the user connects the glucose meter, the manager does not yet know the agent's configuration and sends a response to the agent's association request with the result *accepted-unknown-config*. See E.2.2.2 and E.2.2.3 for the corresponding PDU examples.
- b) As a consequence of this, the agent negotiates its configuration information to the manager. After getting confirmation from the manager accepting the agent's configuration, the agent device is ready to send measurements. Both devices enter the Operating state. See E.3.2.2 and E.3.2.3 for the corresponding PDU examples.
- c) Subsequently, the manager may request the MDS object attributes of the agent by sending a data message with the "Remote Operation Invoke | Get" command. As a response, the agent reports its MDS object attributes to the manager using a data message with the "Remote Operation Response | Get" command. See E.4.1.2 and E.4.1.3 for the corresponding PDU examples.
- d) If the measurement was not taken prior to association, as a next step, the user of the agent device takes a single measurement. The measurement data are transmitted to the manager using a confirmed event report. After having successfully received the measurement data, the manager sends a confirmation to the agent. See E.5.1 and E.5.2 for the corresponding PDU examples.
- e) The user ends the measurement session (e.g., by pushing a proper button on the device, or just by not using the device for a duration longer than a certain time period). As a consequence, the agent disassociates from the manager by sending an association release request. The manager responds with an association release response. See E.6.1 and E.6.2 for the corresponding PDU examples.
- f) When the agent requests to associate to the manager for the next measurement session (e.g., the next day), the result in the manager's response is *accepted*, as it already knows the agent's configuration from the previous measurement session. Both devices transition directly to the Operating state.
- g) Finally, the last two steps shown are similar as in item d) and item e). The user takes a single confirmed measurement followed by releasing the association.