
**Health informatics — Personal health
device communication —**

Part 10417:

Device specialization — Glucose meter

*Informatique de santé — Communication entre dispositifs médicaux sur le site
des soins —*

Partie 10417: Spécialisation des dispositifs — Glucomètre



STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017



COPYRIGHT PROTECTED DOCUMENT

© IEEE 2015

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO or IEEE at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Institute of Electrical and Electronics Engineers, Inc
3 Park Avenue, New York
NY 10016-5997, USA

stds.ipr@ieee.org
www.ieee.org

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

IEEE Standards documents are developed within the IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (IEEE-SA) Standards Board. The IEEE develops its standards through a consensus development process, approved by the American National Standards Institute, which brings together volunteers representing varied viewpoints and interests to achieve the final product. Volunteers are not necessarily members of the Institute and serve without compensation. While the IEEE administers the process and establishes rules to promote fairness in the consensus development process, the IEEE does not independently evaluate, test, or verify the accuracy of any of the information contained in its standards.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is called to the possibility that implementation of this standard may require the use of subject matter covered by patent rights. By publication of this standard, no position is taken with respect to the existence or validity of any patent rights in connection therewith. ISO/IEEE is not responsible for identifying essential patents or patent claims for which a license may be required, for conducting inquiries into the legal validity or scope of patents or patent claims or determining whether any licensing terms or conditions provided in connection with submission of a Letter of Assurance or a Patent Statement and Licensing Declaration Form, if any, or in any licensing agreements are reasonable or non-discriminatory. Users of this standard are expressly advised that determination of the validity of any patent rights, and the risk of infringement of such rights, is entirely their own responsibility. Further information may be obtained from ISO or the IEEE Standards Association.

ISO/IEEE 11073-10417 was prepared by the 11073 Committee of the Engineering in Medicine and Biology Society of the IEEE (as IEEE Std 11073-10417-2015). It was adopted by Technical Committee ISO/TC 215, *Health informatics*, in parallel with its approval by the ISO member bodies, under the “fast-track procedure” defined in the Partner Standards Development Organization cooperation agreement between ISO and IEEE. Both parties are responsible for the maintenance of this document.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017

IEEE Std 11073-10417™-2015

(Revision of
IEEE Std 11073-10417-2011)

Health informatics—Personal health device communication

Part 10417: Device Specialization— Glucose Meter

Sponsor

IEEE 11073™ Standards Committee
of the
IEEE Engineering in Medicine and Biology Society

Approved 11 June 2015

IEEE-SA Standards Board

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017

Abstract: Within the context of the ISO/IEEE 11073 family of standards for device communication, a normative definition of communication between personal telehealth glucose meter devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes) is established by this standard in a manner that enables plug-and-play interoperability. Appropriate portions of existing standards are leveraged, including ISO/IEEE 11073 terminology, information models, application profile standards, and transport standards. The use of specific term codes, formats, and behaviors in telehealth environments restricting optionality in base frameworks in favor of interoperability are specified. A common core of communication functionality for personal telehealth glucose meters is defined in this standard.

Keywords: glucose meter, IEEE 11073-10417™, medical device communication, personal health devices

The Institute of Electrical and Electronics Engineers, Inc.
3 Park Avenue, New York, NY 10016-5997, USA

Copyright © 2015 by The Institute of Electrical and Electronics Engineers, Inc. All rights reserved. Published 2 July 2015. Printed in the United States of America.

IEEE is a registered trademark in the U.S. Patent & Trademark Office, owned by The Institute of Electrical and Electronics Engineers, Incorporated.

PDF: ISBN 978-0-7381-9746-3 STD20244
Print: ISBN 978-0-7381-9747-0 STDPD20244

IEEE prohibits discrimination, harassment, and bullying.

For more information, visit <http://www.ieee.org/web/aboutus/whatis/policies/p9-26.html>.

No part of this publication may be reproduced in any form, in an electronic retrieval system or otherwise, without the prior written permission of the publisher.

Important Notices and Disclaimers Concerning IEEE Standards Documents

IEEE documents are made available for use subject to important notices and legal disclaimers. These notices and disclaimers, or a reference to this page, appear in all standards and may be found under the heading “Important Notice” or “Important Notices and Disclaimers Concerning IEEE Standards Documents.”

Notice and Disclaimer of Liability Concerning the Use of IEEE Standards Documents

IEEE Standards documents (standards, recommended practices, and guides), both full-use and trial-use, are developed within IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (“IEEE-SA”) Standards Board. IEEE (“the Institute”) develops its standards through a consensus development process, approved by the American National Standards Institute (“ANSI”), which brings together volunteers representing varied viewpoints and interests to achieve the final product. Volunteers are not necessarily members of the Institute and participate without compensation from IEEE. While IEEE administers the process and establishes rules to promote fairness in the consensus development process, IEEE does not independently evaluate, test, or verify the accuracy of any of the information or the soundness of any judgments contained in its standards.

IEEE does not warrant or represent the accuracy or content of the material contained in its standards, and expressly disclaims all warranties (express, implied and statutory) not included in this or any other document relating to the standard, including, but not limited to, the warranties of: merchantability; fitness for a particular purpose; non-infringement; and quality, accuracy, effectiveness, currency, or completeness of material. In addition, IEEE disclaims any and all conditions relating to: results; and workmanlike effort. IEEE standards documents are supplied “AS IS” and “WITH ALL FAULTS.”

Use of an IEEE standard is wholly voluntary. The existence of an IEEE standard does not imply that there are no other ways to produce, test, measure, purchase, market, or provide other goods and services related to the scope of the IEEE standard. Furthermore, the viewpoint expressed at the time a standard is approved and issued is subject to change brought about through developments in the state of the art and comments received from users of the standard.

In publishing and making its standards available, IEEE is not suggesting or rendering professional or other services for, or on behalf of, any person or entity nor is IEEE undertaking to perform any duty owed by any other person or entity to another. Any person utilizing any IEEE Standards document, should rely upon his or her own independent judgment in the exercise of reasonable care in any given circumstances or, as appropriate, seek the advice of a competent professional in determining the appropriateness of a given IEEE standard.

IN NO EVENT SHALL IEEE BE LIABLE FOR ANY DIRECT, INDIRECT, INCIDENTAL, SPECIAL, EXEMPLARY, OR CONSEQUENTIAL DAMAGES (INCLUDING, BUT NOT LIMITED TO: PROCUREMENT OF SUBSTITUTE GOODS OR SERVICES; LOSS OF USE, DATA, OR PROFITS; OR BUSINESS INTERRUPTION) HOWEVER CAUSED AND ON ANY THEORY OF LIABILITY, WHETHER IN CONTRACT, STRICT LIABILITY, OR TORT (INCLUDING NEGLIGENCE OR OTHERWISE) ARISING IN ANY WAY OUT OF THE PUBLICATION, USE OF, OR RELIANCE UPON ANY STANDARD, EVEN IF ADVISED OF THE POSSIBILITY OF SUCH DAMAGE AND REGARDLESS OF WHETHER SUCH DAMAGE WAS FORESEEABLE.

Translations

The IEEE consensus development process involves the review of documents in English only. In the event that an IEEE standard is translated, only the English version published by IEEE should be considered the approved IEEE standard.

Official statements

A statement, written or oral, that is not processed in accordance with the IEEE-SA Standards Board Operations Manual shall not be considered or inferred to be the official position of IEEE or any of its committees and shall not be considered to be, or be relied upon as, a formal position of IEEE. At lectures, symposia, seminars, or educational courses, an individual presenting information on IEEE standards shall make it clear that his or her views should be considered the personal views of that individual rather than the formal position of IEEE.

Comments on standards

Comments for revision of IEEE Standards documents are welcome from any interested party, regardless of membership affiliation with IEEE. However, IEEE does not provide consulting information or advice pertaining to IEEE Standards documents. Suggestions for changes in documents should be in the form of a proposed change of text, together with appropriate supporting comments. Since IEEE standards represent a consensus of concerned interests, it is important that any responses to comments and questions also receive the concurrence of a balance of interests. For this reason, IEEE and the members of its societies and Standards Coordinating Committees are not able to provide an instant response to comments or questions except in those cases where the matter has previously been addressed. For the same reason, IEEE does not respond to interpretation requests. Any person who would like to participate in revisions to an IEEE standard is welcome to join the relevant IEEE working group.

Comments on standards should be submitted to the following address.

Secretary, IEEE-SA Standards Board
445 Hoes Lane
Piscataway, NJ 08854 USA

Laws and regulations

Users of IEEE Standards documents should consult all applicable laws and regulations. Compliance with the provisions of any IEEE Standards document does not imply compliance to any applicable regulatory requirements. Implementers of the standard are responsible for observing or referring to the applicable regulatory requirements. IEEE does not, by the publication of its standards, intend to urge action that is not in compliance with applicable laws, and these documents may not be construed as doing so.

Copyrights

IEEE draft and approved standards are copyrighted by IEEE under U.S. and international copyright laws. They are made available by IEEE and are adopted for a wide variety of both public and private uses. These include both use, by reference, in laws and regulations, and use in private self-regulation, standardization, and the promotion of engineering practices and methods. By making these documents available for use and adoption by public authorities and private users, IEEE does not waive any rights in copyright to the documents.

Photocopies

Subject to payment of the appropriate fee, IEEE will grant users a limited, non-exclusive license to photocopy portions of any individual standard for company or organizational internal use or individual, non-commercial use only. To arrange for payment of licensing fees, please contact Copyright Clearance Center, Customer Service, 222 Rosewood Drive, Danvers, MA 01923 USA; +1 978 750 8400. Permission to photocopy portions of any individual standard for educational classroom use can also be obtained through the Copyright Clearance Center.

Updating of IEEE Standards documents

Users of IEEE Standards documents should be aware that these documents may be superseded at any time by the issuance of new editions or may be amended from time to time through the issuance of amendments, corrigenda, or errata. An official IEEE document at any point in time consists of the current edition of the document together with any amendments, corrigenda, or errata then in effect.

Every IEEE standard is subjected to review at least every ten years. When a document is more than ten years old and has not undergone a revision process, it is reasonable to conclude that its contents, although still of some value, do not wholly reflect the present state of the art. Users are cautioned to check to determine that they have the latest edition of any IEEE standard.

In order to determine whether a given document is the current edition and whether it has been amended through the issuance of amendments, corrigenda, or errata, visit the IEEE-SA Website at <http://ieeexplore.ieee.org/xpl/standards.jsp> or contact IEEE at the address listed previously. For more information about the IEEE-SA or IEEE's standards development process, visit the IEEE-SA Website at <http://standards.ieee.org>.

Errata

Errata, if any, for all IEEE standards can be accessed on the IEEE-SA Website at the following URL: <http://standards.ieee.org/findstds/errata/index.html>. Users are encouraged to check this URL for errata periodically.

Patents

Attention is called to the possibility that implementation of this standard may require use of subject matter covered by patent rights. By publication of this standard, no position is taken by the IEEE with respect to the existence or validity of any patent rights in connection therewith. If a patent holder or patent applicant has filed a statement of assurance via an Accepted Letter of Assurance, then the statement is listed on the IEEE-SA Website at <http://standards.ieee.org/about/sasb/patcom/patents.html>. Letters of Assurance may indicate whether the Submitter is willing or unwilling to grant licenses under patent rights without compensation or under reasonable rates, with reasonable terms and conditions that are demonstrably free of any unfair discrimination to applicants desiring to obtain such licenses.

Essential Patent Claims may exist for which a Letter of Assurance has not been received. The IEEE is not responsible for identifying Essential Patent Claims for which a license may be required, for conducting inquiries into the legal validity or scope of Patents Claims, or determining whether any licensing terms or conditions provided in connection with submission of a Letter of Assurance, if any, or in any licensing agreements are reasonable or non-discriminatory. Users of this standard are expressly advised that determination of the validity of any patent rights, and the risk of infringement of such rights, is entirely their own responsibility. Further information may be obtained from the IEEE Standards Association.

Participants

At the time this IEEE standard was completed, the Personal Health Devices Working Group had the following membership:

Daidi Zhong, Chair
Michael J. Kirwan, Chair
Raymond A. Strickland, Vice-Chair
Craig Carlson, Vice-Chair

Karsten Aalders	Seungchul Chae	Eric Freudenthal
Charles R. Abbruscato	Rahul Chauhan	Matthias Frohner
Nabil Abujbara	James Cheng	Ndifor Cyril Fru
Maher Abuzaid	Peggy Chien	Ken Fuchs
James Agnew	David Chiu	Jing Gao
Haidar Ahmad	Chia-Chin Chong	Xuemei Gao
Manfred Aigner	Saeed A. Choudhary	Marcus Garbe
Jorge Alberola	Jinhan Chung	John Garguilo
Murtaza Ali	Malcolm Clarke	Rick Geimer
Rolf Ambuehl	John A. Cogan	Igor Gejdos
David Aparisi	John T. Collins	Ferenc Gerbovics
Lawrence Arne	Cory Condek	Nicolae Goga
Diego B. Arquillo	Todd H. Cooper	Julian Goldman
Serafin Arroyo	David Cornejo	Raul Gonzalez Gomez
Muhammad Asim	Douglas Coup	Chris Gough
Merat Bagha	Nigel Cox	Channa Gowda
Doug Baird	Hans Crommenacker	Charles M. Gropper
David Baker	Tomio Crosley	Amit Gupta
Anindya Bakshi	David Culp	Jeff Guttmacher
Ananth Balasubramanian	Allen Curtis	Rasmus Haahr
Sunlee Bang	Eyal Dassau	Christian Habermann
M. Jonathan Barkley	David Davenport	Michael Hagerty
Gilberto Barrón	Russell Davis	Jerry Hahn
David Bean	Sushil K. Deka	Robert Hall
John Bell	Ciro de la Vega	Nathaniel Hamming
Rudy Belliardi	Pedro de-las-Heras-Quiros	Rickey L. Hampton
Daniel Bernstein	Jim DelloStritto	Sten Hanke
George A. Bertos	Matthew d'Entremont	Jordan Hartmann
Chris Biernacki	Lane Desborough	Kai Hassing
Ola Bjørsne	Kent Dicks	Marc Daniel Haunschild
Thomas Blackadar	Hyoungdo Do	Wolfgang Heck
Marc Blanchet	Xiaolian Duan	Nathaniel Heintzman
Thomas Bluethner	Brian Dubreuil	Charles Henderson
Douglas P. Bogia	Sourav Dutta	Jun-Ho Her
Xavier Boniface	Jakob Ehrensvarð	Takashi Hibino
Shannon Boucousis	Fredrik Einberg	Timothy L. Hirou
Julius Broma	Roger M. Ellingson	Allen Hobbs
Lyle G. Bullock, Jr.	Michihiro Enokida	Alex Holland
Bernard Burg	Javier Escayola Calvo	Arto Holopainen
Chris Burns	Mark Estes	Kris Holtzclaw
Anthony Butt	Leonardo Estevez	Robert Hoy
Jeremy Byford-Rew	Roger Feeley	Frank Hsu
Satya Calloji	Bosco T. Fernandes	Anne Huang
Carole C. Carey	Christoph Fischer	Sen-Der Huang
Santiago Carot-Nemesio	Morten Flintrup	Zhiqiang Huang
Randy W. Carroll	Joseph W. Forler	Ron Huby
Simon Carter	Russell Foster	David Hughes

Robert D. Hughes	Romain Marmot	Giovanna Sannino
Jiyoung Huh	Sandra Martinez	Jose A. Santos-Cadenas
Hugh Hunter	Miguel Martínez de Espronceda	Stefan Saueremann
Hitoshi Ikeda	Cámara	John Sawyer
Yutaka Ikeda	Peter Mayhew	Guillaume Schatz
Philip O. Isaacson	Jim McCain	Alois Schloegl
Atsushi Ito	László Meleg	Paul S. Schluter
Michael Jaffe	Alexander Mense	Lars Schmitt
Praduman Jain	Ethan Metsger	Mark G. Schnell
Wei Jin	Jinsei Miyazaki	Richard A. Schrenker
Danny Jochelson	Erik Moll	Antonio Scorpiniti
Chris Johnson	Darr Moore	Kwang Seok Seo
Phaneeth Junga	Carsten Mueglitz	Riccardo Serafin
Akiyoshi Kabe	Piotr Murawski	Sid Shaw
Steve Kahle	Soundharya Nagasubramanian	Frank Shen
Tomio Kamioka	Jae-Wook Nah	Liqun Shen
Kei Kariya	Alex Neefus	Bozhi Shi
Andy Kaschl	Trong-Nghia Nguyen-Dobinsky	Min Shih
Junzo Kashihara	Michael E. Nidd	Mazen Shihabi
Kohichi Kashiwagi	Tetsu Nishimura	Redmond Shouldice
Ralph Kent	Jim Niswander	Sternly K. Simon
Laurie M. Kermes	Hiroaki Niwamoto	Marjorie Skubic
Ikuo Keshi	Thomas Norgall	Robert Smith
Junhyung Kim	Anand Noubade	Ivan Soh
Minho Kim	Yoshiteru Nozoe	Motoki Sone
Min-Joon Kim	Abraham Ofek	Emily Sopensky
Taekon Kim	Brett Olive	Rajagopalan Srinivasan
Tetsuya Kimura	Begonya Otal	Andreas Staubert
Alfred Kloos	Charles Palmer	Nicholas Steblay
Jeongmee Koh	Bud Panjwani	Beth Stephen
Jean-Marc Koller	Carl Pantiskas	Lars Steubesand
John Koon	Harry P. Pappas	John (Ivo) Stivoric
Patty Krantz	Mikey Paradis	Raymond A. Strickland
Raymond Krasinski	Hanna Park	Chandrasekaran Subramaniam
Alexander Kraus	Jong-Tae Park	Hermann Suominen
Ramesh Krishna	Myungeun Park	Lee Surprenant
Geoffrey Kruse	Soojun Park	Ravi Swami
Falko Kuester	Phillip E. Pash	Ray Sweidan
Rafael Lajara	TongBi Pei	Jin Tan
Pierre Landau	Lucian Pestritu	Haruyuyki Tatsumi
Jaechul Lee	Soren Petersen	John W. Thomas
JongMuk Lee	James Petisce	Jonas Tirén
Kyong Ho Lee	Peter Piction	Alexandra Todiruta
Rami Lee	Michael Pliskin	James Tomcik
Sungkee Lee	Jeff Price	Janet Traub
Woojae Lee	Harald Prinzhorn	Jesús Daniel Trigo
Yonghee Lee	John Quinlan	Gary Tschautscher
Joe Lenart	Arif Rahman	Masato Tsuchid
Kathryn A. Lesh	Tanzilur Rahman	Ken Tubman
Qiong Li	Steve Ray	Yoshihiro Uchida
Ying Li	Phillip Raymond	Sunil Unadkat
Patrick Lichter	Tim Reilly	Fabio Urbani
Jisoon Lim	Barry Reinhold	Philipp Urbauer
Joon-Ho Lim	Brian Reinhold	Laura Vanzago
John Lin	Melvin I. Reynolds	Alpo Värri
Wei-Jung Lo	John G. Rhoads	Dalimar Velez
Charles Lowe	Jeffrey S. Robbins	Naveen Verma
Don Ludolph	Moskowitz Robert	Rudi Voon
Christian Luszick	Timothy Robertson	Isobel Walker
Bob MacWilliams	David Rosales	David Wang
Srikanth Madhurbootheswaran	Bill Saltzstein	Jerry P. Wang
Miriam L. Makhoul	Benedikt Salzbrunn	Yao Wang

Yi Wang
Steve Warren
Fujio Watanabe
Toru Watsuji
Mike Weng
Kathleen Wible
Paul Williamson

Jan Wittenber
Jia-Rong Wu
Will Wykeham
Ariton Xhafa
Yaxi Yan
Ricky Yang
Melanie S. Yeung

Done-Sik Yoo
Jianchao Zeng
Jason Zhang
Zhiqiang Zhang
Thomas Zhao
Miha Zoubek
Szymon Zyskoter

The following members of the individual balloting committee voted on this standard. Balloters may have voted for approval, disapproval, or abstention.

John Ballingall
Giberto Barrón
Lyle G. Bullock, Jr.
Keith Chow
Joseph El Youssef
Randall Groves
Kai Hassing
Werner Hoelzl

Noriyuki Ikeuchi
Atsushi Ito
Piotr Karocki
Patrick Keith-Hynes
Patrick Kinney
Robert Kircher
Michael J. Kirwan
Nick S. A. Nikjoo

Henry Pinto
Melvin I. Reynolds
Bartien Sayogo
Lars Schmitt
Raymond A. Strickland
Walter Struppeler
Jan Wittenber
Oren Yuen

When the IEEE-SA Standards Board approved this standard on 11 June 2015, it had the following membership:

John Kulick, *Chair*
Jon Walter Rosdahl, *Vice Chair*
Richard H. Hulett, *Past Chair*
Konstantinos Karachalios, *Secretary*

Masayuki Ariyoshi
Ted Burse
Stephen Dukes
Jean-Philippe Faure
J. Travis Griffith
Gary Hoffman
Michael Janezic

Joseph L. Koepfinger*
David I. Law
Hung Ling
Andrew Myles
T. W. Olsen
Glenn Parsons
Ronald C. Petersen
Annette D. Reilly

Stephen J. Shellhammer
Adrian P. Stephens
Yatin Trivedi
Phillip Winston
Don Wright
Yu Yuan
Daidi Zhong

*Member Emeritus

Julie Alessi, *IEEE-SA Content Production and Management*

Kathryn Bennett, *IEEE-SA Operational Program Management*

Introduction

This introduction is not part of IEEE Std 11073-10417™-2015, Health informatics—Personal health device communication—Part 10417: Device Specialization—Glucose Meter.

ISO/IEEE 11073 standards enable communication between medical devices and external computer systems. This document uses the optimized framework created in IEEE Std 11073-20601-2015^a and describes a specific, interoperable communication approach for glucose meters. These standards align with and draw on the existing clinically focused standards to provide support for communication of data from clinical or personal health devices.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017

^aFor information on references, see Clause 2.

Contents

1. Overview	1
1.1 Scope	1
1.2 Purpose	1
1.3 Context	2
2. Normative references.....	2
3. Definitions, acronyms, and abbreviations	2
3.1 Definitions	2
3.2 Acronyms and abbreviations	3
4. Introduction to ISO/IEEE 11073 personal health devices	4
4.1 General	4
4.2 Introduction to IEEE 11073-20601 modeling constructs.....	4
5. Glucose meter device concepts and modalities	5
5.1 General	5
6. Glucose meter domain information model	6
6.1 Overview	6
6.2 Class extensions.....	7
6.3 Object instance diagram	7
6.4 Types of configuration.....	8
6.5 Medical device system object.....	9
6.6 Numeric objects.....	12
6.7 Real-time sample array objects.....	20
6.8 Enumeration objects	20
6.9 PM-store objects.....	25
6.10 Scanner objects.....	29
6.11 Class extension objects.....	29
6.12 Glucose meter information model extensibility rules	29
7. Glucose meter service model.....	29
7.1 General	29
7.2 Object access services.....	29
7.3 Object access event report services	30
8. Glucose meter communication model	32
8.1 Overview	32
8.2 Communication characteristics.....	32
8.3 Association procedure	32
8.4 Configuring procedure.....	34
8.5 Operating procedure	38
8.6 Time synchronization	39
9. Test associations.....	39
9.1 Behavior with standard configuration.....	39
9.2 Behavior with extended configurations	39
10. Conformance	40
10.1 Applicability	40

STANDARD.PDF.COM Click to view the full PDF of ISO/IEEE 11073-10417:2017

10.2 Conformance specification	40
10.3 Levels of conformance	40
10.4 Implementation conformance statements	41
Annex A (informative) Bibliography	45
Annex B (normative) Any additional ASN.1 definitions	46
B.1 Device and sensor status bit mapping	46
Annex C (normative) Allocation of identifiers	47
C.1 General	47
C.2 Definitions of terms and codes	47
C.3 Systematic derivations of terms and codes	48
Annex D (informative) Message sequence examples	51
Annex E (informative) Protocol data unit examples	53
E.1 General	53
E.2 Association information exchange	53
E.3 Configuration information exchange	56
E.4 GET MDS attributes service	59
E.5 Data reporting	61
E.6 Disassociation	62

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017

Health informatics—Personal health device communication

Part 10417: Device Specialization— Glucose Meter

IMPORTANT NOTICE: IEEE Standards documents are not intended to ensure safety, health, or environmental protection, or ensure against interference with or from other devices or networks. Implementers of IEEE Standards documents are responsible for determining and complying with all appropriate safety, security, environmental, health, and interference protection practices and all applicable laws and regulations.

This IEEE document is made available for use subject to important notices and legal disclaimers. These notices and disclaimers appear in all publications containing this document and may be found under the heading “Important Notice” or “Important Notices and Disclaimers Concerning IEEE Documents.” They can also be obtained on request from IEEE or viewed at <http://standards.ieee.org/IPR/disclaimers.html>.

1. Overview

1.1 Scope

Within the context of the ISO/IEEE 11073 family of standards for device communication, this standard establishes a normative definition of communication between personal telehealth glucose meter devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes) in a manner that enables plug-and-play interoperability. It leverages appropriate portions of existing standards, including ISO/IEEE 11073 terminology, information models, application profile standards, and transport standards. It specifies the use of specific term codes, formats, and behaviors in telehealth environments restricting optionality in base frameworks in favor of interoperability. This standard defines a common core of communication functionality for personal telehealth glucose meters.

1.2 Purpose

This standard addresses the need for an openly defined, independent standard that support information exchange to and from personal health devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes). Interoperability is key to growing the potential market for these devices and enabling people to be better informed participants in the management of their health.

1.3 Context

See IEEE Std 11073-20601™-2014¹ for an overview of the environment within which this standard is written.

This standard defines the device specialization for the insulin pump, being a specific agent type, and provides a description of the device concepts, its capabilities, and its implementation according to this standard.

This standard is based on IEEE Std 11073-20601™-2014² which in turn draws information from both ISO/IEEE 11073-10201:2004 [B3]³ and ISO/IEEE 11073-20101:2004 [B4]. The medical device encoding rules (MDERs) used within this standard are fully described in Annex F of IEEE Std 11073-20601-2014.

This standard reproduces relevant portions of the nomenclature found in ISO/IEEE 11073-10101:2004 [B2] and adds new nomenclature codes for the purposes of this standard. Among this standard and IEEE Std 11073-20601-2014, all required nomenclature codes for implementation are documented.

NOTE—In this standard, ISO/IEEE 11073-104zz is used to refer to the collection of device specialization standards that utilize IEEE Std 11073-20601-2014, where zz can be any number from 01 to 99, inclusive.⁴

2. Normative references

The following referenced documents are indispensable for the application of this document (i.e., they must be understood and used, so that each referenced document is cited in text and its relationship to this document is explained). For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments or corrigenda) applies.

IEEE Std 11073-20601-2014, Health informatics—Personal health device communication—Application Profile—Optimized Exchange Protocol.^{5, 6}

3. Definitions, acronyms, and abbreviations

3.1 Definitions

For the purposes of this document, the following terms and definitions apply. The *IEEE Standards Dictionary Online* should be consulted for terms not defined in this clause.⁷

agent: A node that collects and transmits personal health data to an associated manager.

class: In object-oriented modeling, it describes the attributes, methods, and events that objects instantiated from the class utilize.

¹ Information on references can be found in Clause 2.

² ISO/IEEE publications are available from the ISO Central Secretariat, 1, ch. de la Voie-Creuse, Case postale 56, CH-1211, Geneva 20, Switzerland (<http://www.iso.ch/>). ISO/IEEE publications are also available in the United States from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, Piscataway, NJ 08854-4141, USA (<http://standards.ieee.org/>).

³ The numbers in brackets correspond to those of the bibliography in Annex A.

⁴ Notes in text, tables, and figures are given for information only and do not contain requirements needed to implement the standard.

⁵ The IEEE standards or products referred to in this clause are trademarks of the Institute of Electrical and Electronics Engineers, Inc.

⁶ IEEE publications are available from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, Piscataway, NJ 08854-4141, USA (<http://standards.ieee.org/>).

⁷ *IEEE Standards Dictionary Online* subscription is available at:

http://www.ieee.org/portal/innovate/products/standard/standards_dictionary.html.

compute engine: *See:* **manager.**

device: A term used to refer to a physical apparatus implementing either an agent or a manager role.

glucagon: Naturally occurring hormone released by the pancreas when glucose levels are low.

glucose: Commonly referred to as “sugar,” it is the major source of energy used by the body cells.

glucose meter: A medical device for determining the approximate concentration of glucose in the blood.

handle: An unsigned 16-bit number that is locally unique and identifies one of the object instances within an agent.

manager: A node receiving data from one or more agent systems. Some examples of managers include a cellular phone, health appliance, set top box, or computer system.

obj-handle: *See:* **handle.**

object: In object-oriented modeling, a particular instantiation of a class. The instantiation realizes attributes, methods, and events from the class.

occlusion: Total obstruction of the infusion set that prevents administering insulin.

personal health device: A device used in personal health applications.

personal telehealth device: *See:* **personal health device.**

3.2 Acronyms and abbreviations

APDU	application protocol data unit
ASN.1	Abstract Syntax Notation One
AST	alternative site testing
DIM	domain information model
EUI-64	extended unique identifier (64 bits)
HbA1c	hemoglobin bound to glucose (the A1c form)
HCP	health care provider
ICS	implementation conformance statements
ISF	insulin sensitivity factor
MDC	medical device communication
MDER	medical device encoding rules
MDS	medical device system
MOC	managed object class
OID	object identifier
PDU	protocol data unit
PHD	personal health device
VMO	virtual medical object
VMS	virtual medical system

4. Introduction to ISO/IEEE 11073 personal health devices

4.1 General

This standard and the remainder of the series of ISO/IEEE 11073 personal health device (PHD) standards fit in the larger context of the ISO/IEEE 11073 series of standards. The full suite of standards enables agents to interconnect and interoperate with managers and with computerized health-care information systems. See IEEE Std 11073-20601-2014 for a description of the guiding principles for this series of ISO/IEEE 11073 Personal Health Device standards.

IEEE Std 11073-20601-2014 supports the modeling and implementation of an extensive set of personal health devices. This standard defines aspects of the glucose meter device. It describes all aspects necessary to implement the application layer services and data exchange protocol between an ISO/IEEE 11073 PHD glucose meter agent and a manager. This standard defines a subset of the objects and functionality contained in IEEE Std 11073-20601-2014 and extends and adds definitions where appropriate. All new definitions are given in Annex B in Abstract Syntax Notation One (ASN.1). Nomenclature codes referenced in this standard, which are not defined in IEEE Std 11073-20601-2014, are normatively defined in Annex C.

4.2 Introduction to IEEE 11073-20601 modeling constructs

4.2.1 General

The ISO/IEEE 11073 series of standards, and in particular IEEE Std 11073-20601-2014, is based on an object-oriented systems management paradigm. The overall system model is divided into three principal components: the domain information model (DIM), the service model, and the communication model. See IEEE Std 11073-20601-2014 for a detailed description of the modeling constructs.

4.2.2 Domain information model

The DIM is a hierarchical model that describes an agent as a set of objects. These objects and their attributes represent the elements that control behavior and report on the status of the agent and data that an agent can communicate to a manager. Communication between the agent and the manager is defined by the application protocol in the IEEE Std 11073-20601-2014.

4.2.3 Service model

The service model defines the conceptual mechanisms for the data exchange services. Such services are mapped to messages that are exchanged between the agent and the manager. Protocol messages within the ISO/IEEE 11073 series of standards are defined in ASN.1. The messages defined in IEEE Std 11073-20601-2014 can coexist with messages defined in other standard application profiles defined in the ISO/IEEE 11073 series of standards.

4.2.4 Communication model

In general, the communication model supports the topology of one or more agents communicating over logical point-to-point connections to a single manager. For each logical point-to-point connection, the

dynamic system behavior is defined by a connection state machine as specified in IEEE Std 11073-20601-2014.

4.2.5 Implementing the models

An agent implementing this standard shall implement all mandatory elements of the information, service, and communication models as well as all conditional elements where the condition is met. The agent should implement the recommended elements, and it may implement any combination of the optional elements. A manager implementing this standard shall utilize at least one of the mandatory, conditional, recommended, or optional elements. In this context, *utilize* means to use the element as part of the primary function of the manager device. For example, a manager whose primary function is to display data would need to display a piece of data in the element in order to utilize it.

5. Glucose meter device concepts and modalities

5.1 General

This clause presents the general concepts of glucose meters. In the context of personal health devices in this family of standards, a glucose meter is a device that measures the concentration of glucose in the blood. Glucose, or the concentration of blood sugar in the blood, is the primary source of energy for the body's cells. The glucose level is tightly regulated in the human body and is normally maintained between approximately 70 mg/dL and 150 mg/dL (4 mmol/L and 8 mmol/L). The total amount of glucose in the circulating blood is, therefore, approximately 3.5 g to 7.5 g (assuming an ordinary adult blood volume of 5 L). Glucose levels rise after meals and are usually lowest in the morning, before the first meal of the day.

In a healthy adult male of 75 kg with a blood volume of 5 L, a blood glucose level of 100 mg/dL (5.5 mmol/L) corresponds to a total of approximately 5 g (1/5 oz and equivalent to a commercial sugar packet) of glucose in the blood and approximately 45 g (1.5 oz) in the total body fluid (which includes blood and interstitial fluid) and on average will be approximately 60% of the total body weight in men.

The failure to maintain blood glucose in the normal range leads to conditions of persistently high (hyperglycemia) or low (hypoglycemia) blood sugar. Diabetes mellitus, which is characterized by persistent hyperglycemia from several causes, is the most prominent disease related to the failure to regulate blood sugar. Fructose and galactose are also sugars found in the blood; however, only glucose levels are regulated via insulin and glucagon.

Countries that use the metric system generally use mmol/L. The United States uses mg/dL. To convert blood glucose readings, utilize the following conversions:

Divide the mg/dL by 18.02 to get mmol/L (or multiply by 0.0555)

Multiply the mmol/L by 18.02 to get mg/dL (or divide by 0.0555)

The glucose meters considered in this specialization are typically handheld instruments that require a sample of blood or body fluid to perform the glucose measurement. The glucose concentration measured by various techniques can be classified into different types defined by three elements: sample type, sample source, and concentration reference method. Table 1 shows all the glucose concentration types defined in this standard.

Table 1—Glucose concentration types

Sample type	Sample source	Reference method
Blood	Capillary	Whole blood
		Plasma
	Venous	Whole blood
		Plasma
	Arterial	Whole blood
		Plasma
	Undetermined	Whole blood
		Plasma
Interstitial fluid	N/A	N/A
Control solution	N/A	N/A

NOTE—The blood glucose concentration may be indirectly derived from an interstitial fluid (ISF) sample, which is a common technique used in continuous glucose monitoring. A control solution is normally used for glucose meter quality control.

In addition to glucose measurement, glucose meters generally provide a means for the user to associate information on meals, exercise, and medications with a glucose measurement. Advanced devices may also allow users to customize device settings and to provide additional information related to their diabetes treatment and disease management.

Glucose meters are usually small, portable devices that are carried around by the user so that blood glucose measurements may be taken as needed, whether or not the user is in a network environment where communications with a manager can be established. Hence, measurement data are typically logged within the meter and can be retrieved at a later time, either in whole or in part, when the meter is connected to a manager network. There are two typical use cases for the transfer of measurement data to a manager:

- By the user in a non-health-care environment. A user may connect the meter to a personal manager device such as a personal computer or a portable communications device such as a cell phone. In this case, the user would download the most recent logged measurement data from the meter for near-term trend analysis or for transfer of data to an external electronic health network service. The transfer of data would happen immediately on connection with the manager application and require no initiation by the user. This is a temporary storage model of the meter.
- By a health care professional in an office or clinic environment. The health care professional would download all logged measurement data from the meter for longer-term analysis, such as the data logged since the patient's last appointment. The transfer of data would be controlled entirely by the manager application and would not necessarily happen automatically when a connection is established. This is a long-term storage model of the meter.

This standard supports configurations that allow for support of both temporary and long-term storage models.

6. Glucose meter domain information model

6.1 Overview

This clause describes the domain information model of the glucose meter.

6.2 Class extensions

In this standard, no class extensions are defined with respect to IEEE Std 11073-20601-2014.

6.3 Object instance diagram

The object instance diagram of the glucose meter domain information model, which is defined for the purposes of this standard, is shown in Figure 1.

The objects of the DIM, as shown in Figure 1, are described in 6.5 to 6.11. See 6.5 through 6.11 for descriptions of the different glucose meter objects (e.g., the glucose meter medical device system (MDS) object, the glucose numeric object, and the enumeration object). See 6.12 for rules for extending the glucose meter information model beyond elements as described in this standard. Each clause that describes an object of the glucose meter contains the following information:

- The nomenclature code used to identify the class of the object. One example where this code is used is the configuration event, where the object class is reported for each object. This allows the manager to determine whether the class of the object being specified is a numeric, real-time sample array, enumeration, scanner, or PM-store class.
- The attributes of the object. Each object has attributes that represent and convey information on the physical device and its data sources. Each object has a Handle attribute that identifies the object instance within an agent. Attribute values are accessed and modified using methods such as GET and SET. Attribute types are defined using an ASN.1. The ASN.1 definitions for new attribute types specific to this standard are in Annex B, and the ASN.1 definitions for existing attribute types referenced in this standard are in IEEE Std 11073-20601-2014.
- The methods available on the object.
- The potential events generated by the object. The data are sent to the manager using events.
- The available services such as getting or setting attributes.

The attributes for each class are defined in tables that specify the name of the attribute, its value, and its qualifier. The qualifiers mean:

- M: Attribute is mandatory,
- C: Attribute is conditional and depends on the condition stated in the Remark or Value column (if IEEE Std 11073-20601-2014 is referenced, then it contains the conditions),
- R: Attribute is recommended,
- NR: Attribute is not recommended, and
- O: Attribute is optional.

Mandatory attributes shall be implemented by an agent. Conditional attributes shall be implemented if the condition applies and may be implemented otherwise. Recommended attributes should be implemented by the agent. Not recommended attributes should not be implemented by the agent. Optional attributes may be implemented on an agent.

The attributes can be either static, dynamic, or observational as specified in IEEE Std 11073-20601-2014.

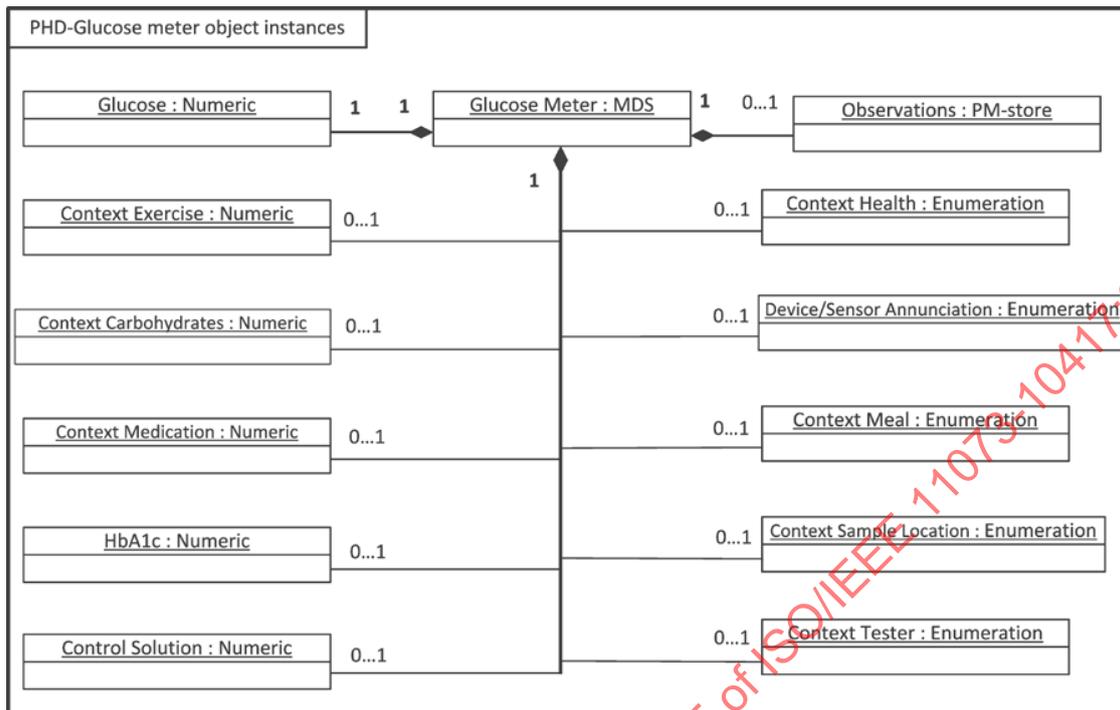


Figure 1—Glucose meter—domain information model

6.4 Types of configuration

6.4.1 General

As specified in IEEE Std 11073-20601-2014, there are two styles of configuration available. Subclauses 6.4.2 and 6.4.3 briefly introduce standard and extended configurations.

6.4.2 Standard configuration

Standard configurations are defined in the ISO/IEEE 11073-104zz specializations (such as this standard) and are assigned a well-known identifier (Dev-Configuration-Id). The usage of a standard configuration is negotiated at association time between the agent and the manager. If the manager acknowledges that it understands and wants to operate using the configuration, then the agent can begin sending measurements immediately. If the manager does not understand the configuration, the agent provides the configuration prior to transmitting measurement information.

The standard configuration 1700 (0x06A4) is deprecated with the release of this version of the 10417 standard.

Standard configuration 1701 (0x06A5) contains a glucose numeric object and a control solution numeric object as defined in 6.6.7.

A new standard configuration 1702 (0x06A6) is introduced in this version of standard 10417. The new standard configuration contains a glucose numeric object, a control solution object, and a meal context object, and recommends the use of Base-Offset-Time attributes for time reporting.

As defined in 8.3.1 of IEEE Std 11073-20601-2014, if the extended configuration of the specialization implemented by an agent is one that makes use of PM stores and only reports measurements using segment data events and if the standard configuration does not support PM stores, an agent is not required to support the corresponding standard configuration. As defined in 7.4.3.6.1 of 20601, Managers released based on this specification shall support both standard configurations 1701 (0x06A5) and 1702 (0x06A6).

6.4.3 Extended configuration

In extended configurations, the agent’s configuration is not predefined in a standard. The agent determines which objects, attributes, and values will be used in a configuration and assigns a configuration identifier. When the agent associates with a manager, it negotiates an acceptable configuration. Typically, the manager does not recognize the agent’s configuration on the first connection, so the manager responds that the agent needs to send the configuration information as a configuration event report. If, however, the manager already understands the configuration, either because it was preloaded in some way or the agent had previously associated with the manager, then the manager responds that the configuration is known and no further configuration information needs to be sent.

6.5 Medical device system object

6.5.1 MDS object attributes

Table 2 summarizes the attributes of the glucose meter MDS object. The nomenclature code to identify the MDS object class is MDC_MOC_VMS_MDS_SIMP.

Table 2—MDS object attributes

Attribute name	Value	Qualifier
Handle	0	M
System-Type	Attribute not present. See IEEE Std 11073-20601-2014.	C
System-Type-Spec-List	{MDC_DEV_SPEC_PROFILE_GLUCOSE, 2}	M
System-Model	{“Manufacturer”, “Model”}	M
System-Id	Extended unique identifier (64 bits) (EUI-64)	M
Dev-Configuration-Id	Extended configs: 0x4000–0x7FFF Standard config: 0x06A6 (1702) Standard config: 0x06A5 (1701)	M
Attribute-Value-Map	See IEEE Std 11073-20601-2014.	C
Production-Specification	See IEEE Std 11073-20601-2014.	O
Mds-Time-Info	See IEEE Std 11073-20601-2014.	C
Date-and-Time	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time	See IEEE Std 11073-20601-2014.	R
Relative-Time	See IEEE Std 11073-20601-2014.	C
HRes-Relative-Time	See IEEE Std 11073-20601-2014.	C
Date-and-Time-Adjustment	See IEEE Std 11073-20601-2014.	C
Power-Status	<i>onBattery or onMains</i>	O
Battery-Level	See IEEE Std 11073-20601-2014.	O
Remaining-Battery-Time	See IEEE Std 11073-20601-2014.	O
Reg-Cert-Data-List	See IEEE Std 11073-20601-2014.	O
Confirm-Timeout	See IEEE Std 11073-20601-2014.	O
Transport-Timeout	See IEEE Std 11073-20601 2014.	O
NOTE—See IEEE Std 11073-20601-2014 for information on whether an attribute is static or dynamic.		

In the response to a Get MDS object command, only implemented attributes and their corresponding values are returned.

See IEEE Std 11073-20601-2014 for descriptive explanations of the individual attributes as well as for information on attribute ID and attribute type.

The Dev-Configuration-Id attribute holds a locally unique 16-bit identifier that identifies the device configuration instance. The Device Configuration Identifiers for standard configurations are listed in Table 2. For a glucose meter agent with extended configuration, this identifier is chosen in the range of extended-config-start to extended-config-end (see IEEE Std 11073-20601-2014) as shown in Table 2.

The agent sends the Dev-Configuration-Id during the Associating state (see 8.3) to identify its configuration for the duration of the association. If the manager already holds the configuration information relating to the Dev-Configuration-Id, it recognizes the Dev-Configuration-Id. Then the Configuring state (8.4) is skipped, and the agent and manager enter the Operating state. If the manager does not recognize the Dev-Configuration-Id, the agent and manager enter the Configuring state.

If an agent implements multiple IEEE 11073-104zz specializations, System-Type-Spec-List is a list of type/version pairs, each referencing the respective device specialization and version of that specialization.

6.5.2 MDS object methods

Table 3 defines the methods (actions) of the glucose meter agent's MDS object. These methods are invoked using the Action service. In Table 3, the Subservice type name column defines the name of the method; the Mode column defines whether the method is invoked as an unconfirmed action (i.e., roiv-cmip-action from IEEE Std 11073-20601-2014) or a confirmed action (i.e., roiv-cmip-confirmed-action); the Subservice type (action-type) column defines the nomenclature code to use in the action-type field of an action request and response (see IEEE Std 11073-20601-2014); the Parameters (action-info-args) column defines the associated ASN.1 data structure (see IEEE Std 11073-20601-2014 for ASN.1 definitions) to use in the action message for the action-info-args field of the request; and the Results (action-info-args) column defines the structure to use in the action-info-args of the response.

Table 3—MDS object methods

Service	Subservice type name	Mode	Subservice type (action-type)	Parameters (action-info-args)	Results (action-info-args)
ACTION	Set-Time	Confirmed	MDC_ACT_SET_TIME	SetTimeInvoke	—
ACTION	Set-Base-Offset-Time	Confirmed	MDC_ACT_SET_BO_TIME	SetBOTimeInvoke	—

— **Set-Time**

This method allows the manager to set a real-time clock in the agent with the absolute time. The agent indicates whether the Set-Time command is valid using the mds-time-capab-set-clock bit in the Mds-Time-Info attribute (see IEEE Std 11073-20601-2014).

— **Set-Base-Offset-Time**

This method allows the manager to set a real-time clock in the agent with the base time and offset. The agent indicates whether the Set-Base-Offset-Time command is valid using the mds-time-capab-set-clock bit in the Mds-Time-Info attribute (see IEEE Std 11073-20601-2014).

If the agent supports the Base-Offset-Time-Stamp attribute, this method shall be implemented.

Agents following only this device specialization and no others shall send event reports using agent-initiated measurement data transmission. Agents following this device specialization as well as others shall send event reports in the appropriate fashion. During the association procedure (see 8.3), data-req-mode-capab shall be set to the appropriate value for the event report style. As a result, the manager shall assume the glucose meter agent does not support any of the MDS-Data-Request features (see IEEE Std 11073-20601-2014 for additional information). Thus, implementation of the MDS-Data-Request method/action is not required in this standard and is not shown in Table 3.

6.5.3 MDS object events

Table 4 defines the events that can be sent by the glucose meter MDS object.

Table 4—Glucose meter MDS object events

Service	Subservice type name	Mode	Subservice type (event-type)	Parameters (event-info)	Results (event-reply-info)
EVENT REPORT	MDS-Configuration-Event	Confirmed	MDC_NOTI_CONFIG	ConfigReport	ConfigReport Rsp
	MDS-Dynamic-Data-Update-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_FIXED	ScanReportInfoFixed	—
	MDS-Dynamic-Data-Update-Var	Confirmed	MDC_NOTI_SCAN_REPORT_VAR	ScanReportInfoVar	—
	MDS-Dynamic-Data-Update-MP-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_MP_FIXED	ScanReportInfoMP Fixed	—
	MDS-Dynamic-Data-Update-MP-Var	Confirmed	MDC_NOTI_SCAN_REPORT_MP_VAR	ScanReportInfoMP Var	—

— **MDS-Configuration-Event**

This event is sent by the glucose meter agent during the configuring procedure if the manager does not already know the glucose meter agent’s configuration from past associations or because the manager has not been implemented to recognize the configuration according to the glucose meter device specialization. The event provides static information about the supported measurement capabilities of the glucose meter agent.

MDS-Dynamic-Data-Update-Var

This event provides dynamic measurement data from the glucose meter agent for the glucose numeric object. These data are reported using a generic attribute list variable format. The event is sent as an unsolicited message by the agent (i.e., an agent-initiated measurement data transmission). See 8.5.3 for more information on unsolicited event reporting.

— **MDS-Dynamic-Data-Update-Fixed**

This event provides dynamic measurement data from the glucose meter agent for the glucose numeric object. These data are reported in the fixed format defined by the Attribute-Value-Map attribute of the object(s). The event is sent as an unsolicited message by the agent (i.e., an agent-initiated measurement data transmission). See 8.5.3 for more information on unsolicited event reporting.

- **MDS-Dynamic-Data-Update-MP-Var**
This is the same as MDS-Dynamic-Data-Update-Var but allows inclusion of data from multiple people.
- **MDS-Dynamic-Data-Update-MP-Fixed**
This is the same as MDS-Dynamic-Data-Update-Fixed but allows inclusion of data from multiple people.

NOTE—IEEE Std 11073-20601-2014 requires that managers support all of the MDS object events listed Table 4.

6.5.4 Other MDS services

6.5.4.1 GET service

A glucose meter agent shall support the GET service, which is provided by the MDS object to retrieve the values of all implemented MDS object attributes. The GET service can be invoked as soon as the glucose meter agent receives the Association Response and moves to the Associated state, including the Operating and Configuring substates.

The manager may request the MDS object attributes of the glucose meter agent; in which case, the manager shall send the “Remote Operation Invoke | Get” message (see roiv-cmip-get in IEEE Std 11073-20601-2014) with the reserved MDS handle value of 0. The glucose meter agent shall report its MDS object attributes to the manager using the “Remote Operation Response | Get” message (see rors-cmip-get in IEEE Std 11073-20601-2014). See Table 5 for a summary of the GET service including some message fields.

Table 5—Glucose meter MDS object GET service

Service	Remark	Field	Value	Qualifier
roiv-cmip-get	Manager GET service request of agents MDS attributes.	obj-handle	0	M
		attribute-id-list	Dynamic	O
rors-cmip-get	Agent GET service response to GET service request by manager.	obj-handle	0	M
		attribute-list	Dynamic	M

See 8.5.2 for details on the procedure for getting the MDS object attributes.

6.5.4.2 SET service

The glucose meter specialization does not require an implementation to support the MDS object SET service.

6.6 Numeric objects

6.6.1 General

The glucose meter DIM (see Figure 1) contains numeric objects that represent aspects of blood glucose and associated medical context. The nomenclature code to identify the numeric class is MDC_MOC_VMO_METRIC_NU. Table 6 shows attributes that are common to all the numeric types of the glucose meter agent.

Table 6—Common glucose numeric object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	Defined in each table below.	M
Supplemental-Types	See IEEE Std 11073-20601-2014.	NR
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated mss-cat-manual	M
Metric-Structure-Small	See IEEE Std 11073-20601-2014.	NR
Measurement-Status	See IEEE Std 11073-20601-2014.	NR
Metric-Id	See IEEE Std 11073-20601-2014.	C
Metric-Id-List	See IEEE Std 11073-20601-2014.	NR
Metric-Id-Partition	See IEEE Std 11073-20601-2014.	NR
Unit-Code	See IEEE Std 11073-20601-2014.	M
Attribute-Value-Map	See IEEE Std 11073-20601-2014.	C
Source-Handle-Reference	See IEEE Std 11073-20601-2014.	NR
Label-String	See IEEE Std 11073-20601-2014.	O
Unit-LabelString	See IEEE Std 11073-20601-2014.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Relative-Time-Stamp	See IEEE Std 11073-20601-2014.	O
HiRes-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Measure-Active-Period	See IEEE Std 11073-20601-2014.	C
Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	NR
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	C
Compound-Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	NR
Nu-Observed-Value	See IEEE Std 11073-20601-2014.	NR
Compound-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	NR
Accuracy	See IEEE Std 11073-20601-2014.	R

Subclauses 6.6.2 through 6.6.6 describe the numeric objects that are defined for use in the glucose meter. Each object represents a specific aspect of blood glucose measurement or an associated medical context. The class is denoted by the Type attribute. The description of each numeric object defines the data or events it produces, the possible states, and where appropriate, its behavior. The respective tables define the numeric values generated by the agent in response to a change in state.

Sometimes, the interpretation of one attribute value in an object depends on other attribute values in the same object. For example, Unit-Code and Unit-LabelString provide context for the observed values. Whenever a contextual attribute changes, the agent shall report these changes to the manager using an MDS object event (see 6.5.3) prior to reporting any of the dependent values.

The numeric object does not support any methods, events, or other services.

For standard configurations, the optional attributes are initially not present. See IEEE Std 11073-20601-2014 for descriptive explanations on the individual attributes as well as for information on attribute ID and attribute type.

6.6.2 Blood glucose

Table 7 summarizes the attributes of the blood glucose numeric object. The blood glucose numeric object shall be supported by a glucose meter agent.

Table 7 —Blood glucose numeric object attributes

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x06A5)		Standard configuration (Dev-Configuration-Id = 0x06A6)	
	Value	Qualifier	Values	Qualifier	Values	Qualifier
Handle	See IEEE Std 11073-20601-2014 {MDC_PART_SCADA, MDC_CONC_GLU_CAPILLARY_ WHOLEBLOOD or MDC_CONC_GLU_CAPILLARY_ PLASMA or MDC_CONC_GLU_VENOUS_ WHOLEBLOOD or MDC_CONC_GLU_VENOUS_PLASMA A or MDC_CONC_GLU_ARTERIAL_ WHOLEBLOOD or MDC_CONC_GLU_ARTERIAL_ PLASMA or MDC_CONC_GLU_UNDETERMINED_ WHOLEBLOOD or MDC_CONC_GLU_UNDETERMINED_ PLASMA or MDC_CONC_GLU_ISF}	M	{MDC_PART_SCADA, MDC_CONC_GLU_ UNDETERMINED_ PLASMA}	M	{MDC_PART_SCADA, MDC_CONC_GLU_ UNDETERMINED_ PLASMA}	M
Type						
Metric-Spec- Small	mss-avail-intermittent mss-avail-stored- data mss-upd-aperiodic mss-msmt- aperiodic mss-acc-agent-initiated. The mss-cat-manual shall only be set if the reading is manually entered.	M	mss-avail-intermittent mss-avail- stored-data mss-upd-aperiodic mss- msmt-aperiodic mss-acc-agent- initiated	M	mss-avail-intermittent mss-avail-stored- data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent- initiated	M
Unit-Code	MDC_DIM_MILLI_G_PER_DL or MDC_DIM_MILLI_MOLE_PERL	M	MDC_DIM_MILLI_G_PER_DL	M	MDC_DIM_MILLI_G_PER_DL	M
Attribute- Value-Map	See IEEE Std 11073-20601-2014.	C	MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_ABS	M	MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_TIME_STAMP_BO	M
Absolute- Time-Stamp	See IEEE Std 11073-20601-2014.	C	If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073- 20601-2014 apply.	C	If fixed format is used and the standard configuration is not adjusted, this attribute is mandatory; otherwise, the conditions from IEEE Std 11073-20601-2014 apply.	C

Table 7—Blood glucose numeric object attributes (continued)

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x06A5)		Standard configuration (Dev-Configuration-Id = 0x06A6)	
	Value	Qualifier	Values	Qualifier	Values	Qualifier
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R	See IEEE Std 11073-20601-2014.	C	See IEEE Std 11073-20601-2014.	C
Relative-Time-Stamp	See IEEE Std 11073-20601-2014.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2014.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2014.	NR
HiRes-Time-Stamp	See IEEE Std 11073-20601-2014.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2014.	C	Attribute not initially present. If present, follow IEEE Std 11073-20601-2014.	C
Measure-Active-Period	See IEEE Std 11073-20601-2014.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2014.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2014.	NR
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	C	See IEEE Std 11073-20601-2014.	M	See IEEE Std 11073-20601-2014.	M
Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	C	This type of observed value is not allowed because the Basic-Nu-Observed-Value is mandatory, and IEEE Std 11073-20601-2014 mandates that one and only one type of observed value can be used.	C	This type of observed value is not allowed because the Basic-Nu-Observed-Value is mandatory, and IEEE Std 11073-20601-2014 mandates that one and only one type of observed value can be used.	C
Compound-Simple-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	NR	This type of observed value is not allowed because the Basic-Nu-Observed-Value is mandatory, and IEEE Std 11073-20601-2014 mandates that one and only one type of observed value can be used.	C	This type of observed value is not allowed because the Basic-Nu-Observed-Value is mandatory, and IEEE Std 11073-20601-2014 mandates that one and only one type of observed value can be used.	C
Accuracy	See IEEE Std 11073-20601-2014.	R	Attribute not initially present. If present, follow IEEE Std 11073-20601-2014.	NR	Attribute not initially present. If present, follow IEEE Std 11073-20601-2014.	NR

NOTE—See IEEE Std 11073-20601-2014 for information on whether an attribute is static or dynamic.

The blood glucose numeric object does not support any methods, events, or other services.

For a glucose agent with a standard configuration, the AttrValMap structure (see IEEE Std 11073-20601-2014) of the Attribute-Value-Map attribute shall contain the attribute ID and attribute length information of the Basic-Nu-Observed-Value and Absolute-Time-Stamp or Base-Offset-Time-Stamp attribute in the same order as indicated in Table 7.

In case a blood glucose measurement needs to be further associated with a meal, sample location, and tester information, the additional Enumeration objects (i.e., context carbohydrates, context sample location, and context tester) can be used. See 6.8 for detail.

In standard configurations 1701 (0x06A5) and 1702 (0x06A6), or in an extended configuration that does not include the Device and Sensor Status Annunciation object, a glucose measurement that is above the capabilities of the device sensor shall be indicated with an observed value of +INFINITY, and a glucose measurement that is below the capabilities of the device sensor shall be indicated with an observed value of -INFINITY.

For measurements that exceed the capabilities of the device sensor that are reported using the extended configuration, the glucose agent shall either set the appropriate flags in the device and sensor status (GlucoseDevStat) or report the measurement using the aforementioned +/- INFINITY values but the sensor shall not send over-range flags and an over-range measurement value.

6.6.3 Hemoglobin bound to glucose A1c form (HbA1c)

HbA1c, which is also known as A1c or glycated hemoglobin, is used as the long-term measure of blood sugar control. The A1c test measures how many A1c hemoglobin cells (a specific part of red blood cells) have sugar attached to them. Because these cells live for approximately 4 months, this test indicates how well blood sugar has been controlled over the previous few months. The American Diabetes Association [B1] recommends an A1c result of 7% or less to help reduce the risk of long-term complications of diabetes. Table 8 identifies the measured, calculated, or manually entered values for recording HbA1c data.

Table 8—HbA1c numeric object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	{MDC_PART_SCADA, MDC_CONC_HBA1C}.	M
Unit-Code	MDC_DIM_PERCENT.	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	M
NOTE—See IEEE Std 11073-20601-2014 for information on whether an attribute is static or dynamic.		

If the HbA1c value is entered manually, the mss-cat-manual bit shall be set in Metric-Spec-Small as well.

6.6.4 Context exercise

The level of exercise undertaken in a period can be important to record to balance food intake and insulin dose. Where there are issues over control of blood glucose, a review of exercise may be helpful in the care and management of the person. Table 9 identifies the values a person can enter on the glucose device to record his or her exercise regimen.

Table 9—Context exercise numeric object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_EXERCISE}	M
Unit-Code	MDC_DIM_PERCENT	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Measure-Active-Period	See IEEE Std 11073-20601-2014—this indicates the duration of exercise.	M
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2014—this indicates the intensity of exercise ranging from 0 to 100.	M
NOTE—See IEEE Std 11073-20601-2014 for information on whether an attribute is static or dynamic.		

The context exercise numeric object does not support any methods, events, or other services.

If the Exercise value is entered manually, the mss-cat-manual bit shall be set in Metric-Spec-Small as well.

6.6.5 Context medication

Treatment for diabetes is most effective when the effects of medication on blood glucose levels are monitored. The ability to track medication with a test result can inform a physician as to whether a particular medication, or a combination of medicines, is effective. Table 10 identifies the values a person can enter on the glucose device to record his or her medication regimen.

Table 10—Context medication numeric object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	{MDC_PART_PHD_DM, MDC_CTXT_MEDICATION}	M
Metric-Id	MDC_CTXT_MEDICATION_RAPIDACTING or MDC_CTXT_MEDICATION_SHORTACTING or MDC_CTXT_MEDICATION_INTERMEDIATEACTING or MDC_CTXT_MEDICATION_LONGACTING or MDC_CTXT_MEDICATION_PREMIX	M
Unit-Code	MDC_DIM_MILLI_G or MDC_DIM_MILLI_L or MDC_DIM_INTL_UNIT	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	M
NOTE—See IEEE Std 11073-20601-2014 for information on whether an attribute is static or dynamic.		

If the Medication value is entered manually, the mss-cat-manual bit shall be set in Metric-Spec-Small as well.

6.6.6 Context carbohydrates

Recording carbohydrates intake can be an important aid in insulin dose management. Whereas there are issues over control of blood glucose, a review of carbohydrates may be helpful in the care and management of the person. Table 11 enables the person to record the amount of carbohydrates ingested as this can directly affect the level of glucose in the blood.

Table 11 —Context carbohydrates numeric object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_CARB}	M
Metric-Id	MDC_CTXT_GLU_CARB_BREAKFAST or MDC_CTXT_GLU_CARB_LUNCH or MDC_CTXT_GLU_CARB_DINNER or MDC_CTXT_GLU_CARB_SNACK or MDC_CTXT_GLU_CARB_DRINK or MDC_CTXT_GLU_CARB_SUPPER or MDC_CTXT_GLU_CARB_BRUNCH or MDC_CTXT_GLU_CARB_UNDETERMINED or MDC_CTXT_GLU_CARB_OTHER or MDC_CTXT_GLU_CARB_NO_ENTRY or MDC_CTXT_GLU_CARB_NO_INGESTION	M
Unit-Code	MDC_DIM_G	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	M
NOTE—See IEEE Std 11073-20601-2014 for information on whether an attribute is static or dynamic.		

If the Carbohydrates value is entered manually, the mss-cat-manual bit shall be set in Metric-Spec-Small as well.

6.6.7 Control solution

Table 12 summarizes the attributes of the control solution numeric object. In standard configurations 1701 (0x06A5) and 1702 (0x06A6), the control solution numeric object shall be supported by a glucose meter agent.

STANDARDSISO.COM: Click to view the PDF of ISO/IEEE 11073-10417:2017

Table 12 —Control solution numeric object attributes

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x06A5)		Standard configuration (Dev-Configuration-Id = 0x06A6)	
	Value	Qualifier	Value	Qualifier	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M		M	2	M
Type	{MDC_PART_SCADA, MDC_CONC_GLU_CONTROL}	M	{MDC_PART_SCADA, MDC_CONC_GLU_CONTROL}	M	{MDC_PART_SCADA, MDC_CONC_GLU_CONTROL}	M
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated	M	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated	M	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated	M
Metric-Id	MDC_CONC_GLU_CONTROL_ LEVEL_LOW or MDC_CONC_GLU_CONTROL_ LEVEL_MEDIUM or MDC_CONC_GLU_CONTROL_ LEVEL_HIGH or MDC_CONC_GLU_CONTROL_ LEVEL_UNDETERMINED	M	MDC_CONC_GLU_CONTROL_ LEVEL_UNDETERMINED	M	MDC_CONC_GLU_CONTROL_ LEVEL_UNDETERMINED	M
Unit-Code	MDC_DIM_MILLI_G_PER_DL or MDC_DIM_MILLI_MOLE_PERL	M	MDC_DIM_MILLI_G_PER_DL	M	MDC_DIM_MILLI_G_PER_DL	M
Attribute-Value-Map	See IEEE Std 11073-20601-2014.	C	MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_ID_PHYSIO, then MDC_ATTR_TIME_STAMP_ABS	M	MDC_ATTR_NU_VAL_OBS_BASIC, then MDC_ATTR_ID_PHYSIO, then MDC_ATTR_TIME_STAMP_BO	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C	See IEEE Std 11073-20601-2014.	C	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R	See IEEE Std 11073-20601-2014.	R	See IEEE Std 11073-20601-2014.	R
Basic-Nu-Observed-Value	See IEEE Std 11073-20601-2014.	C	See IEEE Std 11073-20601-2014.	M	See IEEE Std 11073-20601-2014.	M

In standard configurations 1701 (0x06A5) and 1702 (0x06A6), or in an extended configuration that does not include the Device and Sensor Status Annunciation object, a control solution measurement that is above the capabilities of the device sensor shall be indicated with an observed value of +INFINITY, and a glucose measurement that is below the capabilities of the device sensor shall be indicated with an observed value of -INFINITY.

If a device supports the Context Sample Location enumeration object and reports an MDC_CONC_GLU_CONTROL measurement, then the device shall also report a corresponding MDC_CTXT_GLU_SAMPLELOCATION_CTRLsolution measurement.

6.7 Real-time sample array objects

Real-time sample array objects are not required by this standard.

6.8 Enumeration objects

6.8.1 General

The blood glucose meter uses a number of optional enumeration objects to represent data that are related to blood glucose. The nomenclature code to identify the enumeration class is MDC_MOC_VMO_METRIC_ENUM. The attribute structure shown in Table 13 is common to all enumeration types. Subclauses 6.8.2 through 6.8.6 define the precise definitions for each enumeration type and take precedence.

Table 13—Common glucose enumeration object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	Defined in each enumeration table below.	M
Supplemental-Types	See IEEE Std 11073-20601-2014.	NR
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored-data mss-upd-aperiodic mss-msmt-aperiodic mss-acc-agent-initiated mss-cat-manual	M
Metric-Structure-Small	See IEEE Std 11073-20601-2014.	NR
Measurement-Status	See IEEE Std 11073-20601-2014.	NR
Metric-Id	See IEEE Std 11073-20601-2014.	NR
Metric-Id-List	See IEEE Std 11073-20601-2014.	NR
Metric-Id-Partition	See IEEE Std 11073-20601-2014.	NR
Unit-Code	See IEEE Std 11073-20601-2014.	NR
Attribute-Value-Map	See IEEE Std 11073-20601-2014.	C
Source-Handle-Reference	See IEEE Std 11073-20601-2014.	NR
Label-String	See IEEE Std 11073-20601-2014.	O
Unit-LabelString	See IEEE Std 11073-20601-2014.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Relative-Time-Stamp	See IEEE Std 11073-20601-2014.	O
HiRes-Time-Stamp	See IEEE Std 11073-20601-2014.	O
Measure-Active-Period	See IEEE Std 11073-20601-2014.	O
Enum-Observed-Value-Simple-OID	See IEEE Std 11073-20601-2014.	O
Enum-Observed-Value-Simple-Bit-Str	See IEEE Std 11073-20601-2014.	O
Enum-Observed-Value-Basic-Bit-Str	See IEEE Std 11073-20601-2014.	O
Enum-Observed-Value-Simple-Str	See IEEE Std 11073-20601-2014.	O
Enum-Observed-Value	See IEEE Std 11073-20601-2014.	O
Enum-Observed-Value-Partition	See IEEE Std 11073-20601-2014.	O

Subclauses 6.8.2 through 6.8.6 describe the possible uses of the glucose enumeration object. Each use is an instance of the enumeration class with a particular Type value. The interpretation of associated values is dependent on the Type value. The description of each enumeration object defines all the possible states and, where appropriate, its behavior. The respective tables define the glucose enumeration types generated by the agent in response to a change in state.

The enumeration object does not support any methods, events, or other services. Event reports for these objects are generated by the MDS object.

See IEEE Std 11073-20601-2014 for descriptive explanations on the individual attributes as well as for information on attribute id and attribute type.

6.8.2 Device and sensor status annunciation

The device and sensor status annunciation object allows glucose meter specific errors to be recorded to track important troubleshooting information for manufacturers. Faulty sensor detection and signal irregularities are closely associated with a glucose meter, applicable to telehealth use cases. An Enumeration object fulfills this need.

An additional Enumeration object containing the running status of the device and sensor assembly is also provided. If this object is to be implemented, then the object identifier (OID) Type and bit assignments shall be implemented as described in this clause. The nomenclature code to identify the enumeration object class is MDC_MOC_VMO_METRIC_ENUM. Refer to Table 14 for the set of attributes of this object.

This object is instantiated only in extended configurations. A manager should support the interpretation of this object to enable reporting of these occurrences. An agent should support this object to transmit these occurrences.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017

Table 14—Device and sensor annunciation status attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	{MDC_PART_PHD_DM, MDC_GLU_METER_DEV_STATUS}	M
Supplemental-Types	See IEEE Std 11073-20601-2014.	NR
Metric-Spec-Small	mss-avail-intermittent mss-avail-stored- data mss-upd-aperiodic mss-msmt- aperiodic mss-acc-agent-initiated	M
Metric-Structure-Small	See IEEE Std 11073-20601-2014.	NR
Measurement-Status	See IEEE Std 11073-20601-2014.	O
Metric-Id	See IEEE Std 11073-20601-2014.	NR
Metric-Id-List	See IEEE Std 11073-20601-2014.	NR
Metric-Id-Partition	See IEEE Std 11073-20601-2014.	NR
Unit-Code	See IEEE Std 11073-20601-2014.	NR
Attribute-Value-Map	See IEEE Std 11073-20601-2014.	C
Source-Handle-Reference	See IEEE Std 11073-20601-2014.	NR
Label-String	See IEEE Std 11073-20601-2014.	O
Unit-LabelString	See IEEE Std 11073-20601-2014.	O
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Ste 11073-20601-2014	R
Relative-Time-Stamp	See IEEE Std 11073-20601-2014.	C
HiRes-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Enum-Observed-Value-Simple-OID	See IEEE Std 11073-20601-2014.	O
Enum-Observed-Value-Simple-Bit-Str	See following text.	NR
Enum-Observed-Value-Basic-Bit-Str	See following text.	R
Enum-Observed-Value-Simple-Str	See IEEE Std 11073-20601-2014.	NR
Enum-Observed-Value	See following text.	NR
Enum-Observed-Value-Partition	See IEEE Std 11073-20601-2014.	O
NOTE 1—See IEEE Std 11073-20601-2014 for information on whether an attribute is static or dynamic. NOTE 2—See 6.3 for a description of the qualifiers.		

An agent explicitly expresses the existence of annunciations by setting the appropriate bits in the Enum-Observed-Value-Basic-Bit-Str attribute, as defined in Table 15. It is recommended to use the Enum-Observed-Value-Basic-Bit-Str attribute as it consumes fewer payload octets than the Enum-Observed-Value-Simple-Bit-Str attribute. The Enum-Observed-Value attribute should not be used, as it unnecessarily complicates the modeling of the object. If a manager supports the interpretation of this object, it shall be able to interpret the entire set of presented conditions. An agent may implement any subset of these same conditions. Note that a manager shall interpret these bits only within the context of this attribute and only within this device specialization as other specializations may use corresponding terms for different purposes.

Table 15—Mapping of device, sensor, and signal status to object Bit-Str attribute

Device or sensor condition	GlucoseDevStat mnemonic
Agent reports that the battery is low and needs replacing.	device-battery-low
Agent reports that the sensor is malfunctioning or faulting.	sensor-malfunction
Agent reports that there is not enough blood/control solution on the strip.	sensor-sample-size-insufficient
Agent reports that the strip was inserted incorrectly.	sensor-strip-insertion
Agent reports that the strip is not the right type for the device.	sensor-strip-type-incorrect
Agent reports that the reading or value is higher than the sensor can process.	sensor-result-too-high
Agent reports that the reading or value is lower than the sensor can process.	sensor-result-too-low
Agent reports that the ambient temperature is too high for a valid test/result.	sensor-temp-too-high ^a
Agent reports that the ambient temperature is too low for a valid test/result.	sensor-temp-too-low ^a
Agent reports that the reading was interrupted or the strip was pulled too soon.	sensor-read-interrupt
A general device fault has occurred in the agent.	device-gen-fault
Agent reports that the ambient temperature is out of range for a valid test/result.	sensor-temp-out-of-range ^a

^a The agent shall not indicate both sensor-temp-too-high and sensor-temp-too-low at the same time. If either the sensor-temp-too-high or sensor-temp-too-low bits are set, the agent shall set the sensor-temp-out-of-range bit as well. The agent shall only use sensor-temp-out-of-range by itself if sensor-temp-too-high or sensor-temp-too-low cannot be determined by the device.

The specific bit mappings of GlucoseDevStat are defined in Annex B.

6.8.3 Context meal

A blood sugar measurement (or referred to as a reading) may be further associated with information on meal relationship when this measurement is taken. The blood sugar level can be significantly affected by the testing time relative to the meal time. Table 16 defines the meal condition at the time when the blood sugar measurement is taken.

Table 16—Context meal enumeration object attributes

Attribute name	Extended configuration		Standard configuration (Dev-Configuration-Id = 0x06A6)	
	Value	Qualifier	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M	3	M
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_MEAL}.	M	{MDC_PART_PHD_DM, MDC_CTXT_GLU_MEAL}.	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R	See IEEE Std 11073-20601-2014.	R
Enum-Observed-Value-Simple-OID	One of the following nomenclature value shall be used: MDC_CTXT_GLU_MEAL_PREPRANDIAL MDC_CTXT_GLU_MEAL_POSTPRANDIAL MDC_CTXT_GLU_MEAL_FASTING MDC_CTXT_GLU_MEAL_BEDTIME MDC_CTXT_GLU_MEAL_CASUAL	M	One of the following nomenclature value shall be used: MDC_CTXT_GLU_MEAL_PREPRANDIAL MDC_CTXT_GLU_MEAL_POSTPRANDIAL MDC_CTXT_GLU_MEAL_FASTING MDC_CTXT_GLU_MEAL_BEDTIME MDC_CTXT_GLU_MEAL_CASUAL	M

6.8.4 Context sample location

A blood sugar measurement may be further characterized by the blood sample location. Table 17 defines the possible blood locations where the blood sample may be taken.

Table 17—Context sample location enumeration object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_SAMPLELOCATION}	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Enum-Observed-Value-Simple-OID	One of the following nomenclature value shall be used: MDC_CTXT_GLU_SAMPLELOCATION_FINGER MDC_CTXT_GLU_SAMPLELOCATION_AST MDC_CTXT_GLU_SAMPLELOCATION_EARLOBE MDC_CTXT_GLU_SAMPLELOCATION_CTRL SOLUTION MDC_CTXT_GLU_SAMPLELOCATION_OTHER MDC_CTXT_GLU_SAMPLELOCATION_UNDETERMINED	M

6.8.5 Context tester

The precision (or validity) of a blood sugar measurement can be impacted by whom and where the measurement is performed. Table 18 defines the possible cases of testers who may perform the blood sugar measurement.

Table 18—Context tester enumeration object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_TESTER}	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Enum-Observed-Value-Simple-OID	One of the following nomenclature value shall be used: MDC_CTXT_GLU_TESTER_SELF MDC_CTXT_GLU_TESTER_HCP MDC_CTXT_GLU_TESTER_LAB	M

6.8.6 Context health

Stress is an important factor when monitoring blood sugar levels, as excessive stress can cause these levels to rise. Stress hormones such as epinephrine and cortisol are released and, as a result, can significantly raise the blood sugar levels. Table 19 defines the various levels of health a person feels when taking a glucose measurement. Although the state of health is a matter of perception, it enables a dialog between patient and physician to discuss matters that may affect therapy. *Minor* and *major* are related to the general health or the level of illness of the person. *Menses* refers to the female menstrual cycle, and *stress* refers to physiological or psychological stress. In the event of multiple readings, the most impactful on the result shall be noted.

Table 19—Context health enumeration object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
Type	{MDC_PART_PHD_DM, MDC_CTXT_GLU_HEALTH}	M
Absolute-Time-Stamp	See IEEE Std 11073-20601-2014.	C
Base-Offset-Time-Stamp	See IEEE Std 11073-20601-2014.	R
Enum-Observed-Value-Simple-OID	One of the following nomenclature value shall be used: MDC_CTXT_GLU_HEALTH_MINOR MDC_CTXT_GLU_HEALTH_MAJOR MDC_CTXT_GLU_HEALTH_MENSES MDC_CTXT_GLU_HEALTH_STRESS MDC_CTXT_GLU_HEALTH_NONE	M

6.9 PM-store objects

6.9.1 General

In the context of personal health devices, glucose meters are highly portable due to their convenient sizes and are normally carried around with users so that blood glucose measurements may be taken as needed. More often than not, blood glucose measurements are taken at a time when out of the network and when manager/agent associations cannot be established. It is also common that a given set of measurements made by glucose meters may need to be uploaded to more than one manager, for example, in the home and at a medical facility.

To support dual usage, an agent may provide two or more configurations. One configuration may use a temporary measurement storage model that uploads the most recent data immediately on association (agent initiated) with little user intervention, such as might be used by a typical home user that uploads measurements frequently to a personal computer or a mobile device such as a cell phone. Another configuration may use a long-term measurement storage model that uploads data at the request of the manager, such as might be used by the patient's physician or other health care professionals.

The long-term storage model is realized using PM-stores. Any configuration that does not include a PM-store object utilizes agent-initiated event reports to transmit the observations. The use of temporarily stored data as defined in IEEE Std 11073-20601-2014 is most useful for small numbers of measurements and is subject to automatic deletion during upload.

Alternatively, in the case where a large number of measurements may be stored or if automatic deletion is to be avoided, a PM-store configuration should be used. Any configuration with a PM-store for persistent storage shall disable agent-initiated transmission and shall enable access to the PM-store transmissions. As a result, this standard describes a mechanism using PM-store to hold measurements for longer durations. The data held in PM-store objects are deleted by user actions via the manager or user interface on the device, and the capacity is limited only by the amount of memory.

6.9.2 Persistent store model

The PM-store model utilizes a PM-segment for each type of object to be persistently stored (see Figure 2). The segment holding glucose readings shall be present if the PM-store is implemented. The other segments are optional and hold observations from the supporting medical context objects that are implemented. Each entry shall include one of the time formats in the segm-entry-header so a manager can correlate entries across the different segments. Entries in the supported medical context PM-segments do not require a correlating result in the GlucoseSeg PM-segment, and can therefore be independent of a glucose measurement. This model was selected to reduce the transmission sizes as much as possible. If a particular medical context object is not supported, then the segment is not required to exist. If a person does not enter any data of that type when a reading is taken (e.g., the person does not respond to a prompt for what was eaten recently), then the entry in the PM-segment is not created. The PM-segments that are zero to many in Figure 2 behave this way because of the unknown number of timestamp changes, which are used to determine a common notion of time.

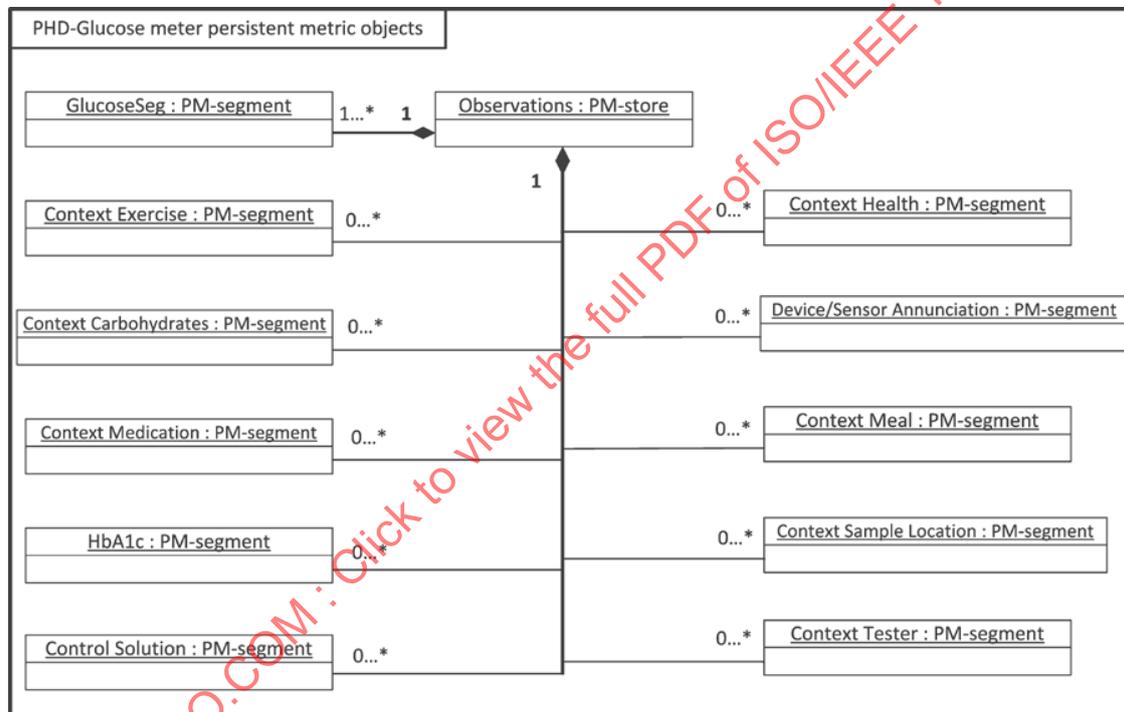


Figure 2—Glucose meter—persistent store model

6.9.3 PM-store object attributes

Table 20 defines the attributes of the PM-store objects that shall be implemented by the agent. The nomenclature code to identify the PM-store objects is MDC_MOC_VMO_PMSTORE.

Table 20 —Glucose meter PM-store object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Handle	See IEEE Std 11073-20601-2014.	M
PM-Store-Capab	See IEEE Std 11073-20601-2014.	M
Store-Sample-Algorithm	See IEEE Std 11073-20601-2014.	M
Store-Capacity-Count	See IEEE Std 11073-20601-2014.	M
Store-Usage-Count	See IEEE Std 11073-20601-2014.	M
Operational-State	See IEEE Std 11073-20601-2014.	M
PM-Store-Label	See IEEE Std 11073-20601-2014.	M
Sample-Period	See IEEE Std 11073-20601-2014.	NR
Number-Of-Segments	Number dependent on context support or time changes.	M
Clear-Timeout	See IEEE Std 11073-20601-2014.	C

Some considerations when using the PM-Store-Capab are as follows:

- If the agent creates new segments because of time changes as described in the “Comparable time” clause of IEEE Std 11073-20601-2014, then pmsc-var-no-of-segm shall be set.
- If the agent is recording episodic data in the PM-store, then the pmsc-epi-seg-entries shall be set.
- The remaining bits are agent specific.

6.9.4 PM-store object methods

Table 21 defines the methods of the PM-store objects.

Table 21 —Glucose meter PM-store object methods

Service	Subservice type name	Mode	Subservice type (action-type)	Parameters (action-info-args)	Results (action-info-args)
ACTION	Clear-Segments	Confirmed	MDC_ACT_SEG_CLR	SegmSelection	(empty)
ACTION	Get-Segment-Info	Confirmed	MDC_ACT_SEG_GET_INFO	SegmSelection	SegmentInfoList
ACTION	Get-Segment-Id-List	Confirmed	MDC_ACT_SEG_GET_ID_LIST	(empty)	SegmIdList
ACTION	Trig-Segment-Data-Xfer	Confirmed	MDC_ACT_SEG_TRIG_XFER	TrigSegmDataXferReq	TrigSegmDataXferRsp

- **Clear-Segments**
This method allows the manager to delete the data currently stored in one or more selected PM-segments. All entries in the selected PM-segments are deleted.
- **Get-Segment-Info**
This method allows the manager to retrieve the PM-segment attributes.
- **Get-Segment-Id-List**
This method allows the manager to retrieve a list of the instance numbers of all the PM-segments of a PM-store.
- **Trig-Segment-Data-Xfer**
This method allows the manager to initiate the transfer of the data entries stored in the PM-segment object.

6.9.5 PM-store object events

Table 22 defines the events sent by the PM-store objects.

Table 22—Glucose meter PM-store object events

Service	Subservice type name	Mode	Subservice type (event-type)	Parameters (event-info)	Results (event-reply-info)
EVENT REPORT	Segment-Data-Event	Confirmed	MDC_NOTI_SEGMENT_DATA	SegmentDataEvent	SegmentDataResult

— **Segment-Data-Event**

This event allows the agent to send the data entries stored in the PM-segment object. This event is triggered by the manager using the Trig-Segment-Data-Xfer action.

6.9.6 PM-store object services

6.9.6.1 GET service

The PM-store object supports the GET service to retrieve the values of all PM-store object attributes. The GET service may be invoked as soon as the agent is in the Operating state.

6.9.7 PM-segment objects

Each of the PM-store objects contains a corresponding PM-segment object.

Table 23 defines the attributes of the PM-segment object contained in the PM-store object that represents the stored glucose measurements. The nomenclature code to identify the PM-segment object class is MDC_MOC_PM_SEGMENT.

Table 23—Common PM-segment object attributes

Attribute name	Extended configuration	
	Value	Qualifier
Instance Number	See IEEE Std 11073-20601-2014.	M
PM-Segment-Entry-Map	See IEEE Std 11073-20601-2014.	M
PM-Seg-Person-Id	See IEEE Std 11073-20601-2014.	C
Sample-Period	See IEEE Std 11073-20601-2014.	C
Operational-State	See IEEE Std 11073-20601-2014.	M
Segment-Label	See IEEE Std 11073-20601-2014.	M
Segment-Start-Abs-Time	See IEEE Std 11073-20601-2014.	C
Segment-End-Abs-Time	See IEEE Std 11073-20601-2014.	C
Segment-Start-BO-Time	See IEEE Std 11073-20601-2014.	R
Segment-End-BO-Time	See IEEE Std 11073-20601-2014.	R
Segment-Date-and-Time-Adjustment	See IEEE Std 11073-20601-2014.	C
Segment-Usage-Count	See IEEE Std 11073-20601-2014.	M
Segment-Statistics	See IEEE Std 11073-20601-2014.	O
Fixed-Segment-Data	Segment data transferred as an array of entries in a format as specified in the PM-Segment-Entry-Map attribute.	M
Confirm-Timeout	See IEEE Std 11073-20601-2014.	O
Transfer-Timeout	See IEEE Std 11073-20601-2014.	M

The Fixed-Segment-Data attribute stores the actual measurements or context logs. When the Fixed-Segment-Data attribute is transmitted, all entries in the event report are formatted according to the PM-Segment-Entry-Map. Each entry stores a single sample point, which may consist of a set of attributes.

6.10 Scanner objects

Scanner objects are not required by this standard.

6.11 Class extension objects

In this standard, no class extension objects are defined with respect to IEEE Std 11073-20601-2014.

6.12 Glucose meter information model extensibility rules

The glucose meter domain information model of this standard may be extended by including vendor-specific metrics and attributes as required. For example, a vendor might include a cholesterol measurement in addition to the glucose measurement. Any object or attribute extensions implemented should follow the guidelines of this standard as closely as possible.

A glucose meter agent having a configuration with extensions beyond the standard configuration, as specified in this standard, shall use a configuration ID in the range of IDs reserved for extended configurations (see IEEE Std 11073-20601-2014).

7. Glucose meter service model

7.1 General

The service model defines the conceptual mechanisms for data exchange services. These services are mapped to messages that are exchanged between the agent and the manager. Protocol messages within the ISO/IEEE 11073 series of standards are defined in ASN.1. See IEEE Std 11073-20601-2014 for a detailed description of the personal health device service model. Subclauses 7.2 and 7.3 define the specifics of object access and event reporting services for a glucose meter agent according to this standard.

7.2 Object access services

The object access services of IEEE Std 11073-20601-2014 are used to access the objects defined in the domain information model of the glucose device.

The following generic object access services are supported by a glucose meter agent according to this standard:

- **GET service:** used by the manager to retrieve the values of the agent MDS and PM-store object attributes. The list of glucose meter MDS object attributes is given in 6.5.4.1, and the list of glucose meter PM Store attributes is given in 6.9.3.

- **SET service:** used by the manager to set the values of the agent object attributes. No settable attributes are defined for a glucose meter agent according to this standard.
- **Event report service:** used by the agent to send configuration reports and measurement data to the manager. The list of event reports for the glucose meter device specialization is given in 6.5.3.
- **Action service:** used by the manager to invoke actions (or methods) supported by the agent. An example is Set-Time action, which is used to set a real-time clock with the absolute time at the agent.

Table 24 summarizes the object access services described in this standard.

7.3 Object access event report services

The event report service (see Table 24) is used by the agent to report its information (e.g., measurements). Event reports in this standard are a property of the MDS object only. The event reports used in this standard are defined in IEEE Std 11073-20601-2014.

The following conditions apply for a glucose meter agent according to this standard:

- Event reports shall be used in confirmed mode.
- Agent-initiated mode shall be supported for measurement data transmission.

A glucose meter agent designed to operate in an environment where data may be collected from multiple people may use one of the multiple-person event report styles to transmit all the data from each person in a single event. If this functionality is not required, the agent may use the single-person event report styles, which have reduced overhead.

A manager shall support both single-person and multiple-person event reports. A glucose meter agent may support either one or both single-person and multiple-person event reports. The formats for single- and multiple-person reports are described in IEEE Std 11073-20601-2014.

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017

Table 24—Glucose meter object access services

Service	Subservice type name	Mode	Subservice type	Parameters	Result	Remarks
GET	<na>	<implied Confirmed>	<na>	GetArgument Simple = (obj-handle = 0), attribute-id-list <optional>	GetResultSimple = (obj-handle = 0), attribute-list	Allows the manager to retrieve the value of an attribute of an object in the agent.
	<na>	<implied Confirmed>	<na>	GetArgument Simple = (obj-handle = handle of PM-Store object), attribute-id-list <optional>	GetResultSimple = (obj-handle = handle of PM-Store object), attribute-list	Allows the manager to retrieve the values of all PM-store object attributes.
EVENT REPORT	MDS-Configuration-Event	Confirmed	MDC_NOTI_CONFIG	ConfigReport	ConfigReportRsp	Configuration Report to inform manager of the agent's configuration.
	MDS-Dynamic-Data-Update-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_FIXED	ScanReport InfoFixed	—	Data Report to provide dynamic data to manager for some or all of the agent's objects in fixed format.
	MDS-Dynamic-Data-Update-Var	Confirmed	MDC_NOTI_SCAN_REPORT_VAR	ScanReport InfoVar	—	Data Report to provide dynamic data to manager for some or all of the agent's objects in variable format.
	MDS-Dynamic-Data-Update-MP-Fixed	Confirmed	MDC_NOTI_SCAN_REPORT_MP_FIXED	ScanReport InfoMPFixed	—	This is the same as MDS-Dynamic-Data-Update-Fixed but allows inclusion of data from multiple people.
	MDS-Dynamic-Data-Update-MP-Var	Confirmed	MDC_NOTI_SCAN_REPORT_MP_VAR	ScanReport InfoMPVar	—	This is the same as MDS-Dynamic-Data-Update-Var but allows inclusion of data from multiple people.
ACTION	Set-Time	Confirmed	MDC_ACT_SET_TIME	SetTime Invoke	—	Manager method to invoke the agent to set time to requested value.
	Set-Base-Offset-Time	Confirmed	MDC_ACT_SET_BO_TIME	SetBOTime Invoke	—	Manager method to invoke the agent to set time to requested value.
	Clear-Segments	Confirmed	MDC_ACT_SEG_CLR	SegmSelection	—	Allows the manager to clear some or all of the entries contained in PM-segment objects.
	Get-Segment-Info	Confirmed	MDC_ACT_SEG_GET_INFO	SegmSelection	SegmentInfoList	Allows the manager to retrieve information about some or all PM-segment objects.
	Get-Segment-Id-List	Confirmed	MDC_ACT_SEG_GET_ID_LIST	(empty)	SegmIdList	Allows the manager to retrieve a list of the instance numbers of all the PM-segments of a PM-store.
	Trig-Segment-Data-Xfer	Confirmed	MDC_ACT_SEG_TRIG_XFER	TrigSegmData XferReq	TrigSegmDataXfer Rsp	Allows the manager to begin sending segment data.

8. Glucose meter communication model

8.1 Overview

This clause describes the general communication model and procedures of the glucose meter agent as defined in IEEE Std 11073-20601-2014. Therefore, the respective parts of IEEE Std 11073-20601-2014 are not reproduced; rather, the specific choices and restrictions with respect to optional elements (e.g., objects, attributes, and actions) and specific extensions (e.g., nomenclature terms) are specified.

For an illustrative overview of the various message transactions during a typical measurement session, see the sequence diagram for the example use case in Annex D and the corresponding protocol data unit (PDU) examples in Annex E.

8.2 Communication characteristics

In this subclause, limits on the size of an application protocol data unit (APDU) transmitted or to be received by a glucose agent are defined. Small limits allow for simple implementations in terms of low cost and complexity.

A glucose agent implementing only this device specialization shall not transmit any APDU larger than N_{tx} and shall be capable of receiving any APDU up to a size of N_{rx} . For this standard, N_{tx} shall be 64 512 octets for implementations supporting persistent metric storage. In the absence of the persistent metric storage capability, N_{tx} shall be 5120 octets. For this standard, N_{rx} shall be 224 octets.

For a glucose agent implementing functions from other device specializations, an upper bound estimation of the APDU sizes brings the following: An agent shall not transmit any APDU larger than the sum of N_{tx} of all the device specializations implemented and shall be capable of receiving any APDU up to the sum of N_{rx} of all the device specializations implemented. If these numbers are higher than the maximum size determined in IEEE Std 11073-20601-2014, the latter shall be applied.

In case the APDU size limit does not allow for the inclusion of a certain amount of multiple pending measurements at the agent, they shall be sent using multiple event reports. See 8.5.3 for the maximum number of measurements allowed for inclusion in a single event report.

8.3 Association procedure

8.3.1 General

Unless otherwise stated, the association procedure for a glucose meter agent and manager according to this standard shall be pursued as specified in IEEE Std 11073-20601-2014.

8.3.2 Agent procedure—association request

In the association request sent by the agent to the manager:

- The version of the association procedure used by the agent shall be set to `assoc-version1` (i.e., `assoc-version = 0x80000000`).

- The DataProtoList structure element of the data protocol identifier shall be set to data-proto-id-20601 (i.e., *data-proto-id* = 0x5079).
- The *data-proto-info* field shall contain a PhdAssociationInformation structure that shall contain the following parameter values:
 - 1) If a glucose agent relies on a feature introduced in a specific version of the 20601 protocol, the agent shall only indicate support for that specific version of 20601 protocol or higher. The agent's supported protocol version(s) shall be indicated by setting the appropriate protocol-version bit(s).
 - i) Major features introduced with version 2 of the protocol are:
BOT to handle multiple time changes efficiently
 - ii) Major features introduced in version 3 of the protocol are:
Get Segment Id List to support reporting a large number of PM-Segments
Reporting time faults using the Date-Time-Adjustment value 7FFFFFFF
 - 2) At least the MDERs shall be supported (i.e., *encoding-rules* = 0x8000).
 - 3) The version of the nomenclature used shall be set to nom-version1 (i.e., *nomenclature-version* = 0x80000000).
 - 4) The field *functional-units* may have the test association bits set but shall not have any other bits set.
 - 5) The field *system-type* shall be set to sys-type-agent (i.e., *system-type* = 0x00800000).
 - 6) The *system-id* field shall be set to the value of the System-Id attribute of the MDS object of the agent. The manager may use this field to determine the identity of the glucose meter with which it is associating and, optionally, to implement a simple access restriction policy.
 - 7) The *dev-config-id* field shall be set to the value of the Dev-Configuration-Id attribute of the MDS object of the agent.
 - 8) If the agent supports only the glucose meter specialization, then the field indicating the data request modes (*data-req-mode-capab*) supported by the glucose meter agent shall be set to *data-req-supp-init-agent*.
 - 9) If the agent supports only the glucose meter specialization, then *data-req-init-manager-count* shall be set to zero, and *data-req-init-agent-count* shall be set to 1.

8.3.3 Manager procedure—association response

In the association response message sent by the manager:

- The *result* field shall be set to an appropriate response from those defined in IEEE Std 11073-20601-2014. For example, if all other conditions of the association protocol are satisfied, *accepted* is returned when the manager recognizes the *dev-config-id* of the agent and *accepted-unknown-config* otherwise.

In the DataProtoList structure element, the data protocol identifier shall be set to data-proto-id-20601 (i.e., *data-proto-id* = 0x5079).

- The *data-proto-info* field shall be filled in with a PhdAssociationInformation structure that shall contain the following parameter values:
 - 1) The manager shall respond to protocol versions supported by setting the appropriate bit in the protocol-version.
 - 2) The manager shall respond with a single selected encoding rule that is supported by both agent and manager. The manager shall support at least the MDERs.

- 3) The version of the nomenclature used shall be set to *nom-version1* (i.e., *nomenclature-version* = 0x80000000).
- 4) The field *functional-units* shall have all bits reset except for those relating to a test association.
- 5) The field *system-type* shall be set to *sys-type-manager* (i.e., *system-type* = 0x80000000).
- 6) The *system-id* field shall contain the unique system ID of the manager, which shall be a valid EUI-64 type identifier.
- 7) The field *dev-config-id* shall be *manager-config-response* (0).
- 8) The field *data-req-mode-capab* shall be 0.
- 9) The fields *data-req-init-*-count* shall be 0.

8.4 Configuring procedure

8.4.1 General

The agent enters the Configuring state if it receives an association response of *accepted-unknown-config*. In this case, the configuration procedure as specified in IEEE Std 11073-20601-2014 shall be followed. Subclause 8.4.2 specifies the configuration notification and response messages for a glucose meter agent with standard configuration ID 0x06A5 (1701), and 8.4.2 specifies the configuration notification and response messages for a glucose meter agent with a standard configuration ID 0x06A6 (1702) as introduced in this version of 10417. Normally, a manager would already know the standard configuration. However, standard configuration devices are required to send their configuration, if requested. This covers a case where an agent associates with a manager that does not have preconfigured knowledge of the standard configuration (e.g., due to a version mismatch between agent and manager).

The agent shall support the GET service for the MDS attributes during the Configuring state.

8.4.2 Glucose meter—standard configuration (0x06A5)

8.4.2.1 Agent procedure

The agent performs the configuration procedure using a “Remote Operation Invoke | Confirmed Event Report” message with an *MDC_NOTI_CONFIG* event to send its configuration to the manager (see IEEE Std 11073-20601-2014). The *ConfigReport* structure is used for the *event-info* field (see Table 4). For a glucose meter agent with standard configuration 1701 with ID 0x06A5, the format and contents of the configuration notification message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x70	CHOICE.length = 112
0x00 0x6E	OCTET STRING.length = 110
0x00 0x01	<i>invoke-id</i> (differentiates this message from any other outstanding)
0x01 0x01	CHOICE (Remote Operation Invoke Confirmed Event Report)
0x00 0x68	CHOICE.length = 104
0x00 0x00	<i>obj-handle</i> = 0 (MDS object)
0xFF 0xFF 0xFF 0xFF	<i>event-time</i> (set to 0xFFFFFFFF if <i>RelativeTime</i> is not supported)
0x0D 0x1C	<i>event-type</i> = <i>MDC_NOTI_CONFIG</i>
0x00 0x5E	<i>event-info.length</i> = 94 (start of <i>ConfigReport</i>)

0x06	0xA5			config-report-id (Dev-Configuration-Id value)
0x00	0x02			config-obj-list.count = 2 Measurement objects will be “announced”
0x00	0x58			config-obj-list.length = 88
0x00	0x06			obj-class = MDC_MOC_VMO_METRIC_NU
0x00	0x01			obj-handle = 1 (→ 1 st Measurement is blood glucose)
0x00	0x04			attributes.count = 4
0x00	0x24			attributes.length = 36
0x09	0x2F			attribute-id = MDC_ATTR_ID_TYPE
0x00	0x04			attribute-value.length = 4
0x00	0x02			MDC_PART_SCADA
0x72	0x70			MDC_CONC_GLU_UNDETERMINED_PLASMA
0x0A	0x46			attribute-id = MDC_ATTR_METRIC_SPEC_SMALL
0x00	0x02			attribute-value.length = 2
0xF0	0x40			intermittent, stored data, upd & msmt aperiodic, agent init, measured
0x09	0x96			attribute-id = MDC_ATTR_UNIT_CODE
0x00	0x02			attribute-value.length = 2
0x08	0x52			MDC_DIM_MILLI_G_PER_DL
0x0A	0x55			attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00	0x0C			attribute-value.length = 12
0x00	0x02			AttrValMap.count = 2
0x00	0x08			AttrValMap.length = 8
0x0A	0x4C	0x00	0x02	MDC_ATTR_NU_VAL_OBS_BASIC value length = 2
0x09	0x90	0x00	0x08	MDC_ATTR_TIME_STAMP_ABS value length = 8
0x00	0x06			obj-class = MDC_MOC_VMO_METRIC_NU
0x00	0x02			obj-handle = 2 (→ 2 nd Measurement is control solution)
0x00	0x04			attributes.count = 4
0x00	0x24			attributes.length = 36
0x09	0x2F			attribute-id = MDC_ATTR_ID_TYPE
0x00	0x04			attribute-value.length = 4
0x00	0x02			MDC_PART_SCADA
0x71	0xD0			MDC_CONC_GLU_CONTROL
0x0A	0x46			attribute-id = MDC_ATTR_METRIC_SPEC_SMALL
0x00	0x02			attribute-value.length = 2
0xF0	0x40			intermittent, stored data, upd & msmt aperiodic, agent init, measured
0x09	0x96			attribute-id = MDC_ATTR_UNIT_CODE
0x00	0x02			attribute-value.length = 2
0x08	0x52			MDC_DIM_MILLI_G_PER_DL
0x0A	0x55			attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00	0x0C			attribute-value.length = 12
0x00	0x02			AttrValMap.count = 2
0x00	0x08			AttrValMap.length = 8
0x0A	0x4C	0x00	0x02	MDC_ATTR_NU_VAL_OBS_BASIC value length = 2
0x09	0x90	0x00	0x08	MDC_ATTR_TIME_STAMP_ABS value length = 8

8.4.2.2 Manager procedure

The manager shall respond to a configuration notification message using a “Remote Operation Response | Confirmed Event Report” data message with an MDC_NOTI_CONFIG event using the ConfigReportRsp structure for the *event-info* field (see Table 4). As a response to the standard configuration notification

message in 8.4.2.1, the format and contents of the manager’s configuration notification response message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x16	CHOICE.length = 22
0x00 0x14	OCTET STRING.length = 20
0x00 0x01	invoke-id (differentiates this message from any other outstanding)
0x02 0x01	CHOICE (Remote Operation Response Confirmed Event Report)
0x00 0x0E	CHOICE.length = 14
0x00 0x00	obj-handle = 0 (MDS object)
0x05 0x14 0xDB 0x12	currentTime
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x04	event-reply-info.length = 4
0x06 0xA5	ConfigReportRsp.config-report-id = 1701
0x00 0x00	ConfigReportRsp.config-result = accepted-config

8.4.3 Glucose meter—standard configuration (0x06A6)

8.4.3.1 Agent procedure

The agent performs the configuration procedure using a “Remote Operation Invoke | Confirmed Event Report” message with an MDC_NOTI_CONFIG event to send its configuration to the manager (see IEEE Std 11073-20601-2014). The ConfigReport structure is used for the *event-info* field (see Table 4). For a glucose meter agent with standard configuration ID 0x06A6, the format and contents of the configuration notification message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x96	CHOICE.length = 150
0x00 0x94	OCTET STRING.length = 148
0x00 0x02	invoke-id = 2 (differentiates this message from any other outstanding)
0x01 0x01	CHOICE (Remote Operation Invoke Confirmed Event Report Simple)
0x00 0x8E	CHOICE.length = 142
0x00 0x00	obj-handle = 0 (MDS object)
0xFF 0xFF 0xFF 0xFF	event-time (set to 0xFFFFFFFF if RelativeTime is not supported)
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x84	event-info.length = 132 (start of ConfigReport)
0x06 0xA6	config-report-id = 06A6 (Dev-Configuration-Id value=1702)
0x00 0x03	config-obj-list.count = 3 objects will be “announced”
0x00 0x7E	config-obj-list.length = 126
0x00 0x05	obj-class = MDC_MOC_VMO_METRIC_NU
0x00 0x01	obj-handle = 1 (→ 1st Measurement is blood glucose)
0x00 0x04	attributes.count = 4
0x00 0x24	attributes.length = 36
0x0A 0x46	attribute-id = MDC_ATTR_METRIC_SPEC_SMALL
0x00 0x02	attribute-value.length = 2
0xF0 0x40	intermittent, stored data, upd & msmt aperiodic, agent init, measured
0x0A 0x55	attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00 0x0C	attribute-value.length = 12
0x00 0x02	AttrValMap.count = 2
0x00 0x08	AttrValMap.length = 8
0x0A 0x4C 0x00 0x02	MDC_ATTR_NU_VAL_OBS_BASIC value length = 2

0x0A	0x82	0x00	0x08	MDC_ATTR_TIME_STAMP_BO value length = 8
0x09	0x96			attribute-id = MDC_ATTR_UNIT_CODE
0x00	0x02			attribute-value.length = 2
0x08	0x52			MDC_DIM_MILLI_G_PER_DL
0x09	0x2F			attribute-id = MDC_ATTR_ID_TYPE
0x00	0x04			attribute-value.length = 4
0x00	0x02			MDC_PART_SCADA
0x72	0x70			MDC_CONC_GLU_UNDETERMINED_PLASMA
0x00	0x06			obj-class = MDC_MOC_VMO_METRIC_NU
0x00	0x02			obj-handle = 2 (→ 2nd Measurement is control solution)
0x00	0x04			attributes.count = 4
0x00	0x24			attribute-value.length = 36
0x0A	0x46			attribute-id = MDC_ATTR_METRIC_SPEC_SMALL
0x00	0x02			attribute-value.length = 2
0xF0	0x40			intermittent, stored data, upd & msmt aperiodic, agent init, measured
0x0A	0x55			attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00	0x0C			attribute-value.length = 12
0x00	0x02			AttrValMap.count = 2
0x00	0x08			AttrValMap.length = 8
0x0A	0x4C	0x00	0x02	MDC_ATTR_NU_VAL_OBS_BASIC value length = 2
0x0A	0x82	0x00	0x08	MDC_ATTR_TIME_STAMP_BO value length = 8
0x09	0x96			attribute-id = MDC_ATTR_UNIT_CODE
0x00	0x02			attribute-value.length = 2
0x08	0x52			MDC_DIM_MILLI_G_PER_DL
0x09	0x2F			attribute-id = MDC_ATTR_ID_TYPE
0x00	0x04			attribute-value.length = 4
0x00	0x02			MDC_PART_SCADA
0x71	0xD0			MDC_CONC_GLU_CONTROL
0x00	0x05			obj-class = MDC_MOC_VMO_METRIC_ENUM
0x00	0x03			obj-handle = 3 (→ 3rd object is Context-Meal)
0x00	0x03			attributes.count = 3
0x00	0x1E			attributes.length = 30
0x0A	0x46			attribute-id = MDC_ATTR_METRIC_SPEC_SMALL
0x00	0x02			attribute-value.length = 2
0xF0	0x40			intermittent, stored data, upd & msmt aperiodic, agent init, measured
0x0A	0x55			attribute-id = MDC_ATTR_ATTRIBUTE_VAL_MAP
0x00	0x0C			attribute-value.length = 12
0x00	0x02			AttrValMap.count = 2
0x00	0x08			AttrValMap.length = 8
0x0A	0x49			attribute-id = MDC_ATTR_ENUM_OBS_VAL_SIMP_OID
0x00	0x04			attribute-value.length = 4
0x0A	0x82	0x00	0x08	MDC_ATTR_TIME_STAMP_BO value length = 8
0x09	0x2F			attribute-id = MDC_ATTR_ID_TYPE
0x00	0x04			attribute-value.length = 4
0x00	0x80	0x72	0x48	MDC_PART_PHD_DM MDC_CTXT_GLU_MEAL

8.4.3.2 Manager procedure

The manager shall respond to a configuration notification message using a “Remote Operation Response | Confirmed Event Report” data message with an MDC_NOTI_CONFIG event using the ConfigReportRsp structure for the *event-info* field (see Table 4). As a response to the standard configuration notification

message in 8.4.2.1, the format and contents of the manager's configuration notification response message are as follows:

0xE7 0x00	APDU CHOICE Type (PrstApdu)
0x00 0x16	CHOICE.length = 22
0x00 0x14	OCTET STRING.length = 20
0x00 0x02	invoke-id (differentiates this message from any other outstanding)
0x02 0x01	CHOICE (Remote Operation Response Confirmed Event Report)
0x00 0x0E	CHOICE.length = 14
0x00 0x00	obj-handle = 0 (MDS object)
0x05 0x14 0xDB 0x12	currentTime
0x0D 0x1C	event-type = MDC_NOTI_CONFIG
0x00 0x04	event-reply-info.length = 4
0x06 0xA6	ConfigReportRsp.config-report-id = 1702
0x00 0x00	ConfigReportRsp.config-result = accepted-config

8.5 Operating procedure

8.5.1 General

Measurement data and status information are communicated from the glucose meter agent during the Operating state. If not stated otherwise, the operating procedure for a glucose meter agent of this standard shall be as specified in IEEE Std 11073-20601-2014.

8.5.2 GET glucose meter MDS and PM-store attributes

The glucose meter shall support the GET service for MDS and PM-store objects (if it has PM-store objects) according to IEEE Std 11073-20601-2014.

See Table 5 for a summary of the GET service.

If the manager leaves the *attribute-id-list* field in the roiv-cmip-get service message empty, the glucose meter agent shall respond with a rors-cmip-get service message in which the attribute-list contains a list of all implemented attributes of the MDS object. This allows the glucose meter agent to store a predefined transmission template for its response message and to modify just the varying parts at fixed locations before sending.

If the manager requests specific MDS object attributes, indicated by the elements in *attribute-id-list*, and the agent supports this capability, the glucose meter agent shall respond with a rors-cmip-get service message in which the attribute-list contains a list of the requested attributes of the MDS object that are implemented. It is not required for a glucose meter agent to support this capability. If this capability is not implemented, the glucose meter agent shall respond with a "Remote Operation Error Result" (roer) service message (see IEEE Std 11073-20601-2014) with the error-value field set to no-such-action (9).

8.5.3 Measurement data transmission

See Table 4 and Table 22 for a summary of the event report services available for measurement data transfer.

For temporary store measurement, data transfer for a glucose meter agent of this standard shall always be initiated by the glucose meter (see agent-initiated measurement data transmission in IEEE Std 11073-20601-2014). To limit the amount of data being transported within an APDU, the glucose meter agent shall not include more than 25 temporarily stored measurements in a single event report. If more than 25 pending measurements are available for transmission, they shall be sent using multiple event reports. If multiple glucose measurements are available, up to 25 measurements should be transmitted within a single event report. Alternatively, they may be transmitted using a single event report for each glucose measurement. However, the former strategy is recommended to reduce overall message size and power consumption.

For PM-store transfers, the manager inspects the available segments and retrieves all applicable data.

8.6 Time synchronization

Time synchronization may be employed between a glucose meter and a manager to coordinate the clocks used when reporting physiological events. Note that the mechanism for synchronizing an agent to a manager is outside the scope of this standard. If time synchronization is used, then this shall be reported in the Mds-Time-Info attribute of the MDS object.

9. Test associations

A glucose meter may implement a wide range of behaviors in a test association that enable a manufacturer to test features of a product in a comprehensive manner. It is also possible for a glucose meter not to support test associations at all. This clause defines a simple behavior that simulates the generation of a measurement in the context of a standard device configuration.

9.1 Behavior with standard configuration

To facilitate automated standardized test processes, a glucose meter that presents the standard configuration ID and enters into a test association should be able to simulate the arrival of measurement data from the device measurement engine. It should not be necessary for an operator to perform a test for the measurement data to be generated.

After the agent enters the Operating state, it simulates the reception of an event from the measurement engine representing a blood glucose measurement of 999 mg/dL. To the extent possible, this measurement is observed only by those components of the agent that understand the test association. When the event is propagated into a numeric object, the test-data bit of the measurement-status attribute shall be set if the measurement-status attribute is supported. An agent is not required to use the measurement-status attribute if it would not normally do so outside of a test association.

The agent should send the events reports for all simulated measures within 30 s of entering the Operating state. The test association is terminated in a manner consistent with the agent's normal behavior for terminating an association.

9.2 Behavior with extended configurations

This specification does not define a test association that uses an extended configuration.

10. Conformance

10.1 Applicability

This standard shall be used in conjunction with IEEE Std 11073-20601-2014.

An implementation or a system can conform to the following elements of this standard:

- Domain information model class hierarchy and object definitions (object attributes, notifications, methods, and data type definitions)
- Nomenclature code values
- Protocol and service models
- Communication service model (association and configuration)

10.2 Conformance specification

This standard offers levels of conformance with respect to strict adherence to the standard device and the use of extensions for:

- Information model of a specific device
- Use of attributes, value ranges, and access methods

A vendor shall specify the level of conformance for an implementation based on this standard and provide details of the way in which the definitions of this standard and any extensions are applied.

Specifications shall be provided in the form of a set of implementation conformance statements (ICS) as detailed in 10.4.

Because this standard is used in conjunction with IEEE Std 11073-20601-2014, the ICS should be created for this standard first. The ICS created for IEEE Std 11073-20601-2014 may then refer to the ICS for this standard where applicable.

10.3 Levels of conformance

10.3.1 General

This standard defines the following levels of conformance.

10.3.2 Conformance level 1: base conformance

The application uses elements of the information, service, and communication models (object hierarchy, actions, event reports, and data type definitions) and the nomenclature scheme defined in IEEE Std 11073-20601-2014 and ISO/IEEE 11073-104zz standards. All mandatory features defined in the object definition tables and in the ICS tables are implemented. Furthermore, any conditional, recommended, or optional features that are implemented shall follow the requirements in IEEE Std 11073-20601-2014 and ISO/IEEE 11073-104zz documents.

**10.3.3 Conformance level 2: extended nomenclature
(ASN.1 and/or ISO/IEEE 11073-10101:2004 [B2])**

Conformance level 2 meets conformance level 1 but also uses or adds extensions in at least one of the information, service, communication, or nomenclature models. These extensions shall conform to nomenclature codes from ASN.1 and/or within the ISO/IEEE 11073-10101:2004 [B2] framework (0xF000 through 0xFFFF). These extensions should be defined in ICS tables pointing toward their reference.

10.4 Implementation conformance statements**10.4.1 General format**

The ICS are provided as an overall conformance statement document that comprises a set of tables in the form given by the templates in the following clauses.

Each ICS table has the following columns:

Index	Feature	Reference	Req./Status	Support	Comment
-------	---------	-----------	-------------	---------	---------

The table column headings have the following meaning:

- Index: an identifier (e.g., a tag) of a specific feature.
- Feature: briefly describes the characteristic for which a conformance statement is being made.
- Reference: to the clause/paragraph within this document or to an external source for the definition of the feature (may be empty).
- Req./Status: specifies the conformance requirement (e.g., mandatory or recommended)—in some cases, this standard does not specify conformance requirements but requests the status of a particular feature be provided.
- Support: specifies the presence or absence of a feature and any description of the characteristics of the feature in the implementation. This column is to be filled out by the implementer.
- Comment: contains any additional information on the feature. This column is to be filled out by the implementer.

Subclauses 10.4.2 through 10.4.6 specify the format of the specific ICS tables.

10.4.2 General implementation conformance statement

The general ICS specify the versions/revisions that are supported by the implementation and high-level system behavior.

Table 25 shows the general ICS.

Table 25—11073-10417 general ICS table

Index	Feature	Reference	Req./Status	Support	Comment
EN 11073-10417-1	Implementation description	—	Identification of the device/application. Description of functionality.		
GEN 11073-10417-2	Standards followed and their revisions	(Standard documents)	(Set of existing revisions)	(Set of supported revision)	
GEN 11073-10417-3	Nomenclature document used and revision	(Standard documents)	(Set of existing revisions)	(Set of supported revisions)	
GEN 11073-10417-4	Conformance adherence—level 1	See 10.3.3	Base conformance declaration that device meets the following IEEE Std 11073-10417 conformance requirements: a) All mandatory requirements shall be implemented. b) If implemented, conditional, recommended, and optional requirements shall conform to standard.	Yes/No (No is not expected as No implies that the implementation is non-conformant)	
GEN 11073-10417-5	Conformance adherence—level 2	See 6.3	In addition to GEN 11073-10417-4, if the device implements extensions and/or additions, they shall conform to nomenclature codes from ASN.1 and/or 10101 framework. These extensions should also be defined in ICS tables pointing toward their reference.	Yes/No	
GEN 11073-10417-6	Object containment tree	See 6.3	Provide object containment diagram showing relations between object instances used by the application. A conforming implementation uses only object relations as defined in the DIM.		
GEN 11073-10417-7	Nomenclature document used and revision	(Standard documents)	(Set of existing revisions)	(Set of supported revision)	
GEN 11073-10417-8	Data structure encoding	—	—	Description of encoding method(s) for ASN.1 data structures	
GEN 11073-10417-9	Use of private objects	—	Does the implementation use objects that are not defined in the DIM?	Yes/No (If yes: explain in Table 26)	
GEN 11073-10417-10	Use of private nomenclature extensions	—	Does the implementation use private extensions to the nomenclature (i.e., 0xF000 through 0xFFFF codes from ISO/IEEE 11073-10101:2004 [B2])? Private Nomenclature extensions are <i>only</i> allowed if the standard nomenclature does not include the specific terms required by the application.	Yes/No (If yes: explain in Table 29)	
GEN 11073-10417-11	11073-20601 conformance		Provide the conformance report required by IEEE Std 11073-20601-2014.		

^a The prefix GEN11073-10417- is used for the index in the general ICS table.

10.4.3 DIM MOC implementation conformance statement

The DIM MOC ICS define which objects are implemented. Information on each object shall be provided as a separate row in the template of Table 26.

Table 26—Template for DIM MOC ICS table

Index	Feature	Reference	Req./Status	Support	Comment
MOC- <i>n</i>	Object description	Reference to the clause in the standard or other location where the object is defined.	Implemented	Specify restrictions, e.g., max. number of supported instances	

The *n* in the Index column should be the object handle for implementations that have predefined objects. Otherwise the Index column shall simply be a unique number (1..*m*).

All private objects should be specified and include either a reference to the definition for the object, or where no publicly available reference is available, the definition of the object should be appended to the conformance statement.

The Support column should indicate any restrictions for the object implementation.

An object containment diagram (class instance diagram) should be provided as part of the DIM MOC ICS.

10.4.4 MOC attribute ICS

For each supported object as defined in the DIM MOC ICS, a MOC attribute ICS has to be provided that defines which attributes are used/supported by the implementation, including any inherited attributes. Table 27 is a template only.

Table 27—Template for MOC attribute ICS table

Index	Feature	Reference	Req./Status	Support	Comment
ATTR- <i>n-x</i>	Attribute name. Extended attributes shall include the Attribute ID also.	Fill in the reference to the ASN.1 structure if the attribute is not defined in this standard.	M = Mandatory C = Conditional R = Recommended O = Optional (as per definition in Attribute Definition Tables)	Implemented? Yes/No Static/Dynamic Specify restrictions (e.g., value ranges). Describe how attribute is accessed (e.g., Get, Set, sent in config event report, sent in a data event report). Describe any specific restrictions.	

All private attributes should be specified and include reference to the definition for the attribute. Where no publicly available reference is available, the definition of the attribute should be appended to the conformance statement.

The Support column shall specify whether the attribute is implemented; for extension attributes, whether the attribute value is static or dynamic; any value ranges; restrictions on attribute access or availability; and any other information.

The *n* in the Index column refers to the ID of the managed object for which the table is supplied (i.e., the index of the managed object as specified in the MOC ICS). There is one separate table for each supported managed object.

The *x* in the Index column is a unique serial number (1..*m*).

NOTE—The attribute definition tables in the standard define a minimum mandatory set of attributes for each object.

10.4.5 MOC notification implementation conformance statement

The MOC notification ICS specify all implemented notifications (typically in form of the event report service) that are emitted by the agent. Table 28 provides a template for use. One table has to be provided for each object that supports special object notifications.

Table 28—Template for MOC notification ICS table

Index	Feature	Reference	Req./Status	Support	Comment
NOTI- <i>n-x</i>	Notification name and Notification ID	Reference to the clause in the standard or other location where the event is defined.		The Support column shall specify how the notification is sent and any restrictions.	

The *n* in the Index column refers to the ID of the managed object for which the table is supplied (i.e., the index of the managed object as specified in the POC ICS). There is one separate table for each managed object that supports specific object notifications (i.e., events).

The *x* in the Index column of Table 28 is a unique serial number (1..*m*).

All private notifications should be specified and include reference to the definition for the notification. Where no publicly available reference is available, the definition of the notification should be appended to the conformance statement.

10.4.6 MOC nomenclature conformance statement

The MOC nomenclature ICS specify all nonstandard nomenclature codes that are utilized by the agent. Table 29 provides a template for use. One row of the table is to be used for each nomenclature element.

Table 29—Template for MOC nomenclature ICS table

Index	Feature	Reference	Req./Status	Support	Comment
NOME- <i>n</i>	Nomenclature name and nomenclature value	Reference to the clause in the standard or other location where the nomenclature is defined or used.		Describe how the nomenclature is used. Describe any specific restrictions.	

The *n* in the Index column is a unique serial number (1..*m*).

Annex A

(informative)

Bibliography

Bibliographical references are resources that provide additional or helpful material but do not need to be understood or used to implement this standard. Reference to these resources is made for informational use only.

[B1] American Diabetes Association, “Standards of medical care in diabetes—2006,” *Diabetes Care*, vol. 29, suppl. 1, Jan. 2006.

[B2] ISO/IEEE 11073-10101:2004, Health informatics—Point-of-care medical device communication—Part 10101: Nomenclature.⁹

[B3] ISO/IEEE 11073-10201:2004, Health informatics—Point-of-care medical device communication—Part 10201: Domain information model.

[B4] ISO/IEEE 11073-20101:2004, Health informatics—Point-of-care medical device communication—Part 20101: Application profile—Base standard.

[B5] ITU-T Rec. X.680-2002, Information technology—Abstract Syntax Notation One (ASN.1): Specification of basic notation.¹⁰

⁹ ISO/IEEE publications are available from the ISO Central Secretariat, 1, ch. de la Voie-Creuse, Case postale 56, CH-1211, Geneva 20, Switzerland (<http://www.iso.ch/>). ISO/IEEE publications are also available in the United States from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, Piscataway, NJ 08854-4141, USA (<http://standards.ieee.org/>).

¹⁰ ITU publications are available from the International Telecommunications Union, Place des Nations, 1211 Geneva 20, Switzerland (<http://www.itu.in/>).

Annex B

(normative)

Any additional ASN.1 definitions

B.1 Device and sensor status bit mapping

The threshold extensions to the enumeration class require the following ASN.1 structure definitions:

```
GlucoseDevStat ::= BITS-16 {  
    device-battery-low(0),  
    sensor-malfunction(1),  
    sensor-sample-size-insufficient(2),  
    sensor-strip-insertion(3),  
    sensor-strip-type-incorrect(4),  
    sensor-result-too-high(5),  
    sensor-result-too-low(6),  
    sensor-temp-too-high(7),  
    sensor-temp-too-low(8),  
    sensor-read-interrupt(9),  
    device-gen-fault(10),  
    sensor-temp-out-of-range(11)  
}
```

STANDARDSISO.COM : Click to view the full PDF of ISO/IEEE 11073-10417:2017

Annex C

(normative)

Allocation of identifiers

C.1 General

This annex contains the nomenclature codes used in this document and not found in IEEE Std 11073-20601-2014. For those not contained in this annex, the normative definition is found in IEEE Std 11073-20601-2014.

C.2 Definitions of terms and codes

The format used here follows that of ISO/IEEE 11073-10101:2004 [B2].

```

/*****
* From Medical supervisory control and data acquisition (MDC_PART_SCADA)
*****/
#define MDC_CONC_GLU_CAPILLARY_WHOLEBLOOD 29112/* */
#define MDC_CONC_GLU_CAPILLARY_PLASMA 29116/* */
#define MDC_CONC_GLU_VENOUS_WHOLEBLOOD 29120/* */
#define MDC_CONC_GLU_VENOUS_PLASMA 29124/* */
#define MDC_CONC_GLU_ARTERIAL_WHOLEBLOOD 29128/* */
#define MDC_CONC_GLU_ARTERIAL_PLASMA 29132/* */
#define MDC_CONC_GLU_UNDETERMINED_WHOLEBLOOD 29292/* */
#define MDC_CONC_GLU_UNDETERMINED_PLASMA 29296/* */
#define MDC_CONC_GLU_CONTROL 29136/* */
#define MDC_CONC_GLU_CONTROL_LEVEL_LOW 29300/* */
#define MDC_CONC_GLU_CONTROL_LEVEL_MEDIUM 29304/* */
#define MDC_CONC_GLU_CONTROL_LEVEL_HIGH 29308/* */
#define MDC_CONC_GLU_ISE 29140/* */
#define MDC_CONC_GLU_CONTROL_LEVEL_UNDETERMINED 29312/* */
#define MDC_CONC_HBA1C 29148/* */

/*****
* From Personal Health Device Disease Management (MDC_PART_PHD_DM)
*****/
#define MDC_GLU_METER_DEV_STATUS 29144/* */
#define MDC_CTXT_GLU_EXERCISE 29152/* */
#define MDC_CTXT_GLU_CARB 29156/* */
#define MDC_CTXT_GLU_CARB_UNDETERMINED 29157/* */
#define MDC_CTXT_GLU_CARB_OTHER 29158/* */
#define MDC_CTXT_GLU_CARB_NO_ENTRY 29159/* */
#define MDC_CTXT_GLU_CARB_BREAKFAST 29160/* */
#define MDC_CTXT_GLU_CARB_NO_INGESTION 29161/* */
#define MDC_CTXT_GLU_CARB_LUNCH 29164/* */
#define MDC_CTXT_GLU_CARB_DINNER 29168/* */
#define MDC_CTXT_GLU_CARB_SNACK 29172/* */
#define MDC_CTXT_GLU_CARB_DRINK 29176/* */
#define MDC_CTXT_GLU_CARB_SUPPER 29180/* */

```

```
#define MDC_CTXT_GLU_CARB_BRUNCH          29184/* */
#define MDC_CTXT_MEDICATION                29188/* */
#define MDC_CTXT_MEDICATION_RAPIDACTING    29192/* */
#define MDC_CTXT_MEDICATION_SHORTACTING    29196/* */
#define MDC_CTXT_MEDICATION_INTERMEDIATEACTING 29200/* */
#define MDC_CTXT_MEDICATION_LONGACTING     29204/* */
#define MDC_CTXT_MEDICATION_PREMIX         29208/* */
#define MDC_CTXT_GLU_HEALTH                29212/* */
#define MDC_CTXT_GLU_HEALTH_MINOR          29216/* */
#define MDC_CTXT_GLU_HEALTH_MAJOR          29220/* */
#define MDC_CTXT_GLU_HEALTH_MENSES        29224/* */
#define MDC_CTXT_GLU_HEALTH_STRESS         29228/* */
#define MDC_CTXT_GLU_HEALTH_NONE           29232/* */
#define MDC_CTXT_GLU_SAMPLELOCATION         29236/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_UNDETERMINED 29237/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_OTHER   29238/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_FINGER   29240/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_AST     29244/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_EARLOBE 29248/* */
#define MDC_CTXT_GLU_SAMPLELOCATION_CTRL SOLUTION 29252/* */
#define MDC_CTXT_GLU_MEAL                  29256/* */
#define MDC_CTXT_GLU_MEAL_PREPRANDIAL      29260/* */
#define MDC_CTXT_GLU_MEAL_BEDTIME          29261/* */
#define MDC_CTXT_GLU_MEAL_POSTPRANDIAL     29264/* */
#define MDC_CTXT_GLU_MEAL_FASTING          29268/* */
#define MDC_CTXT_GLU_MEAL_CASUAL           29272/* */
#define MDC_CTXT_GLU_TESTER                29276/* */
#define MDC_CTXT_GLU_TESTER_SELF           29280/* */
#define MDC_CTXT_GLU_TESTER_HCP            29284/* */
#define MDC_CTXT_GLU_TESTER_LAB            29288/* */
```

```
/* From Dimensions (MDC_PART_DIM)
*****
#define MDC_DIM_MILLI_L                    1618 /* mL */
#define MDC_DIM_MILLI_G                    1746 /* mg */
#define MDC_DIM_MILLI_G_PER_DL              2130 /* mg dL-1 */
#define MDC_DIM_MILLI_MOLE_PER_L           4722 /* mmol L-1 */
#define MDC_DIM_G                           1728 /* g */
#define MDC_DIM_INTL_UNIT                   5472 /* International unit */
```

C.3 Systematic derivations of terms and codes

Systematic derivations of terms and codes are outlined in Table C.1

