

# ISO

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION

## ADDENDUM 1 TO ISO RECOMMENDATION R 407

YOKE TYPE VALVE CONNECTIONS  
FOR SMALL MEDICAL GAS CYLINDERS  
USED FOR ANAESTHETIC AND RESUSCITATION PURPOSES

1st EDITION  
November 1972

COPYRIGHT RESERVED

The copyright of ISO Recommendations and ISO Standards belongs to ISO Member Bodies. Reproduction of these documents, in any country, may be authorized therefore only by the national standards organization of that country, being a member of ISO.

For each individual country the only valid standard is the national standard of that country.

Printed in Switzerland

Also issued in French and Russian. Copies to be obtained through the national standards organizations.

## FOREWORD

Addendum 1 to ISO Recommendation R 407-1964 was drawn up by Technical Committee ISO/TC 58, *Gas cylinders*.

It was approved in April 1972 by the Member Bodies of the following countries :

Belgium	India	Romania
Canada	Ireland	South Africa, Rep. of
Czechoslovakia	Israel	Sweden
Egypt, Arab Rep. of	Italy	Switzerland
France	Japan	United Kingdom
Germany	New Zealand	U.S.A.
Hungary	Norway	

The Member Body of the following country expressed disapproval of the document on technical grounds :

Austria

STANDARDSISO.COM : Click to view the full PDF of ISO R 407:1964

Addendum 1 – November 1972 – to ISO Recommendation R 407-1964


**YOKE TYPE VALVE CONNECTIONS  
FOR SMALL MEDICAL GAS CYLINDERS  
USED FOR ANAESTHETIC AND RESUSCITATION PURPOSES**

Page 3, CONTENTS : add the following new entry :

“5.9 Outlet connection for medical air”

Page 11, section 5 : add the following new clause :

**5.9 Outlet connection for medical air**

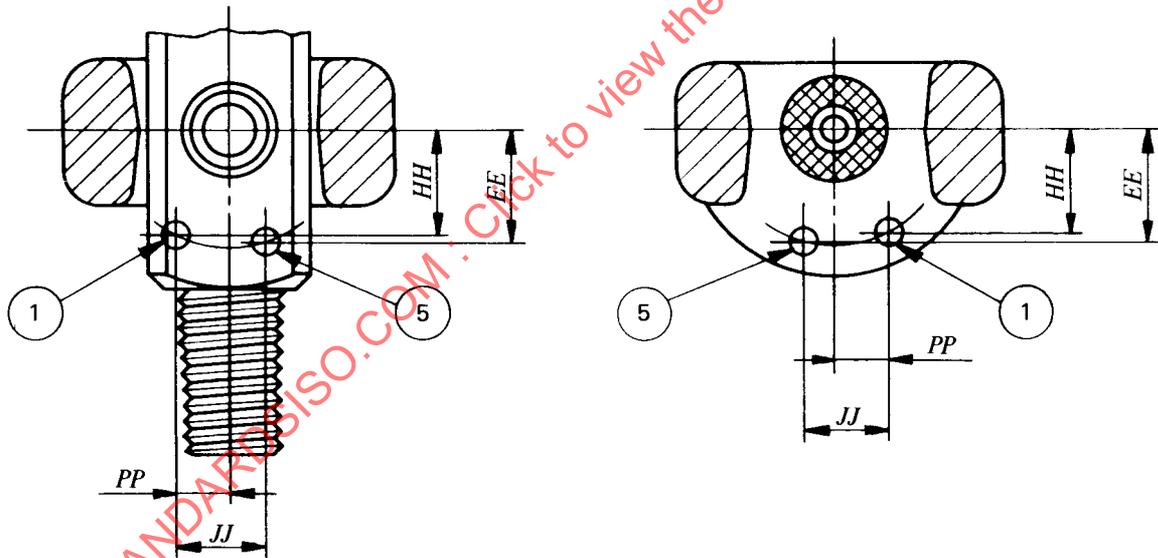

Dimensions	inches	millimetres
<i>EE</i>	0.535 ± 0.003	13.6 ± 0.07
<i>HH</i>	0.487 ± 0.003	12.4 ± 0.07
<i>PP</i>	0.281 ± 0.005	7.15 ± 0.15
<i>JJ</i>	0.455 ± 0.003	11.55 ± 0.07