

**ISO**

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION

**ISO RECOMMENDATION**

**R 868**

PLASTICS

**DETERMINATION OF INDENTATION HARDNESS OF PLASTICS  
BY MEANS OF A DUROMETER (SHORE HARDNESS)**

1st EDITION

November 1968

**COPYRIGHT RESERVED**

The copyright of ISO Recommendations and ISO Standards belongs to ISO Member Bodies. Reproduction of these documents, in any country, may be authorized therefore only by the national standards organization of that country, being a member of ISO.

For each individual country the only valid standard is the national standard of that country.

Printed in Switzerland

Also issued in French and Russian. Copies to be obtained through the national standards organizations.

STANDARDSISO.COM : Click to view the full PDF of ISO/R 868:1968

## BRIEF HISTORY

The ISO Recommendation R 868, *Plastics – Determination of indentation hardness of plastics by means of a durometer (Shore hardness)*, was drawn up by Technical Committee ISO/TC 61, *Plastics*, the Secretariat of which is held by the United States of America Standards Institute (USASI).

Work on this question led, in 1965, to the adoption of a Draft ISO Recommendation.

In September 1966, this Draft ISO Recommendation (No. 988) was circulated to all the ISO Member Bodies for enquiry. It was approved, subject to a few modifications of an editorial nature, by the following Member Bodies :

Australia	India	South Africa, Rep. of
Austria	Iran	Spain
Belgium	Ireland	Sweden
Brazil	Israel	Switzerland
Bulgaria	Italy	Thailand
Canada	Japan	Turkey
Chile	Korea, Rep. of	U.A.R.
Czechoslovakia	Netherlands	United Kingdom
Finland	Poland	U.S.A.
Germany	Portugal	U.S.S.R.
Hungary	Romania	

Two Member Bodies opposed the approval of the Draft :

France  
New Zealand

The Draft ISO Recommendation was then submitted by correspondence to the ISO Council, which decided, in November 1968, to accept it as an ISO RECOMMENDATION.

STANDARDSISO.COM : Click to view the full PDF of ISO/R 868:1968

## PLASTICS

**DETERMINATION OF INDENTATION HARDNESS OF PLASTICS  
BY MEANS OF A DUROMETER (SHORE HARDNESS)**

## 1. SCOPE

- 1.1 This ISO Recommendation describes the procedure for determining the indentation hardness of plastics by means of durometers of two types; durometer Type A is used for softer plastics and durometer Type D for harder plastics (see Note, clause 7.2). The method permits measurement either of the initial indentation or of indentation after specified periods of time, or both.

NOTE. – The durometers and the methods described in this ISO Recommendation are referred to as Type A Shore and Type D Shore durometers and durometer methods.

- 1.2 These methods are empirical tests intended primarily for control purposes. No simple relationship exists between indentation hardness determined by this method and any fundamental property of the material tested. For specification purposes, it is recommended that ISO Recommendation R 48, *Determination of hardness of vulcanized natural and synthetic rubbers*, should be used for the softer materials.

## 2. PRINCIPLE

This method measures the penetration of a specified indenter forced into the material under specified conditions. The indentation hardness is inversely related to the penetration and is dependent on the modulus of elasticity and the viscoelastic properties of the material. The shape of the indenter and the force applied to it influence the results obtained so that there may be no simple relationship between the results obtained with one type of durometer and those obtained with either another type of durometer or another instrument for measuring hardness.

## 3. APPARATUS

The durometers, Types A and D, consist of the following components :

- 3.1 *Presser foot*, with a hole between 2.5 and 3.5 mm in diameter, centred at least 6 mm from any edge of the foot.
- 3.2 *Indenter*, formed from a hardened steel rod between 1.10 and 1.40 mm in diameter to the shape and dimensions shown in Figure 1, for Type A durometers, and Figure 2, for Type D durometers.
- 3.3 *Indicating device*, for reading the extent of protrusion of the point of the indenter beyond the face of the presser foot; this may be read directly in terms of units ranging from zero, for the full protrusion of  $2.50 \pm 0.04$  mm, to 100, for nil protrusion obtained by placing the pressure foot and indenter in firm contact with a flat piece of glass.
- 3.4 *Calibrated spring*, for applying force to the indenter in accordance with one of the following equations :
- (a) Force in grammes-force =  $56 + 7.66 H_A$   
where  $H_A$  is hardness reading on Type A durometer;
- (b) Force in grammes-force =  $45.36 H_D$   
where  $H_D$  is hardness reading on Type D durometer.

## 4. TEST PIECE

- 4.1 For the determination of hardness by the Type A Shore durometer method, the test piece should be at least 5 mm thick, and by the Type D Shore durometer method, at least 3 mm thick. A test piece may be composed of thinner layers to obtain the necessary thickness, but determinations made on such test pieces may not agree with those made on one-piece test pieces because the surfaces between plies may not be in complete contact.
- 4.2 The dimensions of the test piece should be sufficient to permit measurements at least 12 mm away from any edge, unless it is known that identical results are obtained when measurements are made at a lesser distance from an edge. The surface of the test piece should be flat over an area sufficient to permit the presser foot to be in contact with the test piece over an area having a radius of at least 6 mm from the indenter point. Satisfactory durometer hardness determinations cannot be made on rounded, uneven, or rough surfaces.

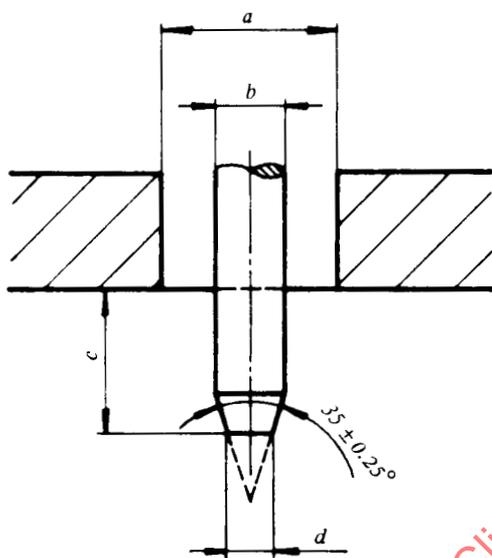


FIG. 1 - Indenter for Type A durometer

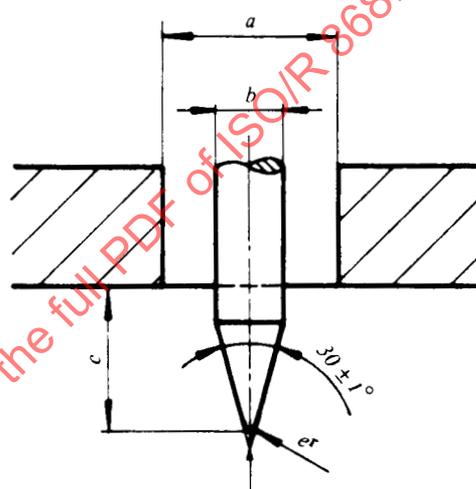


FIG. 2 - Indenter for Type D durometer

<i>a</i>	$3 \pm 0.5$ mm
<i>b</i>	$1.25 \pm 0.15$ mm
<i>c</i>	$2.5 \pm 0.04$ mm
<i>d</i>	$0.79 \pm 0.03$ mm
<i>e</i>	$0.1 \pm 0.012$ mm

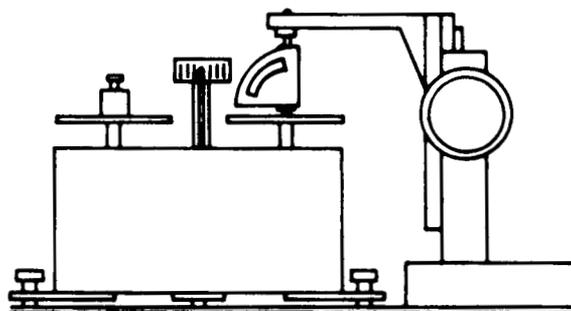


FIG. 3 - Apparatus for calibration of durometer spring