

---

---

## Quasi-static calibration procedure for belt force transducers

*Procédure d'étalonnage quasi-statique pour capteurs d'efforts pour  
ceintures*

STANDARDSISO.COM : Click to view the full PDF of ISO/TS 17242:2014



STANDARDSISO.COM : Click to view the full PDF of ISO/TS 17242:2014



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 General specifications</b> .....	<b>2</b>
3.1 General.....	2
3.2 Limitations or the application of the test belt strap.....	2
<b>4 Test conditions</b> .....	<b>3</b>
4.1 Test method.....	3
4.2 Clamping length.....	3
4.3 Test velocity.....	3
4.4 Belt strap.....	3
4.5 Load relieving.....	3
4.6 Data acquisition.....	3
4.7 Data evaluation.....	3
4.8 Sensor excitation.....	4
4.9 Environmental conditions.....	4
<b>5 Calibration procedure</b> .....	<b>4</b>
5.1 Conditioning.....	4
5.2 Test preparation.....	4
5.3 Calibration test.....	4
5.4 Data storage.....	4
5.5 Data evaluation.....	4
5.6 Documentation.....	5
<b>Annex A (normative) Test setup</b> .....	<b>6</b>
<b>Annex B (normative) Evaluation method</b> .....	<b>7</b>
<b>Annex C (informative) Belt strap characteristics</b> .....	<b>10</b>
<b>Annex D (informative) Applications notes</b> .....	<b>12</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 22, *Road vehicles*, Subcommittee SC 12, *Passive safety crash protection systems*.

STANDARDSISO.COM : Click to view the full PDF of ISO/TS 17242:2014

# Quasi-static calibration procedure for belt force transducers

## 1 Scope

The objective of this Technical Specification is to provide a procedure to calibrate seat belt force transducers with loading capacities up to 25 kN and consistent test specifications and sequences in order to improve comparability of measurement results between testing laboratories.

## 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 376, *Metallic materials — Calibration of force-proving instruments used for the verification of uniaxial testing machines*

ISO 5084, *Textiles — Determination of thickness of textiles and textile products*

ISO 6487, *Road vehicles — Measurement techniques in impact tests — Instrumentation*

ISO 13499, *Road vehicles — Multimedia data exchange format for impact tests*

ECE-R16, *Safety-belts, restraint systems, child restraint systems and ISOFIX child restraint systems for occupants of power-driven vehicles*

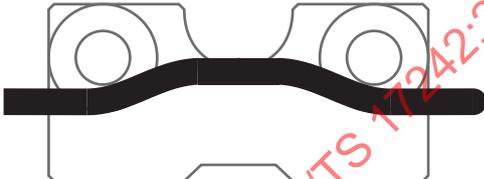
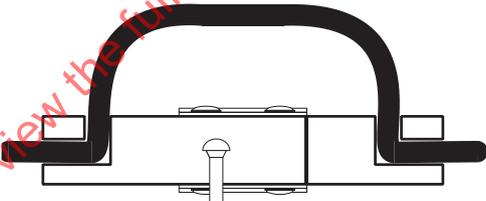
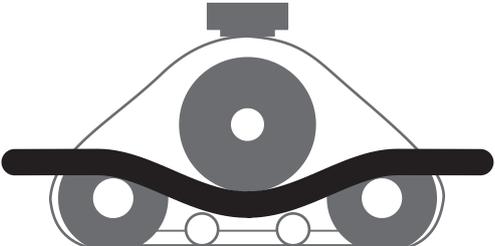
SAE-J2517, *Hybrid III Family Chest Potentiometer Calibration Procedure*

### 3 General specifications

#### 3.1 General

The described measurement procedure refers to belt force transducers with the specifications according to [Table 1](#) and a loading capacity of up to 25 kN.

**Table 1 — Design categorization of belt force transducers**

Type	Description	Belt Orientation
1	Baffle (test belt strap according to Annex 3)	
2	Loop (test belt strap according to customer requirement)	
3	Clamping (test belt strap according to customer requirement)	
4	3-Bolt (test belt strap according to customer requirement)	

#### 3.2 Limitations of the application of the test belt strap

In general, the standardized calibration belt strap (see [C.1](#)) is only recommended for the calibration of belt force transducers which are to be utilized in tests that focuses on comparability between different laboratories (such as during development efforts). In case absolute values have to be obtained, the seat belt webbing designated for subsequent testing purposes is to be used for calibration.<sup>1)</sup>

Calibration using the standardized calibration belt strap shall be done for highly dynamically loaded transducers as shown in Type 1 (baffle). Consequently Types 2, 3, 4, and *Type 1 transducers for quasi-static loads and measurement ranges up to 500 N* (i.e. comfort measurements) are to be excluded.

**NOTE** If required (e.g. by the user or the test protocol), Type 1 transducers with measurement ranges beyond 500 N should be calibrated with a specimen of the seat belt webbing which is designated for subsequent testing purposes. For the calibration of Types 2, 3, 4, and Type 1 transducers for quasi-static loads and measurement ranges below 500 N, a specimen of the seat belt webbing which is designated for subsequent testing purposes will be necessary.

1) Measurement of absolute values shows significant variation for type 1 transducers. A different measurement principle is recommended.

The belt strap type used for calibration as well as the strap's average thickness (see [Annex C](#)) shall be identified in the calibration report.

If a non-standardized belt strap is supplied, it is also recommended to perform a calibration using the standardized belt strap for traceability.

## 4 Test conditions

The calibration test shall be performed under the conditions identified below.

### 4.1 Test method

A continuous loading up to the transducer's full scale range<sup>2)</sup> shall be applied.

### 4.2 Clamping length

As shown in [Annex A](#), the belt force transducer is tested on a belt strap specimen clamped into the universal tension machine. The free clamping length shall be within  $375 \text{ mm} \pm 75 \text{ mm}$ .

### 4.3 Test velocity

The speed of displacement of the tension machine for the continuous loading shall be within  $170 \text{ mm/min} \pm 30 \text{ mm/min}$ .

### 4.4 Belt strap

A standardized belt strap specimen as defined in [Annex C](#) should be utilized.<sup>3)</sup>

### 4.5 Load relieving

The hysteresis is not verified.

### 4.6 Data acquisition

In case of polynomial regression, the zero offset shall not be corrected prior to the test. So the amplifier offset should be considered for the error of measurement of the whole measurement channel. The filter settings shall comply with the ISO 6487 specifications.

### 4.7 Data evaluation

For the evaluation, the first loading sequence<sup>4)</sup> recorded with a minimum sampling rate of  $100 \text{ Hz}$ <sup>5)</sup> shall be considered in a range from 2 % to 100 % of the transducer's calibration range (e.g.  $0,32 \text{ kN} - 16 \text{ kN}$  @  $16 \text{ kN}$  sensor range)<sup>6)</sup>. The nonlinearity is displayed as a percentage in % of the calibration range.

---

2) See transducer data sheet.

3) Other belt strap types have to be identified in the calibration report.

4) No preloading procedures.

5) To reach appropriate accuracy.

6) Ensure the comparison standard is traceable (e.g. ISO 376).

## 4.8 Sensor excitation

The sensor excitation voltage, as well as the sensor connection, shall be in accordance to the customer requirements and shall be recorded.<sup>7)</sup>

## 4.9 Environmental conditions

The calibration test shall be performed under monitored environmental conditions within a temperature range of 19 °C to 23 °C and a Relative Humidity of 10 % to 70 %. For acclimatization purposes, the transducers as well as the belt strap specimen should be kept in this environment for a period of 8 h prior to the calibration.

## 5 Calibration procedure

Proceed with the following steps to perform the calibration test.

### 5.1 Conditioning

An adequate warm-up time for the data acquisition system, test and reference transducer should be allowed to reach thermal equilibrium.

### 5.2 Test preparation

The sensor offset should be measured under no load condition. A new belt strap shall be inserted and centred in the fixations<sup>8)</sup>. The test transducer shall be mounted centred and perpendicular in accordance to the sensor user's manual. The belt strap preload shall not exceed 0,2 % of the calibration range (while holding the transducer in place).

### 5.3 Calibration test

In case of linear regression, prior to the test the sensor's zero offset shall be corrected. In case of polynomial regression, the zero offset shall not be corrected prior to the test<sup>9)</sup>. Only one loading sequence with one belt strap per test transducer up to a force level of 101 % of the transducer's calibration range shall be performed within the given velocity range. The calibration data shall be acquired continuously. There are no requirements for the load relieving sequence.

### 5.4 Data storage

The data storage format is optional<sup>10)</sup>.

### 5.5 Data evaluation

A Linear Equation following [B.1](#) or a Third Degree Polynomial without any offset correction as defined in [B.2](#)<sup>11)</sup> should be determined from the recorded data points.

---

7) Excitation voltage as well as pin assignment and if excitation sensing was utilized shall be stated in calibration report.

8) Fixation by clamp or loop (ECE-R16 conform).

9) Use of the calibration coefficient as defined in SAE-J2517: Prior to a crash test, the original zero offset level should be preserved by either not zeroing the transducer or the amount that was zeroed should be added during post-processing.

10) ISO 13499 recommends: incl. time channel, output test sensor, output reference sensor, and travel distance.

11) If the calibrated transducer is used in tests, the hardware offset shall not be corrected.

## 5.6 Documentation

The test report shall include the following:

- temperature;
- humidity;
- belt strap type;
- strap thickness;<sup>12)</sup>
- sensitivity in kN/mV/V and mV/kN/V (for linear regression) or a third degree polynomial equation in the form  $F = AS^3+BS^2+CS+M$ ;<sup>13)</sup>
- the polynomial coefficients in kN/mV/V (polynomial coefficient's significant digits: 3rd degree: 9 (e.g. 0,001 234 567 89), 2nd degree: 6 (e.g. 1,234 56), 1st degree: 3 (e.g. 12,3));
- measured sensor offset in unloaded condition in mV/V;<sup>14)</sup>
- nonlinearity as a percentage in % of the transducer's calibration range.

---

12) See page 13 "Measurement of Test Belt Strap Thickness".

13) See page 11 "Polynomial Regression".

14) To check the offset magnitude of the data acquisition system.

## Annex A (normative)

### Test setup

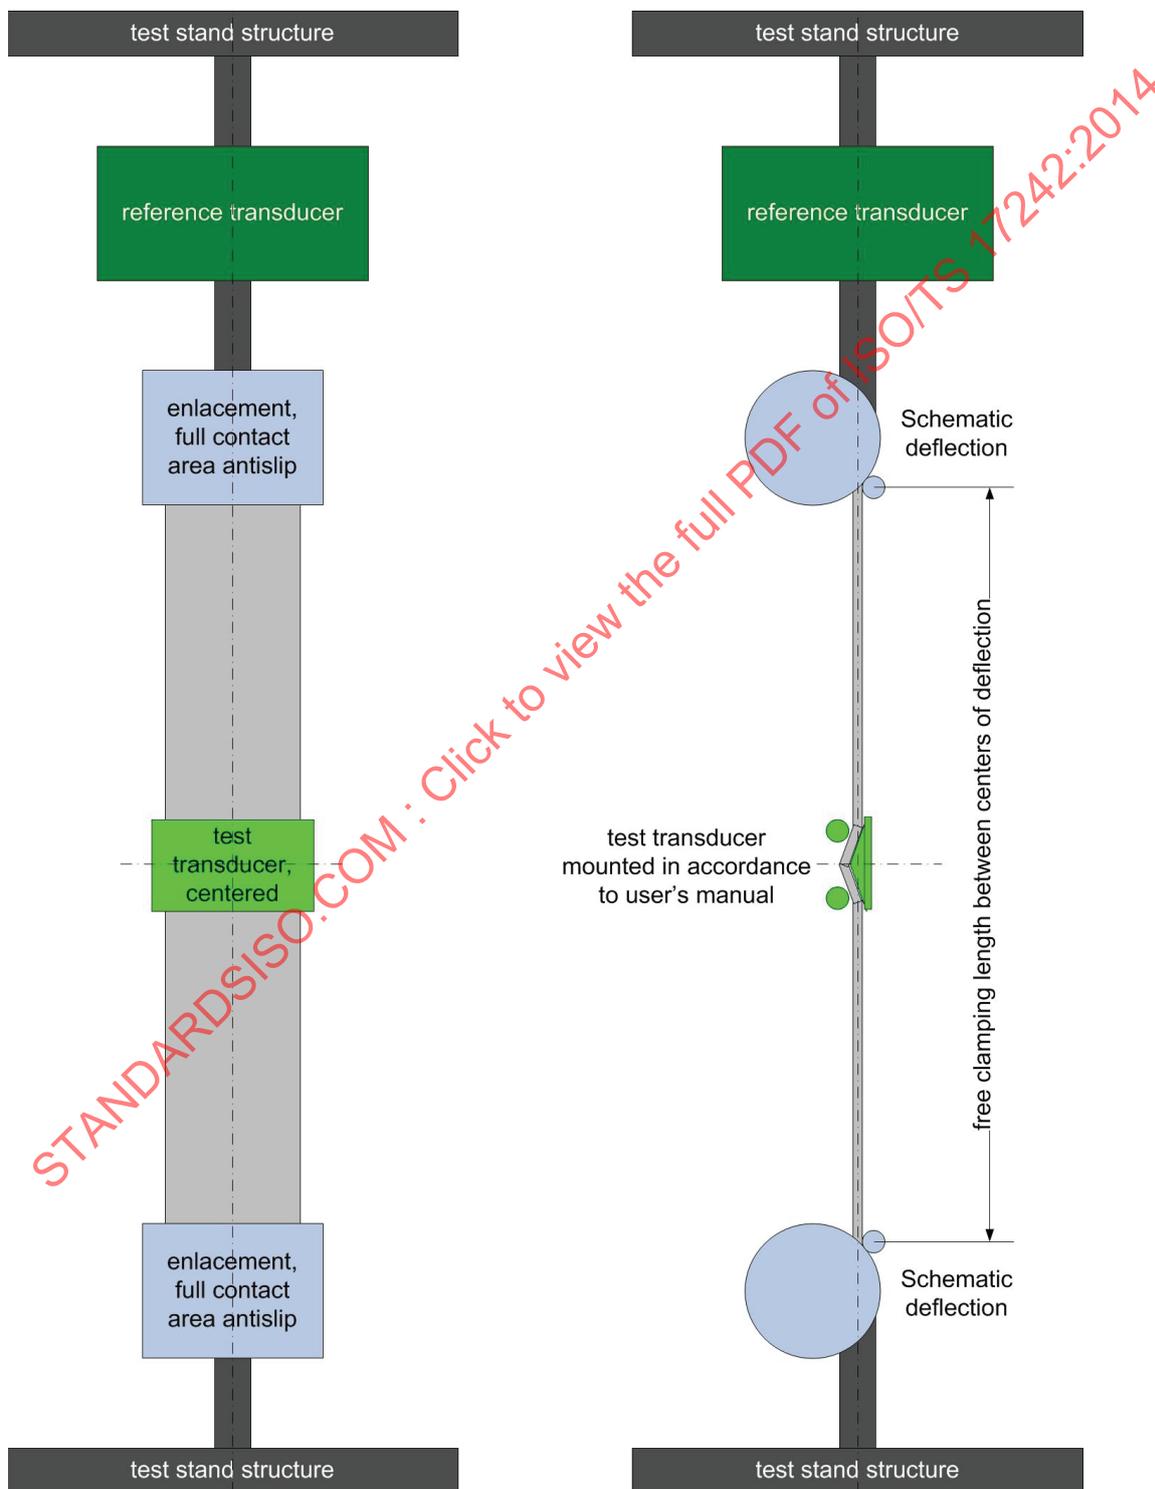


Figure A.1 — Schematic calibration test setup

## Annex B (normative)

### Evaluation method

#### B.1 Linear regression

For the software linearization a least-squares fit method applied through the point of origin is used:

The starting point of the linearized line is identical with the starting point of the measurement. This point is set to zero (point of origin). This measurement is independent of the defined evaluation interval (see 4.7). The resulting linear equation is

$$F_i = b (S_i - S_0) + D \quad (\text{B.1})$$

where

$$S_0 = 0;$$

$$D = 0.$$

For the linearization, the square sum of the difference between measured value and linearized value must be minimal:

$$\sigma = \sum_{i=1}^n [F_i - (b (S_i - S_0) + D)]^2 \quad (\text{B.2})$$

The differentiation is equated to zero:

$$S_i, F_i = \text{measured}$$

From this will follow:

$$b = \frac{\sum_{i=1}^n (F_i - D)}{\sum_{i=1}^n (S_i - S_0)} \quad (\text{B.3})$$

$$a = \frac{1}{b}$$

#### Key

- F is the actual force in kN
- S is the sensor output reading in mV/V
- D is the calculated offset in kN (linear regression)
- a is the sensitivity in mV/kN/V
- b is the inverse sensitivity in kN/mV/V
- $\sigma$  is the deviation

## B.2 Polynomial regression

For the polynomial approximation, a least-squares fit method shall be utilized to determine the polynomial coefficients A, B, C, and M.

With mesh points ( $S_i; F_i$ ) the third degree polynomial will acquire the general form:

$$F_i = A \cdot S_i^a + B \cdot S_i^2 + C \cdot S_i + M \tag{B.4}$$

The function values  $F_i$  are complemented by residues  $r_i$  (corrections)

$$F_i + r_i = A \cdot S_i^a + B \cdot S_i^2 + C \cdot S_i + M \tag{B.5}$$

Applied on the mesh points the observation formulae follow:

$$r_1 = A \cdot S_1^a + B \cdot S_1^2 + C \cdot S_1 + M - F_1 \tag{B.6}$$

↓

$$r_i = A \cdot S_i^a + B \cdot S_i^2 + C \cdot S_i + M - F_i$$

The observation equations are squared and then pooled.

$$\begin{aligned} \sum r_i^2 = & \sum A^2 \cdot S_i^6 \\ & + 2 \sum AB \cdot S_i^5 + 2 \sum AC \cdot S_i^4 + 2 \sum AM \cdot S_i^a \\ & - 2 \sum A \cdot F_i \cdot S_i^a \\ & + 2 \sum B^2 \cdot S_i^4 \\ & + 2 \sum BC \cdot S_i^a + 2 \sum BM \cdot S_i^2 \\ & - 2 \sum B \cdot F_i \cdot S_i^2 + \sum C^2 \cdot S_i^2 + 2 \sum CM \cdot S_i - 2 \sum C \cdot F_i \cdot S_i + M^2 - 2M \cdot F_i + F_i^2 \end{aligned}$$

To determine the minimum of the residues  $r_i$ , the observation formula's sum of squares are differentiated and equated to zero.

$$\frac{d(\sum r_i^2)}{dA} = 2 \sum A \cdot S_i^6 + \sum B \cdot S_i^5 + \sum C \cdot S_i^4 + \sum M \cdot S_i^a - \sum F_i \cdot S_i^a = 0$$

$$\frac{d(\sum r_i^2)}{dB} = \sum A \cdot S_i^5 + 2 \sum B \cdot S_i^4 + \sum C \cdot S_i^a + \sum M \cdot S_i^2 - \sum F_i \cdot S_i^2 = 0$$

$$\frac{d(\sum r_i^2)}{dC} = \sum A \cdot S_i^4 + \sum B \cdot S_i^a + 2 \sum C \cdot S_i^2 + \sum M \cdot S_i - \sum F_i \cdot S_i = 0$$

$$\frac{d(\sum r_i^2)}{dM} = \sum A \cdot S_i^a + \sum B \cdot S_i^2 + \sum C \cdot S_i + 2 \sum M - \sum F_i = 0$$

A linear system of equations results from putting in the mesh points ( $x_i; y_i$ ). Coefficients A, B, C, and M and therefore the equalization polynomial through the point of origin can be calculated.

**Key**

F is the actual force in kN

S is the sensor output reading in mV/V

M is the physical offset prior to the test in kN (polynomial regression)

A, B, and C are the calibration coefficients

STANDARDSISO.COM : Click to view the full PDF of ISO/TS 17242:2014

## Annex C (informative)

### Belt strap characteristics

#### C.1 Specifications for the standardized calibration belt strap

For the calibration of the belt force transducers, a test belt strap with the specifications shown below should be utilized

##### C.1.1 Construction

Normal band equal on both sides, bonding K2/2, doubleshot.

##### C.1.2 Width

47 mm to 49 mm

##### C.1.3 Thickness

1,25 mm to 1,35 mm

##### C.1.4 Weight

64 g/m to 68 g/m

##### C.1.5 Minimum breaking load

≥30 kN

##### C.1.6 Strain

14 % to 16 % at 10 kN

##### C.1.7 Colouring/Finishing

Spin dying

##### C.1.8 Number of chaining threads

300 ± 10

##### C.1.9 Number of filling threads

66 ± 5 (1/100 mm)

The belt strap shall be stored in a packed condition. Furthermore it should be protected from sunlight.

NOTE The test belt strap as defined above is only permitted to be used for highly dynamically loaded transducers according to Type 1 (baffle). For other transducers, the test belt strap which is in accordance with customer requirements should be chosen.