
**Solid mineral fuels — Determination
of Chlorine content**

Combustibles minéraux solides — Dosage de la teneur en chlore

STANDARDSISO.COM : Click to view the full PDF of ISO/TS 18806:2014



STANDARDSISO.COM : Click to view the full PDF of ISO/TS 18806:2014



COPYRIGHT PROTECTED DOCUMENT

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
4.1 Method A — High temperature combustion in oxygen	1
4.2 Method B — Bomb combustion	1
5 Reagent	2
5.1 Method A	2
5.2 Method B	2
6 Apparatus	2
6.1 Method A	2
6.2 Method B	4
7 Preparation of sample	4
8 Procedure	5
8.1 Blank Value Determination	5
8.2 Method A	5
8.3 Method B — Bomb Combustion	5
9 Determination of dissolved chloride	6
9.1 General	6
9.2 Determination by ion chromatography	6
10 Calculation and expression of results	7
11 Test report	7
Annex A (normative) Quality control	8
Annex B (Informative) Results of the German Interlaboratory comparison 2009 for DIN 51727:2011 “Solid fuels-Determination of the chlorine content”	9
Bibliography	11

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT), see the following URL: [Foreword — Supplementary information](#).

The committee responsible for this document is ISO/TC 27, *Solid mineral fuels*, Subcommittee SC 5, *Methods of Analysis*.

STANDARDSISO.COM : Click to view the full PDF of ISO/TS 18806:2014

Solid mineral fuels — Determination of Chlorine content

1 Scope

This Technical Specification specifies two methods (high temperature combustion and bomb combustion) for the determination of chlorine in solid mineral fuels. It is applicable to hard coals, brown coals, coke, and tailings.

The chlorine in the digestion solution can be determined using different methods, e.g. an ion-selective electrode, coulometric or potentiometric titration, spectrophotometry, or ion chromatography. In this Technical Specification, the ion chromatographic separation with conductivity detection is described.

The method is applicable to determine the chlorine content higher than 0,005 per cent mass fraction.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 687, *Solid mineral fuels — Coke — Determination of moisture in the general analysis test sample*

ISO 1170, *Coal and coke — Calculation of analyses to different bases*

ISO 1213-2, *Solid mineral fuels — Vocabulary — Part 2: Terms relating to sampling, testing and analysis*

ISO 5068-2, *Brown coals and lignites — Determination of moisture content — Part 2: Indirect gravimetric method for moisture in the analysis sample*

ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*

ISO 11722, *Solid mineral fuels — Hard coal — Determination of moisture in the general analysis test sample by drying in nitrogen*

EN ISO 10304-1, *Water quality — Determination of dissolved anions by liquid chromatography of ions — Part 1: Determination of bromide, chloride, fluoride, nitrate, nitrite, phosphate and sulfate*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1213-2 apply.

4 Principle

4.1 Method A — High temperature combustion in oxygen

The sample is combusted at high temperature in an oxygen atmosphere. The gaseous combustion products including the formed chloride are collected in a trap filled with water, in which they are dissolved.

4.2 Method B — Bomb combustion

The sample is combusted in a high pressure bomb in an oxygen atmosphere. The formed chloride is collected in an absorption solution inside the bomb.

5 Reagent

5.1 Method A

5.1.1 **Oxygen**, pure, with an assay of at least 99,5 % volume fraction.

5.1.2 **Combustion aid (optional)**, spectroscopic carbon or iron phosphate (FePO_4).

5.2 Method B

5.2.1 **Oxygen**, pure, with an assay of at least 99,5 % volume fraction.

5.2.2 **Combustion aid (optional)**, paraffin, benzoic acid, polyethylene combustion bags, acetobutyrate capsules, or other suitable materials.

5.2.3 **Fuse**, ignition wire (e.g. platinum) and cotton fuse (optional).


Note A possible contribution of the cotton fuse to the chlorine content should be considered.

5.2.4 **Absorption solution**, either eluent used for ion chromatographic determination, or alkaline solution (e.g. 0,2 mol/l KOH or 0,1 mol/l NaOH), or deionised water.

6 Apparatus

6.1 Method A

6.1.1 **Fused silica combustion tube, absorber, and headpiece**, the sintered glass discs in the absorber and the headpiece shall have a pore size of 90 μm to 150 μm (see [Figure 1](#)).

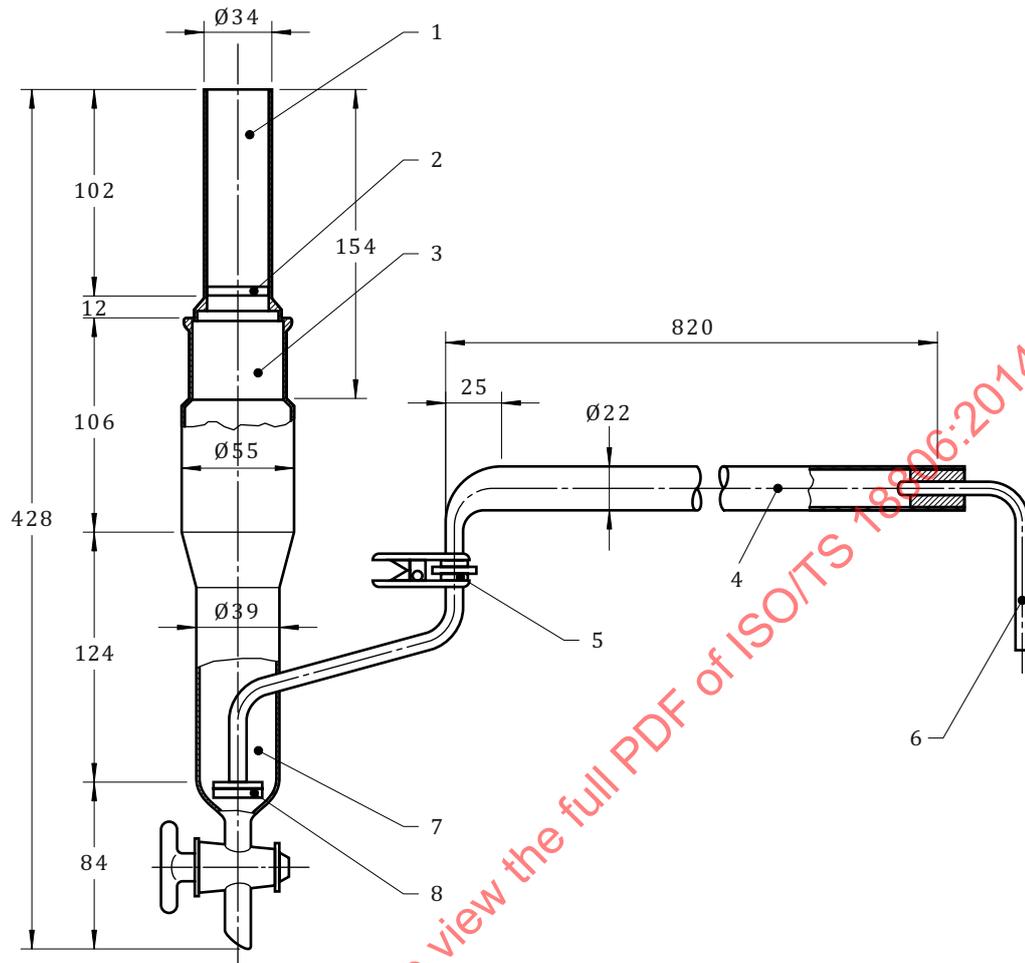


Key

- 1 headpiece
- 2 sintered glass disc
- 3 V45/50 conical ground joint (ISO 383)
- 4 combustion tube
- 5 VS 13 spherical joint (ISO 641)
- 6 oxygen inlet
- 7 absorber
- 8 sintered glass disc

Figure 1 — Apparatus for Method A

6.1.2 Porcelain combustion boat, with handle, e.g. 70 mm long, 10 mm wide, and 7 mm deep.

6.1.3 Silica pusher, with iron inlay (see [Figure 2](#)).

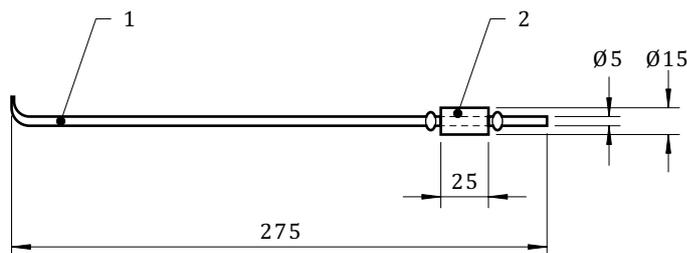

Key

- 1 silica pusher
- 2 iron inlay

Figure 2 — Silica pusher

6.1.4 Magnet.

6.1.5 Electrical tube furnace, about 300 mm long, capable of being heated to at least 1 300 °C and maintained at $(1\,250 \pm 25)$ °C.

6.1.6 Flow meter.

6.1.7 Oxygen inlet, consisting of a pierced silicon stopper with a glass tube.

6.2 Method B

6.2.1 Digestion unit

6.2.1.1 Digestion bomb, with inner surface that is resistant to corrosion by acidic gases formed or emitted during combustion.

6.2.1.2 Pressure regulator, to control the filling of the bomb with oxygen and discharging afterwards.

6.2.1.3 Pressure gauge, with relieve valve operating at 3,5 MPa.

6.2.1.4 Ignition circuit.

If appropriate, the equipment for determination of calorific value according to ISO 1928 can be used simultaneously for chlorine determination. Attention is drawn to the fact that deionised water should be used as absorption solution and that 10 ml instead of 1 ml (as in ISO 1928) are used.

6.2.2 Crucible, of silica, nickel-chromium, platinum, or similar non-reactive material that is resistant to corrosion by acidic gases formed or emitted during combustion.

7 Preparation of sample

The coal or coke used for the determination of the chlorine content is the general analysis test sample ground to pass a sieve of 212 µm aperture. Expose the sample in a thin layer for the minimum time required for the moisture content to reach approximate equilibrium with the laboratory atmosphere. Before commencing the determination, mix the air-dried sample.

After weighing the test portion (see 8.2.2 or 8.3.2), determine the moisture content using a further portion of the test sample by the method described in ISO 687, ISO 5068-2, or ISO 11722, as appropriate.

8 Procedure

8.1 Blank Value Determination

Blank values shall be measured by performing a complete analysis (method A or method B, whatever used for analysis of samples) without sample but including combustion aid, if used. Blank values should be measured on a daily basis or when series of analyses are started.

8.2 Method A

8.2.1 Preparation

Adjust the tube furnace to ensure a temperature of $(1\ 250 \pm 25)$ °C in the combustion zone. Place the combustion tube in the furnace so that its projecting vertical section with the spherical ground joint is as near as possible to the hottest zone to prevent any condensation of combustion products.

Adjust the oxygen flow to $(1 \pm 0,1)$ l/min.

Mix samples having more than 30 % mass fraction ash with 0,1 g to 0,2 g of combustion aid to achieve uniform combustion.

8.2.2 Combustion procedure

Weigh, to an accuracy of 0,1 mg, about 50 mg to 1 000 mg (depending on the chlorine concentration) of the sample prepared according to [Clause 7](#) into a combustion boat. Push the boat into the combustion tube using the silica pusher until the tube can be closed with the oxygen inlet.

NOTE Carefully place the front end of the pusher into the handle of the combustion boat. Otherwise problems to remove the boat after test might occur.

Fill the absorber with 150 ml deionised water. After starting the oxygen flow, mount the headpiece on the absorber and fill it with 20 ml deionised water.

To prevent deflagration, initially use the magnet to move the pusher together with the combustion boat containing the sample into the combustion zone so far only, that the front section of the sample is ignited only. After the sample has reached red heat (approximately one minute after ignition), push it into the combustion zone to burn it completely. High temperature coke samples can be pushed into the combustion zone directly.

Combustion time is depending on the ash of the sample. It is about 20 mins for coals having 10 % to 20 % mass fraction ash. After combustion has been terminated, transfer the absorption liquid from headpiece and absorber into a 250 ml volumetric flask. Rinse headpiece and absorber with deionised water and add to the flask. Fill up to the mark with deionised water (V_D).

8.3 Method B — Bomb Combustion

8.3.1 Preparation

Bomb parts shall be inspected regularly for wear and corrosion; particular attention shall be paid to the condition of the threads of the main closure. Manufacturers' instructions and any local regulations regarding the safe handling and use of the bomb shall be observed. Before starting a test ensure that no gas leakage occurs.

NOTE Gas leakage can be checked easily by complete immersing the pressurized bomb in cold water.

8.3.2 Combustion procedure

Weigh, to an accuracy of 0,1 mg, about 50 mg to 1 000 mg (depending on the chlorine concentration) of the sample prepared according to [Clause 7](#) into a crucible.

Note If appropriate, chlorine can be determined simultaneously with calorific value according to ISO 1928 (for details see [6.2.1](#)).

If not easily combusting samples are to be analysed, weigh into e.g. acetobutyrate capsules or use a combustion aid, e.g. benzoic acid.

Fill 10 ml of the absorption solution ([5.2.4](#)) into the bomb and wet the inner surface of the bomb, e.g. by carefully rotating it. Select an absorption solution that is capable to absorb the acidic combustion products completely.

Place the crucible in its support and fix it. Attach the ignition wire and assemble the bomb. Charge the bomb slowly with oxygen to a pressure of maximum $(3,0 \pm 0,2)$ MPa. Initiate the combustion by firing the fuse. After the combustion is completed let the bomb cool down to ambient temperature. Release the pressure at a moderate rate and dismantle the bomb carefully.

Transfer the chlorine absorbed solution into a volumetric flask by either

- Addition of, e.g. 40 ml absorption solution ([5.2.4](#)) to the bomb, closing and shaking the bomb in such a manner as to rinse all interior surfaces of the bomb, the combustion crucible, and the pressure release valve with absorbing solution; and/or
- Rinsing all interior surfaces of the bomb, the combustion crucible, and the pressure release valve with absorbing solution ([5.2.4](#)).

Transfer all solutions into a volumetric flask (e.g. 100 ml or 50 ml, depending on the chlorine content) and fill up to the mark (V_D) with absorption solution ([5.2.4](#)).

If appropriate, take an aliquot (V_A), transfer it to another volumetric flask and fill up to the mark (V_M) with absorption solution ([5.2.4](#)).

NOTE Before injecting the sample into the ion chromatograph, an aliquot of the sample solution can be filtered through an, e.g. 0,45 μm disposable filter in order to protect the column.

9 Determination of dissolved chloride

9.1 General

The chloride content in the digestion solution can be determined using different methods, e.g. an ion-selective electrode, coulometric or potentiometric titration, spectrophotometry, or ion chromatography.

In this Technical Specification, the ion chromatographic separation with conductivity detection is described in detail.

9.2 Determination by ion chromatography

9.2.1 General

The ion chromatographic separation with conductivity detection is performed according to EN ISO 10304-1.

As the chromatograms, especially retention times depend on concentrations and matrix, a calibration on the basis of matrix-adjusted reference materials is recommended.

9.2.2 Apparatus

— **Ion Chromatograph**, preferably with conductivity detection.

9.2.3 Reagent

— **Eluent**, suitable for the ion chromatographic equipment used.

10 Calculation and expression of results

Calculate the chlorine content in the solid mineral fuel from the chloride concentration in the digestion solution, the sample mass, blank values (if any, e.g. coming from combustion aid or eluent), and any dilution steps according to Formula (1):

$$w(Cl_{ad}) = \frac{(\beta_S - \beta_B) \times V_D}{m \times 10\,000} \times \frac{V_M}{V_A} \quad (1)$$

where

$w(Cl_{ad})$ is the chlorine content of the sample as analysed (air dried), given in per cent mass fraction;

β_S is the mass concentration of chlorine in V_M , in milligrams per litre;

β_B is the mass concentration of chlorine in the blank determination, in milligrams per litre;

V_D is the volume of the digestion solution, in millilitres (e.g. Method A 250 ml; Method B 50 ml or 100 ml);

NOTE: V_D is the volume used for chloride determination if no dilution is necessary.

V_M is the volume of the (diluted) solution used for chloride determination, in millilitres;

V_A is the volume of the aliquot taken from the digestion solution, in millilitres;

m is the mass of the test portion, in grams;

V_M/V_A is the dilution factor. If no dilution has been made, this term will be equal to one ($V_M/V_A = 1$).

Report the chlorine content in the air-dried sample, as average of duplicate determinations, for per cent mass fractions

- of $>0,1$ % rounded to 0,01 % mass fraction, and
- of $\leq 0,1$ % rounded to 0,001 % mass fraction.

For the calculation of results to other bases, refer to ISO 1170.

11 Test report

The test report shall include the following particulars:

- a) reference to this International Technical Specification (i.e. ISO/TS 18806);
- b) the identification of the sample tested;
- c) the results of the determination.

Annex A (normative)

Quality control

A.1 Blank values

Determine the blank values for each series of analyses if a combustion aid (e.g. benzoic acid) is used. For this purpose combust the combustion aid (e.g. benzoic acid) only.

If combustion aid is used regularly, the use of a blank value control chart is recommended.

A.2 Reproducibility

When starting a series of analyses a control sample (reference material with same matrix as the samples) shall be analysed for a function check of combustion and chromatographic equipment. If appropriate, pure organic substances (e.g. 5-chloro-2-hydroxy-benzoic acid) can be used.

NOTE The use of a control chart for these results is recommended.

STANDARDSISO.COM : Click to view the full PDF of ISO/TS 18806:2014