

## Methods for Evaluating Cryogenic Filters

### 1. SCOPE:

- 1.1 The purpose of this test procedure is to present test methods that can be utilized to evaluate the filtration and operating characteristics of filters that will be utilized in a cryogenic system. The methods presented herein are intended to supplement standard filter testing specifications to allow evaluation of filter performance characteristics in areas that could be affected by extreme low temperatures. The test methods can be utilized to evaluate filters up to and including 60 gpm (230 lpm) capacity. If higher flow rate filters are to be evaluated in accordance with the test methods presented herein, it will be necessary to increase the system flow capacity and the size of effluent sampling system.
- 1.2 The test methods presented herein do not encompass testing of cryogenic bypass relief valves,  $\Delta P$  indicators, gages, or components other than a basic filter housing and element.
- 1.3 This procedure includes equivalent metric units (in parentheses) as reference information, where deemed useful.

### 2. REFERENCES:

#### 2.1 Applicable Documents:

The following publications form a part of this specification to the extent specified herein. The latest issue of Aerospace Recommended Practices and other documents shall apply.

- 2.1.1 SAE Publications: Available from SAE, 400 Commonwealth Drive, Warrendale, PA 15096-0001.

ARP598	The Determination of Particulate Contaminations in Liquids by the Particle Count Method
ARP901	Bubble Point Test Method

SAE Technical Standards Board Rules provide that: "This report is published by SAE to advance the state of technical and engineering sciences. The use of this report is entirely voluntary, and its applicability and suitability for any particular use, including any patent infringement arising therefrom, is the sole responsibility of the user."

SAE reviews each technical report at least every five years at which time it may be reaffirmed, revised, or cancelled. SAE invites your written comments and suggestions.

Copyright 2002 Society of Automotive Engineers, Inc.  
All rights reserved.

Printed in U.S.A.

TO PLACE A DOCUMENT ORDER: (724) 776-4970 FAX: (724) 776-0790 SAE WEB ADDRESS: <http://www.sae.org>

## SAE ARP900 Revision A

2.1.2 U.S. Government Publications: Available from Standardization Documents Order Desk, Building 4D, 700 Robbins Avenue, Philadelphia, PA 19111-5094.

2.1.2.1 Military Specifications:

MIL-P-27401 Type II, Grade C Propellant Pressurizing Agent, Nitrogen

2.1.2.2 Military Standards:

MIL-STD-810 Environmental Test Methods and Engineering Guidelines

3. TEST EQUIPMENT:

3.1 Liquid Nitrogen Source:

The liquid nitrogen source shall be capable of maintaining a constant single phase flow rate of 60 gpm (230 lpm), or a flow rate equal to the test filter's rated flow if less than 60 gpm (230 lpm), at a pressure of 200 psig (1.38 Pascals gauge) for a minimum period of 3 min.

3.2 Membrane Filter Holder:

Holders designed for 47 mm diameter membrane filters shall be used downstream of the test filter. Such holders shall have suitable backing to support the membrane without rupture for the pressure drops involved. The effective filtering area of the holders shall be measured by 4.1.1 of ARP598. It may be necessary to modify the filter holders by installing a polytetrafluoroethylene seal to eliminate external leakage at cryogenic temperatures. Membrane filters of 3.0  $\mu\text{m}$  mean pore size shall be used in the holders for taking effluent samples.

3.3 Desiccator:

A desiccator shall be utilized to remove moisture from the membrane filters prior to test.

3.4 Effluent Optical Inspection Equipment:

The effluent samples obtained during the maximum particle test, specified herein, shall be examined and sized utilizing the microscopic equipment described in the apparatus section of ARP598, Reference 2.1.1.

3.5 Pressure Gages:

All pressure gages shall have an accuracy of +0.5% or better and shall be attached to the system utilizing a minimum of 18 in (46 cm) of 1/4 in (6 mm) tubing to insure an ambient temperature at the pressure gage.

3.6 Differential Pressure Instruments:

All differential pressures shall be observed utilizing a differential pressure gage or transducer with an overall accuracy of better than  $\pm 1\%$ . The pressure lines to the differential indicator shall have a minimum length of 18 in (45.7 cm) of 1/4 in (6 mm) tubing between the gage and the system to insure temperature stabilization at the gage.

3.7 Temperature Measuring Instruments:

A temperature measuring device having an accuracy of  $\pm 10$  °F ( $\pm 6$  °C) at the point of indication shall be utilized to record temperatures. The response time of the temperature indicator shall not be less than 16 °F (9.6 °C) per second.

3.8 Flow Meters:

A turbine flow meter, or any other type flow meter compatible with cryogenic fluids and having traceability to National Technical Information Service, shall be utilized to determine the system flow rate. The overall error of the flow meter and recording system combined shall not exceed a root/mean square of  $\pm 4\%$ .

3.9 Manometer:

A manometer calibrated in 0.1 in (2 mm) subdivisions shall be utilized for pressure measurements below 2 psig (14 kPa).

3.10 Mass Spectrometer Leak Detector:

Detectable minimum leakage of  $1 \times 10^{-5}$  std cc/s.

3.11 Sampling Chamber:

The sampling chamber utilized in the low temperature leakage test system shown in Figure 1 shall have an internal volume of no more than 300 in<sup>3</sup> (5 L) after deducting the volume of the test filter. The complete chamber shall be sealed prior to testing. The sampling port shall be located at the top of the helium sampling box.

4. TEST PROCEDURES:

4.1 Bubble Test:

The test filter shall be subjected to a bubble point test as described in Section 4 of ARP901. The initial bubble point observed shall be recorded and utilized as a reference to determine damage and deformation to the filter element during subsequent testing.

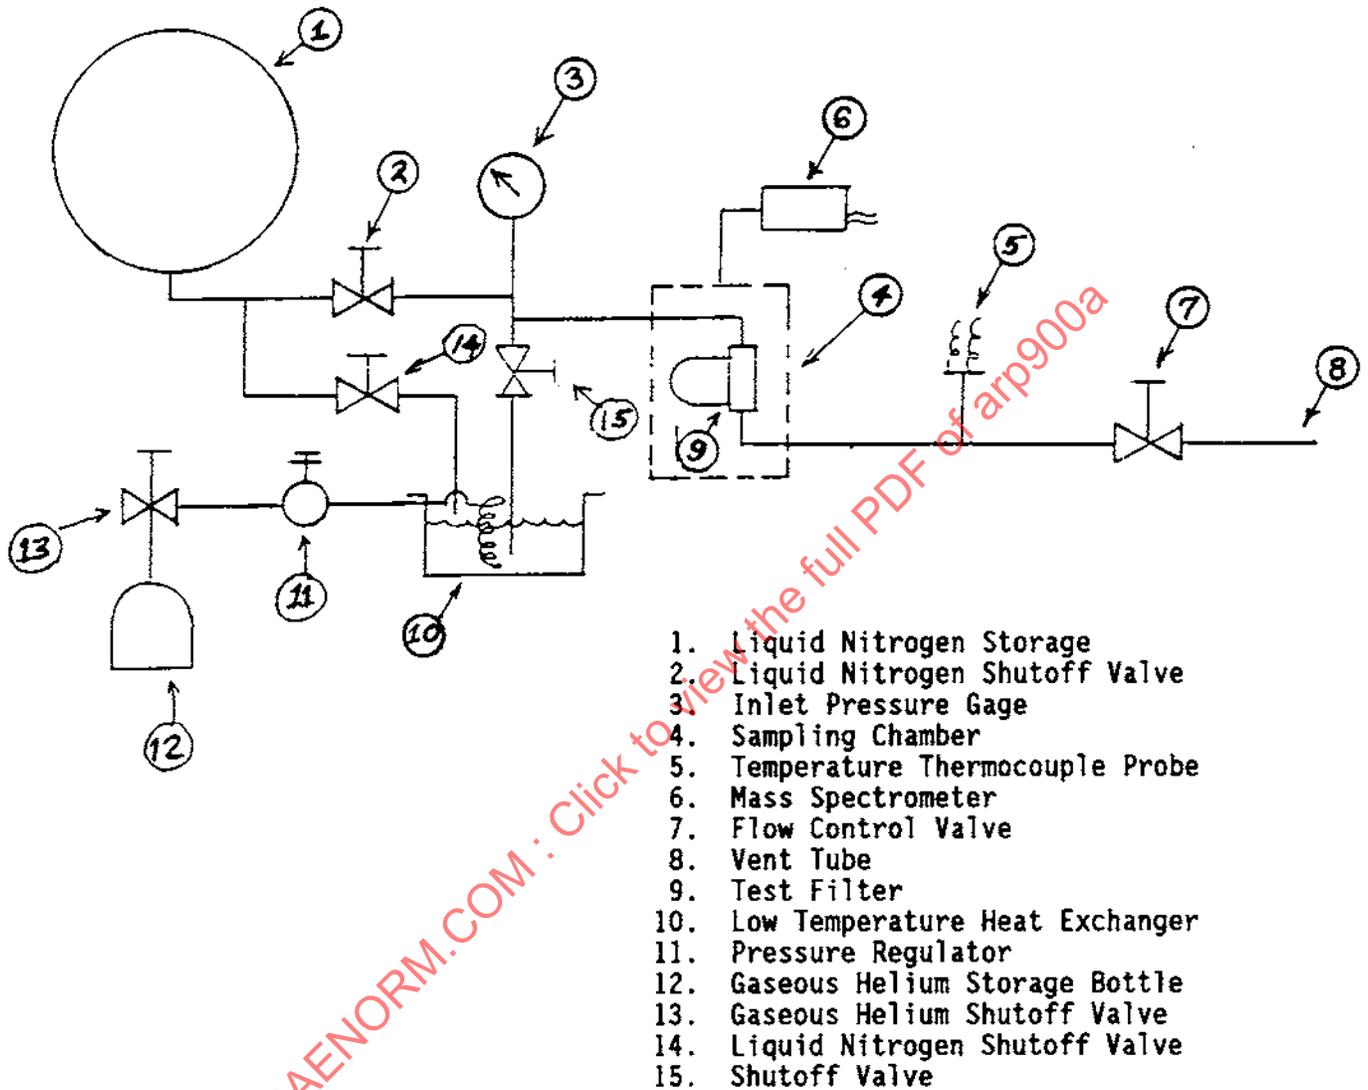


FIGURE 1 - Low Temperature External Leakage Test System

## SAE ARP900 Revision A

### 4.1 (Continued):

Upon completion of the bubble point test, the filter element shall be dried at a temperature of 220 °F (105 °C) for a period of 1 h to eliminate the possibility of residual liquid freezing and causing detrimental effects during subsequent testing.

### 4.2 Low Temperature External Leakage Test:

#### 4.2.1 The test filter shall be installed in a low temperature pressurization system, as shown in Figure 1, in a position that will allow the majority of liquid nitrogen to drain from the filter when flow control valve #7 is opened.

The heat exchanger utilized to reduce the temperature of the gaseous helium shall be filled and maintained at the full level by the adjustment of the liquid nitrogen shutoff valve #14. The heat exchanger shall have the capacity of reducing the temperature of the gaseous helium to -320 °F ± 20 (-196 °C ± 10) at the outlet. The flow control valve #7 shall be opened and the system purged with liquid nitrogen until a temperature of -320 °F ± 20 (-196 °C ± 10) is obtained at the thermocouple, located downstream of the test filter. The temperature at the thermocouple probe shall be maintained at a temperature of -320 °F ± 20 (-196 °C ± 10) for a 1 min period.

The liquid nitrogen shutoff valve #2 shall then be closed and the liquid nitrogen within the system drained, by opening valve #7. The flow control valve #7 shall be closed and the desired proof pressure applied to the inlet port of the test filter, by adjustment of pressure regulator #11.

The pressure shall be maintained for a 20 min period. Indication from the mass spectrometer leak detector should show a leakage rate of less than 1 cc/min.


After the 20 min pressurization period, the gaseous helium shutoff valve #13 shall be closed and the system pressure reduced to zero by opening valve #7. The system vent line #8 shall be long enough to exclude the possibility of contaminating the atmosphere within the sampling chamber #4.

#### 4.2.2 The cool-down and pressurization cycle described shall be repeated three times. There shall be no indication of the helium contamination level within the sampling chamber exceeding the specified limit.

### 4.3 Maximum Particle Test:

#### 4.3.1 A bubble test as described in 4.1 and ARP901 shall be performed on the filter element at room temperature.

A system as shown in Figure 2 shall be utilized to determine the maximum size particle that will pass through the test filter's element. The test system will be designed to minimize all traps or cavities that would entrain the glass beads utilized as a contaminant during testing. A pressurization source or a cryogenic pump can be utilized to establish the required flow rate. Prior to conducting a test program, the system should be thoroughly cleaned and dried.

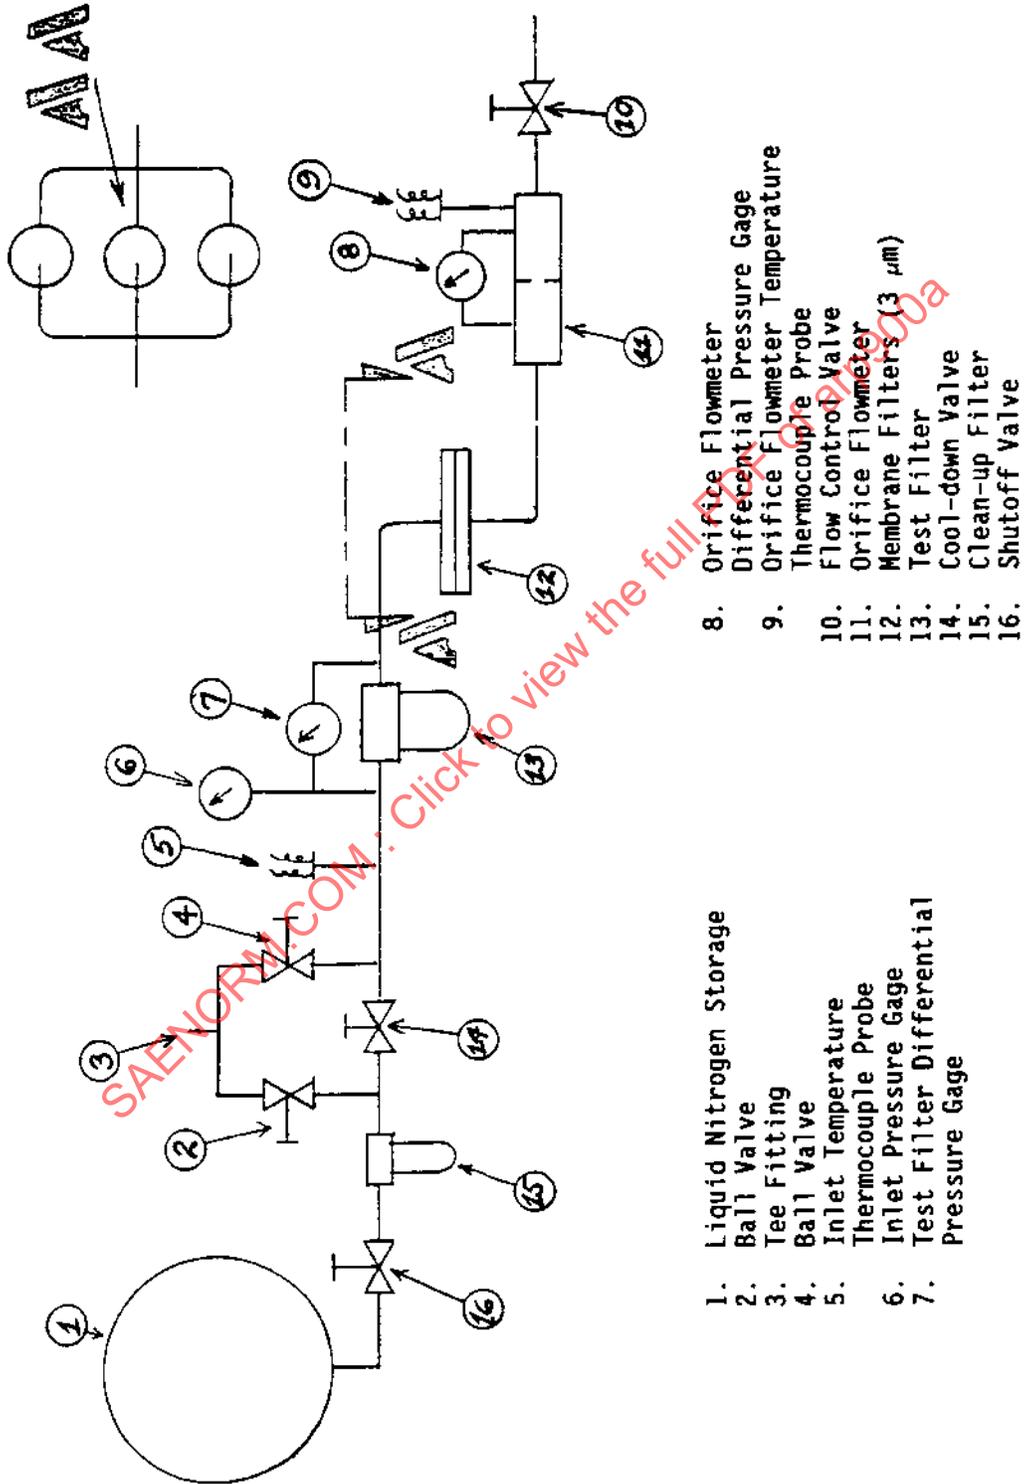

1. Liquid Nitrogen Storage
2. Ball Valve
3. Tee Fitting
4. Ball Valve
5. Inlet Temperature Thermocouple Probe
6. Inlet Pressure Gage
7. Test Filter Differential Pressure Gage

8. Orifice Flowmeter
9. Differential Pressure Gage
10. Orifice Flowmeter Temperature Thermocouple Probe
11. Flow Control Valve
12. Orifice Flowmeter
13. Membrane Filters (3 μm)
14. Test Filter
15. Cool-down Valve
16. Clean-up Filter
17. Shutoff Valve

FIGURE 2 - Maximum Particle Test System

## SAE ARP900 Revision A

### 4.3.1 (Continued):

The membrane filters utilized to obtain the effluent samples shall have a 3  $\mu\text{m}$  pore size, with a 47 mm diameter. One membrane filter shall be utilized to obtain effluent samples at flow rates from 0 to 20 gpm (75 lpm). Two membrane filters shall be installed in parallel to obtain the effluent samples at flow rates from 20 to 40 gpm (75 to 150 lpm). At flow rates from 40 to 60 gpm (150 to 230 lpm), three 47-mm-diameter membrane filter holders shall be utilized in parallel to collect the effluent sample. The membrane filters shall be dried in a desiccator at a temperature of 125 °F (50 °C) for a 1 h period prior to installing in the test system to remove all signs of moisture.

Prior to installing the test filter in the system, a blank run will be performed to insure that residual glass beads have not remained in the test system from previous tests. A fitting shall be installed in the system to duplicate the filter. The contaminant induction valves #2 and #4 shall be placed in the closed position with valve #14 in the open position. A membrane filter, or filters, depending upon flow rate, shall be installed downstream of the test filter.

Valves #10, #14, and #16 shall then be placed in the open position and the system cooled down. Flow control valve #10 shall be slowly adjusted to obtain the test filter's rated flow through the system, after single-phase liquid flow has been obtained, as indicated by a continuous reading of  $-320\text{ }^{\circ}\text{F} \pm 20$  ( $-196\text{ }^{\circ}\text{C} \pm 10$ ) at the inlet temperature thermocouple probe #5. Valve #10 shall be adjusted to maintain the flow rate through the system for a 1 min period. Upon conclusion of the 1 min flow period, valve #16 shall be placed in the closed position and the pressure within the system allowed to decay to zero.

Flow control valve #10 shall then be closed and the system allowed to return to ambient temperature. The pressure within the system, after returning to ambient temperature, shall be bled through valve #10 to atmosphere and the membrane filter removed.

The entire effective membrane filter area should then be examined, utilizing the optical equipment described in Reference 2.1.1 to determine whether any glass beads are present. If signs of glass beads are observed, the complete system will be recleaned, and the test described repeated until there is no evidence of glass beads.

The test filter shall be installed in the system and a membrane filter installed in the filter holders, Item #12. Valve #2 and #4 shall be placed in the closed condition and valves #10, #14, and #16 placed in the open position to allow the system to cool down.

The tee fitting cap #3 shall be removed; the glass beads introduced into the system; and the cap replaced. The quantity and size distribution of glass beads should be equal to the quantity and size required by the basic specification to which this specification is a supplement.

4.3.1 (Continued):

After single-phase flow is obtained through the test filter, as indicated by a constant differential pressure across the filter, and an inlet temperature of  $-320\text{ }^{\circ}\text{F} \pm 20$  ( $-196\text{ }^{\circ}\text{C} \pm 10$ ) at the inlet temperature thermocouple probe, the flow control valve #10 shall be adjusted to maintain rated flow. Valves #2 and #4 shall be opened and valve #14 placed in the closed position. The flow rate through the system shall be maintained for a 1 min period. Valve #16 shall then be placed in the closed position and the system pressure allowed to decay to zero; at that time valve #10 shall be closed and the system allowed to return to ambient temperature. The pressure built up within the system due to thermal expansion, should be periodically vented to atmosphere so as not to exceed the working pressure of the system. The membrane filters utilized to obtain the effluent sample shall then be removed from the system. The entire surface area will then be scanned for the maximum particle per optical equipment in ARP598. If disintegration of the membrane filter is observed at any point on the surface, the test results will be considered invalid and the test repeated.

4.4 Thermal Shock Test:


- 4.4.1 The test filter shall be subjected to a bubble point test as described in 4.1 and ARP901. The initial bubble point observed shall be recorded and utilized as a reference to determine damage and deformation to the filter element during thermal shock.

The test filter shall then be installed in a system, as shown in Figure 3, and subjected to an ambient temperature of  $160\text{ }^{\circ}\text{F}$  ( $70\text{ }^{\circ}\text{C}$ ) for a period of 1 h, or until complete temperature stabilization has occurred; whichever is greater. Temperature stabilization shall be determined as having occurred when a temperature of  $160\text{ }^{\circ}\text{F} \pm 10$  ( $70\text{ }^{\circ}\text{C} \pm 5$ ) is recorded on both the internal and external thermocouple probes.

Flow control valves #8 and #9, located upstream of the test filter shall then be opened and a single phase of liquid flow obtained. Flow control valve #8 shall then be closed and flow control valve #6 opened, allowing the temperature at the outlet port of the filter to be reduced to  $-300\text{ }^{\circ}\text{F}$  ( $-185\text{ }^{\circ}\text{C}$ ) in a 30 s period, or less. The test filter shall then be resubjected to an ambient temperature of  $160\text{ }^{\circ}\text{F}$  ( $70\text{ }^{\circ}\text{C}$ ) until temperature stabilization as occurred. The temperature cycle described shall be repeated 10 times. Upon conclusion of the ten cycles, the filter shall be removed from the test system and disassembled.

- 4.4.2 The element shall then be subjected to a bubble point test. The initial bubble shall compare with the initial bubble point obtained prior to conducting the thermal shock test.

There shall be no evidence of damage or distortion.

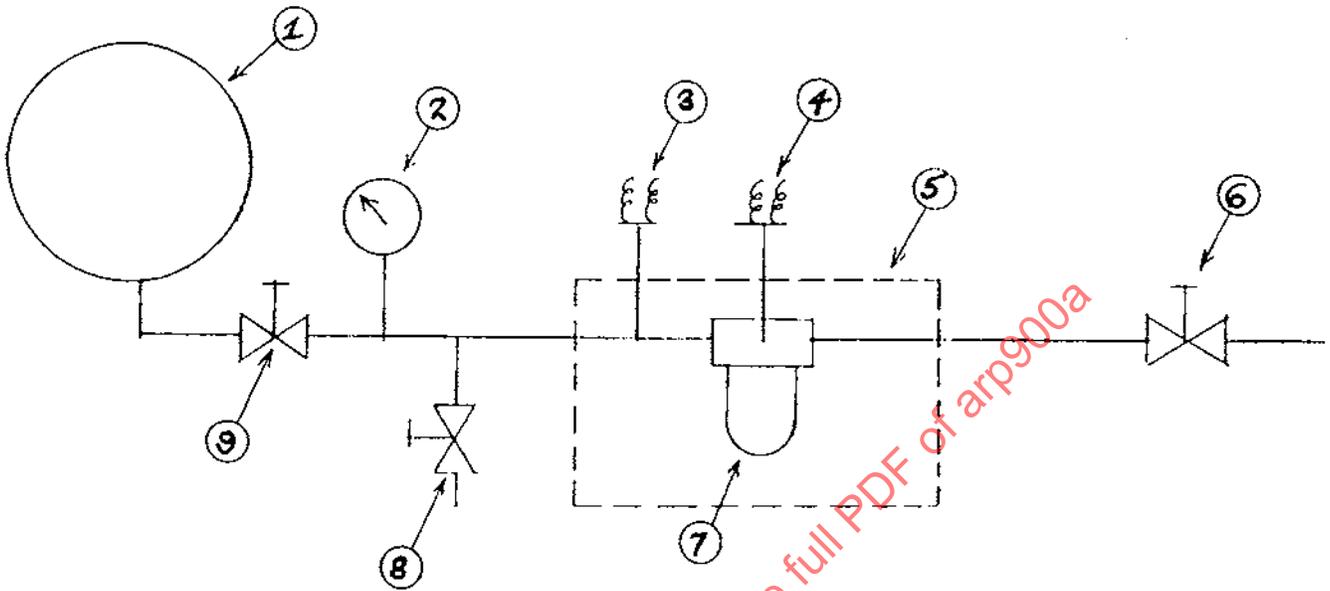

1. Liquid Nitrogen Storage
2. Pressure Gage
3. Inlet Temperature Thermocouple Probe
4. Skin Temperature Thermocouple Probe
5. Temperature Chamber (160 °F)
6. Flow Control Valve
7. Test Filter
8. Cool-down Valve
9. Shutoff Valve

FIGURE 3 - Thermal Shock Test System